

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112525\
 Data File : PS032538.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2025 11:59
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 26 00:54:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.285	7.628	1542.7E6	1812.4E6	340.449	497.175 #
Target Compounds							
2) T	3,5-DICHL...	6.448	0.000	1633268	0	<MDL	N.D. #
3) T	4-Nitroph...	7.134f	0.000	292488	0	<MDL	N.D. #
7) T	MCPA	7.825f	0.000	374930	0	<MDL	N.D. #
8) T	DICHLORPROP	8.185	0.000	543479	0	<MDL	N.D. #
10) T	Pentachlo...	8.711	0.000	3226236	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.274	0.000	2289674	0	<MDL	N.D. #
12) T	2,4,5-T	9.602	10.189	2829617	1916251	<MDL	<MDL #
13) T	2,4-DB	10.154	10.744	530844	1870421	<MDL	<MDL #
14) T	DINOSEB	11.345	0.000	1876139	0	<MDL	N.D. #
15) T	Picloram	11.184	12.184f	204137	5085150	<MDL	<MDL #
16) T	DCPA	11.639	12.184f	1931240	5085150	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112525\
Data File : PS032538.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2025 11:59
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 26 00:54:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

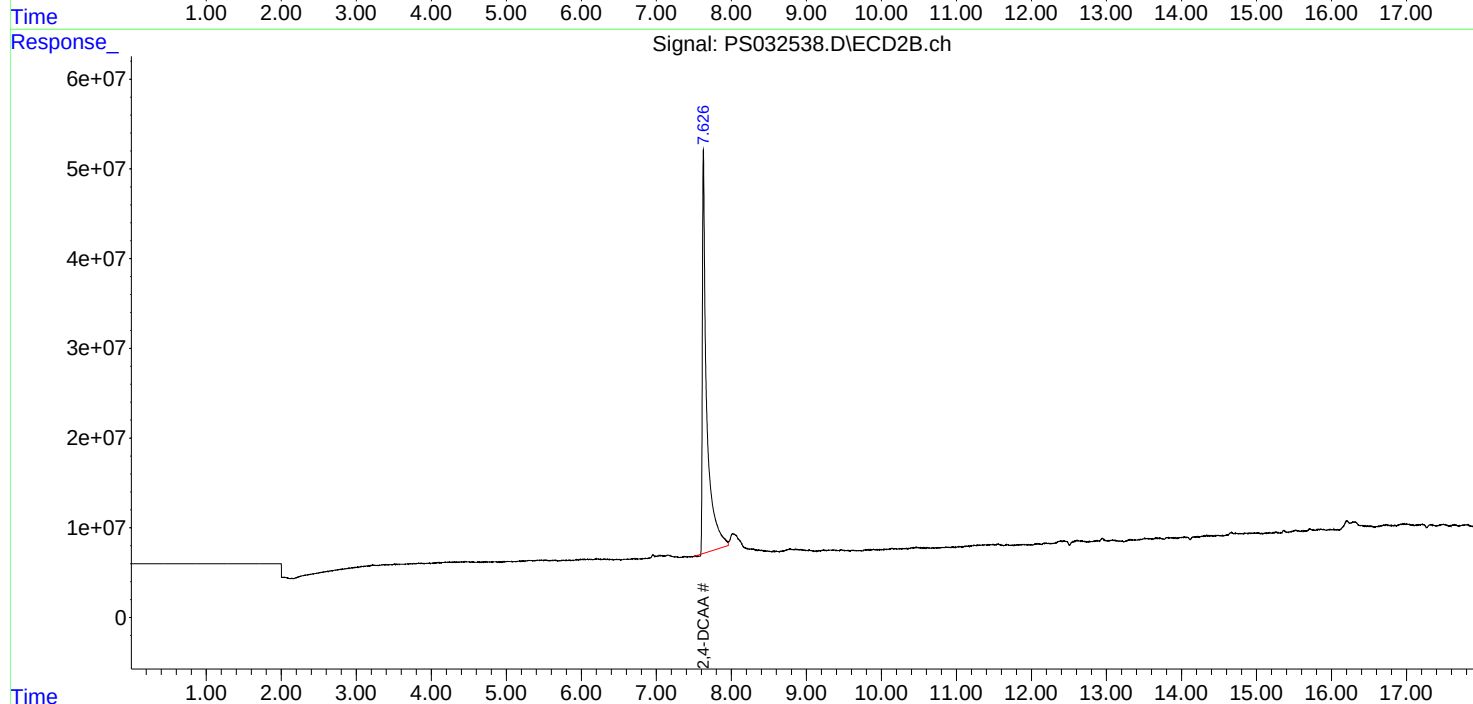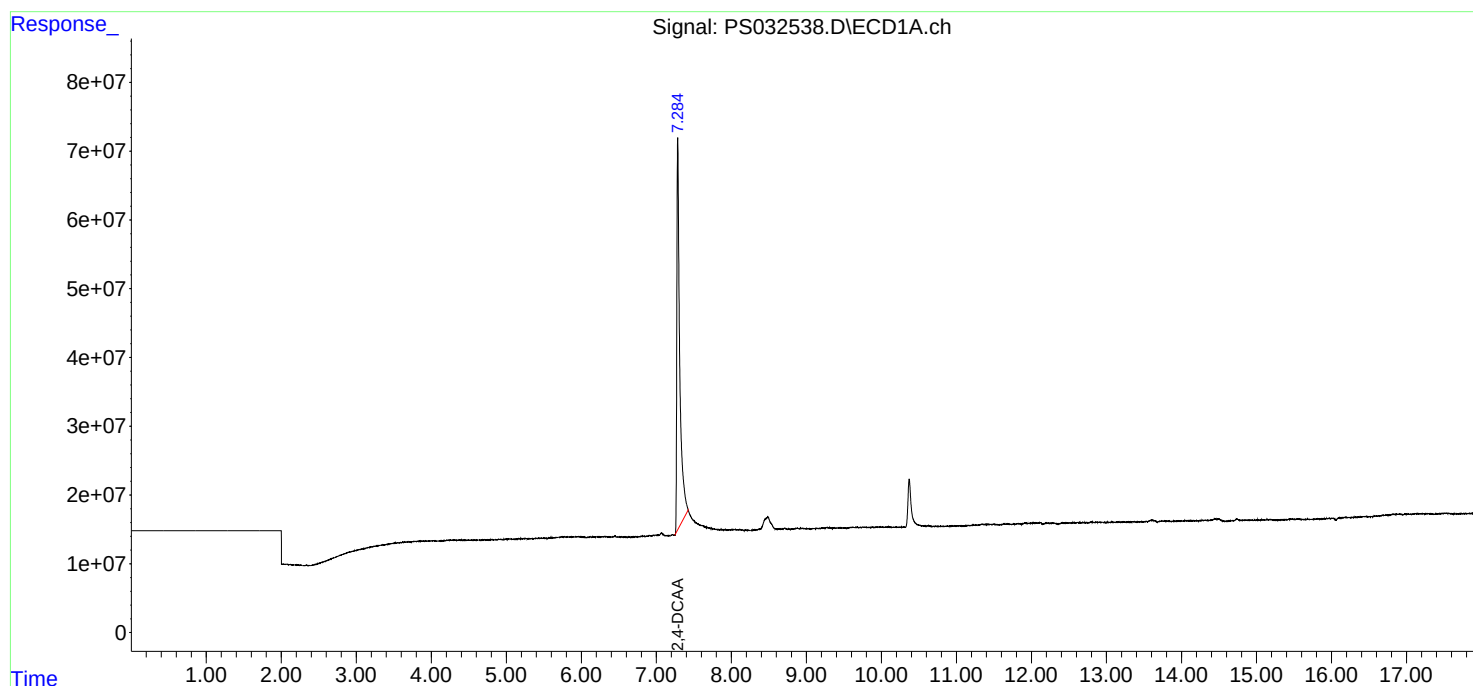


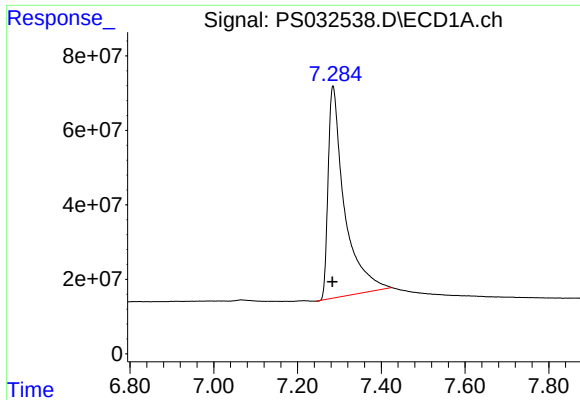

#4 2,4-DCAA

R.T.: 7.285 min
Delta R.T.: 0.001 min
Response: 1542669201
Conc: 340.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

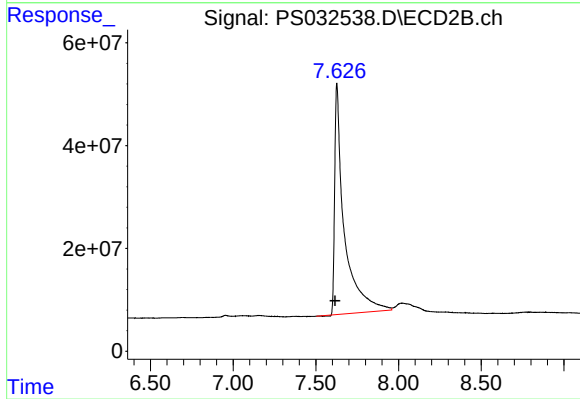

#4 2,4-DCAA

R.T.: 7.628 min
Delta R.T.: 0.011 min
Response: 1812449779
Conc: 497.18 ng/ml