

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112619\
 Data File : PS007828.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Nov 2019 17:29
 Operator : SM\AJ
 Sample : PB125124TB
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB125124TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 26 17:50:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.432	5.156	481.5E6	262.4E6	349.607	373.472
Target Compounds							
1) T	Dalapon	1.992	1.699	184.9E6	204.0E6	102.226	171.764 #
2) T	3,5-DICHL...	0.000	4.490	0	72998485	N.D.	80.801
5) T	DICAMBA	5.521	0.000	34448894	0	6.771	N.D. #
7) T	MCPA	5.896	5.523	25700278	25982346	4.669	8.644 #
9) T	2,4-D	6.482	6.058	75717601	7746781	53.986	9.607 #
10) T	Pentachlo...	0.000	6.444	0	11932394	N.D.	1.219
11) T	2,4,5-TP ...	0.000	6.758	0	73064106	N.D.	18.658
14) T	DINOSEB	0.000	7.945	0	11778537	N.D.	4.052
15) T	Picloram	0.000	8.927	0	18615342	N.D.	3.177



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112619\
Data File : PS007828.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Nov 2019 17:29
Operator : SM\AJ
Sample : PB125124TB
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB125124TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 26 17:50:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

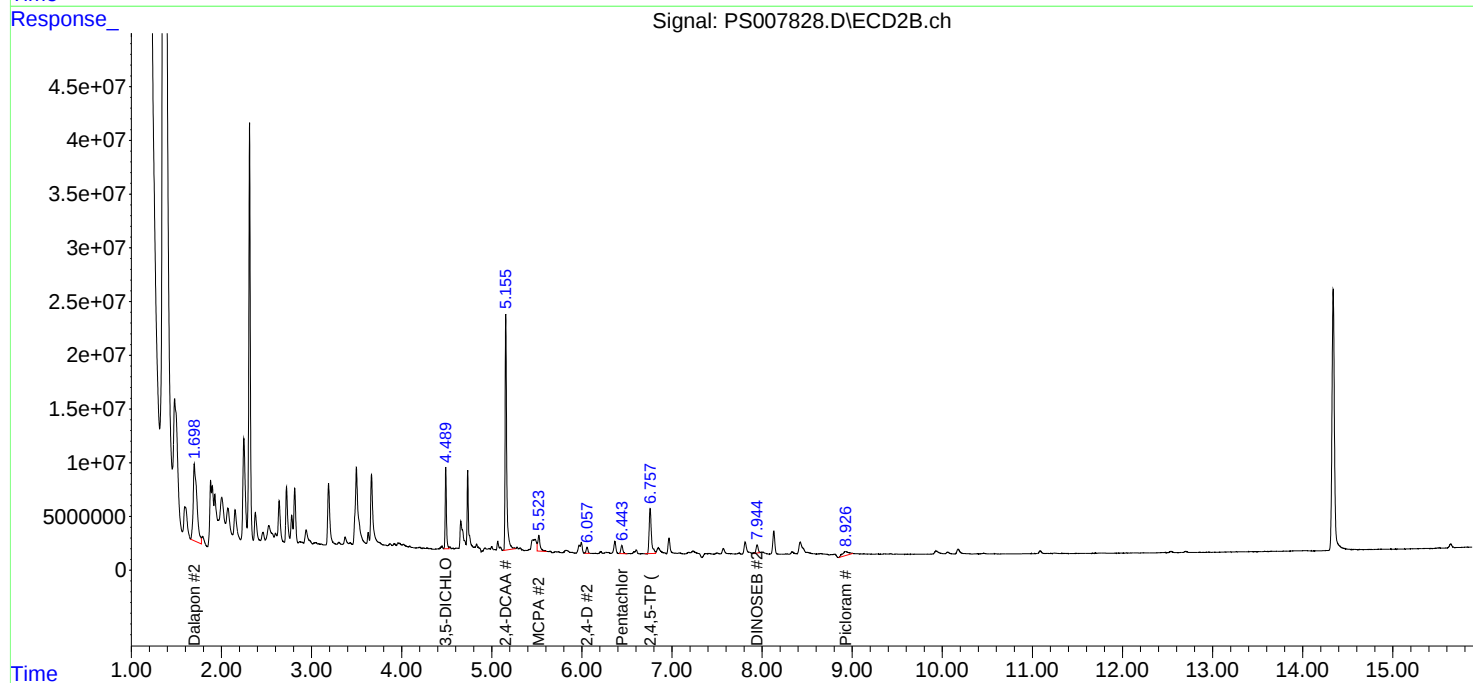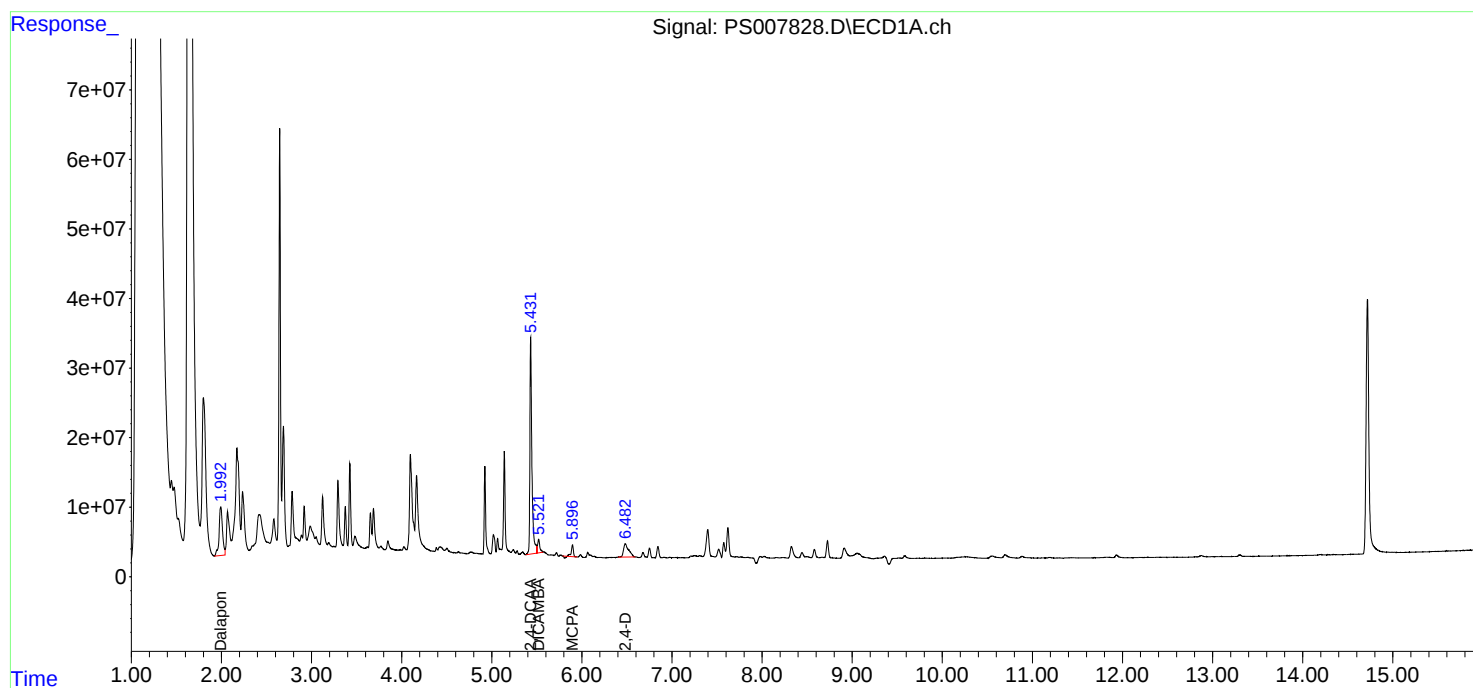


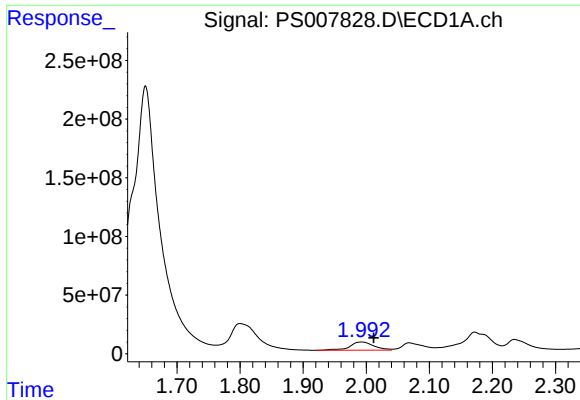

#1 Dalapon


R.T.: 1.992 min
Delta R.T.: -0.020 min
Response: 184945540
Conc: 102.23 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB125124TB

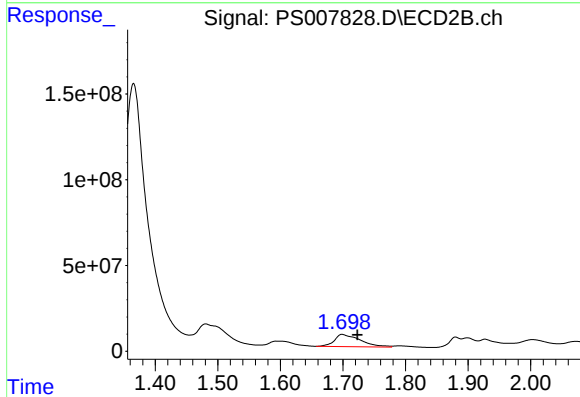


#1 Dalapon

R.T.: 1.699 min
Delta R.T.: -0.024 min
Response: 203952558
Conc: 171.76 ng/ml

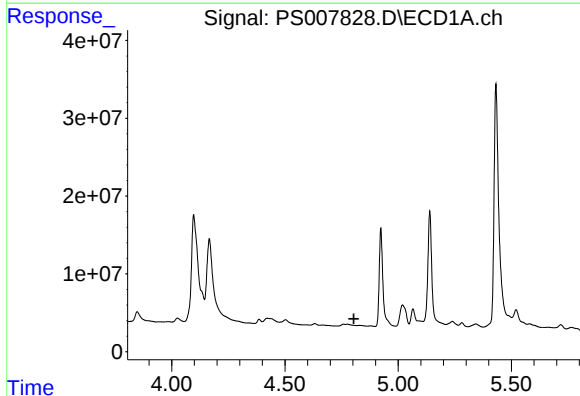


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.804 min
Response: 0
Conc: N.D.

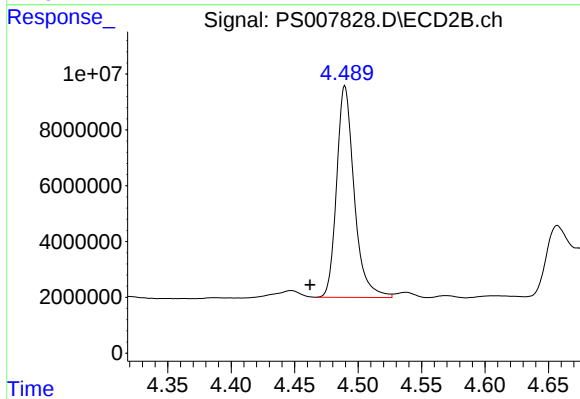

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.490 min
Delta R.T.: 0.028 min
Response: 72998485
Conc: 80.80 ng/ml

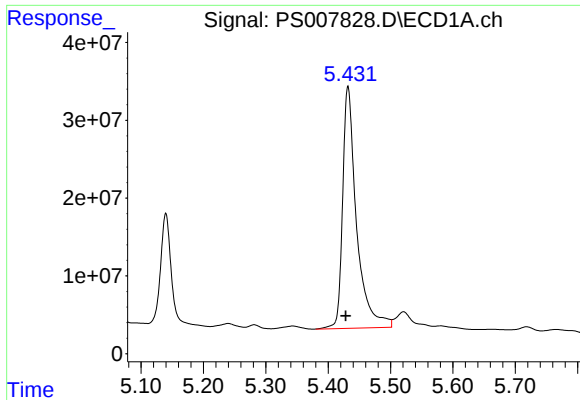

#4 2,4-DCAA


R.T.: 5.432 min
Delta R.T.: 0.004 min
Response: 481472715
Conc: 349.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB125124TB

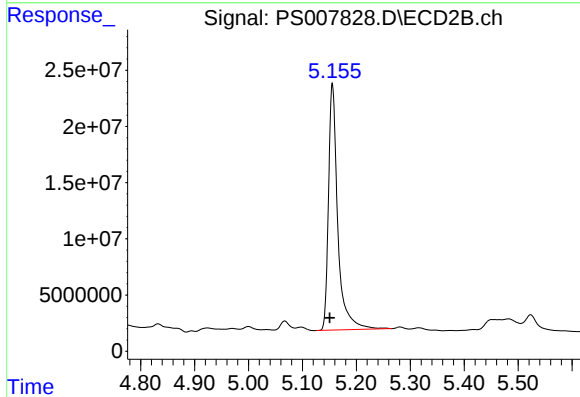


#4 2,4-DCAA

R.T.: 5.156 min
Delta R.T.: 0.005 min
Response: 262387955
Conc: 373.47 ng/ml

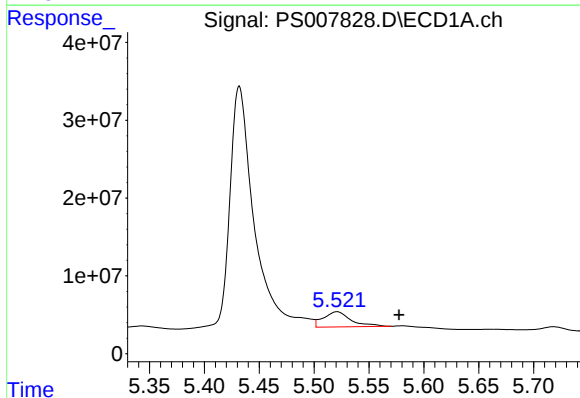


#5 DICAMBA

R.T.: 5.521 min
Delta R.T.: -0.057 min
Response: 34448894
Conc: 6.77 ng/ml

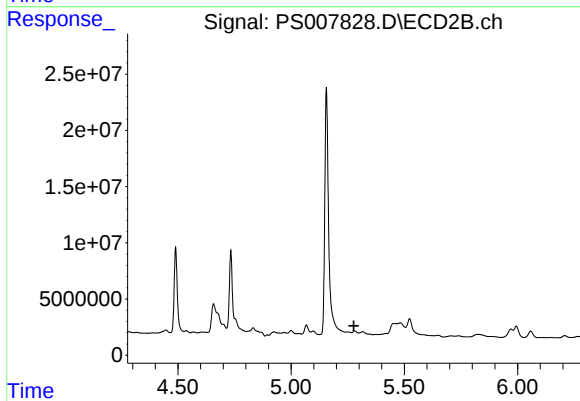

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.277 min
Response: 0
Conc: N.D.

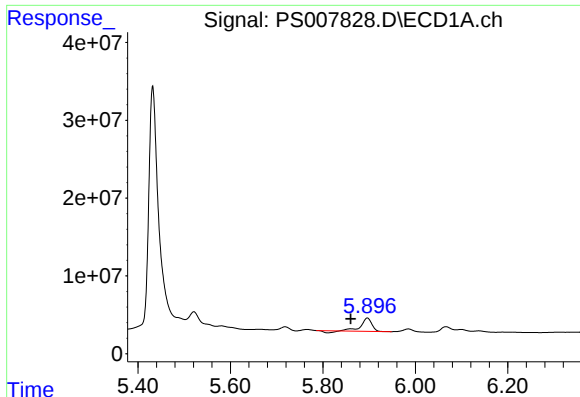

#7 MCPA


R.T.: 5.896 min
Delta R.T.: 0.036 min
Response: 25700278
Conc: 4.67 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB125124TB

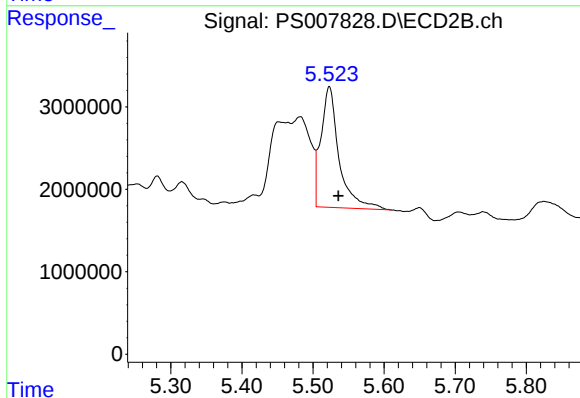


#7 MCPA

R.T.: 5.523 min
Delta R.T.: -0.013 min
Response: 25982346
Conc: 8.64 ug/ml

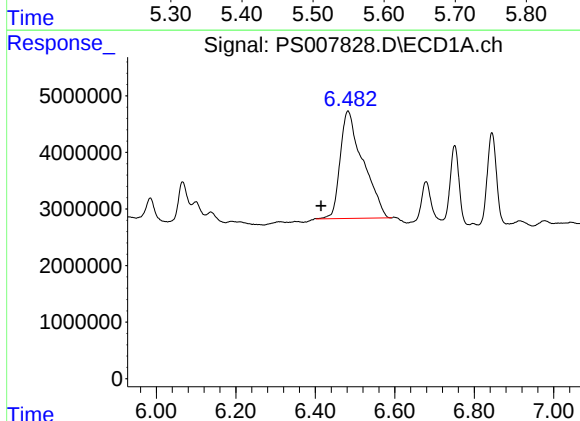


#9 2,4-D

R.T.: 6.482 min
Delta R.T.: 0.068 min
Response: 75717601
Conc: 53.99 ng/ml

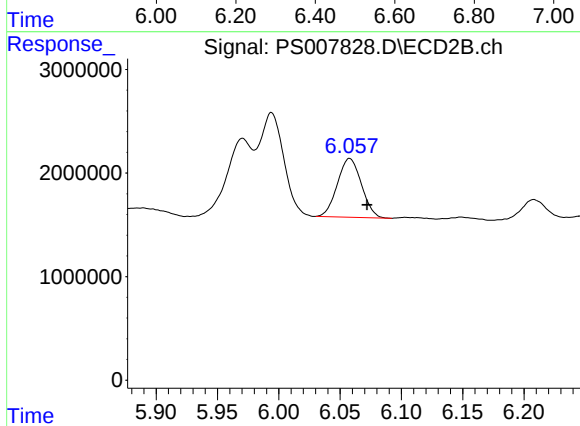

#9 2,4-D


R.T.: 6.058 min
Delta R.T.: -0.014 min
Response: 7746781
Conc: 9.61 ng/ml

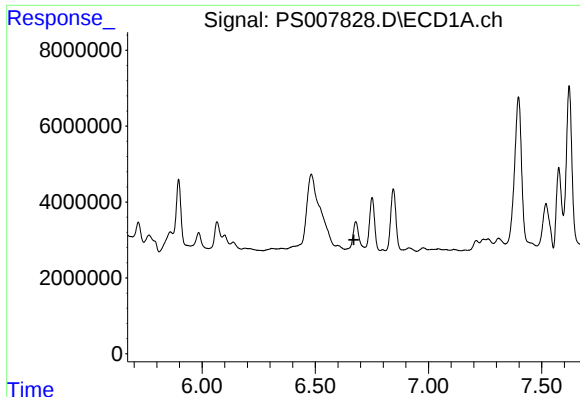

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.671 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB125124TB

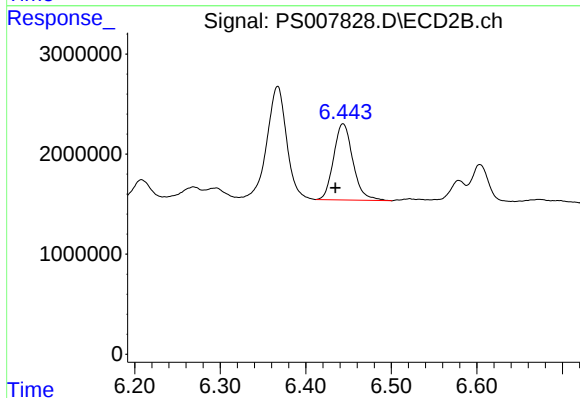


#10 Pentachlorophenol

R.T.: 6.444 min
Delta R.T.: 0.009 min
Response: 11932394
Conc: 1.22 ng/ml

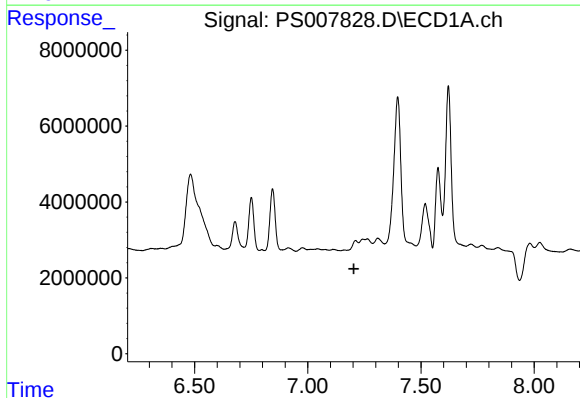


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.203 min
Response: 0
Conc: N.D.

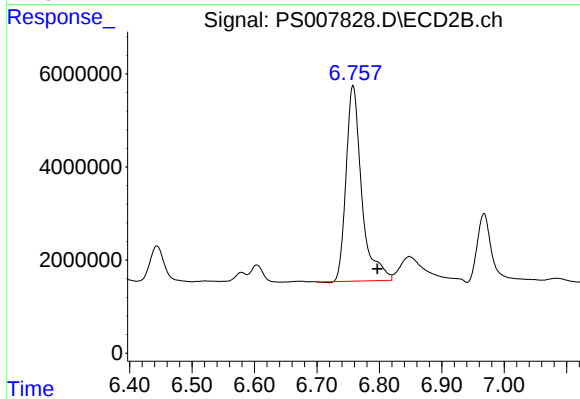

#11 2,4,5-TP (SILVEX)


R.T.: 6.758 min
Delta R.T.: -0.039 min
Response: 73064106
Conc: 18.66 ng/ml

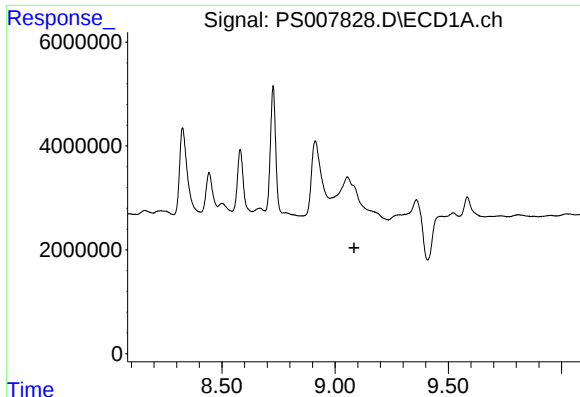

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.083 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB125124TB

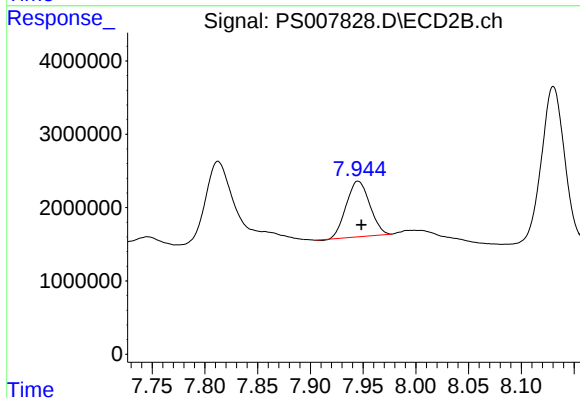


#14 DINOSEB

R.T.: 7.945 min
Delta R.T.: -0.003 min
Response: 11778537
Conc: 4.05 ng/ml

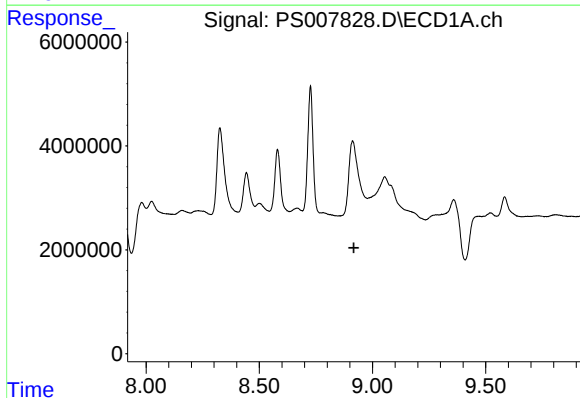

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.918 min
Response: 0
Conc: N.D.

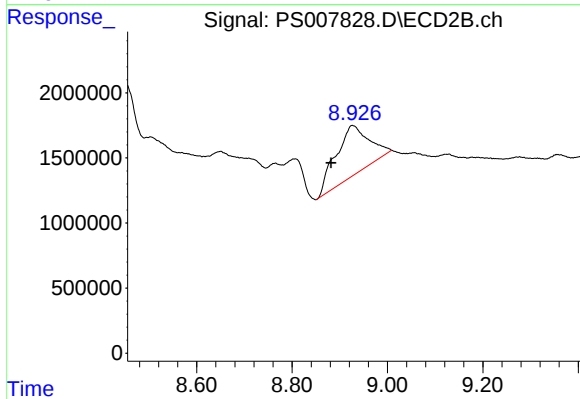

#15 Picloram

R.T.: 8.927 min
Delta R.T.: 0.045 min
Response: 18615342
Conc: 3.18 ng/ml