

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112619\
 Data File : PS007833.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Nov 2019 19:18
 Operator : SM\AJ
 Sample : K5676-34
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SU-04-112219

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 05:51:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.447	5.171	324.3E6	170.4E6	235.495	242.589
Target Compounds							
1) T	Dalapon	2.009	1.715	311.5E6	476.6E6	172.188	401.353 #
2) T	3,5-DICHL...	0.000	4.462	0	6271291	N.D.	6.942
5) T	DICAMBA	5.536	0.000	33928248	0	6.669	N.D. #
9) T	2,4-D	0.000	6.073	0	5788156	N.D.	7.178
10) T	Pentachlo...	0.000	6.382	0	14319475	N.D.	1.462
11) T	2,4,5-TP ...	0.000	6.771	0	82297658	N.D.	21.016
12) T	2,4,5-T	7.532	0.000	32136364	0	3.926	N.D. #
13) T	2,4-DB	0.000	7.582	0	8513051	N.D.	17.414
15) T	Picloram	8.908	0.000	115.8E6	0	10.431	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112619\
Data File : PS007833.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Nov 2019 19:18
Operator : SM\AJ
Sample : K5676-34
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
SU-04-112219

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 05:51:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

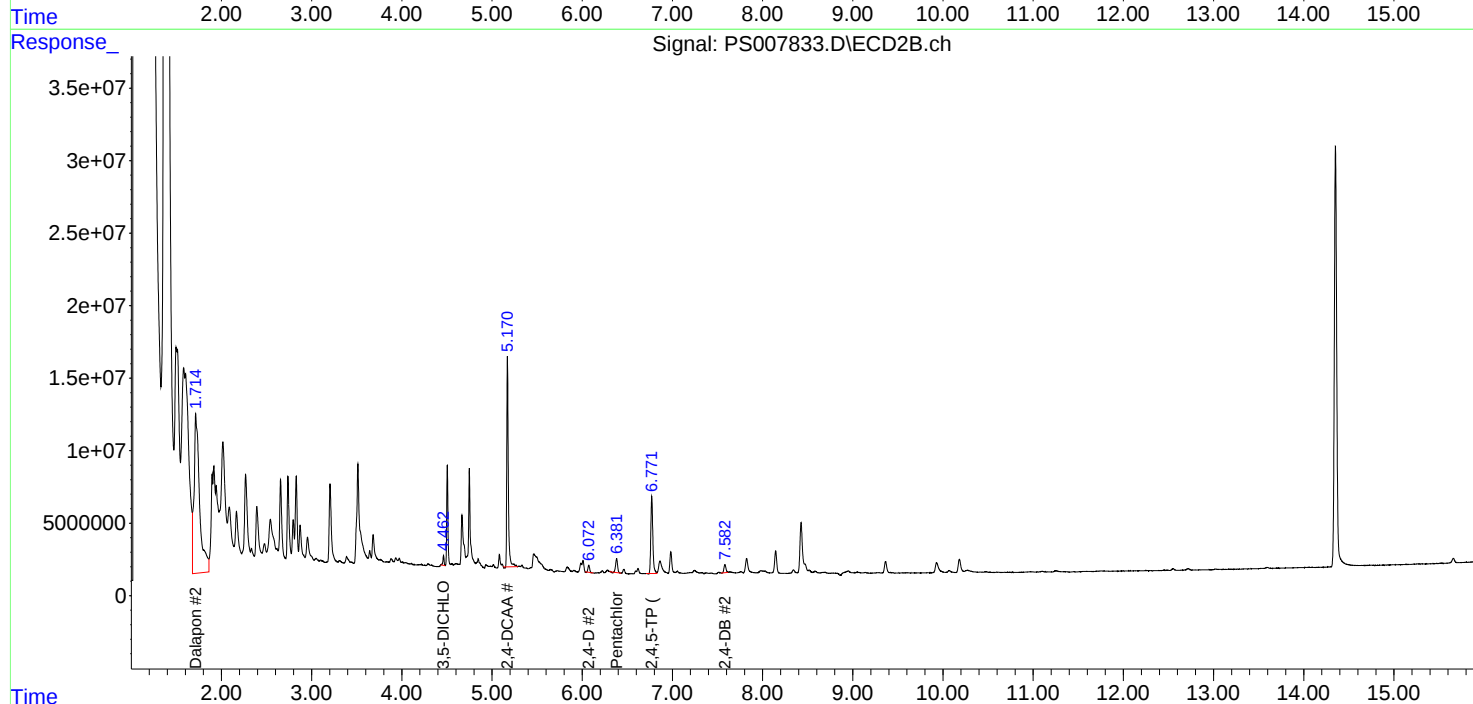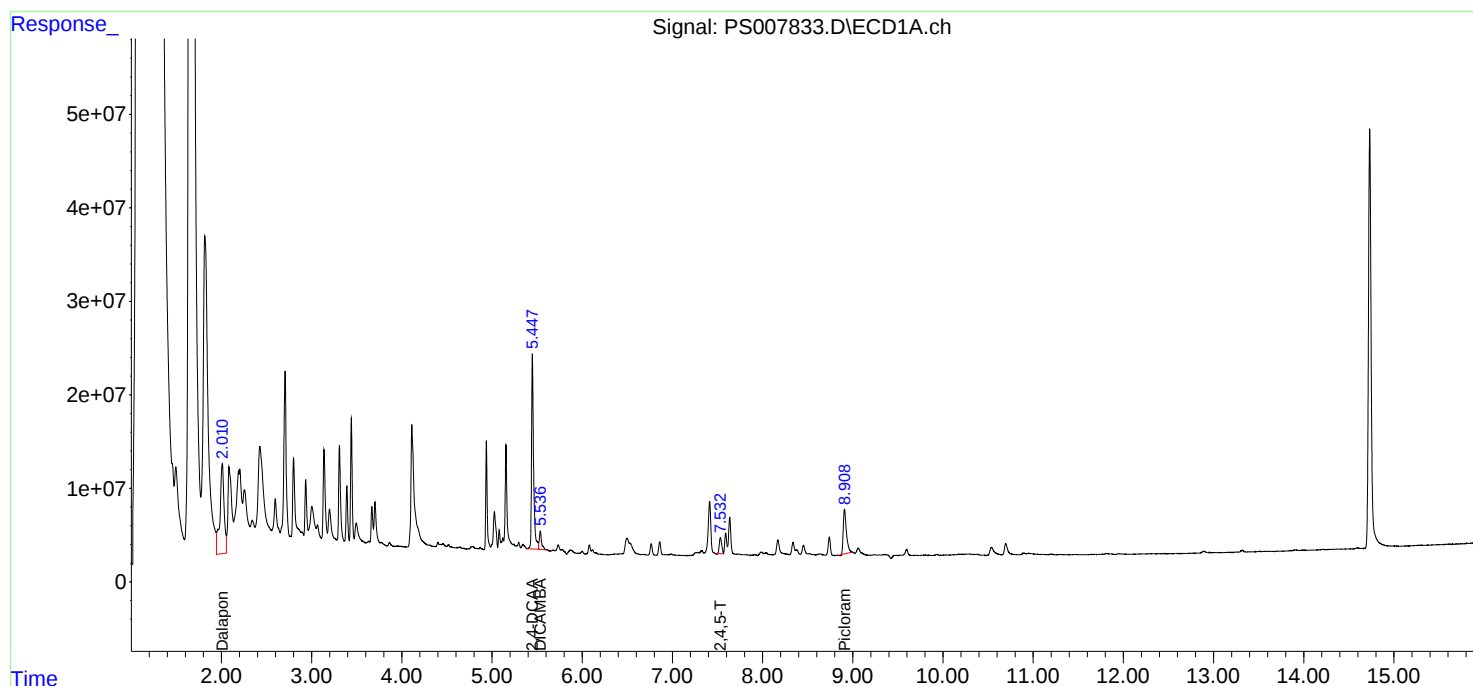


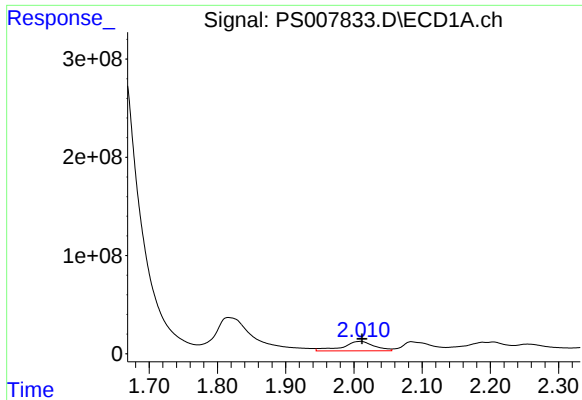

#1 Dalapon


R.T.: 2.009 min
Delta R.T.: -0.003 min
Response: 311519172
Conc: 172.19 ng/ml

Instrument :
ECD_S
ClientSampleId :
SU-04-112219

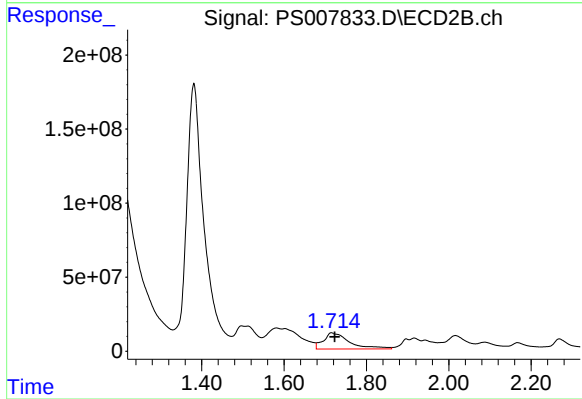


#1 Dalapon

R.T.: 1.715 min
Delta R.T.: -0.008 min
Response: 476568110
Conc: 401.35 ng/ml

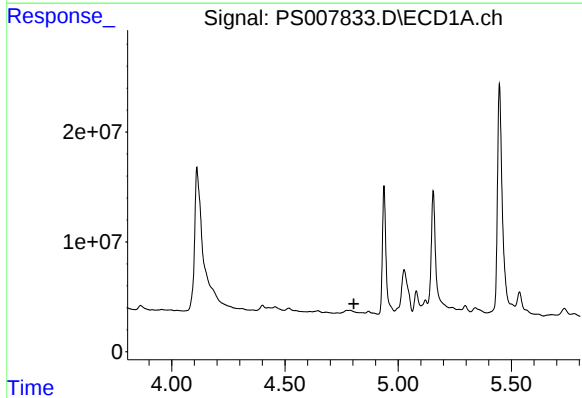


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.804 min
Response: 0
Conc: N.D.

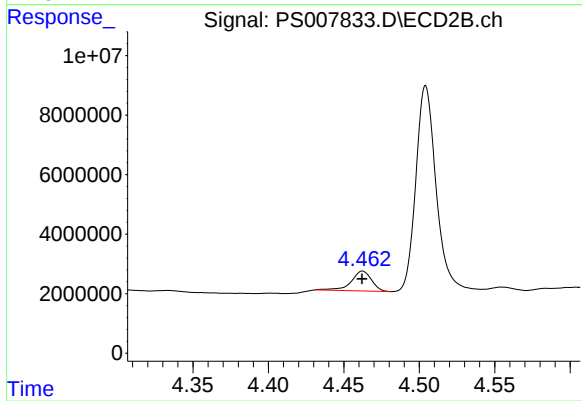

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.462 min
Delta R.T.: 0.000 min
Response: 6271291
Conc: 6.94 ng/ml

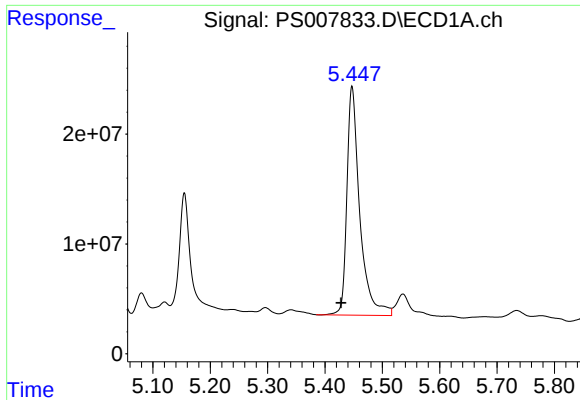

#4 2,4-DCAA


R.T.: 5.447 min
Delta R.T.: 0.019 min
Response: 324319822
Conc: 235.49 ng/ml

Instrument :
ECD_S
ClientSampleId :
SU-04-112219

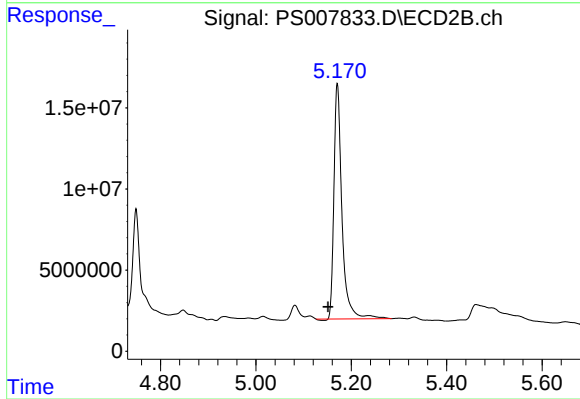


#4 2,4-DCAA

R.T.: 5.171 min
Delta R.T.: 0.020 min
Response: 170434614
Conc: 242.59 ng/ml

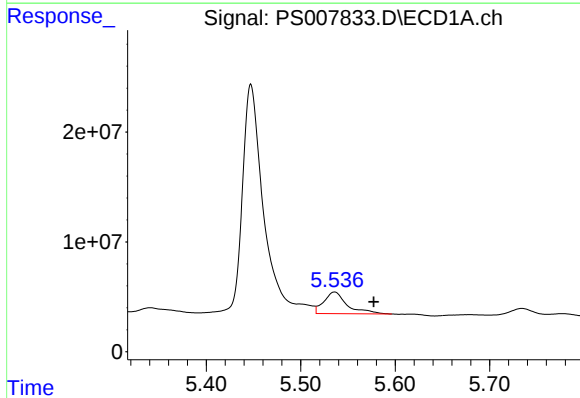


#5 DICAMBA

R.T.: 5.536 min
Delta R.T.: -0.042 min
Response: 33928248
Conc: 6.67 ng/ml

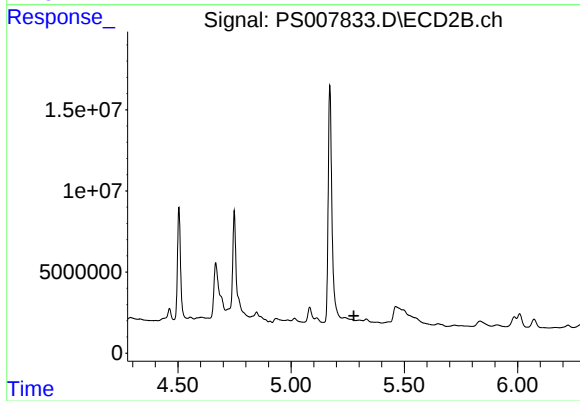

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.277 min
Response: 0
Conc: N.D.

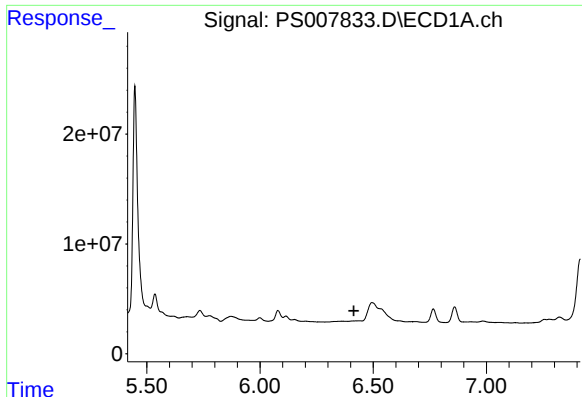

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.414 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SU-04-112219

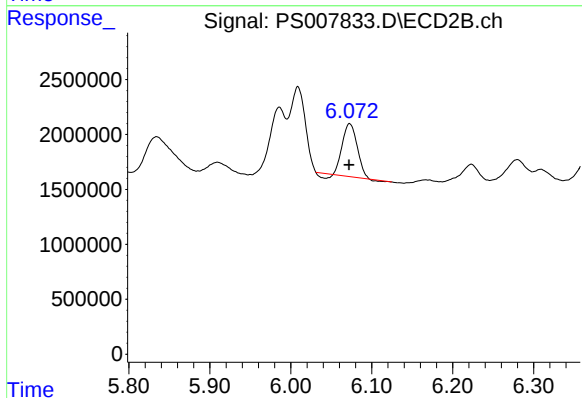


#9 2,4-D

R.T.: 6.073 min
Delta R.T.: 0.000 min
Response: 5788156
Conc: 7.18 ng/ml

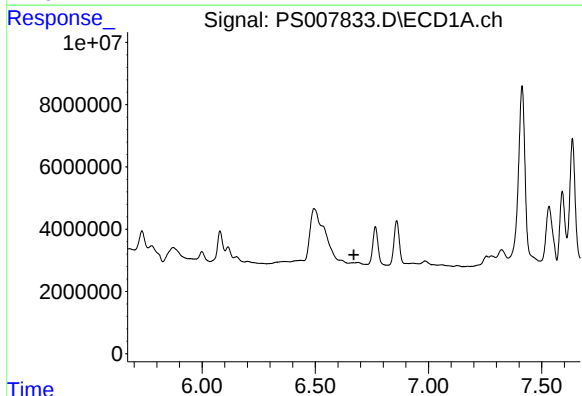


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.671 min
Response: 0
Conc: N.D.

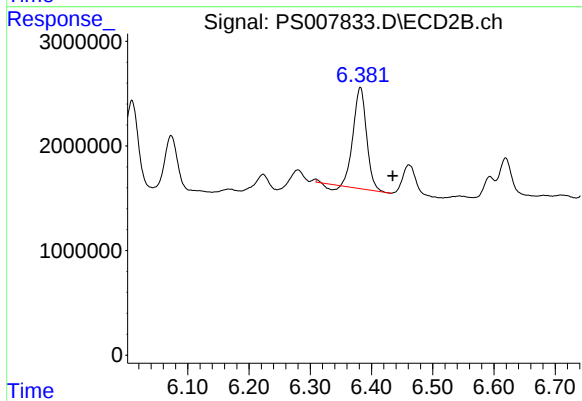

#10 Pentachlorophenol


R.T.: 6.382 min
Delta R.T.: -0.053 min
Response: 14319475
Conc: 1.46 ng/ml

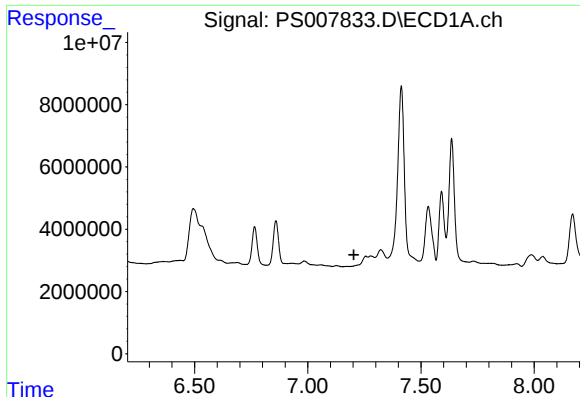

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.203 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SU-04-112219

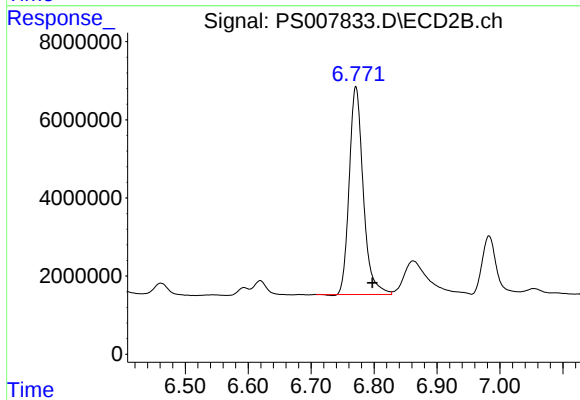


#11 2,4,5-TP (SILVEX)

R.T.: 6.771 min
Delta R.T.: -0.026 min
Response: 82297658
Conc: 21.02 ng/ml

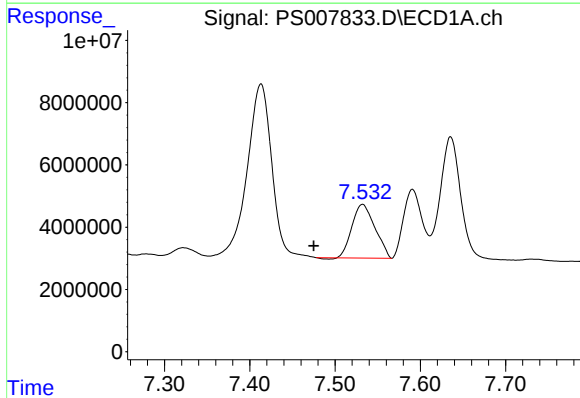


#12 2,4,5-T

R.T.: 7.532 min
Delta R.T.: 0.057 min
Response: 32136364
Conc: 3.93 ng/ml

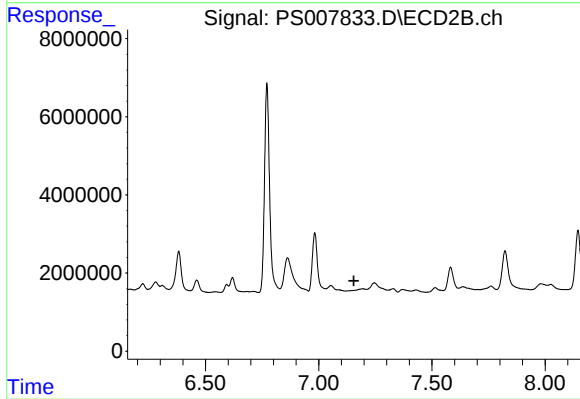

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.156 min
Response: 0
Conc: N.D.

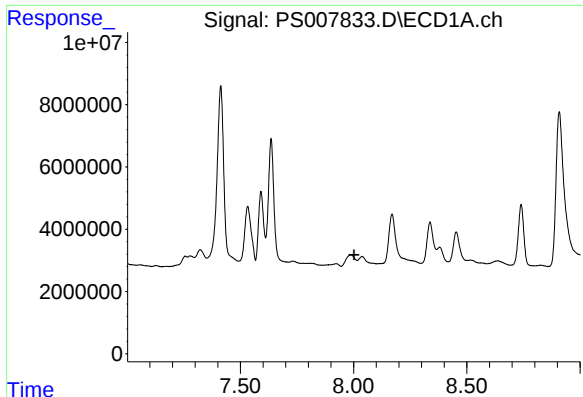

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 8.002 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SU-04-112219

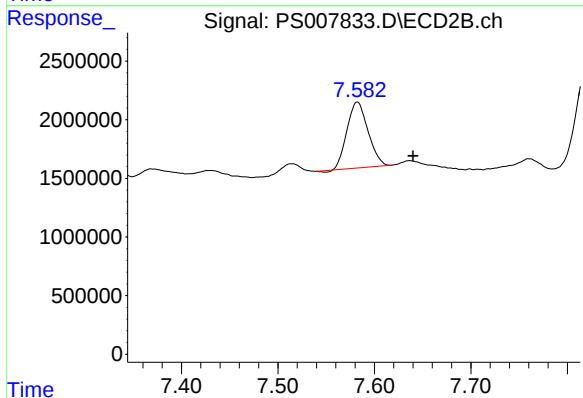


#13 2,4-DB

R.T.: 7.582 min
Delta R.T.: -0.058 min
Response: 8513051
Conc: 17.41 ng/ml

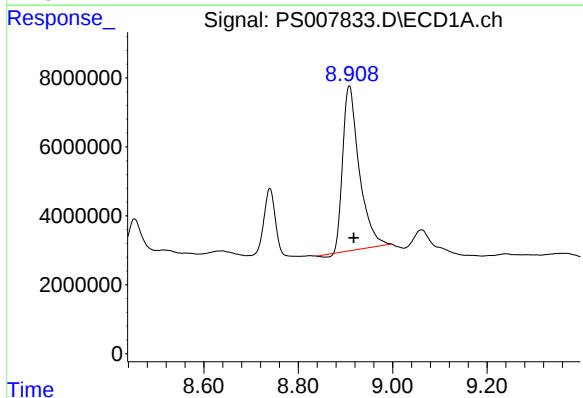

#15 Picloram

R.T.: 8.908 min
Delta R.T.: -0.010 min
Response: 115817651
Conc: 10.43 ng/ml

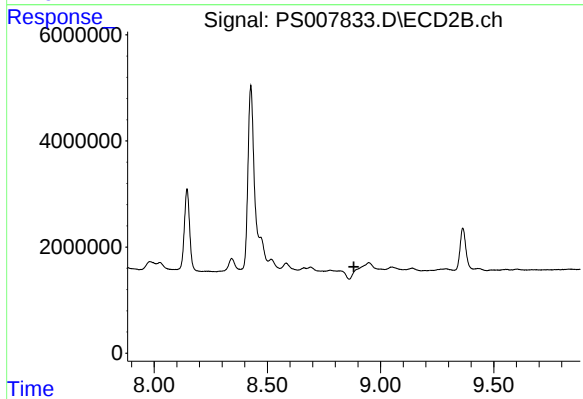

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.882 min
Response: 0
Conc: N.D.