

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112619\
 Data File : PS007836.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Nov 2019 20:24
 Operator : SM\AJ
 Sample : PB125125BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB125125BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 05:52:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.448	5.171	482.4E6	264.7E6	350.279	376.831
Target Compounds							
1) T	Dalapon	2.007	1.715	183.6E6	274.1E6	101.459	230.848 #
2) T	3,5-DICHL...	0.000	4.505	0	72559071	N.D.	80.315
5) T	DICAMBA	5.536	0.000	34463090	0	6.774	N.D. #
7) T	MCPA	5.911	5.538	35524590	26292793	6.454	8.748 #
9) T	2,4-D	0.000	6.073	0	5471134	N.D.	6.785
10) T	Pentachlo...	0.000	6.459	0	16309933	N.D.	1.666
11) T	2,4,5-TP ...	0.000	6.774	0	73464180	N.D.	18.761
12) T	2,4,5-T	7.413	0.000	108.0E6	0	13.190	N.D. #
13) T	2,4-DB	0.000	7.586	0	8322342	N.D.	17.024
14) T	DINOSEB	0.000	7.962	0	12961054	N.D.	4.458
15) T	Picloram	0.000	8.928	0	110.5E6	N.D.	18.852



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112619\
Data File : PS007836.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Nov 2019 20:24
Operator : SM\AJ
Sample : PB125125BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB125125BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 05:52:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

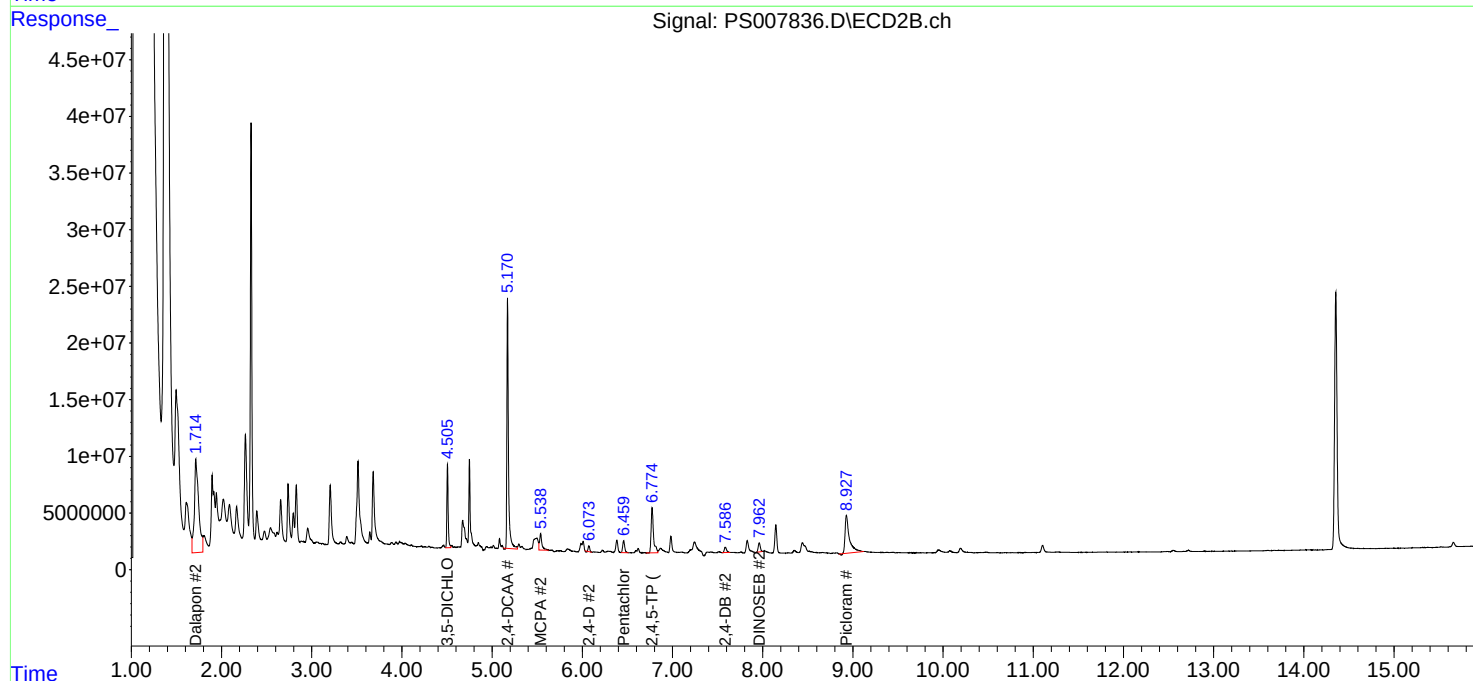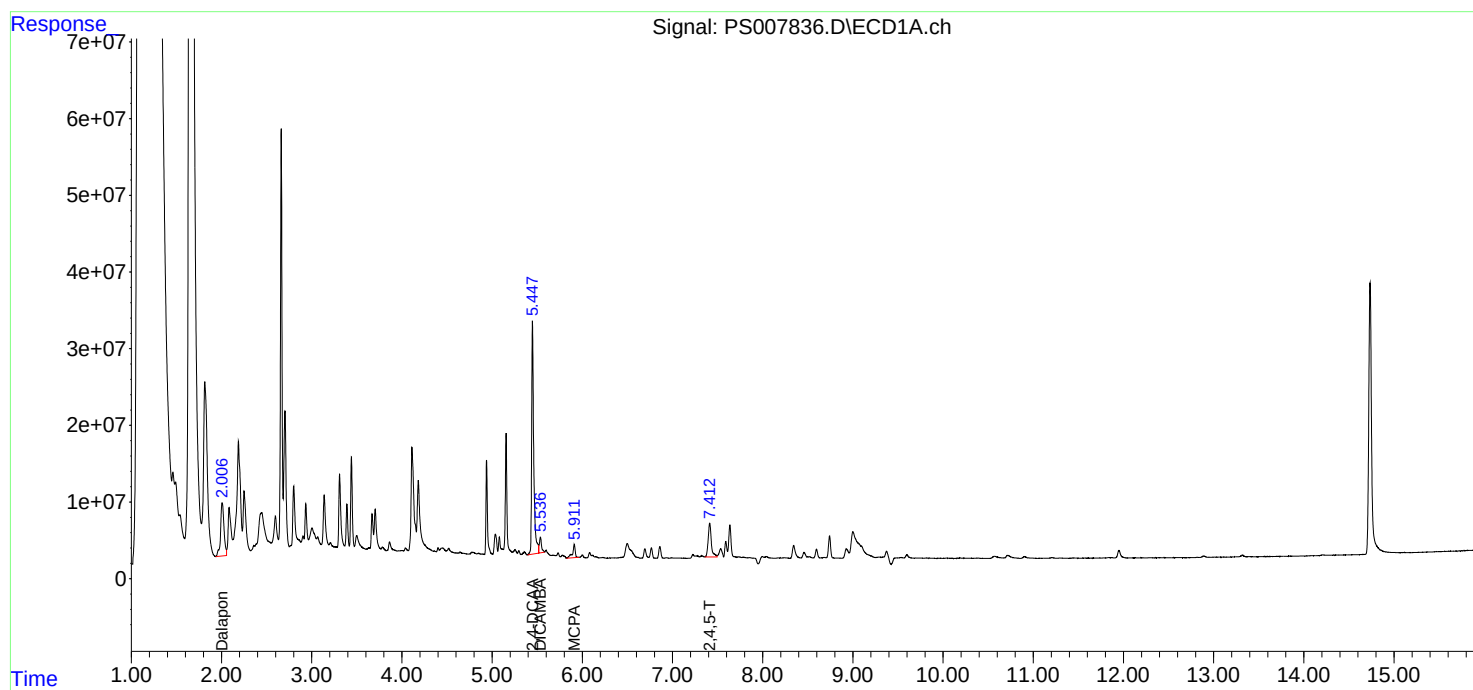


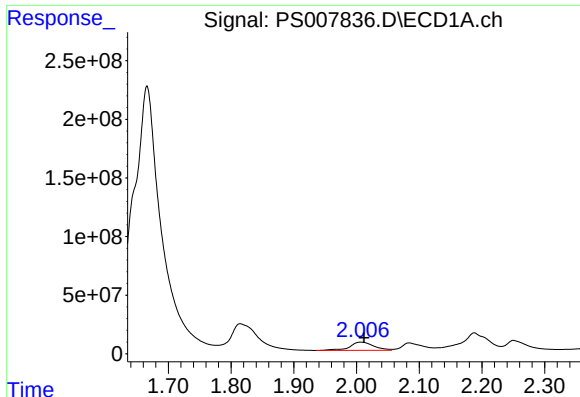

#1 Dalapon


R.T.: 2.007 min
Delta R.T.: -0.005 min
Response: 183557089
Conc: 101.46 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB125125BL

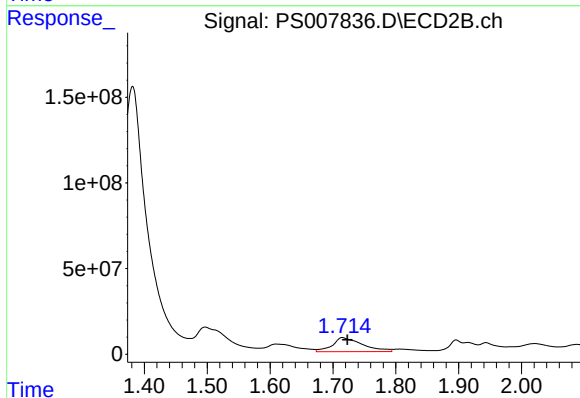


#1 Dalapon

R.T.: 1.715 min
Delta R.T.: -0.008 min
Response: 274110055
Conc: 230.85 ng/ml

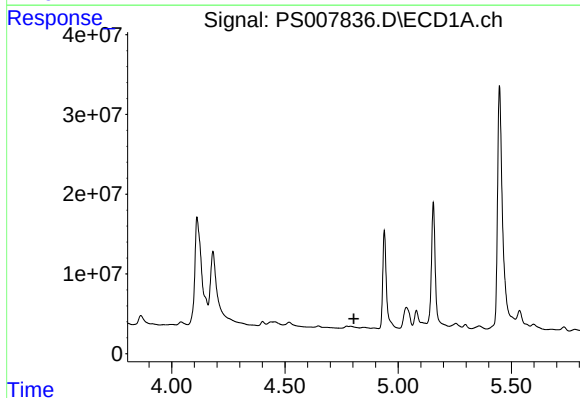


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.804 min
Response: 0
Conc: N.D.

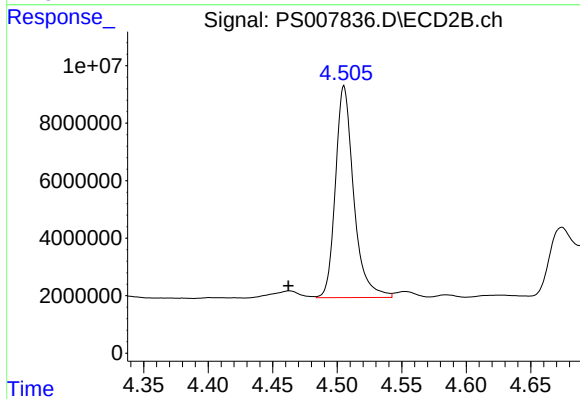

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.505 min
Delta R.T.: 0.043 min
Response: 72559071
Conc: 80.32 ng/ml

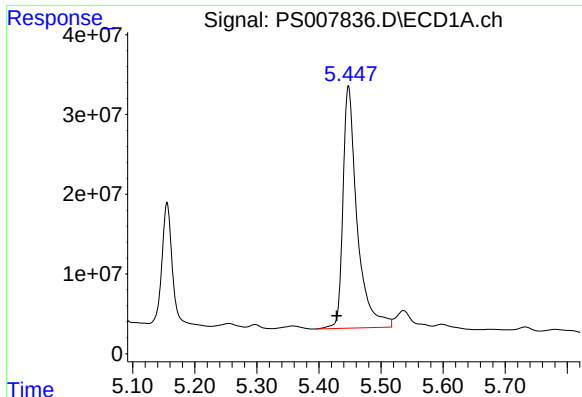

#4 2,4-DCAA


R.T.: 5.448 min
Delta R.T.: 0.019 min
Response: 482398168
Conc: 350.28 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB125125BL

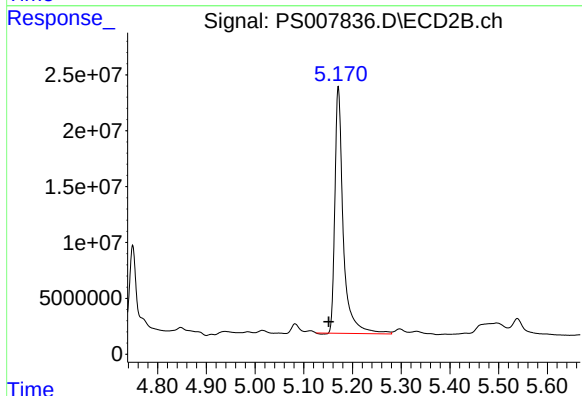


#4 2,4-DCAA

R.T.: 5.171 min
Delta R.T.: 0.020 min
Response: 264747940
Conc: 376.83 ng/ml

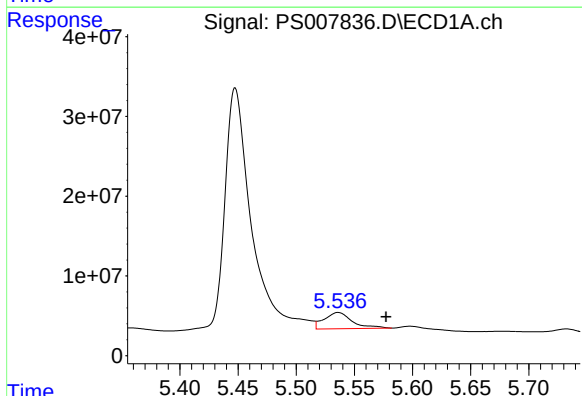


#5 DICAMBA

R.T.: 5.536 min
Delta R.T.: -0.041 min
Response: 34463090
Conc: 6.77 ng/ml

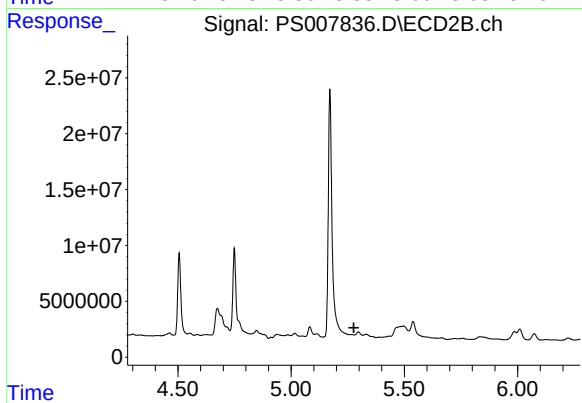

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.277 min
Response: 0
Conc: N.D.

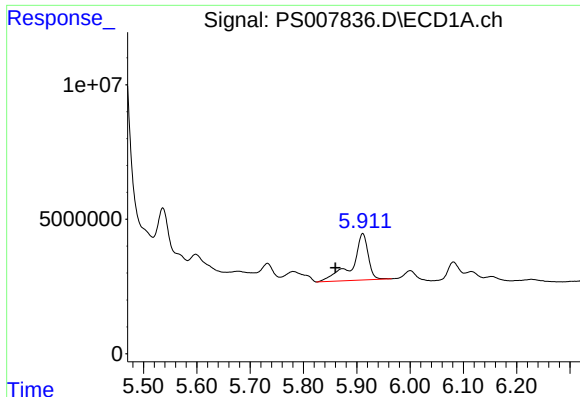

#7 MCPA


R.T.: 5.911 min
Delta R.T.: 0.051 min
Response: 35524590
Conc: 6.45 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB125125BL

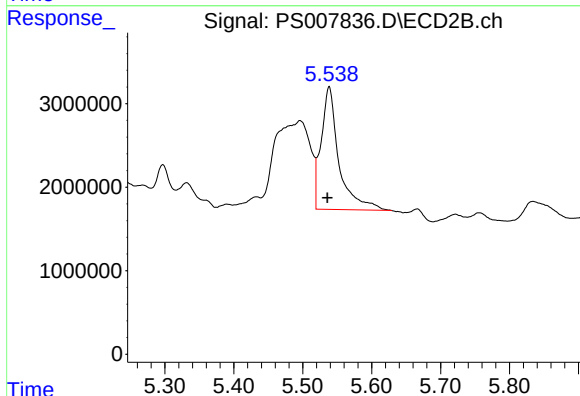


#7 MCPA

R.T.: 5.538 min
Delta R.T.: 0.003 min
Response: 26292793
Conc: 8.75 ug/ml

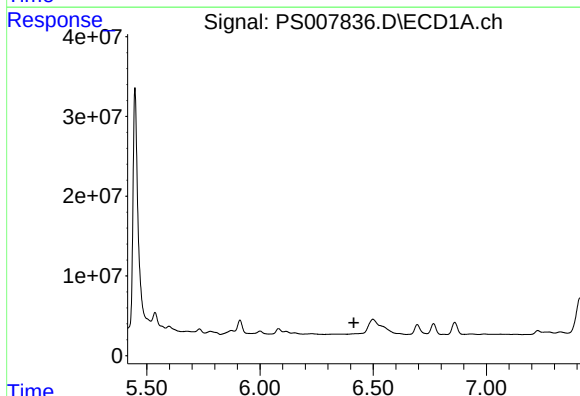


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.414 min
Response: 0
Conc: N.D.

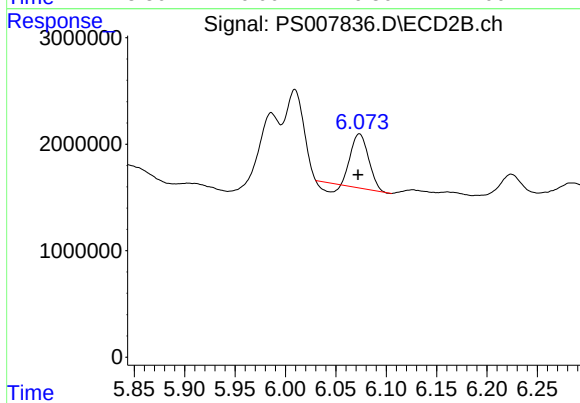

#9 2,4-D


R.T.: 6.073 min
Delta R.T.: 0.001 min
Response: 5471134
Conc: 6.78 ng/ml

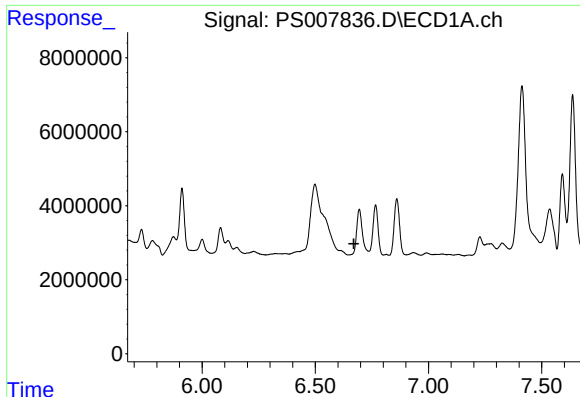

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.671 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB125125BL

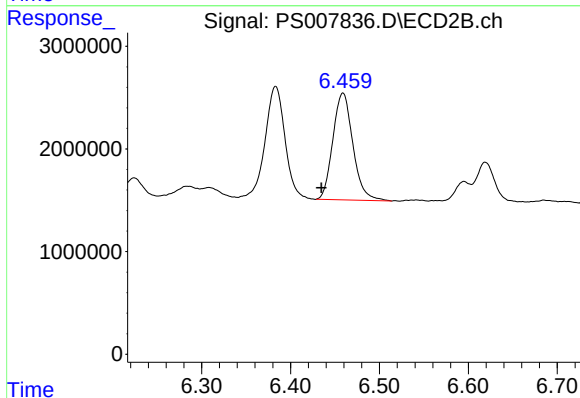


#10 Pentachlorophenol

R.T.: 6.459 min
Delta R.T.: 0.024 min
Response: 16309933
Conc: 1.67 ng/ml

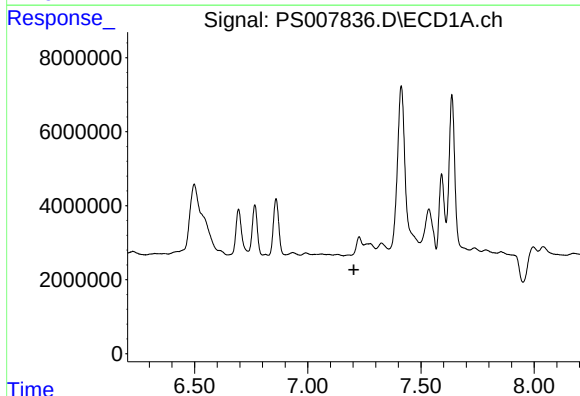


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.203 min
Response: 0
Conc: N.D.

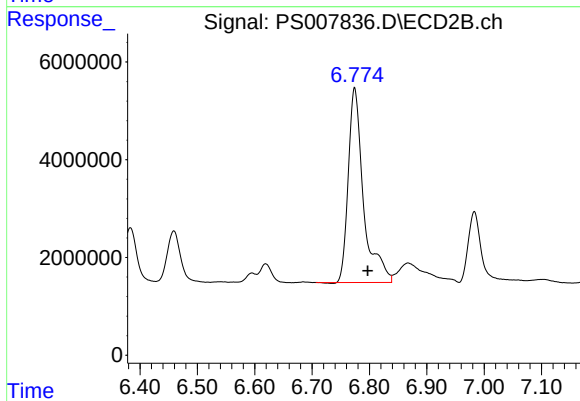

#11 2,4,5-TP (SILVEX)


R.T.: 6.774 min
Delta R.T.: -0.023 min
Response: 73464180
Conc: 18.76 ng/ml

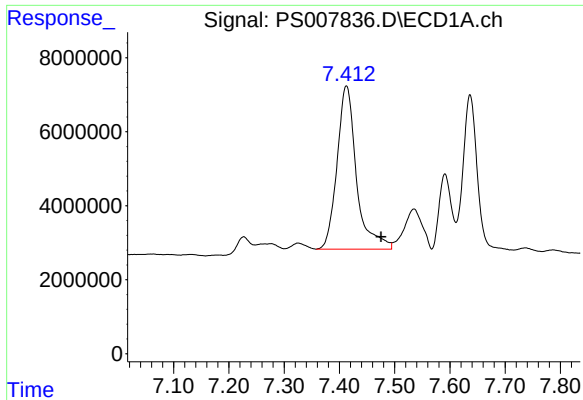

#12 2,4,5-T


R.T.: 7.413 min
Delta R.T.: -0.062 min
Response: 107973363
Conc: 13.19 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB125125BL

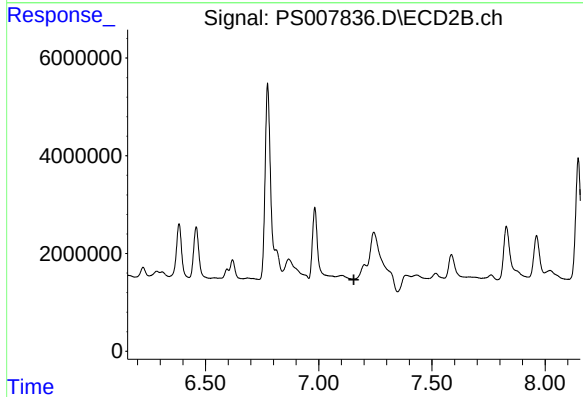


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.156 min
Response: 0
Conc: N.D.

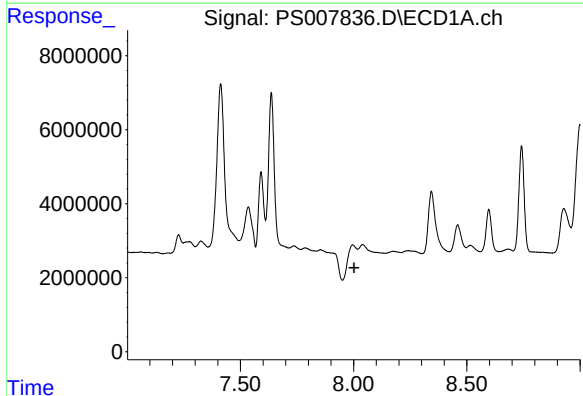


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 8.002 min
Response: 0
Conc: N.D.

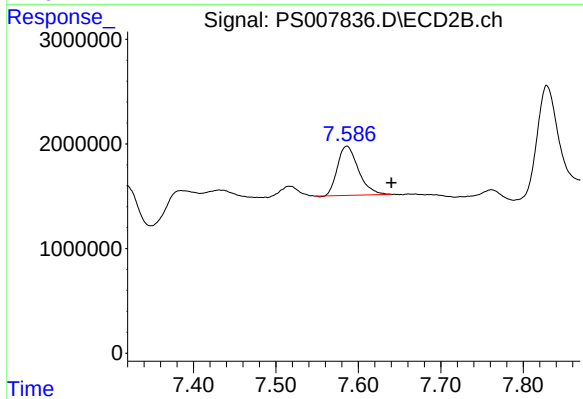

#13 2,4-DB


R.T.: 7.586 min
Delta R.T.: -0.054 min
Response: 8322342
Conc: 17.02 ng/ml

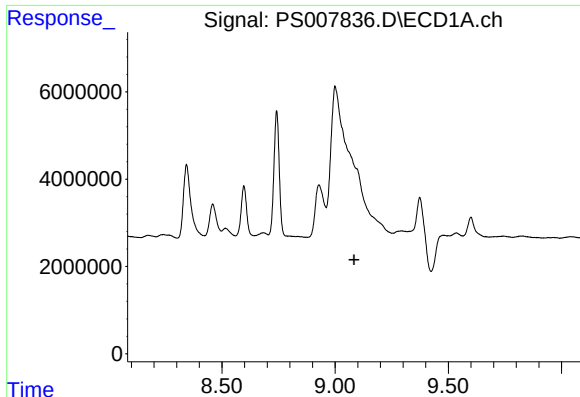

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.083 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB125125BL

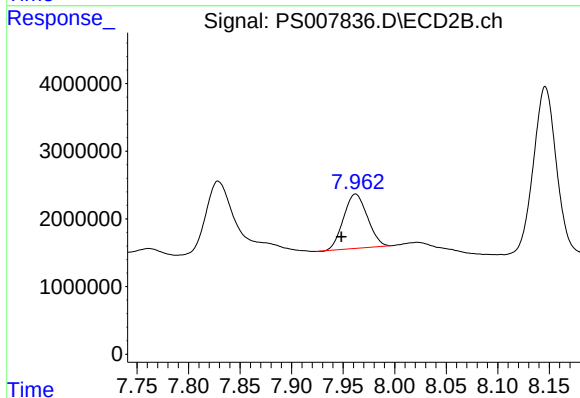


#14 DINOSEB

R.T.: 7.962 min
Delta R.T.: 0.014 min
Response: 12961054
Conc: 4.46 ng/ml

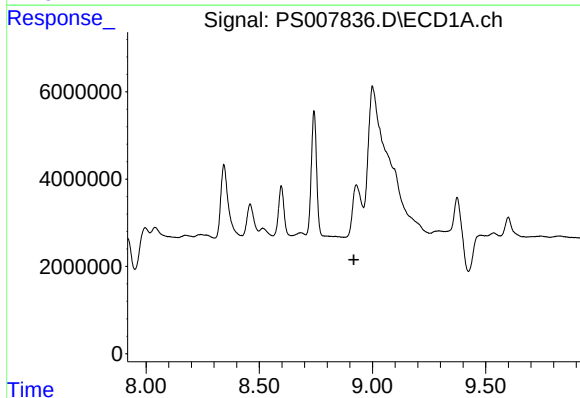

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.918 min
Response: 0
Conc: N.D.

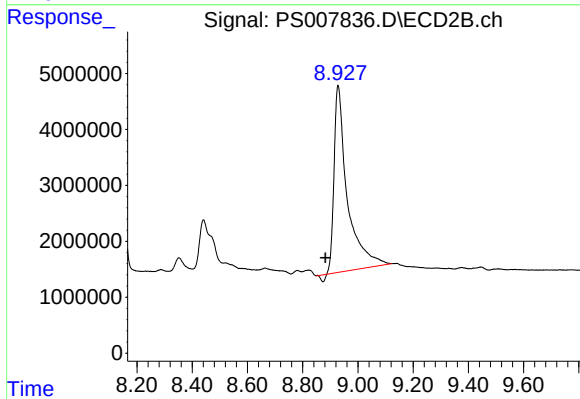

#15 Picloram

R.T.: 8.928 min
Delta R.T.: 0.046 min
Response: 110451605
Conc: 18.85 ng/ml