

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112619\
 Data File : PS007839.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Nov 2019 21:30
 Operator : SM\AJ
 Sample : K5999-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 IDLEWILD-BH-03A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 05:53:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	5.187	0	5915832	N.D.	8.420
Target Compounds							
1) T	Dalapon	2.021	1.726	244.1E6	846.4E6	134.910	712.830 #
2) T	3,5-DICHL...	0.000	4.516	0	48793562	N.D.	54.009
5) T	DICAMBA	5.547	0.000	44551865	0	8.757	N.D. #
7) T	MCPA	5.922	5.550	26138705	24865324	4.749	8.273 #
9) T	2,4-D	0.000	6.085	0	523826	N.D.	<MDL
10) T	Pentachlo...	0.000	6.394	0	25100013	N.D.	2.563
11) T	2,4,5-TP ...	0.000	6.783	0	59195423	N.D.	15.117
12) T	2,4,5-T	7.419	0.000	72601040	0	8.869	N.D. #
13) T	2,4-DB	0.000	7.592	0	12429168	N.D.	25.425
15) T	Picloram	8.920	0.000	73323176	0	6.604	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112619\
Data File : PS007839.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Nov 2019 21:30
Operator : SM\AJ
Sample : K5999-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
IDLEWILD-BH-03A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 05:53:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

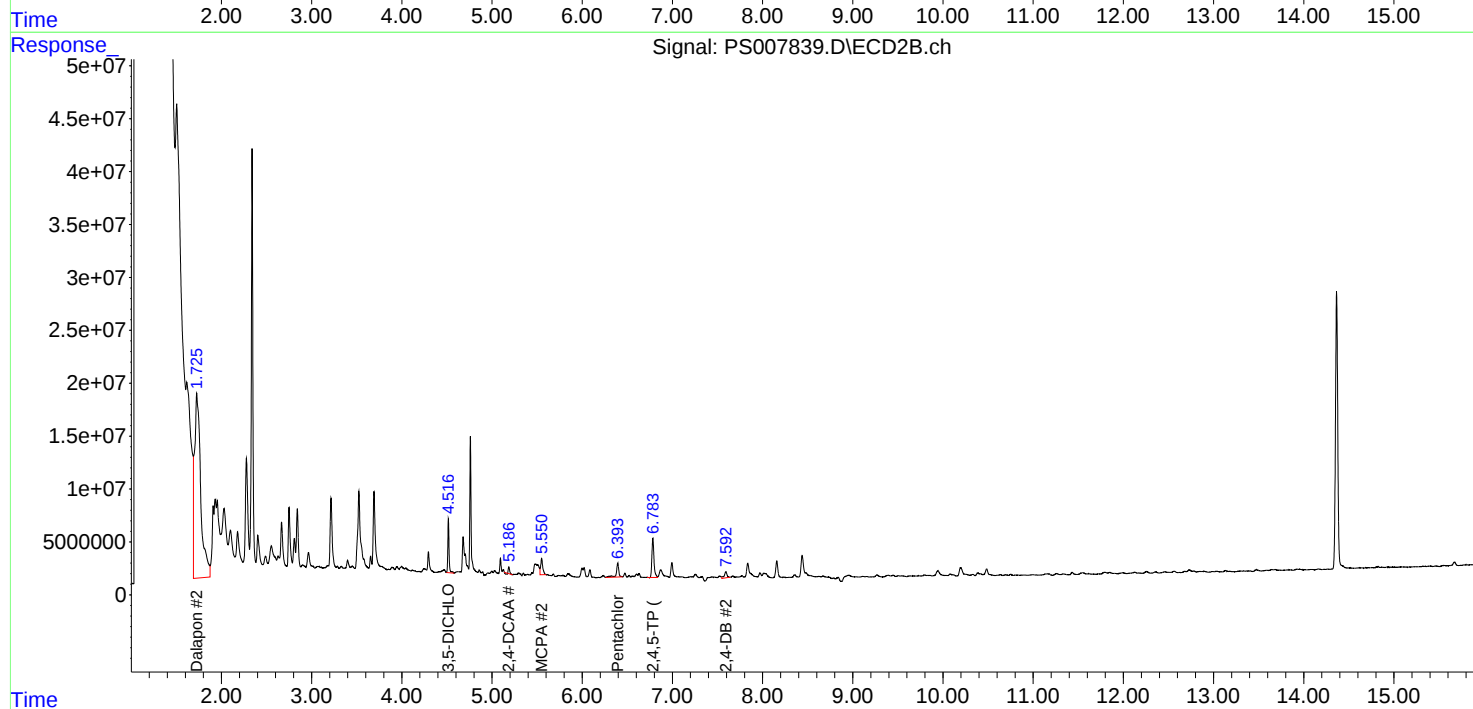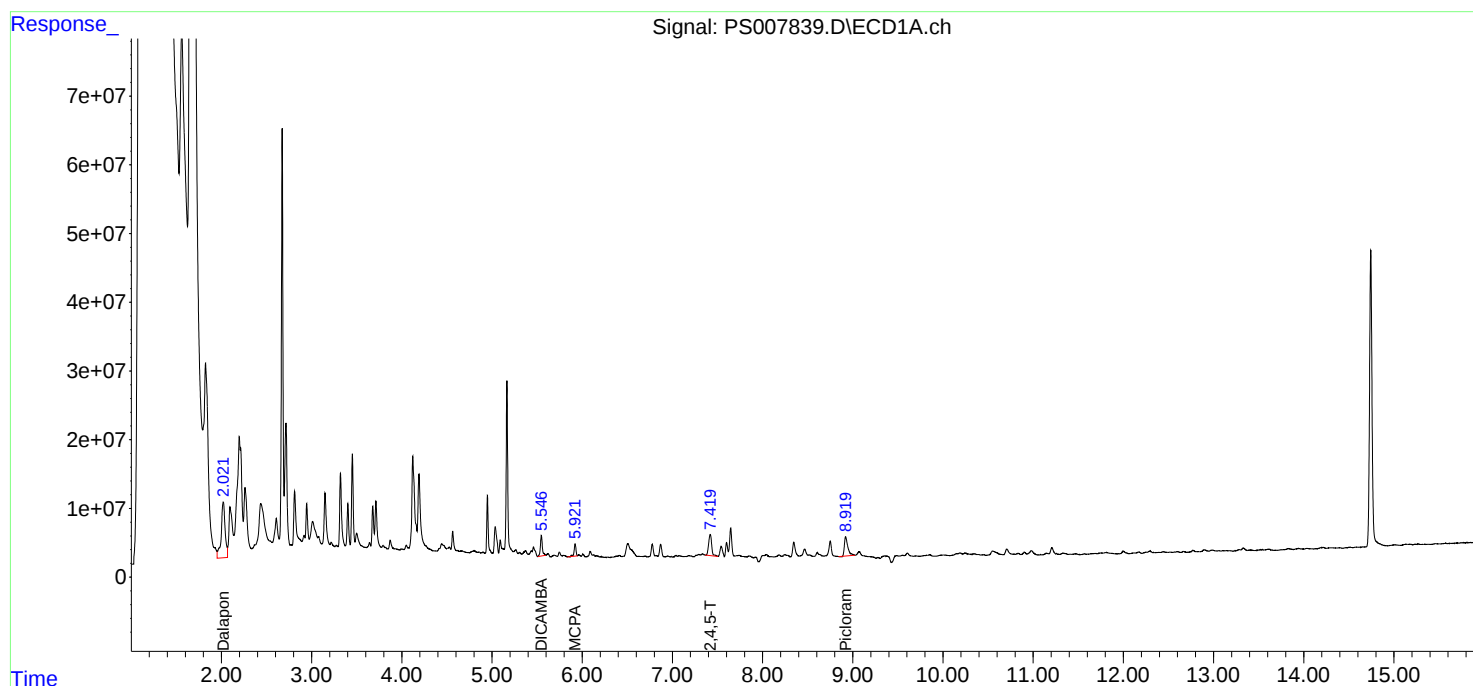


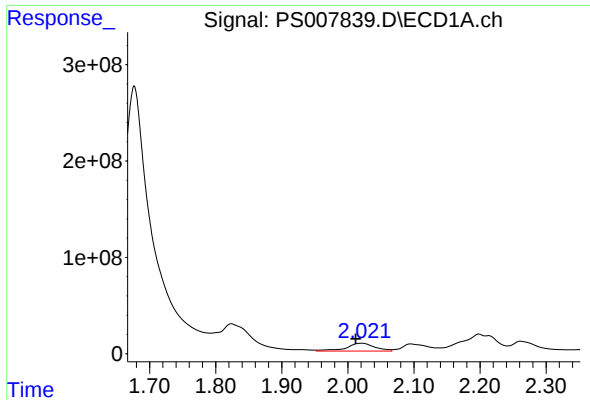

#1 Dalapon


R.T.: 2.021 min
Delta R.T.: 0.009 min
Response: 244076366
Conc: 134.91 ng/ml

Instrument :
ECD_S
ClientSampleId :
IDLEWILD-BH-03A

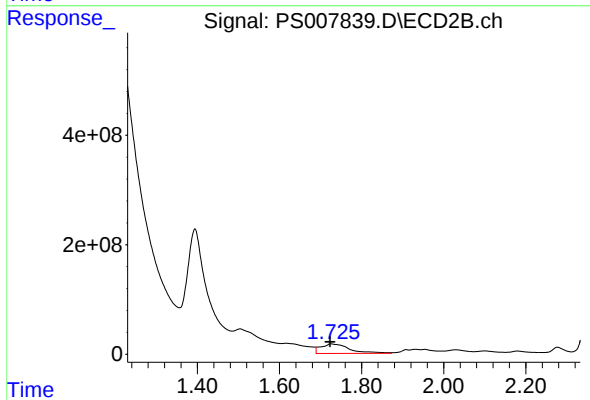


#1 Dalapon

R.T.: 1.726 min
Delta R.T.: 0.003 min
Response: 846415688
Conc: 712.83 ng/ml

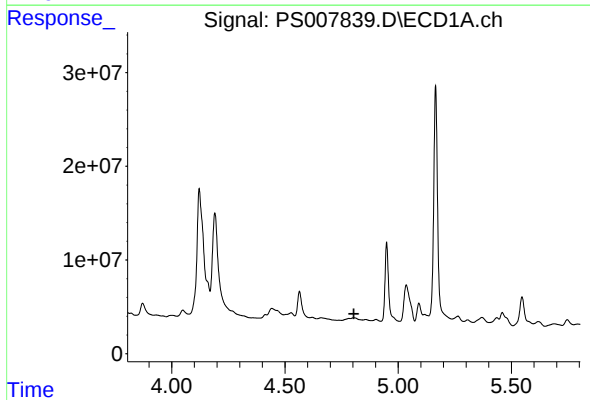


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.804 min
Response: 0
Conc: N.D.

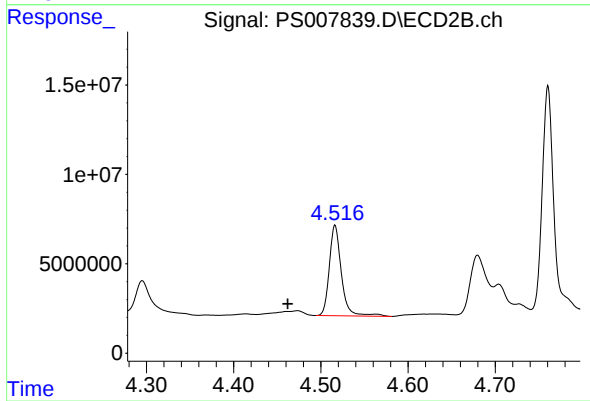

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.516 min
Delta R.T.: 0.054 min
Response: 48793562
Conc: 54.01 ng/ml

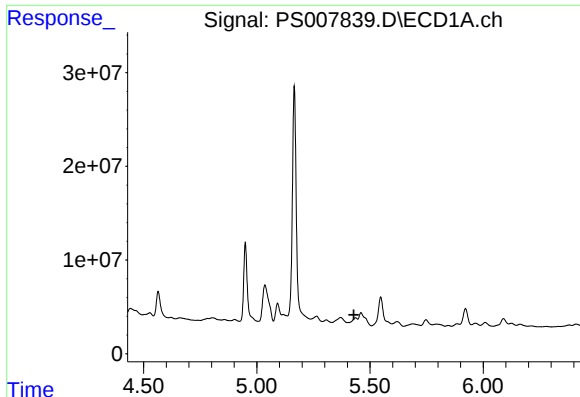

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 5.428 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
IDLEWILD-BH-03A

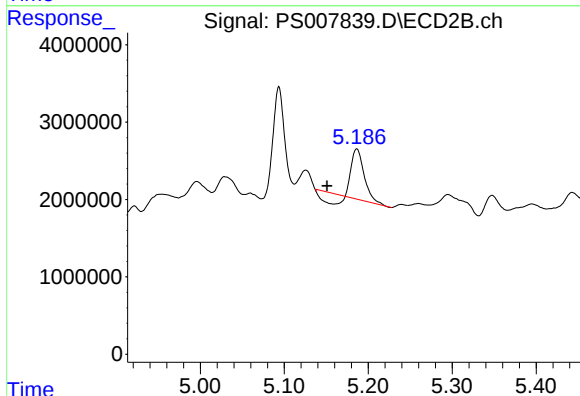


#4 2,4-DCAA

R.T.: 5.187 min
Delta R.T.: 0.036 min
Response: 5915832
Conc: 8.42 ng/ml

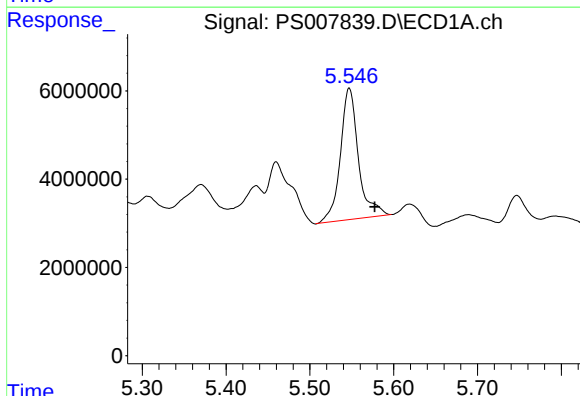


#5 DICAMBA

R.T.: 5.547 min
Delta R.T.: -0.030 min
Response: 44551865
Conc: 8.76 ng/ml

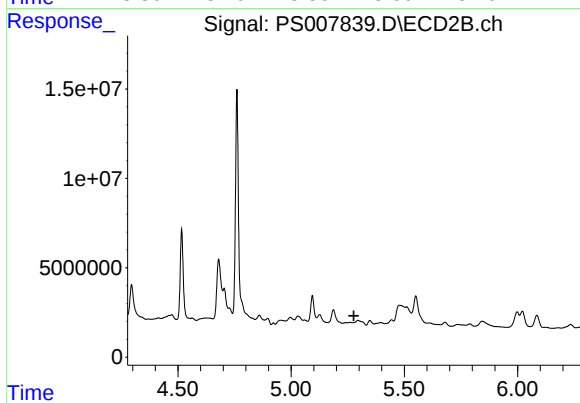

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.277 min
Response: 0
Conc: N.D.

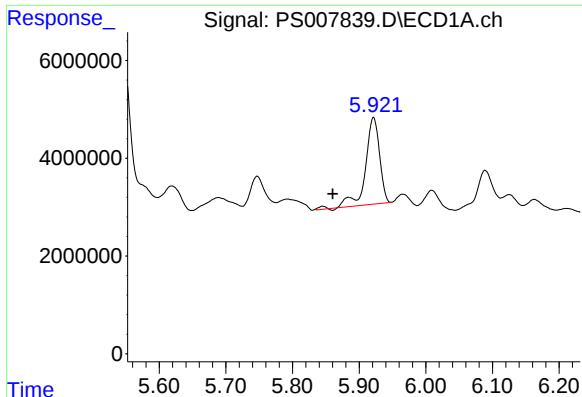

#7 MCPA


R.T.: 5.922 min
Delta R.T.: 0.062 min
Response: 26138705
Conc: 4.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
IDLEWILD-BH-03A

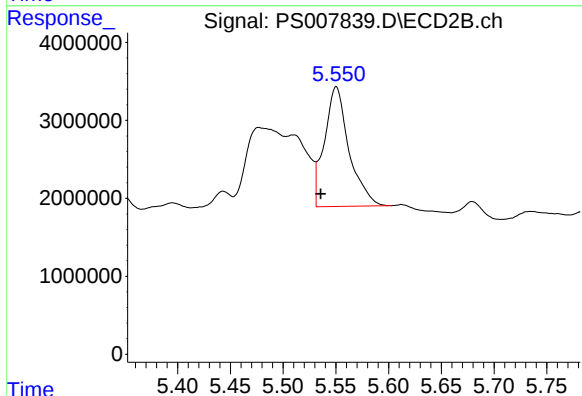


#7 MCPA

R.T.: 5.550 min
Delta R.T.: 0.015 min
Response: 24865324
Conc: 8.27 ug/ml

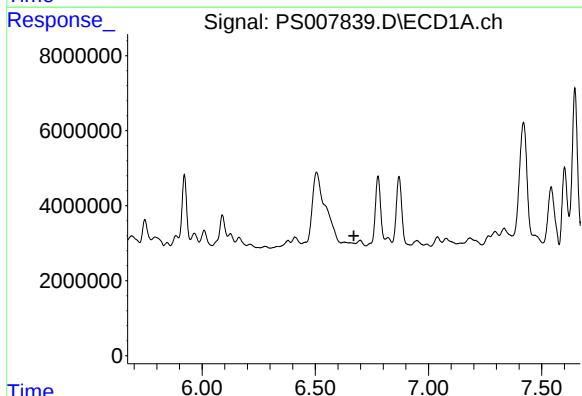


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.671 min
Response: 0
Conc: N.D.

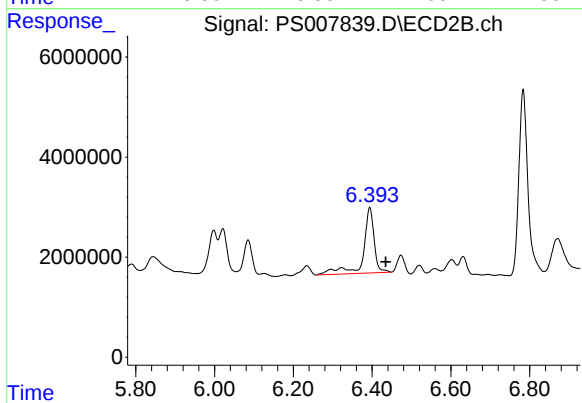

#10 Pentachlorophenol


R.T.: 6.394 min
Delta R.T.: -0.041 min
Response: 25100013
Conc: 2.56 ng/ml

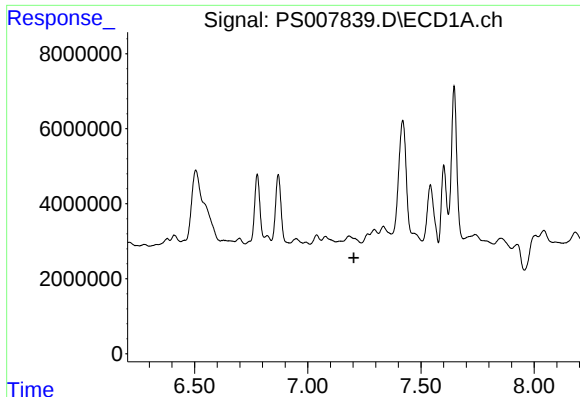

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.203 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
IDLEWILD-BH-03A

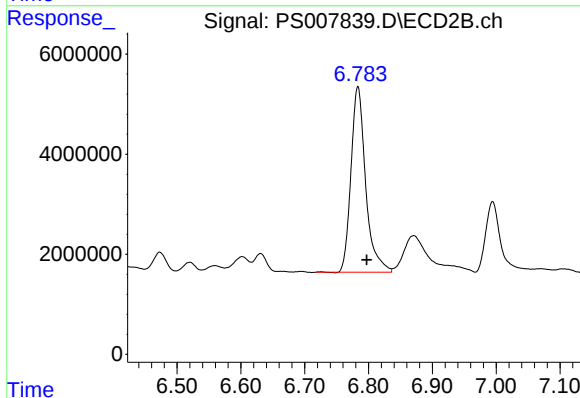


#11 2,4,5-TP (SILVEX)

R.T.: 6.783 min
Delta R.T.: -0.014 min
Response: 59195423
Conc: 15.12 ng/ml

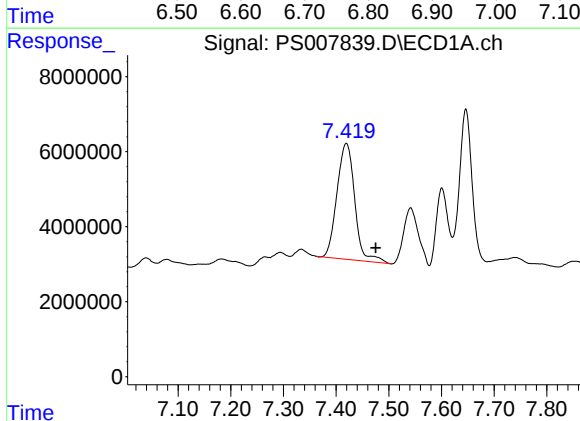


#12 2,4,5-T

R.T.: 7.419 min
Delta R.T.: -0.056 min
Response: 72601040
Conc: 8.87 ng/ml

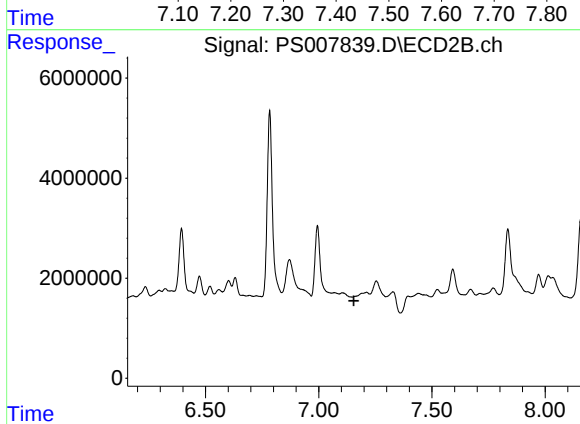

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.156 min
Response: 0
Conc: N.D.

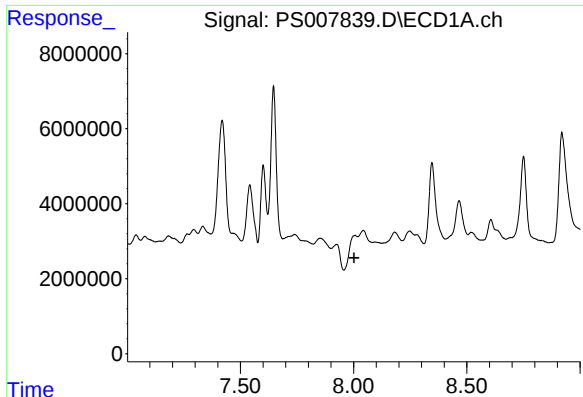

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 8.002 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
IDLEWILD-BH-03A

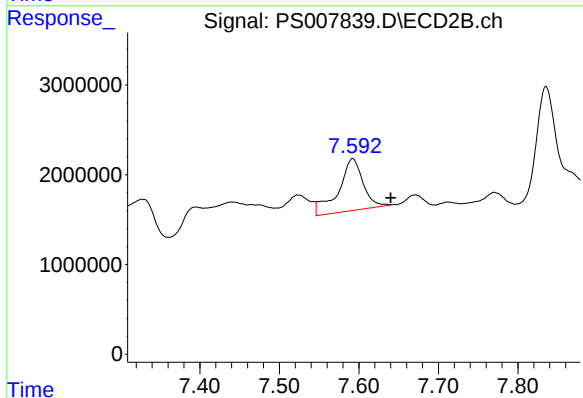


#13 2,4-DB

R.T.: 7.592 min
Delta R.T.: -0.048 min
Response: 12429168
Conc: 25.42 ng/ml

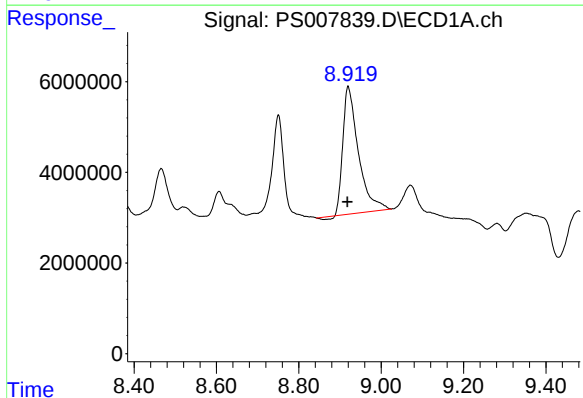

#15 Picloram

R.T.: 8.920 min
Delta R.T.: 0.002 min
Response: 73323176
Conc: 6.60 ng/ml

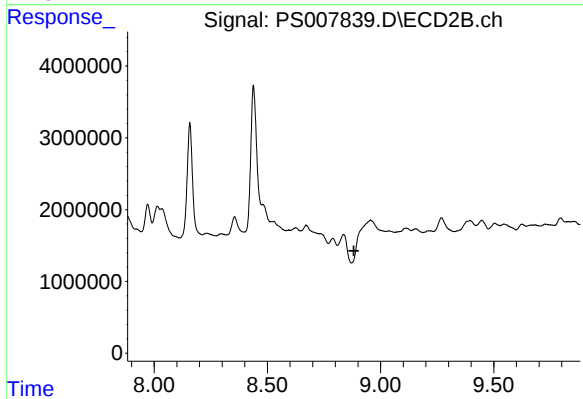

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.882 min
Response: 0
Conc: N.D.