

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112619\
 Data File : PS007846.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2019 00:04
 Operator : SM\AJ
 Sample : K5667-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 NB-07-112519

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 05:55:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.428	5.153	478.8E6	249.4E6	347.668	354.962
Target Compounds							
1) T	Dalapon	1.993	1.699	249.1E6	222.7E6	137.706	187.533 #
2) T	3,5-DICHL...	0.000	4.447	0	6520423	N.D.	7.217
5) T	DICAMBA	5.519	5.211	27683920	8560432	5.442	3.235 #
8) T	DICHLORPROP	0.000	5.810	0	12597532	N.D.	19.209
9) T	2,4-D	6.479	6.056	75978097	8831232	54.171	10.951 #
10) T	Pentachlo...	0.000	6.439	0	16302223	N.D.	1.665
11) T	2,4,5-TP ...	0.000	6.796	0	7090974	N.D.	1.811
12) T	2,4,5-T	7.509	7.209	64762990	40217183	7.911	10.890 #
15) T	Picloram	8.941	8.895	190.8E6	141.8E6	17.180	24.198 #
16) T	DCPA	0.000	8.895	0	141.8E6	N.D.	27.133



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112619\
Data File : PS007846.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2019 00:04
Operator : SM\AJ
Sample : K5667-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
NB-07-112519

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 05:55:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

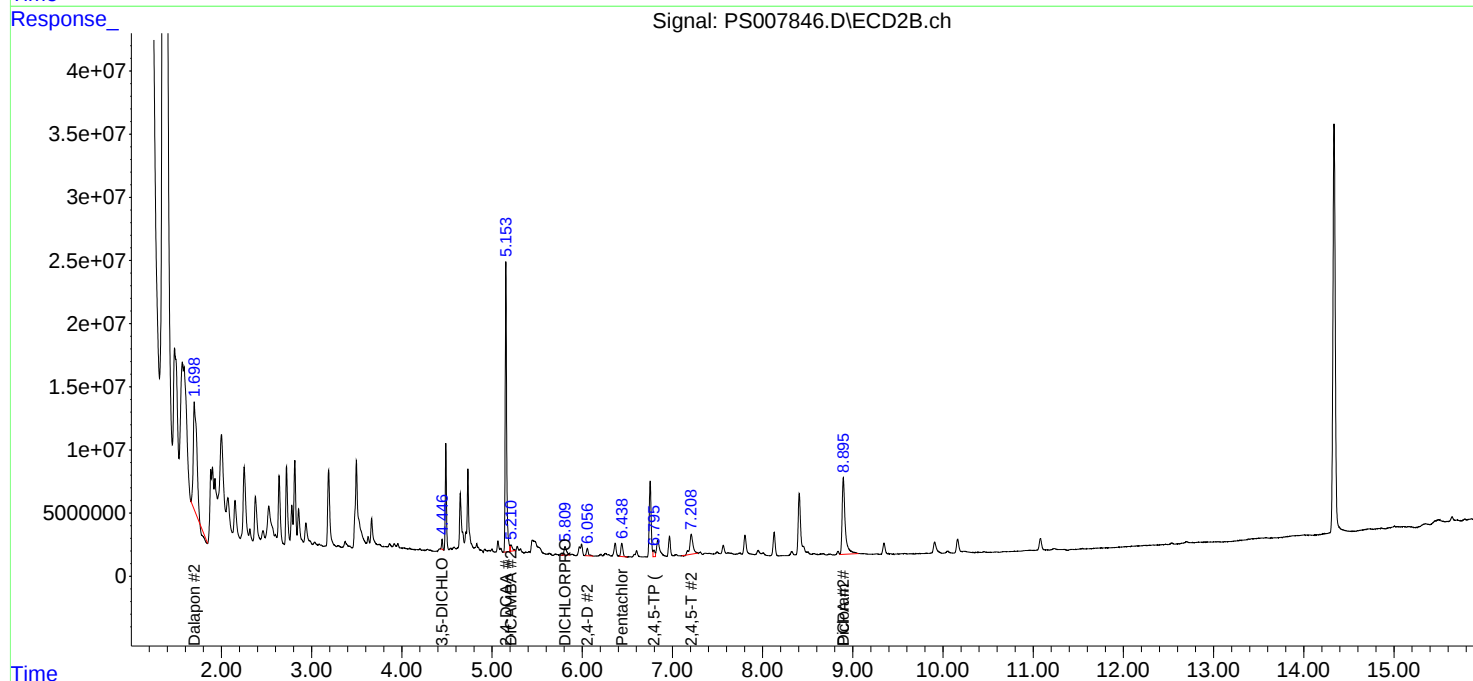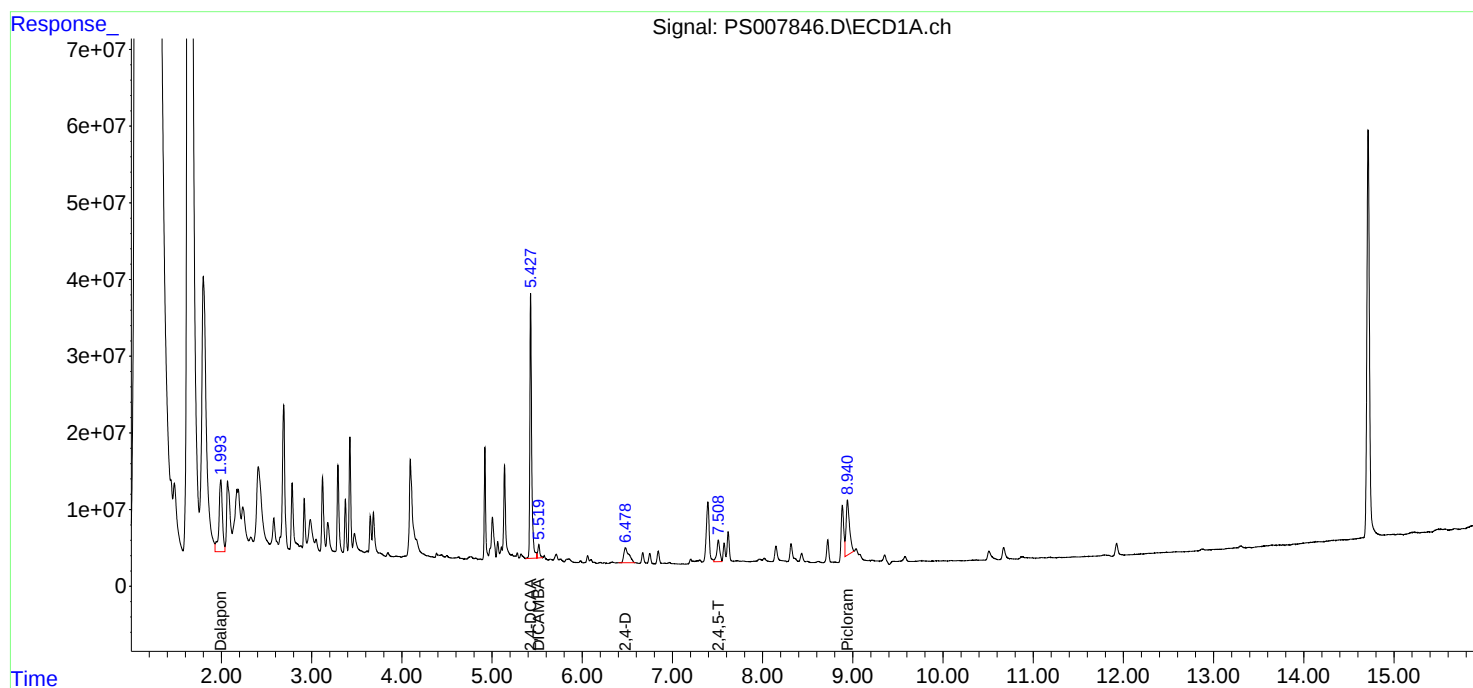


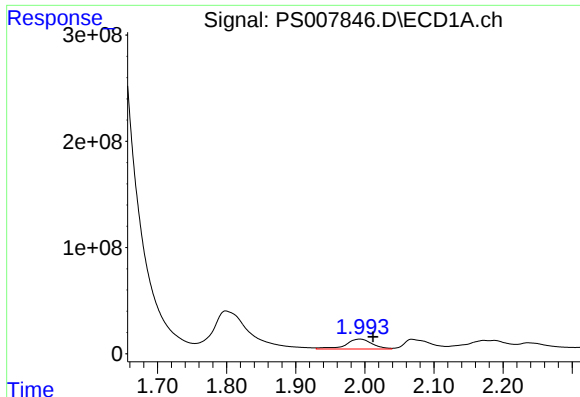

#1 Dalapon


R.T.: 1.993 min
Delta R.T.: -0.019 min
Response: 249134067
Conc: 137.71 ng/ml

Instrument :
ECD_S
ClientSampleId :
NB-07-112519

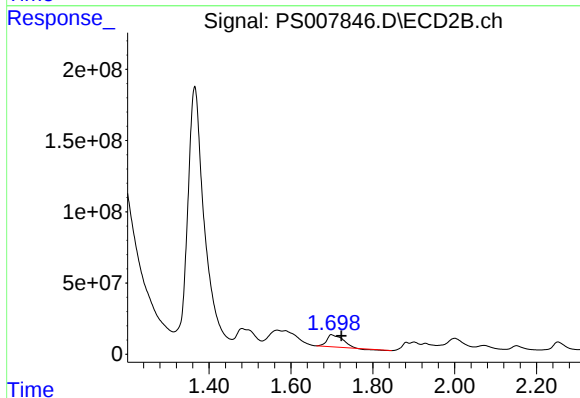


#1 Dalapon

R.T.: 1.699 min
Delta R.T.: -0.024 min
Response: 222676636
Conc: 187.53 ng/ml

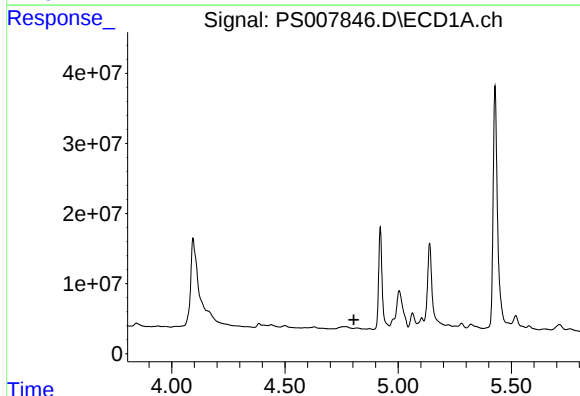


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.804 min
Response: 0
Conc: N.D.

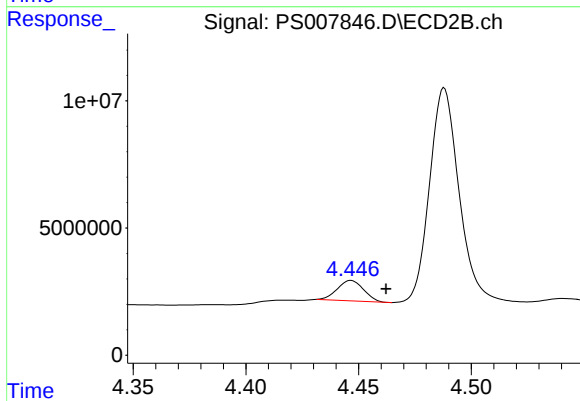

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.447 min
Delta R.T.: -0.016 min
Response: 6520423
Conc: 7.22 ng/ml

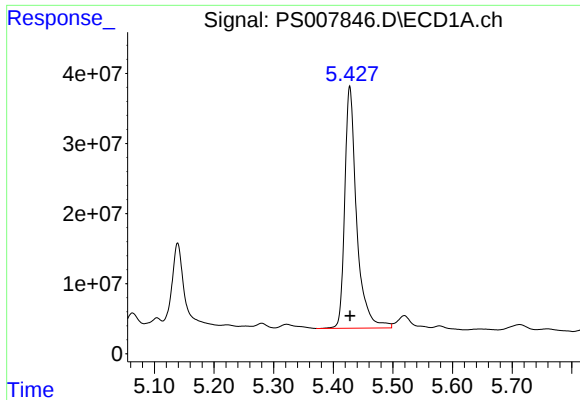

#4 2,4-DCAA


R.T.: 5.428 min
Delta R.T.: 0.000 min
Response: 478803126
Conc: 347.67 ng/ml

Instrument :
ECD_S
ClientSampleId :
NB-07-112519

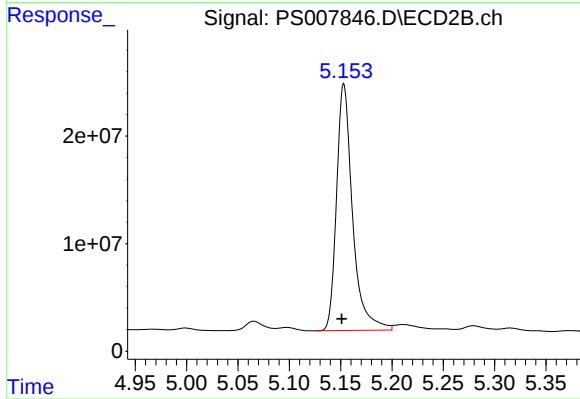


#4 2,4-DCAA

R.T.: 5.153 min
Delta R.T.: 0.002 min
Response: 249383397
Conc: 354.96 ng/ml

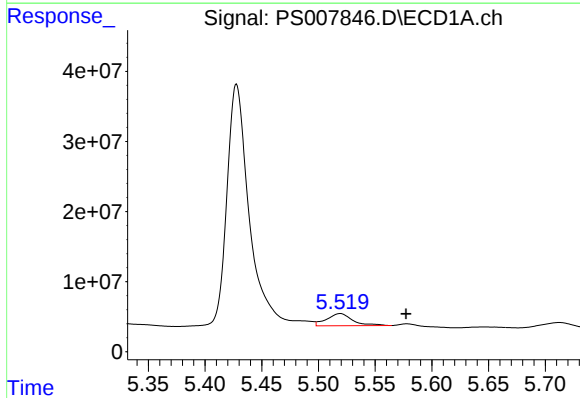


#5 DICAMBA

R.T.: 5.519 min
Delta R.T.: -0.058 min
Response: 27683920
Conc: 5.44 ng/ml

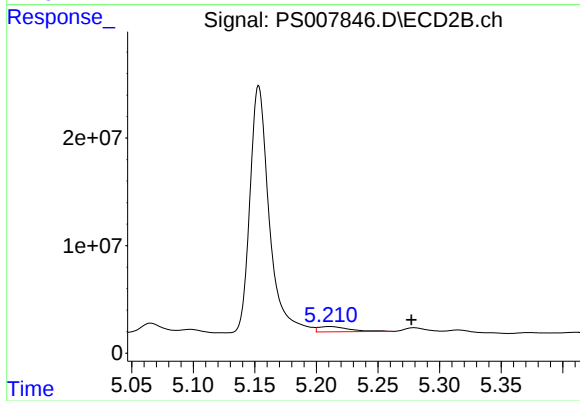

#5 DICAMBA


R.T.: 5.211 min
Delta R.T.: -0.066 min
Response: 8560432
Conc: 3.23 ng/ml

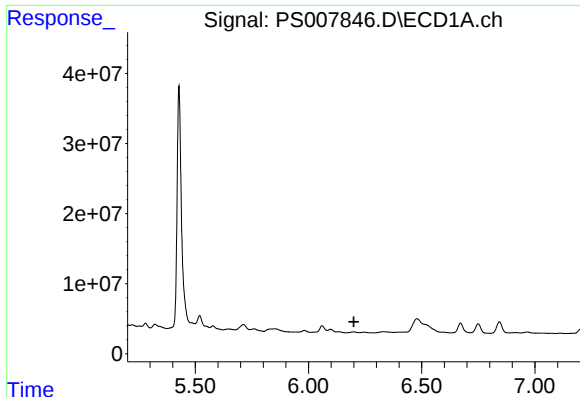

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.200 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
NB-07-112519

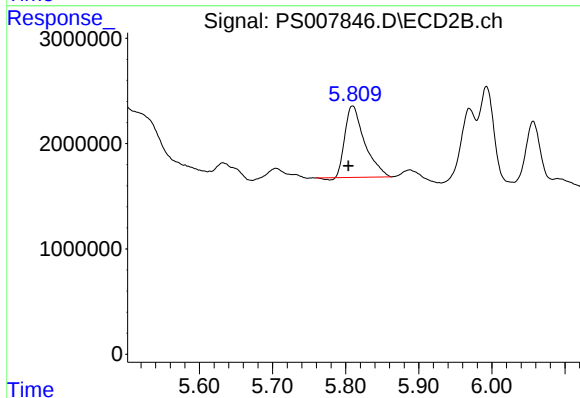


#8 DICHLORPROP

R.T.: 5.810 min
Delta R.T.: 0.006 min
Response: 12597532
Conc: 19.21 ng/ml

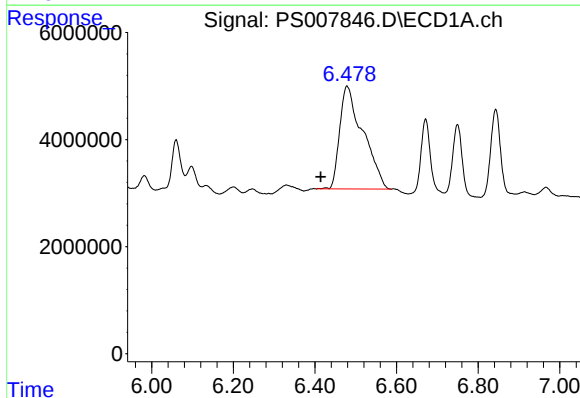


#9 2,4-D

R.T.: 6.479 min
Delta R.T.: 0.065 min
Response: 75978097
Conc: 54.17 ng/ml

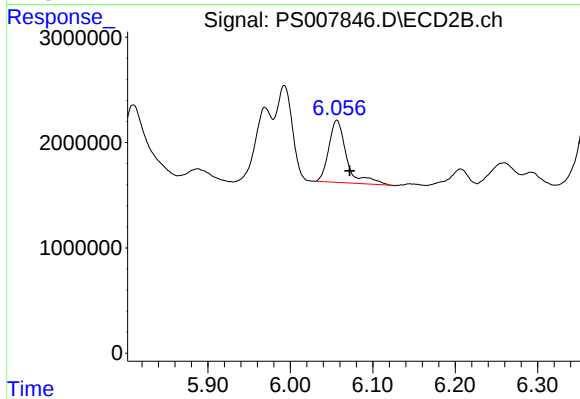

#9 2,4-D


R.T.: 6.056 min
Delta R.T.: -0.016 min
Response: 8831232
Conc: 10.95 ng/ml

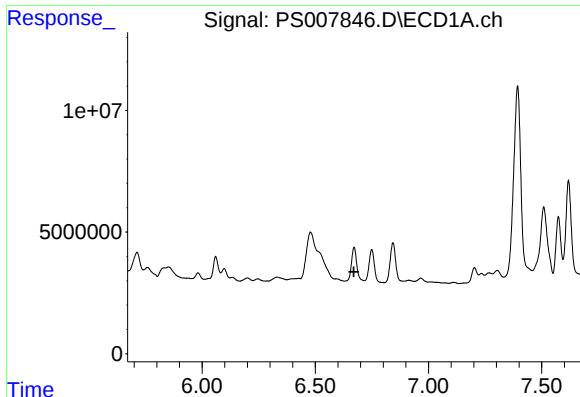

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.671 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
NB-07-112519

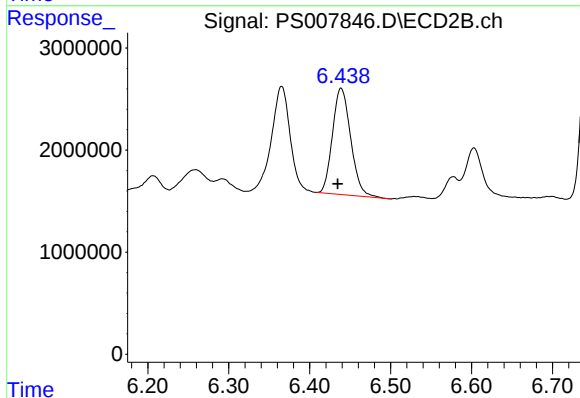


#10 Pentachlorophenol

R.T.: 6.439 min
Delta R.T.: 0.004 min
Response: 16302223
Conc: 1.66 ng/ml

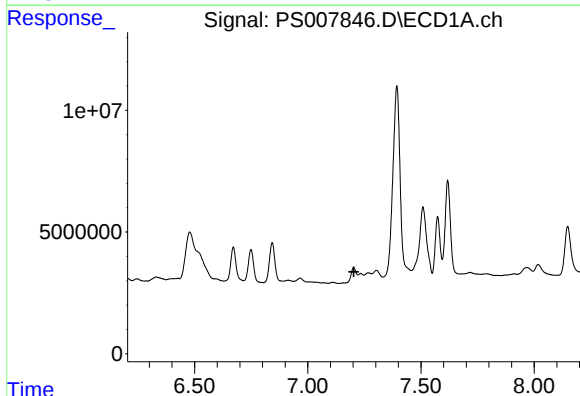


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.203 min
Response: 0
Conc: N.D.

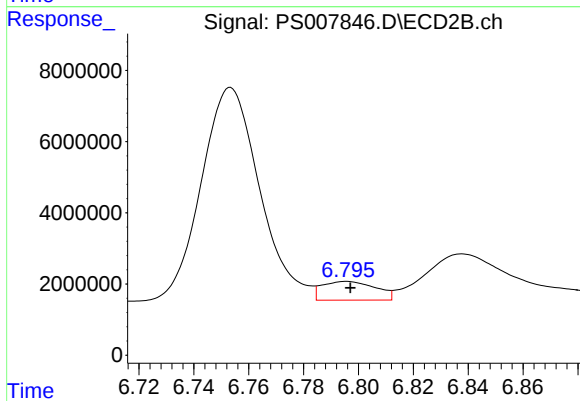

#11 2,4,5-TP (SILVEX)


R.T.: 6.796 min
Delta R.T.: -0.001 min
Response: 7090974
Conc: 1.81 ng/ml

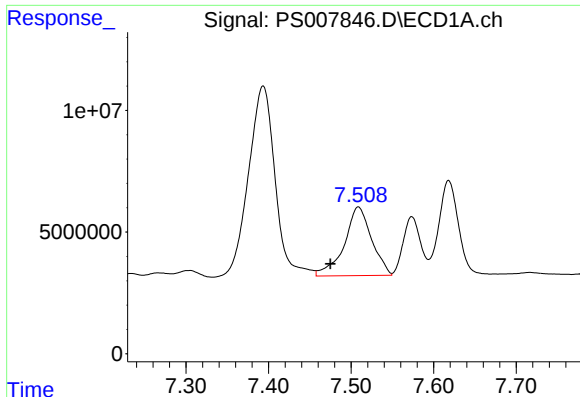

#12 2,4,5-T


R.T.: 7.509 min
Delta R.T.: 0.034 min
Response: 64762990
Conc: 7.91 ng/ml

Instrument :
ECD_S
ClientSampleId :
NB-07-112519

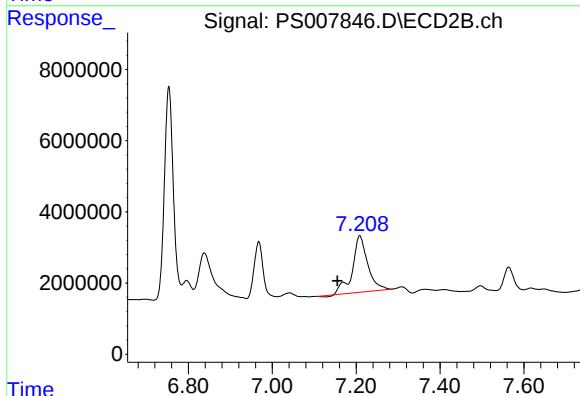


#12 2,4,5-T

R.T.: 7.209 min
Delta R.T.: 0.053 min
Response: 40217183
Conc: 10.89 ng/ml

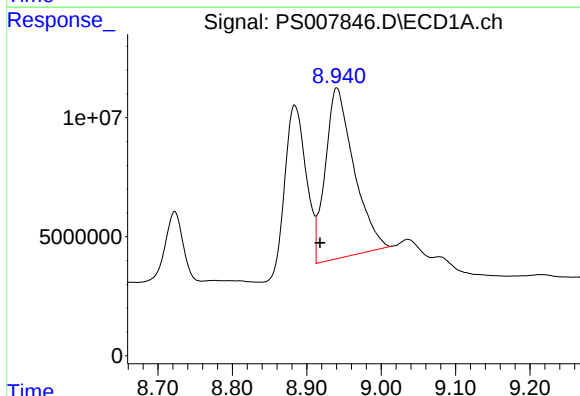


#15 Picloram

R.T.: 8.941 min
Delta R.T.: 0.023 min
Response: 190750546
Conc: 17.18 ng/ml

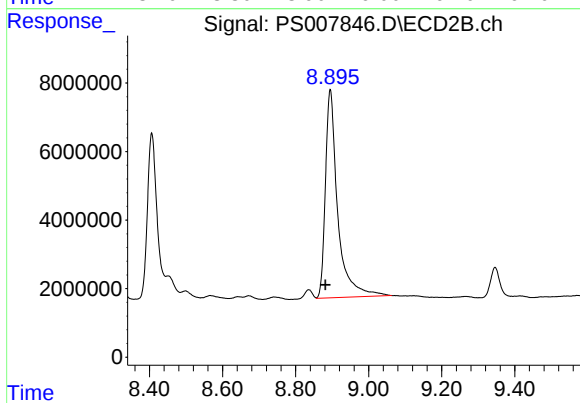

#15 Picloram


R.T.: 8.895 min
Delta R.T.: 0.013 min
Response: 141776054
Conc: 24.20 ng/ml

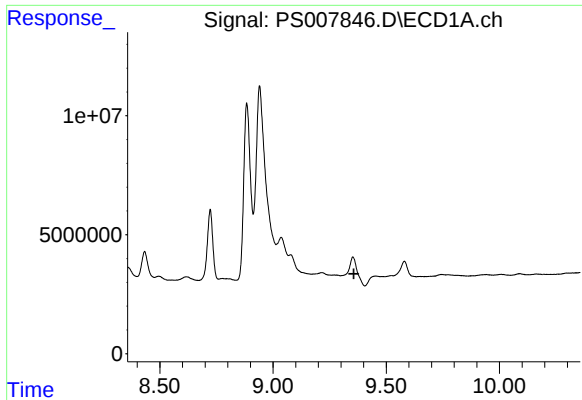

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.357 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
NB-07-112519

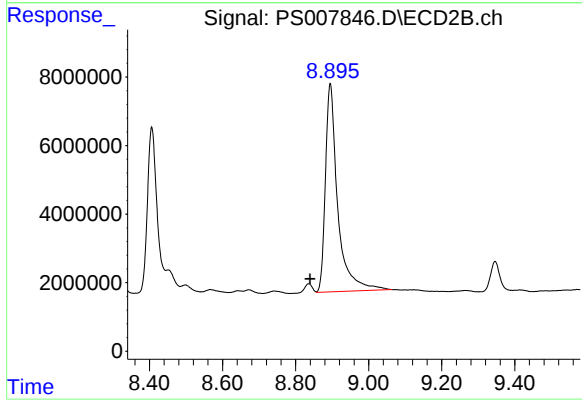

#16 DCPA

R.T.: 8.895 min
Delta R.T.: 0.055 min
Response: 141776054
Conc: 27.13 ng/ml