

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112619\
 Data File : PS007848.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2019 00:47
 Operator : SM\AJ
 Sample : K6013-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 600436752

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 05:55:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.427	5.152	701.0E6	373.0E6	509.038	530.887
Target Compounds							
1) T	Dalapon	1.990	1.699	177.0E6	309.8E6	97.809	260.934 #
2) T	3,5-DICHL...	0.000	4.446	0	7339009	N.D.	8.123
5) T	DICAMBA	5.518	0.000	44879723	0	8.822	N.D. #
9) T	2,4-D	6.478	6.056	74051177	6231544	52.798	7.728 #
10) T	Pentachlo...	0.000	6.365	0	19453003	N.D.	1.987
11) T	2,4,5-TP ...	0.000	6.753	0	71524267	N.D.	18.265
12) T	2,4,5-T	7.510	0.000	32209142	0	3.935	N.D. #
15) T	Picloram	8.887	0.000	103.8E6	0	9.346	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112619\
Data File : PS007848.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2019 00:47
Operator : SM\AJ
Sample : K6013-03
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
600436752

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 05:55:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

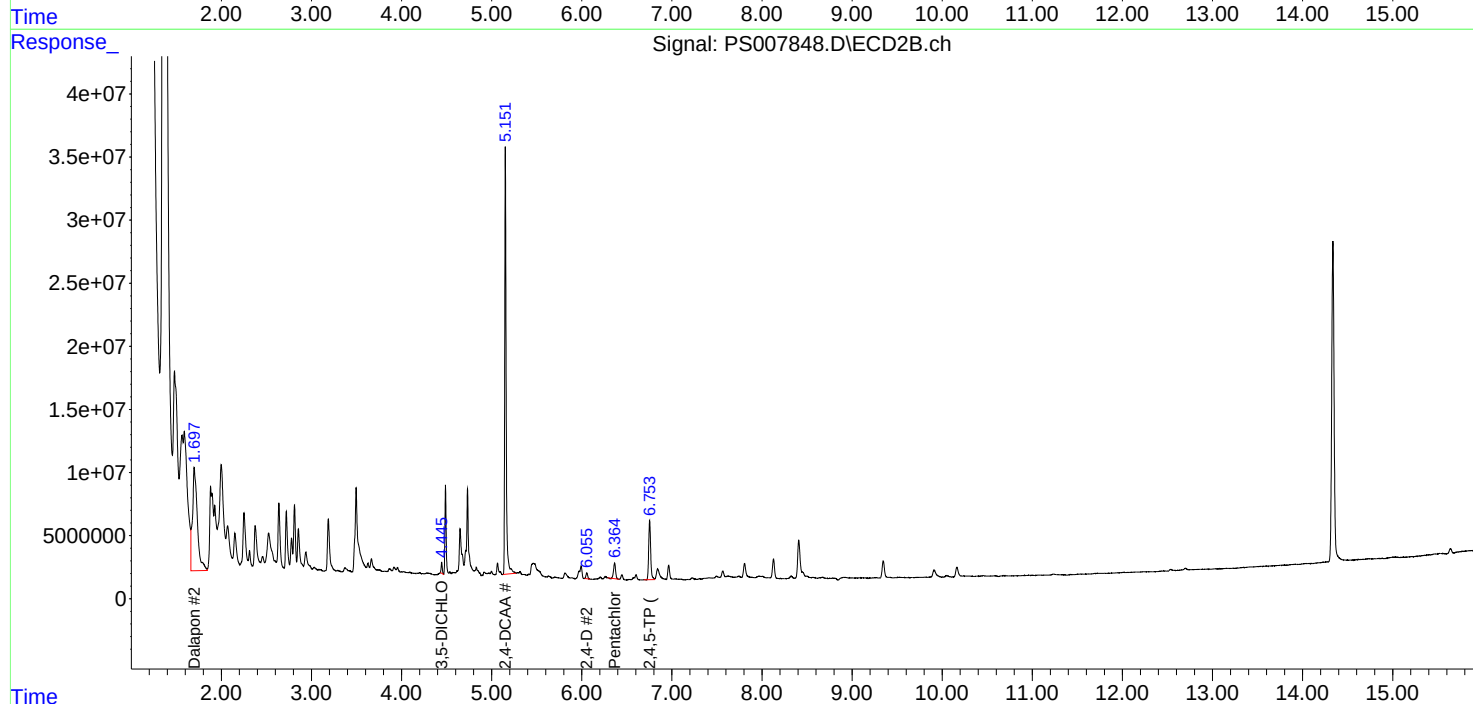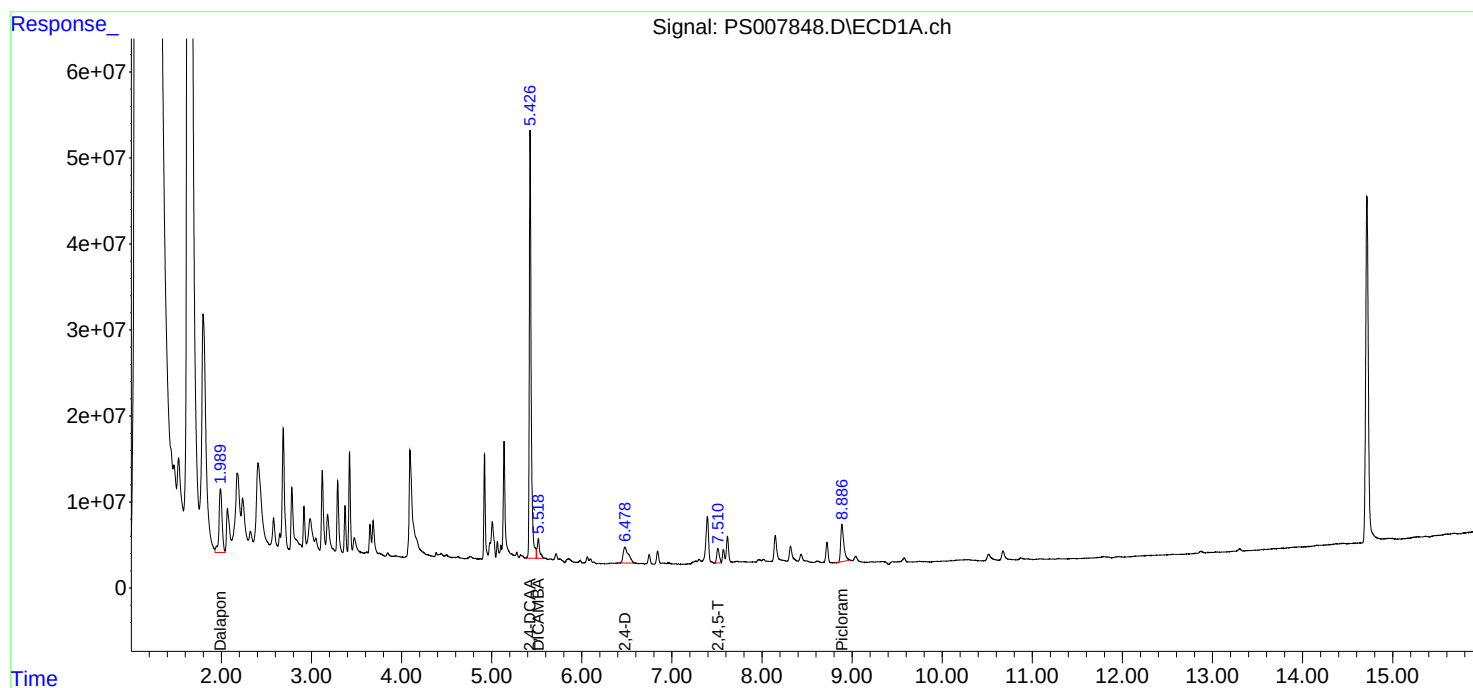


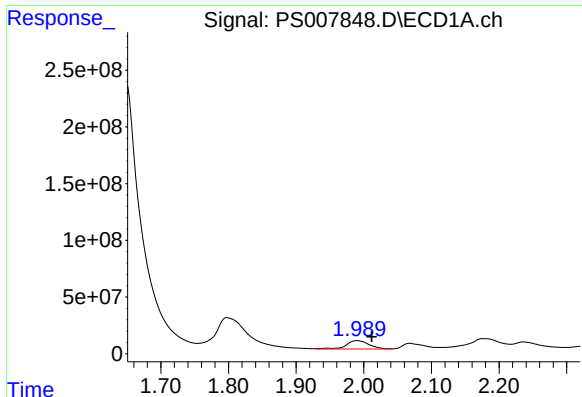

#1 Dalapon


R.T.: 1.990 min
Delta R.T.: -0.022 min
Response: 176953711
Conc: 97.81 ng/ml

Instrument :
ECD_S
ClientSampleId :
600436752

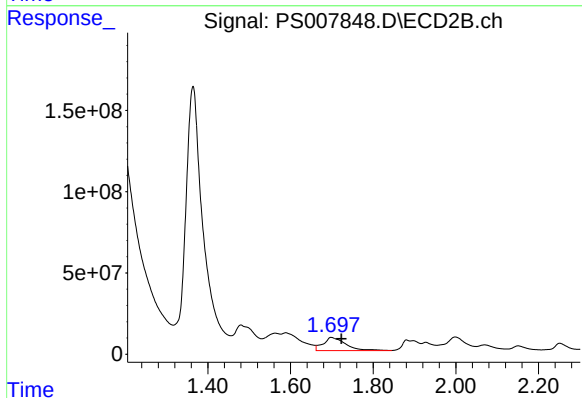


#1 Dalapon

R.T.: 1.699 min
Delta R.T.: -0.025 min
Response: 309834046
Conc: 260.93 ng/ml

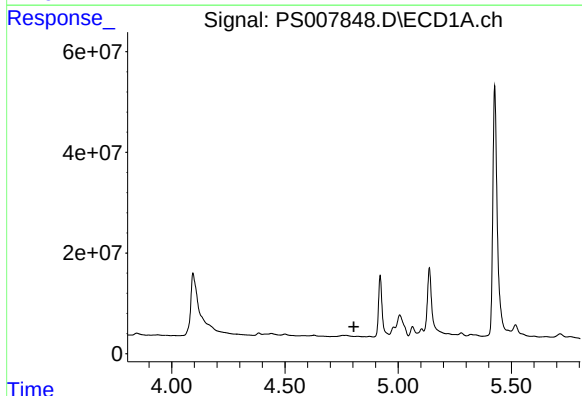


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.804 min
Response: 0
Conc: N.D.

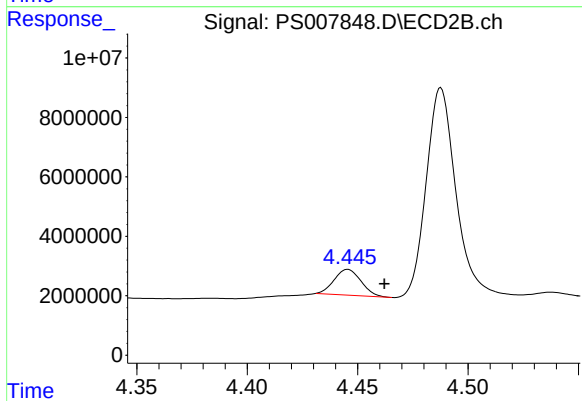

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.446 min
Delta R.T.: -0.017 min
Response: 7339009
Conc: 8.12 ng/ml

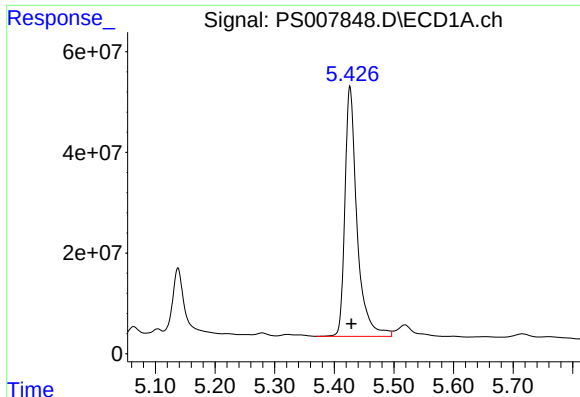

#4 2,4-DCAA


R.T.: 5.427 min
Delta R.T.: -0.002 min
Response: 701038731
Conc: 509.04 ng/ml

Instrument :
ECD_S
ClientSampleId :
600436752

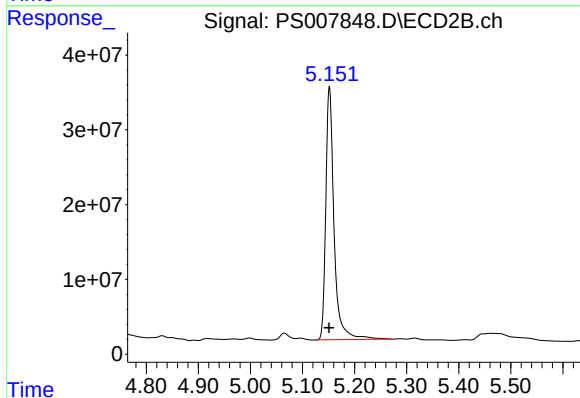


#4 2,4-DCAA

R.T.: 5.152 min
Delta R.T.: 0.000 min
Response: 372982235
Conc: 530.89 ng/ml

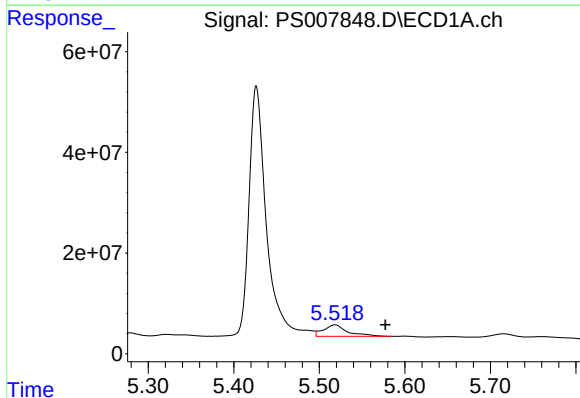


#5 DICAMBA

R.T.: 5.518 min
Delta R.T.: -0.059 min
Response: 44879723
Conc: 8.82 ng/ml

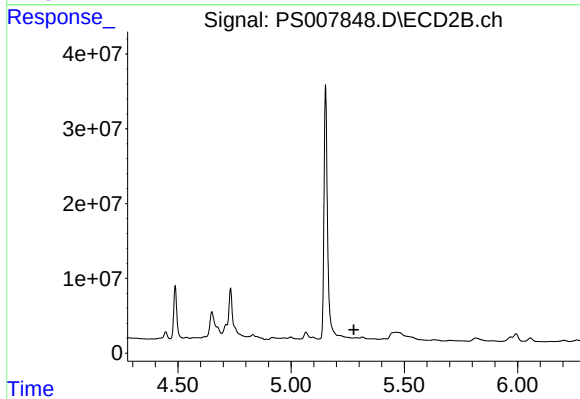

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.277 min
Response: 0
Conc: N.D.

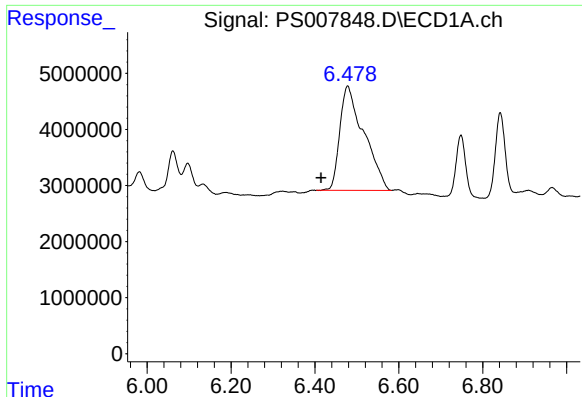

#9 2,4-D


R.T.: 6.478 min
Delta R.T.: 0.064 min
Response: 74051177
Conc: 52.80 ng/ml

Instrument :
ECD_S
ClientSampleId :
600436752

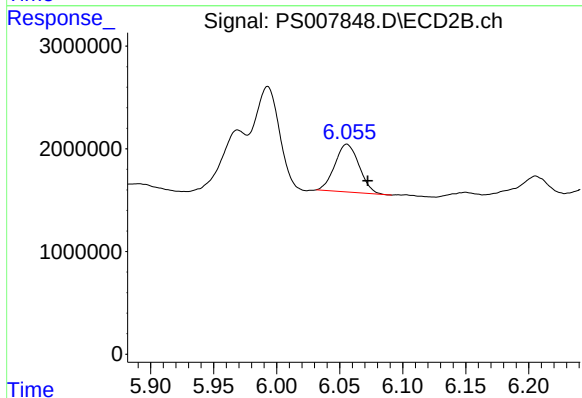


#9 2,4-D

R.T.: 6.056 min
Delta R.T.: -0.016 min
Response: 6231544
Conc: 7.73 ng/ml

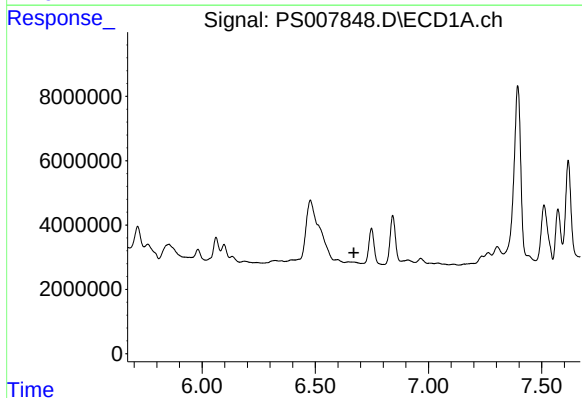


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.671 min
Response: 0
Conc: N.D.

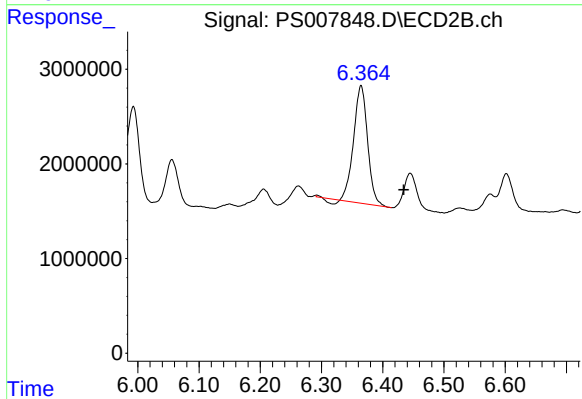

#10 Pentachlorophenol


R.T.: 6.365 min
Delta R.T.: -0.070 min
Response: 19453003
Conc: 1.99 ng/ml

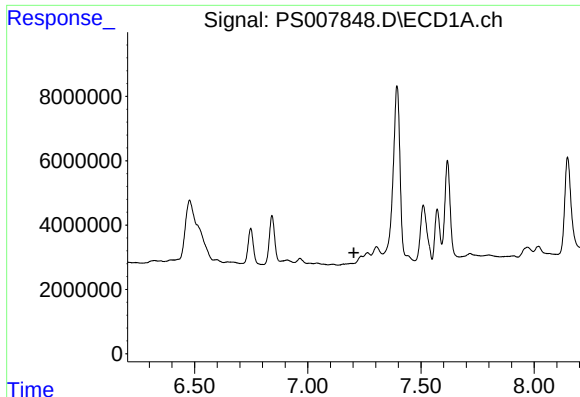

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.203 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
600436752

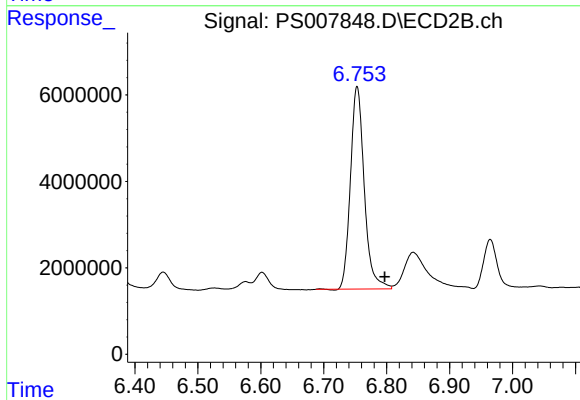


#11 2,4,5-TP (SILVEX)

R.T.: 6.753 min
Delta R.T.: -0.044 min
Response: 71524267
Conc: 18.27 ng/ml

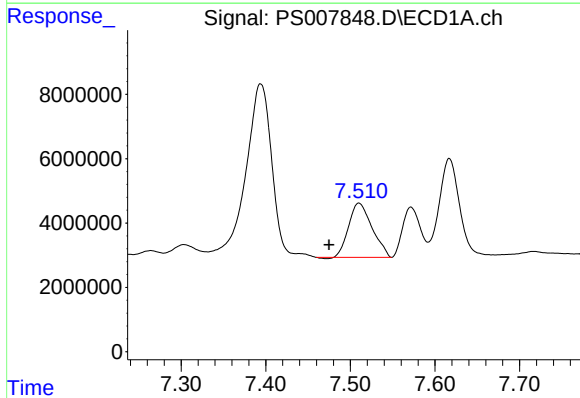


#12 2,4,5-T

R.T.: 7.510 min
Delta R.T.: 0.035 min
Response: 32209142
Conc: 3.93 ng/ml

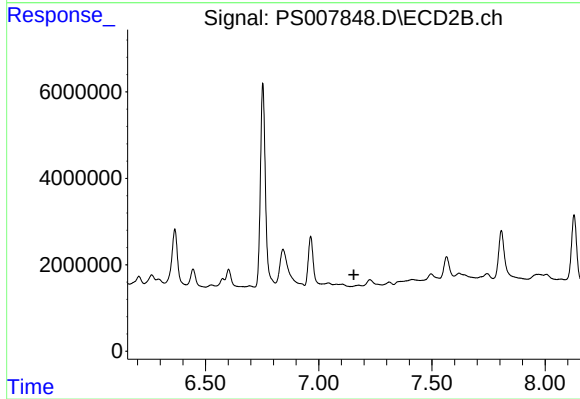

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.156 min
Response: 0
Conc: N.D.

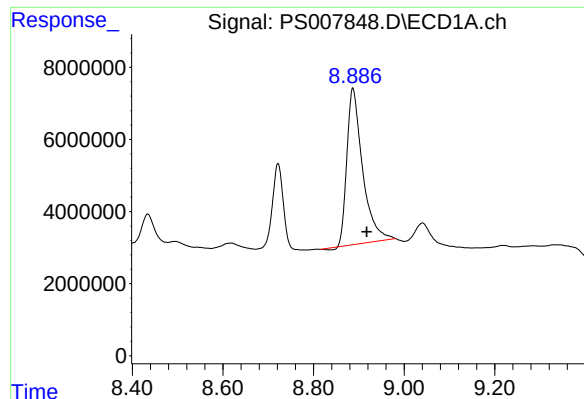

#15 Picloram

R.T.: 8.887 min
Delta R.T.: -0.031 min
Response: 103771801
Conc: 9.35 ng/ml

Instrument :
ECD_S
ClientSampleId :
600436752

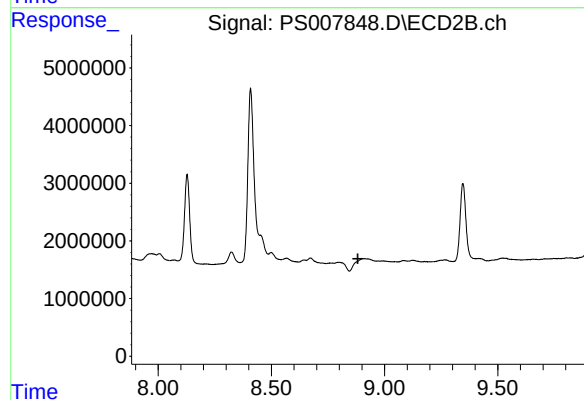

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.882 min
Response: 0
Conc: N.D.