

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112619\
 Data File : PS007853.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2019 08:47
 Operator : SM\AJ
 Sample : K5999-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 09:44:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.450	5.172	107.4E6	54164020	77.995	77.095
Target Compounds							
1) T	Dalapon	2.006	1.715	191.5E6	566.2E6	105.868	476.843 #
2) T	3,5-DICHL...	0.000	4.504	0	78497477	N.D.	86.888
5) T	DICAMBA	5.537	0.000	50717478	0	9.969	N.D. #
7) T	MCPA	5.912	5.538	27301571	24737175	4.960	8.230 #
9) T	2,4-D	0.000	6.073	0	6316553	N.D.	7.833
10) T	Pentachlo...	0.000	6.461	0	6027530	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	6.771	0	72102056	N.D.	18.413
12) T	2,4,5-T	7.409	0.000	123.6E6	0	15.093	N.D. #
13) T	2,4-DB	0.000	7.582	0	8368216	N.D.	17.118
14) T	DINOSEB	0.000	7.959	0	10888636	N.D.	3.745
15) T	Picloram	8.915	8.916	44415133	139.4E6	4.000	23.793 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112619\
Data File : PS007853.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2019 08:47
Operator : SM\AJ
Sample : K5999-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 09:44:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

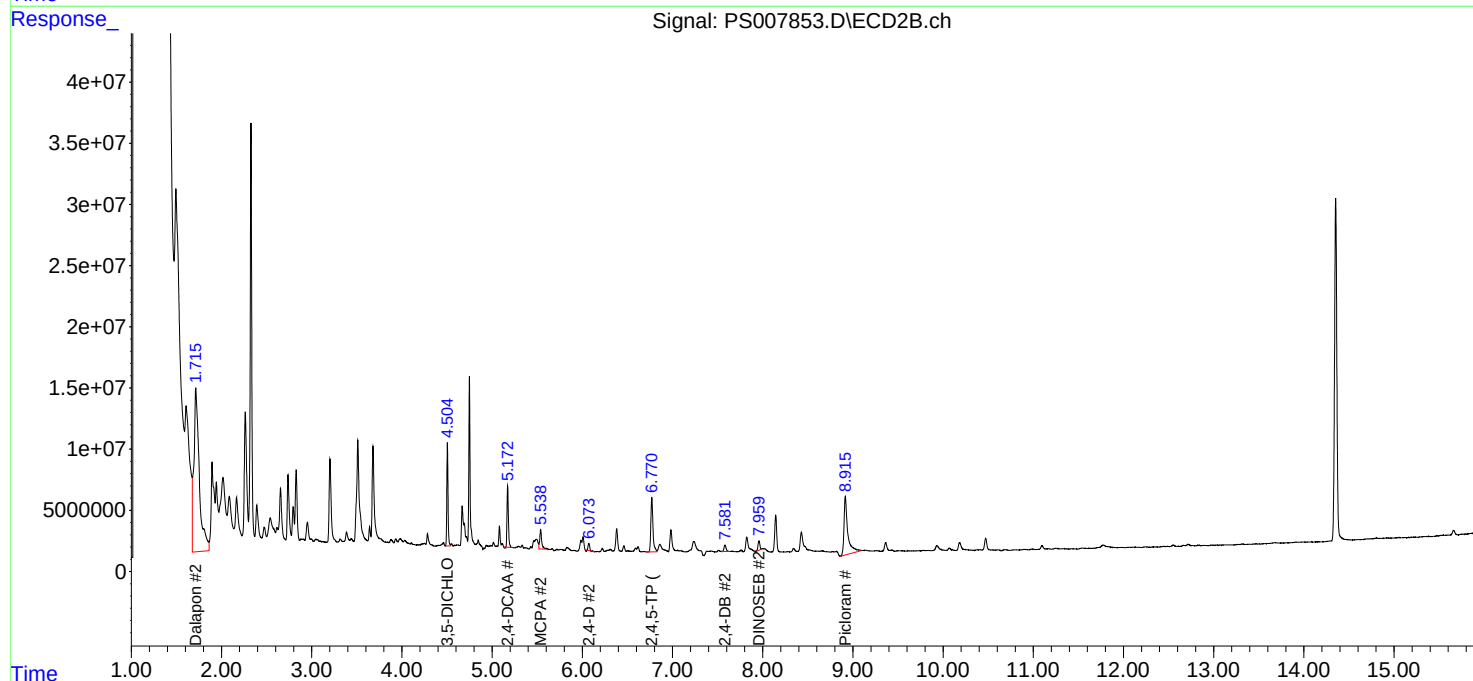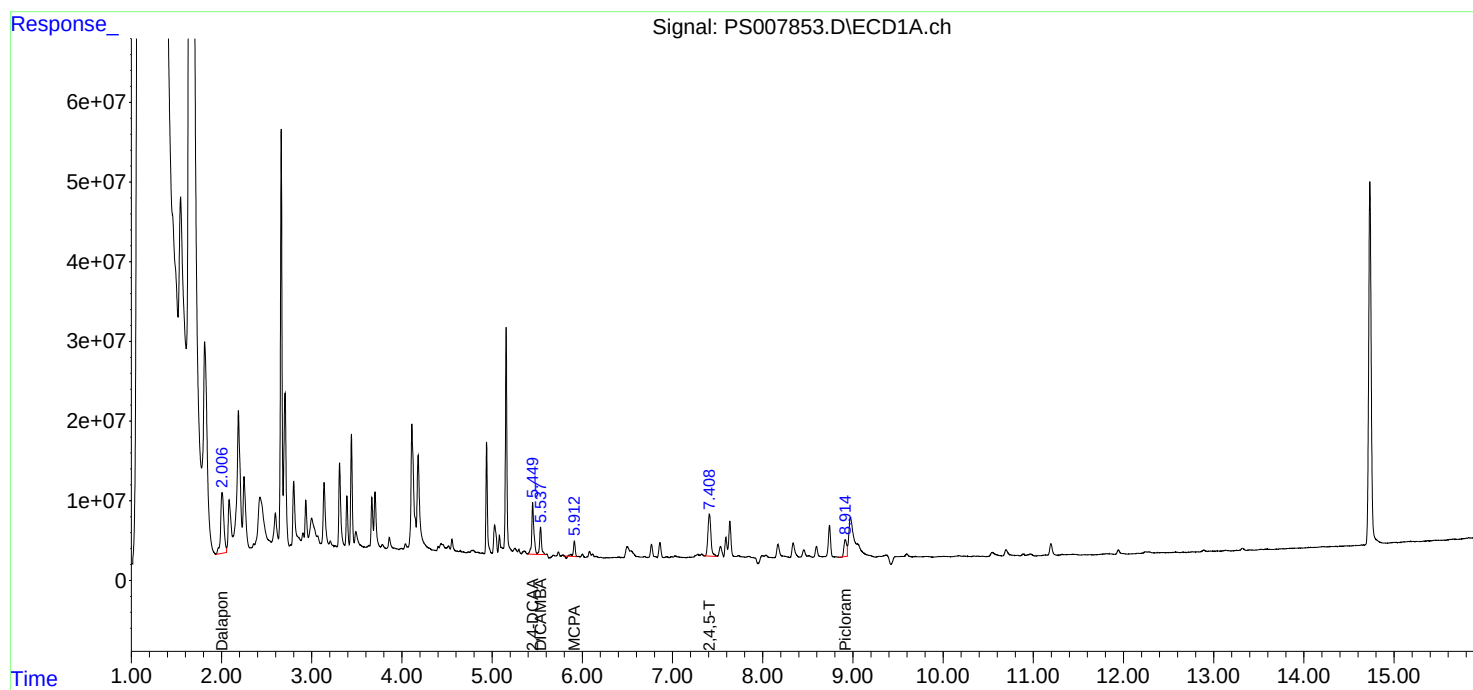


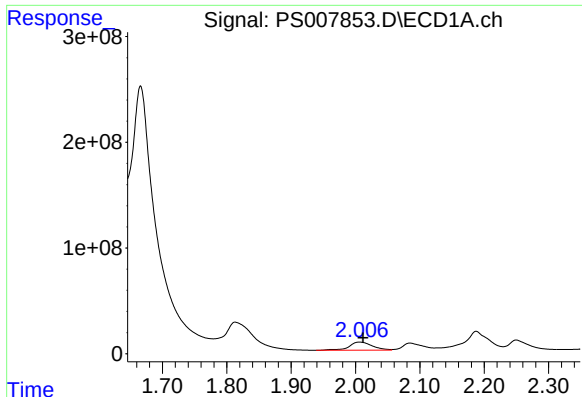

#1 Dalapon


R.T.: 2.006 min
Delta R.T.: -0.006 min
Response: 191534567
Conc: 105.87 ng/ml

Instrument :
ECD_S
ClientSampleId :

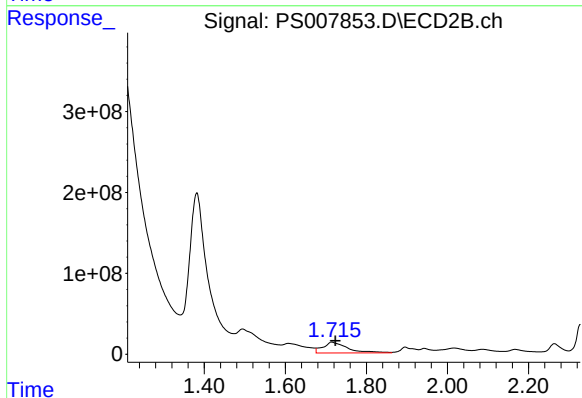


#1 Dalapon

R.T.: 1.715 min
Delta R.T.: -0.008 min
Response: 566205155
Conc: 476.84 ng/ml

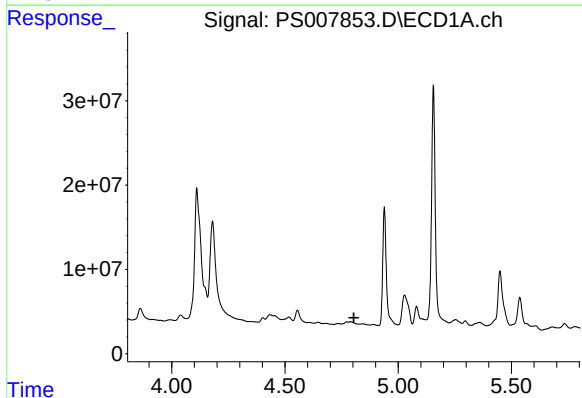


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.804 min
Response: 0
Conc: N.D.

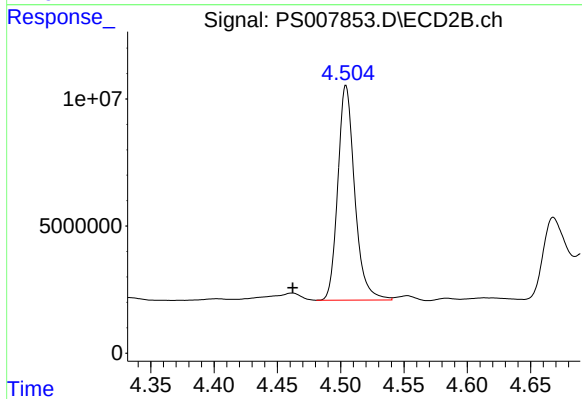

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.504 min
Delta R.T.: 0.042 min
Response: 78497477
Conc: 86.89 ng/ml

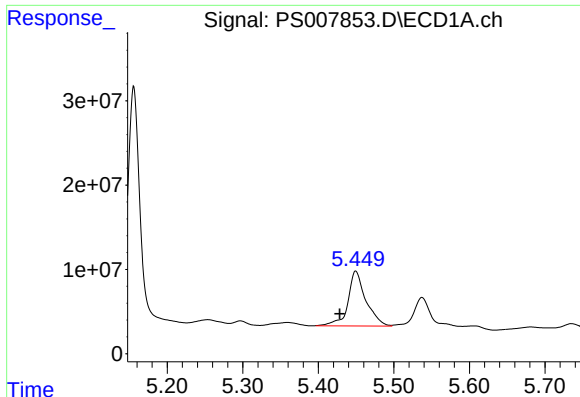

#4 2,4-DCAA


R.T.: 5.450 min
Delta R.T.: 0.021 min
Response: 107413685
Conc: 78.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

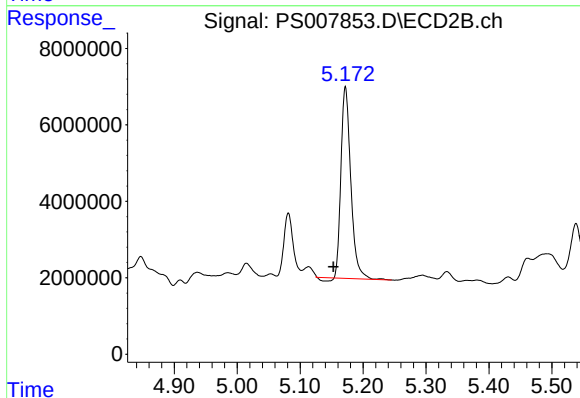


#4 2,4-DCAA

R.T.: 5.172 min
Delta R.T.: 0.020 min
Response: 54164020
Conc: 77.09 ng/ml

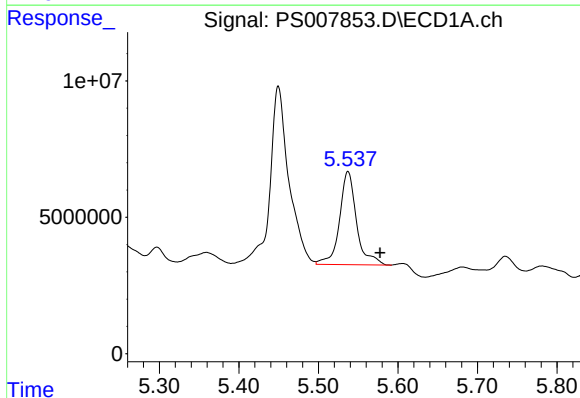


#5 DICAMBA

R.T.: 5.537 min
Delta R.T.: -0.040 min
Response: 50717478
Conc: 9.97 ng/ml

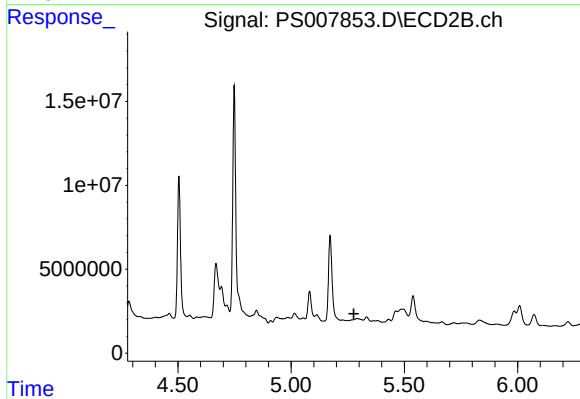

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.277 min
Response: 0
Conc: N.D.

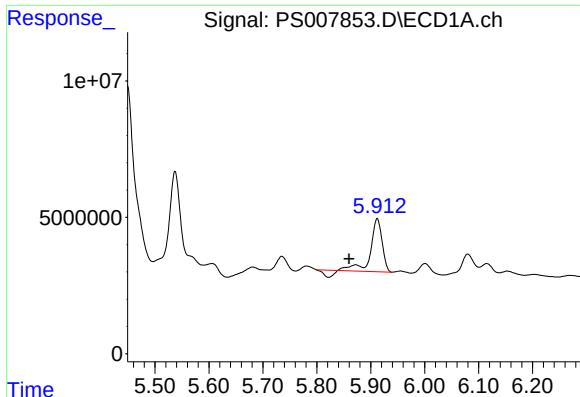

#7 MCPA


R.T.: 5.912 min
Delta R.T.: 0.052 min
Response: 27301571
Conc: 4.96 ug/ml

Instrument :
ECD_S
ClientSampleId :

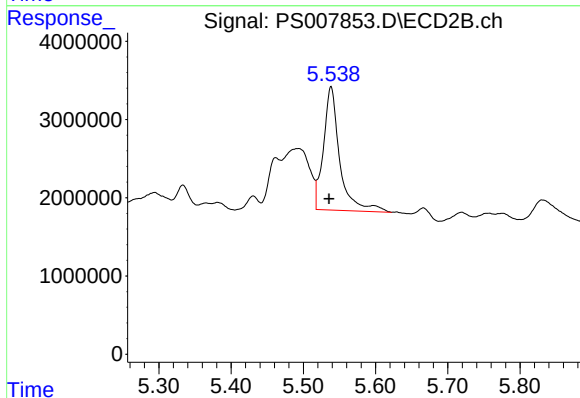


#7 MCPA

R.T.: 5.538 min
Delta R.T.: 0.003 min
Response: 24737175
Conc: 8.23 ug/ml

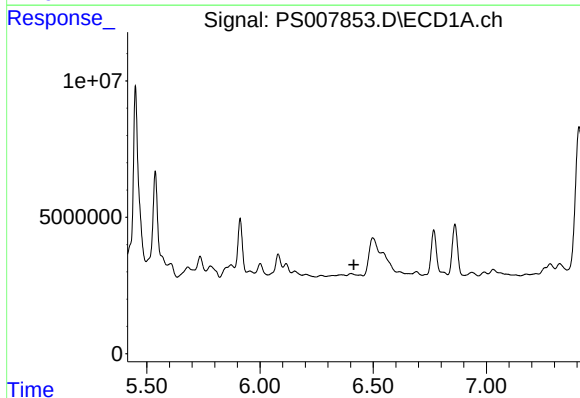


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.414 min
Response: 0
Conc: N.D.

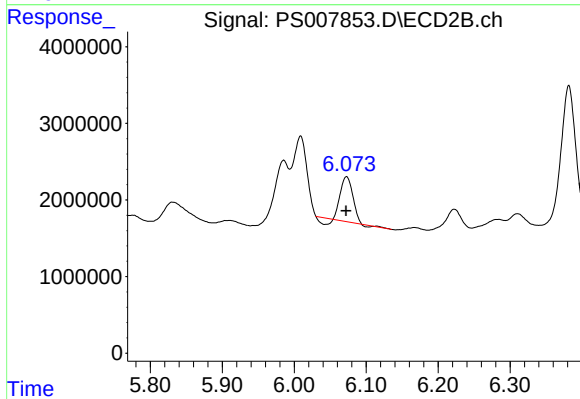

#9 2,4-D


R.T.: 6.073 min
Delta R.T.: 0.000 min
Response: 6316553
Conc: 7.83 ng/ml

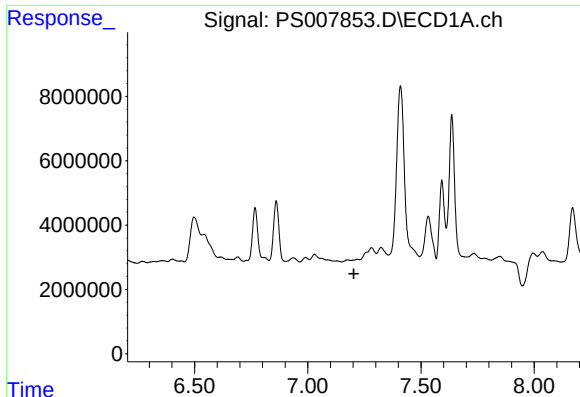

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.203 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

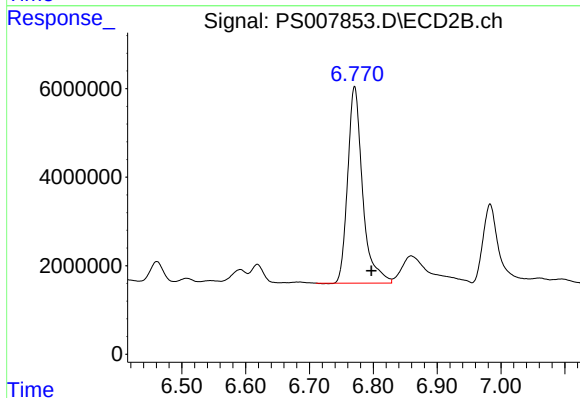


#11 2,4,5-TP (SILVEX)

R.T.: 6.771 min
Delta R.T.: -0.026 min
Response: 72102056
Conc: 18.41 ng/ml

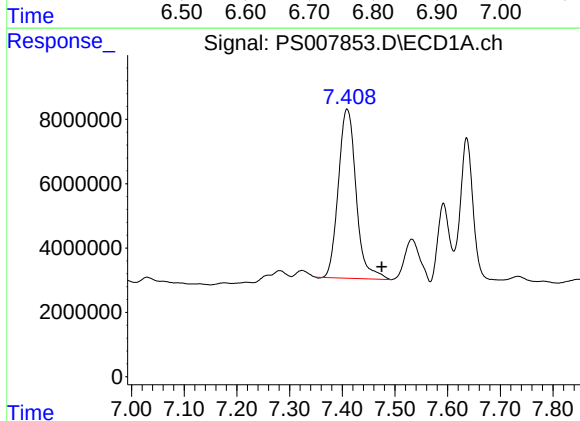


#12 2,4,5-T

R.T.: 7.409 min
Delta R.T.: -0.066 min
Response: 123553171
Conc: 15.09 ng/ml

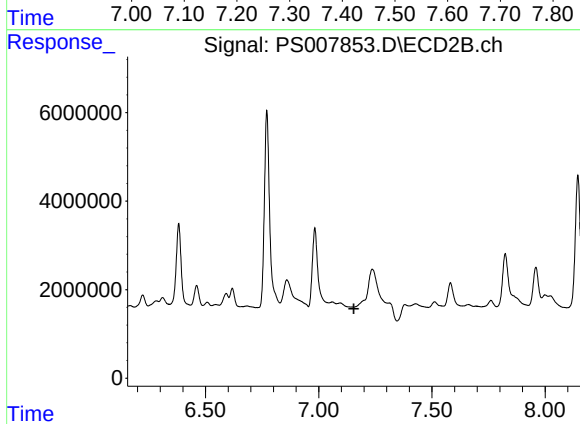

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.156 min
Response: 0
Conc: N.D.

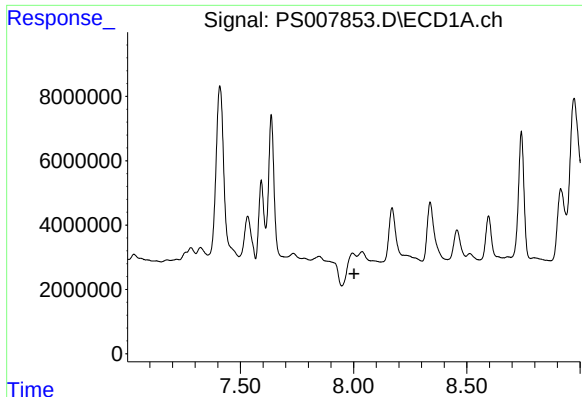

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 8.002 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

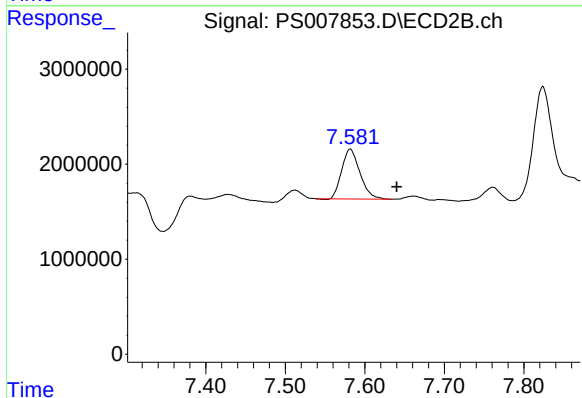


#13 2,4-DB

R.T.: 7.582 min
Delta R.T.: -0.058 min
Response: 8368216
Conc: 17.12 ng/ml

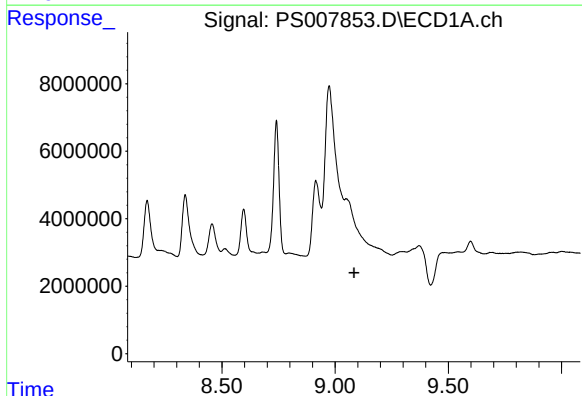


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.083 min
Response: 0
Conc: N.D.

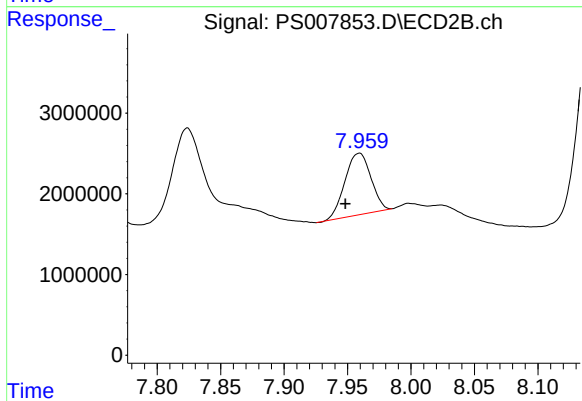

#14 DINOSEB


R.T.: 7.959 min
Delta R.T.: 0.011 min
Response: 10888636
Conc: 3.75 ng/ml

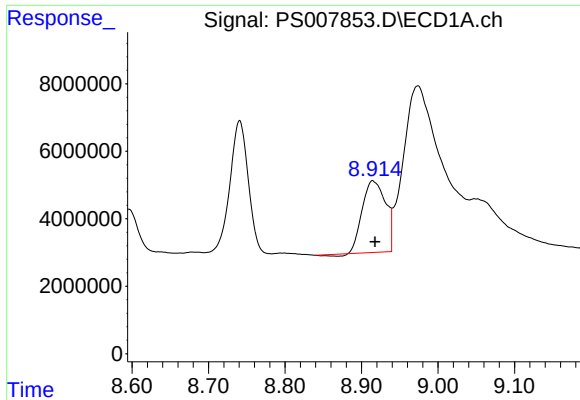

#15 Picloram

R.T.: 8.915 min
Delta R.T.: -0.003 min
Response: 44415133
Conc: 4.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

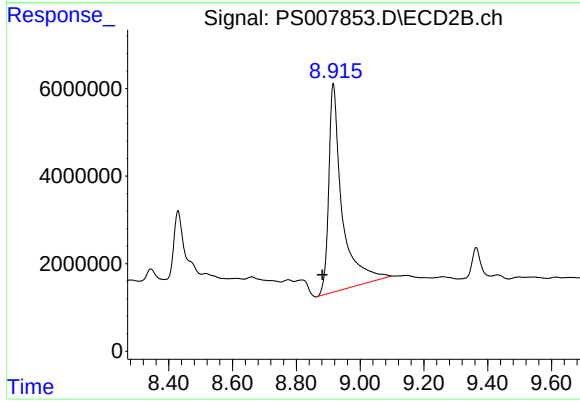

#15 Picloram

R.T.: 8.916 min
Delta R.T.: 0.034 min
Response: 139399612
Conc: 23.79 ng/ml