

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112619\
 Data File : PS007854.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2019 09:08
 Operator : SM\AJ
 Sample : K5999-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 09:44:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.426	5.152	475.7E6	246.7E6	345.411	351.101
Target Compounds							
1) T	Dalapon	1.990	1.697	178.0E6	738.2E6	98.404	621.668 #
2) T	3,5-DICHL...	0.000	4.487	0	44885013	N.D.	49.683
5) T	DICAMBA	5.519	0.000	54914324	0	10.794	N.D. #
7) T	MCPA	5.894	5.521	26230290	21986558	4.765	7.315 #
9) T	2,4-D	0.000	6.055	0	9179643	N.D.	11.384
11) T	2,4,5-TP ...	0.000	6.839	0	14279997	N.D.	3.647
15) T	Picloram	8.890	8.907	77332653	22080732	6.965	3.769 #
16) T	DCPA	0.000	8.907	0	22080732	N.D.	4.226



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112619\
Data File : PS007854.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2019 09:08
Operator : SM\AJ
Sample : K5999-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 09:44:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

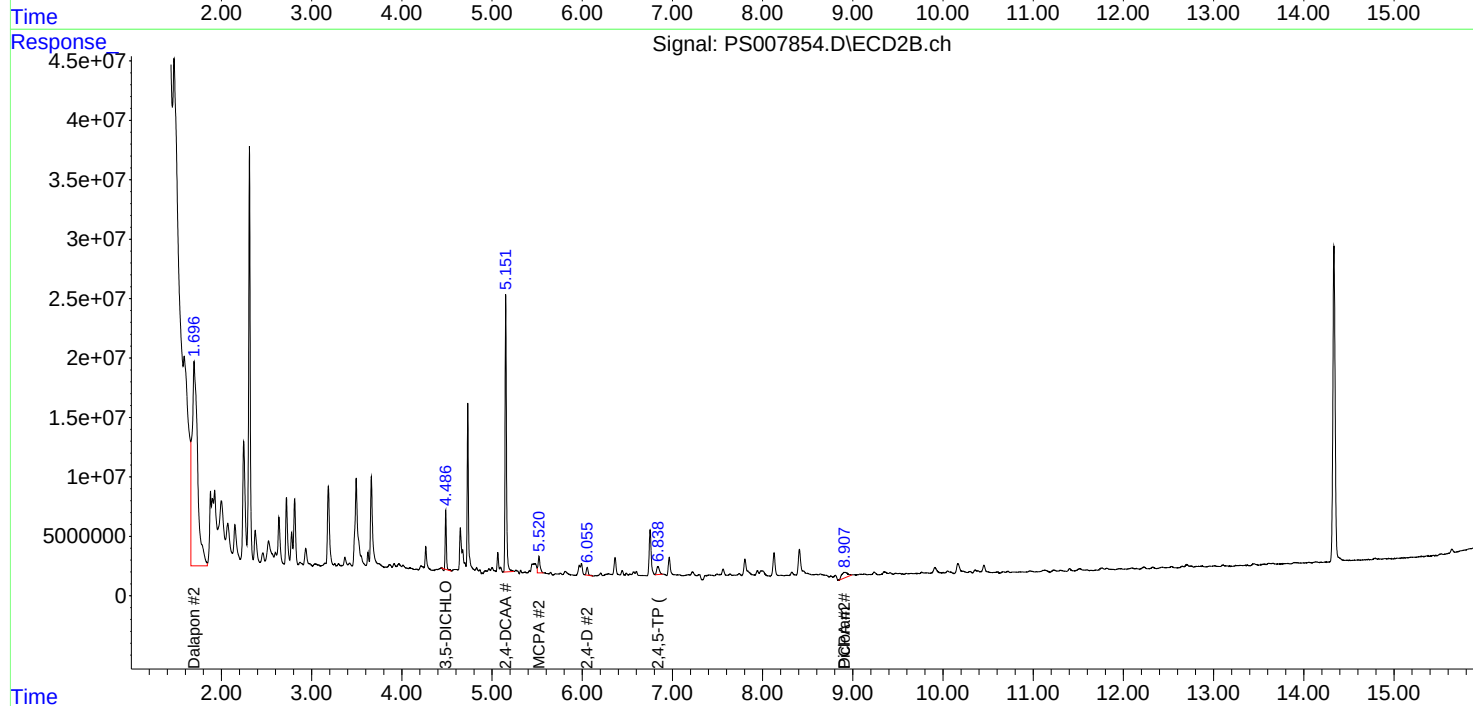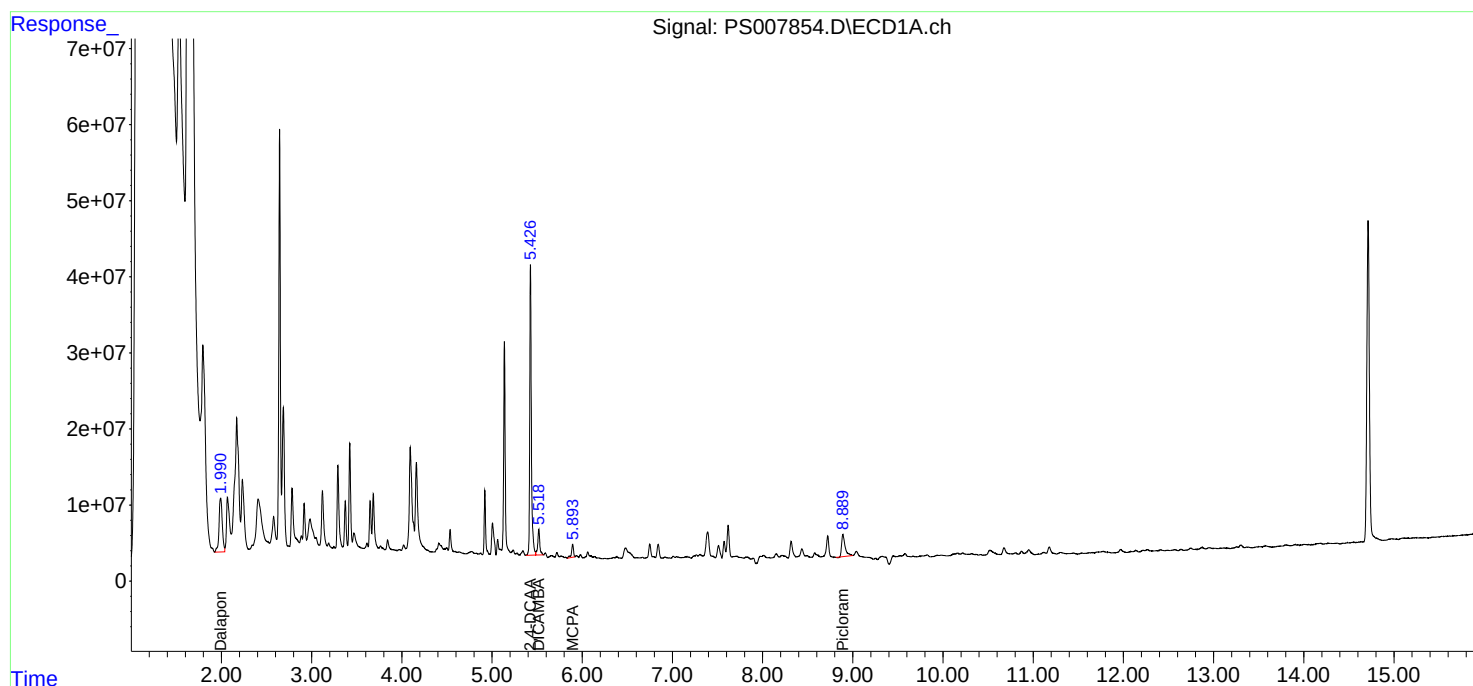


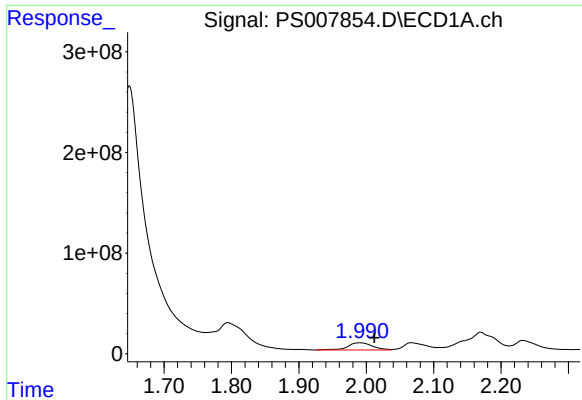

#1 Dalapon


R.T.: 1.990 min
Delta R.T.: -0.022 min
Response: 178029702
Conc: 98.40 ng/ml

Instrument :
ECD_S
ClientSampleId :

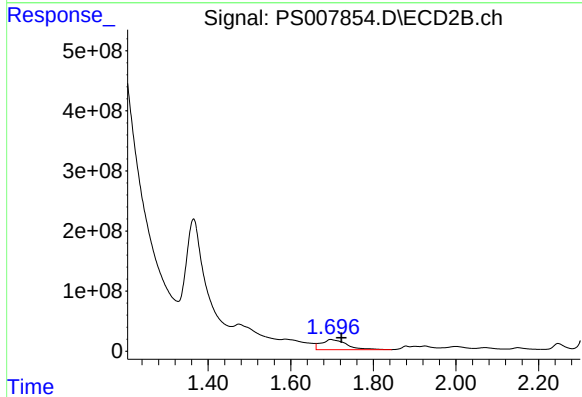


#1 Dalapon

R.T.: 1.697 min
Delta R.T.: -0.026 min
Response: 738170497
Conc: 621.67 ng/ml

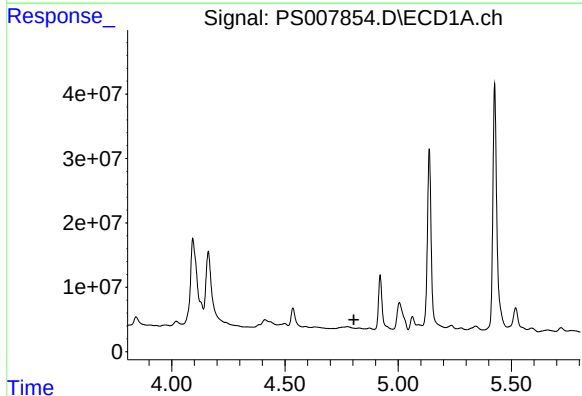


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.804 min
Response: 0
Conc: N.D.

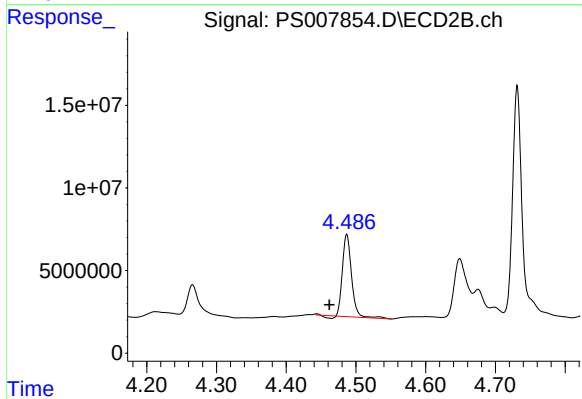

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.487 min
Delta R.T.: 0.025 min
Response: 44885013
Conc: 49.68 ng/ml

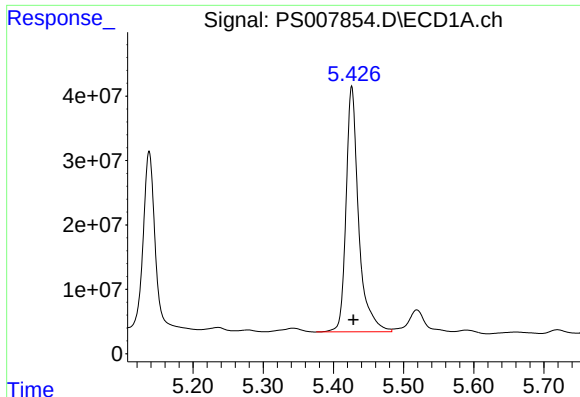

#4 2,4-DCAA


R.T.: 5.426 min
Delta R.T.: -0.002 min
Response: 475694320
Conc: 345.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

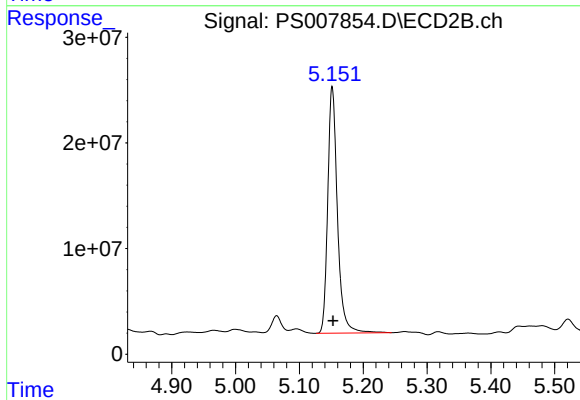


#4 2,4-DCAA

R.T.: 5.152 min
Delta R.T.: -0.001 min
Response: 246671065
Conc: 351.10 ng/ml

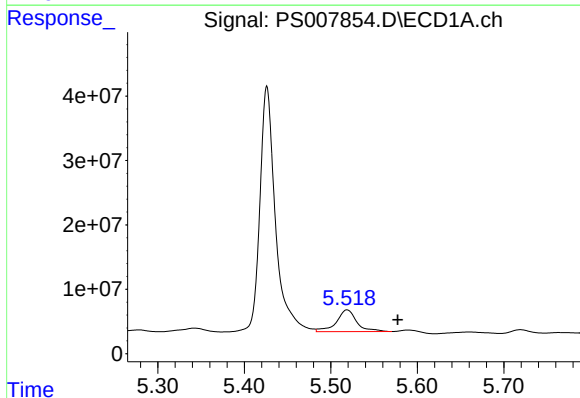


#5 DICAMBA

R.T.: 5.519 min
Delta R.T.: -0.059 min
Response: 54914324
Conc: 10.79 ng/ml

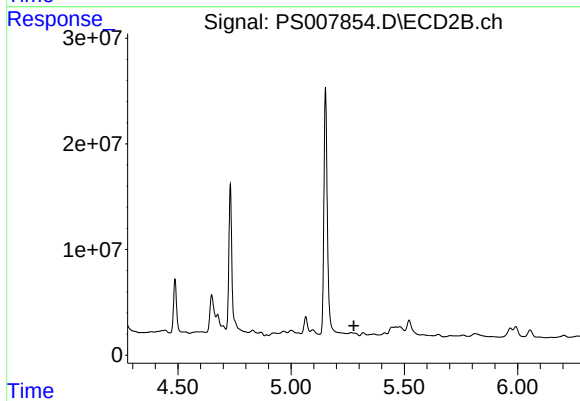

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 5.277 min
Response: 0
Conc: N.D.

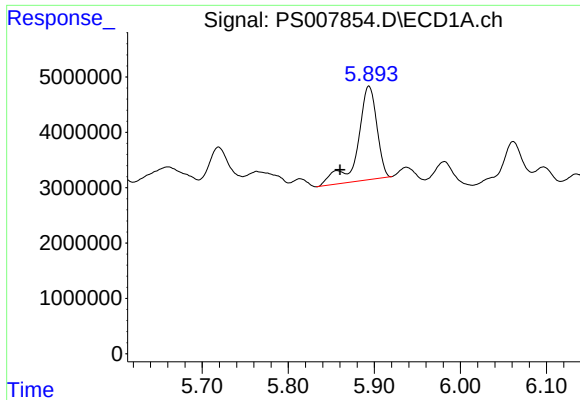

#7 MCPA


R.T.: 5.894 min
Delta R.T.: 0.034 min
Response: 26230290
Conc: 4.77 ug/ml

Instrument :
ECD_S
ClientSampleId :

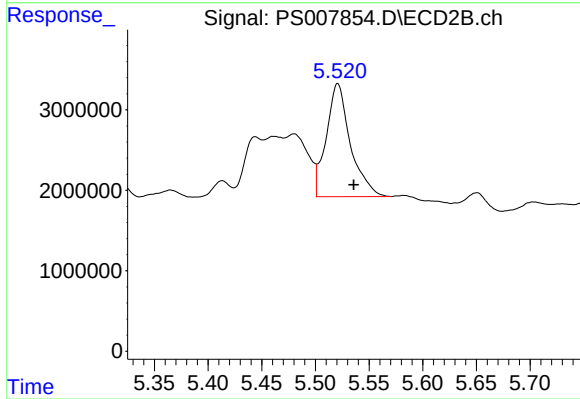


#7 MCPA

R.T.: 5.521 min
Delta R.T.: -0.015 min
Response: 21986558
Conc: 7.31 ug/ml

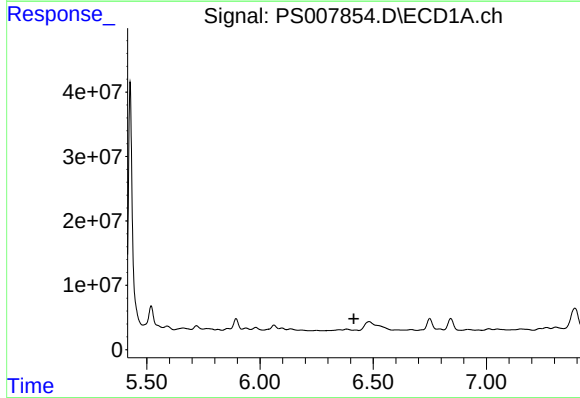


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.414 min
Response: 0
Conc: N.D.

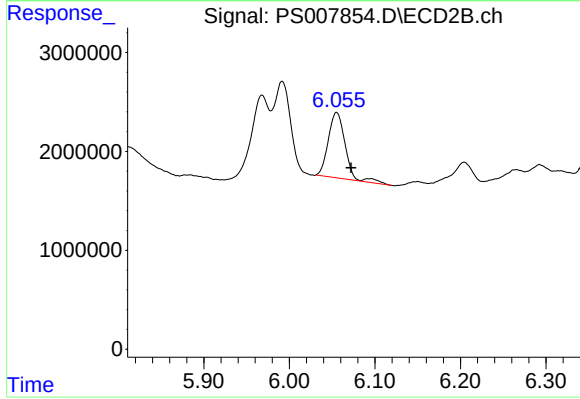

#9 2,4-D


R.T.: 6.055 min
Delta R.T.: -0.017 min
Response: 9179643
Conc: 11.38 ng/ml

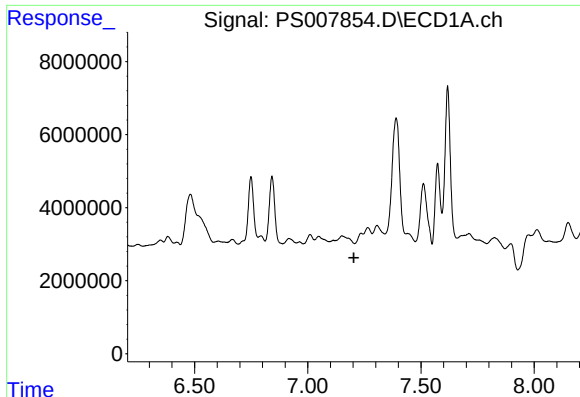

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.203 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

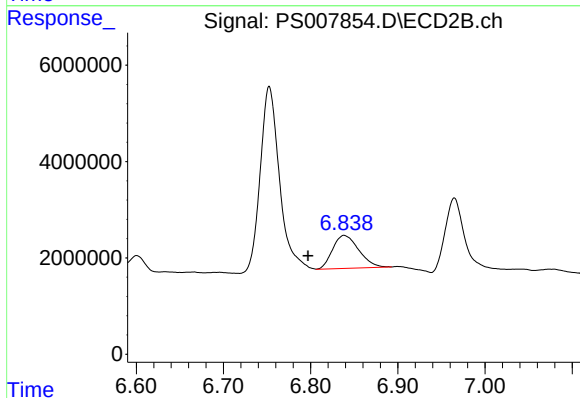


#11 2,4,5-TP (SILVEX)

R.T.: 6.839 min
Delta R.T.: 0.042 min
Response: 14279997
Conc: 3.65 ng/ml

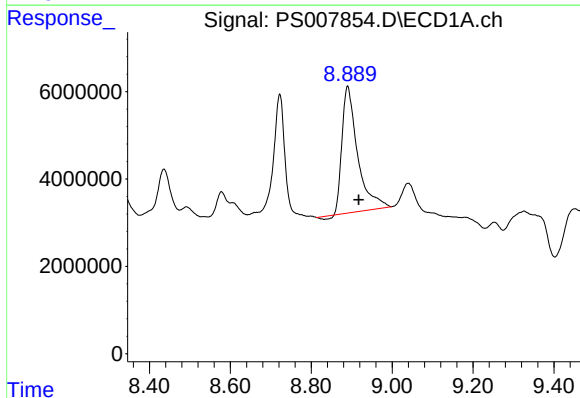


#15 Picloram

R.T.: 8.890 min
Delta R.T.: -0.028 min
Response: 77332653
Conc: 6.96 ng/ml

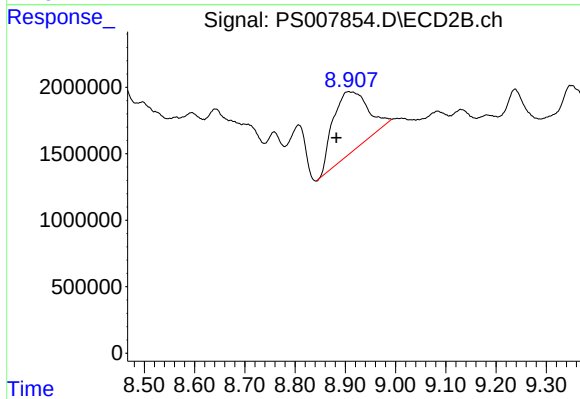

#15 Picloram


R.T.: 8.907 min
Delta R.T.: 0.025 min
Response: 22080732
Conc: 3.77 ng/ml

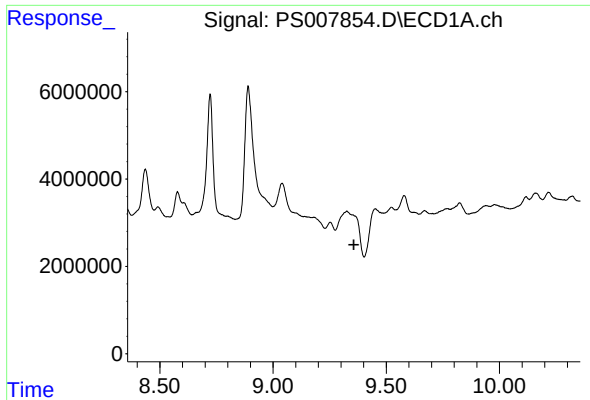

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.357 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

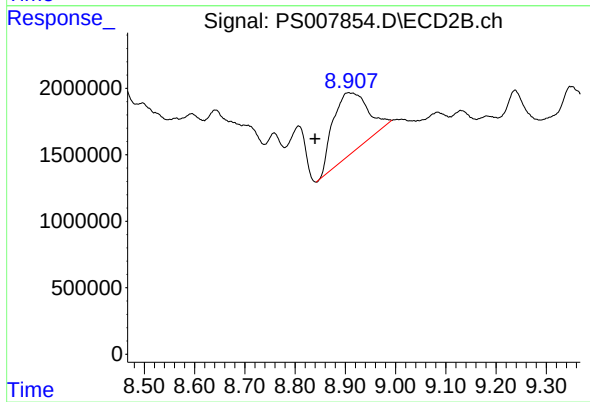

#16 DCPA

R.T.: 8.907 min
Delta R.T.: 0.067 min
Response: 22080732
Conc: 4.23 ng/ml