

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112621\
 Data File : PS017527.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Nov 2021 09:44
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 26 21:38:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111821.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 19 21:46:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.149	0.000	2875623	0	1.829	N.D. #
Target Compounds							
5) T	DICAMBA	7.335	0.000	7883198	0	1.292	N.D. #
8) T	DICHLORPROP	8.026	0.000	3040664	0	1.980	N.D. #
9) T	2,4-D	8.264	0.000	5476109	0	2.931	N.D. #
10) T	Pentachlo...	8.560	8.223	13928735	5943534	<MDL	<MDL #
11) T	2,4,5-TP ...	9.111	0.000	12998538	0	1.560	N.D. #
12) T	2,4,5-T	9.400	8.964	24354287	8328215	2.883	2.504
13) T	2,4-DB	9.950	0.000	10571515	0	6.213	N.D. #
14) T	DINOSEB	11.095	0.000	13308753	0	2.137	N.D. #
15) T	Picloram	10.928	10.776	161.9E6	51872890	13.277	11.888
16) T	DCPA	11.363	10.720	20207426	7691213	1.892	1.745



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112621\
Data File : PS017527.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Nov 2021 09:44
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 26 21:38:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111821.M
Quant Title : 8080.M
QLast Update : Fri Nov 19 21:46:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

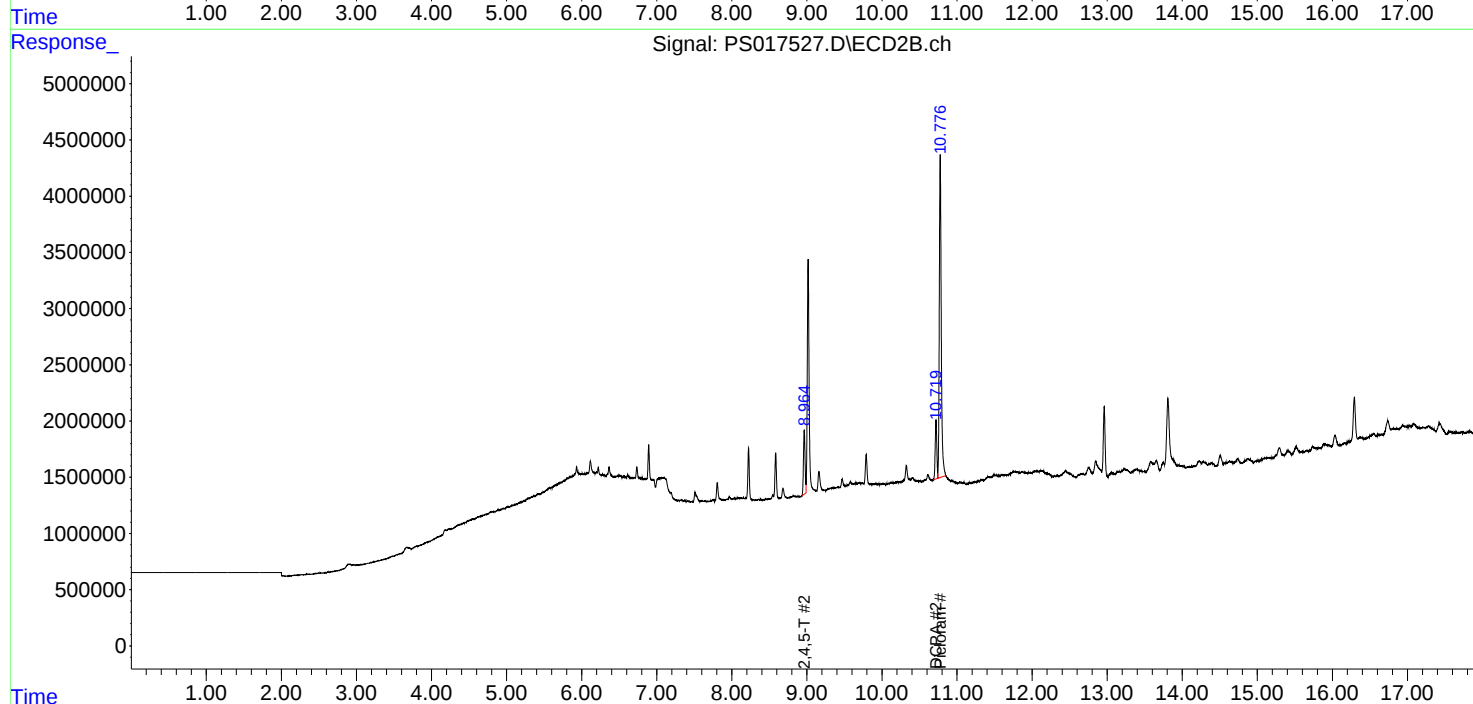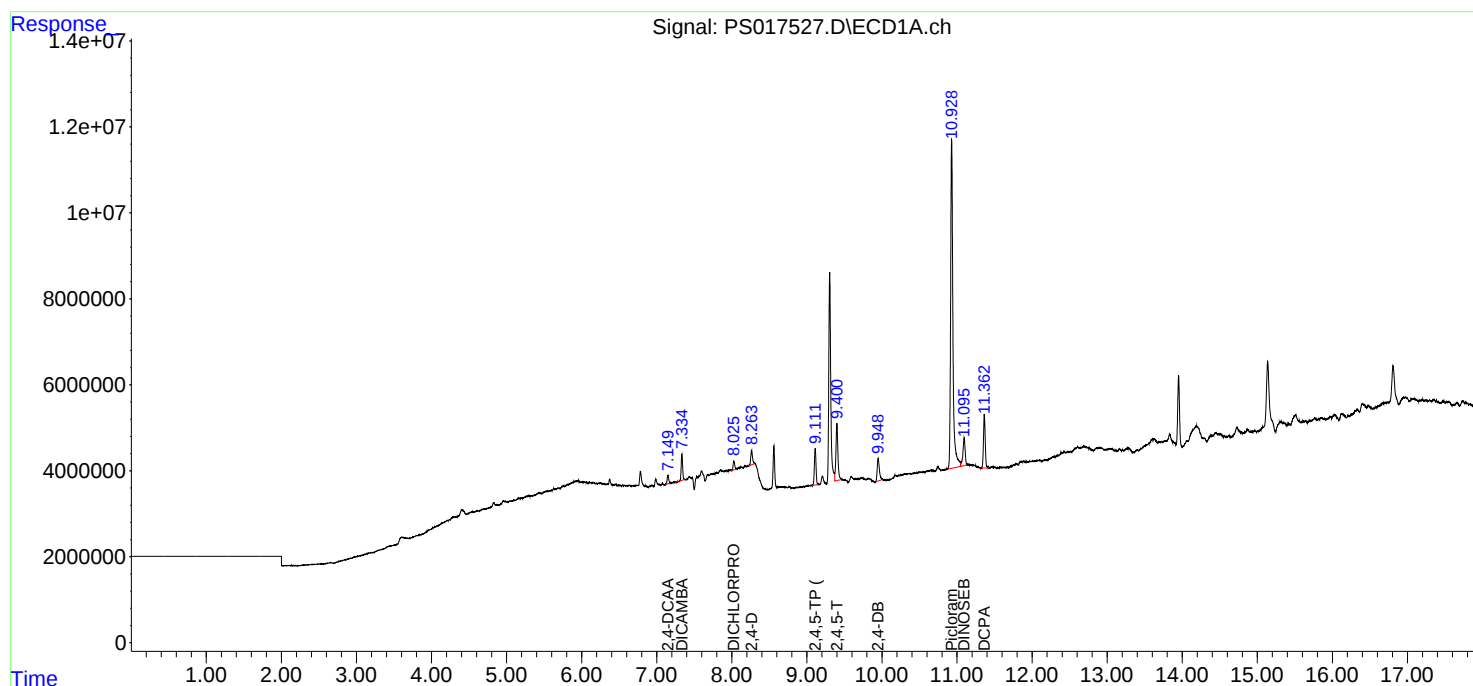


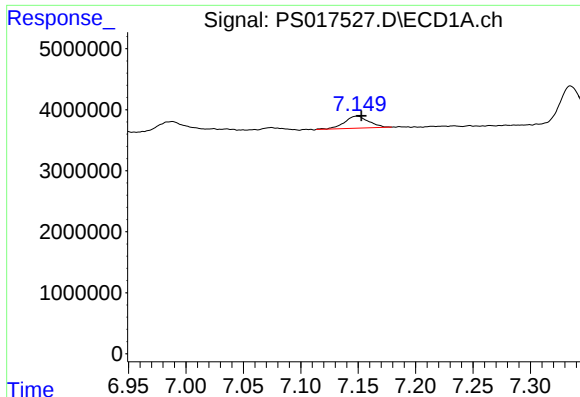

#4 2,4-DCAA


R.T.: 7.149 min
Delta R.T.: -0.003 min
Response: 2875623
Conc: 1.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

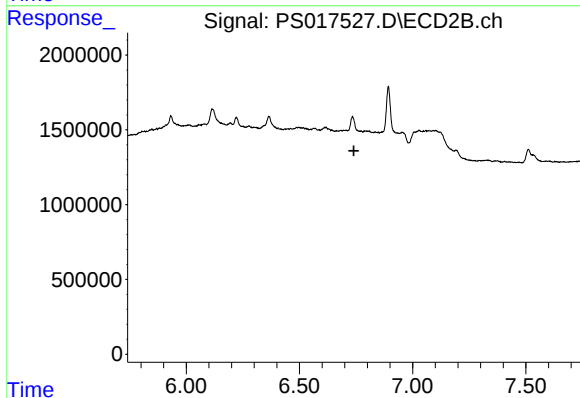


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.740 min
Response: 0
Conc: N.D.

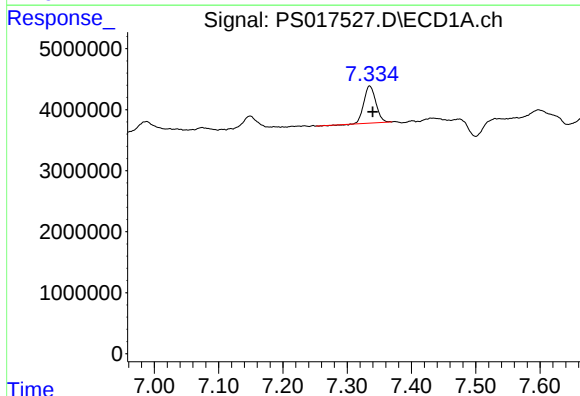


#5 DICAMBA

R.T.: 7.335 min
Delta R.T.: -0.005 min
Response: 7883198
Conc: 1.29 ng/ml

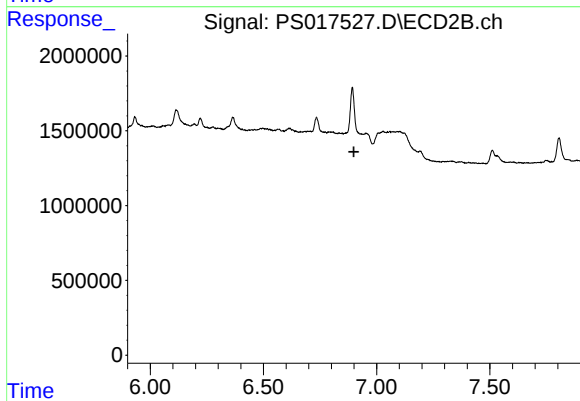

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 6.900 min
Response: 0
Conc: N.D.

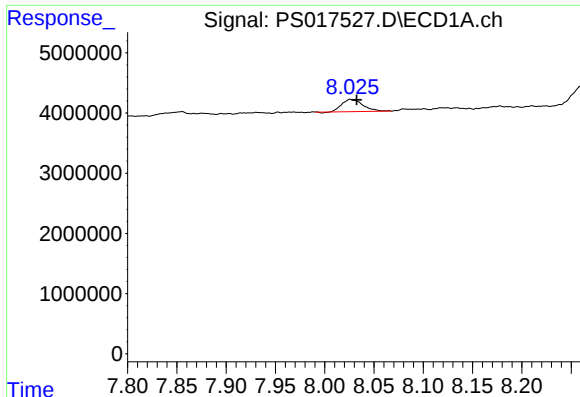

#8 DICHLORPROP


R.T.: 8.026 min
Delta R.T.: -0.007 min
Response: 3040664
Conc: 1.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

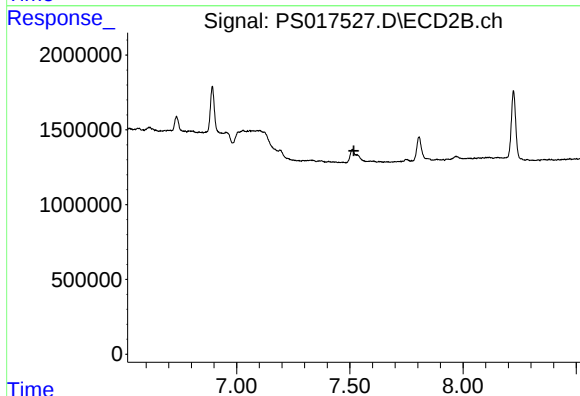


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.518 min
Response: 0
Conc: N.D.

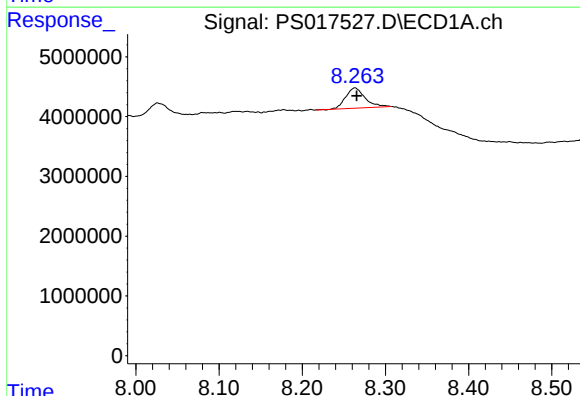


#9 2,4-D

R.T.: 8.264 min
Delta R.T.: -0.002 min
Response: 5476109
Conc: 2.93 ng/ml

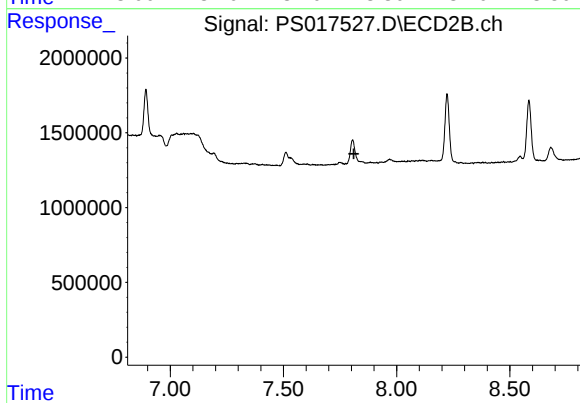

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.811 min
Response: 0
Conc: N.D.

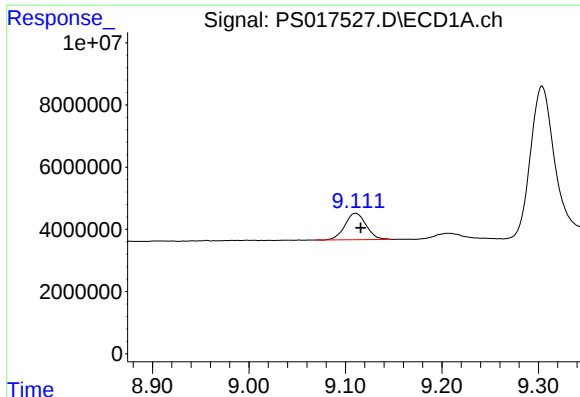

#11 2,4,5-TP (SILVEX)


R.T.: 9.111 min
Delta R.T.: -0.005 min
Response: 12998538
Conc: 1.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

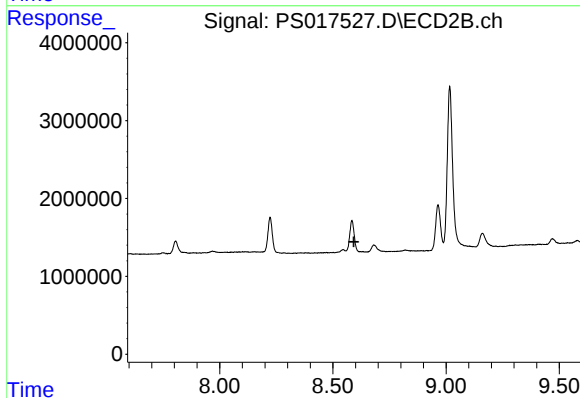


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 8.593 min
Response: 0
Conc: N.D.

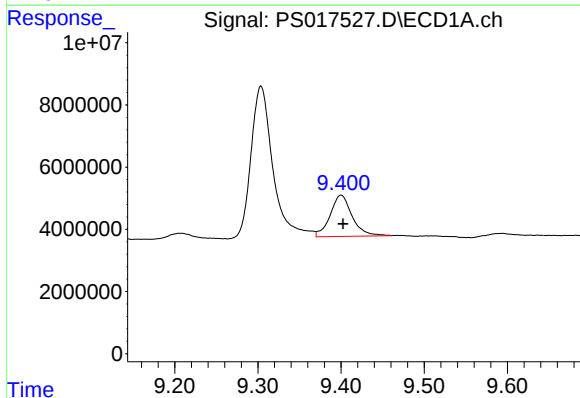


#12 2,4,5-T

R.T.: 9.400 min
Delta R.T.: -0.003 min
Response: 24354287
Conc: 2.88 ng/ml

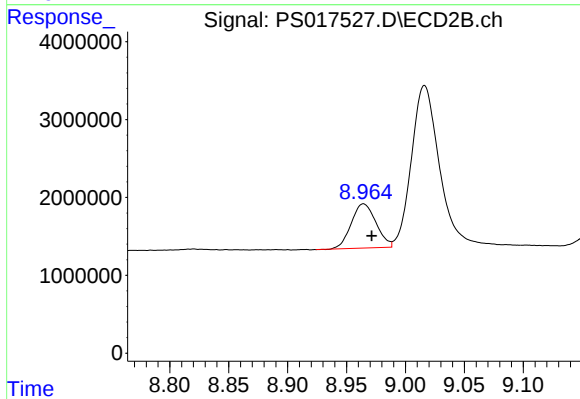

#12 2,4,5-T


R.T.: 8.964 min
Delta R.T.: -0.007 min
Response: 8328215
Conc: 2.50 ng/ml

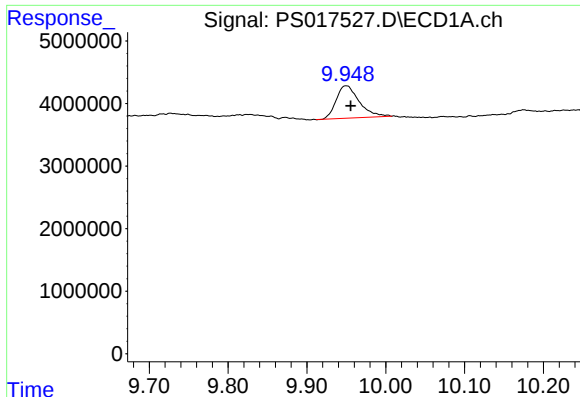

#13 2,4-DB


R.T.: 9.950 min
Delta R.T.: -0.006 min
Response: 10571515
Conc: 6.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

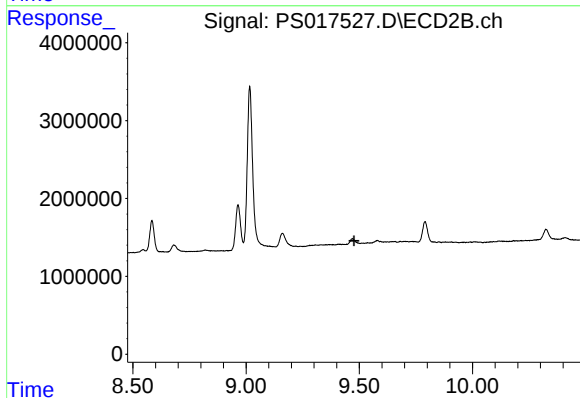


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.477 min
Response: 0
Conc: N.D.

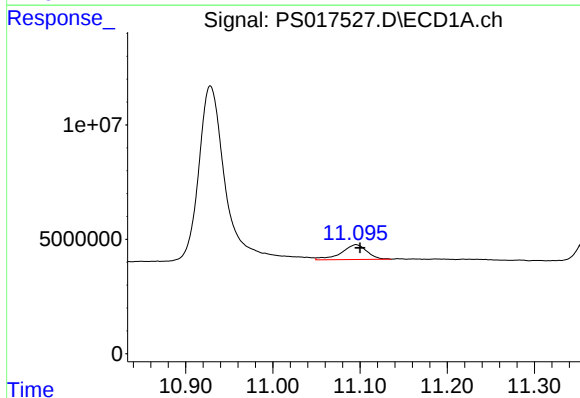


#14 DINOSEB

R.T.: 11.095 min
Delta R.T.: -0.005 min
Response: 13308753
Conc: 2.14 ng/ml

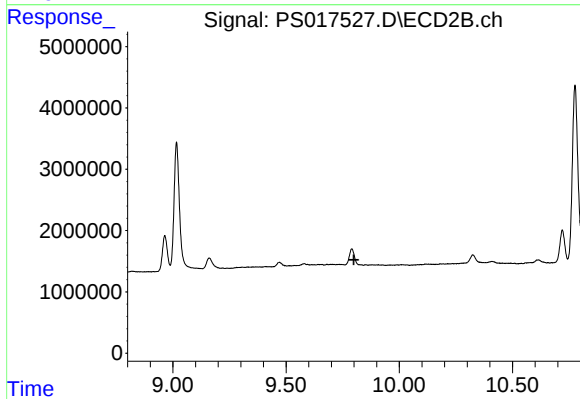

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.799 min
Response: 0
Conc: N.D.

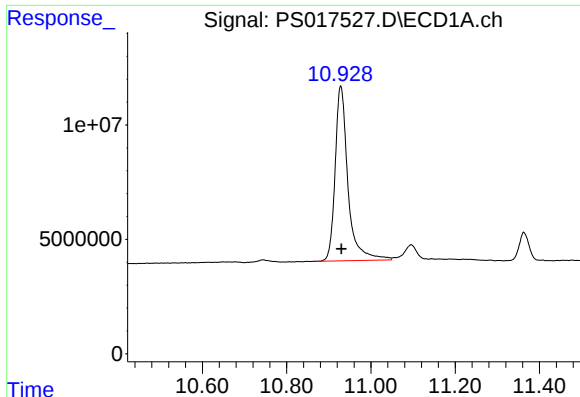

#15 Picloram


R.T.: 10.928 min
Delta R.T.: -0.002 min
Response: 161884080
Conc: 13.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

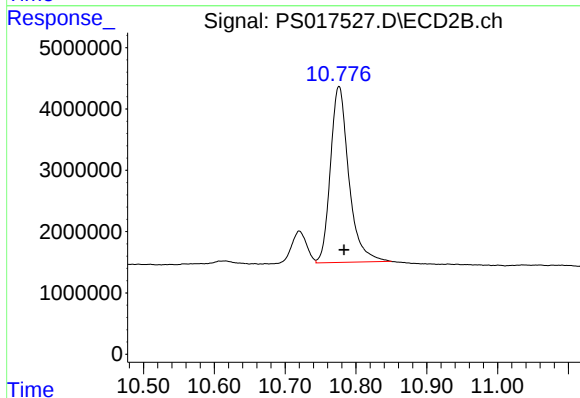


#15 Picloram

R.T.: 10.776 min
Delta R.T.: -0.007 min
Response: 51872890
Conc: 11.89 ng/ml

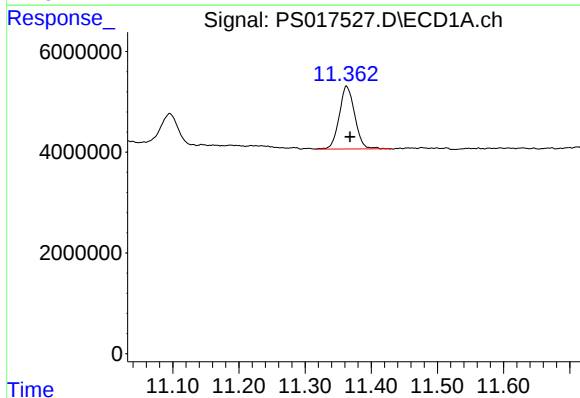

#16 DCPA

R.T.: 11.363 min
Delta R.T.: -0.005 min
Response: 20207426
Conc: 1.89 ng/ml

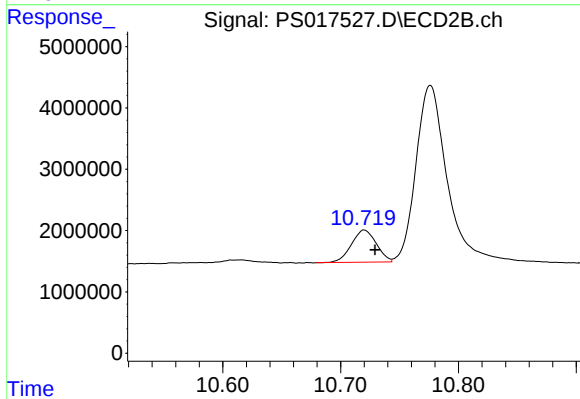

#16 DCPA

R.T.: 10.720 min
Delta R.T.: -0.009 min
Response: 7691213
Conc: 1.75 ng/ml