

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112624\
 Data File : PS028647.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Nov 2024 20:25
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 00:21:07 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 26 14:44:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.226	7.723	1329.9E6	676.4E6	495.809	502.153
Target Compounds							
1) T	Dalapon	2.671f	2.724f	20128970	4464048	6.937	2.044 #
3) T	4-Nitroph...	7.021	0.000	5041075	0	2.933	N.D. #
5) T	DICAMBA	0.000	7.920	0	3262307	N.D.	<MDL
8) T	DICHLORPROP	8.127	8.688f	310909	4480754	<MDL	2.803 #
10) T	Pentachlo...	8.649	0.000	3911984	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.229	9.873	2884389	2384165	<MDL	<MDL #
12) T	2,4,5-T	9.523	10.293	3038160	2245186	<MDL	<MDL #
13) T	2,4-DB	10.110	0.000	526522	0	<MDL	N.D. #
14) T	DINOSEB	11.302	0.000	1962600	0	<MDL	N.D. #
15) T	Picloram	11.119	12.334	22177447	5832495	<MDL	<MDL #
16) T	DCPA	11.595	0.000	4200086	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112624\
Data File : PS028647.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Nov 2024 20:25
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 00:21:07 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
Quant Title : 8080.M
QLast Update : Tue Nov 26 14:44:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

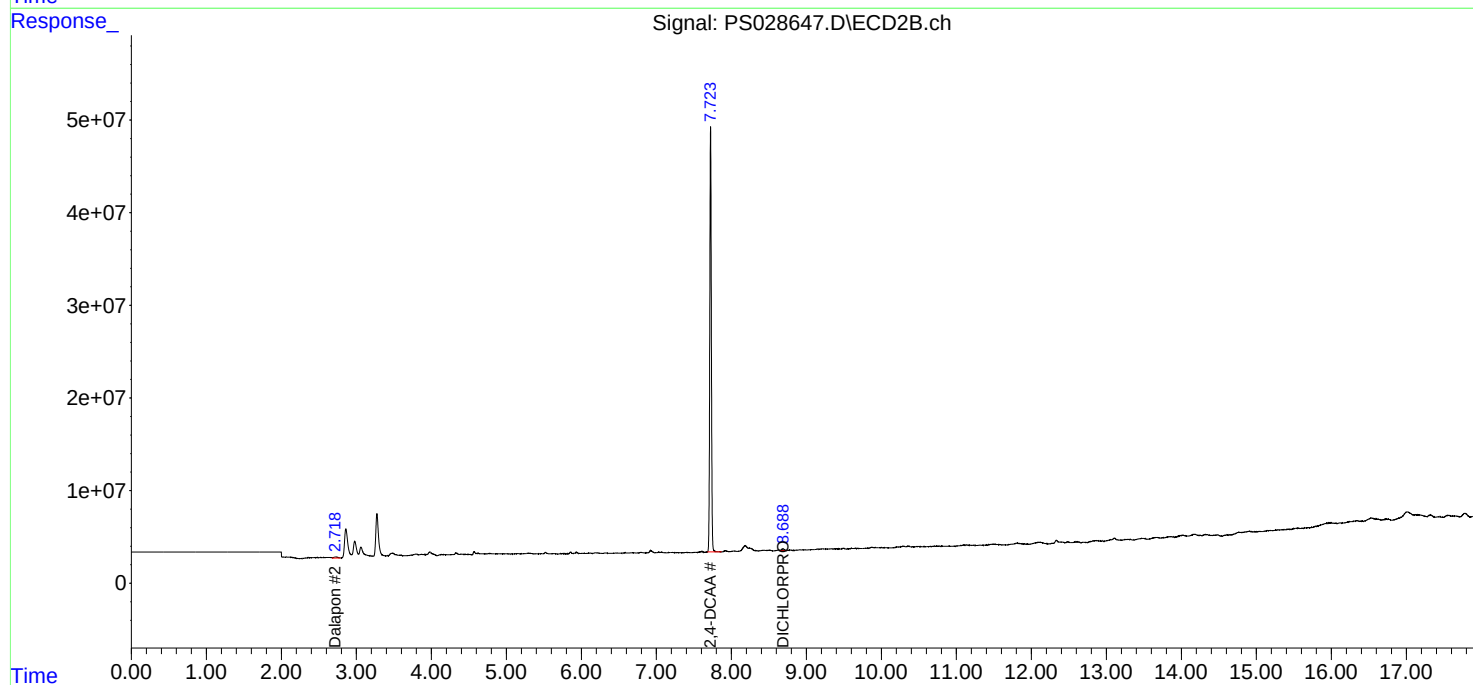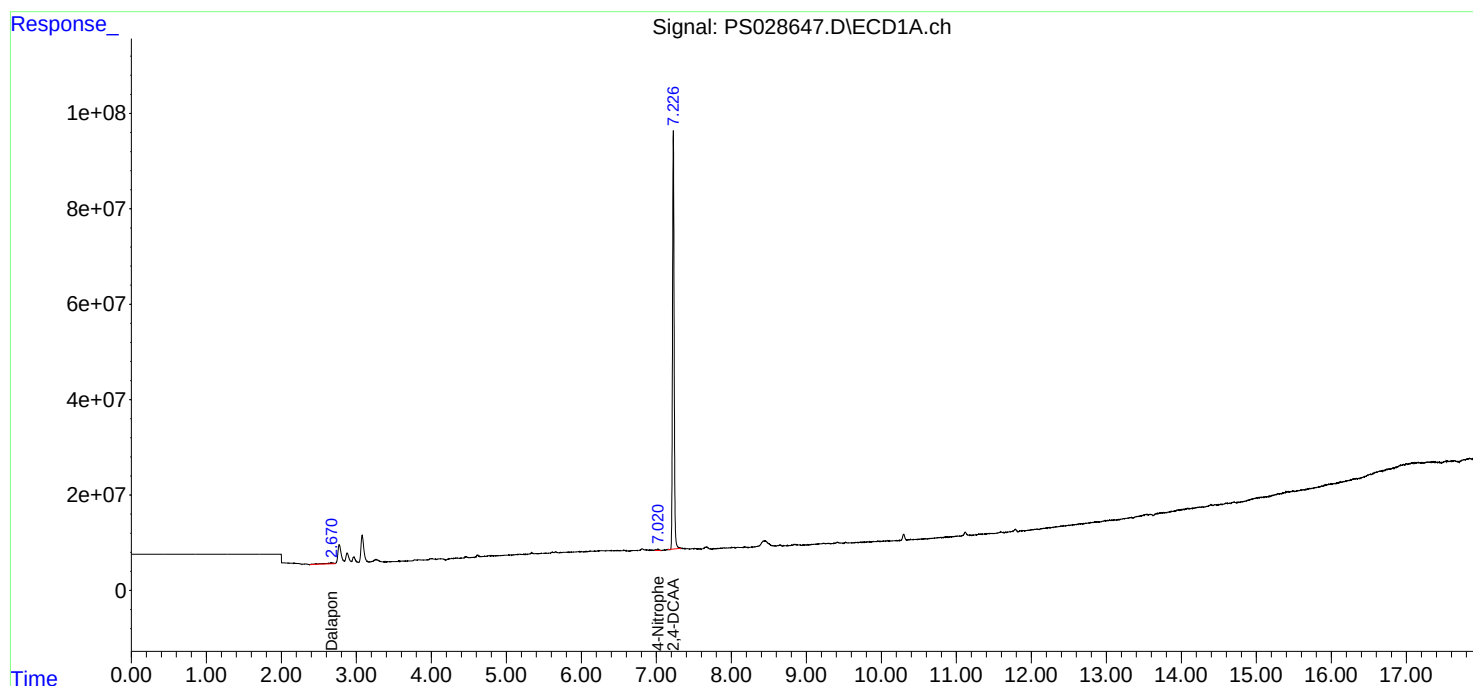


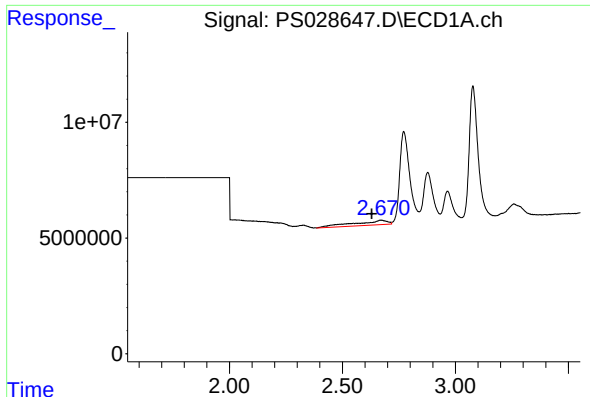

#1 Dalapon


R.T.: 2.671 min
Delta R.T.: 0.041 min
Response: 20128970
Conc: 6.94 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

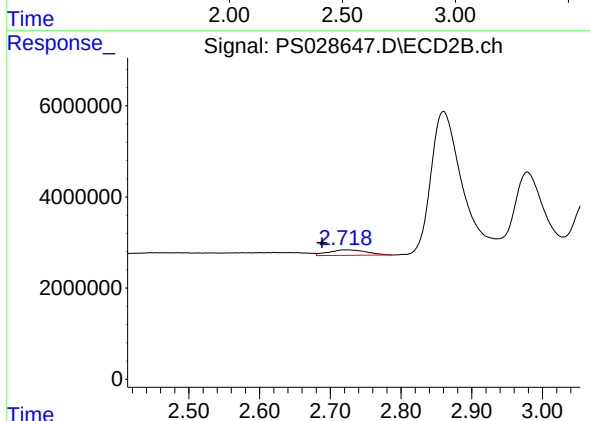


#1 Dalapon

R.T.: 2.724 min
Delta R.T.: 0.036 min
Response: 4464048
Conc: 2.04 ng/ml

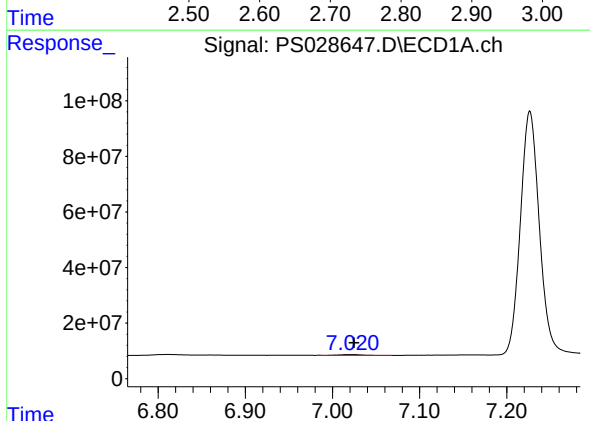


#3 4-Nitrophenol

R.T.: 7.021 min
Delta R.T.: -0.004 min
Response: 5041075
Conc: 2.93 ng/ml

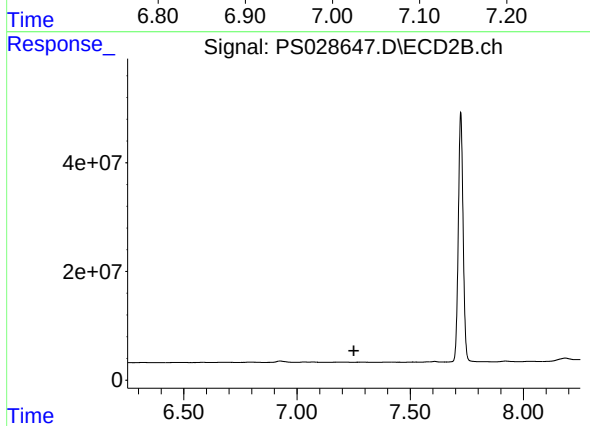

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.251 min
Response: 0
Conc: N.D.

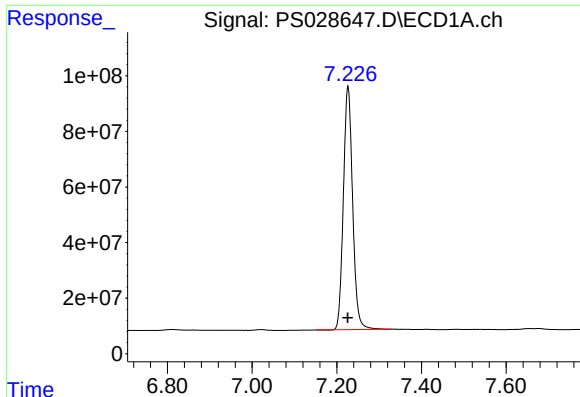

#4 2,4-DCAA


R.T.: 7.226 min
Delta R.T.: 0.000 min
Response: 1329928965
Conc: 495.81 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

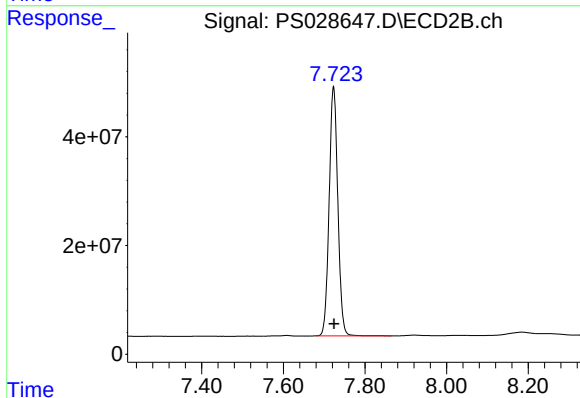


#4 2,4-DCAA

R.T.: 7.723 min
Delta R.T.: -0.001 min
Response: 676414948
Conc: 502.15 ng/ml

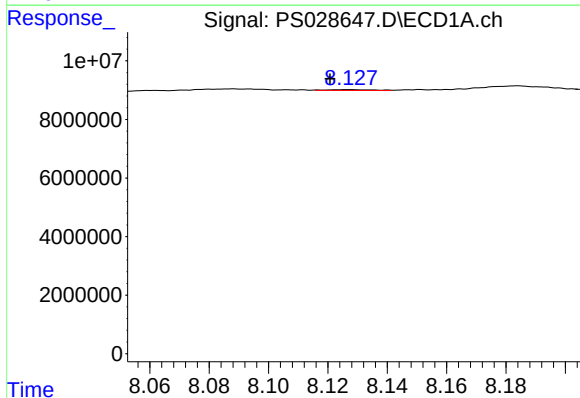

#8 DICHLORPROP

R.T.: 8.127 min
Delta R.T.: 0.006 min
Response: 310909
Conc: N.D.

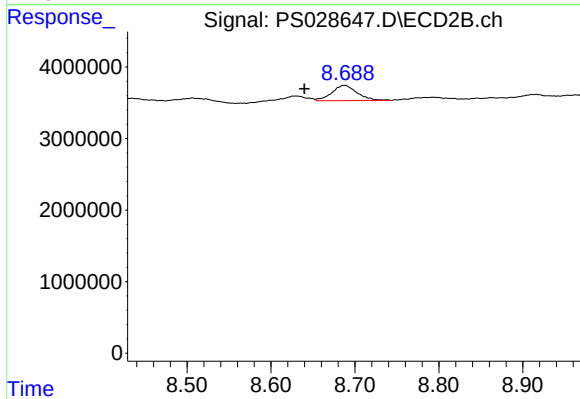

#8 DICHLORPROP

R.T.: 8.688 min
Delta R.T.: 0.048 min
Response: 4480754
Conc: 2.80 ng/ml