

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112624\
 Data File : PS028654.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Nov 2024 23:13
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 00:28:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 26 14:44:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.227	7.724	1323.4E6	671.3E6	493.392	498.330
Target Compounds							
1) T	Dalapon	2.671f	0.000	14742584	0	5.080	N.D. #
2) T	3,5-DICHL...	6.382	0.000	779000	0	<MDL	N.D. #
3) T	4-Nitroph...	7.022	0.000	4793913	0	2.789	N.D. #
5) T	DICAMBA	7.412	7.921	540447	3594569	<MDL	<MDL #
8) T	DICHLORPROP	8.085f	8.689f	315482	4826024	<MDL	3.019 #
10) T	Pentachlo...	8.650	0.000	2933935	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.230	9.873	2538547	3838868	<MDL	<MDL #
12) T	2,4,5-T	9.528	10.293	7130369	5794341	<MDL	<MDL #
13) T	2,4-DB	10.104	0.000	1002272	0	<MDL	N.D. #
14) T	DINOSEB	11.306	0.000	2575709	0	<MDL	N.D. #
15) T	Picloram	11.123	12.335	17211692	6746445	<MDL	<MDL #
16) T	DCPA	11.596	0.000	4729310	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112624\
Data File : PS028654.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Nov 2024 23:13
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 00:28:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
Quant Title : 8080.M
QLast Update : Tue Nov 26 14:44:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

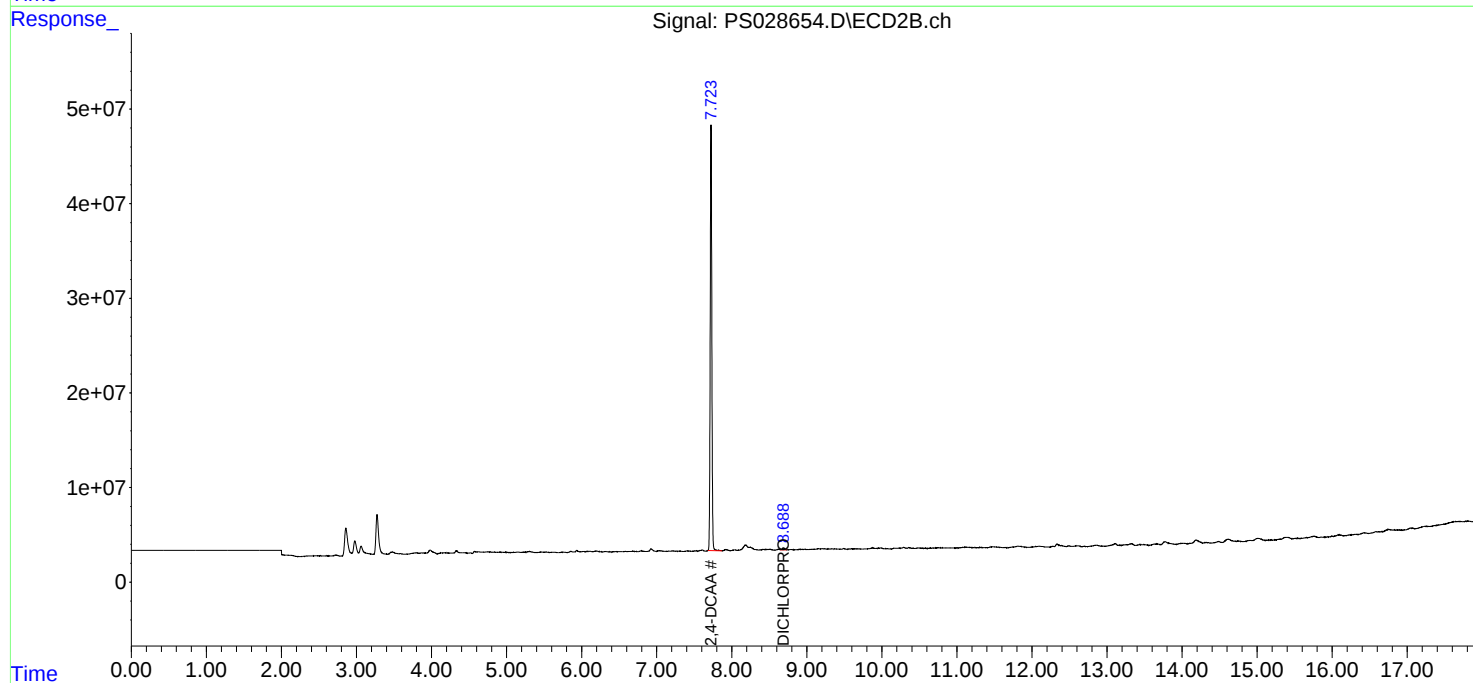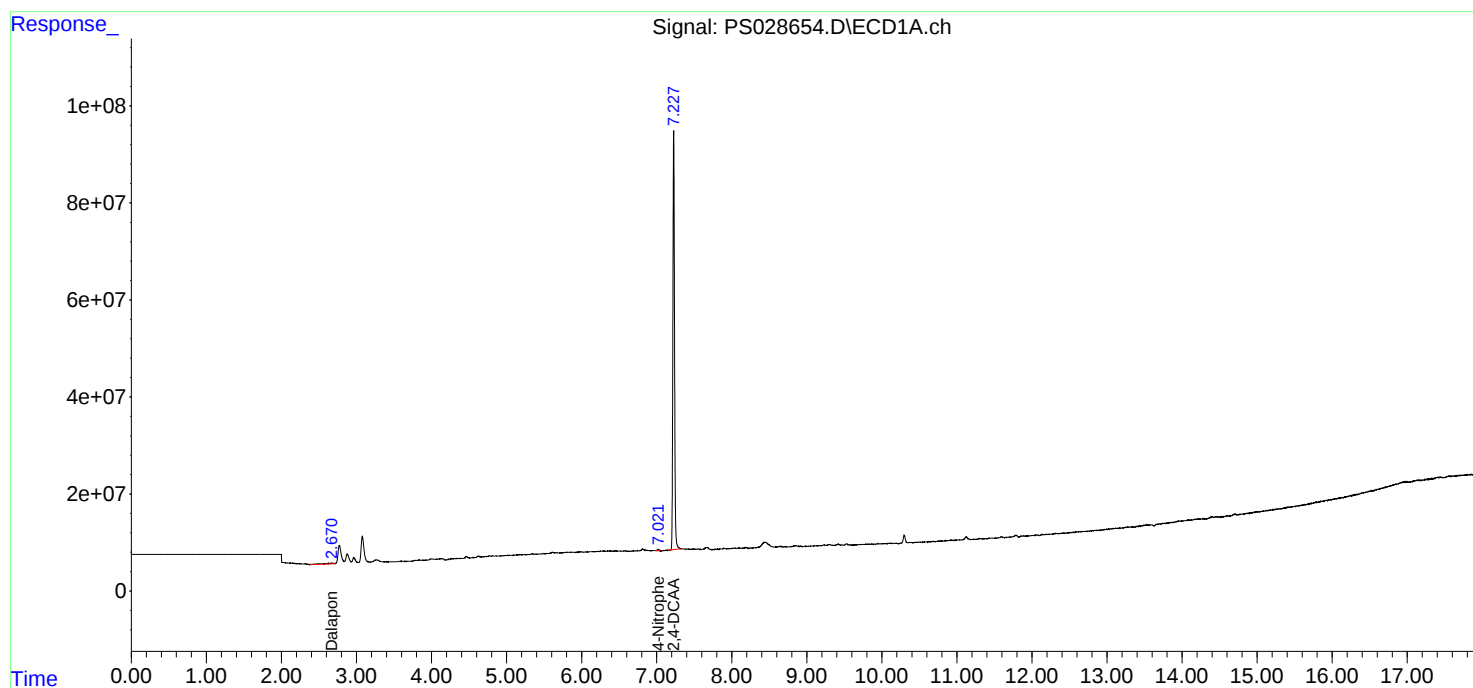


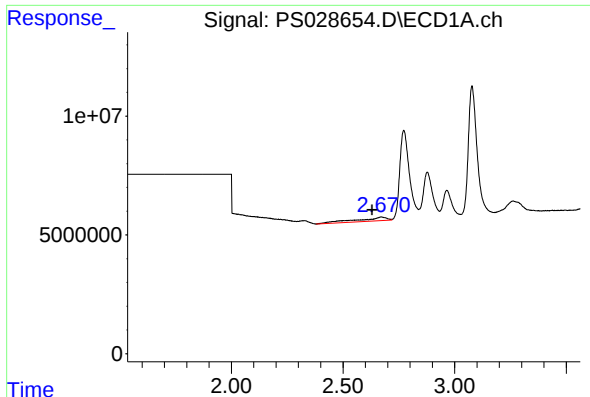

#1 Dalapon


R.T.: 2.671 min
Delta R.T.: 0.041 min
Response: 14742584
Conc: 5.08 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

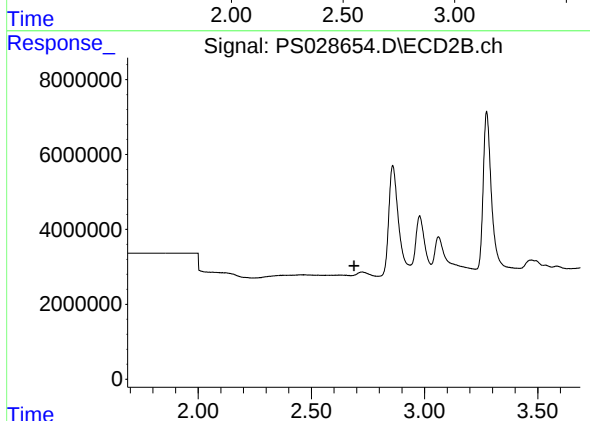


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.688 min
Response: 0
Conc: N.D.

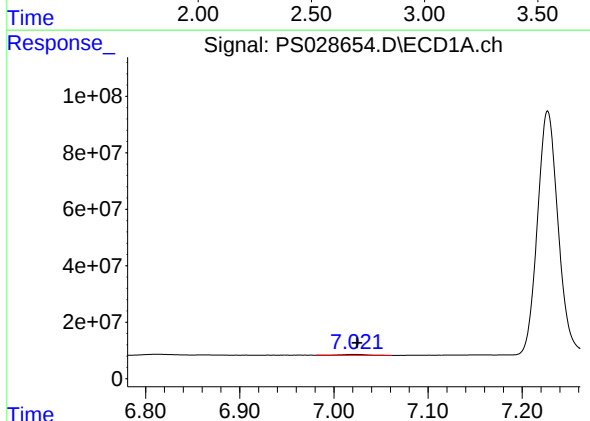


#3 4-Nitrophenol

R.T.: 7.022 min
Delta R.T.: -0.003 min
Response: 4793913
Conc: 2.79 ng/ml

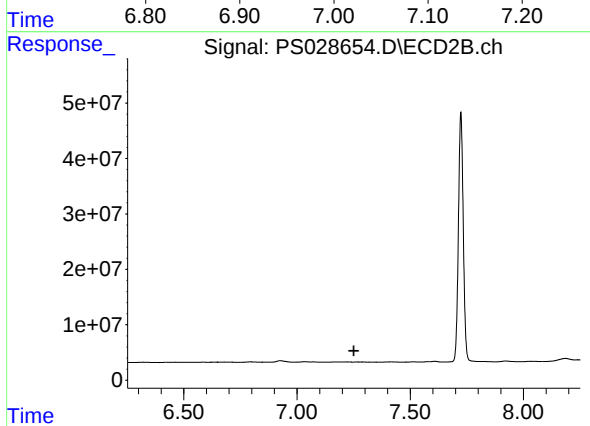

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.251 min
Response: 0
Conc: N.D.

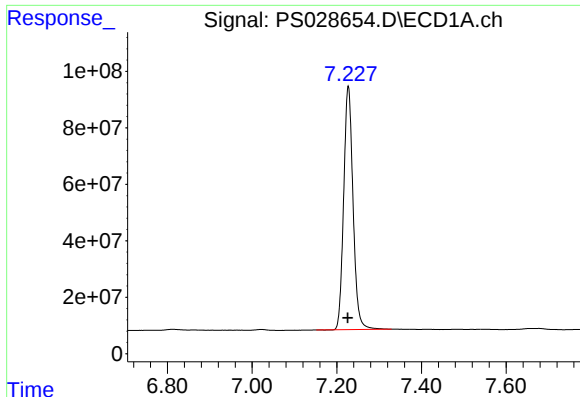

#4 2,4-DCAA


R.T.: 7.227 min
Delta R.T.: 0.001 min
Response: 1323446552
Conc: 493.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

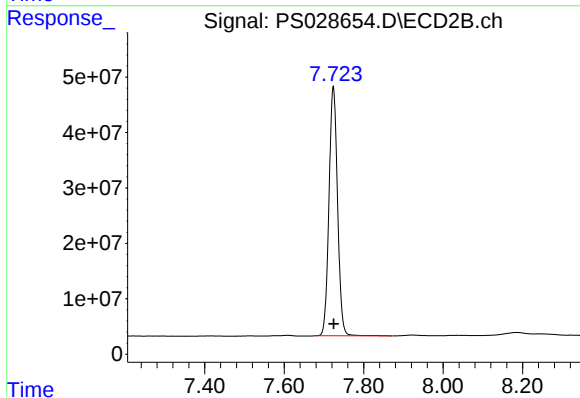


#4 2,4-DCAA

R.T.: 7.724 min
Delta R.T.: 0.000 min
Response: 671265401
Conc: 498.33 ng/ml

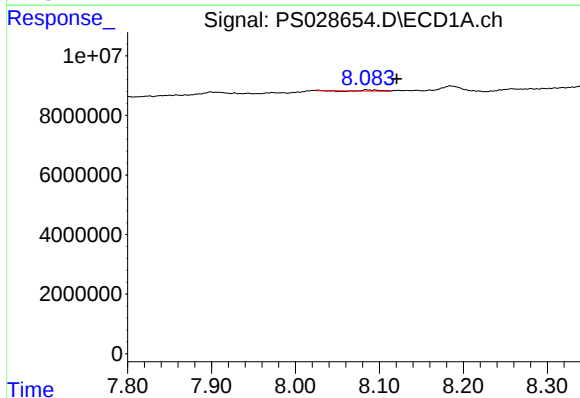

#8 DICHLORPROP

R.T.: 8.085 min
Delta R.T.: -0.036 min
Response: 315482
Conc: N.D.

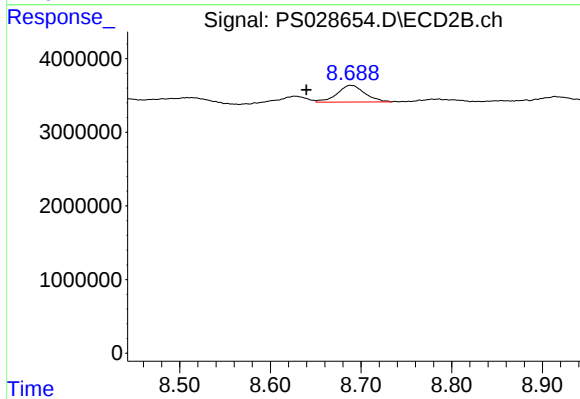

#8 DICHLORPROP

R.T.: 8.689 min
Delta R.T.: 0.049 min
Response: 4826024
Conc: 3.02 ng/ml