

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112624\
 Data File : PS0TEST BS.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Nov 2024 17:13
 Operator : AR\AJ
 Sample : BS TEST
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 08:41:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 26 14:44:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.226	7.724	927.2E6	427.8E6	345.674	317.604
Target Compounds							
2) T	3,5-DICHL...	6.399	6.680	983.2E6	505.2E6	256.728	257.241
3) T	4-Nitroph...	7.024	7.250	351.4E6	201.5E6	204.440	220.914
5) T	DICAMBA	7.413	7.923	2543.2E6	1445.8E6	221.522	234.852
6) T	MCPD	7.592	8.023	146.5E6	92461136	20.072	21.465
7) T	MCPA	7.741	8.266	210.4E6	213.3E6	20.349	34.367 #
8) T	DICHLORPROP	8.120	8.638	781.5E6	422.3E6	251.024	264.185
9) T	2,4-D	8.350	8.968	1044.4E6	477.9E6	309.724	282.630
10) T	Pentachlo...	8.649	9.496	10850.7E6	5639.6E6	246.090	246.367
11) T	2,4,5-TP ...	9.228	9.872	4292.2E6	2547.6E6	234.807	266.970
12) T	2,4,5-T	9.519	10.292	4500.3E6	2395.3E6	239.946	257.275
13) T	2,4-DB	10.094	10.858	650.5E6	249.4E6	183.663	217.488
14) T	DINOSEB	11.303	11.240	540.3E6	293.0E6	35.959	46.678 #
15) T	Picloram	11.110	12.329	6987.5E6	2767.1E6	234.978	214.658
16) T	DCPA	11.595	12.280	4457.2E6	2985.6E6	162.109	269.038 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112624\
Data File : PS0TEST BS.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Nov 2024 17:13
Operator : AR\AJ
Sample : BS TEST
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 08:41:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
Quant Title : 8080.M
QLast Update : Tue Nov 26 14:44:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

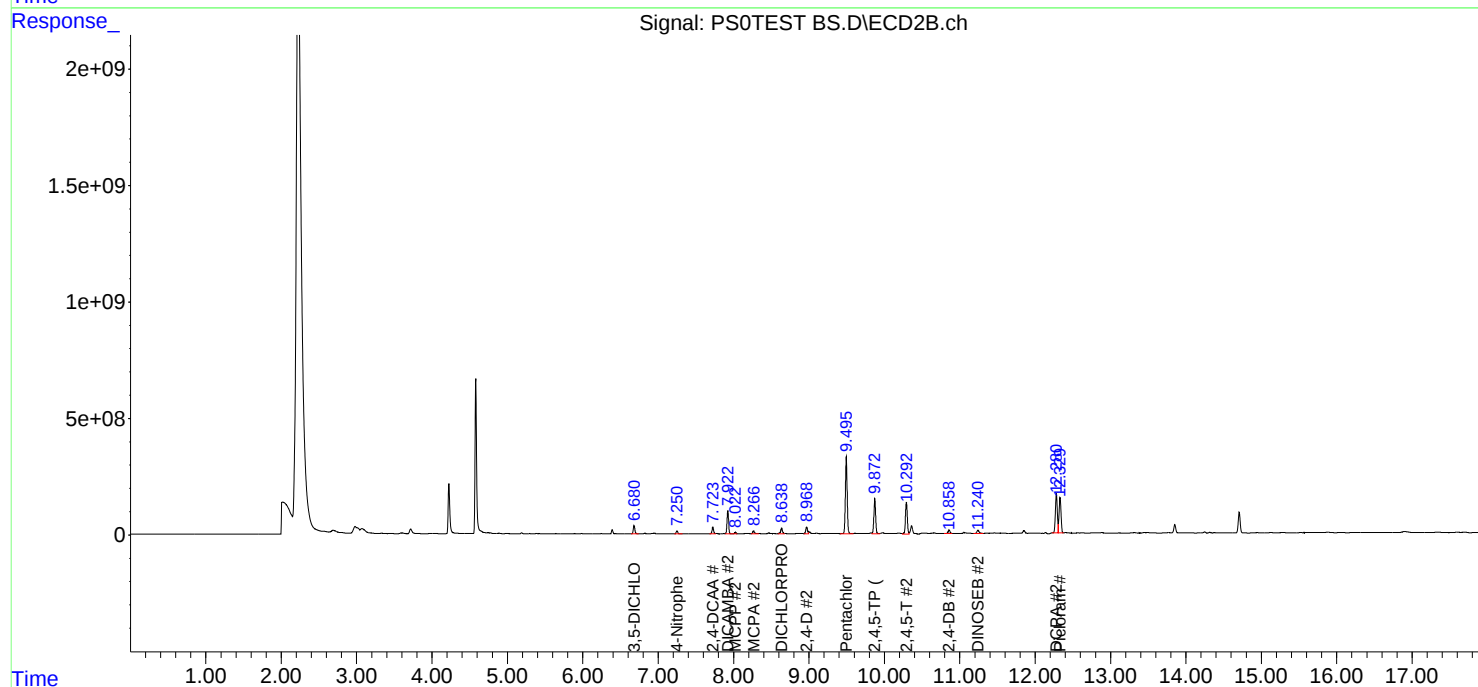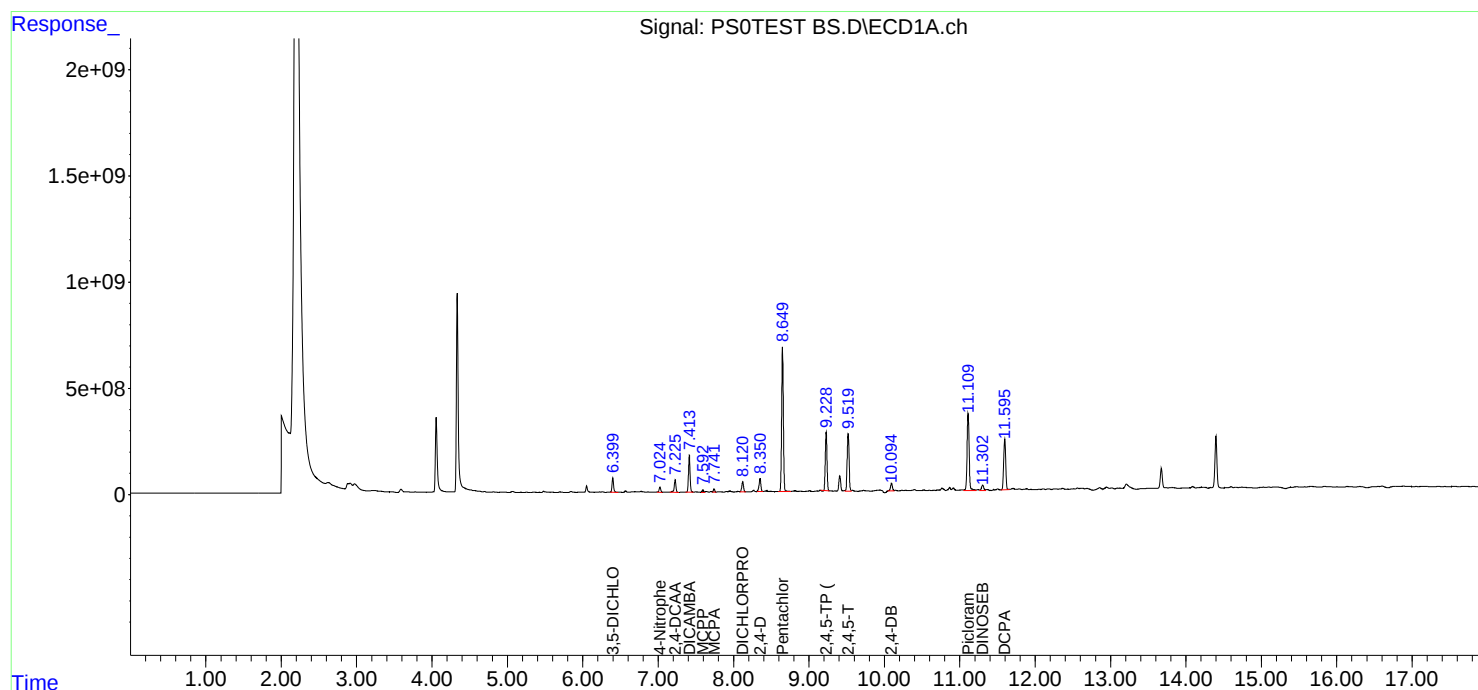


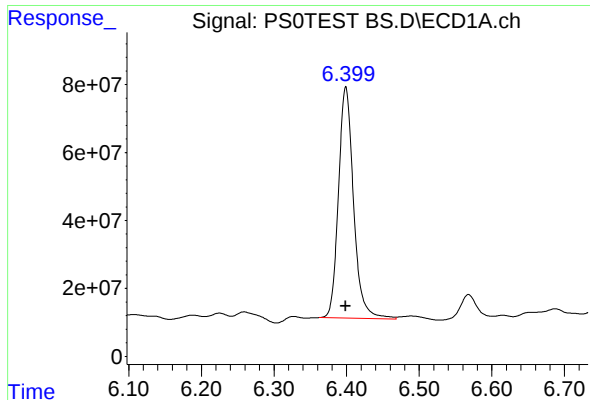

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.399 min
Delta R.T.: 0.000 min
Response: 983179500
Conc: 256.73 ng/ml

Instrument :
ECD_S
ClientSampleId :

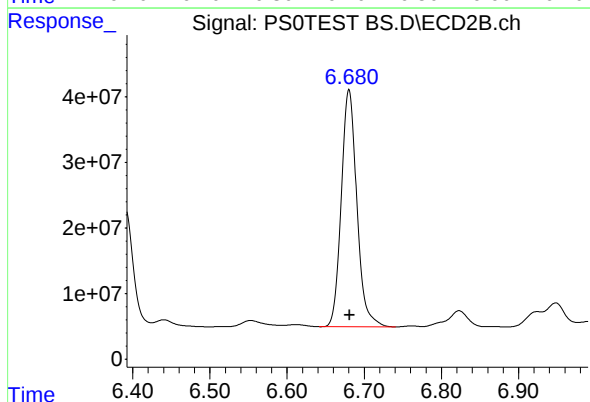


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.680 min
Delta R.T.: 0.000 min
Response: 505245295
Conc: 257.24 ng/ml

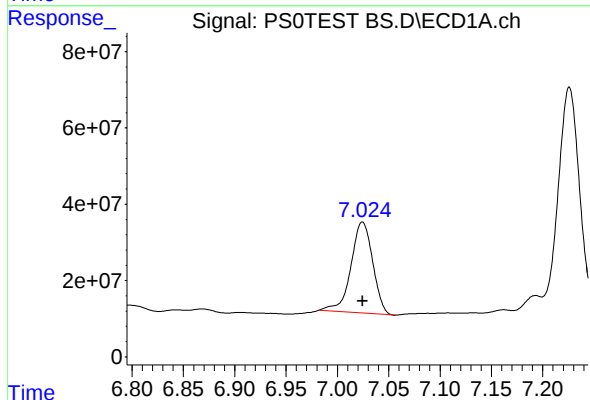


#3 4-Nitrophenol

R.T.: 7.024 min
Delta R.T.: 0.000 min
Response: 351427659
Conc: 204.44 ng/ml

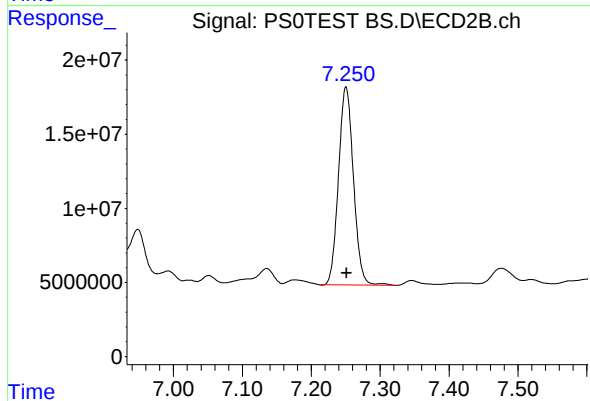

#3 4-Nitrophenol


R.T.: 7.250 min
Delta R.T.: 0.000 min
Response: 201503617
Conc: 220.91 ng/ml

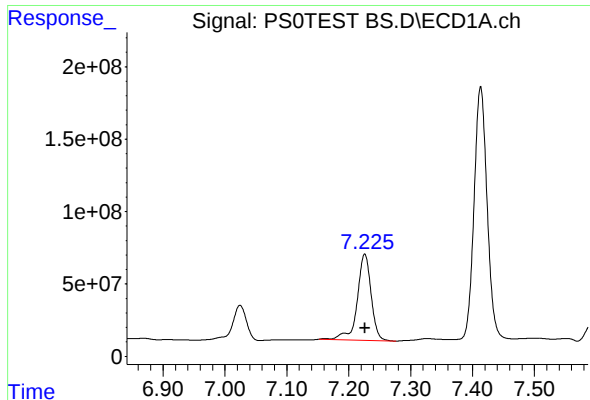

#4 2,4-DCAA


R.T.: 7.226 min
Delta R.T.: 0.000 min
Response: 927215269
Conc: 345.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

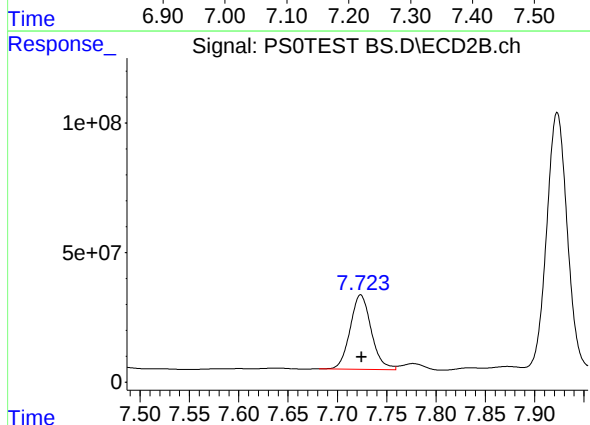


#4 2,4-DCAA

R.T.: 7.724 min
Delta R.T.: 0.000 min
Response: 427822170
Conc: 317.60 ng/ml

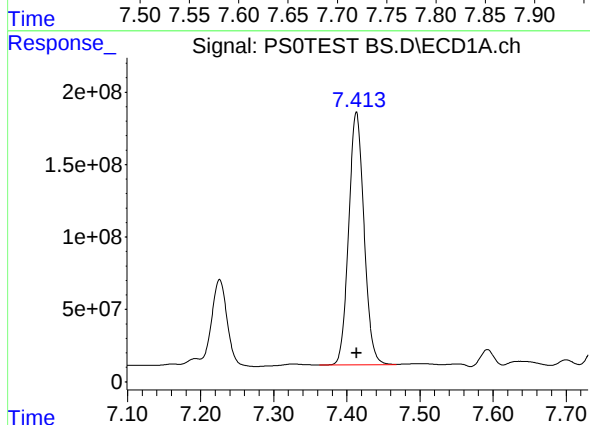


#5 DICAMBA

R.T.: 7.413 min
Delta R.T.: 0.000 min
Response: 2543192141
Conc: 221.52 ng/ml

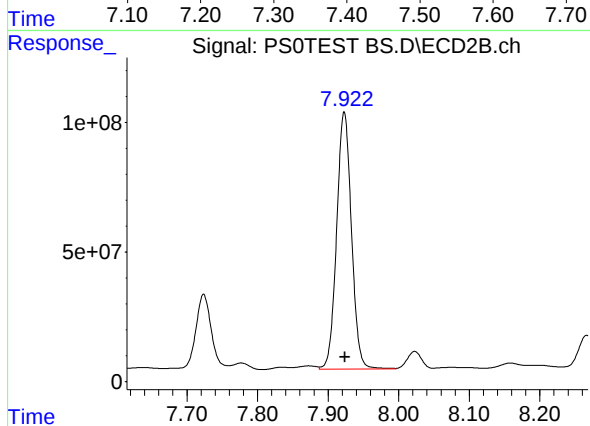

#5 DICAMBA


R.T.: 7.923 min
Delta R.T.: -0.001 min
Response: 1445797208
Conc: 234.85 ng/ml

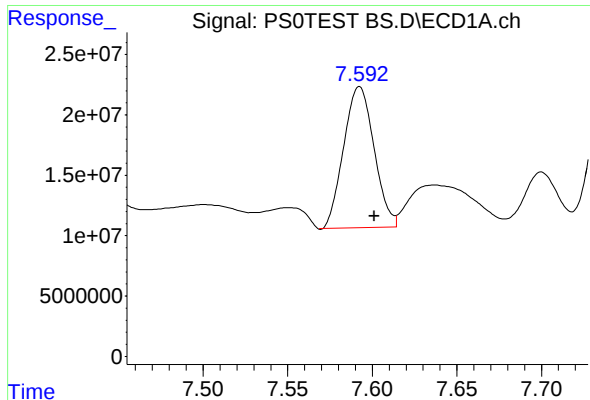

#6 MCPP


R.T.: 7.592 min
Delta R.T.: -0.009 min
Response: 146472157
Conc: 20.07 ug/ml

Instrument :
ECD_S
ClientSampleId :

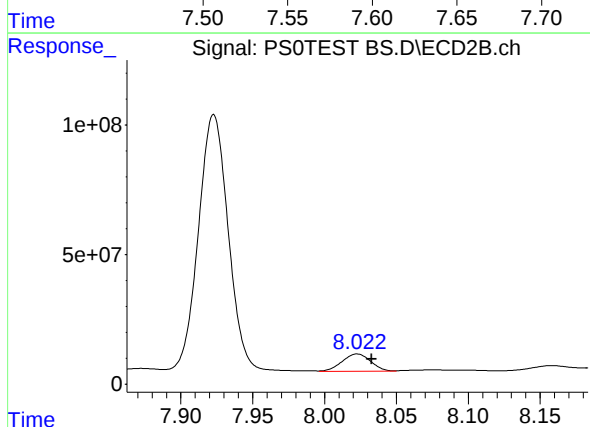


#6 MCPP

R.T.: 8.023 min
Delta R.T.: -0.010 min
Response: 92461136
Conc: 21.46 ug/ml

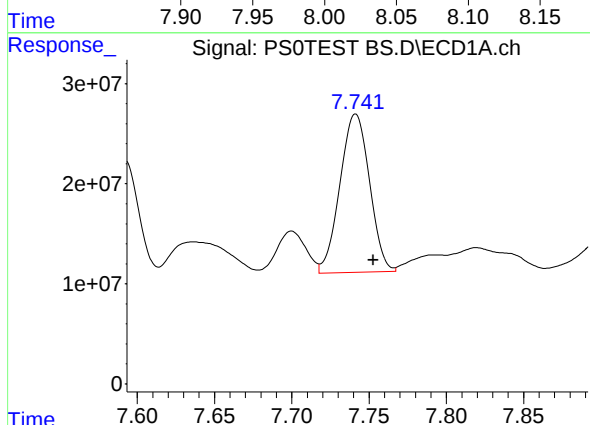


#7 MCPA

R.T.: 7.741 min
Delta R.T.: -0.012 min
Response: 210390555
Conc: 20.35 ug/ml

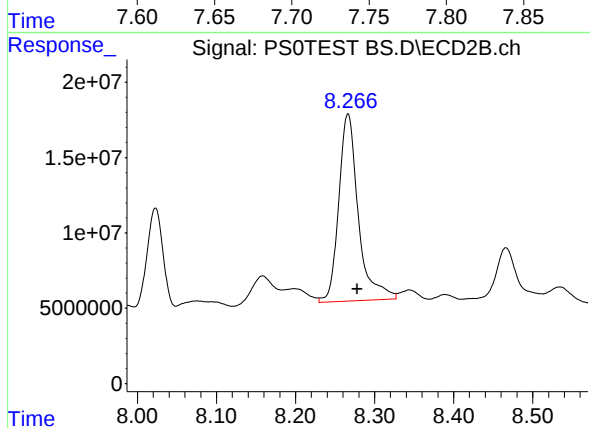

#7 MCPA


R.T.: 8.266 min
Delta R.T.: -0.012 min
Response: 213281790
Conc: 34.37 ug/ml

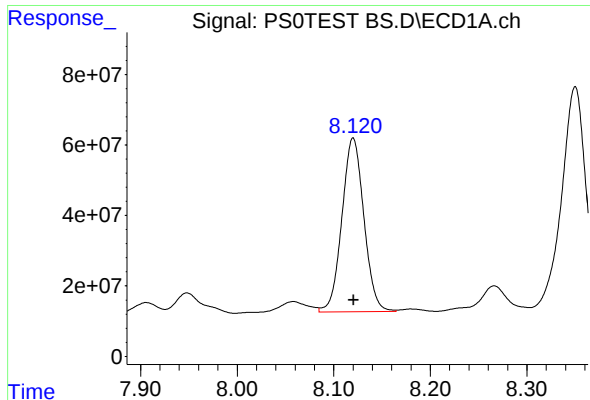

#8 DICHLORPROP


R.T.: 8.120 min
Delta R.T.: 0.000 min
Response: 781464403
Conc: 251.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

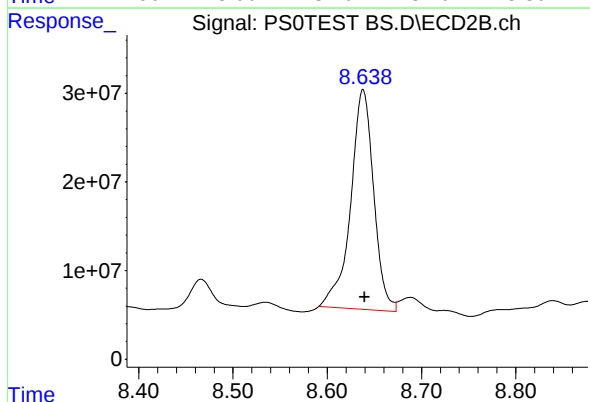


#8 DICHLORPROP

R.T.: 8.638 min
Delta R.T.: -0.002 min
Response: 422330186
Conc: 264.18 ng/ml

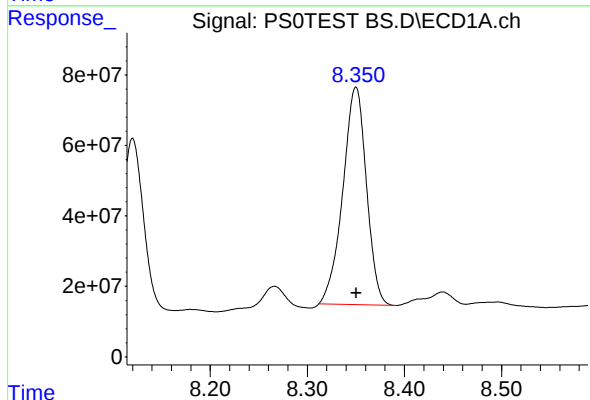


#9 2,4-D

R.T.: 8.350 min
Delta R.T.: 0.000 min
Response: 1044435879
Conc: 309.72 ng/ml

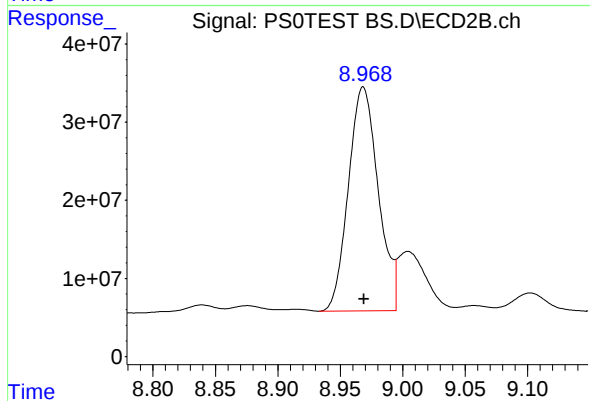

#9 2,4-D


R.T.: 8.968 min
Delta R.T.: 0.000 min
Response: 477918194
Conc: 282.63 ng/ml

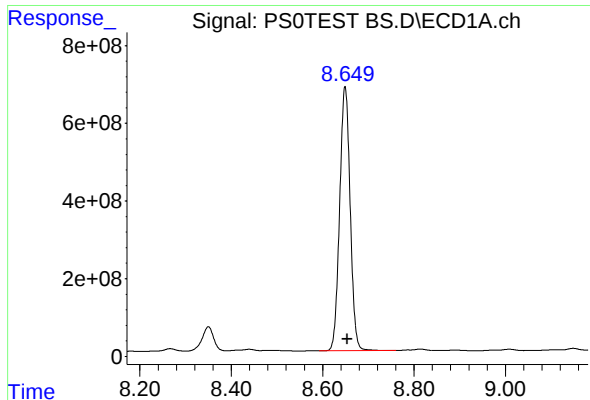

#10 Pentachlorophenol


R.T.: 8.649 min
Delta R.T.: -0.005 min
Response: 10850744436
Conc: 246.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

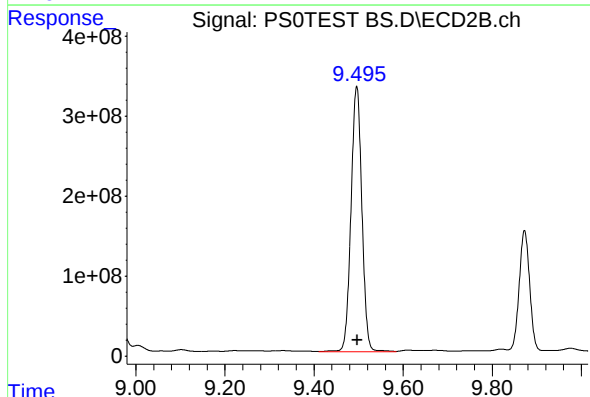


#10 Pentachlorophenol

R.T.: 9.496 min
Delta R.T.: -0.002 min
Response: 5639563360
Conc: 246.37 ng/ml

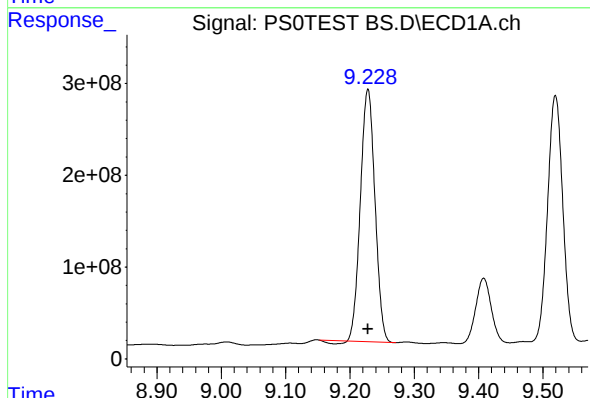


#11 2,4,5-TP (SILVEX)

R.T.: 9.228 min
Delta R.T.: 0.000 min
Response: 4292213505
Conc: 234.81 ng/ml

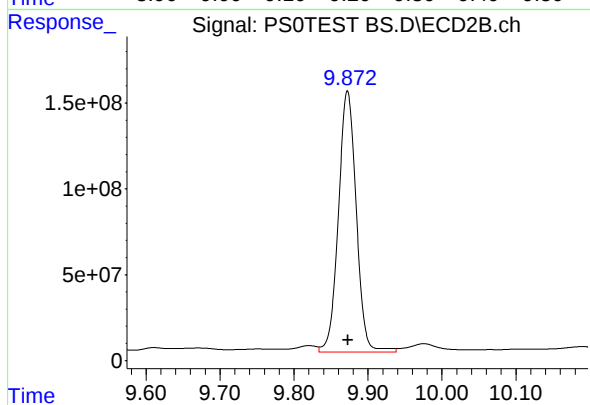

#11 2,4,5-TP (SILVEX)


R.T.: 9.872 min
Delta R.T.: 0.000 min
Response: 2547563511
Conc: 266.97 ng/ml

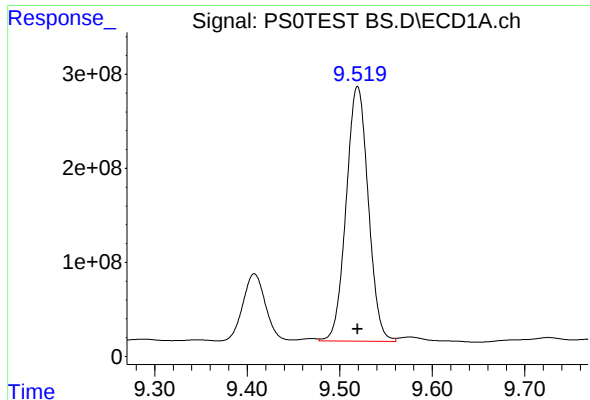

#12 2,4,5-T


R.T.: 9.519 min
Delta R.T.: 0.000 min
Response: 4500306937
Conc: 239.95 ng/ml

Instrument :
ECD_S
ClientSampleId :

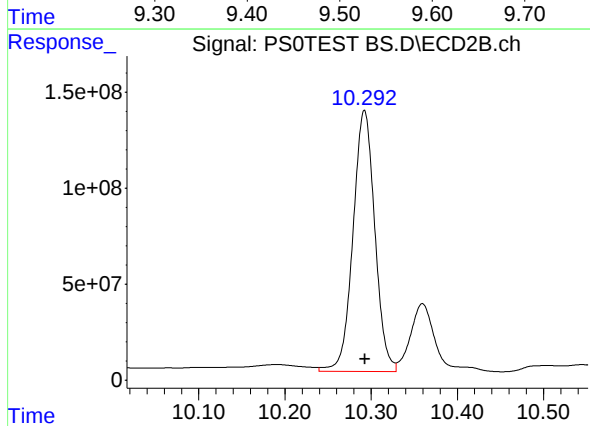


#12 2,4,5-T

R.T.: 10.292 min
Delta R.T.: 0.000 min
Response: 2395306163
Conc: 257.28 ng/ml

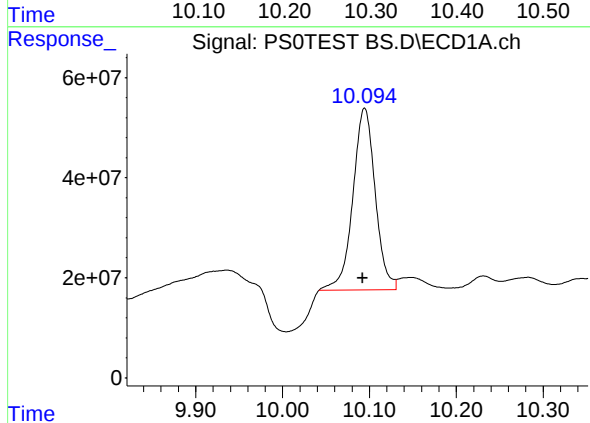


#13 2,4-DB

R.T.: 10.094 min
Delta R.T.: 0.002 min
Response: 650479949
Conc: 183.66 ng/ml

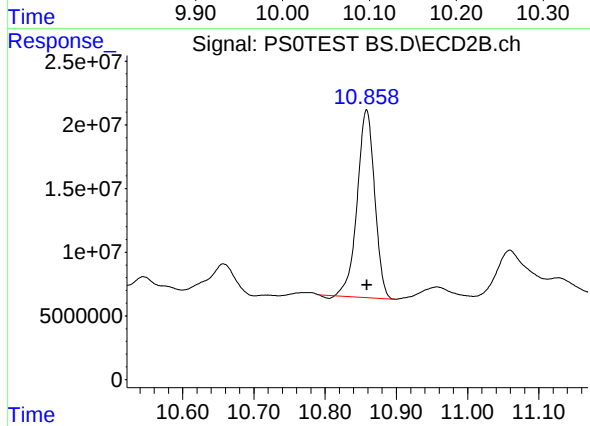

#13 2,4-DB


R.T.: 10.858 min
Delta R.T.: 0.000 min
Response: 249397908
Conc: 217.49 ng/ml

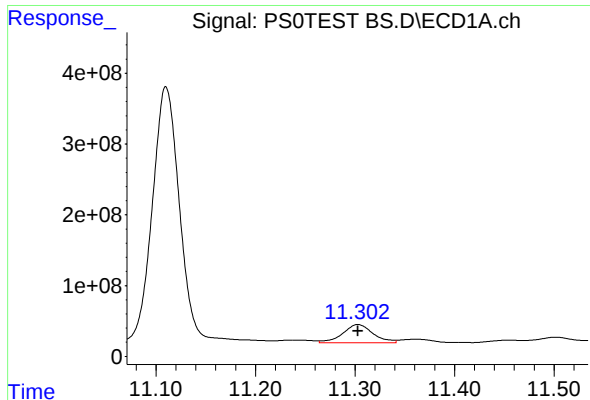

#14 DINOSEB


R.T.: 11.303 min
Delta R.T.: 0.000 min
Response: 540332785
Conc: 35.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

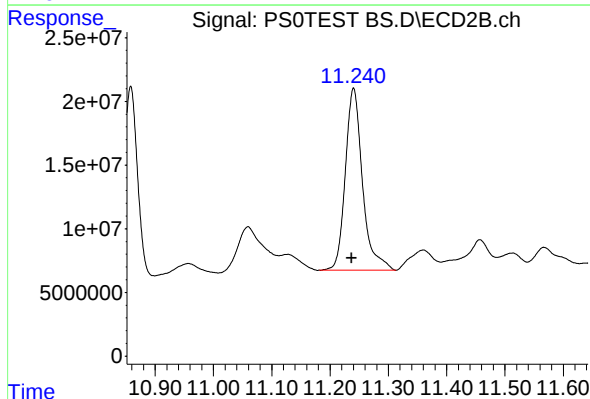


#14 DINOSEB

R.T.: 11.240 min
Delta R.T.: 0.003 min
Response: 292952655
Conc: 46.68 ng/ml

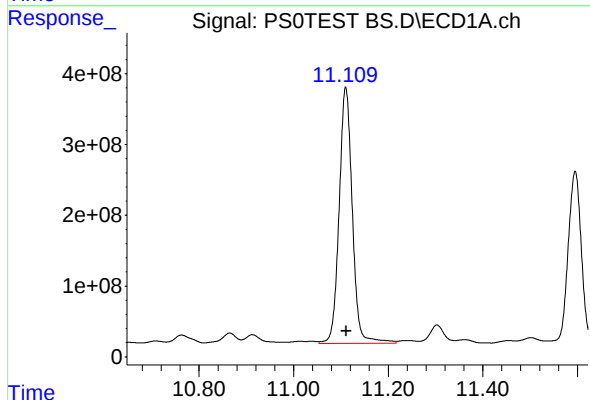


#15 Picloram

R.T.: 11.110 min
Delta R.T.: -0.001 min
Response: 6987500414
Conc: 234.98 ng/ml

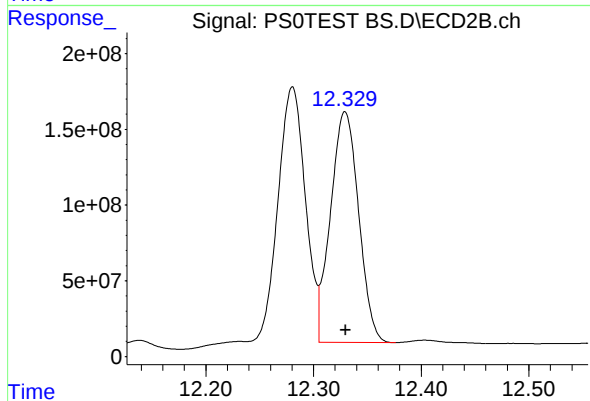

#15 Picloram


R.T.: 12.329 min
Delta R.T.: 0.000 min
Response: 2767088630
Conc: 214.66 ng/ml

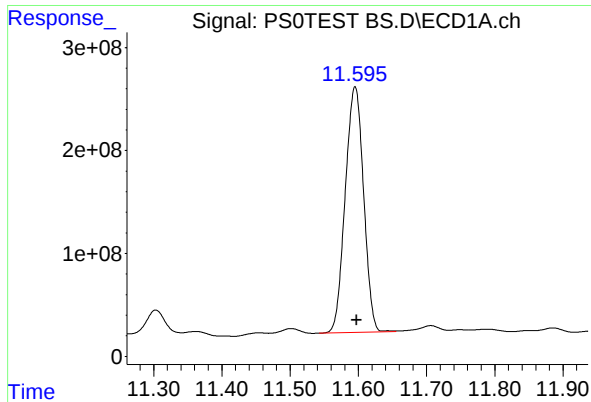

#16 DCPA

R.T.: 11.595 min
Delta R.T.: -0.002 min
Response: 4457220959
Conc: 162.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

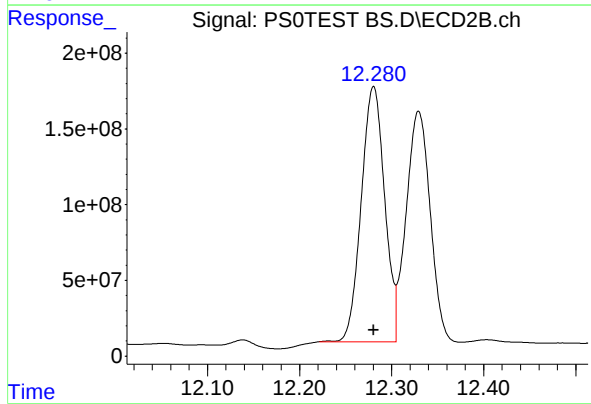

#16 DCPA

R.T.: 12.280 min
Delta R.T.: 0.000 min
Response: 2985569197
Conc: 269.04 ng/ml