

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112624\
 Data File : PS0TEST WITH.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Nov 2024 16:49
 Operator : AR\AJ
 Sample : M4386 WITH HYDRO
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 08:42:53 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 26 14:44:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.225	7.724	1032.0E6	539.0E6	384.733	400.148
Target Compounds							
2) T	3,5-DICHL...	6.399	6.680	3290.0E6	1862.5E6	859.080	948.293
5) T	DICAMBA	7.413	7.923	14444.1E6	8604.0E6	1258.140	1397.612
8) T	DICHLORPROP	8.120	8.638	4083.3E6	2511.4E6	1311.642	1570.976
9) T	2,4-D	8.351	8.968	1718.1E6	948.8E6	509.507	561.104
10) T	Pentachlo...	8.650	9.496	42440.7E6	25180.0E6	962.534	1100.002
11) T	2,4,5-TP ...	9.228	9.873	29123.7E6	18059.2E6	1593.219	1892.497
12) T	2,4,5-T	9.520	10.292	19701.3E6	10704.5E6	1050.426	1149.754
13) T	2,4-DB	10.094	10.857	3311.3E6	1810.7E6	934.947m	1579.016m#
14) T	DINOSEB	11.303	11.238	5485.2E6	2671.8E6	365.039	425.723
15) T	Picloram	11.110	12.329	15519.9E6	6294.6E6	521.909	488.307



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112624\
Data File : PS0TEST WITH.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Nov 2024 16:49
Operator : AR\AJ
Sample : M4386 WITH HYDRO
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 08:42:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
Quant Title : 8080.M
QLast Update : Tue Nov 26 14:44:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

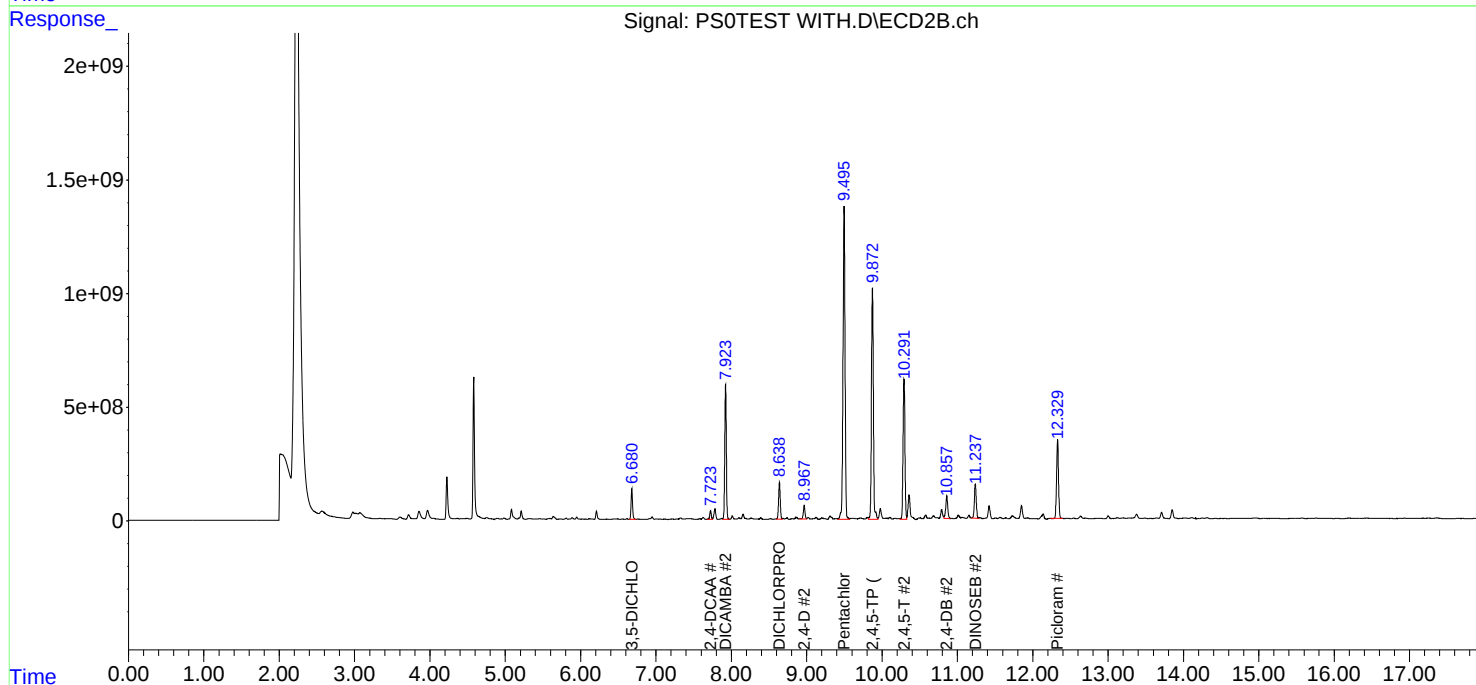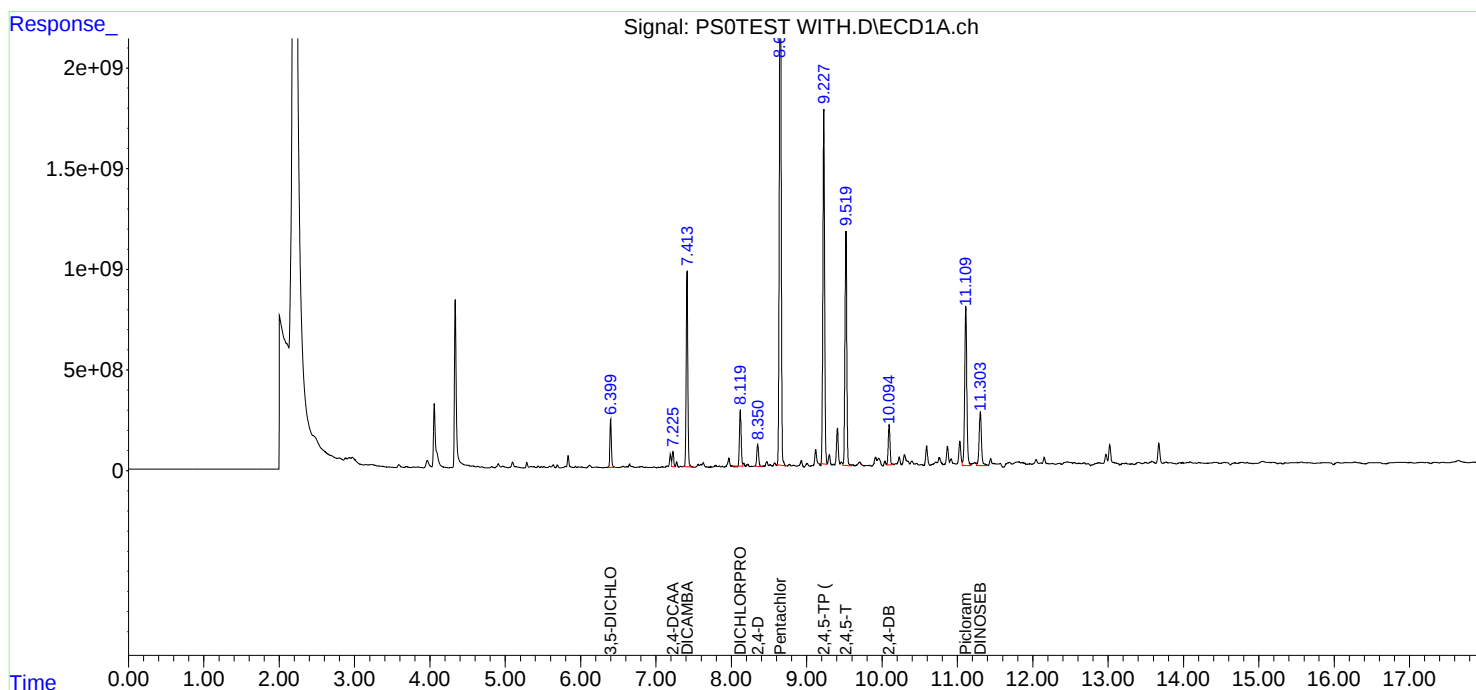


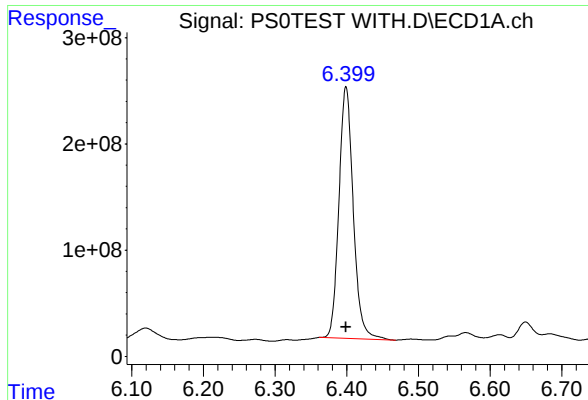

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.399 min
Delta R.T.: 0.000 min
Response: 3289980357
Conc: 859.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

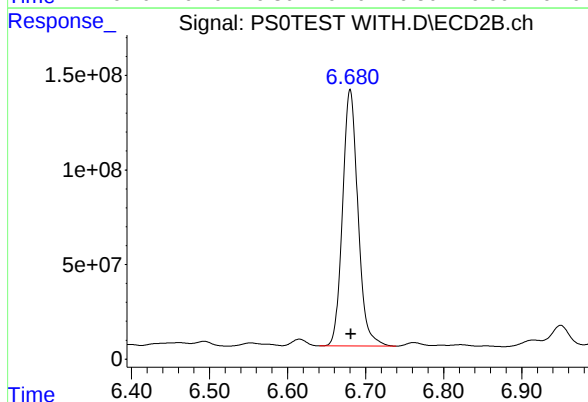


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.680 min
Delta R.T.: 0.000 min
Response: 1862533471
Conc: 948.29 ng/ml

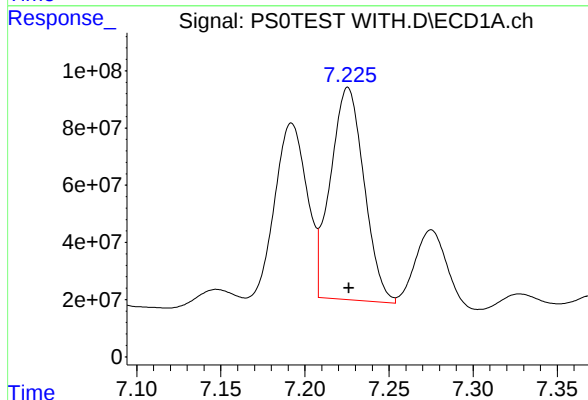


#4 2,4-DCAA

R.T.: 7.225 min
Delta R.T.: 0.000 min
Response: 1031986227
Conc: 384.73 ng/ml

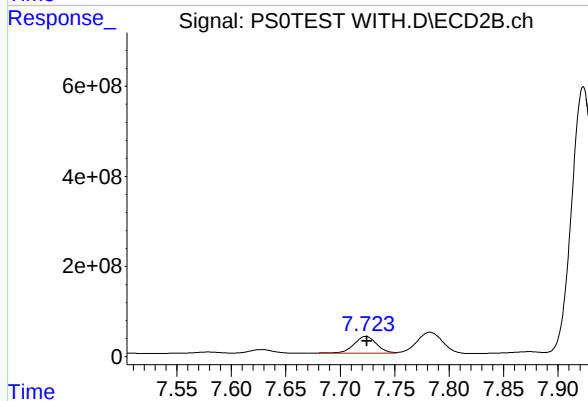

#4 2,4-DCAA

R.T.: 7.724 min
Delta R.T.: -0.001 min
Response: 539010790
Conc: 400.15 ng/ml

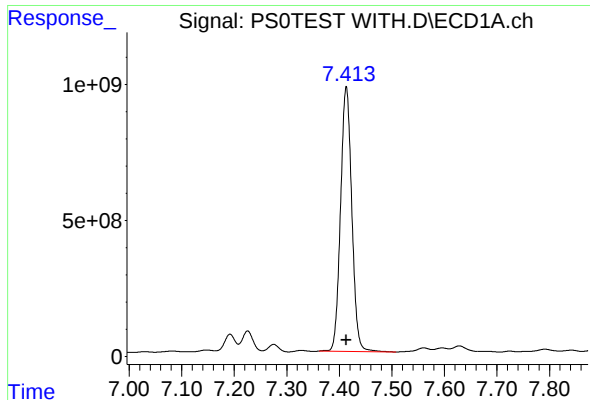


#5 DICAMBA

R.T.: 7.413 min
Delta R.T.: 0.000 min
Response: 14444111712
Conc: 1258.14 ng/ml

Instrument :


ECD_S

ClientSampleId :

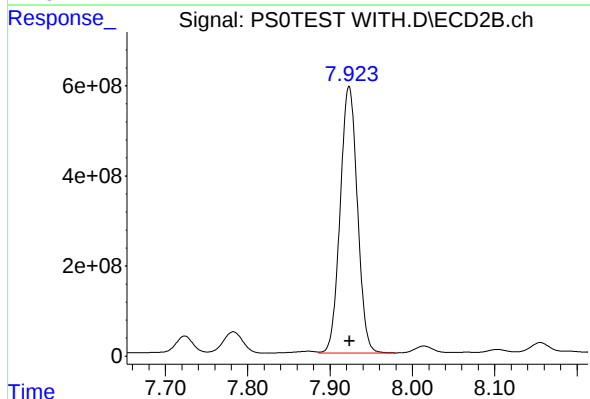


#5 DICAMBA

R.T.: 7.923 min
Delta R.T.: 0.000 min
Response: 8604001234
Conc: 1397.61 ng/ml

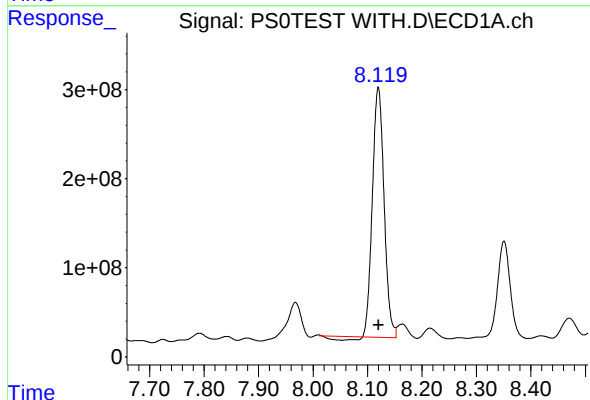


#8 DICHLORPROP

R.T.: 8.120 min
Delta R.T.: 0.000 min
Response: 4083278822
Conc: 1311.64 ng/ml

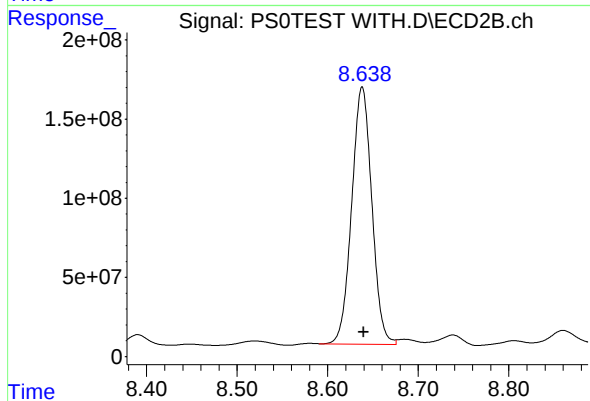

#8 DICHLORPROP


R.T.: 8.638 min
Delta R.T.: -0.002 min
Response: 2511391569
Conc: 1570.98 ng/ml

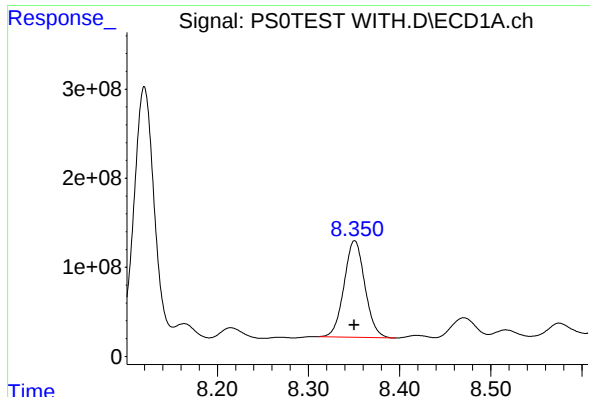

#9 2,4-D


R.T.: 8.351 min
Delta R.T.: 0.000 min
Response: 1718134444
Conc: 509.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

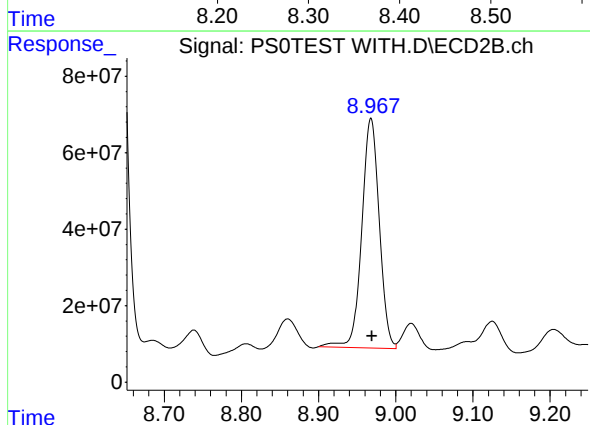


#9 2,4-D

R.T.: 8.968 min
Delta R.T.: -0.001 min
Response: 948809949
Conc: 561.10 ng/ml

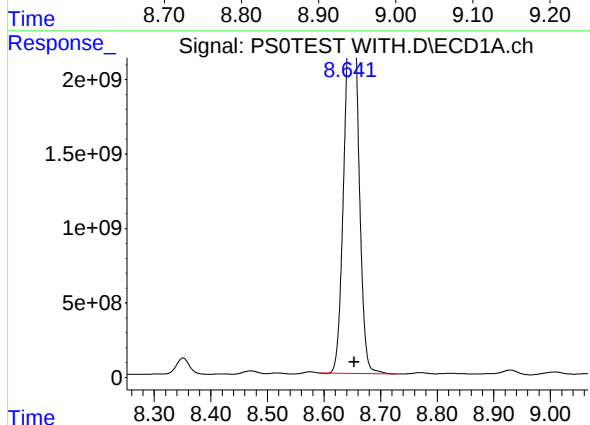


#10 Pentachlorophenol

R.T.: 8.650 min
Delta R.T.: -0.004 min
Response: 42440654308
Conc: 962.53 ng/ml

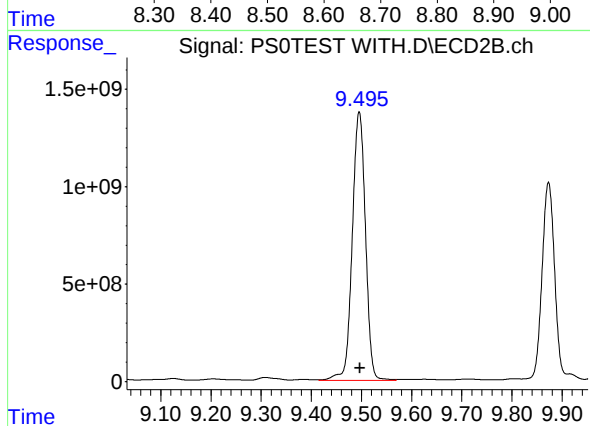

#10 Pentachlorophenol


R.T.: 9.496 min
Delta R.T.: -0.002 min
Response: 25180013851
Conc: 1100.00 ng/ml

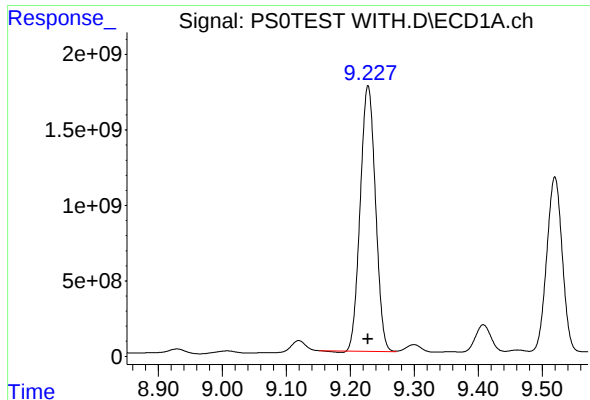

#11 2,4,5-TP (SILVEX)


R.T.: 9.228 min
Delta R.T.: 0.000 min
Response: 29123701038
Conc: 1593.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

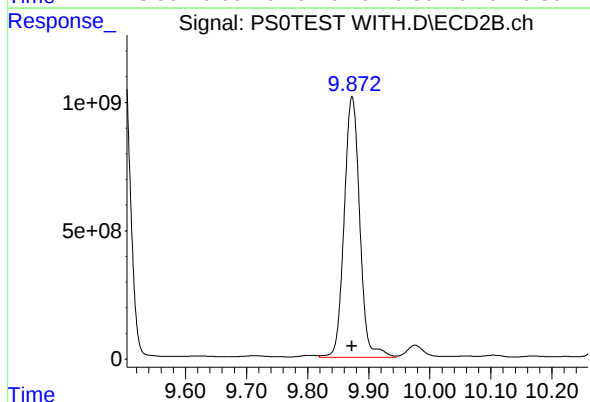


#11 2,4,5-TP (SILVEX)

R.T.: 9.873 min
Delta R.T.: 0.000 min
Response: 18059186228
Conc: 1892.50 ng/ml

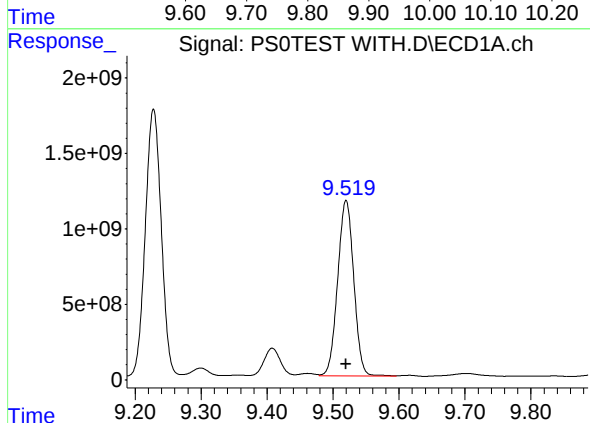


#12 2,4,5-T

R.T.: 9.520 min
Delta R.T.: 0.000 min
Response: 19701282928
Conc: 1050.43 ng/ml

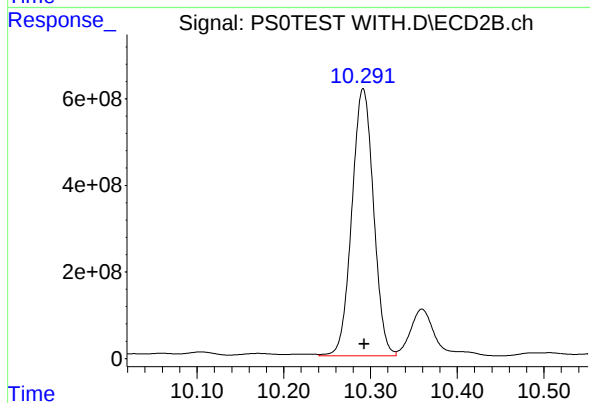

#12 2,4,5-T


R.T.: 10.292 min
Delta R.T.: -0.001 min
Response: 10704537140
Conc: 1149.75 ng/ml

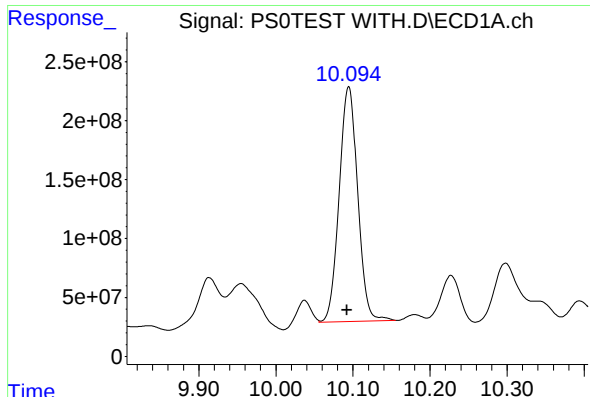

#13 2,4-DB


R.T.: 10.094 min
Delta R.T.: 0.002 min
Response: 3311307636
Conc: 934.95 ng/ml

Instrument :
ECD_S
ClientSampleId :

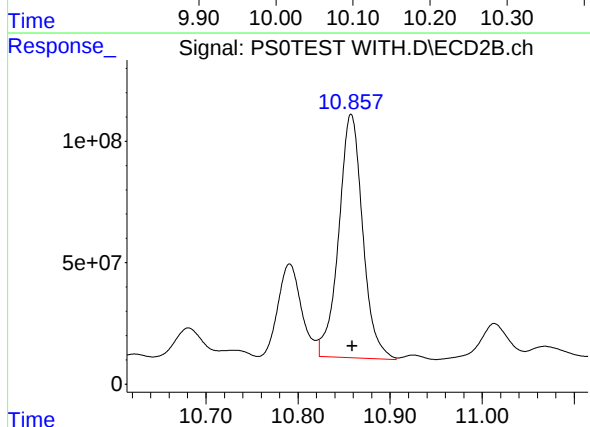


#13 2,4-DB

R.T.: 10.857 min
Delta R.T.: -0.002 min
Response: 1810690440
Conc: 1579.02 ng/ml m

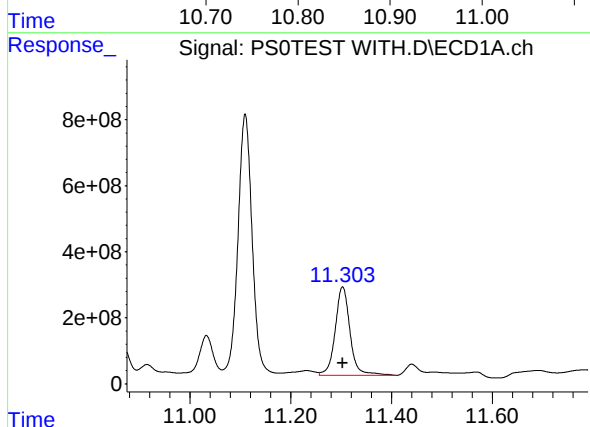


#14 DINOSEB

R.T.: 11.303 min
Delta R.T.: 0.000 min
Response: 5485164456
Conc: 365.04 ng/ml

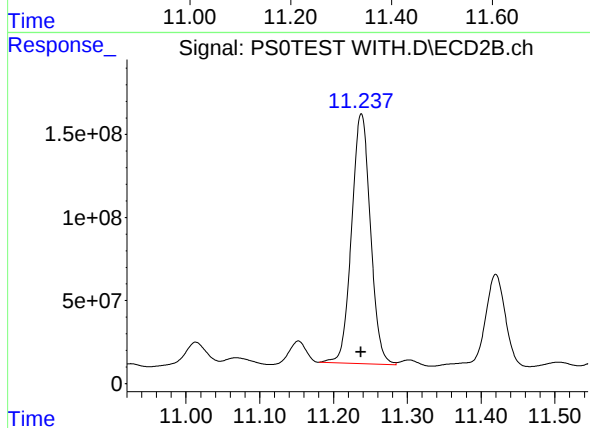

#14 DINOSEB


R.T.: 11.238 min
Delta R.T.: 0.000 min
Response: 2671844585
Conc: 425.72 ng/ml

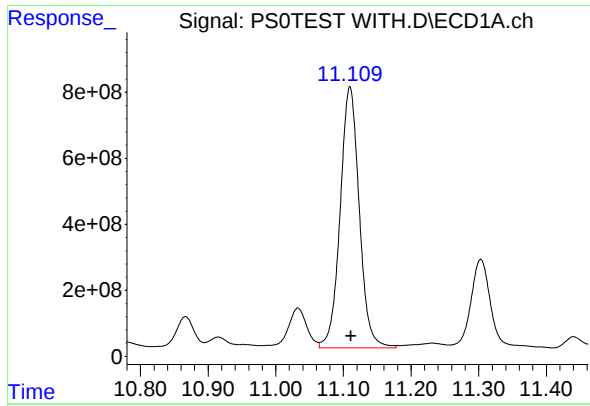

#15 Picloram

R.T.: 11.110 min
Delta R.T.: -0.002 min
Response: 15519883849
Conc: 521.91 ng/ml

Instrument :
ECD_S
ClientSampleId :

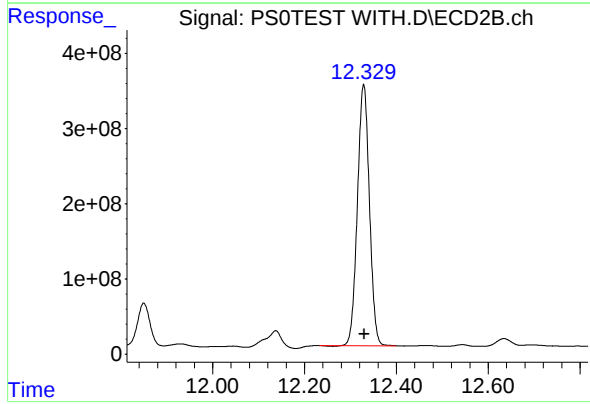

#15 Picloram

R.T.: 12.329 min
Delta R.T.: 0.000 min
Response: 6294611513
Conc: 488.31 ng/ml