

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112625\
 Data File : PS032541.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Nov 2025 09:17
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 26 11:17:24 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.286	7.629	1614.2E6	1890.2E6	356.237	518.508 #
Target Compounds							
2) T	3,5-DICHL...	6.446	0.000	2672735	0	<MDL	N.D. #
7) T	MCPA	7.803	0.000	434340	0	<MDL	N.D. #
8) T	DICHLORPROP	8.173	0.000	271605	0	<MDL	N.D. #
10) T	Pentachlo...	8.706	0.000	2298858	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.271	0.000	2272599	0	<MDL	N.D. #
12) T	2,4,5-T	9.586	10.193	2877368	3582327	<MDL	<MDL #
13) T	2,4-DB	10.147	10.752	661353	4862599	<MDL	1.289 #
14) T	DINOSEB	11.340	11.127	3775687	1478350	<MDL	<MDL #
15) T	Picloram	11.147f	0.000	1496421	0	<MDL	N.D. #
16) T	DCPA	11.647	0.000	5029641	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112625\
Data File : PS032541.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Nov 2025 09:17
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 26 11:17:24 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

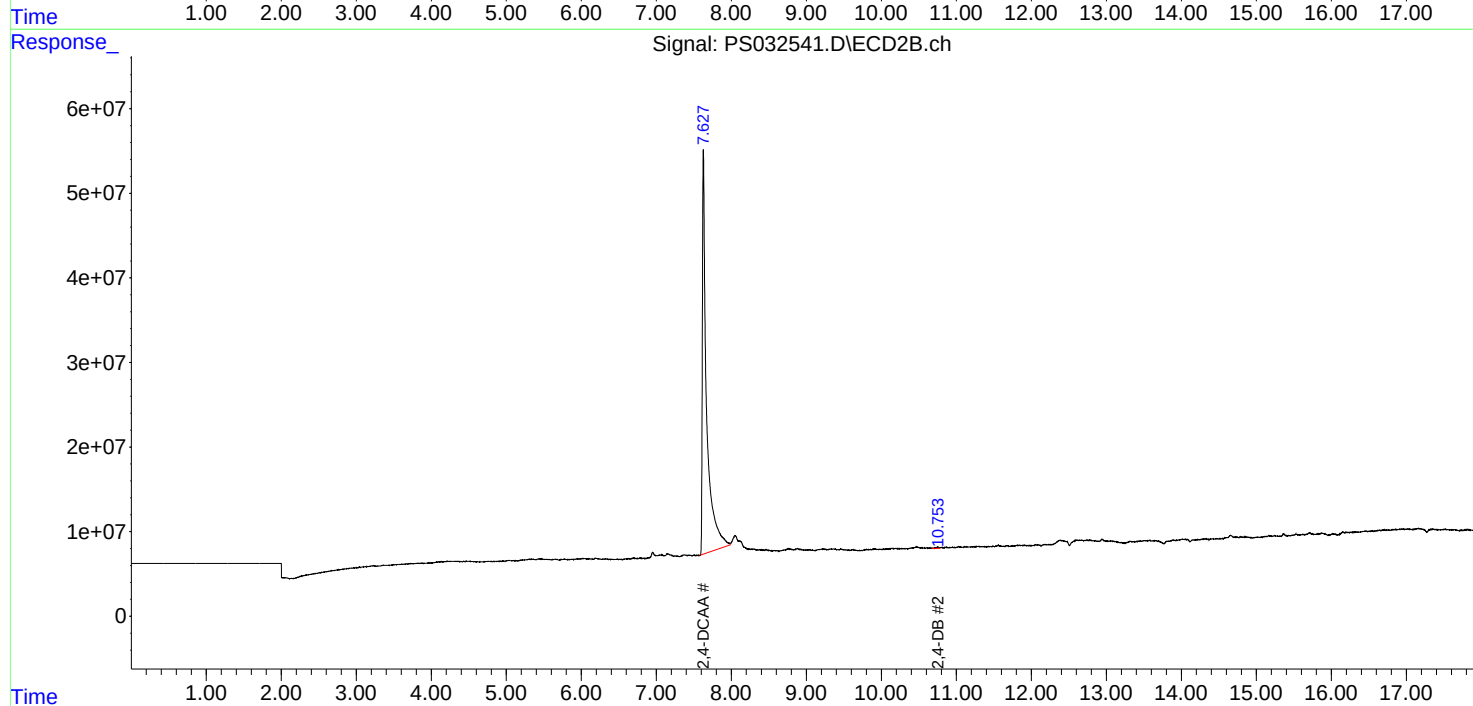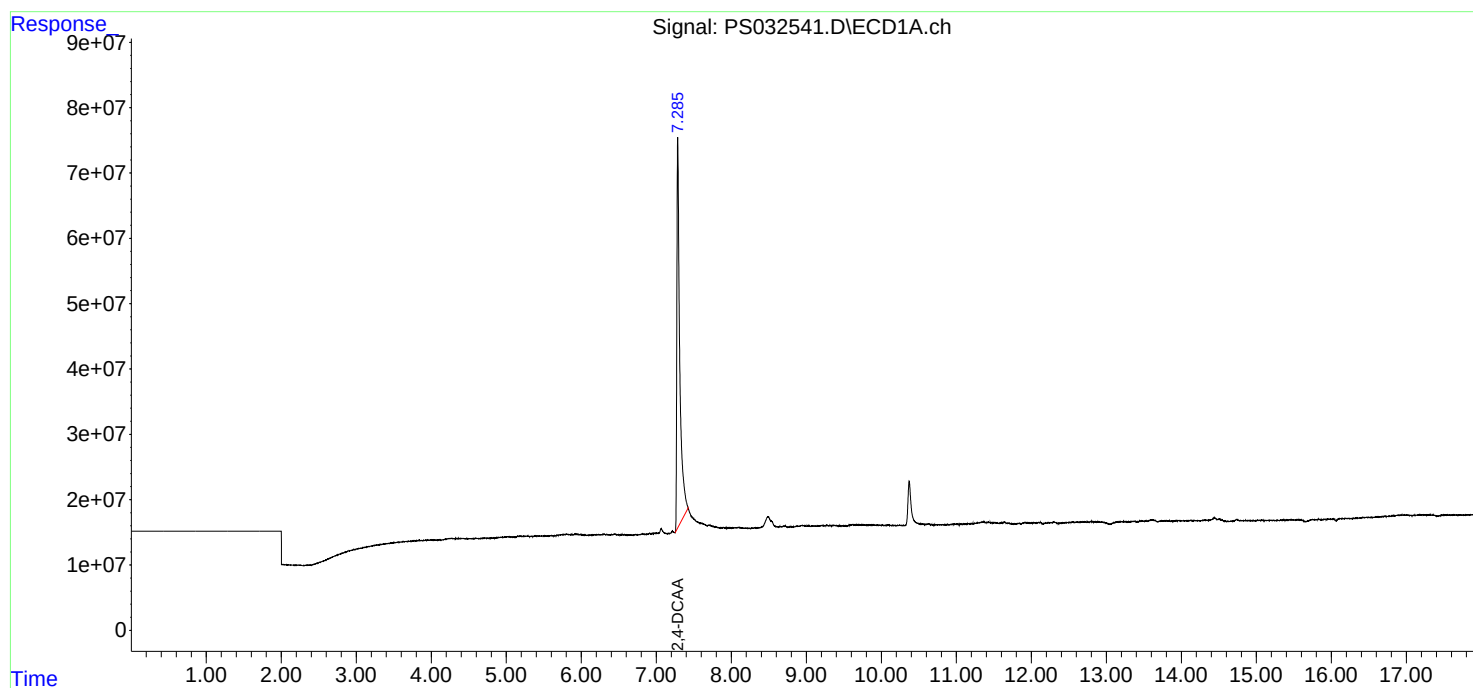


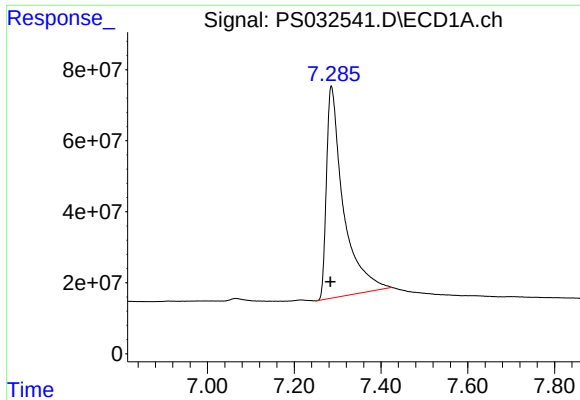

#4 2,4-DCAA


R.T.: 7.286 min
Delta R.T.: 0.002 min
Response: 1614208939
Conc: 356.24 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

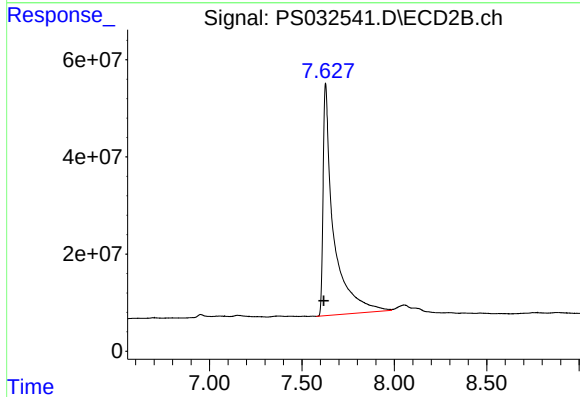


#4 2,4-DCAA

R.T.: 7.629 min
Delta R.T.: 0.012 min
Response: 1890220393
Conc: 518.51 ng/ml

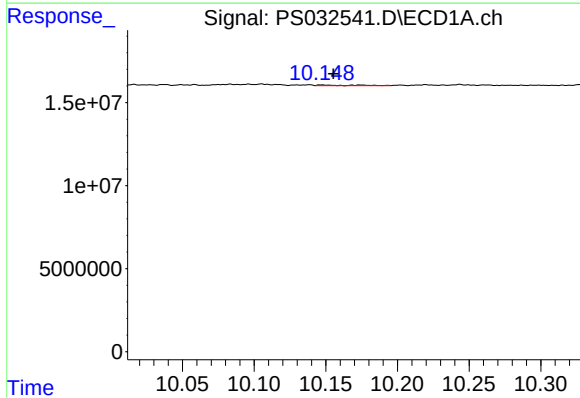

#13 2,4-DB

R.T.: 10.147 min
Delta R.T.: -0.008 min
Response: 661353
Conc: N.D.

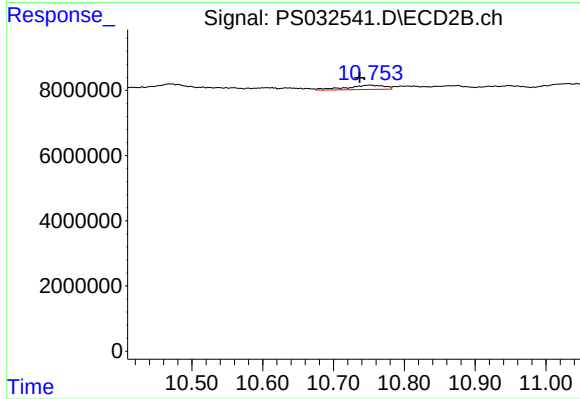

#13 2,4-DB

R.T.: 10.752 min
Delta R.T.: 0.015 min
Response: 4862599
Conc: 1.29 ng/ml