

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112625\
 Data File : PS032543.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Nov 2025 10:50
 Operator : AR\AJ
 Sample : Q3710-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMPRESSOR-EXCAVATION

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 26 11:18:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.291	7.627	417.0E6	595.3E6	92.036	163.293 #
Target Compounds							
1) T	Dalapon	0.000	2.563f	0	2216.6E6	N.D.	318.748
2) T	3,5-DICHL...	6.496f	6.556f	532394	5201525	<MDL	<MDL #
5) T	DICAMBA	7.465	0.000	1372880	0	<MDL	N.D. #
6) T	MCP	7.668	7.893	33231	36022722	<MDL	2.708 #
7) T	MCPA	7.759f	0.000	225.7E6	0	16.813	N.D. #
8) T	DICHLORPROP	8.147f	8.539	28742500	1051851	6.461	<MDL #
9) T	2,4-D	8.414	8.833f	19021185	4637939	4.216	<MDL #
10) T	Pentachlo...	8.701	9.356	11863405	21455513	<MDL	<MDL #
11) T	2,4,5-TP ...	9.286	9.736	6581363	185.6E6	<MDL	6.910 #
12) T	2,4,5-T	9.547f	0.000	171.3E6	0	7.188	N.D. #
13) T	2,4-DB	10.188f	0.000	53289421	0	20.223	N.D. #
14) T	DINOSEB	0.000	11.122	0	31969702	N.D.	1.807
15) T	Picloram	11.165	12.183f	9779525	2026957	<MDL	<MDL #
16) T	DCPA	11.637	12.137	16957539	18435389	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112625\
Data File : PS032543.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Nov 2025 10:50
Operator : AR\AJ
Sample : Q3710-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
COMPRESSOR-EXCAVATION

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 26 11:18:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

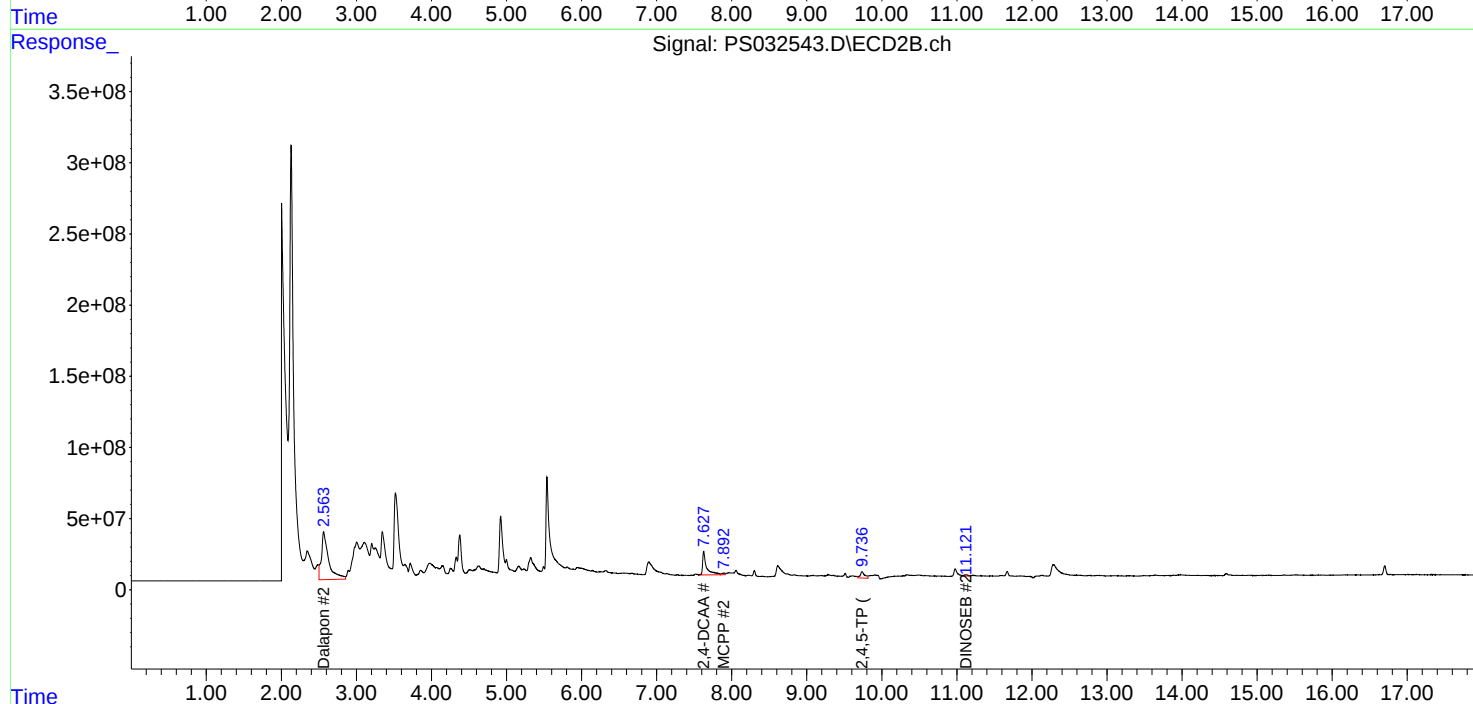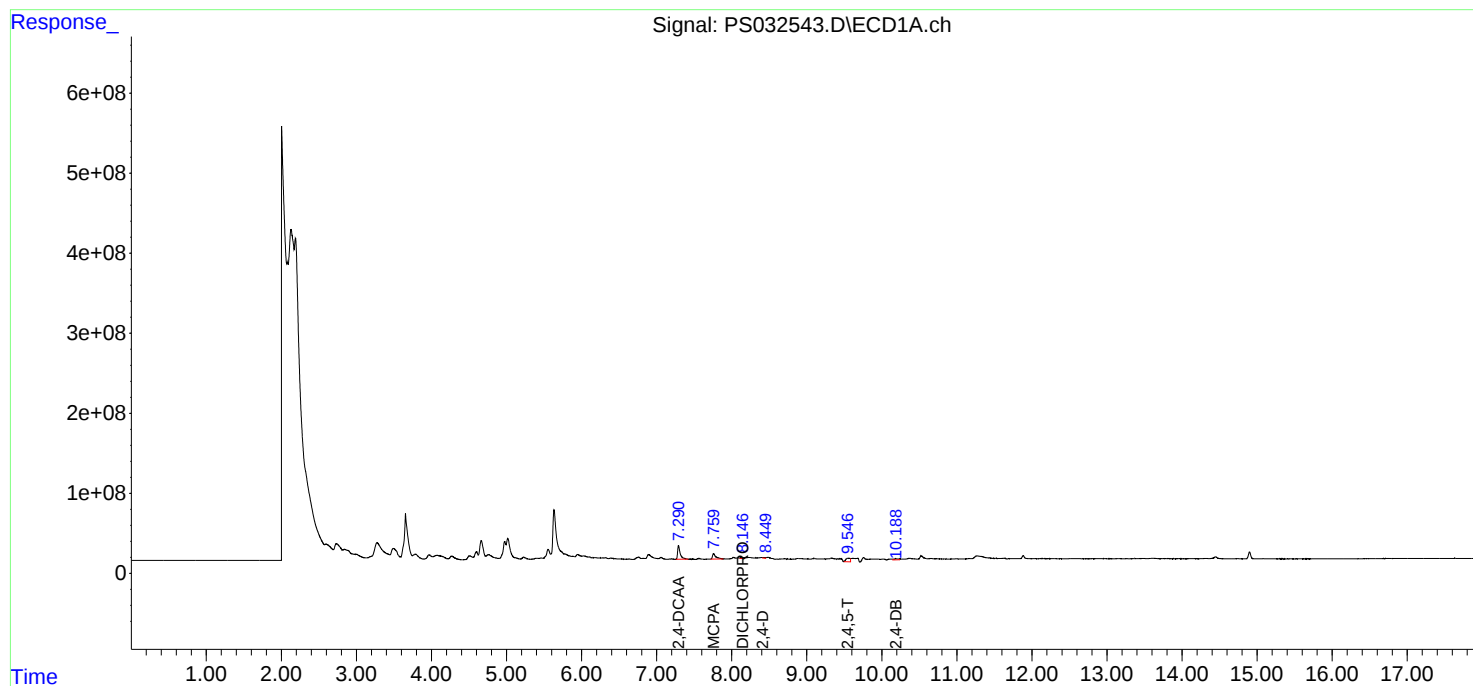


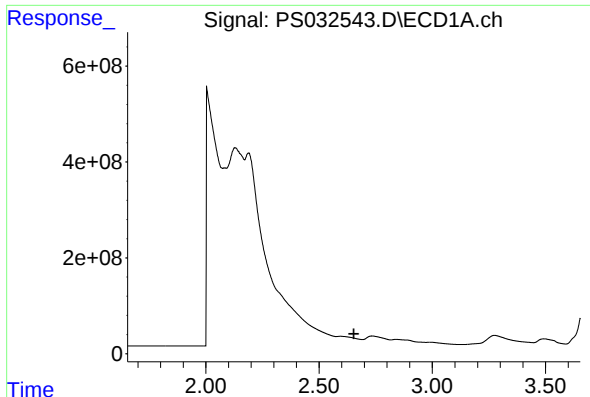

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.654 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMPRESSOR-EXCAVATION

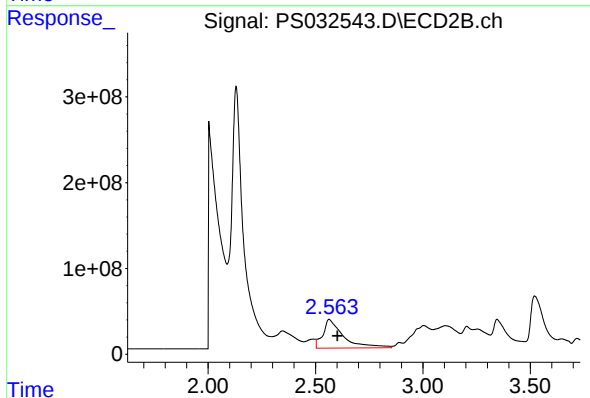


#1 Dalapon

R.T.: 2.563 min
Delta R.T.: -0.040 min
Response: 2216570445
Conc: 318.75 ng/ml

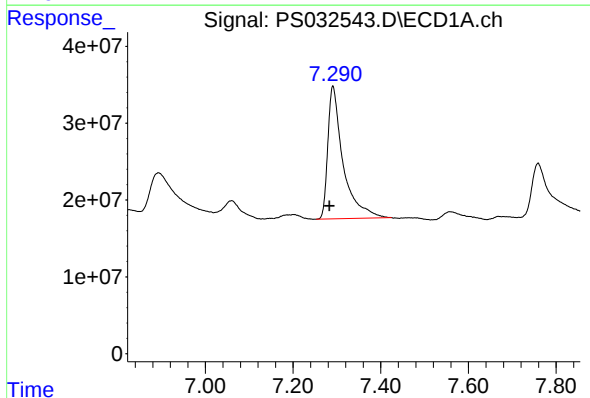


#4 2,4-DCAA

R.T.: 7.291 min
Delta R.T.: 0.007 min
Response: 417041867
Conc: 92.04 ng/ml

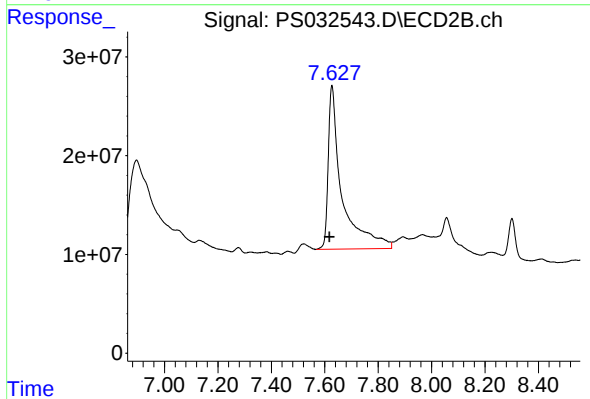

#4 2,4-DCAA


R.T.: 7.627 min
Delta R.T.: 0.010 min
Response: 595285037
Conc: 163.29 ng/ml

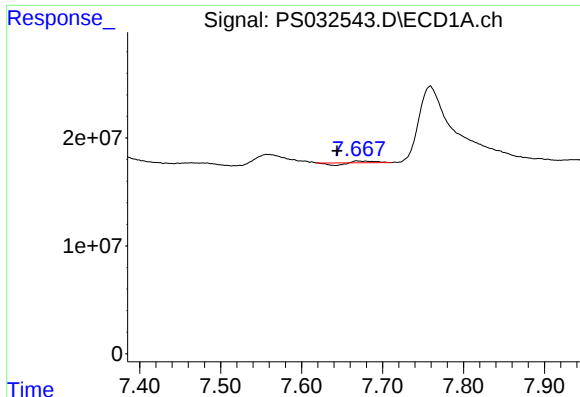

#6 MCPP


R.T.: 7.668 min
Delta R.T.: 0.024 min
Response: 33231
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMPRESSOR-EXCAVATION

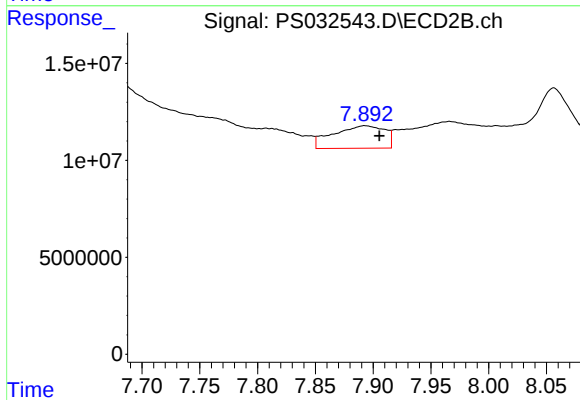


#6 MCPP

R.T.: 7.893 min
Delta R.T.: -0.012 min
Response: 36022722
Conc: 2.71 ug/ml

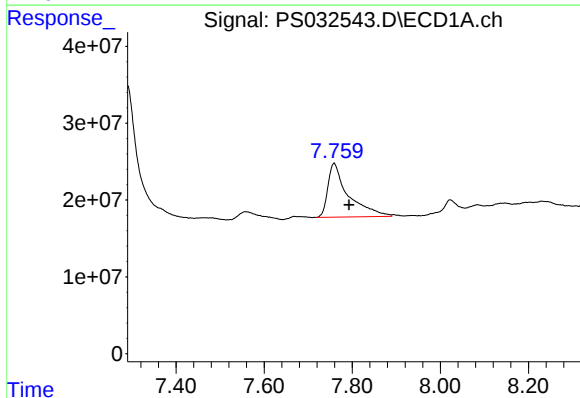


#7 MCPA

R.T.: 7.759 min
Delta R.T.: -0.034 min
Response: 225726468
Conc: 16.81 ug/ml

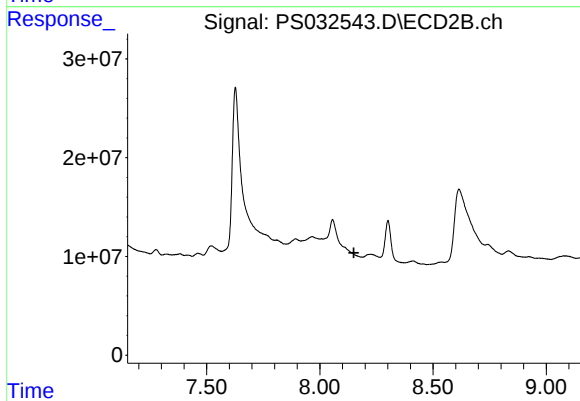

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 8.151 min
Response: 0
Conc: N.D.

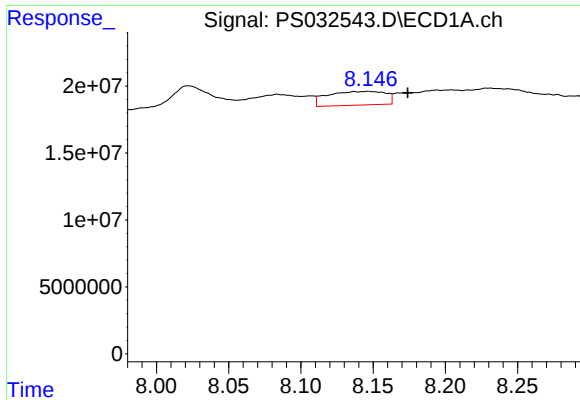

#8 DICHLORPROP


R.T.: 8.147 min
Delta R.T.: -0.027 min
Response: 28742500
Conc: 6.46 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMPRESSOR-EXCAVATION

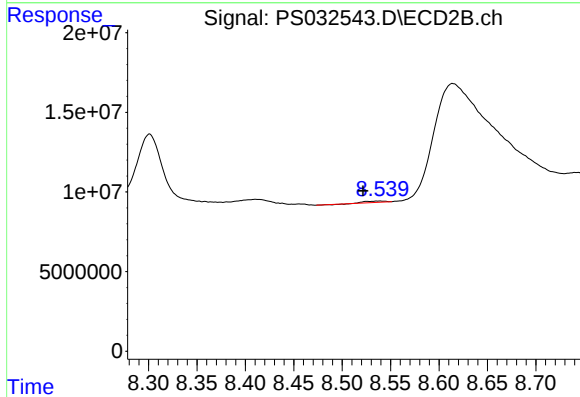


#8 DICHLORPROP

R.T.: 8.539 min
Delta R.T.: 0.017 min
Response: 1051851
Conc: N.D.

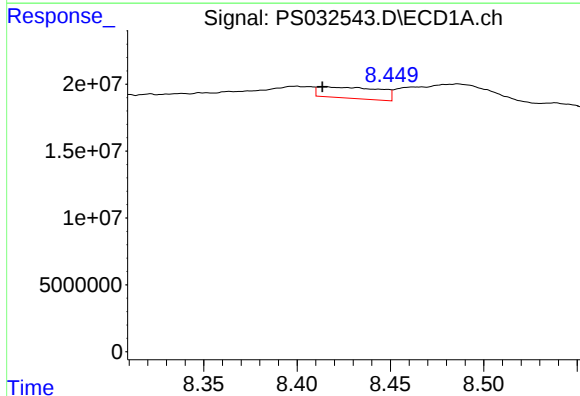


#9 2,4-D

R.T.: 8.414 min
Delta R.T.: 0.000 min
Response: 19021185
Conc: 4.22 ng/ml

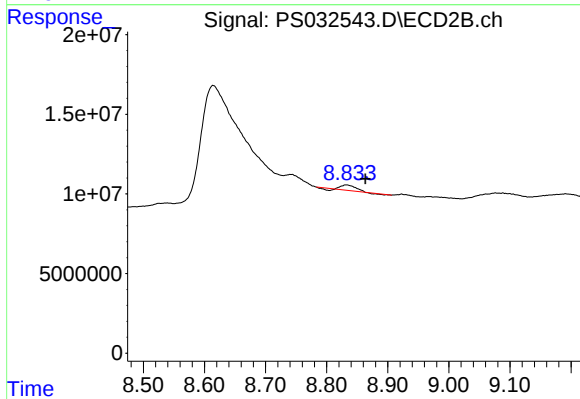

#9 2,4-D


R.T.: 8.833 min
Delta R.T.: -0.031 min
Response: 4637939
Conc: N.D.

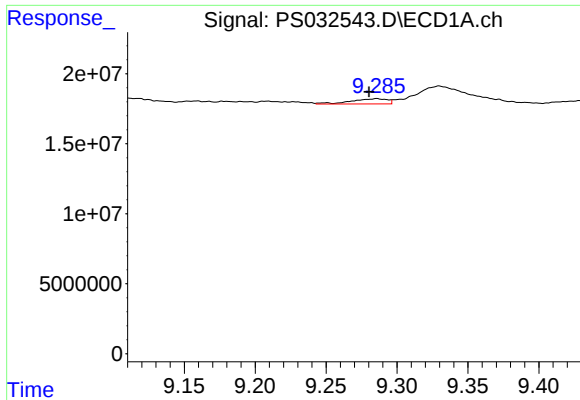

#11 2,4,5-TP (SILVEX)


R.T.: 9.286 min
Delta R.T.: 0.005 min
Response: 6581363
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMPRESSOR-EXCAVATION

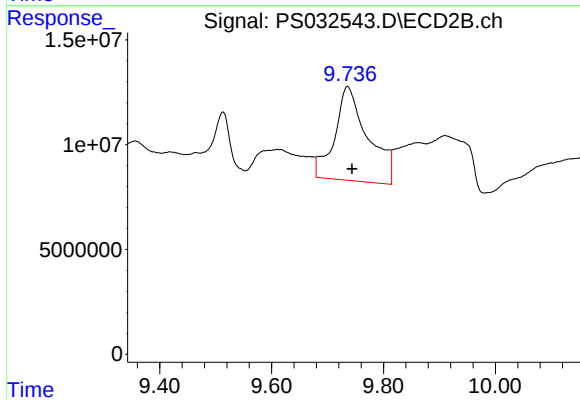


#11 2,4,5-TP (SILVEX)

R.T.: 9.736 min
Delta R.T.: -0.008 min
Response: 185571865
Conc: 6.91 ng/ml

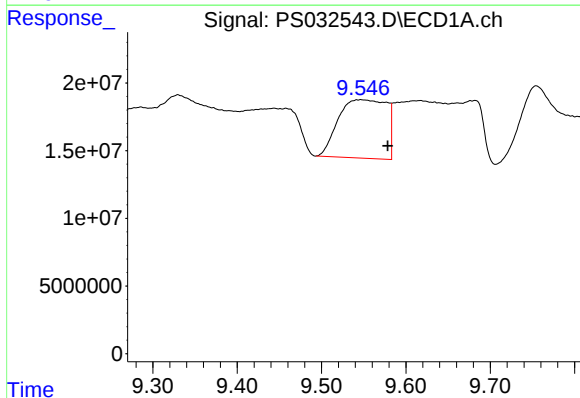


#12 2,4,5-T

R.T.: 9.547 min
Delta R.T.: -0.032 min
Response: 171345791
Conc: 7.19 ng/ml

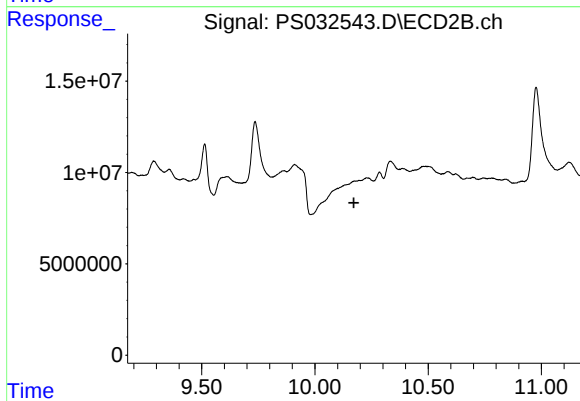

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 10.172 min
Response: 0
Conc: N.D.

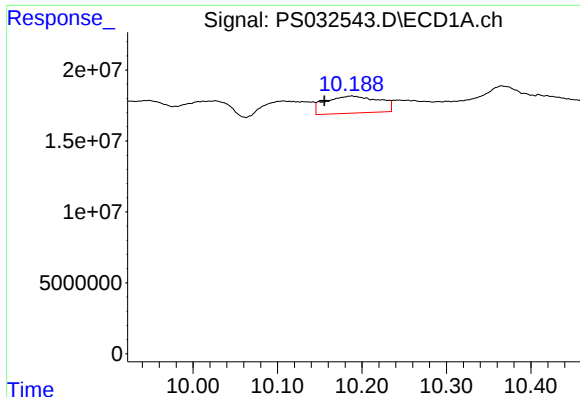

#13 2,4-DB


R.T.: 10.188 min
Delta R.T.: 0.032 min
Response: 53289421
Conc: 20.22 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMPRESSOR-EXCAVATION

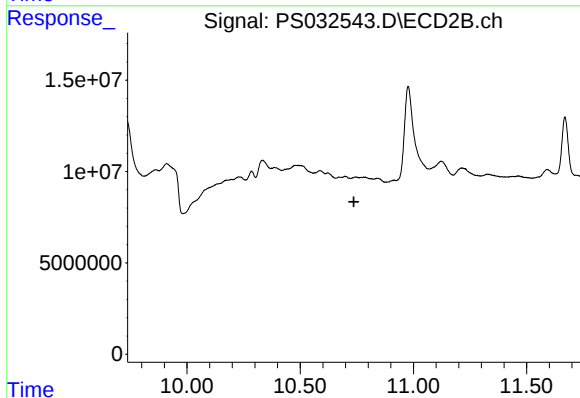


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.737 min
Response: 0
Conc: N.D.

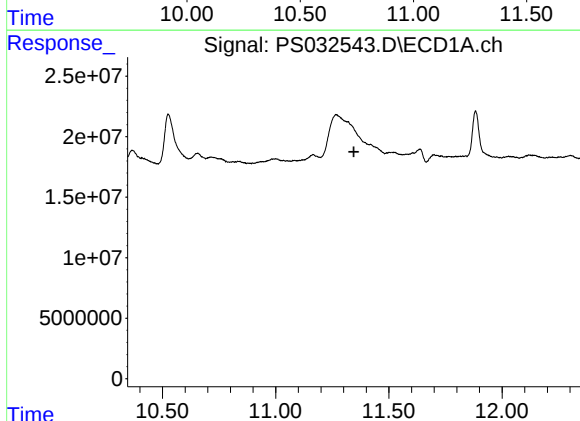

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.345 min
Response: 0
Conc: N.D.

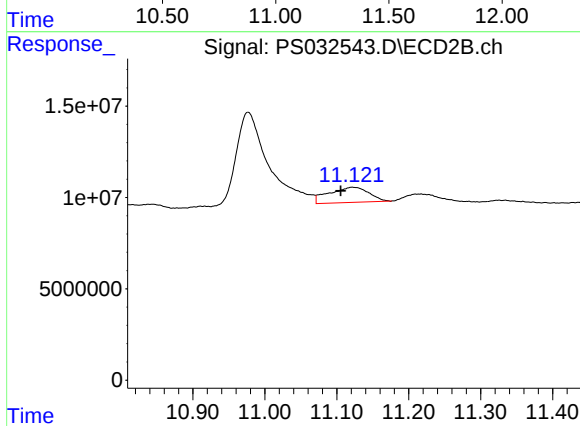

#14 DINOSEB

R.T.: 11.122 min
Delta R.T.: 0.017 min
Response: 31969702
Conc: 1.81 ng/ml