

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112625\
 Data File : PS032544.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Nov 2025 11:14
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 26 13:06:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.288	7.630	1596.4E6	1938.4E6	352.301	531.733 #
Target Compounds							
2) T	3,5-DICHL...	6.446	0.000	2762808	0	<MDL	N.D. #
7) T	MCPA	0.000	8.102f	0	2205708	N.D.	<MDL
8) T	DICHLORPROP	8.193	0.000	774114	0	<MDL	N.D. #
10) T	Pentachlo...	8.716	0.000	4969411	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.274	0.000	2858422	0	<MDL	N.D. #
12) T	2,4,5-T	9.616f	10.193	3935188	3113900	<MDL	<MDL #
13) T	2,4-DB	0.000	10.746	0	1025285	N.D.	<MDL
14) T	DINOSEB	11.350	0.000	8506144	0	<MDL	N.D. #
15) T	Picloram	11.166	12.191f	1588419	11041874	<MDL	<MDL #
16) T	DCPA	11.642	0.000	4248368	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112625\
Data File : PS032544.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Nov 2025 11:14
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 26 13:06:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

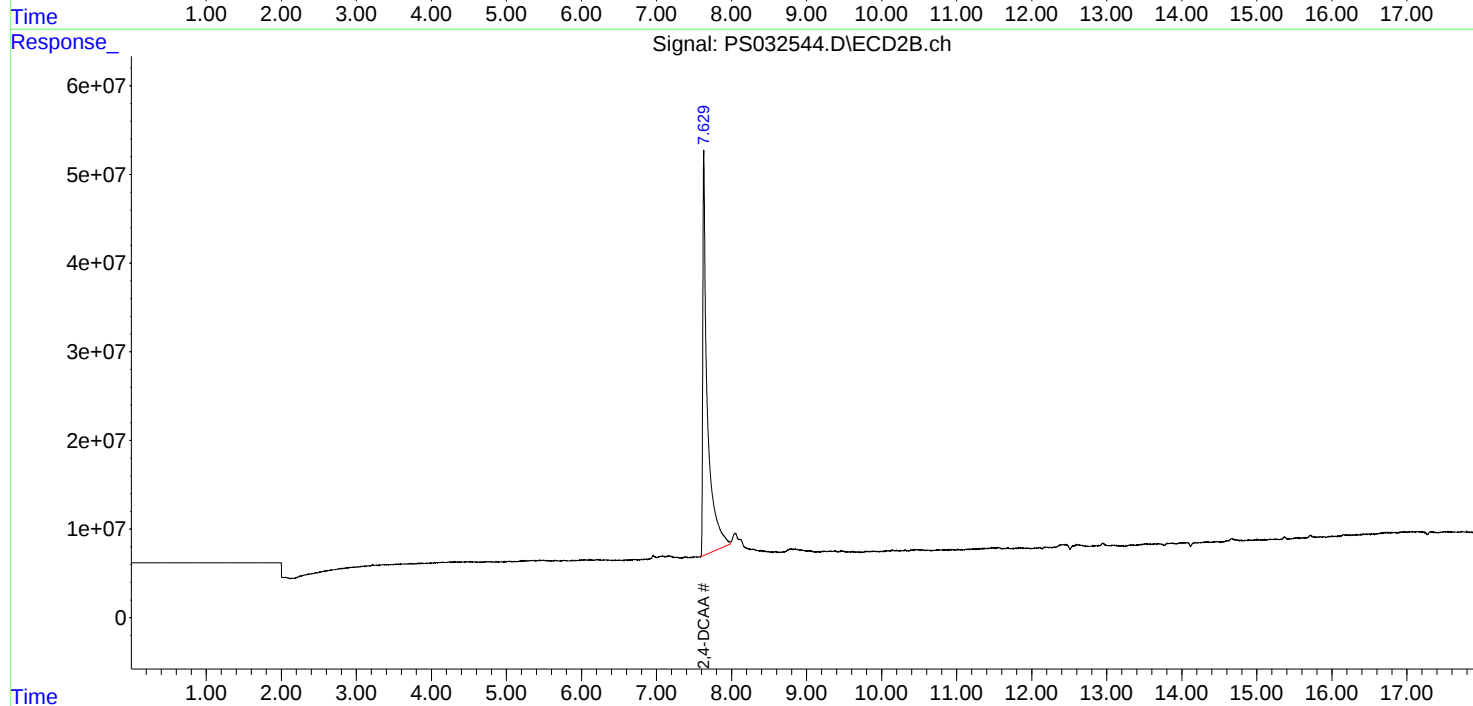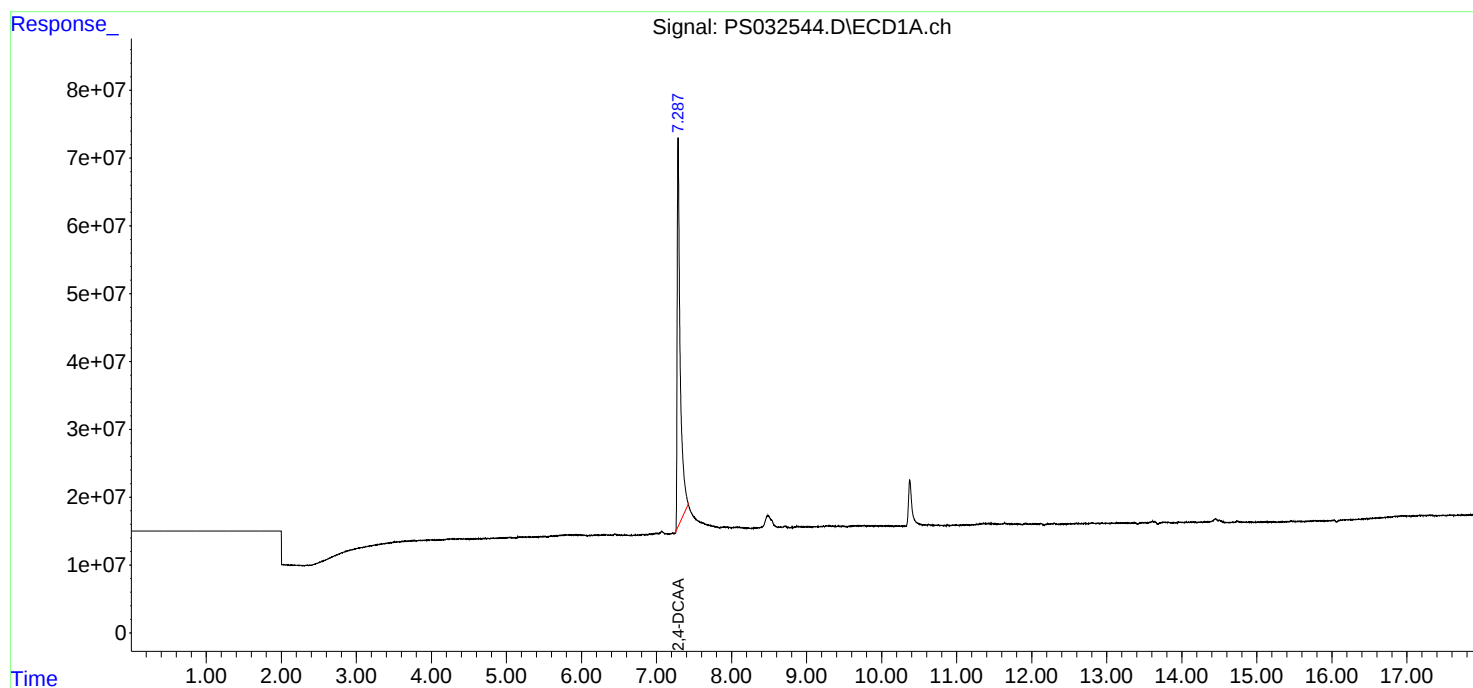


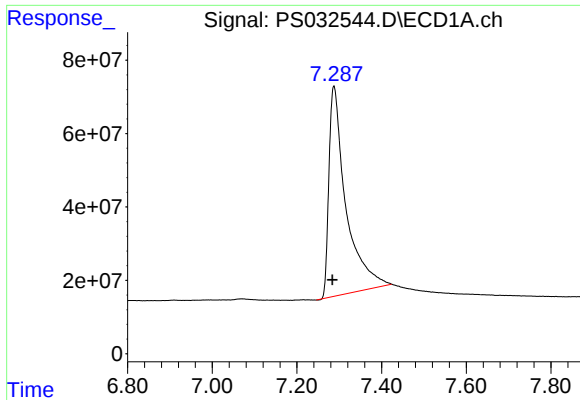

#4 2,4-DCAA

R.T.: 7.288 min
Delta R.T.: 0.004 min
Response: 1596372668
Conc: 352.30 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

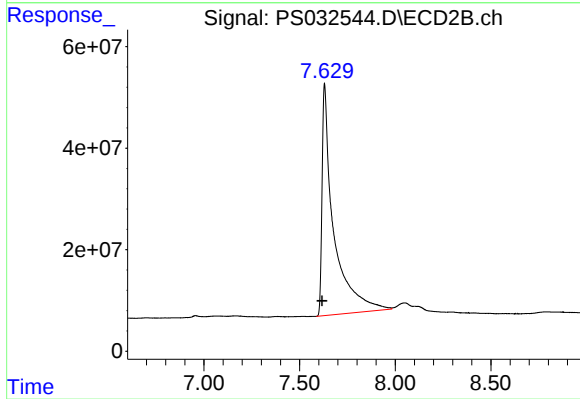

#4 2,4-DCAA

R.T.: 7.630 min
Delta R.T.: 0.013 min
Response: 1938432161
Conc: 531.73 ng/ml