

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112719\
 Data File : PS007859.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2019 13:41
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 15:39:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

5) T	DICAMBA	5.591	0.000	78994117	0	15.527	N.D.	#
10) T	Pentachlo...	0.000	6.435	0	8049533	N.D.	<MDL	
12) T	2,4,5-T	7.414	7.208	191.2E6	111.8E6	23.353	30.284	#
15) T	Picloram	8.955	8.893	574.9E6	323.7E6	51.778	55.247	
16) T	DCPA	0.000	8.837	0	9076680	N.D.	1.737	



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112719\
Data File : PS007859.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2019 13:41
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 15:39:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

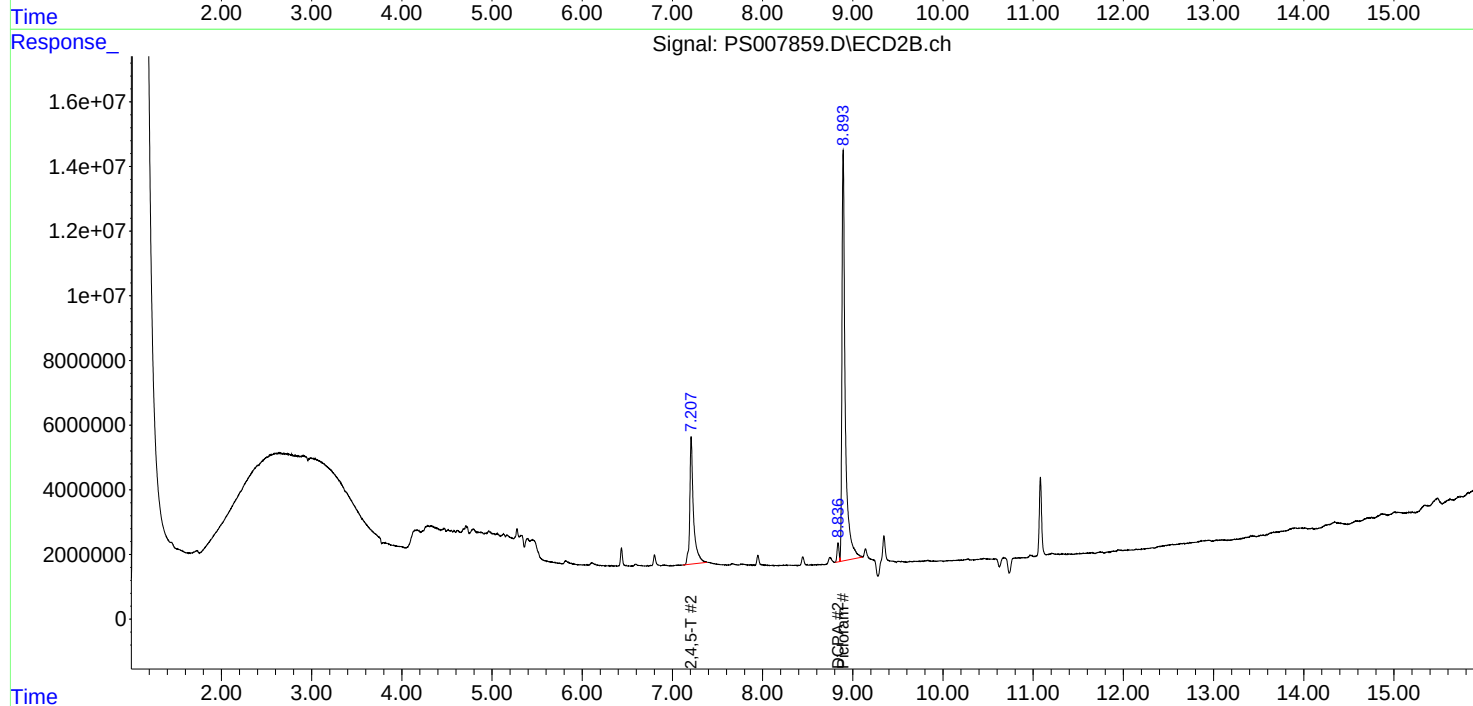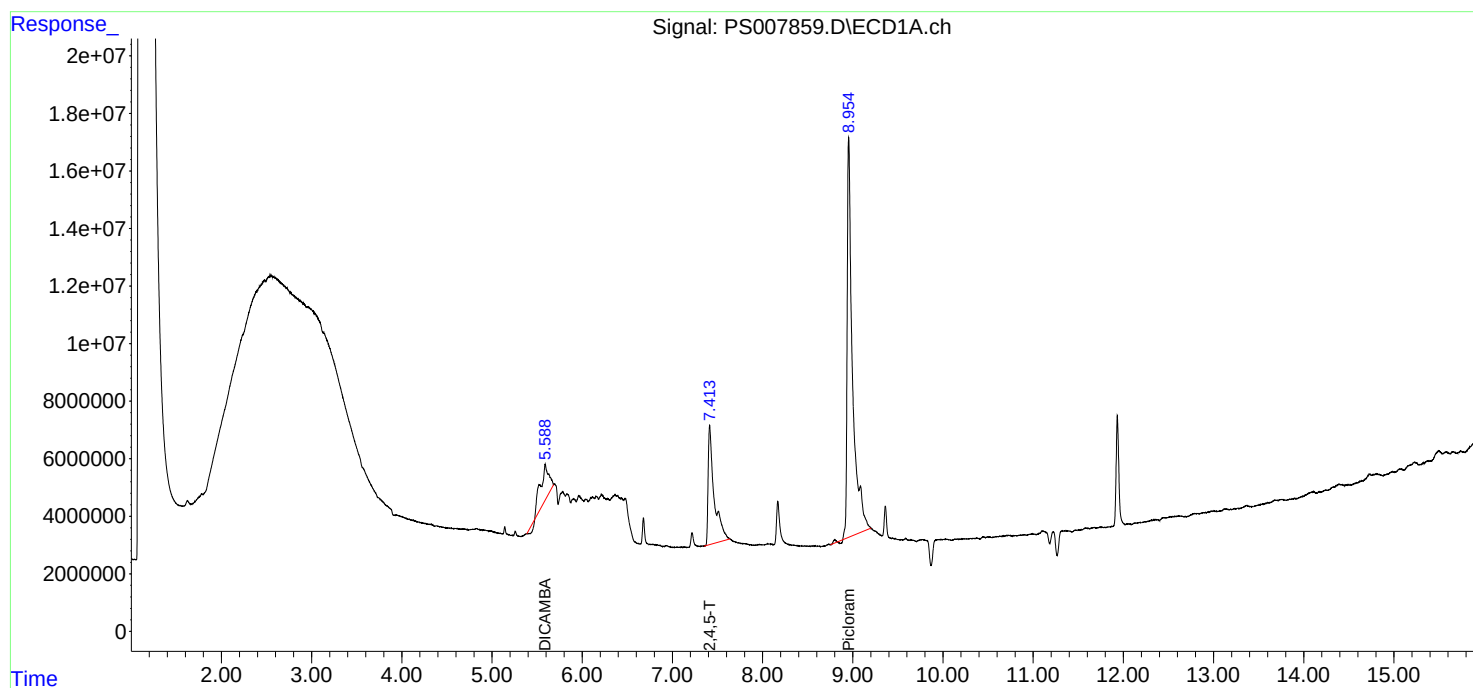


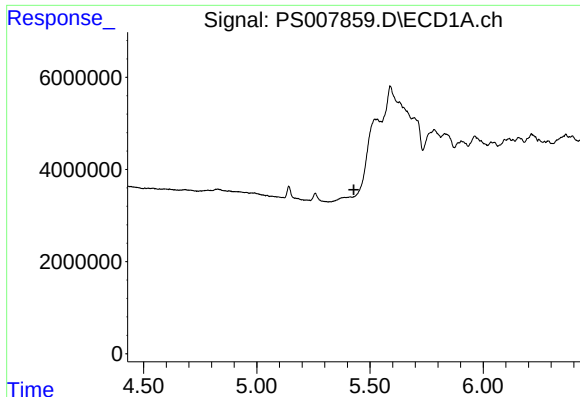

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 5.428 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

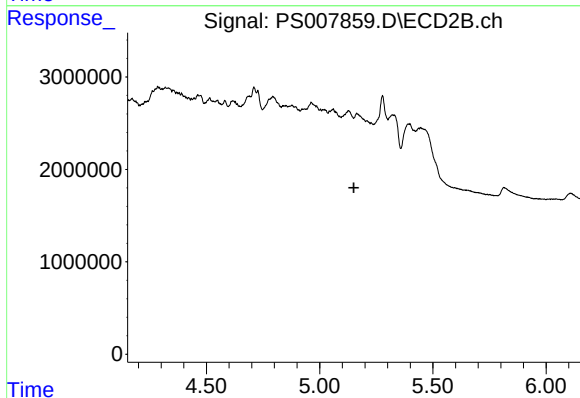


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 5.151 min
Response: 0
Conc: N.D.

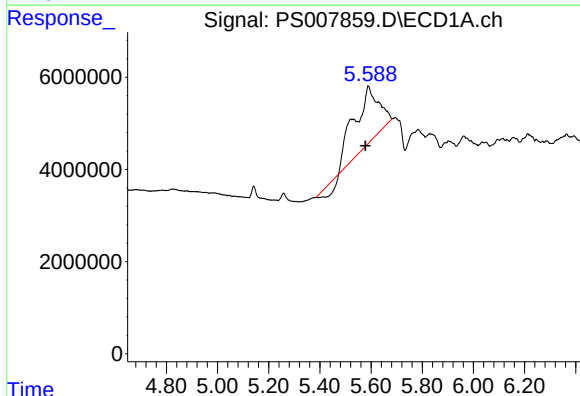


#5 DICAMBA

R.T.: 5.591 min
Delta R.T.: 0.013 min
Response: 78994117
Conc: 15.53 ng/ml

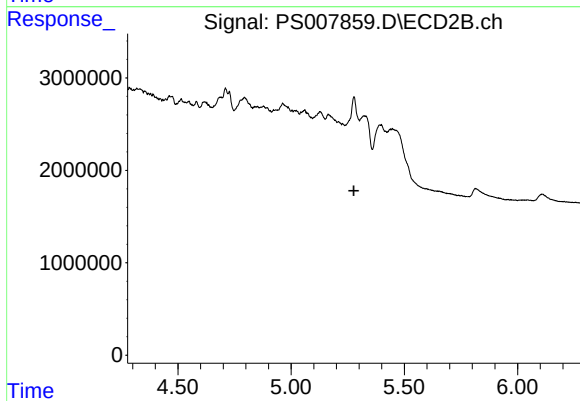

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.277 min
Response: 0
Conc: N.D.

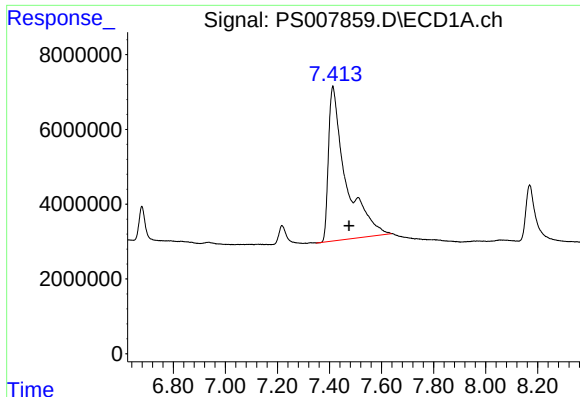

#12 2,4,5-T


R.T.: 7.414 min
Delta R.T.: -0.061 min
Response: 191169834
Conc: 23.35 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

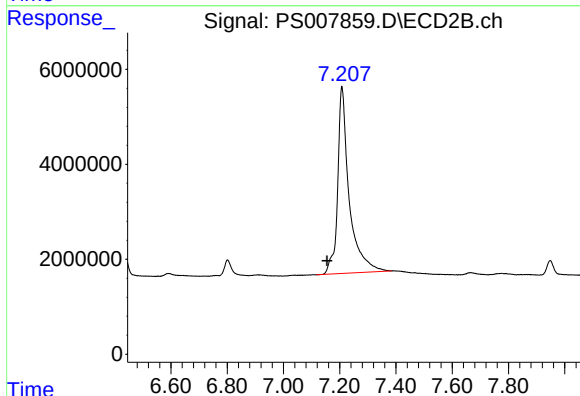


#12 2,4,5-T

R.T.: 7.208 min
Delta R.T.: 0.052 min
Response: 111834115
Conc: 30.28 ng/ml

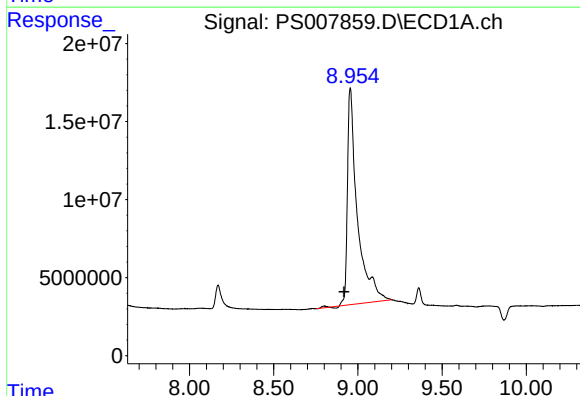


#15 Picloram

R.T.: 8.955 min
Delta R.T.: 0.037 min
Response: 574894710
Conc: 51.78 ng/ml

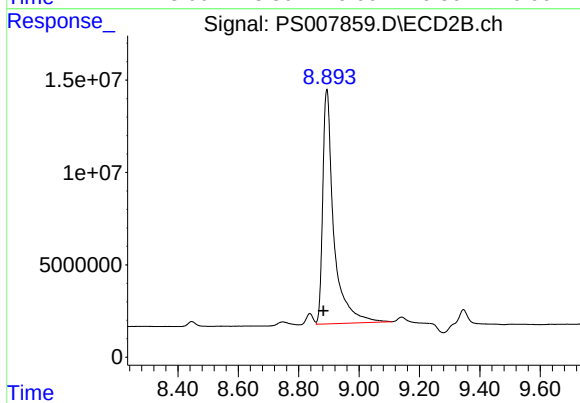

#15 Picloram


R.T.: 8.893 min
Delta R.T.: 0.011 min
Response: 323686348
Conc: 55.25 ng/ml

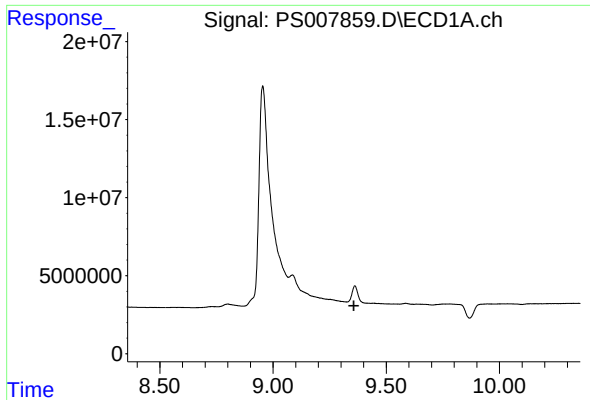

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.357 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

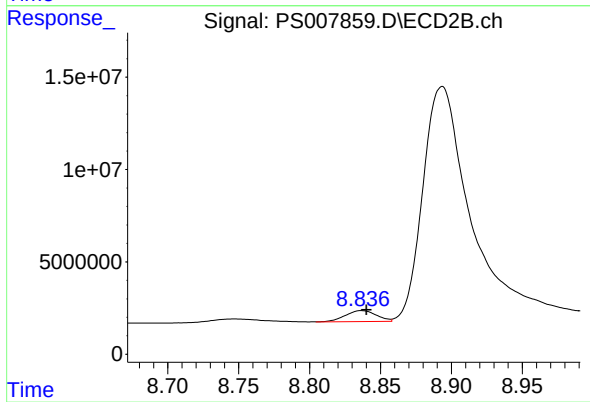

#16 DCPA

R.T.: 8.837 min
Delta R.T.: -0.003 min
Response: 9076680
Conc: 1.74 ng/ml