

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112719\
 Data File : PS007867.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2019 16:36
 Operator : SM\AJ
 Sample : PB125176BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 16:52:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.447	5.153	513.9E6	273.6E6	373.125	389.480
Target Compounds							
1) T	Dalapon	2.009	1.698	196.1E6	211.2E6	108.369	177.852 #
2) T	3,5-DICHL...	0.000	4.487	0	73597873	N.D.	81.465
5) T	DICAMBA	5.537	0.000	57158260	0	11.235	N.D. #
7) T	MCPA	5.912	5.520	44579828	26990587	8.099	8.980
9) T	2,4-D	0.000	6.056	0	7166820	N.D.	8.887
10) T	Pentachlo...	0.000	6.443	0	7734551	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	6.756	0	75251352	N.D.	19.217
12) T	2,4,5-T	7.413	0.000	89535131	0	10.938	N.D. #
14) T	DINOSEB	0.000	7.942	0	11129330	N.D.	3.828
15) T	Picloram	8.921	8.918	38146321	22544007	3.436	3.848



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112719\
Data File : PS007867.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2019 16:36
Operator : SM\AJ
Sample : PB125176BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 16:52:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

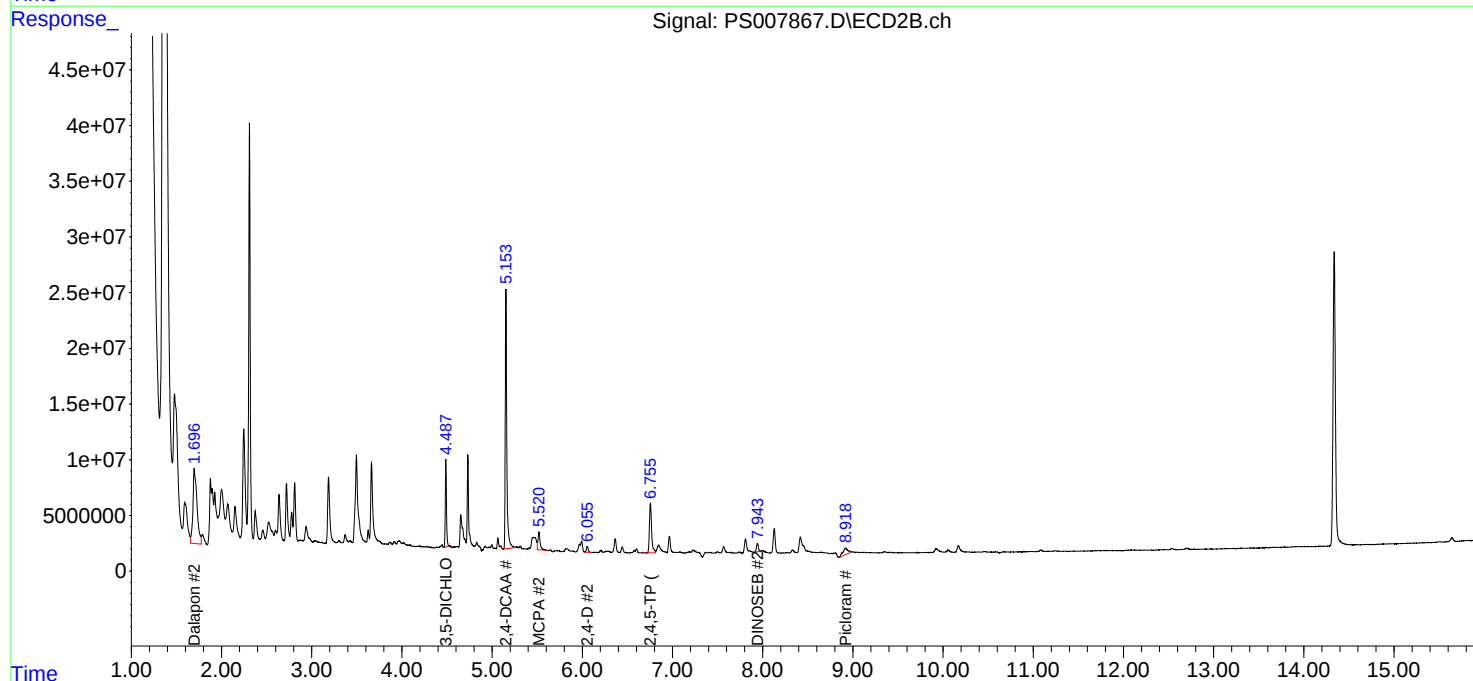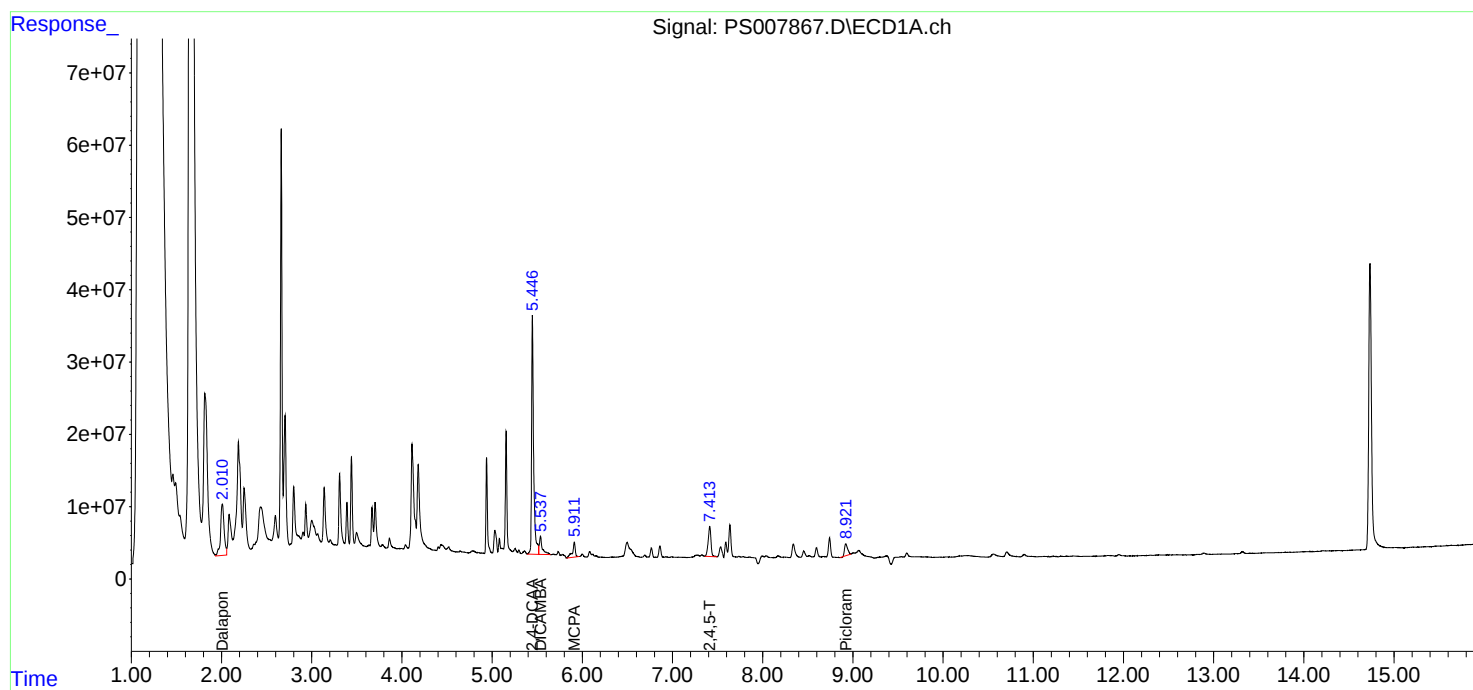


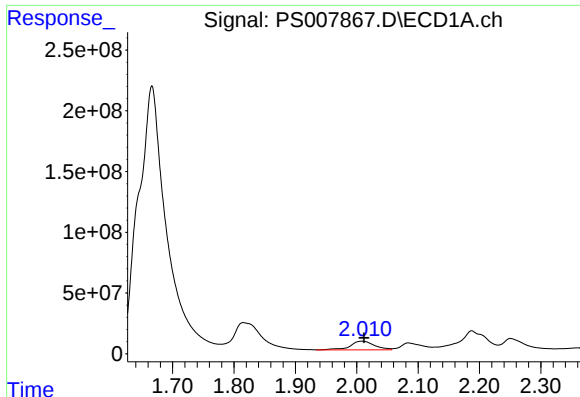

#1 Dalapon


R.T.: 2.009 min
Delta R.T.: -0.003 min
Response: 196059579
Conc: 108.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

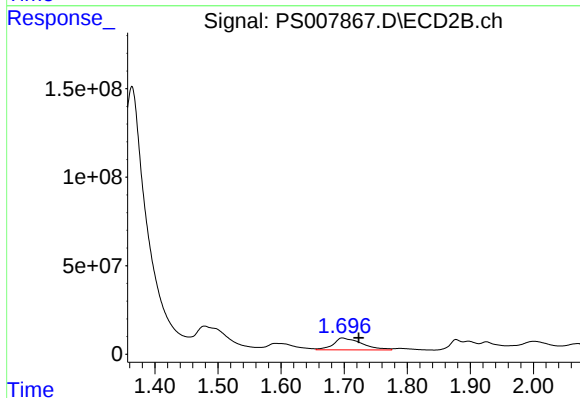


#1 Dalapon

R.T.: 1.698 min
Delta R.T.: -0.026 min
Response: 211181561
Conc: 177.85 ng/ml

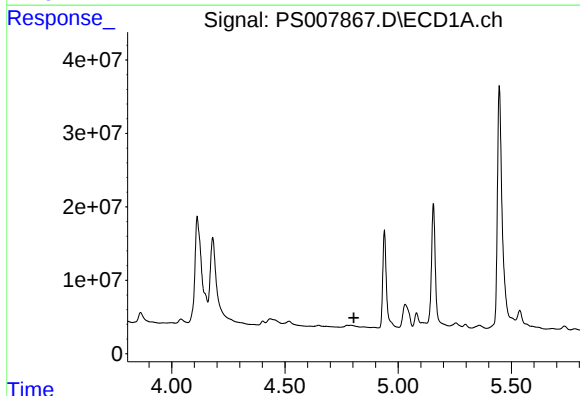


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.804 min
Response: 0
Conc: N.D.

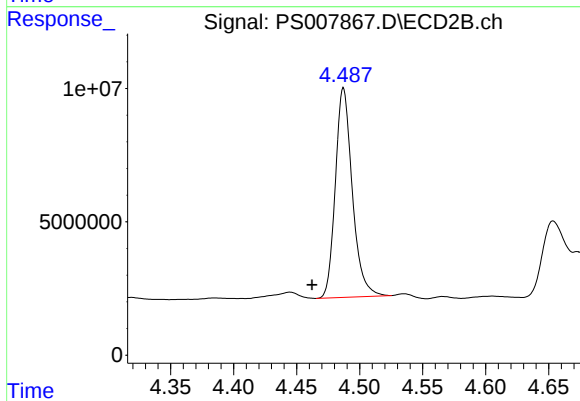

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.487 min
Delta R.T.: 0.025 min
Response: 73597873
Conc: 81.46 ng/ml

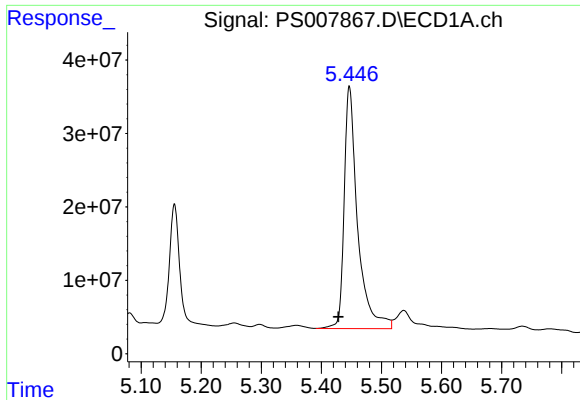

#4 2,4-DCAA


R.T.: 5.447 min
Delta R.T.: 0.019 min
Response: 513862547
Conc: 373.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

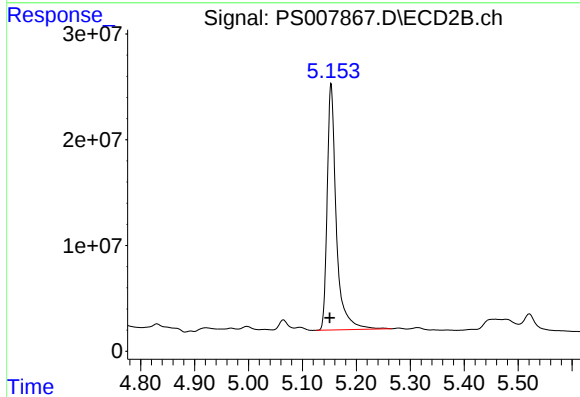


#4 2,4-DCAA

R.T.: 5.153 min
Delta R.T.: 0.002 min
Response: 273634567
Conc: 389.48 ng/ml

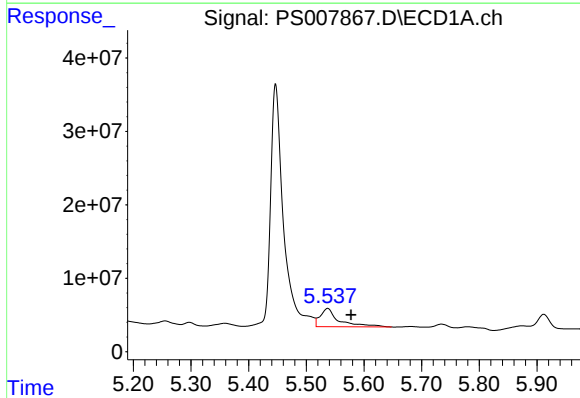


#5 DICAMBA

R.T.: 5.537 min
Delta R.T.: -0.040 min
Response: 57158260
Conc: 11.24 ng/ml

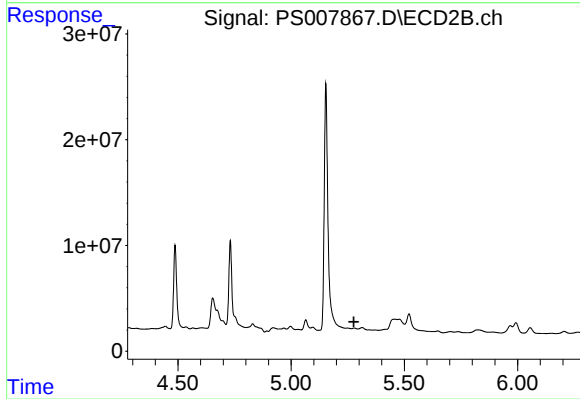

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 5.277 min
Response: 0
Conc: N.D.

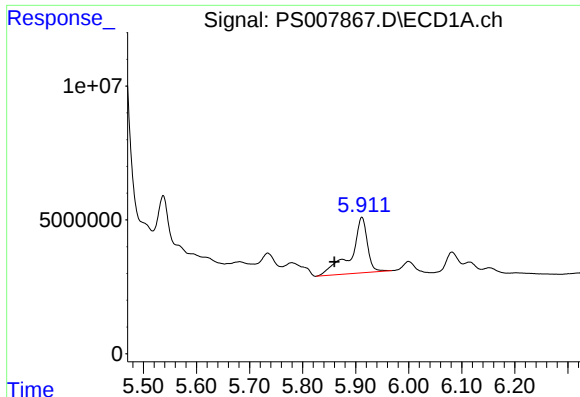

#7 MCPA


R.T.: 5.912 min
Delta R.T.: 0.052 min
Response: 44579828
Conc: 8.10 ug/ml

Instrument :
ECD_S
ClientSampleId :

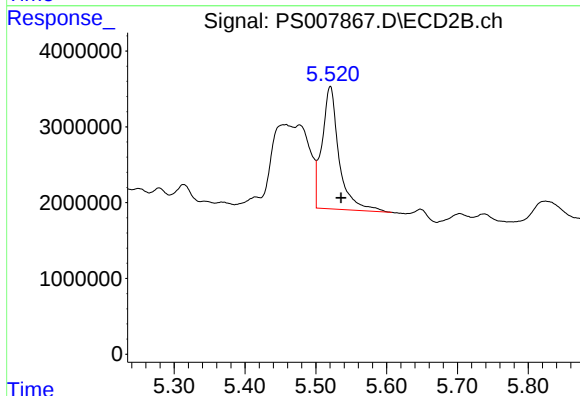


#7 MCPA

R.T.: 5.520 min
Delta R.T.: -0.015 min
Response: 26990587
Conc: 8.98 ug/ml

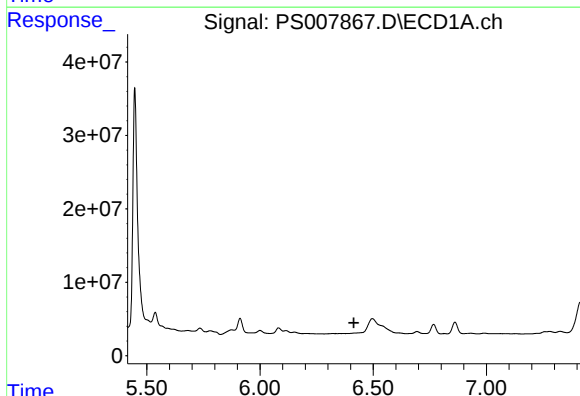


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.414 min
Response: 0
Conc: N.D.

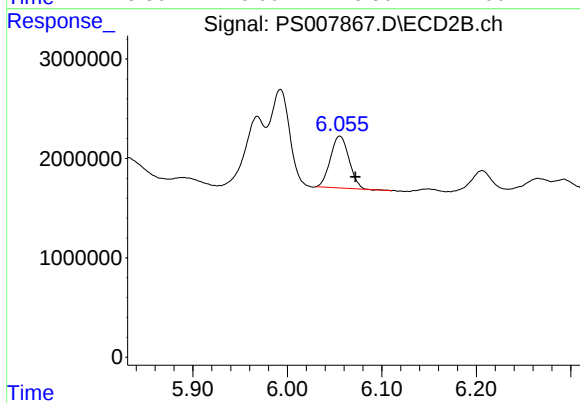

#9 2,4-D


R.T.: 6.056 min
Delta R.T.: -0.017 min
Response: 7166820
Conc: 8.89 ng/ml

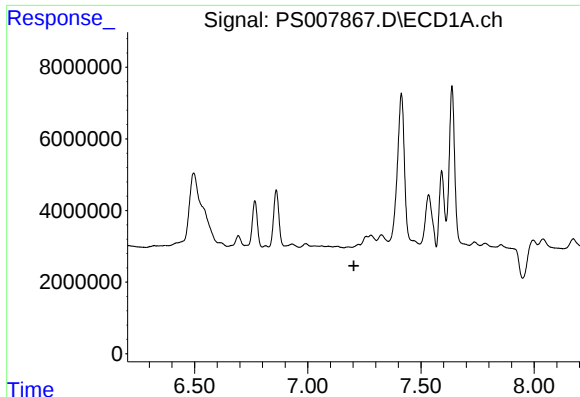

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.203 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

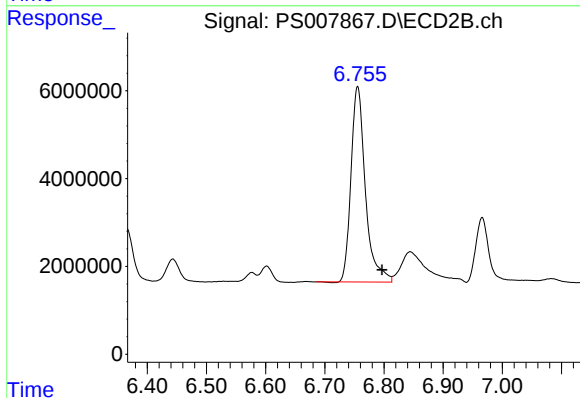


#11 2,4,5-TP (SILVEX)

R.T.: 6.756 min
Delta R.T.: -0.042 min
Response: 75251352
Conc: 19.22 ng/ml

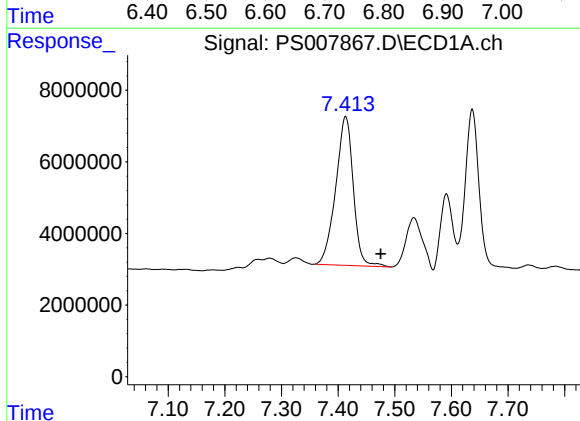


#12 2,4,5-T

R.T.: 7.413 min
Delta R.T.: -0.062 min
Response: 89535131
Conc: 10.94 ng/ml

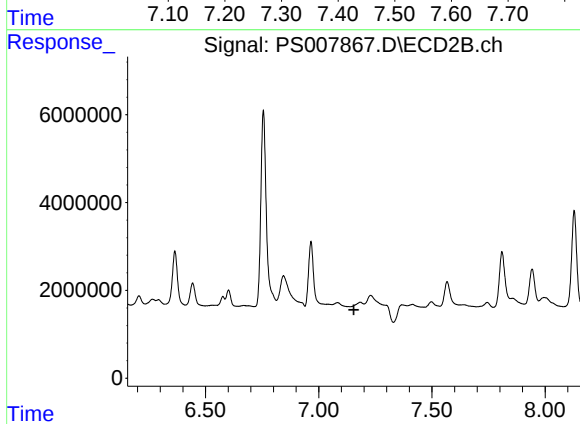

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.156 min
Response: 0
Conc: N.D.

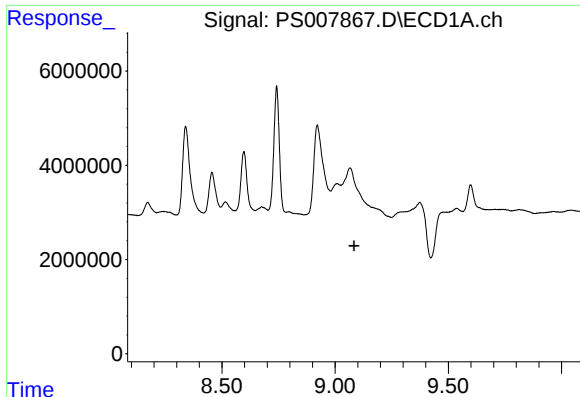

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.083 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

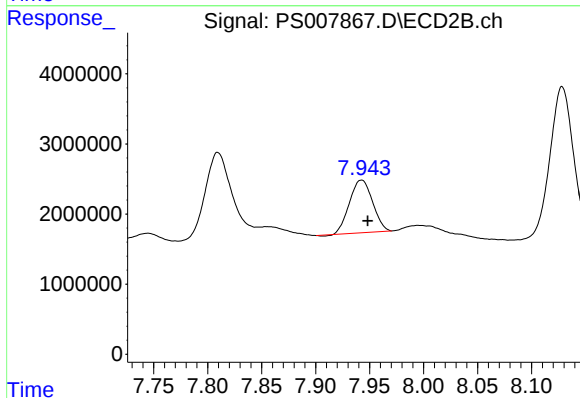


#14 DINOSEB

R.T.: 7.942 min
Delta R.T.: -0.006 min
Response: 11129330
Conc: 3.83 ng/ml

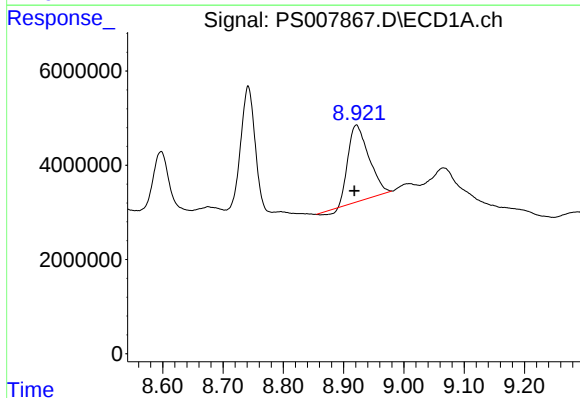

#15 Picloram

R.T.: 8.921 min
Delta R.T.: 0.004 min
Response: 38146321
Conc: 3.44 ng/ml

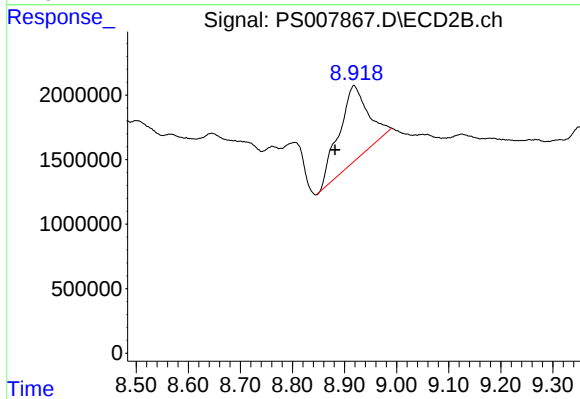

#15 Picloram

R.T.: 8.918 min
Delta R.T.: 0.036 min
Response: 22544007
Conc: 3.85 ng/ml