

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112719\
 Data File : PS007872.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2019 18:26
 Operator : SM\AJ
 Sample : K5675-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 28 02:47:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.410	0.000	753.9E6	0	547.433	N.D. #
Target Compounds							
1) T	Dalapon	2.050	1.681	146.0E6	340.2E6	80.715	286.468 #
2) T	3,5-DICHL...	0.000	4.470	0	53298588	N.D.	58.996
6) T	MCP	0.000	5.430	0	6350567	N.D.	3.269
8) T	DICHLORPROP	0.000	5.796	0	15991840	N.D.	24.385
9) T	2,4-D	6.462	0.000	72250820	0	51.514	N.D. #
11) T	2,4,5-TP ...	0.000	6.829	0	30738037	N.D.	7.850
12) T	2,4,5-T	7.498	0.000	48914925	0	5.975	N.D. #
15) T	Picloram	8.873	0.000	135.7E6	0	12.224	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112719\
Data File : PS007872.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2019 18:26
Operator : SM\AJ
Sample : K5675-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 28 02:47:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

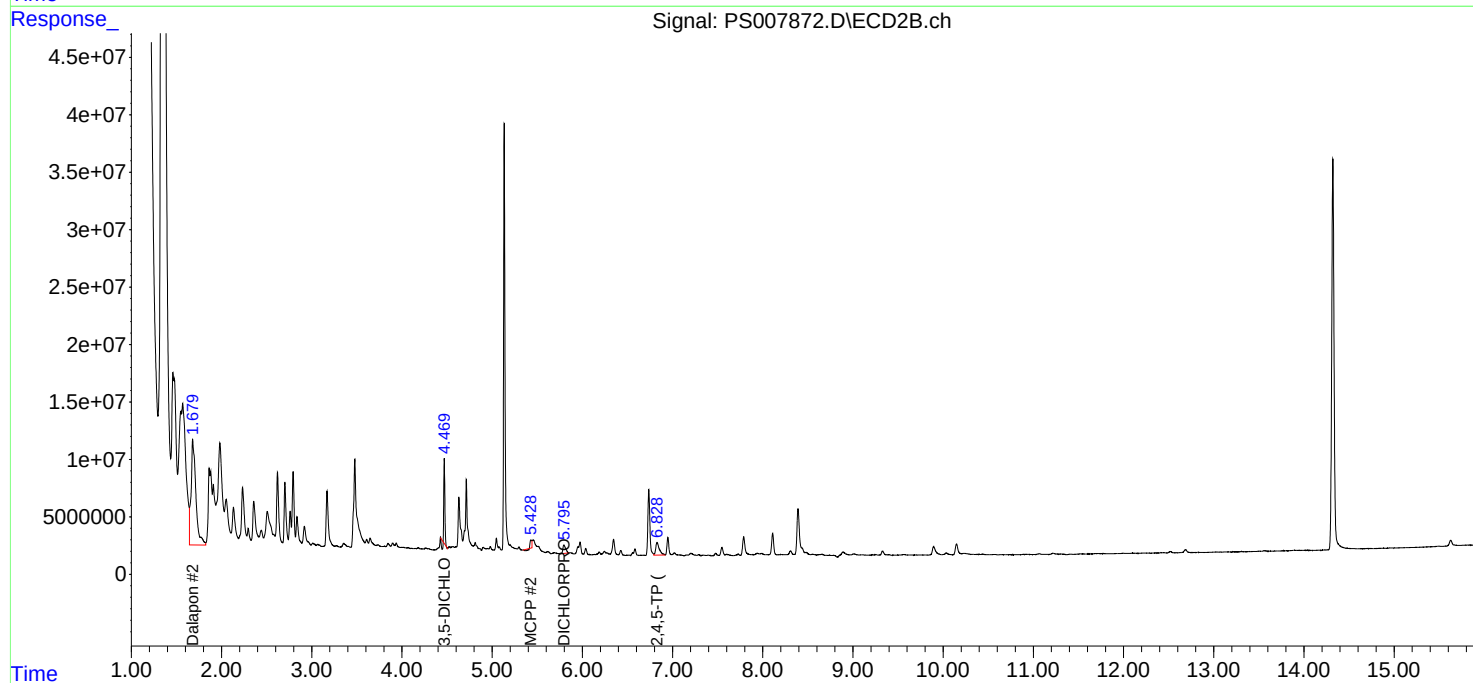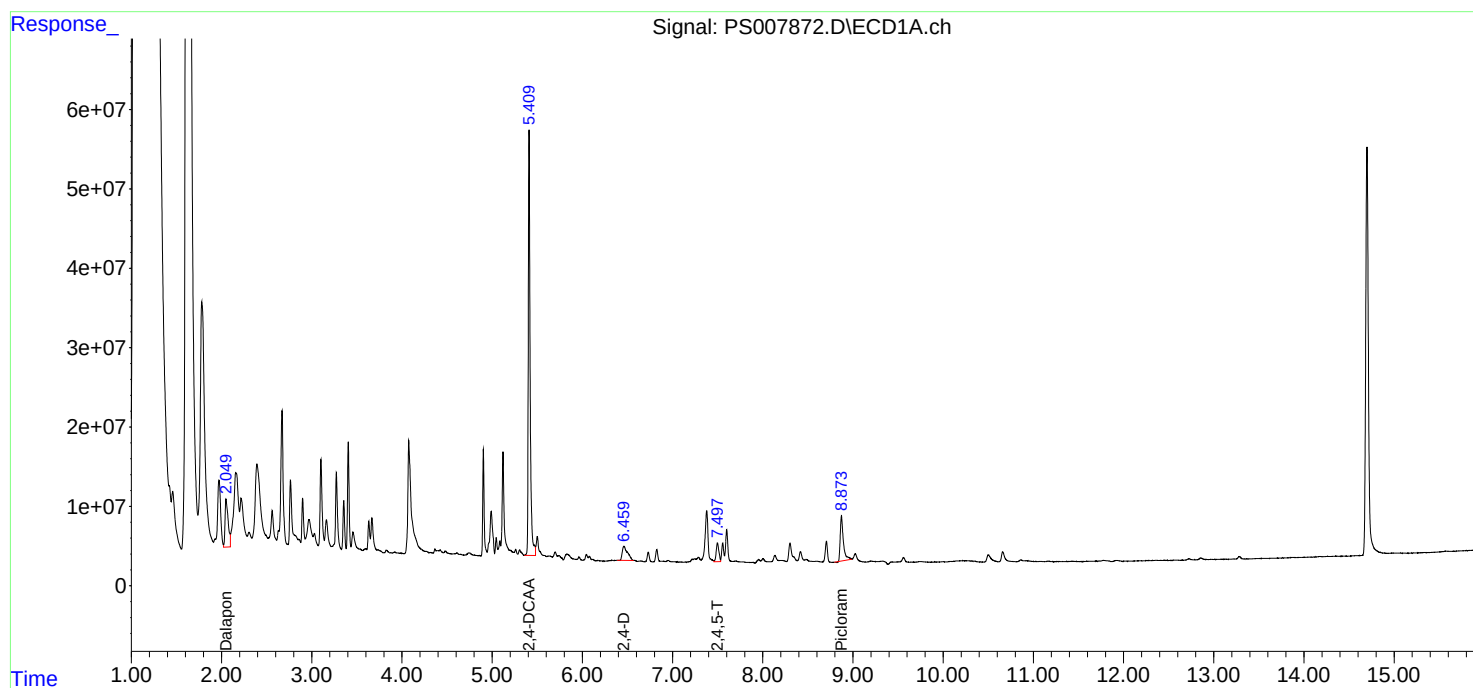


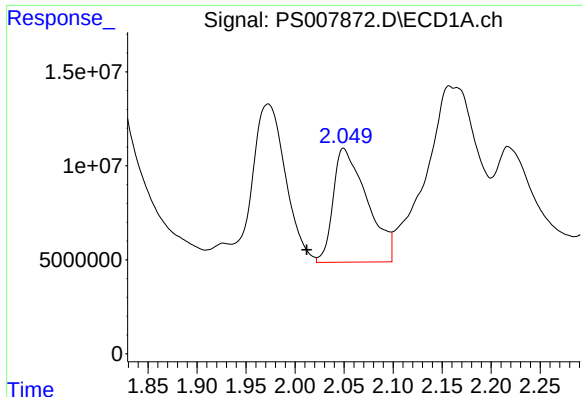

#1 Dalapon


R.T.: 2.050 min
Delta R.T.: 0.038 min
Response: 146028809
Conc: 80.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

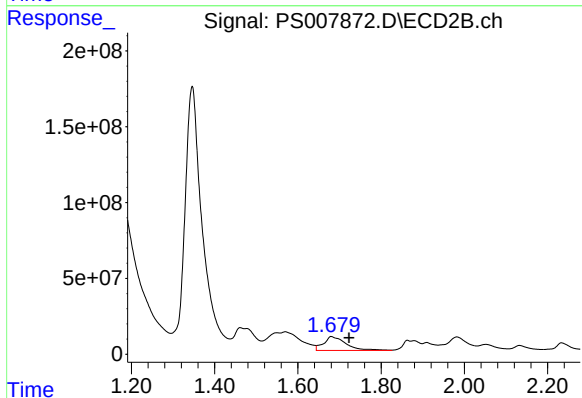


#1 Dalapon

R.T.: 1.681 min
Delta R.T.: -0.043 min
Response: 340152916
Conc: 286.47 ng/ml

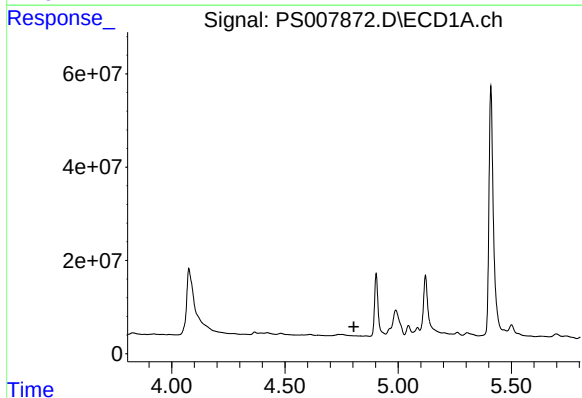


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.804 min
Response: 0
Conc: N.D.

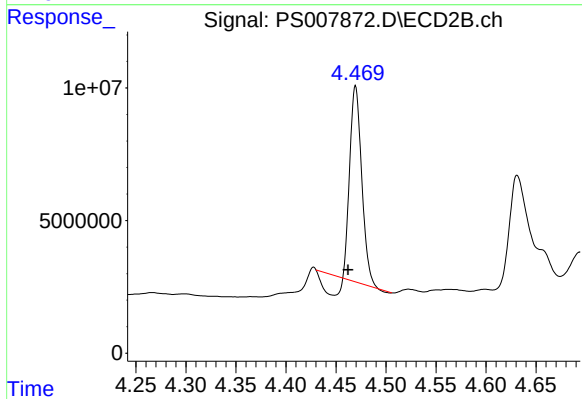

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.470 min
Delta R.T.: 0.008 min
Response: 53298588
Conc: 59.00 ng/ml

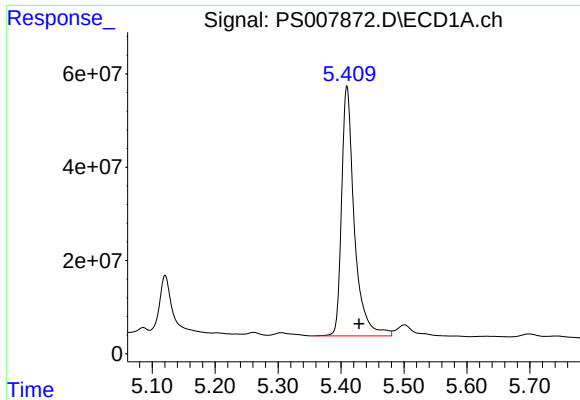

#4 2,4-DCAA


R.T.: 5.410 min
Delta R.T.: -0.019 min
Response: 753916072
Conc: 547.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

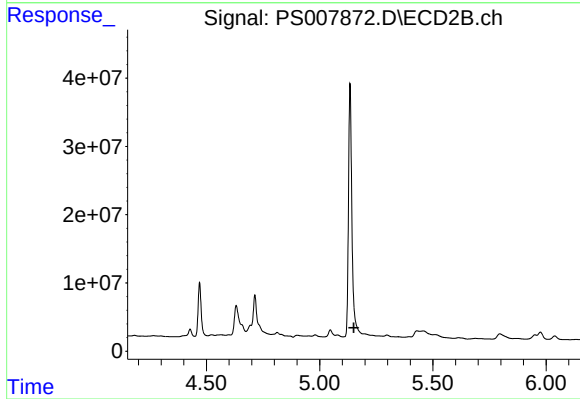


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 5.151 min
Response: 0
Conc: N.D.

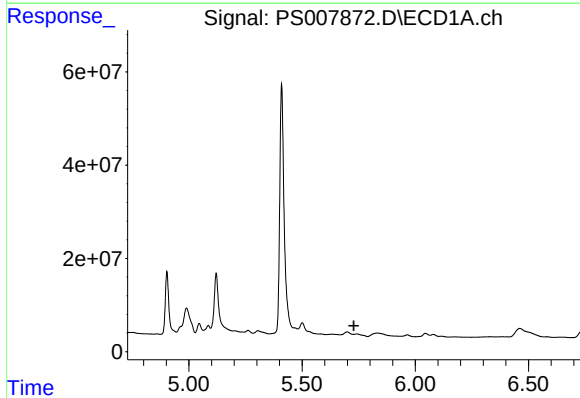


#6 MCP

R.T.: 0.000 min
Exp R.T. : 5.729 min
Response: 0
Conc: N.D.

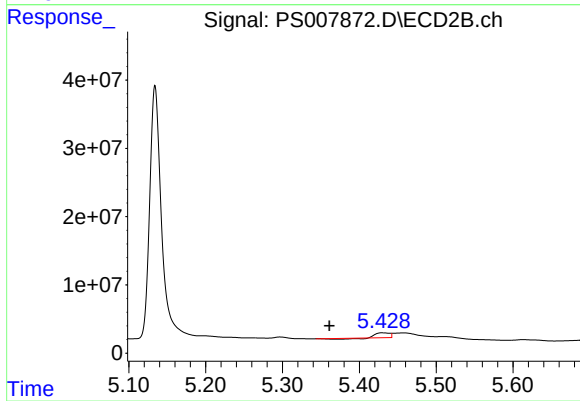

#6 MCP


R.T.: 5.430 min
Delta R.T.: 0.069 min
Response: 6350567
Conc: 3.27 ug/ml

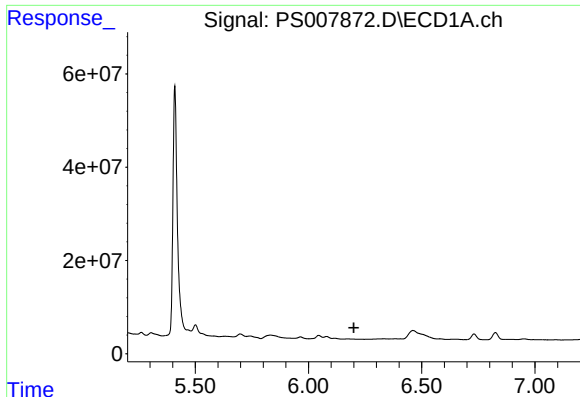

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.200 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

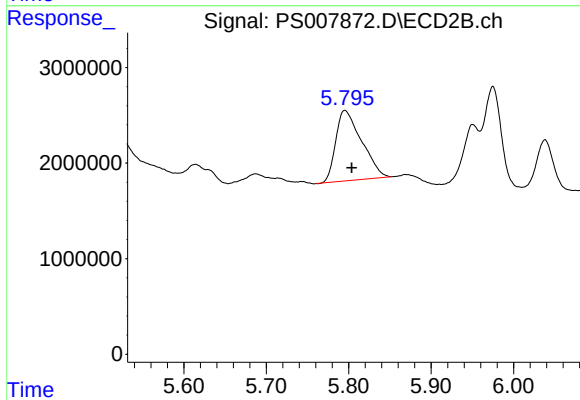


#8 DICHLORPROP

R.T.: 5.796 min
Delta R.T.: -0.008 min
Response: 15991840
Conc: 24.39 ng/ml

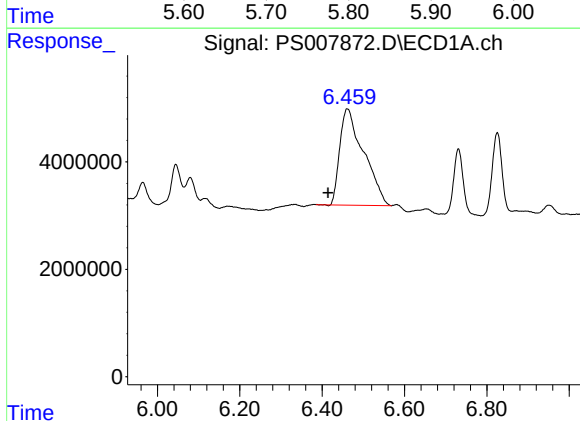


#9 2,4-D

R.T.: 6.462 min
Delta R.T.: 0.047 min
Response: 72250820
Conc: 51.51 ng/ml

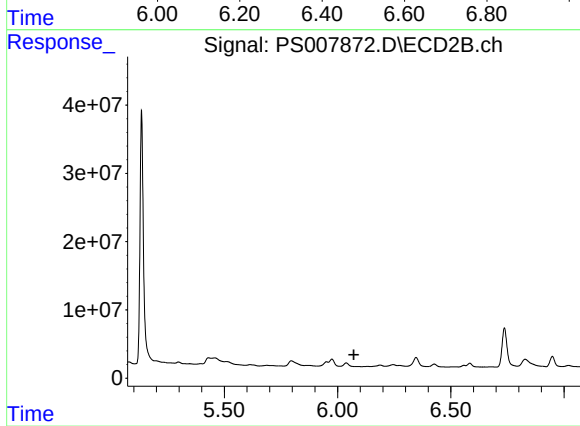

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.072 min
Response: 0
Conc: N.D.

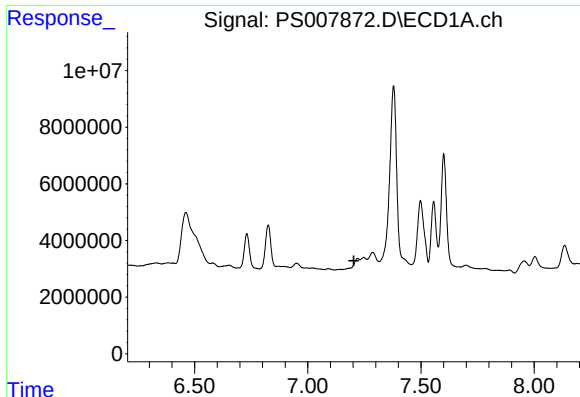

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.203 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

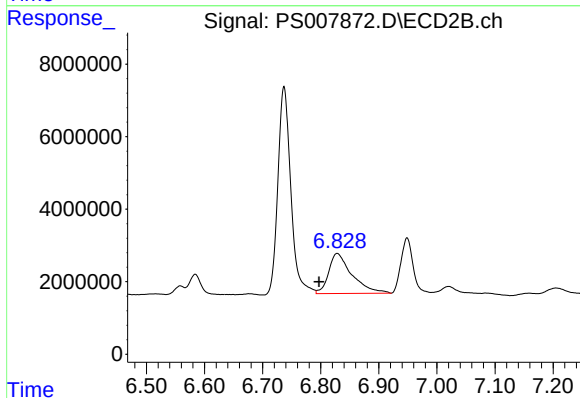


#11 2,4,5-TP (SILVEX)

R.T.: 6.829 min
Delta R.T.: 0.032 min
Response: 30738037
Conc: 7.85 ng/ml

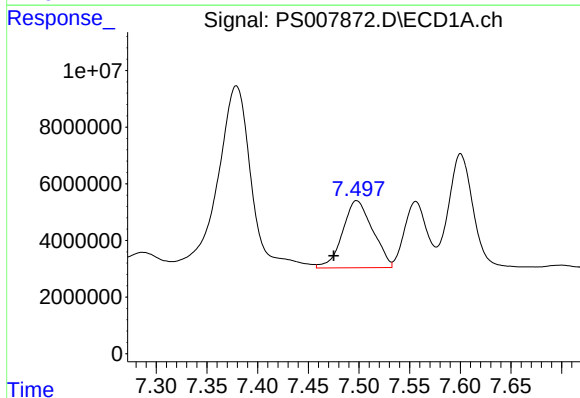


#12 2,4,5-T

R.T.: 7.498 min
Delta R.T.: 0.023 min
Response: 48914925
Conc: 5.98 ng/ml

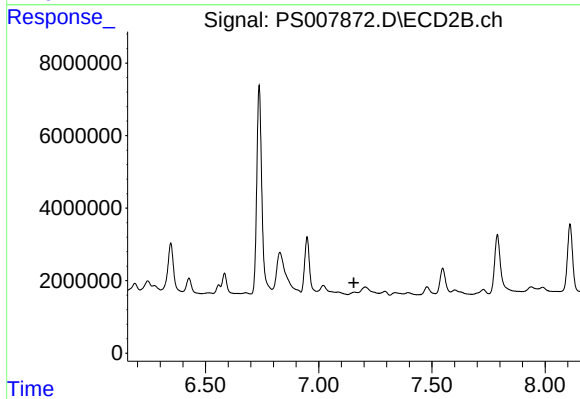

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.156 min
Response: 0
Conc: N.D.

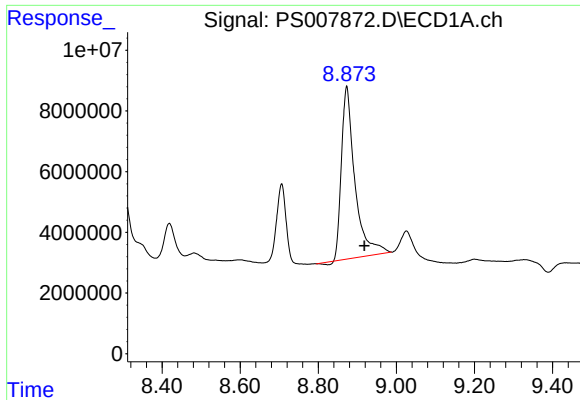

#15 Picloram

R.T.: 8.873 min
Delta R.T.: -0.045 min
Response: 135730313
Conc: 12.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

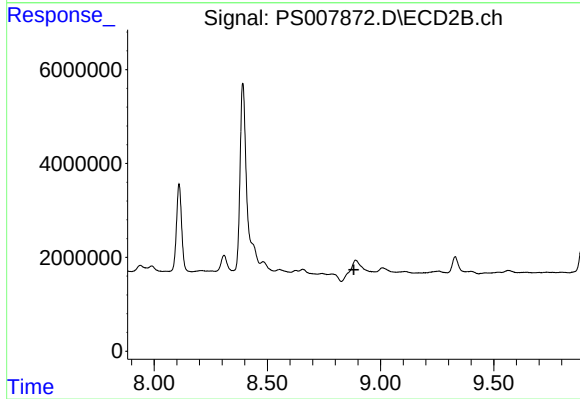

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.882 min
Response: 0
Conc: N.D.