

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112719\
 Data File : PS007875.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2019 19:31
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 28 02:48:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.429	5.153	665.1E6	366.9E6	482.918	522.283
Target Compounds							
5) T	DICAMBA	0.000	5.279	0 13036612		N.D.	4.926
7) T	MCPA	0.000	5.474	0 53256443		N.D.	17.718
9) T	2,4-D	6.479	0.000	78430702	0	55.920	N.D. #
15) T	Picloram	0.000	8.931	0 20248195		N.D.	3.456



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112719\
Data File : PS007875.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2019 19:31
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 28 02:48:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

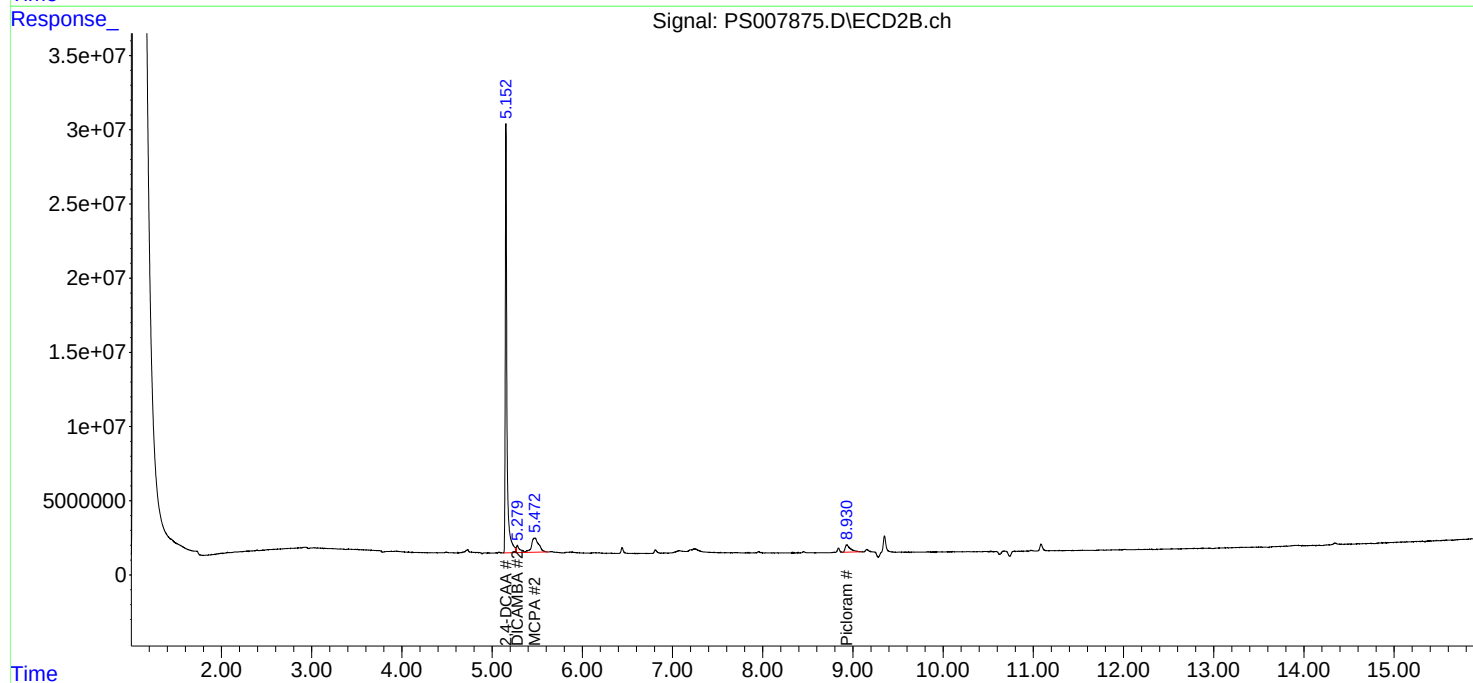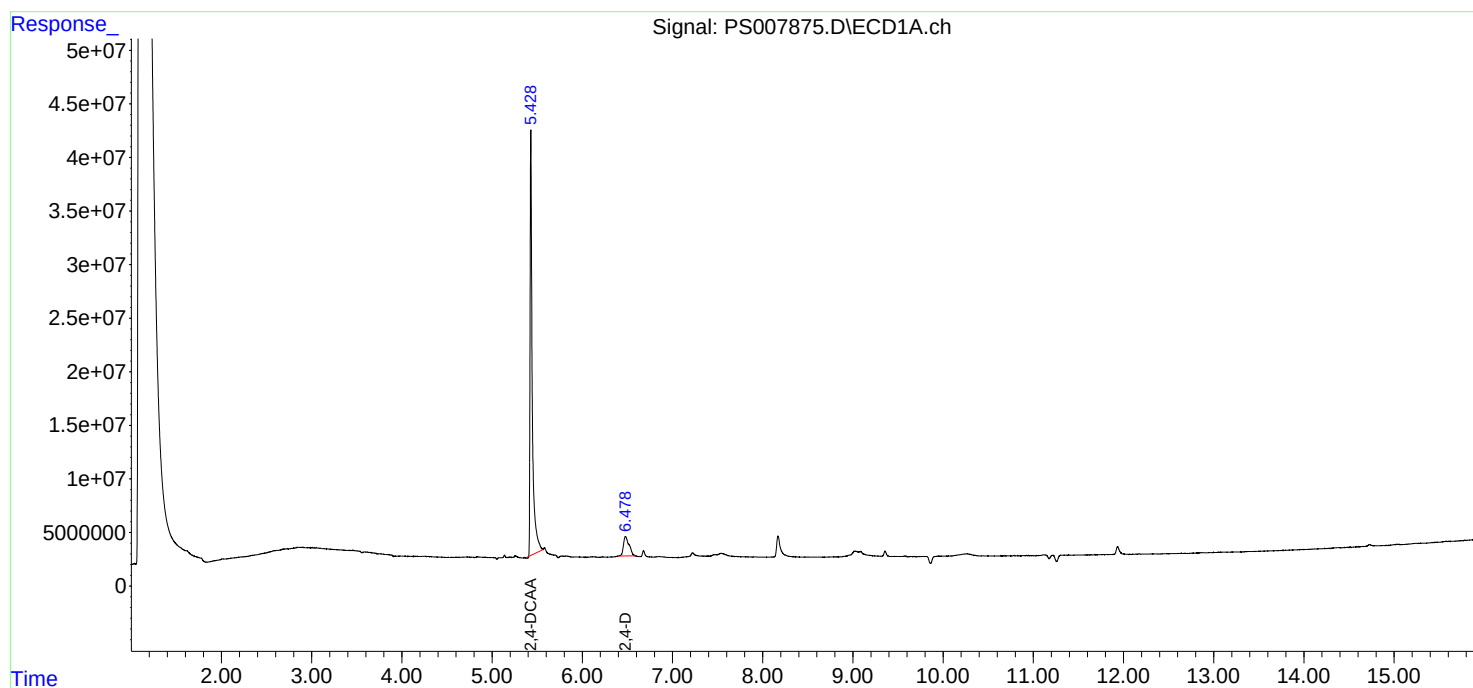


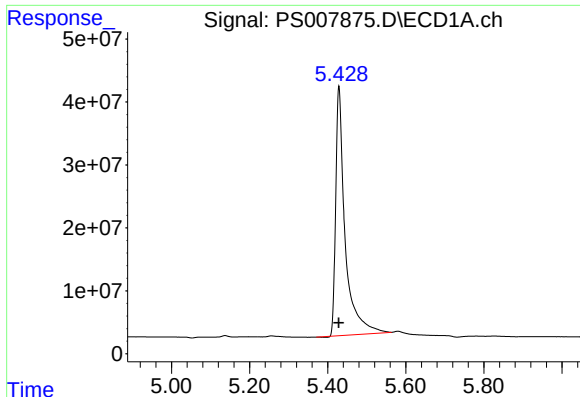

#4 2,4-DCAA


R.T.: 5.429 min
Delta R.T.: 0.000 min
Response: 665067518
Conc: 482.92 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

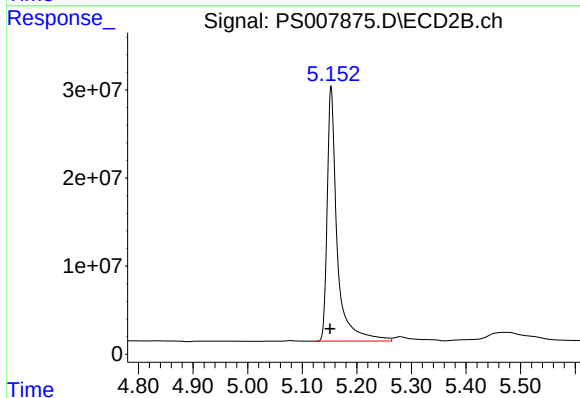


#4 2,4-DCAA

R.T.: 5.153 min
Delta R.T.: 0.002 min
Response: 366937599
Conc: 522.28 ng/ml

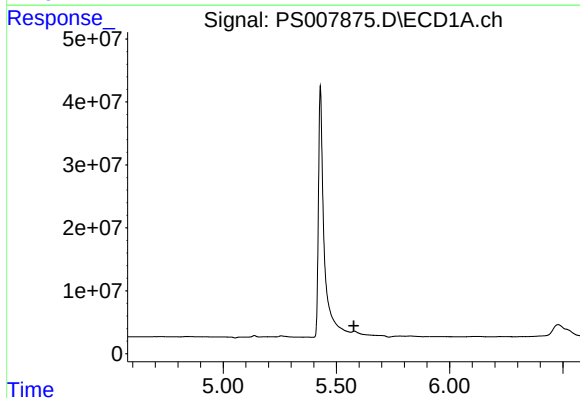


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.577 min
Response: 0
Conc: N.D.

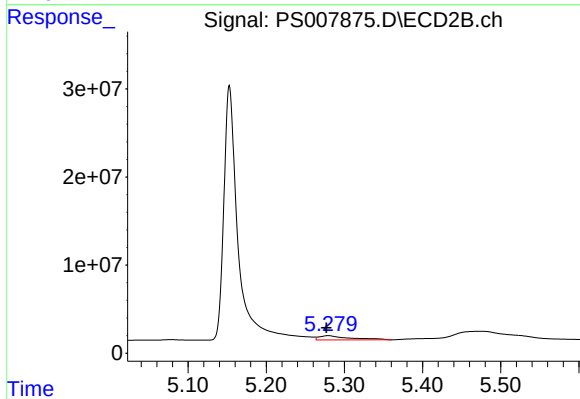

#5 DICAMBA


R.T.: 5.279 min
Delta R.T.: 0.002 min
Response: 13036612
Conc: 4.93 ng/ml

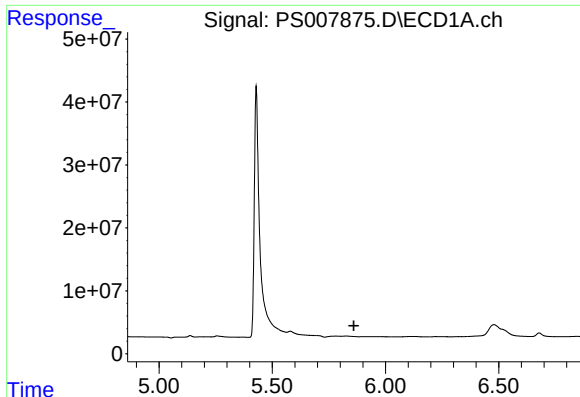

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.860 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

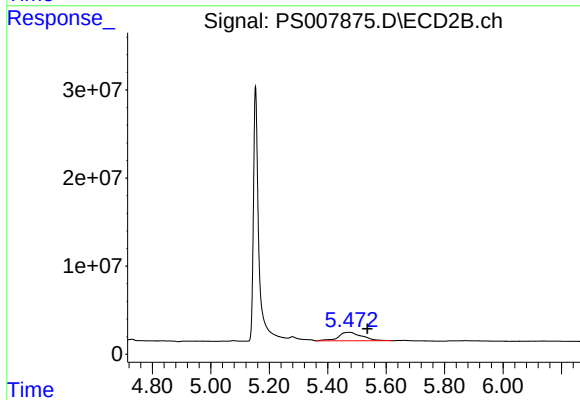


#7 MCPA

R.T.: 5.474 min
Delta R.T.: -0.062 min
Response: 53256443
Conc: 17.72 ug/ml

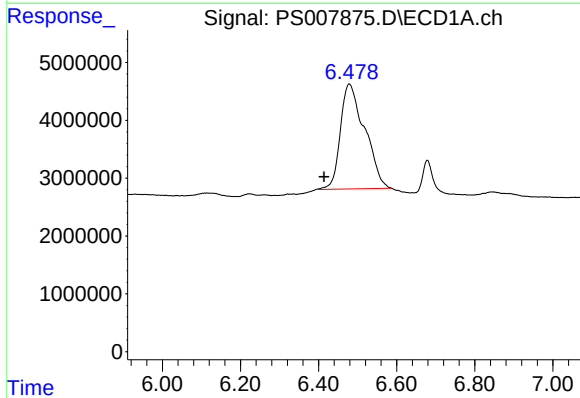


#9 2,4-D

R.T.: 6.479 min
Delta R.T.: 0.064 min
Response: 78430702
Conc: 55.92 ng/ml

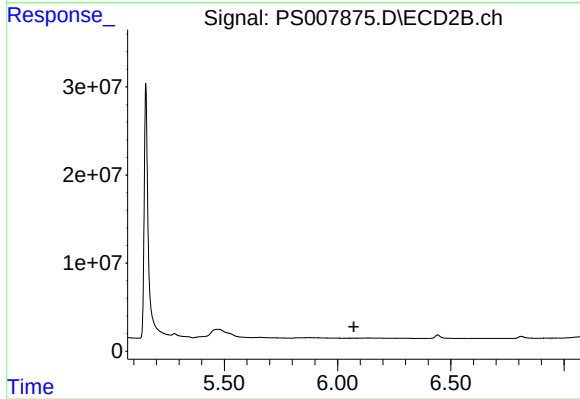

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.072 min
Response: 0
Conc: N.D.

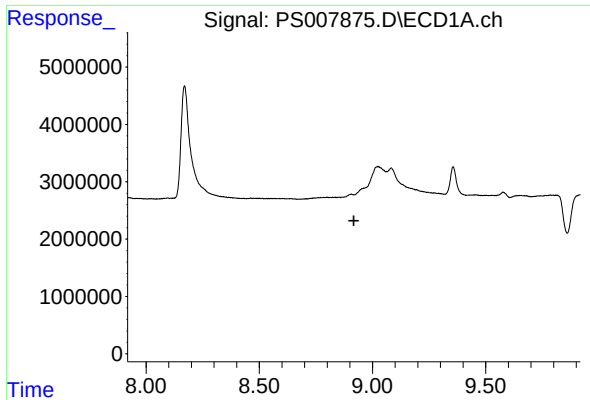

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.918 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

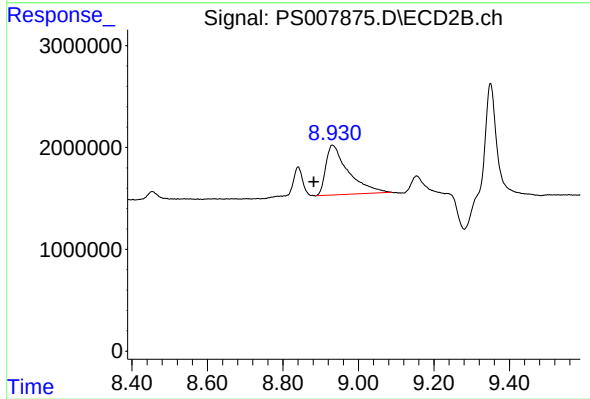

#15 Picloram

R.T.: 8.931 min
Delta R.T.: 0.049 min
Response: 20248195
Conc: 3.46 ng/ml