

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112723\
 Data File : PS024949.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2023 14:12
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 23:46:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 03 15:07:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.356	6.771	1195.9E6	386.5E6	585.772	572.989
Target Compounds							
1) T	Dalapon	2.511	2.565	7945528	5246015	3.298	4.979 #
3) T	4-Nitroph...	6.198	6.369	7106056	523661	5.482	1.193 #
8) T	DICHLORPROP	0.000	7.560	0	2515428	N.D.	3.443
9) T	2,4-D	0.000	7.771f	0	769311	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.614	0	60913	N.D.	<MDL
12) T	2,4,5-T	0.000	9.022	0	3246772	N.D.	<MDL
15) T	Picloram	9.681	10.764	53389967	15438845	3.002	2.541
16) T	DCPA	0.000	10.764	0	15438845	N.D.	3.072



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112723\
Data File : PS024949.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2023 14:12
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 23:46:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
Quant Title : 8080.M
QLast Update : Fri Nov 03 15:07:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

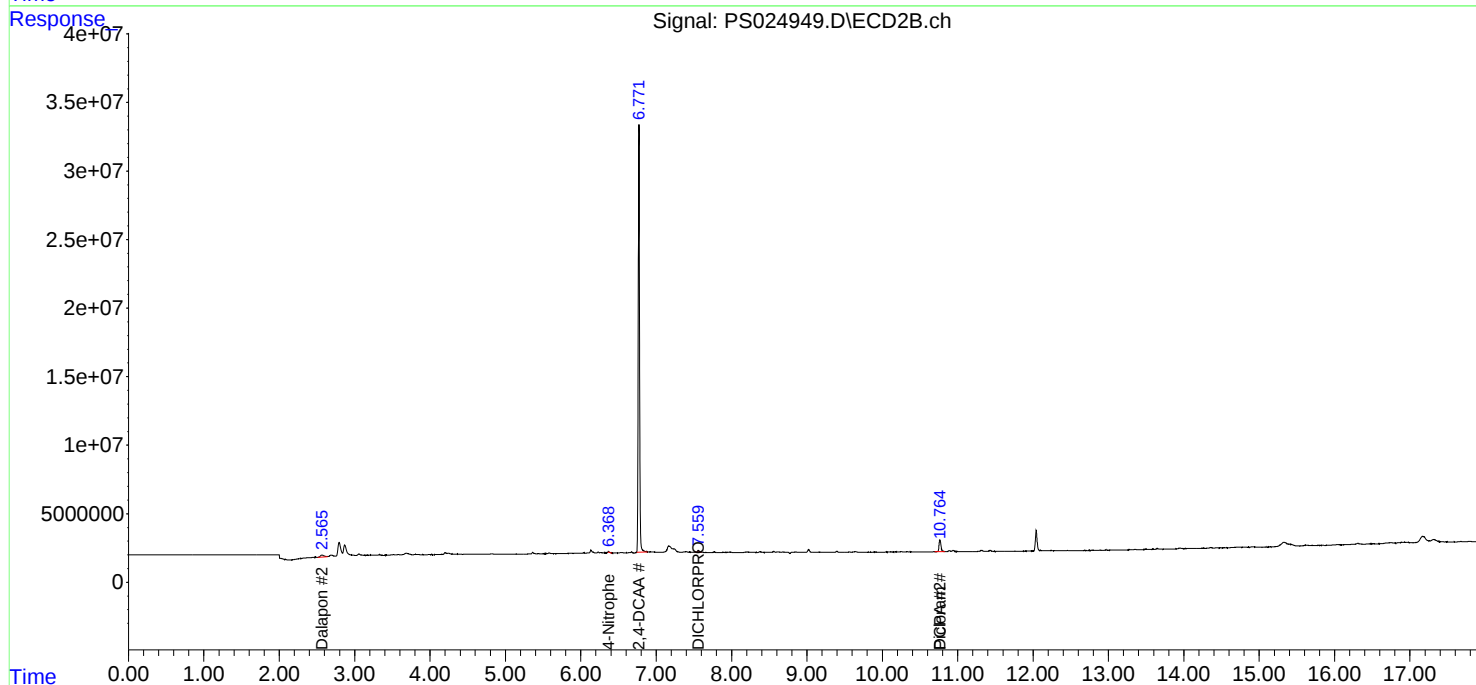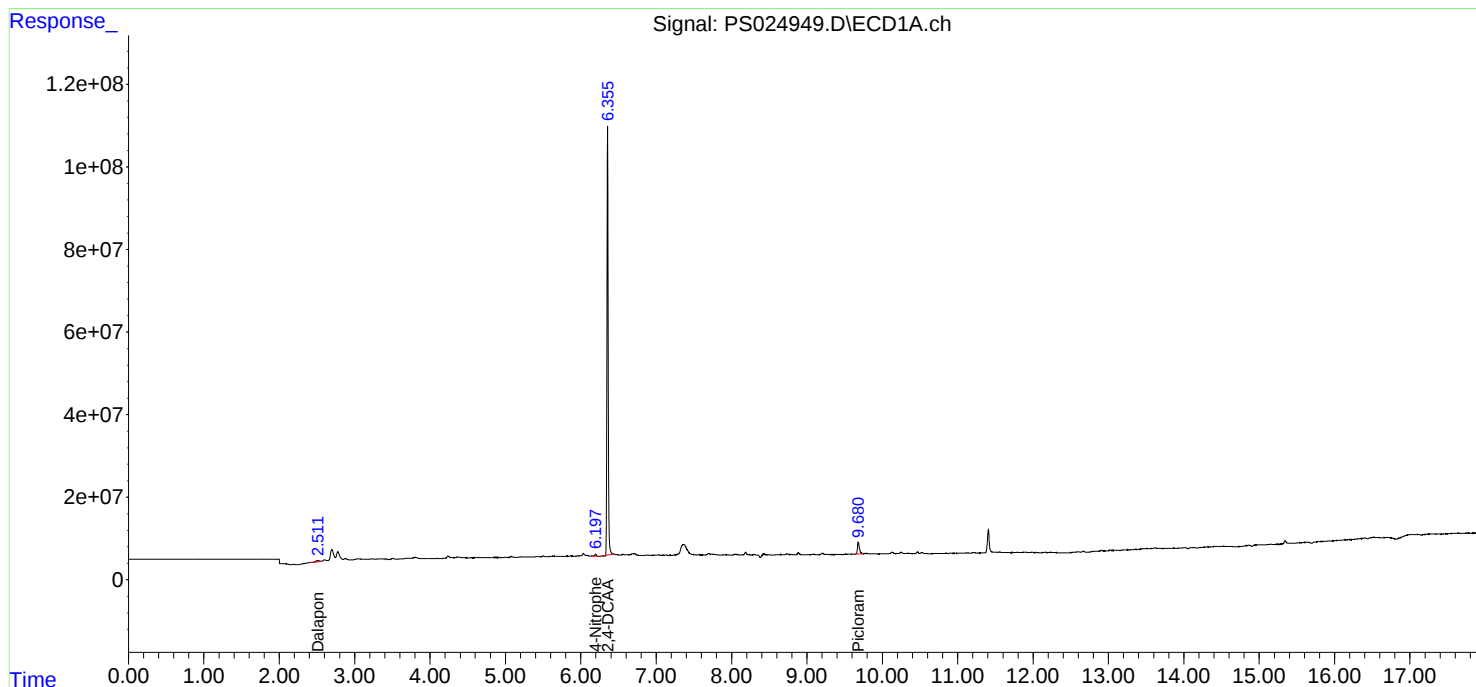


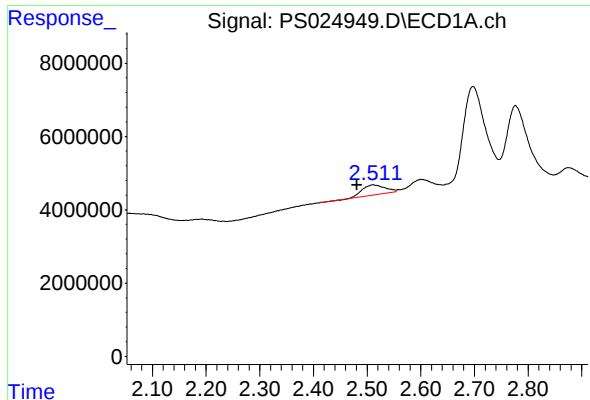

#1 Dalapon


R.T.: 2.511 min
Delta R.T.: 0.030 min
Response: 7945528
Conc: 3.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

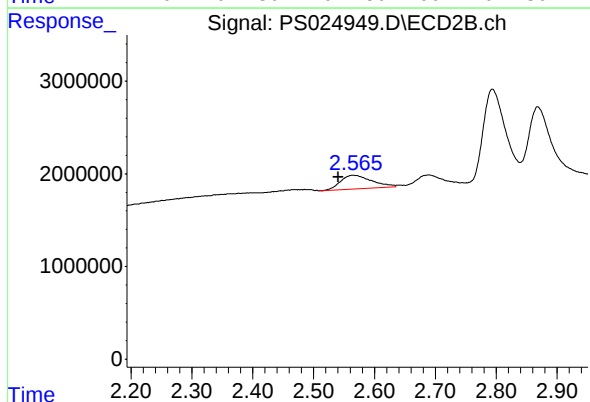


#1 Dalapon

R.T.: 2.565 min
Delta R.T.: 0.025 min
Response: 5246015
Conc: 4.98 ng/ml

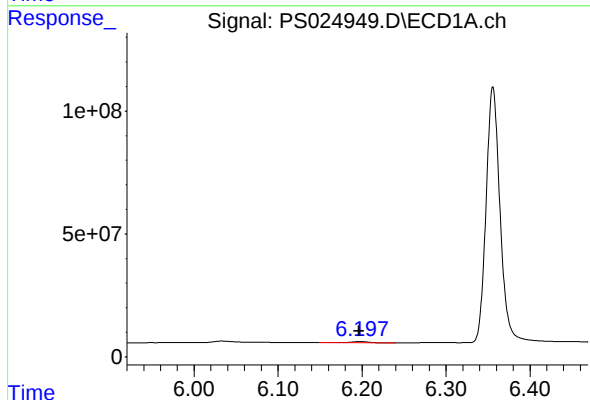


#3 4-Nitrophenol

R.T.: 6.198 min
Delta R.T.: 0.002 min
Response: 7106056
Conc: 5.48 ng/ml

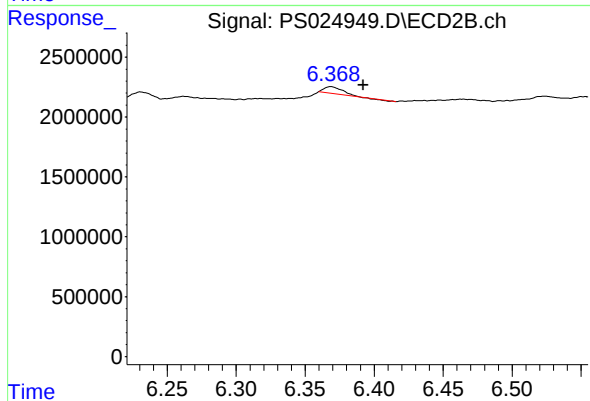

#3 4-Nitrophenol


R.T.: 6.369 min
Delta R.T.: -0.023 min
Response: 523661
Conc: 1.19 ng/ml

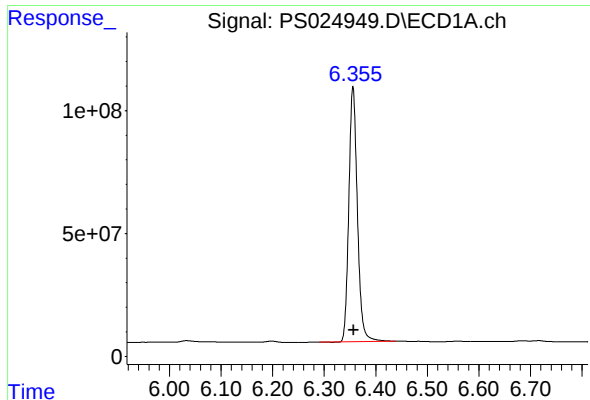

#4 2,4-DCAA


R.T.: 6.356 min
Delta R.T.: -0.001 min
Response: 1195854172
Conc: 585.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

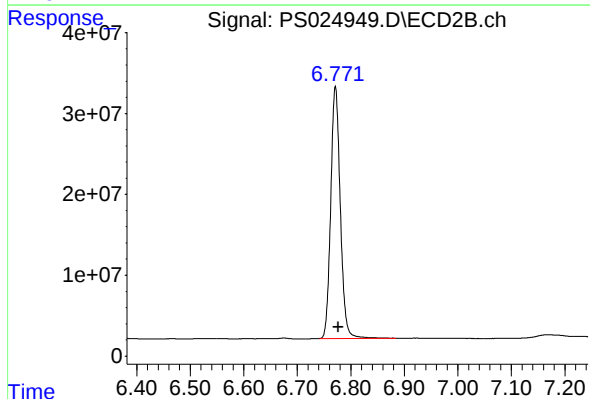


#4 2,4-DCAA

R.T.: 6.771 min
Delta R.T.: -0.005 min
Response: 386537578
Conc: 572.99 ng/ml

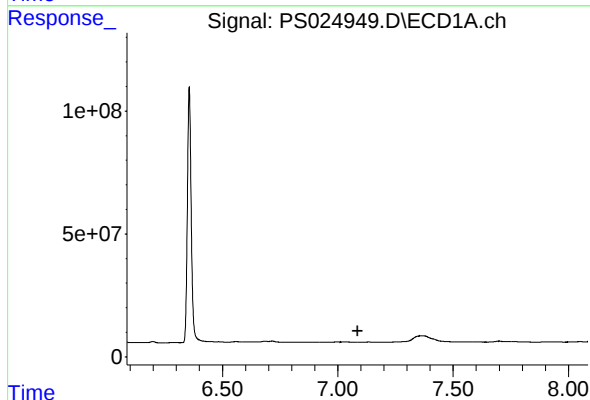


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.085 min
Response: 0
Conc: N.D.

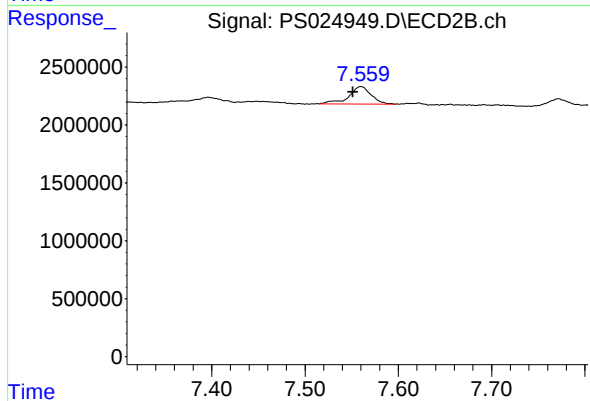

#8 DICHLORPROP


R.T.: 7.560 min
Delta R.T.: 0.009 min
Response: 2515428
Conc: 3.44 ng/ml

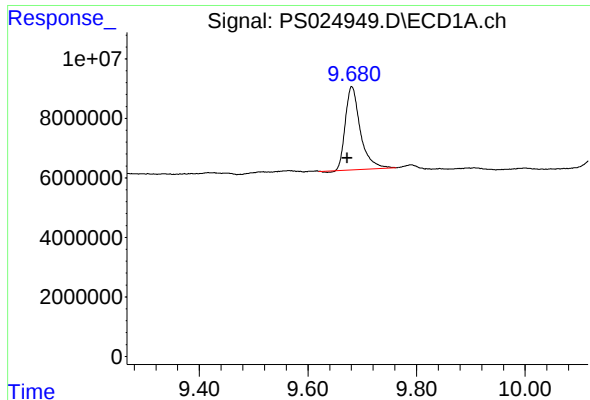

#15 Picloram


R.T.: 9.681 min
Delta R.T.: 0.008 min
Response: 53389967
Conc: 3.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

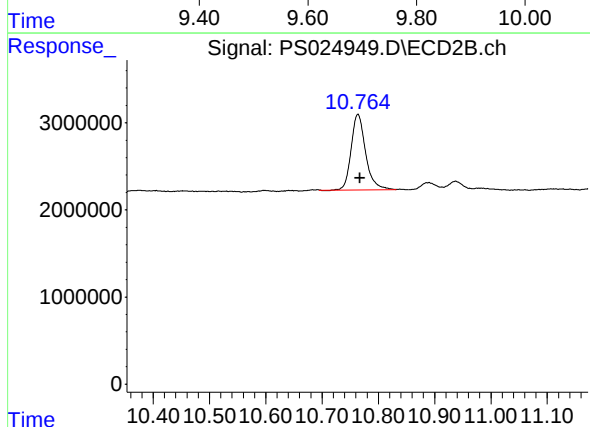


#15 Picloram

R.T.: 10.764 min
Delta R.T.: -0.004 min
Response: 15438845
Conc: 2.54 ng/ml

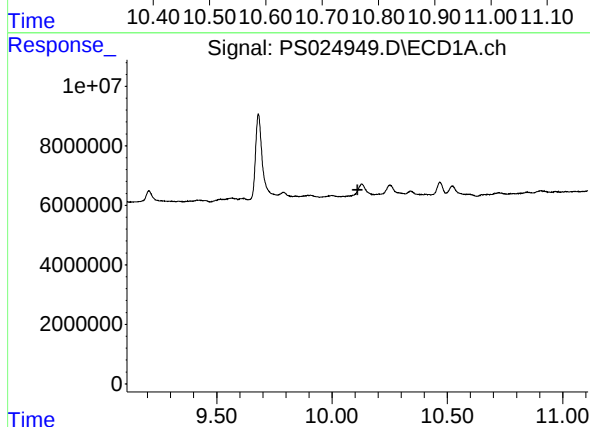

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.111 min
Response: 0
Conc: N.D.

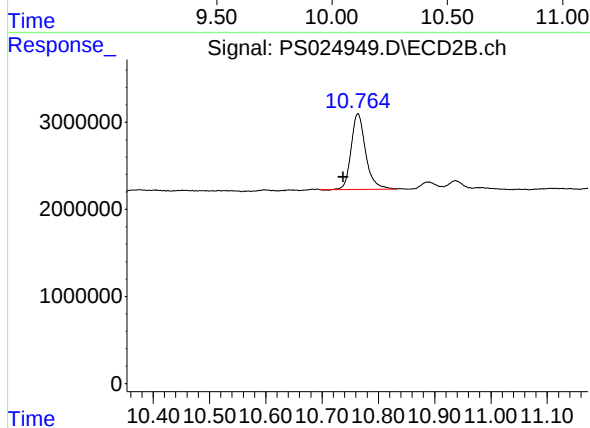

#16 DCPA

R.T.: 10.764 min
Delta R.T.: 0.026 min
Response: 15438845
Conc: 3.07 ng/ml