

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112724\
 Data File : PS028656.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2024 09:03
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 09:44:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 26 14:44:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

1) T	Dalapon	2.671f	0.000	17985033	0	6.198	N.D.	#
2) T	3,5-DICHL...	6.383	0.000	1714791	0	<MDL	N.D.	#
3) T	4-Nitroph...	7.012	0.000	2429067	0	1.413	N.D.	#
5) T	DICAMBA	0.000	7.921	0	2749884	N.D.	<MDL	
6) T	MCP	0.000	8.029	0	2423047	N.D.	<MDL	
8) T	DICHLORPROP	8.090f	8.689f	2857498	4003569	<MDL	2.504	#
11) T	2,4,5-TP ...	9.226	0.000	303032	0	<MDL	N.D.	#
12) T	2,4,5-T	9.527	10.287	2226732	4247636	<MDL	<MDL	#
13) T	2,4-DB	10.114	0.000	501377	0	<MDL	N.D.	#
14) T	DINOSEB	11.297	0.000	1239808	0	<MDL	N.D.	#
15) T	Picloram	11.124	12.333	34085018	8292469	1.146	<MDL	#
16) T	DCPA	11.587	0.000	3060577	0	<MDL	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112724\
Data File : PS028656.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2024 09:03
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 09:44:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
Quant Title : 8080.M
QLast Update : Tue Nov 26 14:44:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

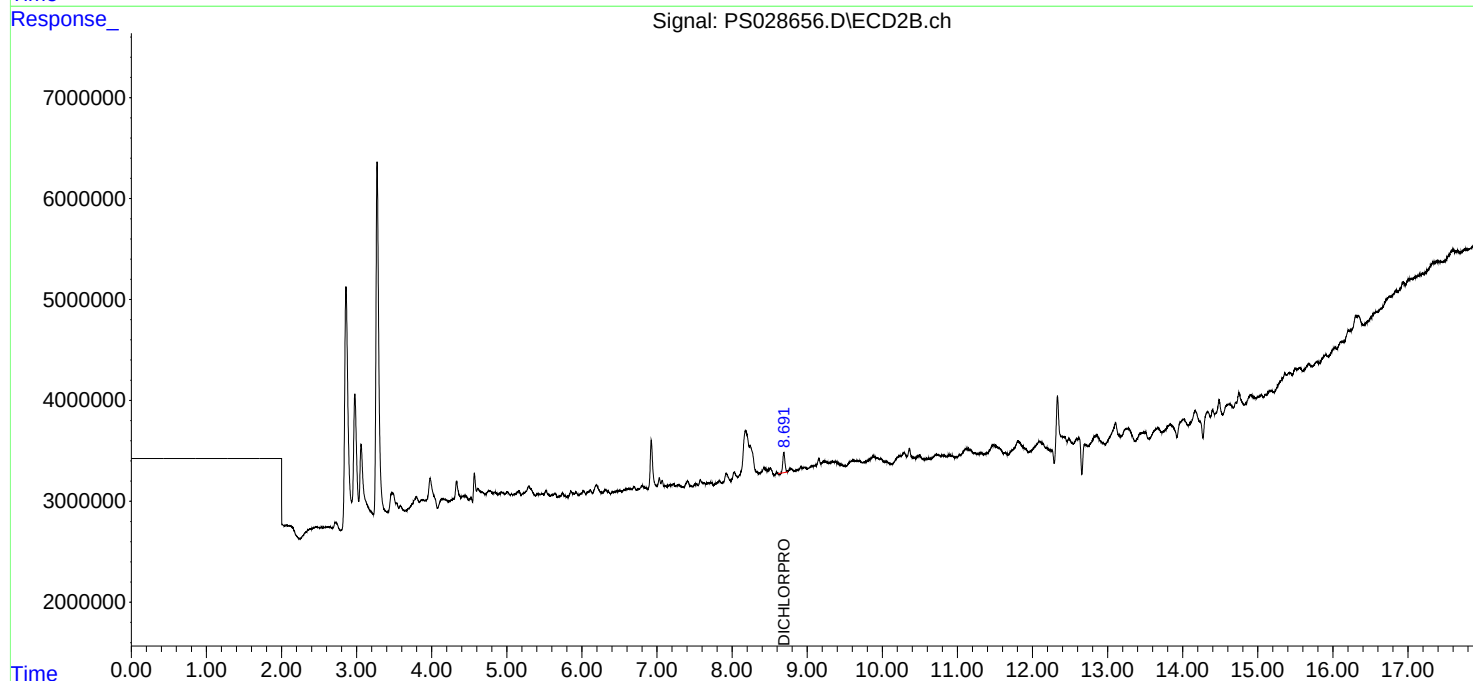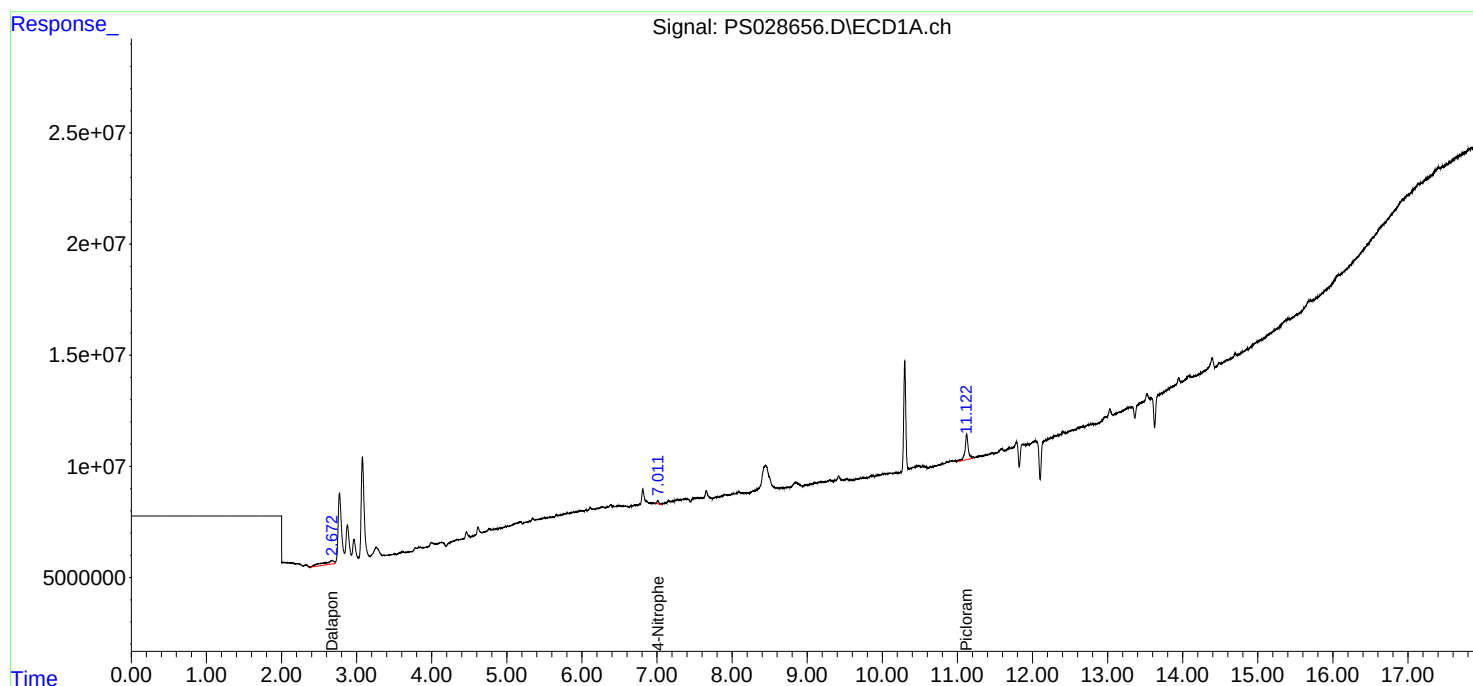


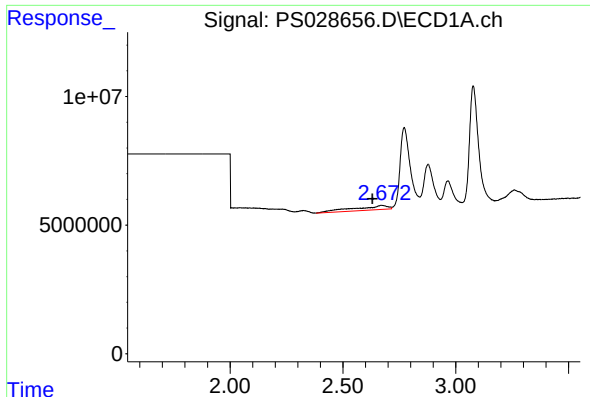

#1 Dalapon


R.T.: 2.671 min
Delta R.T.: 0.041 min
Response: 17985033
Conc: 6.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

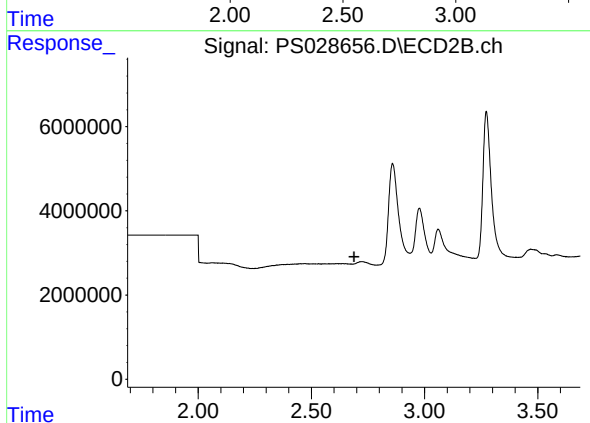


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.688 min
Response: 0
Conc: N.D.

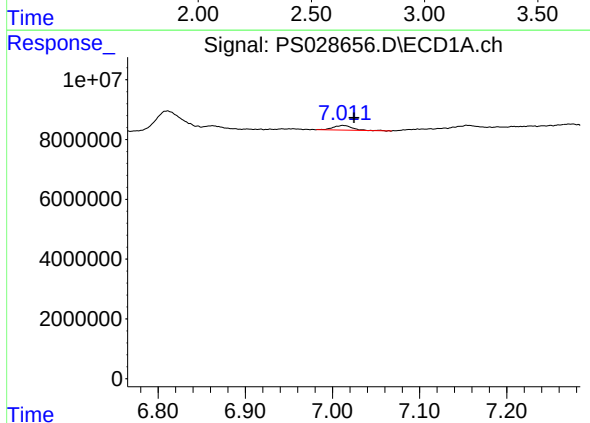


#3 4-Nitrophenol

R.T.: 7.012 min
Delta R.T.: -0.012 min
Response: 2429067
Conc: 1.41 ng/ml

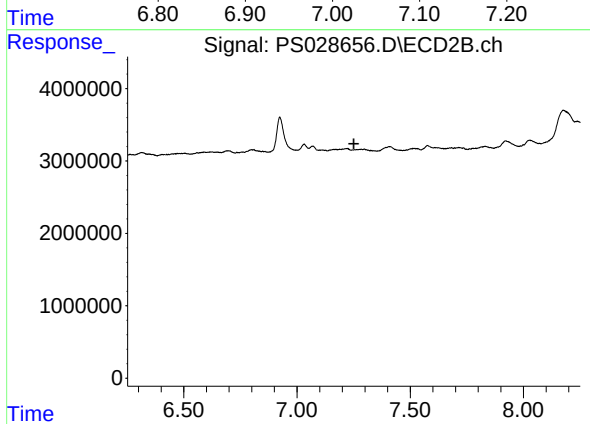

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.251 min
Response: 0
Conc: N.D.

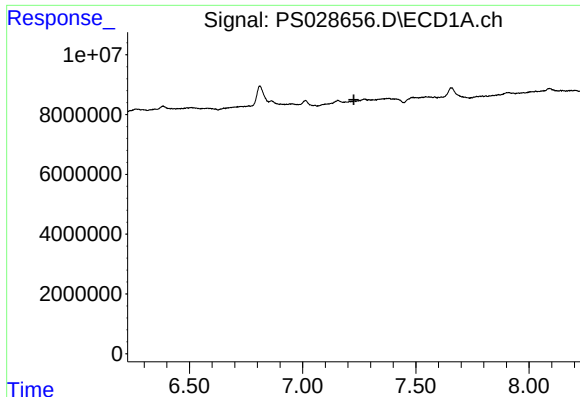

#4 2,4-DCAA


R.T.: 7.273 min
Delta R.T.: 0.047 min
Response: -1424487
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

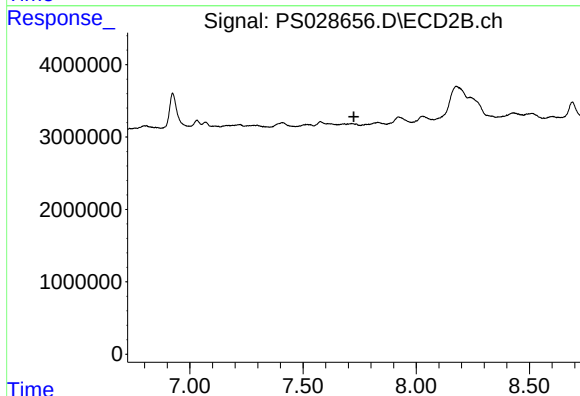


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.725 min
Response: 0
Conc: N.D.

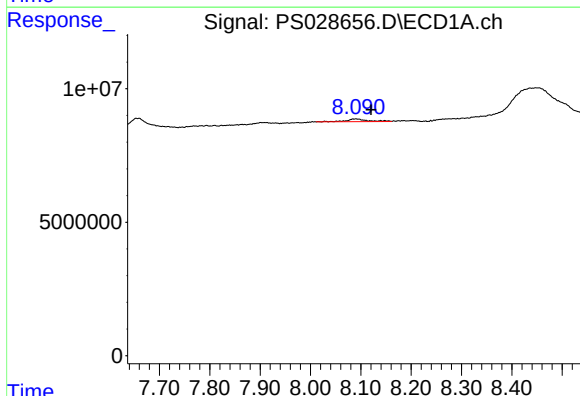


#8 DICHLORPROP

R.T.: 8.090 min
Delta R.T.: -0.031 min
Response: 2857498
Conc: N.D.

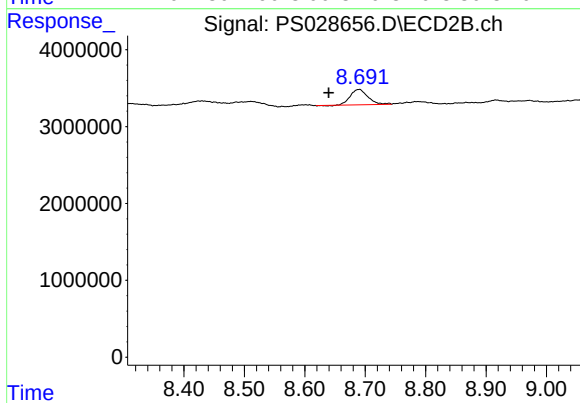

#8 DICHLORPROP


R.T.: 8.689 min
Delta R.T.: 0.050 min
Response: 4003569
Conc: 2.50 ng/ml

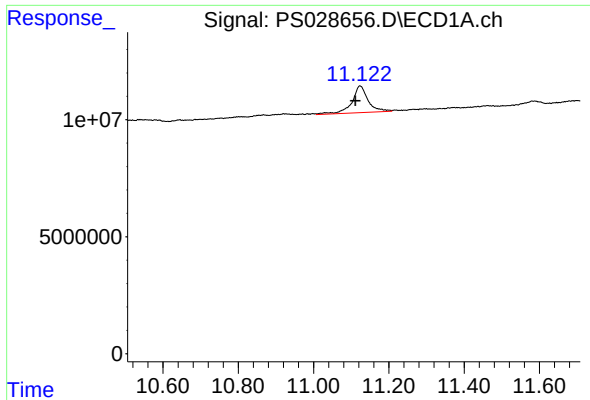

#15 Picloram

R.T.: 11.124 min
Delta R.T.: 0.012 min
Response: 34085018
Conc: 1.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

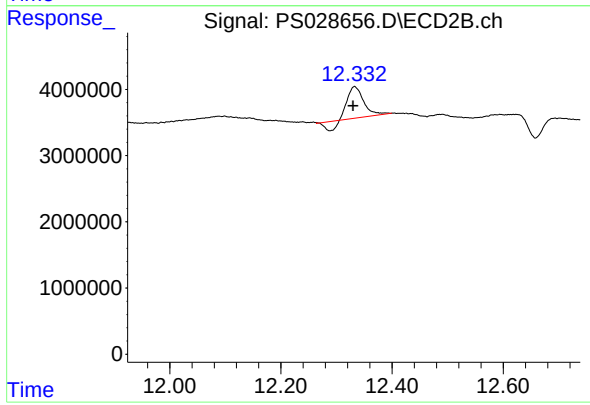

#15 Picloram

R.T.: 12.333 min
Delta R.T.: 0.003 min
Response: 8292469
Conc: N.D.