

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112724\
Data File : PS028662.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2024 17:59
Operator : AR\AJ
Sample : P5000-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
MH-733

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/02/2024
Supervised By :Ankita Jodhani 12/02/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 10:18:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
Quant Title : 8080.M
QLast Update : Tue Nov 26 14:44:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S	2,4-DCAA	7.228	7.724	746.3E6	329.8E6	278.220m	244.861
------	----------	-------	-------	---------	---------	----------	---------

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112724\
Data File : PS028662.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2024 17:59
Operator : AR\AJ
Sample : P5000-05
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
MH-733


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/02/2024
Supervised By :Ankita Jodhani 12/02/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 10:18:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
Quant Title : 8080.M
QLast Update : Tue Nov 26 14:44:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

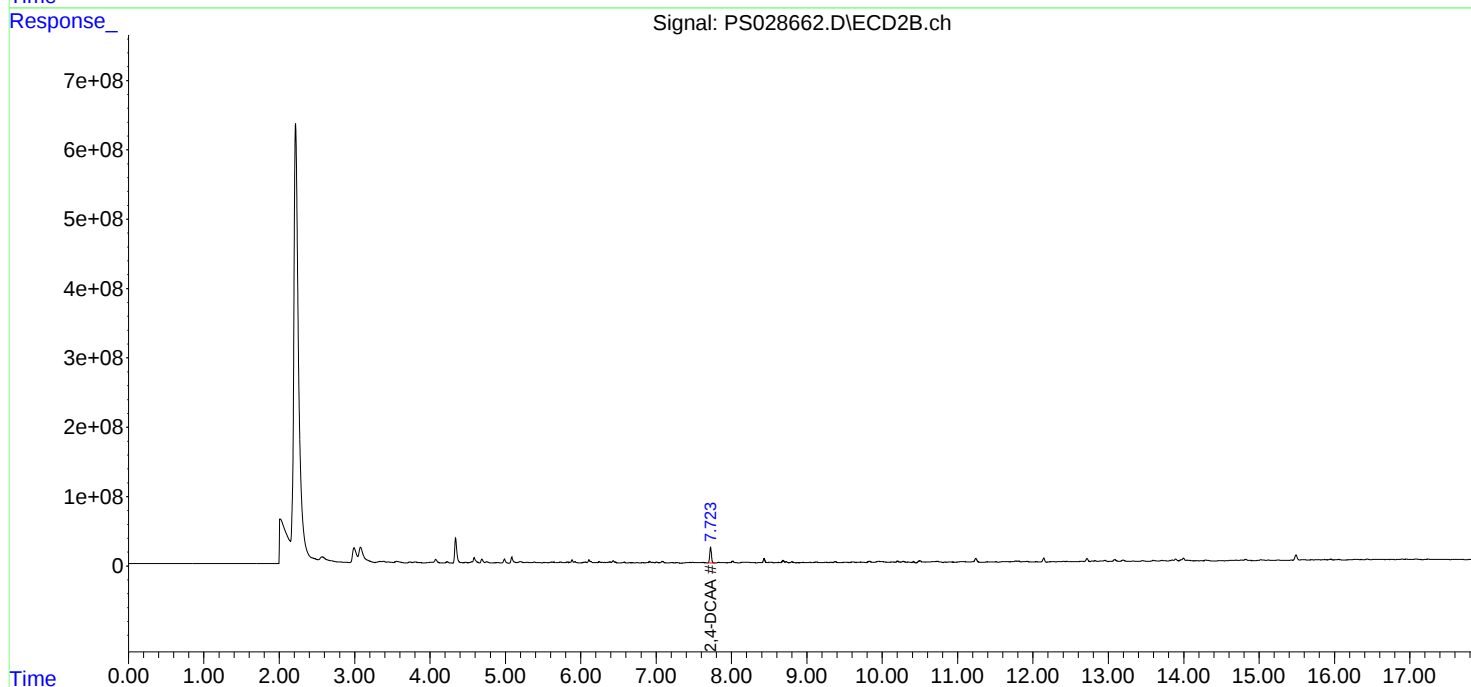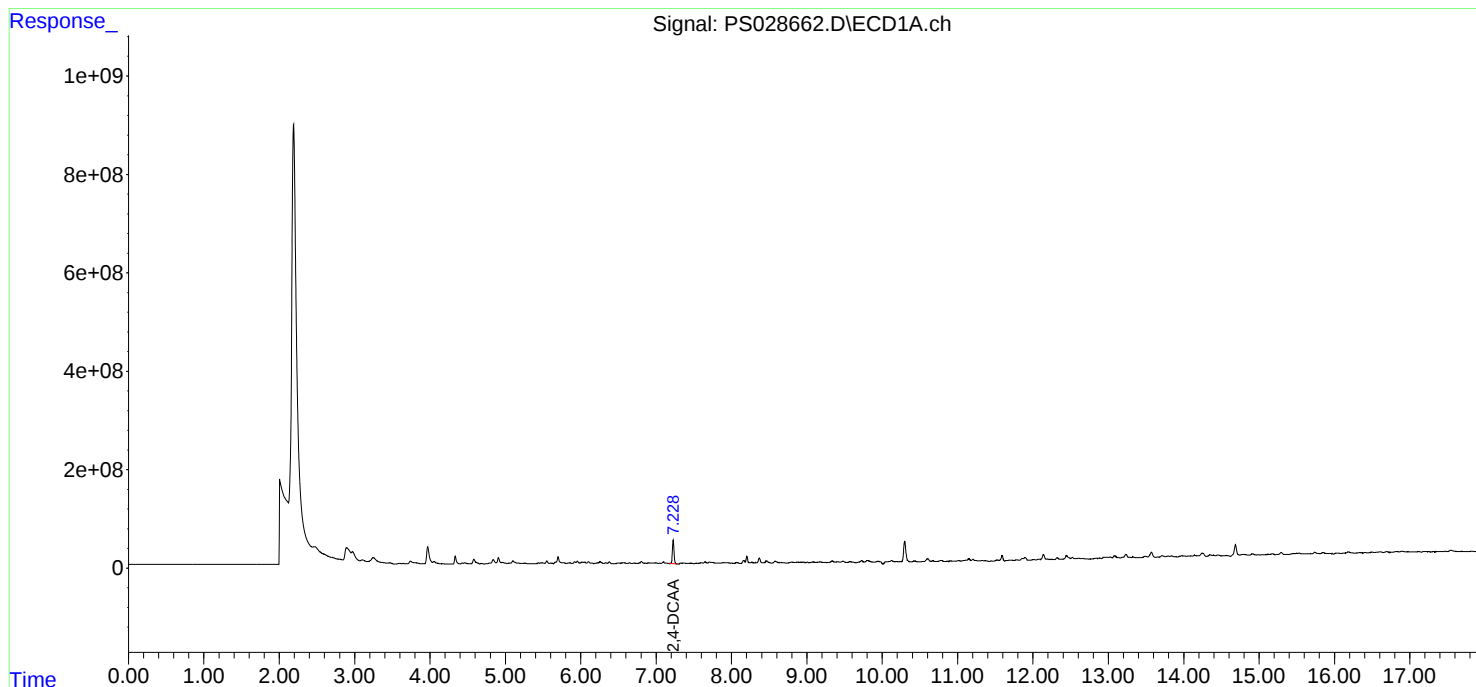

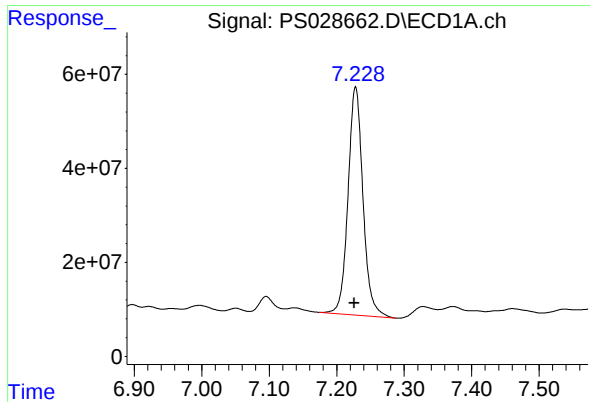


#4 2,4-DCAA

R.T.: 7.228 min
Delta R.T.: 0.001 min
Response: 746280299
Conc: 278.22 ng/ml

Instrument :
ECD_S
ClientSampleId :
MH-733

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/02/2024
Supervised By :Ankita Jodhani 12/02/2024

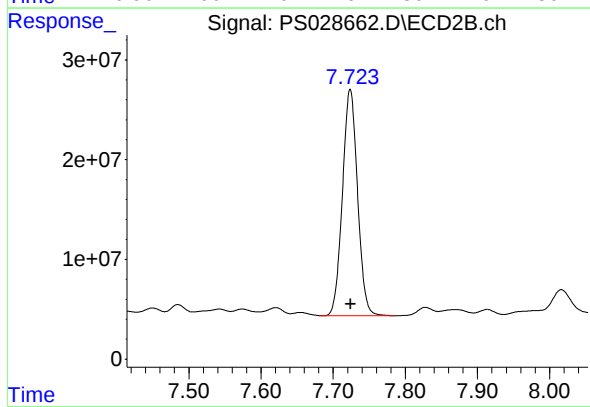

#4 2,4-DCAA

R.T.: 7.724 min
Delta R.T.: 0.000 min
Response: 329834603
Conc: 244.86 ng/ml