

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112725\
 Data File : PS032547.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2025 01:21
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 28 20:20:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	7.287	7.631	1570.7E6	1964.5E6	346.645	538.891	#
Target Compounds								
2) T	3,5-DICHL...	6.449	0.000	3394216	0	<MDL	N.D.	#
3) T	4-Nitroph...	7.129f	0.000	229951	0	<MDL	N.D.	#
6) T	MCP	7.657	0.000	270207	0	<MDL	N.D.	#
7) T	MCPA	7.798	8.104f	170783	2301207	<MDL	<MDL	#
8) T	DICHLORPROP	8.142f	0.000	1690138	0	<MDL	N.D.	#
10) T	Pentachlo...	8.715	0.000	4425577	0	<MDL	N.D.	#
11) T	2,4,5-TP ...	9.278	0.000	3803524	0	<MDL	N.D.	#
12) T	2,4,5-T	9.585	10.138f	579973	1731071	<MDL	<MDL	#
13) T	2,4-DB	10.153	0.000	311411	0	<MDL	N.D.	#
14) T	DINOSEB	11.337	0.000	4151140	0	<MDL	N.D.	#
15) T	Picloram	11.172	12.205	1169872	7750211	<MDL	<MDL	#
16) T	DCPA	11.647	0.000	4020441	0	<MDL	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112725\
Data File : PS032547.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2025 01:21
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 28 20:20:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

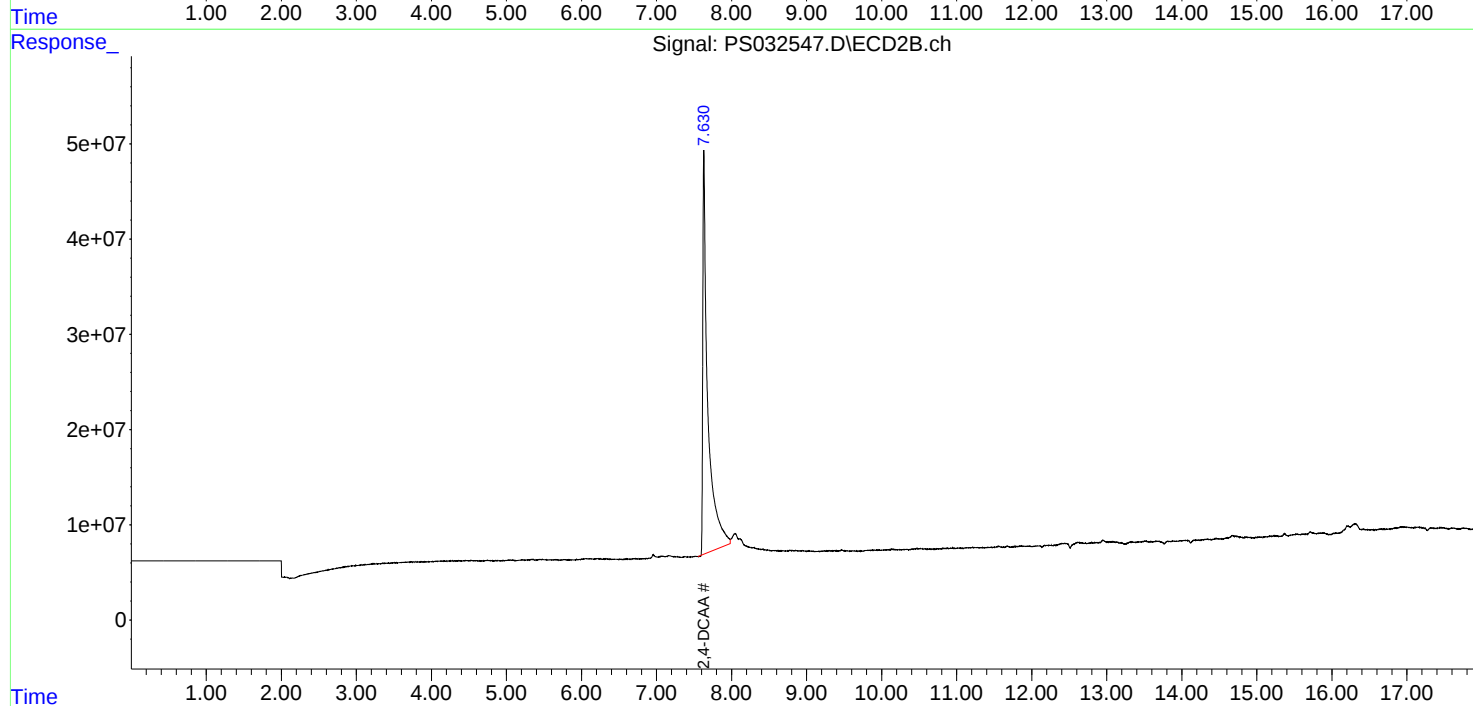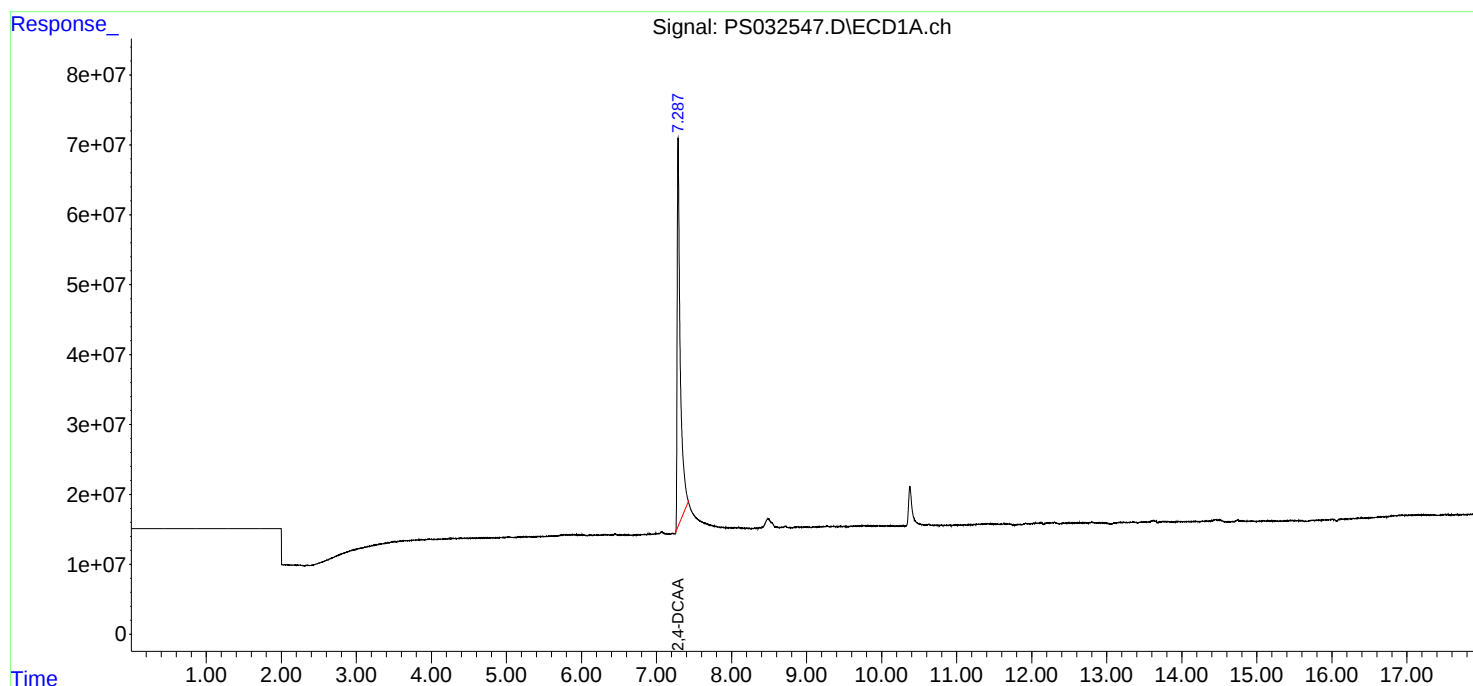


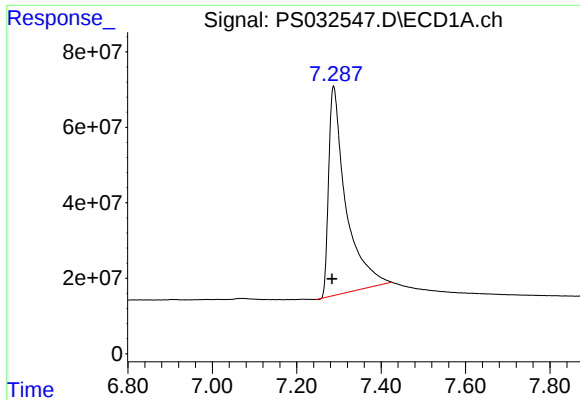

#4 2,4-DCAA

R.T.: 7.287 min
Delta R.T.: 0.004 min
Response: 1570743279
Conc: 346.64 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

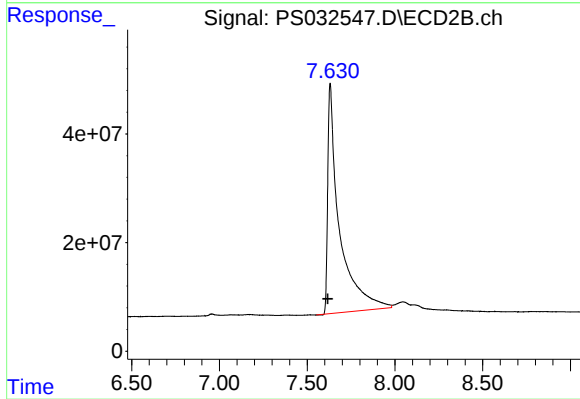

#4 2,4-DCAA

R.T.: 7.631 min
Delta R.T.: 0.014 min
Response: 1964525853
Conc: 538.89 ng/ml