

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112725\
 Data File : PS032560.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2025 07:20
 Operator : AR\AJ
 Sample : SAMPLE/No11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 28 20:25:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.274	7.613	319.2E6	308.5E6	70.453	84.631
Target Compounds							
1) T	Dalapon	0.000	2.568f	0	2668.2E6	N.D.	383.696
2) T	3,5-DICHL...	6.495f	0.000	2534380	0	<MDL	N.D. #
5) T	DICAMBA	7.454	7.842f	238922	12497140	<MDL	<MDL #
7) T	MCPA	7.803	0.000	16432675	0	1.224	N.D. #
8) T	DICHLORPROP	8.145f	0.000	11769810	0	2.646	N.D. #
9) T	2,4-D	8.396	0.000	707477	0	<MDL	N.D. #
10) T	Pentachlo...	8.692	9.354	31245347	23019371	<MDL	<MDL #
11) T	2,4,5-TP ...	9.315f	9.764	16611308	76838865	<MDL	2.861 #
12) T	2,4,5-T	9.569	10.174	26619056	101.9E6	1.117	4.296 #
13) T	2,4-DB	10.165	10.759	220.2E6	64244840	83.547	17.035 #
14) T	DINOSEB	11.358	11.112	182.4E6	21637697	8.767	1.223 #
15) T	Picloram	11.173	12.230	64491504	86119405	3.038	2.316
16) T	DCPA	11.621	12.137	15907916	10818208	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112725\
Data File : PS032560.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2025 07:20
Operator : AR\AJ
Sample : SAMPLE/No11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 28 20:25:34 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

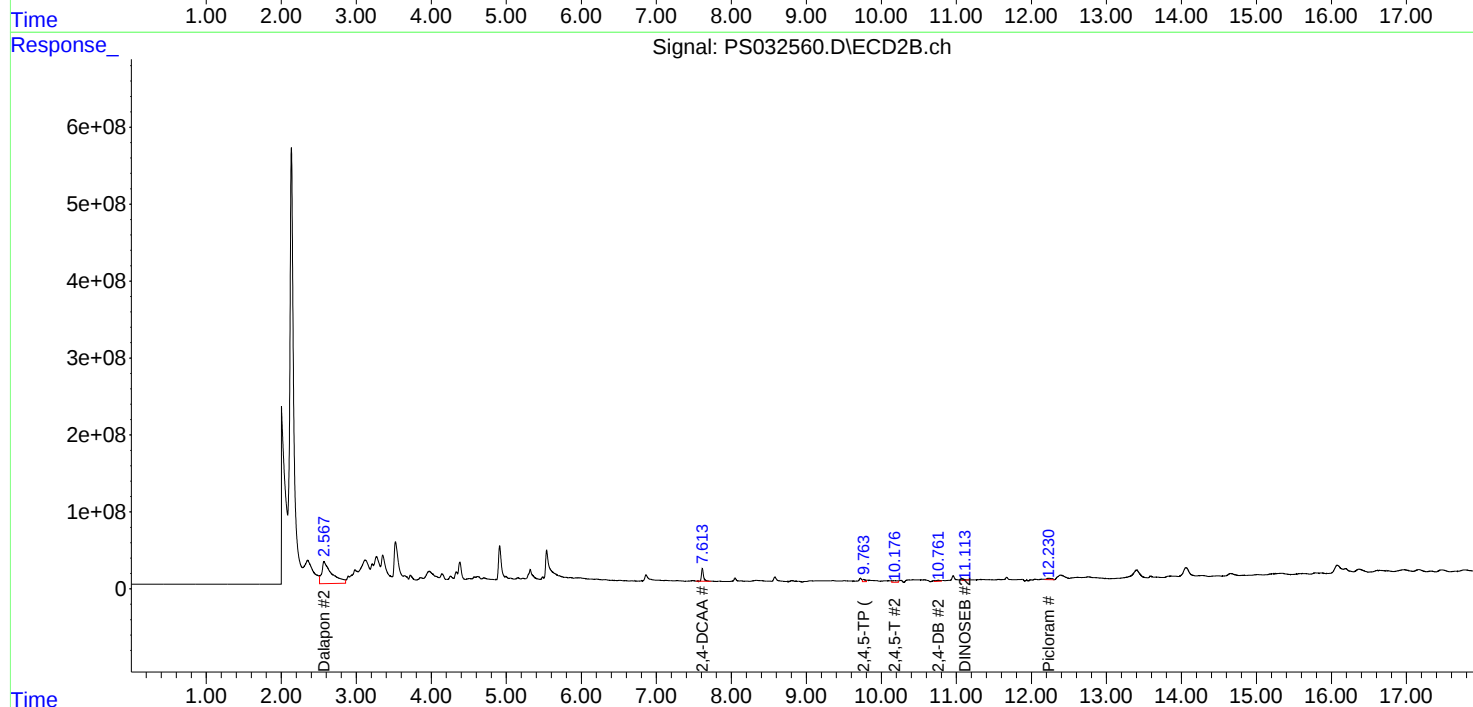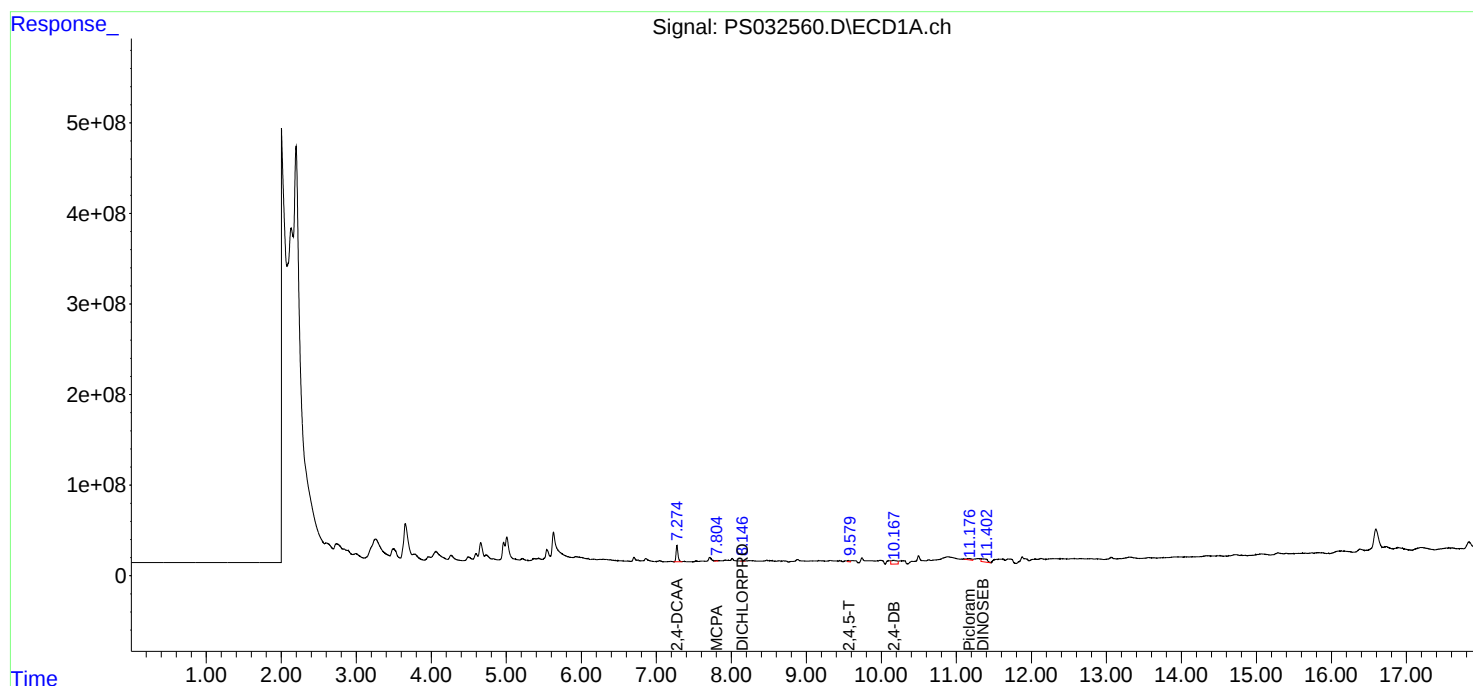


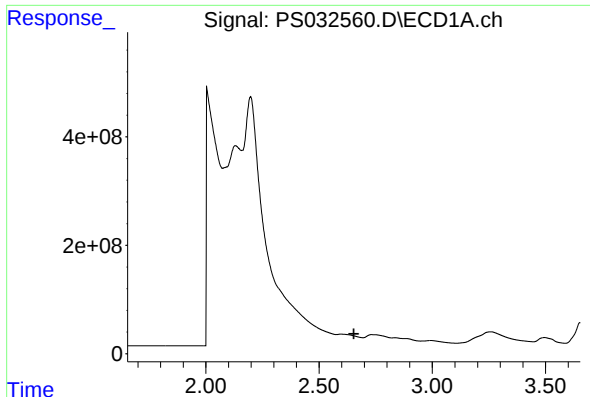

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.654 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

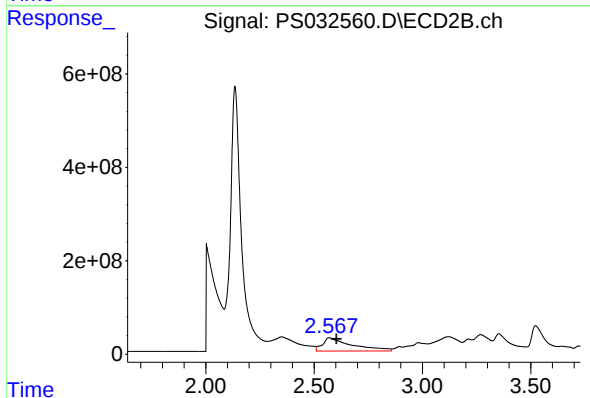


#1 Dalapon

R.T.: 2.568 min
Delta R.T.: -0.035 min
Response: 2668217869
Conc: 383.70 ng/ml

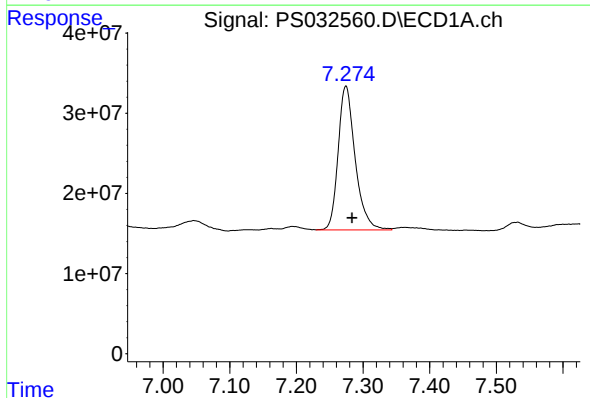


#4 2,4-DCAA

R.T.: 7.274 min
Delta R.T.: -0.009 min
Response: 319241110
Conc: 70.45 ng/ml

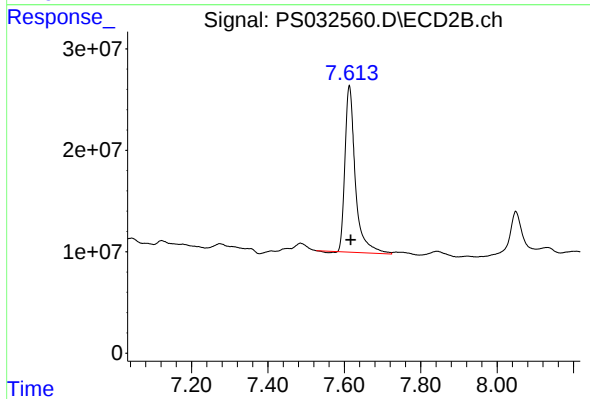

#4 2,4-DCAA


R.T.: 7.613 min
Delta R.T.: -0.004 min
Response: 308522061
Conc: 84.63 ng/ml

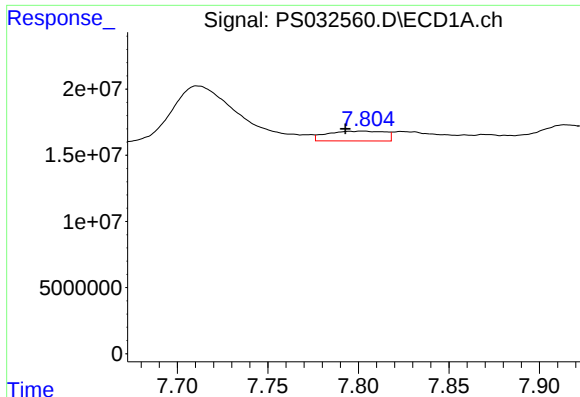

#7 MCPA


R.T.: 7.803 min
Delta R.T.: 0.010 min
Response: 16432675
Conc: 1.22 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

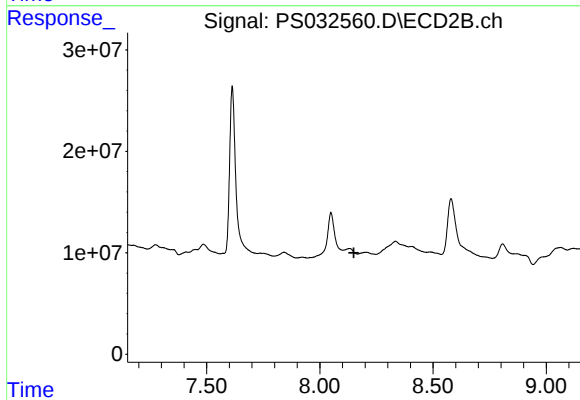


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 8.151 min
Response: 0
Conc: N.D.

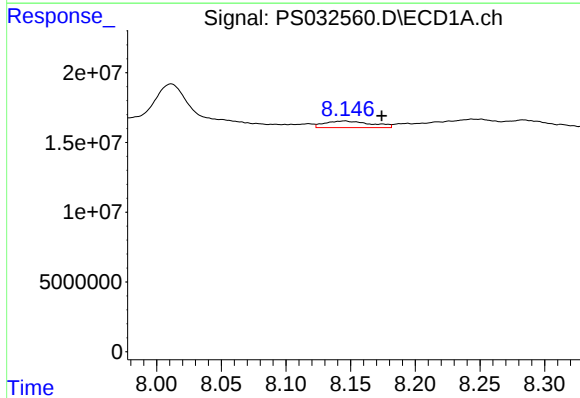


#8 DICHLORPROP

R.T.: 8.145 min
Delta R.T.: -0.029 min
Response: 11769810
Conc: 2.65 ng/ml

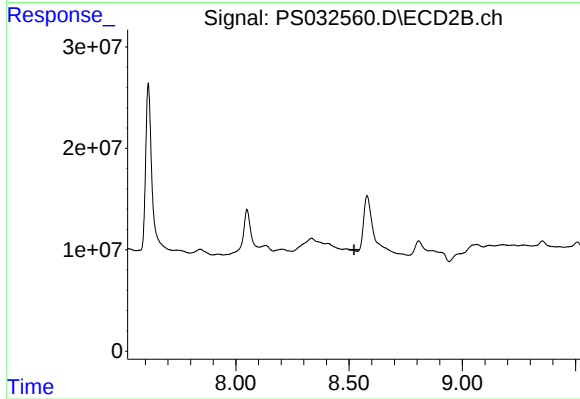

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 8.522 min
Response: 0
Conc: N.D.

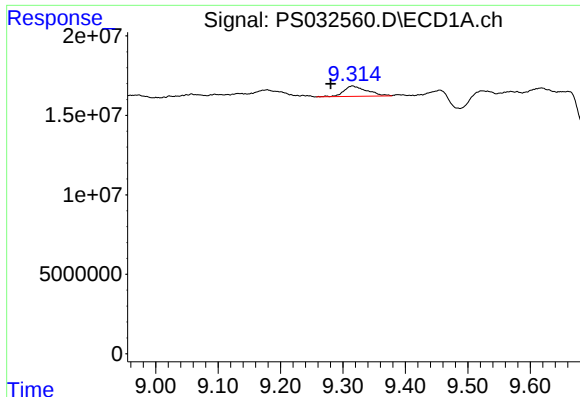

#11 2,4,5-TP (SILVEX)


R.T.: 9.315 min
Delta R.T.: 0.035 min
Response: 16611308
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

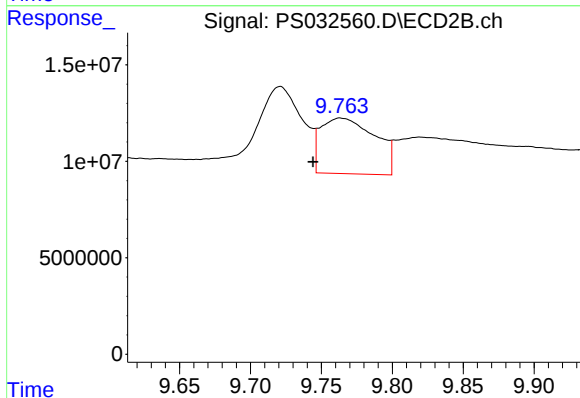


#11 2,4,5-TP (SILVEX)

R.T.: 9.764 min
Delta R.T.: 0.020 min
Response: 76838865
Conc: 2.86 ng/ml

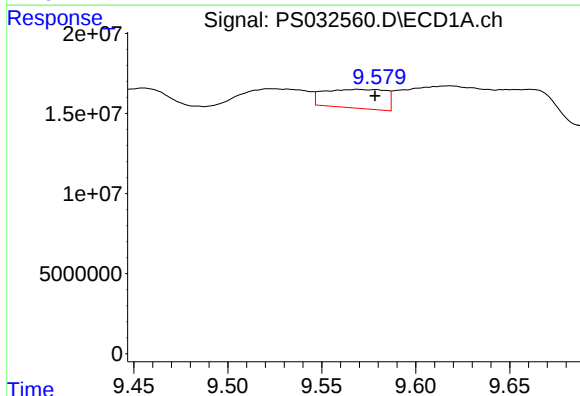


#12 2,4,5-T

R.T.: 9.569 min
Delta R.T.: -0.009 min
Response: 26619056
Conc: 1.12 ng/ml

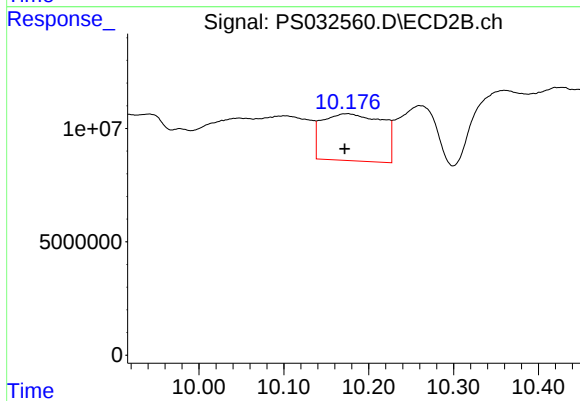

#12 2,4,5-T


R.T.: 10.174 min
Delta R.T.: 0.002 min
Response: 101890051
Conc: 4.30 ng/ml

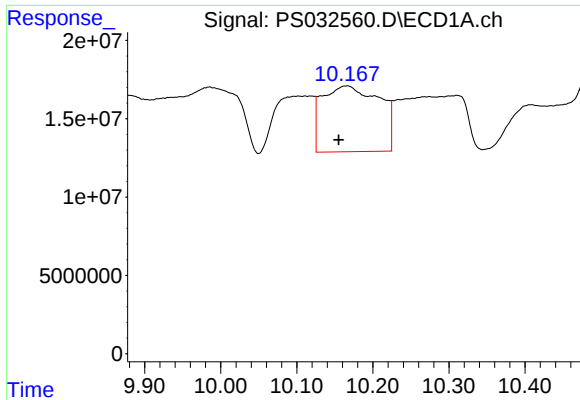

#13 2,4-DB


R.T.: 10.165 min
Delta R.T.: 0.010 min
Response: 220155828
Conc: 83.55 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

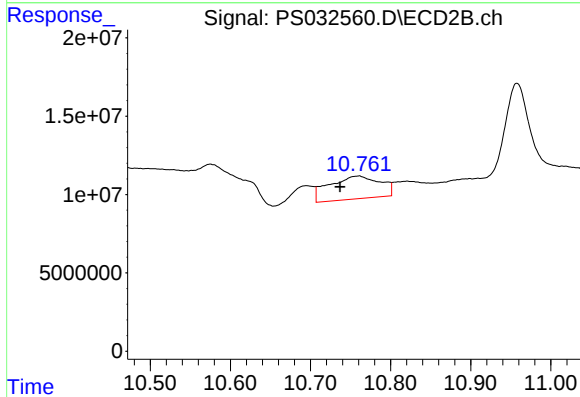


#13 2,4-DB

R.T.: 10.759 min
Delta R.T.: 0.022 min
Response: 64244840
Conc: 17.04 ng/ml

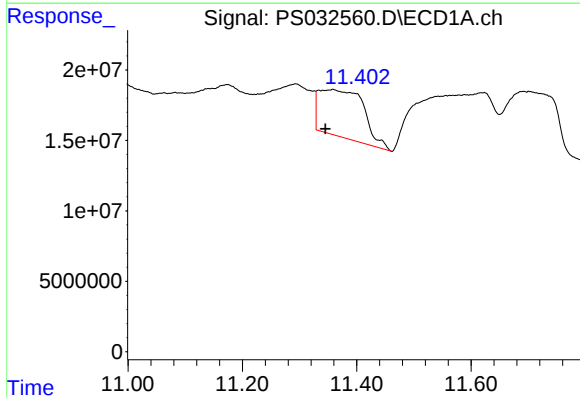


#14 DINOSEB

R.T.: 11.358 min
Delta R.T.: 0.013 min
Response: 182409883
Conc: 8.77 ng/ml

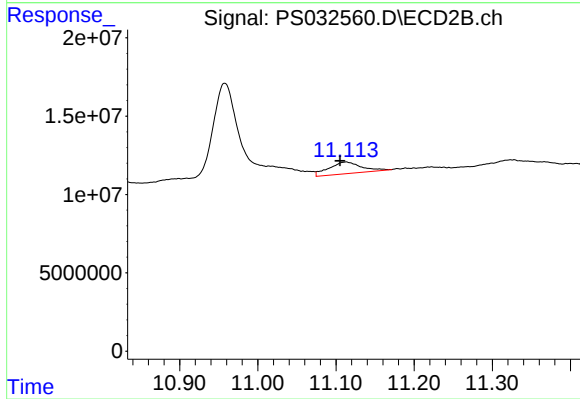

#14 DINOSEB


R.T.: 11.112 min
Delta R.T.: 0.007 min
Response: 21637697
Conc: 1.22 ng/ml

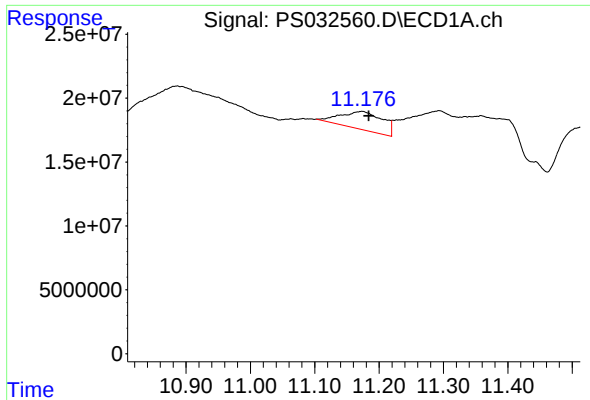

#15 Picloram

R.T.: 11.173 min
Delta R.T.: -0.011 min
Response: 64491504
Conc: 3.04 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

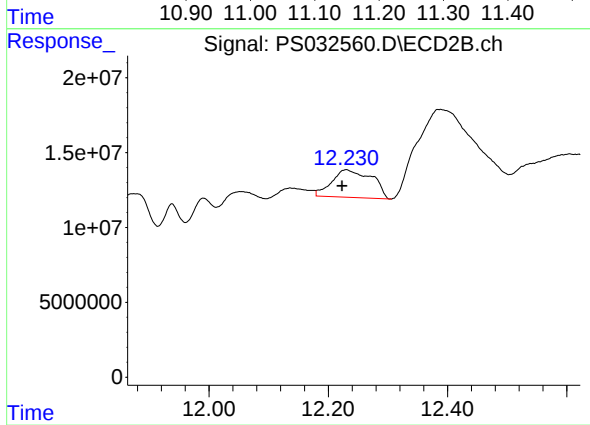

#15 Picloram

R.T.: 12.230 min
Delta R.T.: 0.007 min
Response: 86119405
Conc: 2.32 ng/ml