

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112822\
 Data File : PS021256.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Nov 2022 18:58
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 29 05:32:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111622.M
 Quant Title : 8080.M
 QLast Update : Thu Nov 17 00:46:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.408	6.842	1160.7E6	897.7E6	533.850	593.674
Target Compounds							
1) T	Dalapon	2.534	0.000	530242	0	<MDL	N.D. #
3) T	4-Nitroph...	6.247	0.000	7518695	0	5.565	N.D. #
5) T	DICAMBA	0.000	7.062f	0	8816391	N.D.	1.281
6) T	MCP	6.673f	7.062f	-178575	8816391	N.D.	1.690
7) T	MCPA	6.784f	0.000	12257227	0	1.275	N.D. #
8) T	DICHLORPROP	7.150	7.680f	105118	2782422	<MDL	1.630 #
9) T	2,4-D	7.337	7.979f	1096262	1407853	<MDL	<MDL #
10) T	Pentachlo...	7.573	0.000	1637186	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.124	8.719	2550755	412256	<MDL	<MDL #
12) T	2,4,5-T	8.394	0.000	2838872	0	<MDL	N.D. #
13) T	2,4-DB	8.861	9.541f	2591837	4833649	1.134	4.129 #
14) T	DINOSEB	9.935	9.934	1288825	1042792	<MDL	<MDL #
15) T	Picloram	9.759	10.865	11542733	20279973	<MDL	1.571 #
16) T	DCPA	10.200	10.865	746858	20279973	<MDL	1.694 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112822\
Data File : PS021256.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Nov 2022 18:58
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 29 05:32:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111622.M
Quant Title : 8080.M
QLast Update : Thu Nov 17 00:46:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

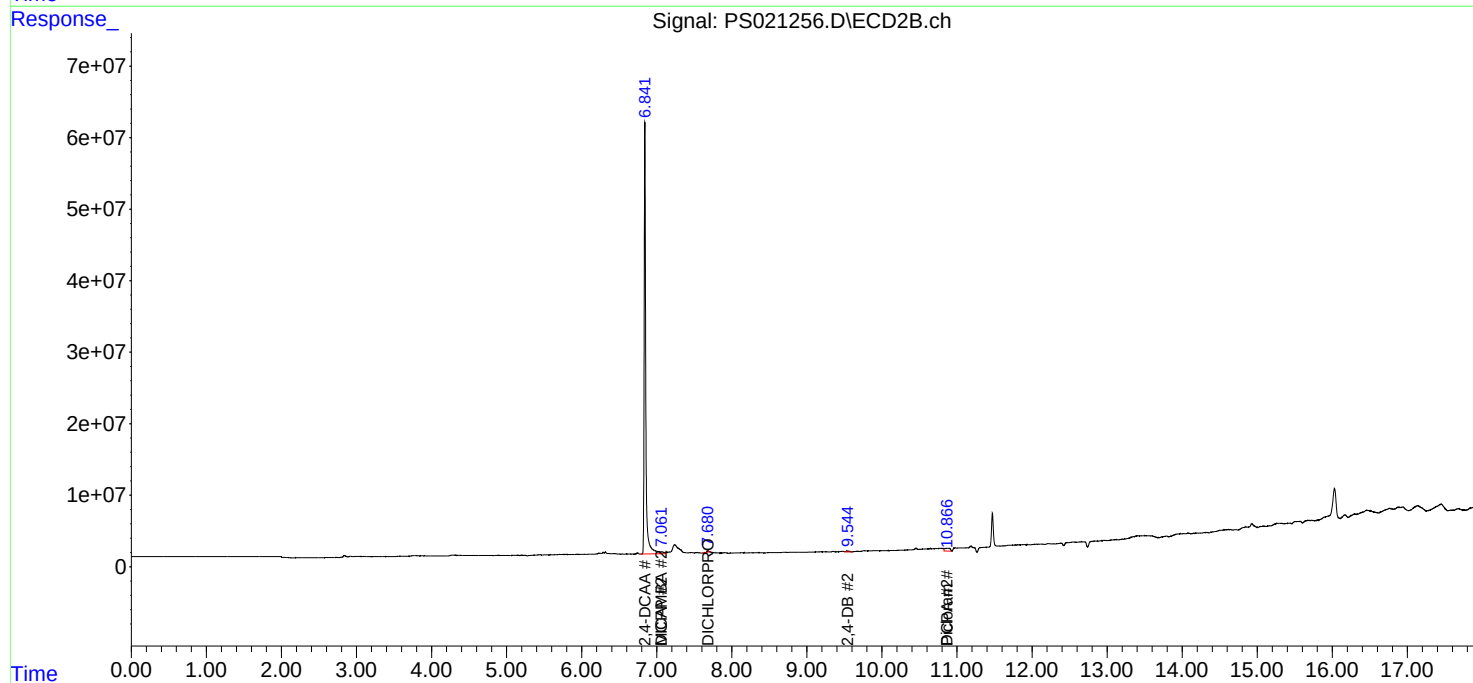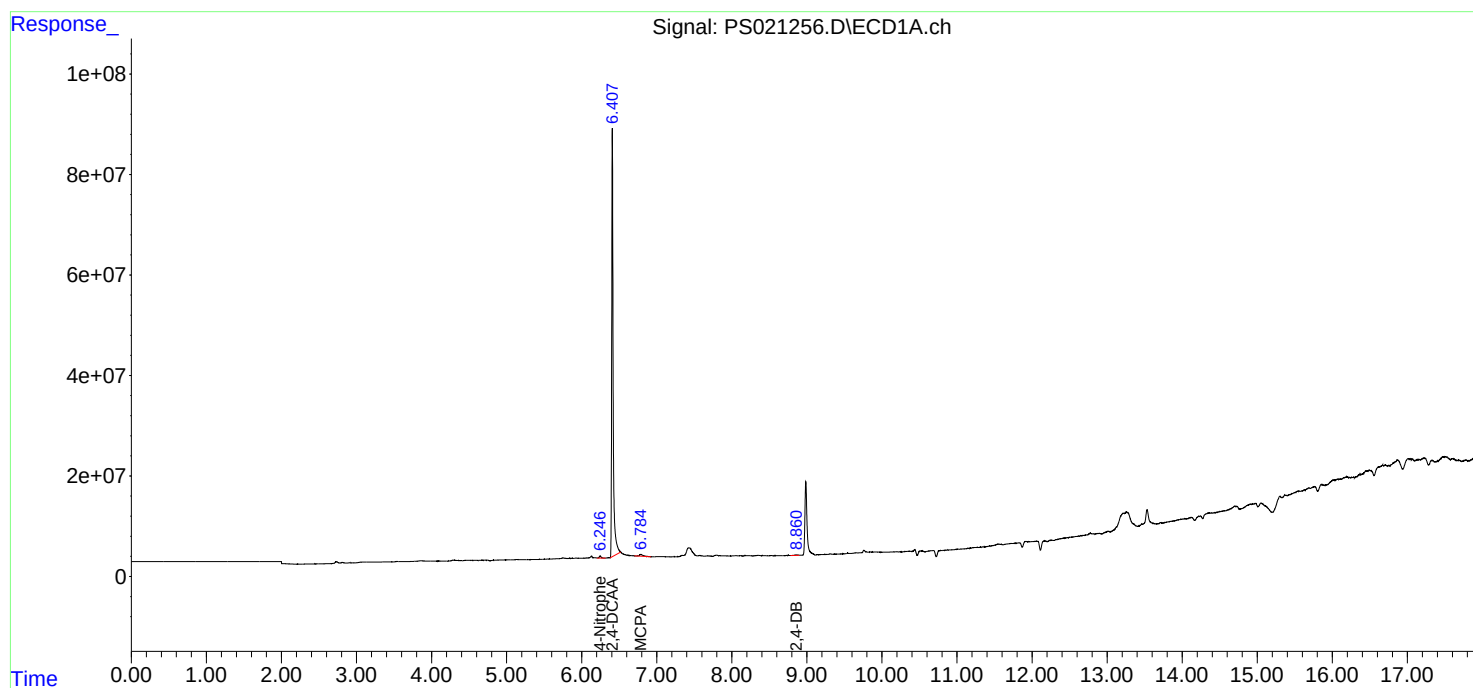


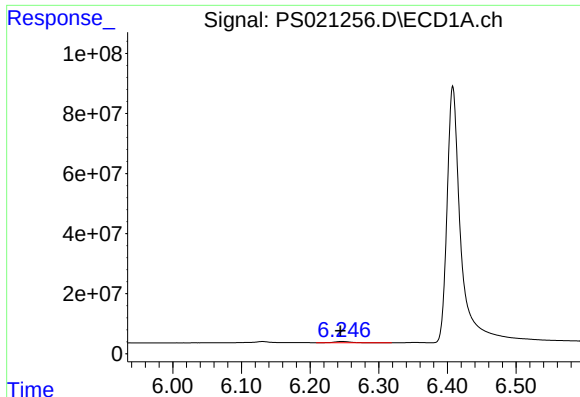

#3 4-Nitrophenol


R.T.: 6.247 min
Delta R.T.: 0.003 min
Response: 7518695
Conc: 5.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

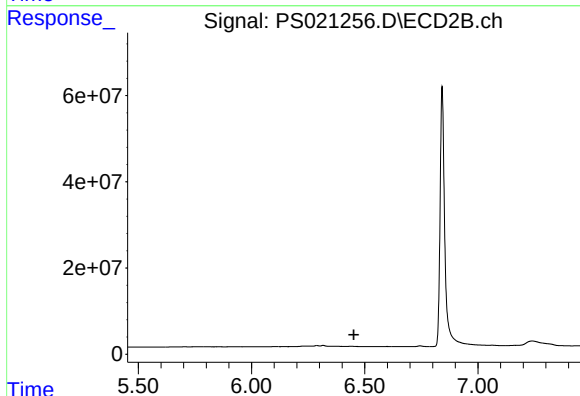


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.452 min
Response: 0
Conc: N.D.

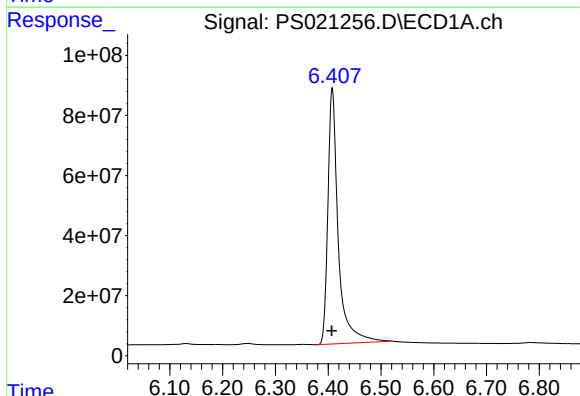


#4 2,4-DCAA

R.T.: 6.408 min
Delta R.T.: 0.001 min
Response: 1160746701
Conc: 533.85 ng/ml

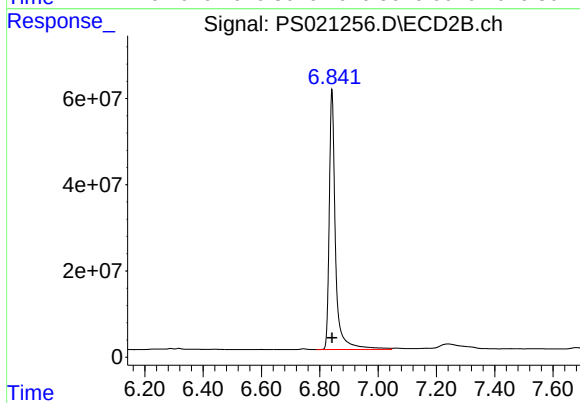

#4 2,4-DCAA


R.T.: 6.842 min
Delta R.T.: 0.000 min
Response: 897704335
Conc: 593.67 ng/ml

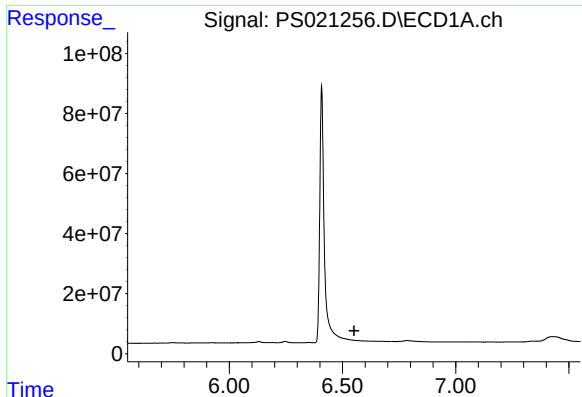

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.551 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

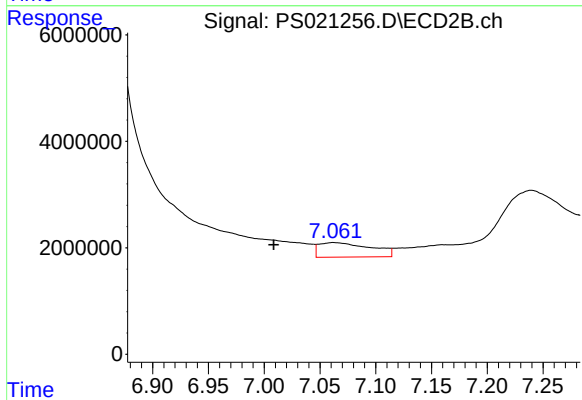


#5 DICAMBA

R.T.: 7.062 min
Delta R.T.: 0.054 min
Response: 8816391
Conc: 1.28 ng/ml

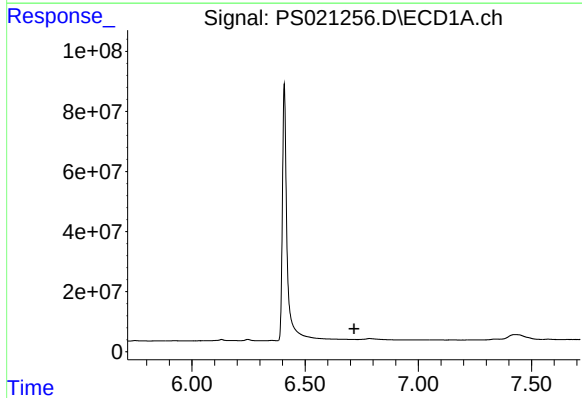


#6 MCP

R.T.: 6.673 min
Delta R.T.: -0.043 min
Response: -178575
Conc: N.D.

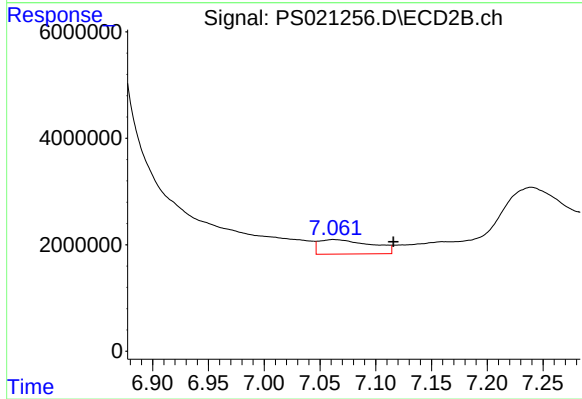

#6 MCP


R.T.: 7.062 min
Delta R.T.: -0.054 min
Response: 8816391
Conc: 1.69 ug/ml

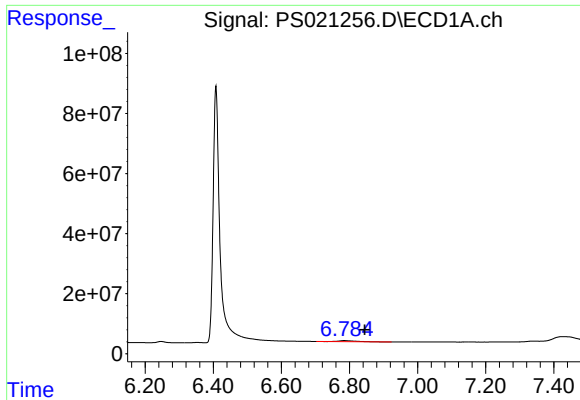

#7 MCPA


R.T.: 6.784 min
Delta R.T.: -0.061 min
Response: 12257227
Conc: 1.28 ug/ml

Instrument :
ECD_S
ClientSampleId :

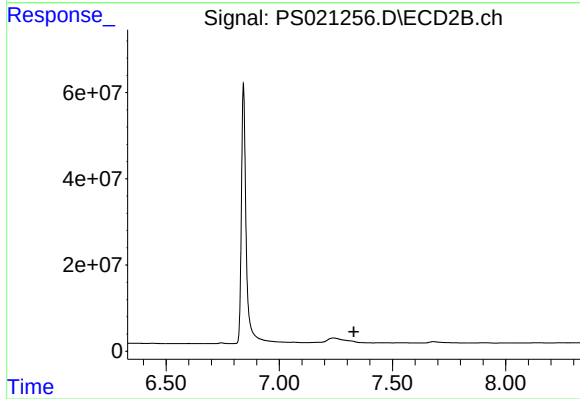


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.330 min
Response: 0
Conc: N.D.

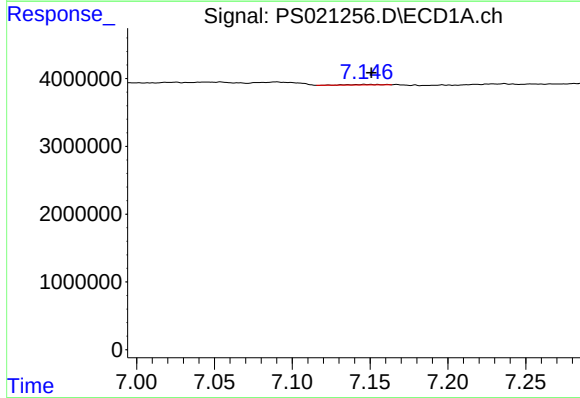


#8 DICHLORPROP

R.T.: 7.150 min
Delta R.T.: -0.001 min
Response: 105118
Conc: N.D.

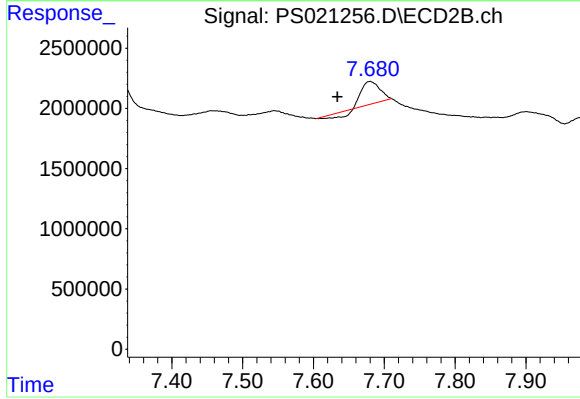

#8 DICHLORPROP


R.T.: 7.680 min
Delta R.T.: 0.046 min
Response: 2782422
Conc: 1.63 ng/ml

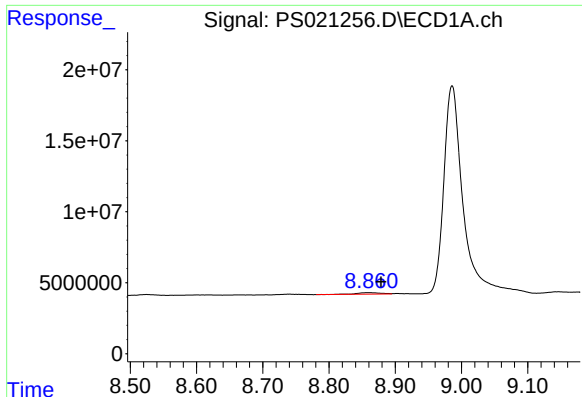

#13 2,4-DB


R.T.: 8.861 min
Delta R.T.: -0.018 min
Response: 2591837
Conc: 1.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

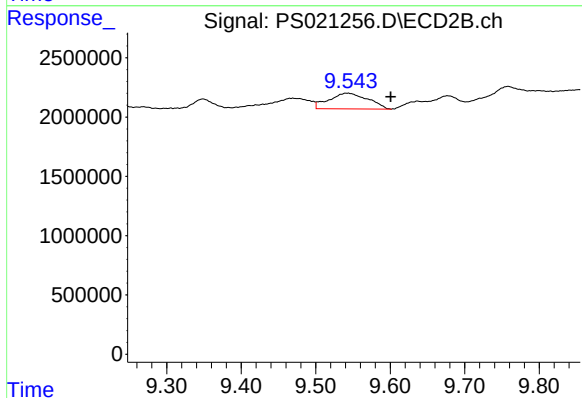


#13 2,4-DB

R.T.: 9.541 min
Delta R.T.: -0.060 min
Response: 4833649
Conc: 4.13 ng/ml

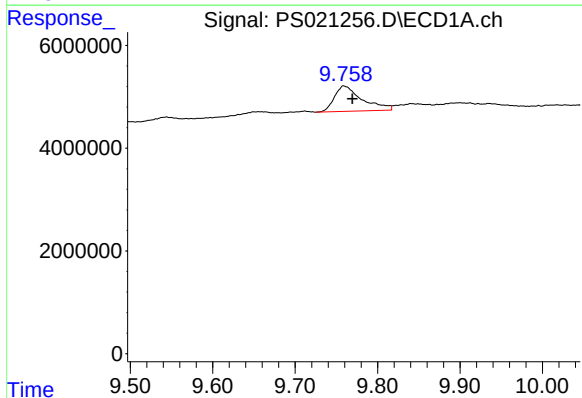


#15 Picloram

R.T.: 9.759 min
Delta R.T.: -0.010 min
Response: 11542733
Conc: N.D.

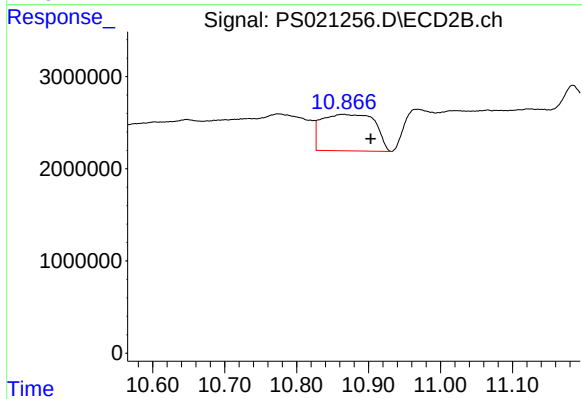

#15 Picloram


R.T.: 10.865 min
Delta R.T.: -0.038 min
Response: 20279973
Conc: 1.57 ng/ml

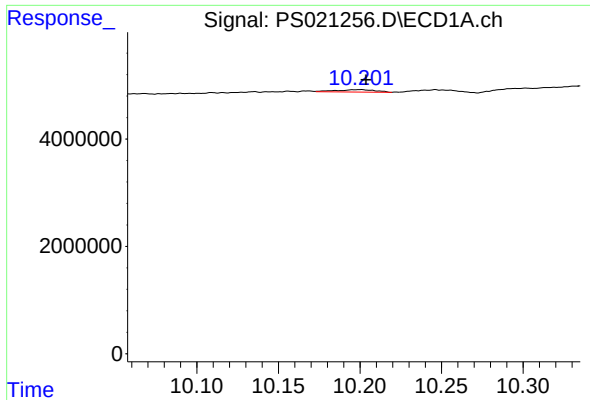

#16 DCPA

R.T.: 10.200 min
Delta R.T.: -0.003 min
Response: 746858
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

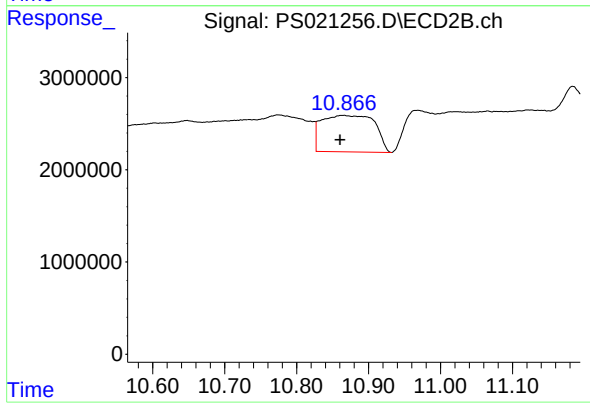

#16 DCPA

R.T.: 10.865 min
Delta R.T.: 0.005 min
Response: 20279973
Conc: 1.69 ng/ml