

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112823\
 Data File : PS024964.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Nov 2023 13:45
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 28 16:40:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.394	0.000	5568686	0	2.488	N.D. #
Target Compounds							
1) T	Dalapon	2.511	2.568	11196218	7809944	3.883	6.809 #
5) T	DICAMBA	0.000	6.930	0	475980	N.D.	<MDL
6) T	MCP	0.000	6.972f	0	1902622	N.D.	<MDL
7) T	MCPA	0.000	7.221	0	7000266	N.D.	2.128
8) T	DICHLORPROP	0.000	7.559	0	1410547	N.D.	1.793
9) T	2,4-D	0.000	7.771f	0	492151	N.D.	<MDL
12) T	2,4,5-T	0.000	9.024f	0	1345657	N.D.	<MDL
13) T	2,4-DB	0.000	9.472	0	839178	N.D.	1.516
15) T	Picloram	9.685	10.765	12931534	4567472	<MDL	<MDL #
16) T	DCPA	0.000	10.765	0	4567472	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112823\
Data File : PS024964.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Nov 2023 13:45
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 28 16:40:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

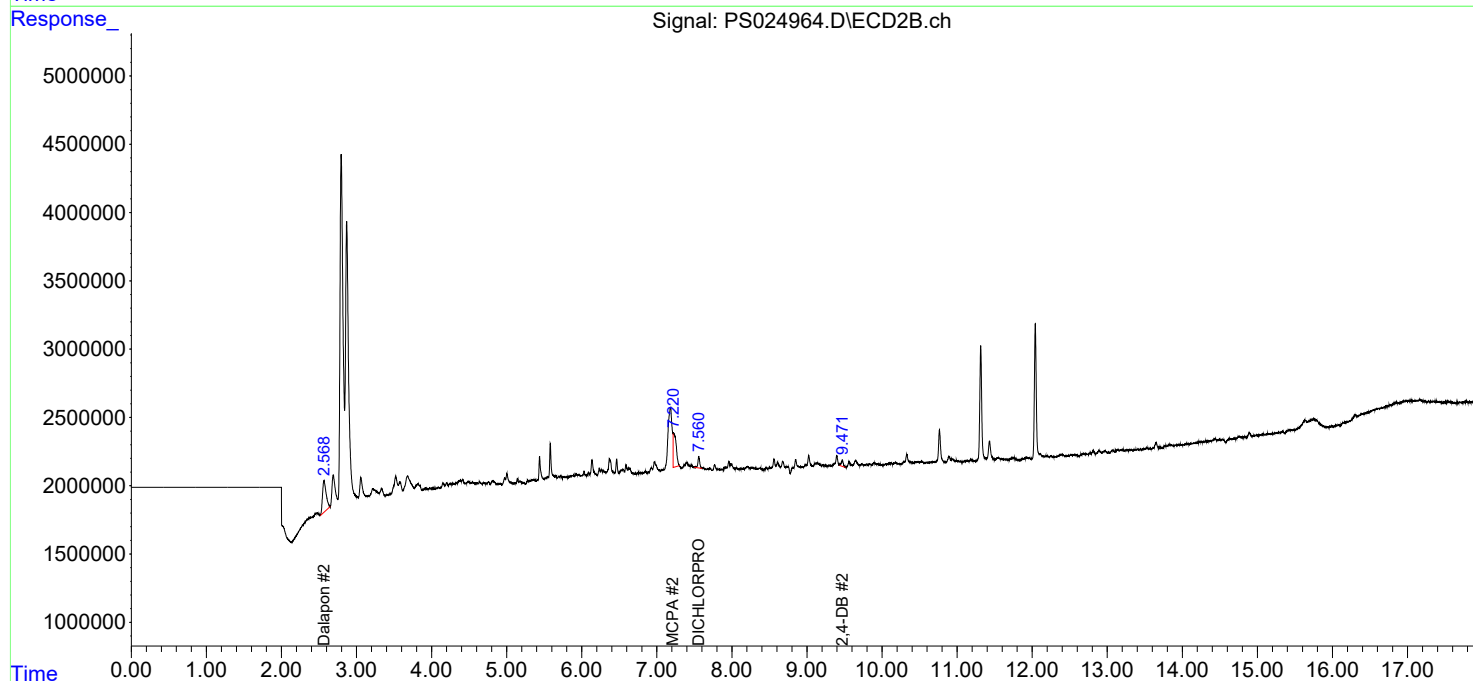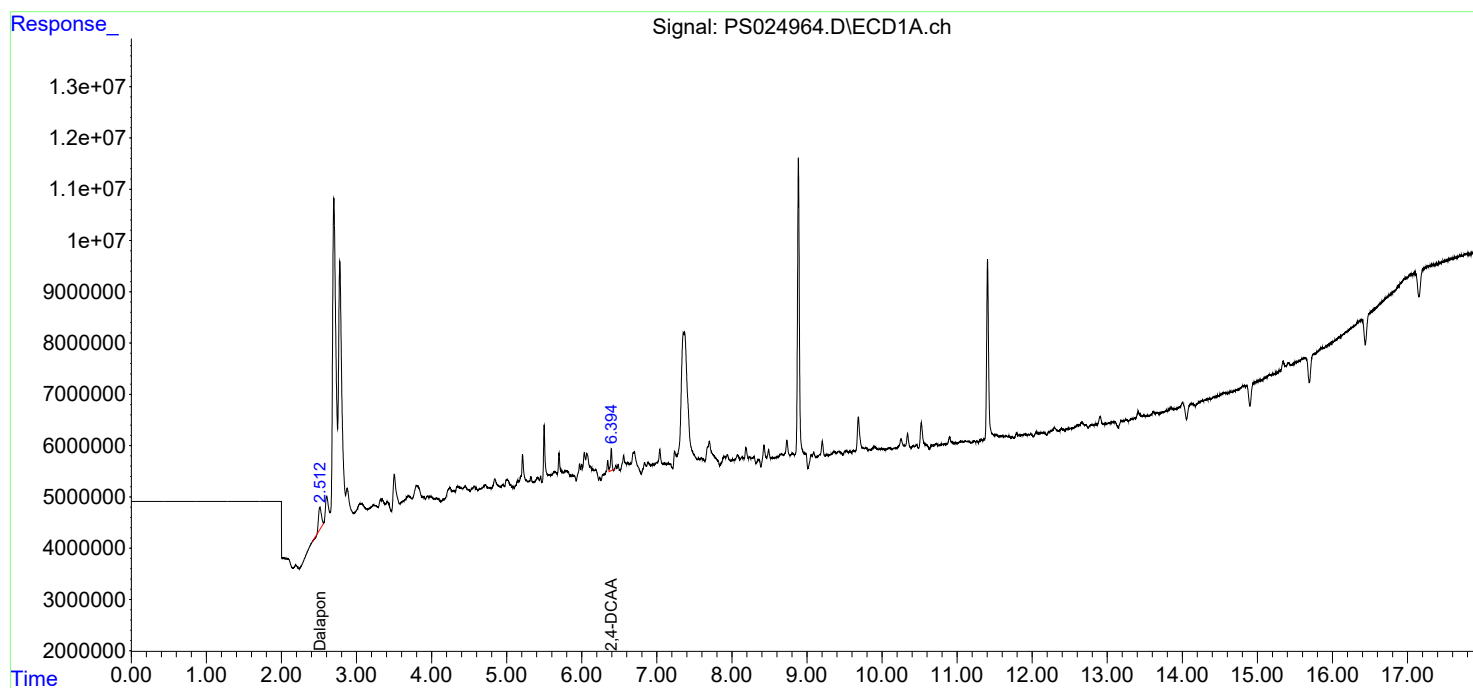


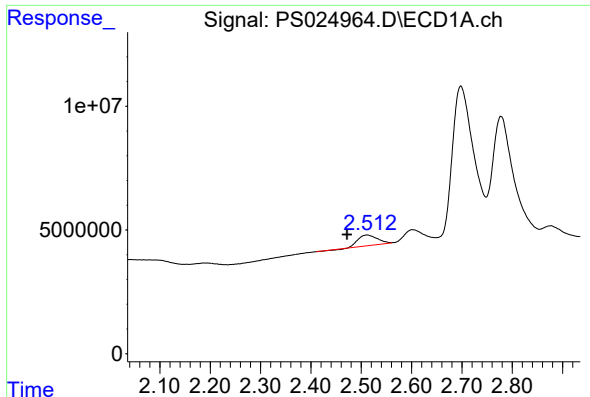

#1 Dalapon


R.T.: 2.511 min
Delta R.T.: 0.039 min
Response: 11196218
Conc: 3.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

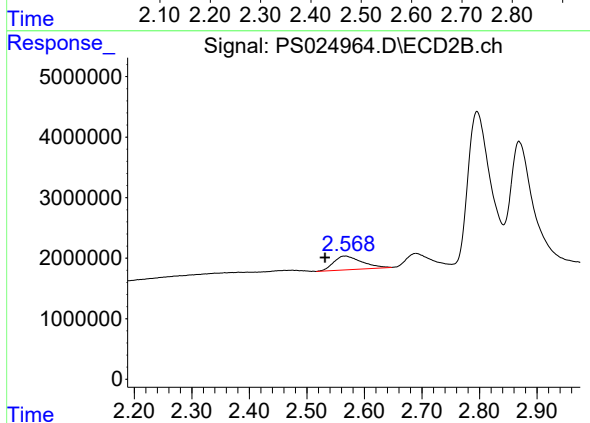


#1 Dalapon

R.T.: 2.568 min
Delta R.T.: 0.037 min
Response: 7809944
Conc: 6.81 ng/ml

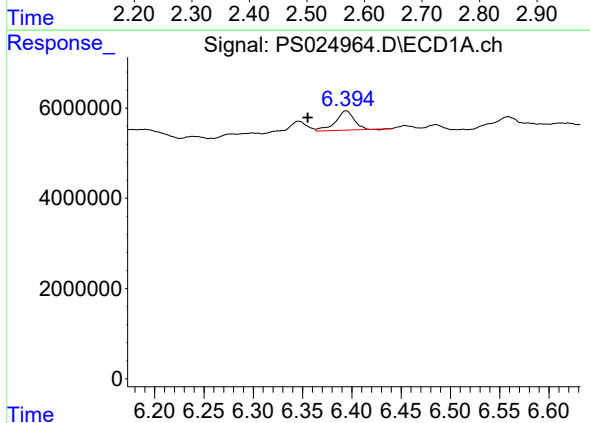


#4 2,4-DCAA

R.T.: 6.394 min
Delta R.T.: 0.039 min
Response: 5568686
Conc: 2.49 ng/ml

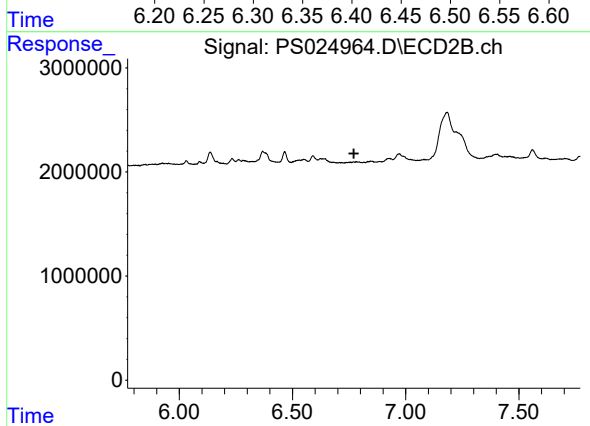

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.771 min
Response: 0
Conc: N.D.

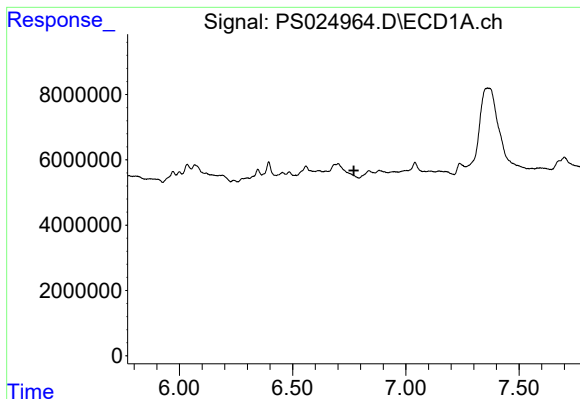

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.771 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

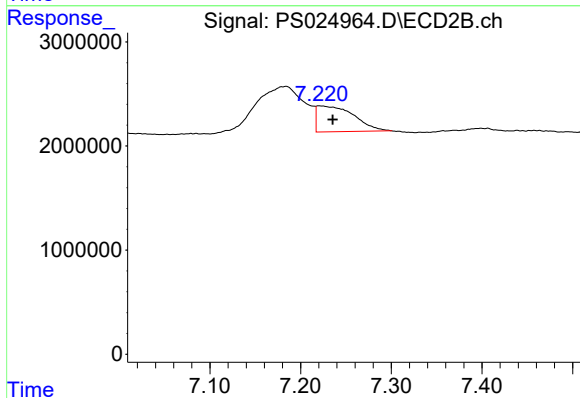


#7 MCPA

R.T.: 7.221 min
Delta R.T.: -0.015 min
Response: 7000266
Conc: 2.13 ug/ml

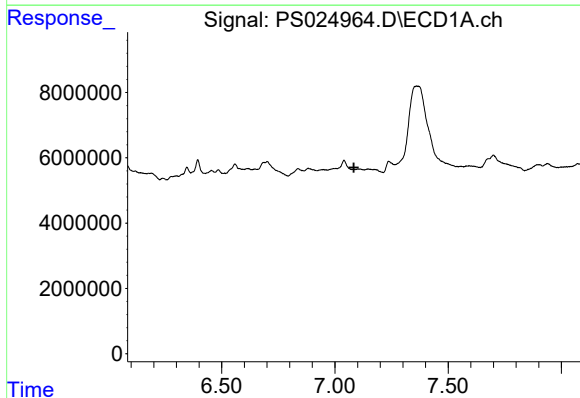


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

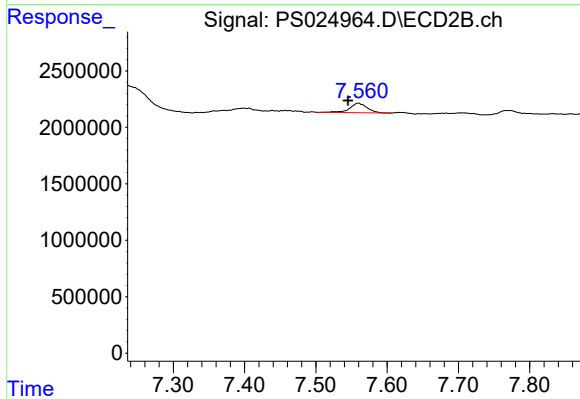

#8 DICHLORPROP


R.T.: 7.559 min
Delta R.T.: 0.014 min
Response: 1410547
Conc: 1.79 ng/ml

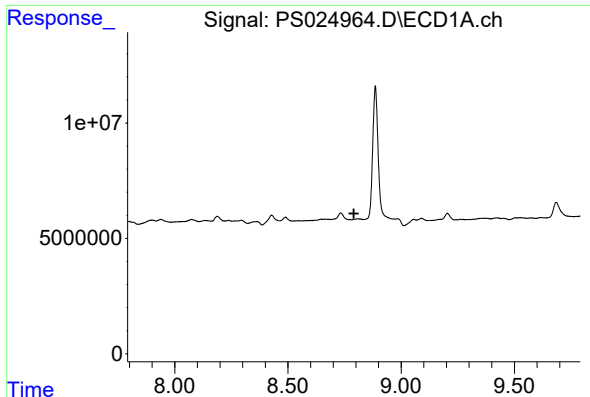

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.791 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

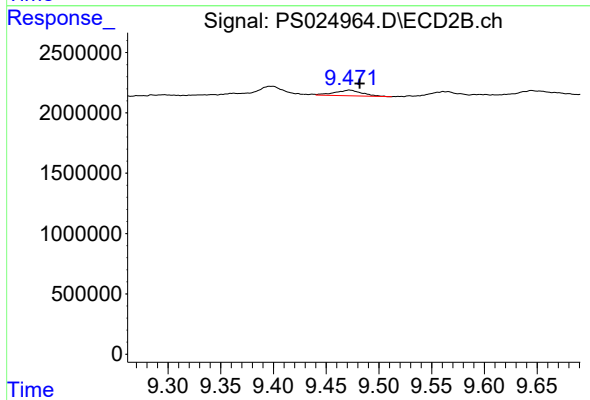

#13 2,4-DB

R.T.: 9.472 min
Delta R.T.: -0.010 min
Response: 839178
Conc: 1.52 ng/ml