

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112823\
 Data File : PS024965.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Nov 2023 14:09
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 28 16:40:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.356	6.772	1168.6E6	378.4E6	522.209	522.207
Target Compounds							
1) T	Dalapon	2.511	2.568	10952987	6114927	3.798	5.331 #
6) T	MCP	6.681	0.000	3691437	0	<MDL	N.D. #
7) T	MCPA	0.000	7.166f	0	23264833	N.D.	7.073
8) T	DICHLORPROP	0.000	7.560	0	3333072	N.D.	4.237
9) T	2,4-D	0.000	7.772f	0	206567	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.562f	0	396026	N.D.	<MDL
12) T	2,4,5-T	0.000	9.024f	0	1428603	N.D.	<MDL
13) T	2,4-DB	0.000	9.475	0	890935	N.D.	1.610
15) T	Picloram	9.686	10.767	13375567	4377338	<MDL	<MDL #
16) T	DCPA	0.000	10.767	0	4377338	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112823\
Data File : PS024965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Nov 2023 14:09
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 28 16:40:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

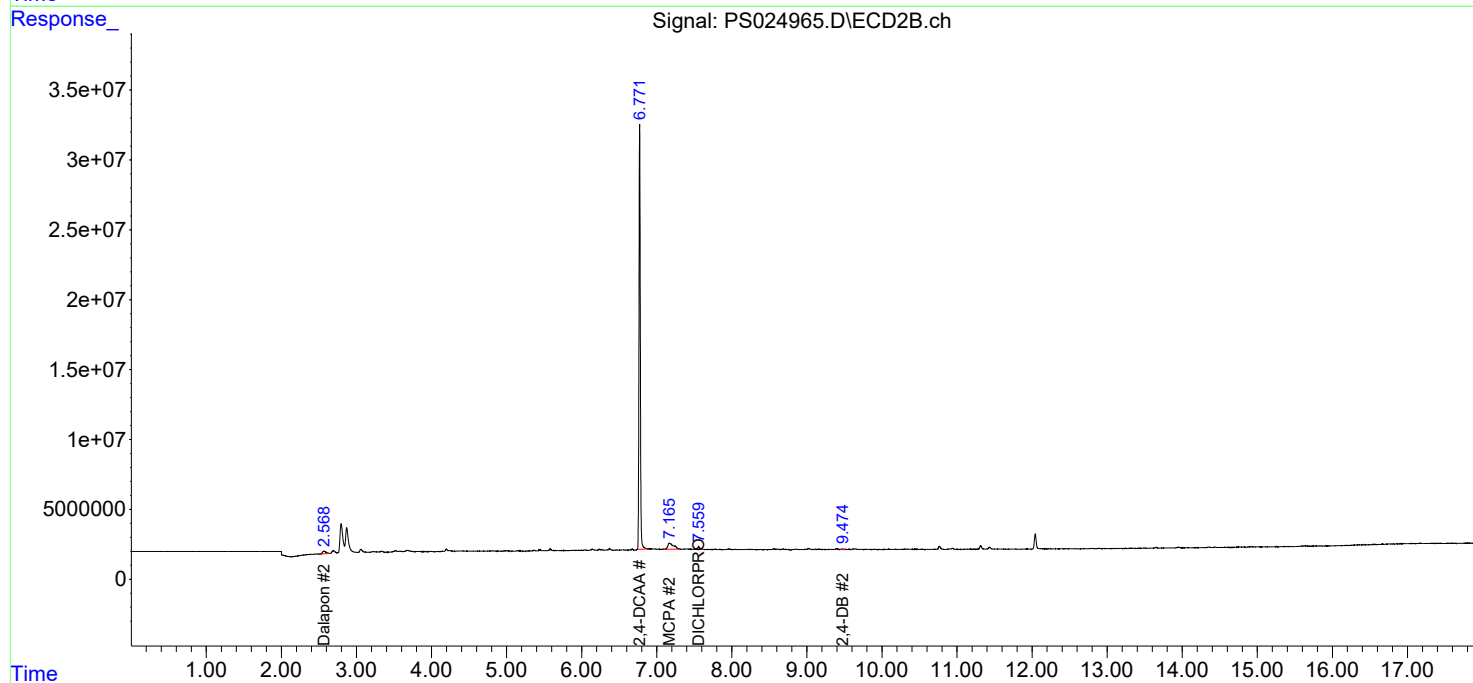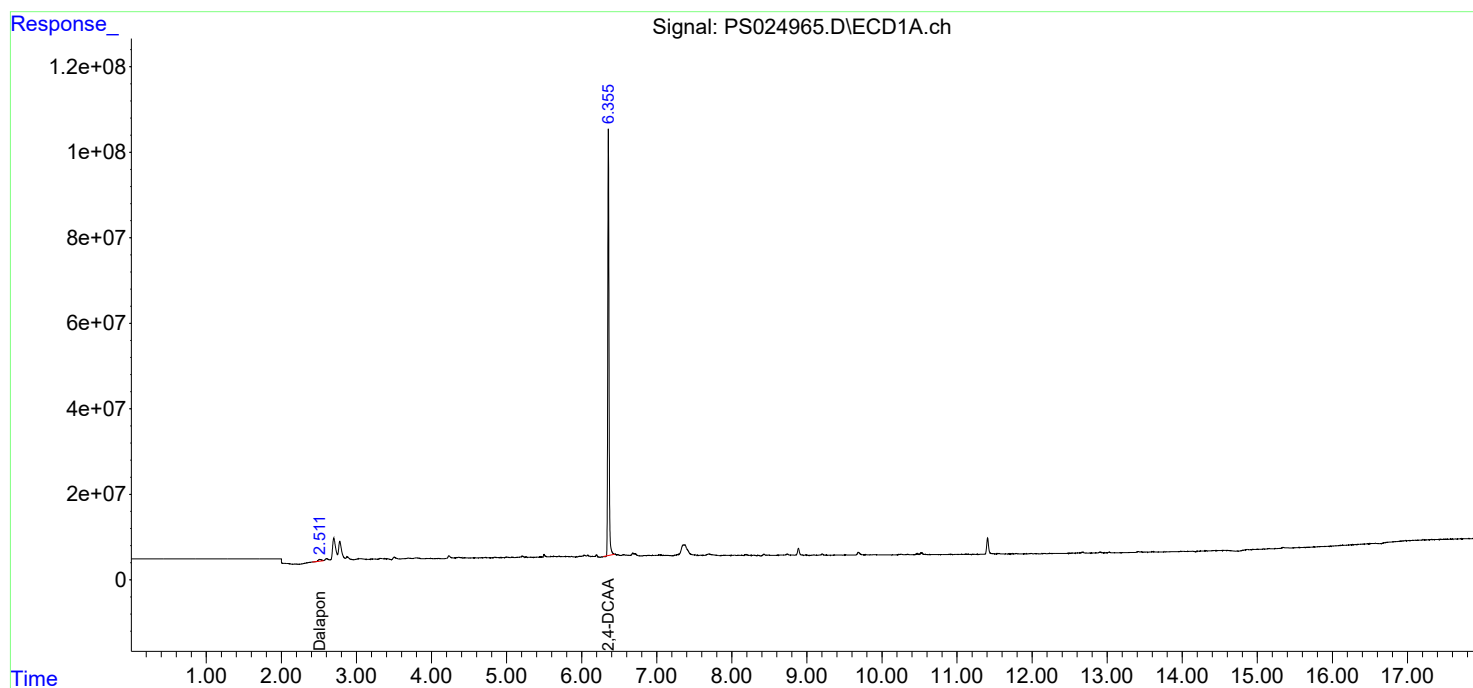


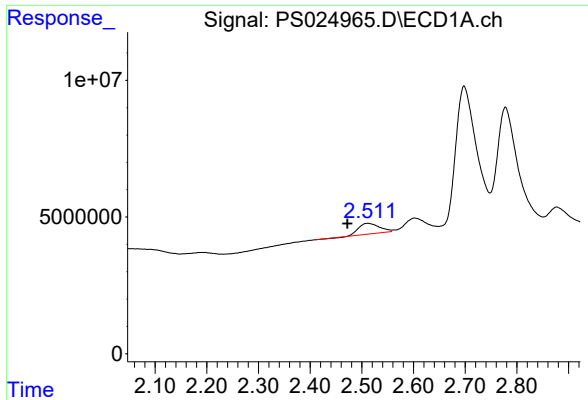

#1 Dalapon


R.T.: 2.511 min
Delta R.T.: 0.039 min
Response: 10952987
Conc: 3.80 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

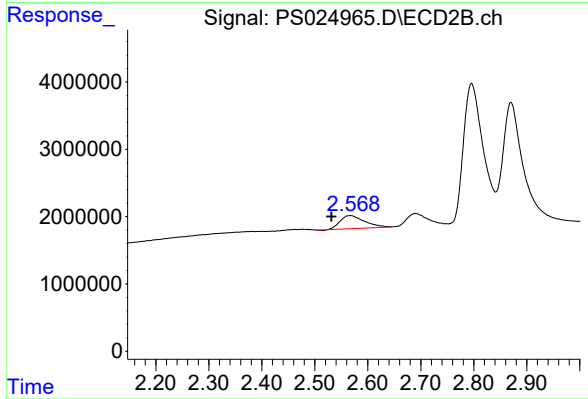


#1 Dalapon

R.T.: 2.568 min
Delta R.T.: 0.036 min
Response: 6114927
Conc: 5.33 ng/ml

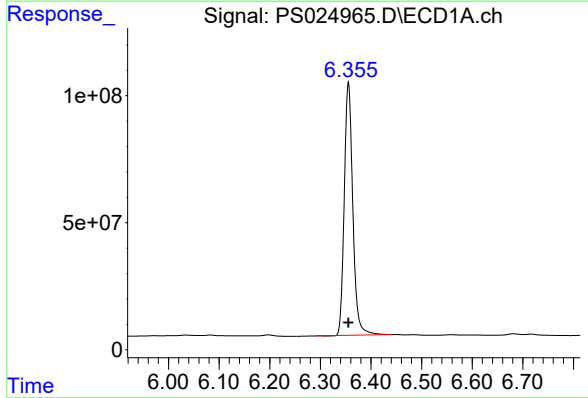


#4 2,4-DCAA

R.T.: 6.356 min
Delta R.T.: 0.000 min
Response: 1168622169
Conc: 522.21 ng/ml

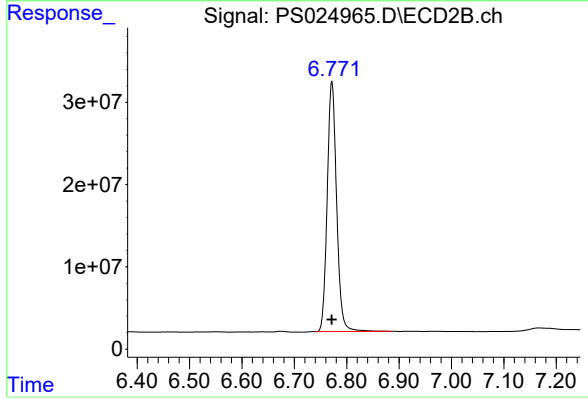

#4 2,4-DCAA


R.T.: 6.772 min
Delta R.T.: 0.000 min
Response: 378367196
Conc: 522.21 ng/ml

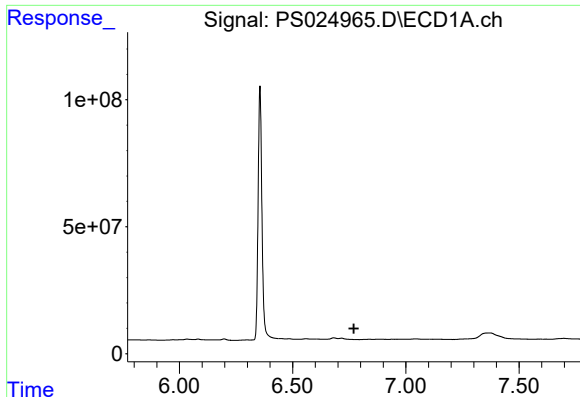

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.771 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

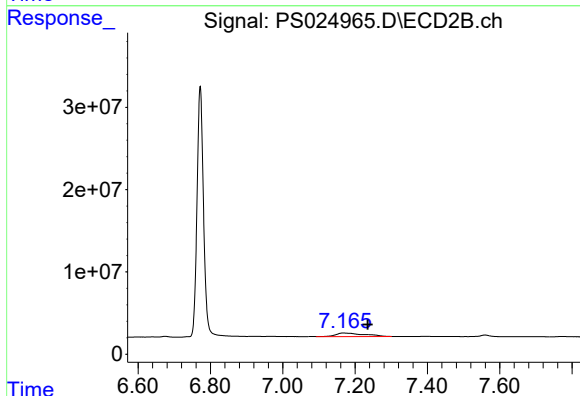


#7 MCPA

R.T.: 7.166 min
Delta R.T.: -0.070 min
Response: 23264833
Conc: 7.07 ug/ml

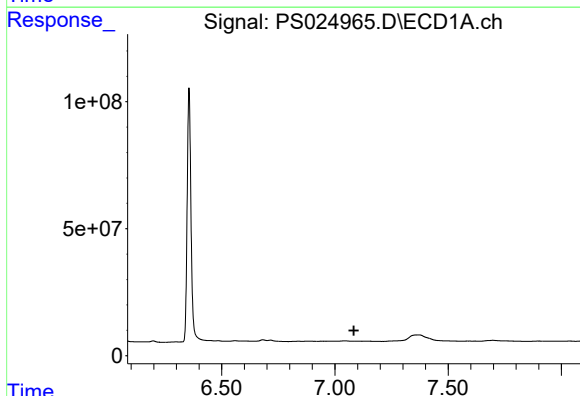


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

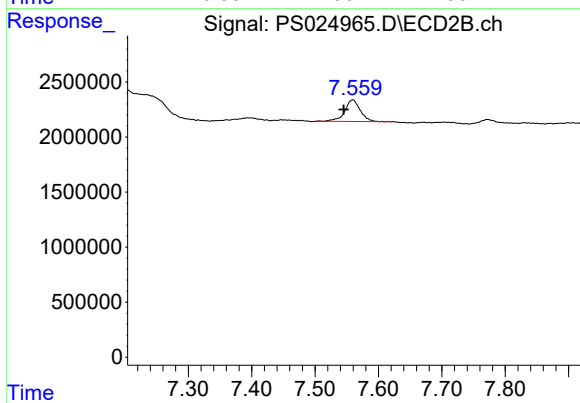

#8 DICHLORPROP


R.T.: 7.560 min
Delta R.T.: 0.014 min
Response: 3333072
Conc: 4.24 ng/ml

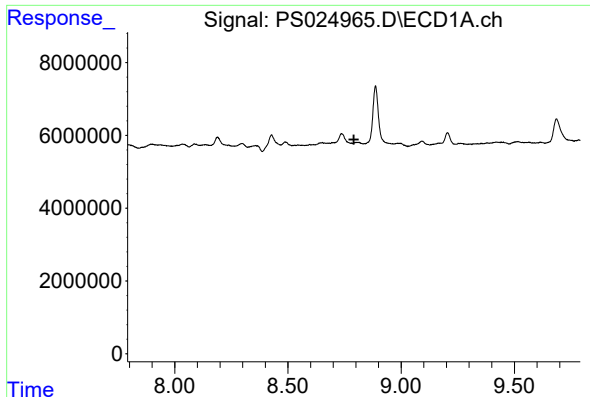

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.791 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

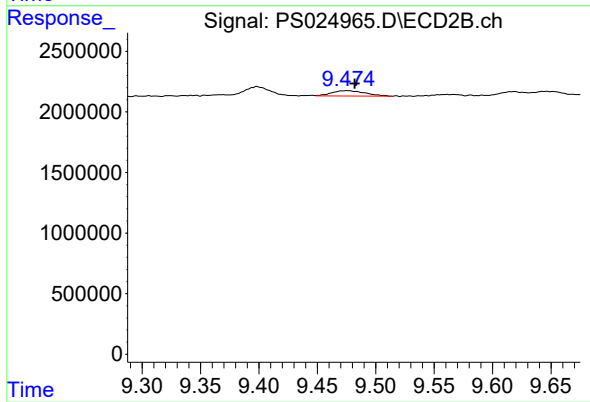

#13 2,4-DB

R.T.: 9.475 min
Delta R.T.: -0.006 min
Response: 890935
Conc: 1.61 ng/ml