

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112918\
 Data File : PS002490.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Nov 2018 21:23
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 29 23:57:29 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 09 15:54:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.401	10.896	168.9E6	166.3E6	554.573	454.594
Target Compounds							
7) T	MCPA	0.000	11.787	0	8559940	N.D.	6.083 #
15) T	Picloram	16.871	0.000	15806081	0	7.443	N.D. #
16) T	DCPA	0.000	16.870	0	112995	N.D.	0.047 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112918\
Data File : PS002490.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Nov 2018 21:23
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 29 23:57:29 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
Quant Title : 8080.M
QLast Update : Fri Nov 09 15:54:35 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

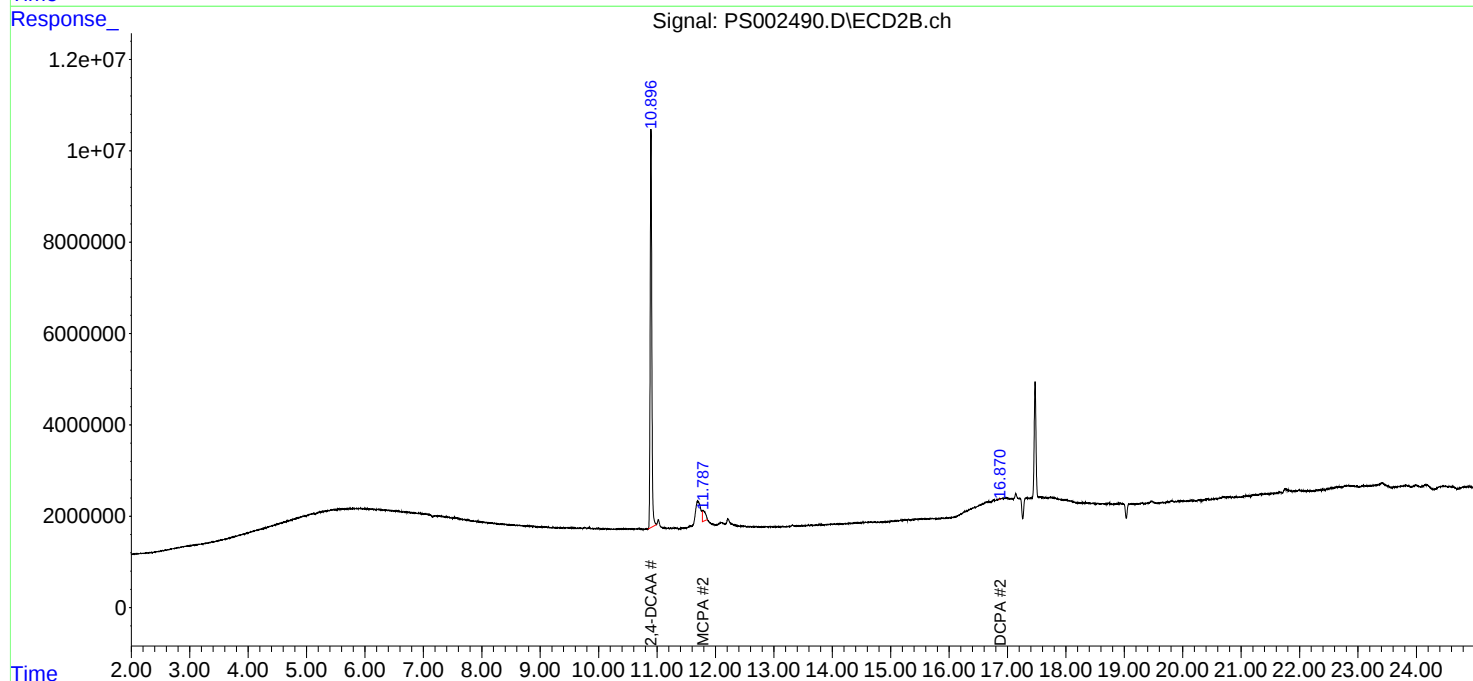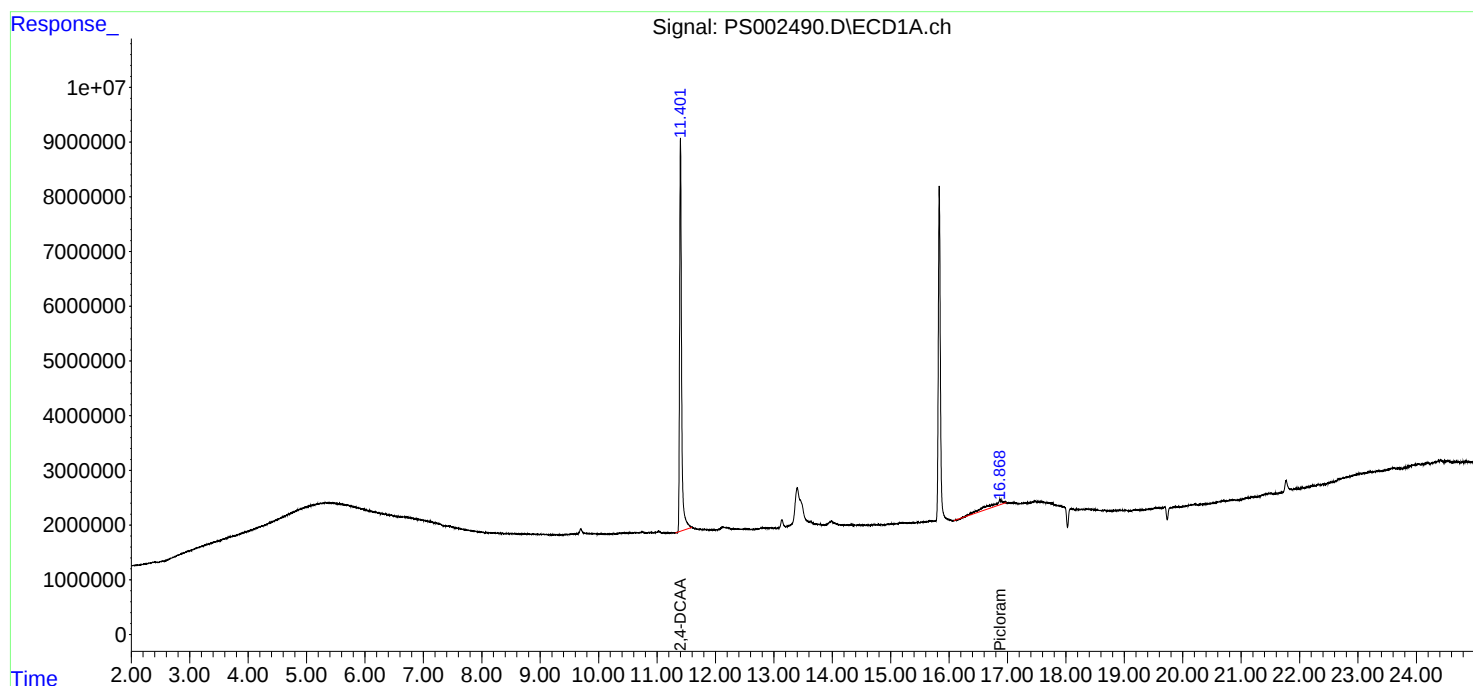


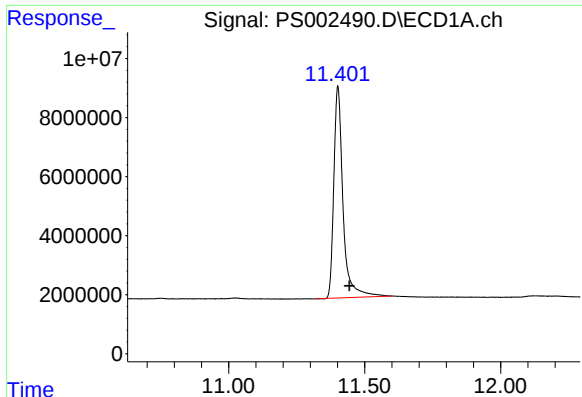

#4 2,4-DCAA


R.T.: 11.401 min
Delta R.T.: -0.042 min
Response: 168922615
Conc: 554.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

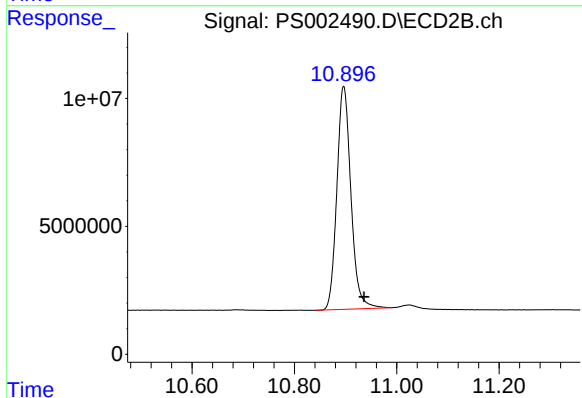


#4 2,4-DCAA

R.T.: 10.896 min
Delta R.T.: -0.040 min
Response: 166341416
Conc: 454.59 ng/ml

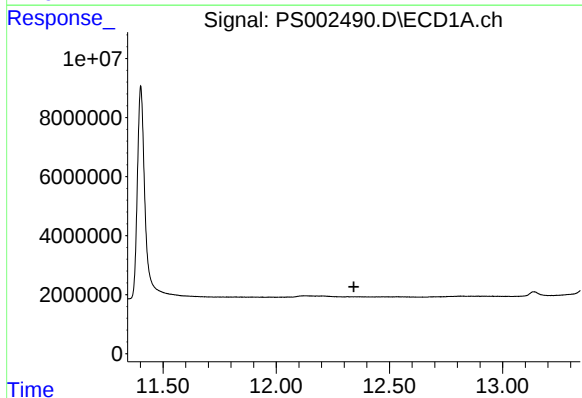


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.343 min
Response: 0
Conc: N.D.

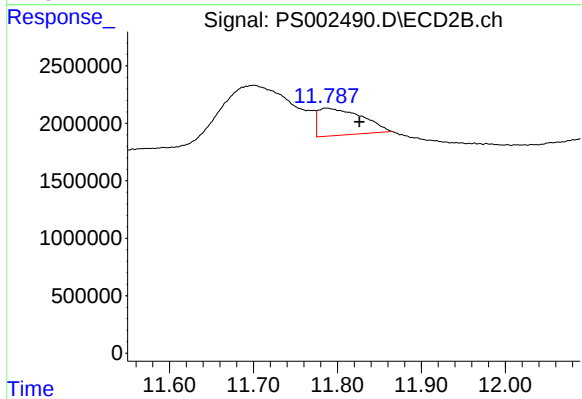

#7 MCPA


R.T.: 11.787 min
Delta R.T.: -0.039 min
Response: 8559940
Conc: 6.08 ug/ml

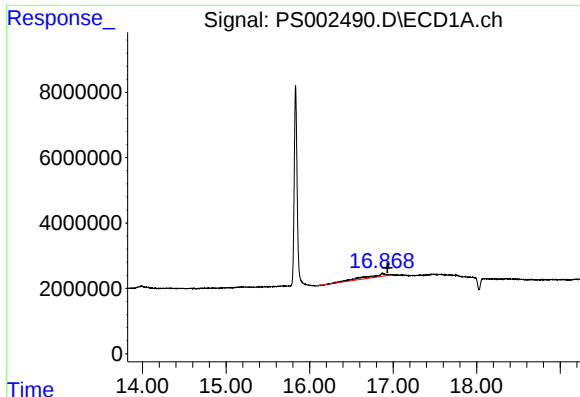

#15 Picloram


R.T.: 16.871 min
Delta R.T.: -0.060 min
Response: 15806081
Conc: 7.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

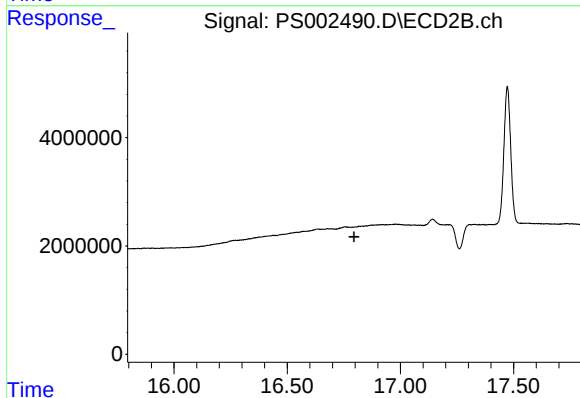


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.795 min
Response: 0
Conc: N.D.

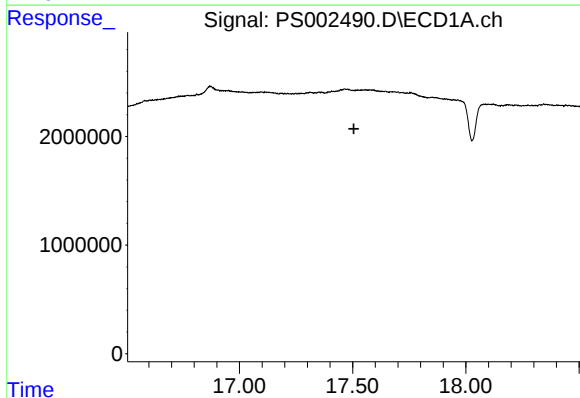

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.506 min
Response: 0
Conc: N.D.

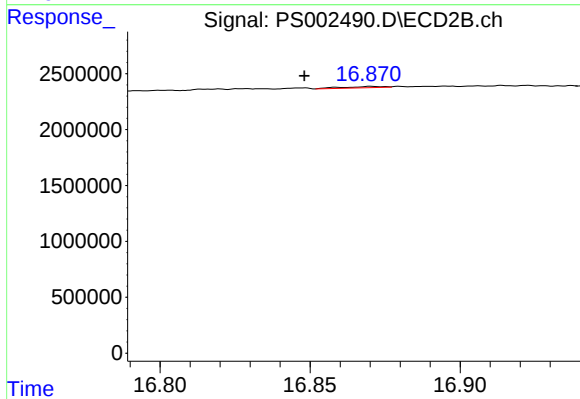

#16 DCPA

R.T.: 16.870 min
Delta R.T.: 0.022 min
Response: 112995
Conc: 0.05 ng/ml