

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112923\
 Data File : PS024972.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Nov 2023 09:21
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 29 23:48:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	6.394	0.000	5225832	0	2.335	N.D.	#
Target Compounds								
1) T	Dalapon	2.511	2.567	13475275	8252452	4.673	7.194	#
5) T	DICAMBA	0.000	6.973f	0	3323101	N.D.	1.073	
6) T	MCPP	0.000	6.973f	0	3323101	N.D.	1.602	
7) T	MCPA	0.000	7.223	0	5439940	N.D.	1.654	
8) T	DICHLORPROP	0.000	7.560	0	1010697	N.D.	1.285	
9) T	2,4-D	7.247	7.770f	9974383	441478	3.284	<MDL	#
11) T	2,4,5-TP ...	0.000	8.608	0	311163	N.D.	<MDL	
12) T	2,4,5-T	0.000	8.981	0	574748	N.D.	<MDL	
13) T	2,4-DB	0.000	9.481	0	610189	N.D.	1.102	
15) T	Picloram	9.685	10.765	47453271	14254089	2.435	2.178	
16) T	DCPA	0.000	10.765	0	14254089	N.D.	2.630	



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112923\
Data File : PS024972.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Nov 2023 09:21
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 29 23:48:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

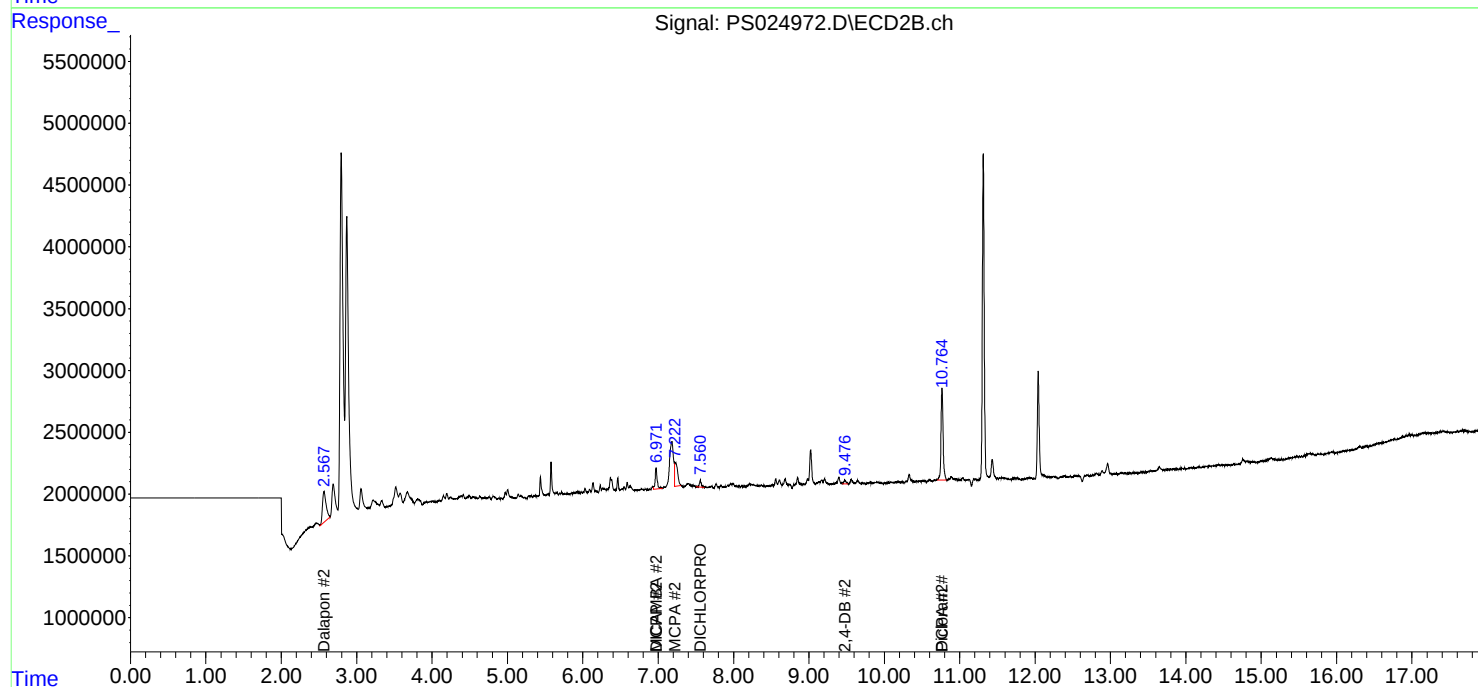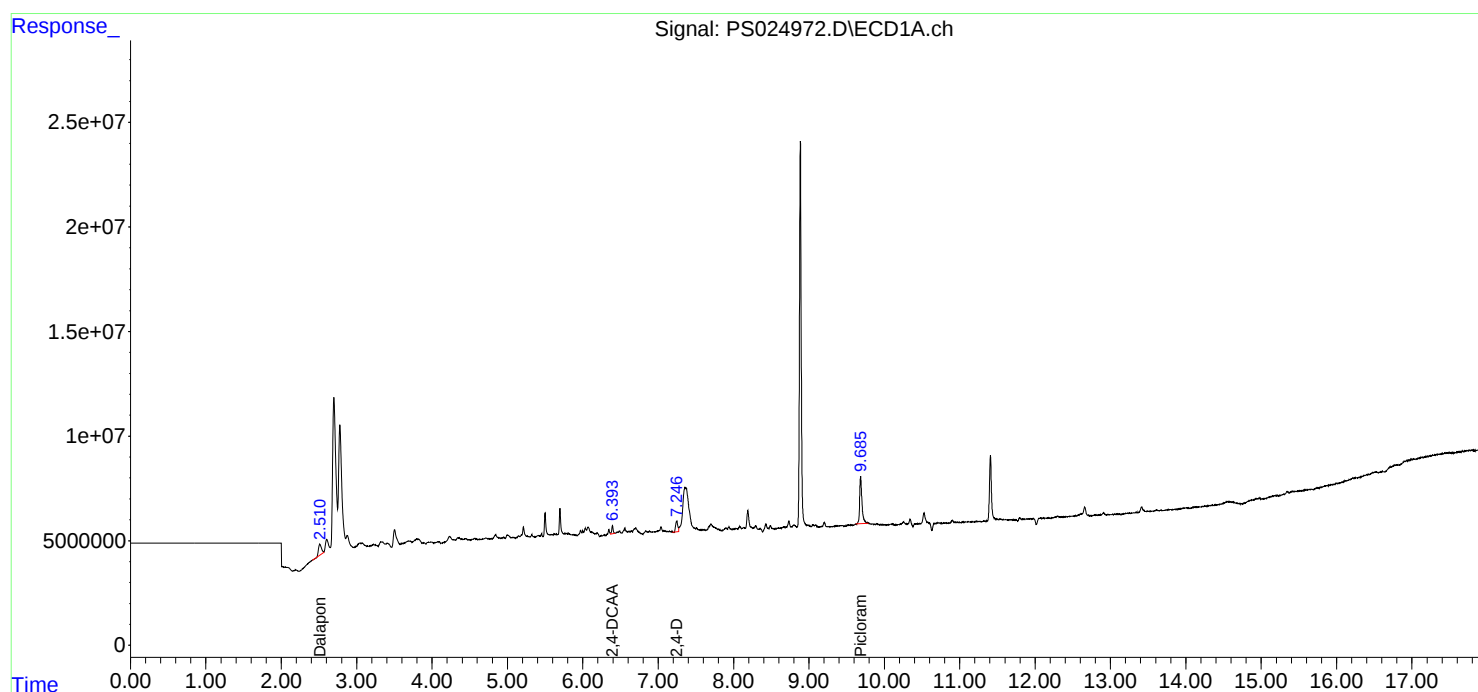


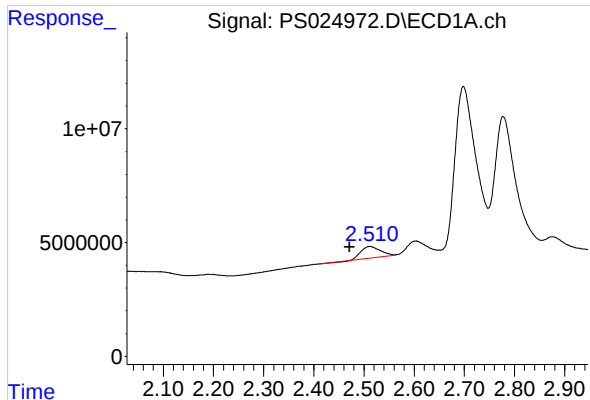

#1 Dalapon


R.T.: 2.511 min
Delta R.T.: 0.039 min
Response: 13475275
Conc: 4.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

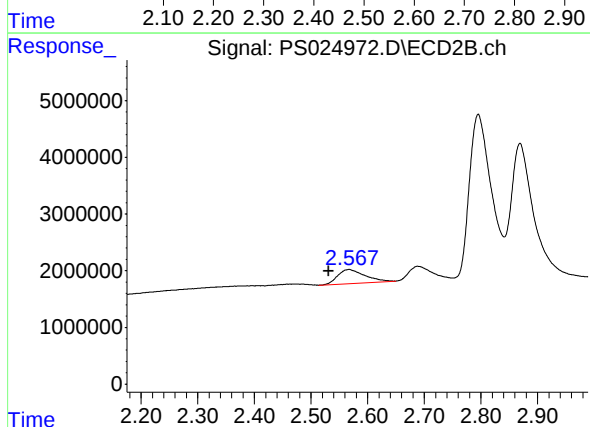


#1 Dalapon

R.T.: 2.567 min
Delta R.T.: 0.036 min
Response: 8252452
Conc: 7.19 ng/ml

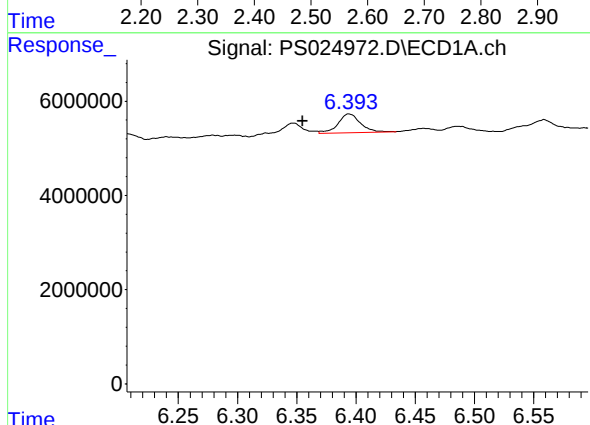


#4 2,4-DCAA

R.T.: 6.394 min
Delta R.T.: 0.039 min
Response: 5225832
Conc: 2.34 ng/ml

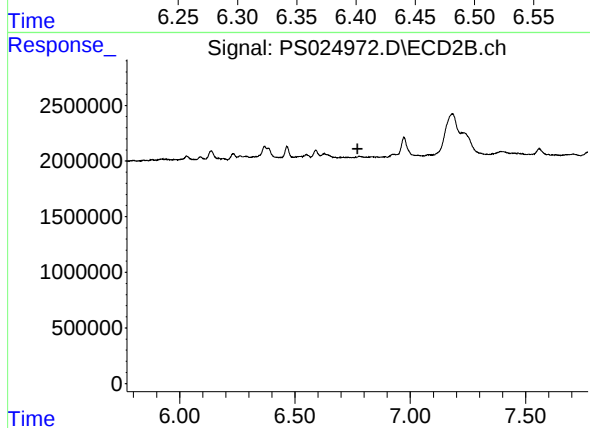

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 6.771 min
Response: 0
Conc: N.D.

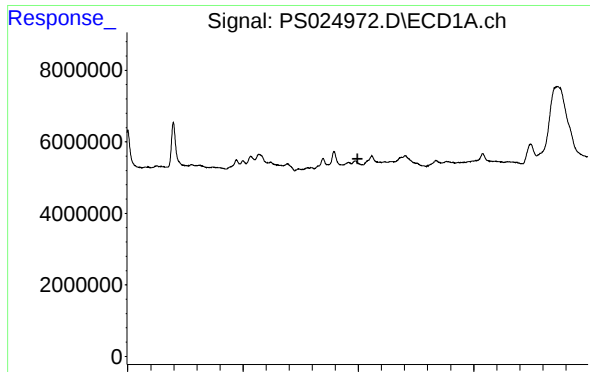

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.496 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

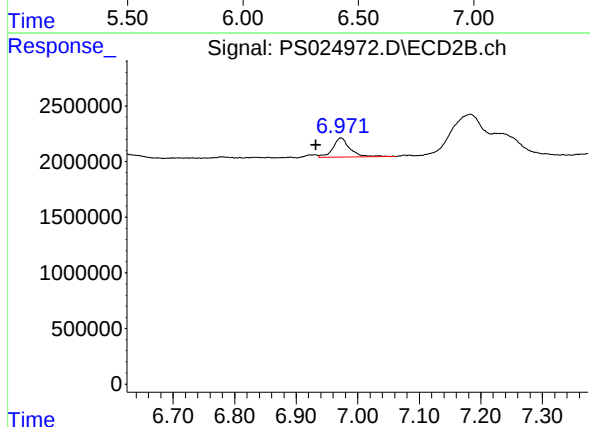


#5 DICAMBA

R.T.: 6.973 min
Delta R.T.: 0.041 min
Response: 3323101
Conc: 1.07 ng/ml

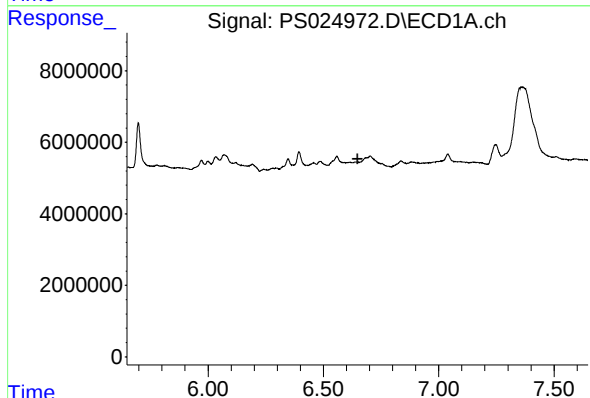


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 6.648 min
Response: 0
Conc: N.D.

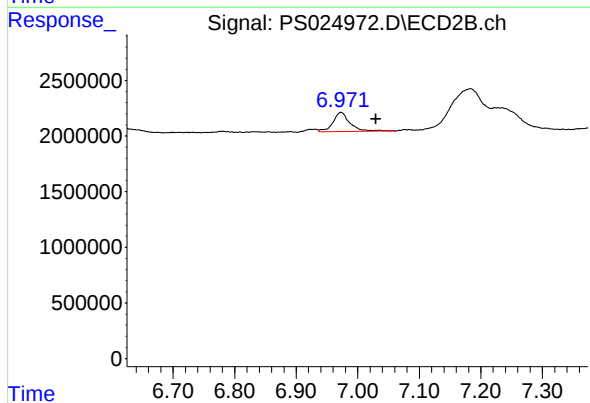

#6 MCPP


R.T.: 6.973 min
Delta R.T.: -0.057 min
Response: 3323101
Conc: 1.60 ug/ml

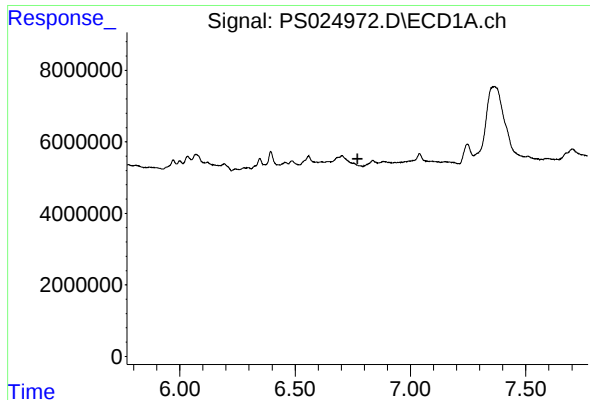

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.771 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

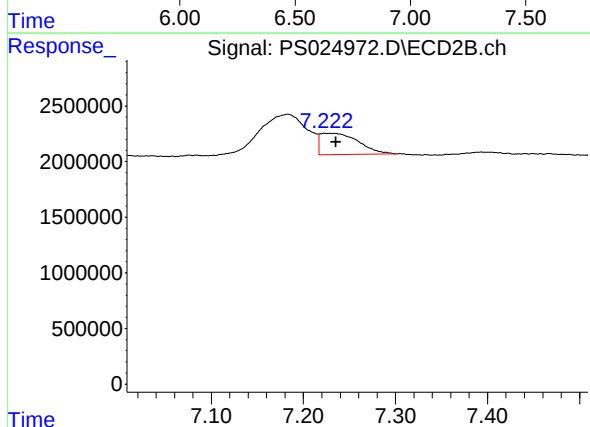


#7 MCPA

R.T.: 7.223 min
Delta R.T.: -0.012 min
Response: 5439940
Conc: 1.65 ug/ml

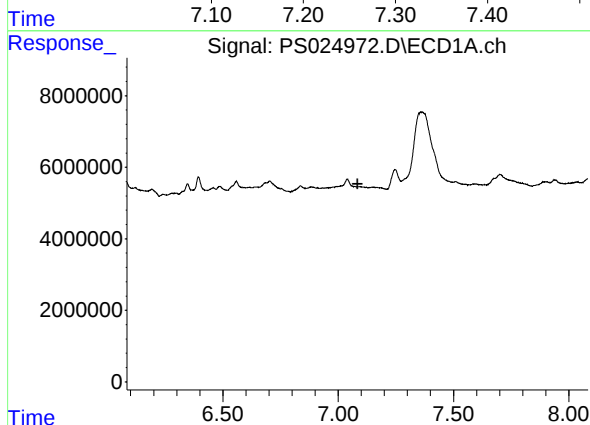


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

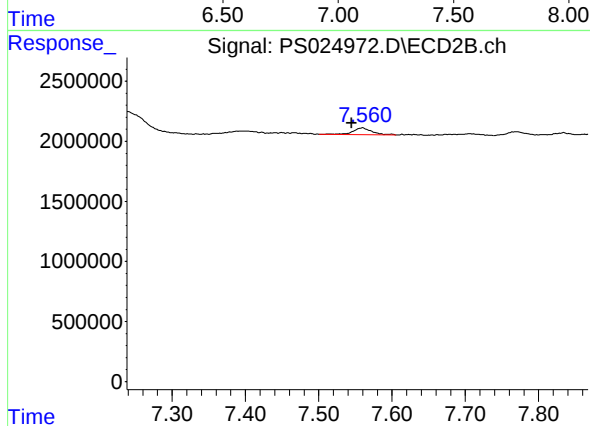

#8 DICHLORPROP


R.T.: 7.560 min
Delta R.T.: 0.015 min
Response: 1010697
Conc: 1.28 ng/ml

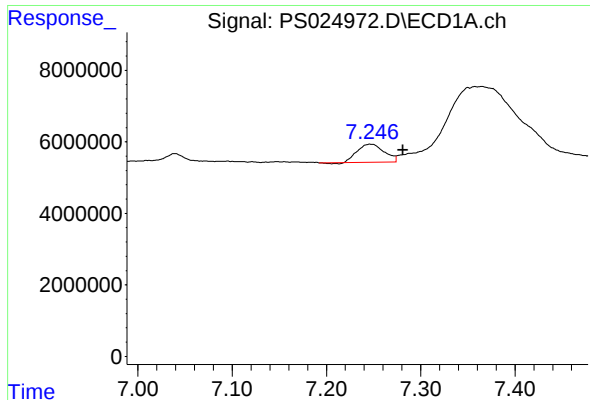

#9 2,4-D


R.T.: 7.247 min
Delta R.T.: -0.034 min
Response: 9974383
Conc: 3.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

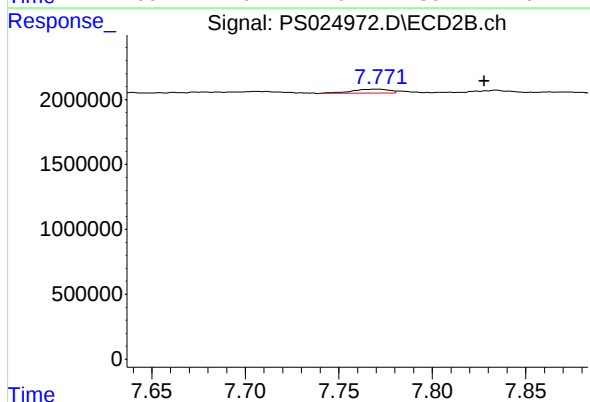


#9 2,4-D

R.T.: 7.770 min
Delta R.T.: -0.058 min
Response: 441478
Conc: N.D.

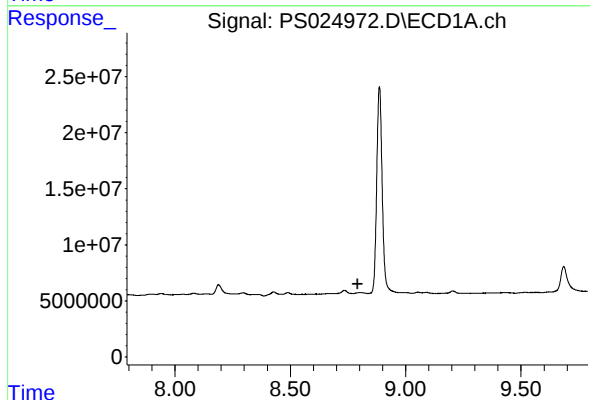


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.791 min
Response: 0
Conc: N.D.

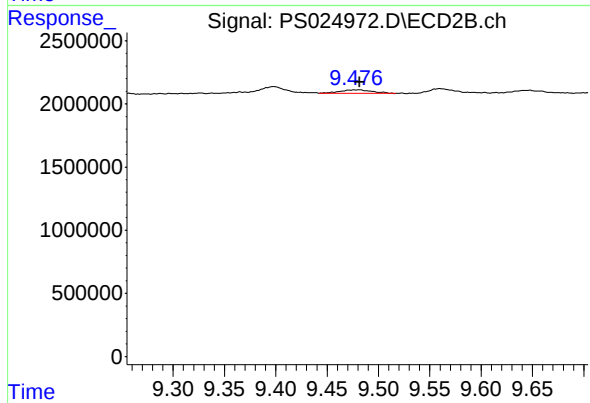

#13 2,4-DB


R.T.: 9.481 min
Delta R.T.: 0.000 min
Response: 610189
Conc: 1.10 ng/ml

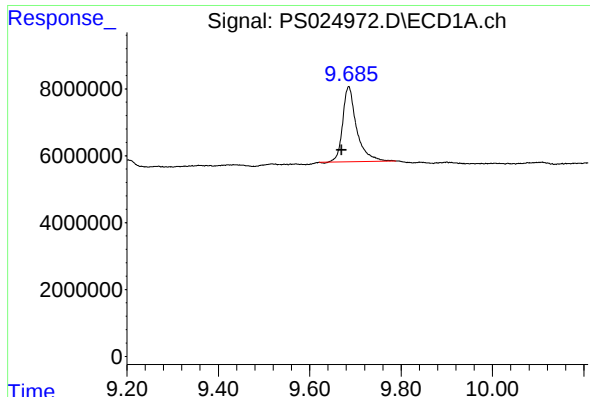

#15 Picloram


R.T.: 9.685 min
Delta R.T.: 0.016 min
Response: 47453271
Conc: 2.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

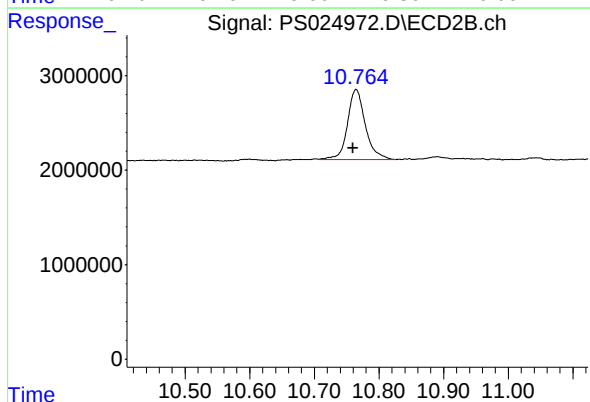


#15 Picloram

R.T.: 10.765 min
Delta R.T.: 0.005 min
Response: 14254089
Conc: 2.18 ng/ml

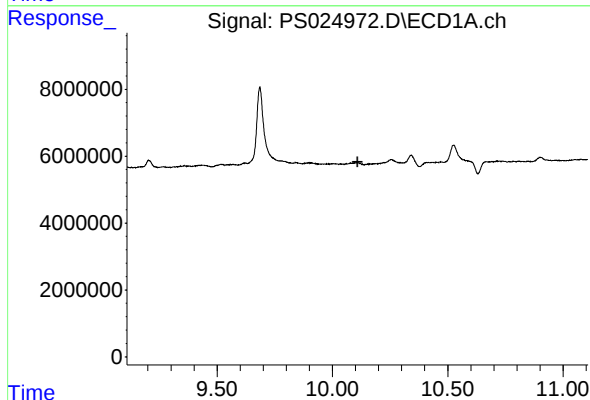

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.109 min
Response: 0
Conc: N.D.

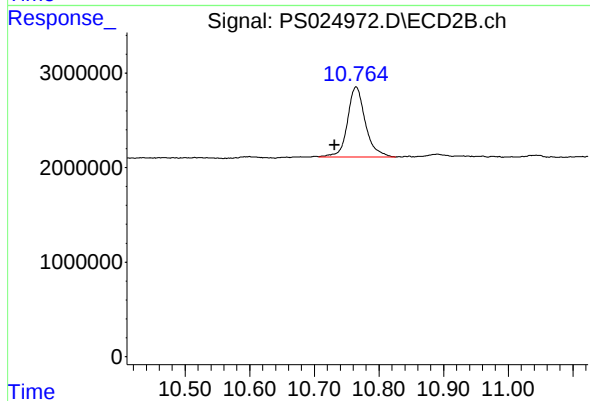

#16 DCPA

R.T.: 10.765 min
Delta R.T.: 0.033 min
Response: 14254089
Conc: 2.63 ng/ml