

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112923\
 Data File : PS024973.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Nov 2023 09:45
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 29 23:48:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.356	6.772	1156.3E6	370.8E6	516.716	511.778
Target Compounds						
1) T Dalapon	2.512f	2.565	11651650	5834797	4.041	5.087 #
3) T 4-Nitroph...	0.000	6.368	0	420237	N.D.	<MDL
5) T DICAMBA	0.000	6.971	0	710164	N.D.	<MDL
6) T MCPP	0.000	6.971f	0	710164	N.D.	<MDL
7) T MCPA	0.000	7.168f	0	20108652	N.D.	6.113
8) T DICHLORPROP	0.000	7.559	0	1138388	N.D.	1.447
12) T 2,4,5-T	0.000	8.984	0	450449	N.D.	<MDL
15) T Picloram	9.687	10.766	34472576	10673937	1.769	1.631
16) T DCPA	0.000	10.766	0	10673937	N.D.	1.969



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112923\
Data File : PS024973.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Nov 2023 09:45
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 29 23:48:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

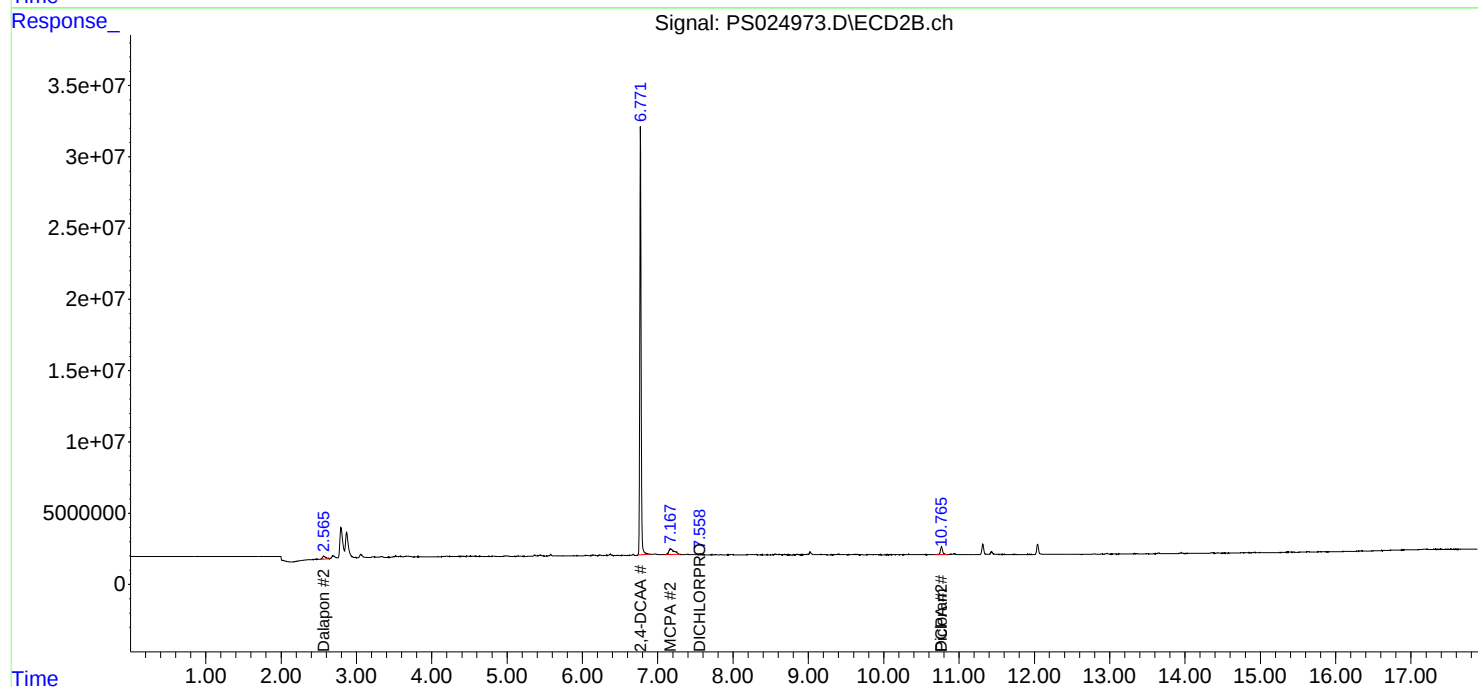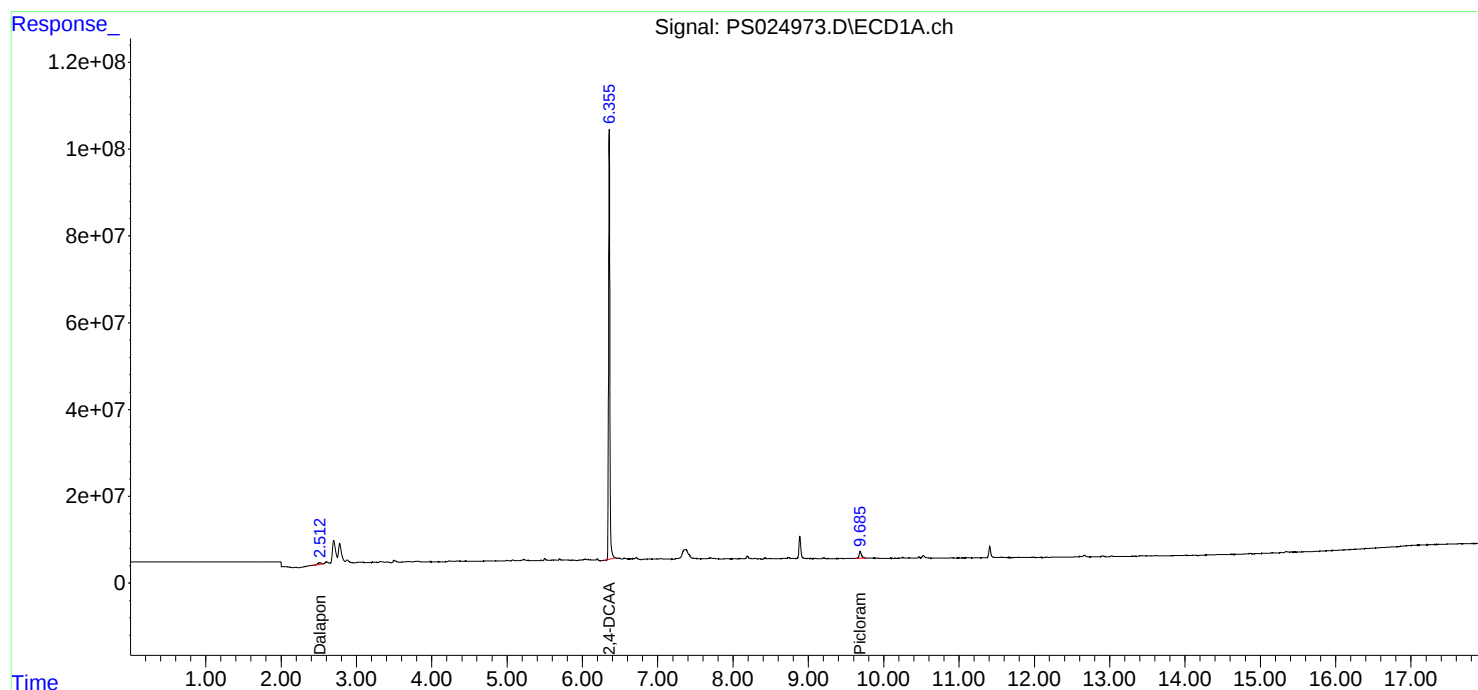


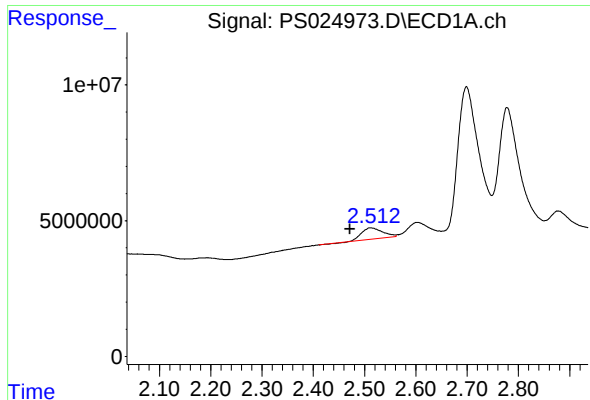

#1 Dalapon


R.T.: 2.512 min
Delta R.T.: 0.040 min
Response: 11651650
Conc: 4.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

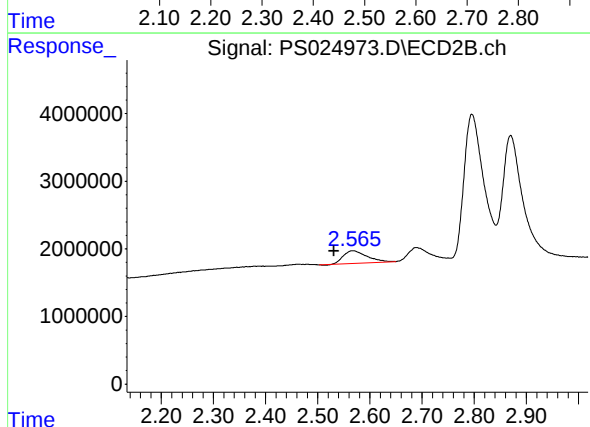


#1 Dalapon

R.T.: 2.565 min
Delta R.T.: 0.034 min
Response: 5834797
Conc: 5.09 ng/ml

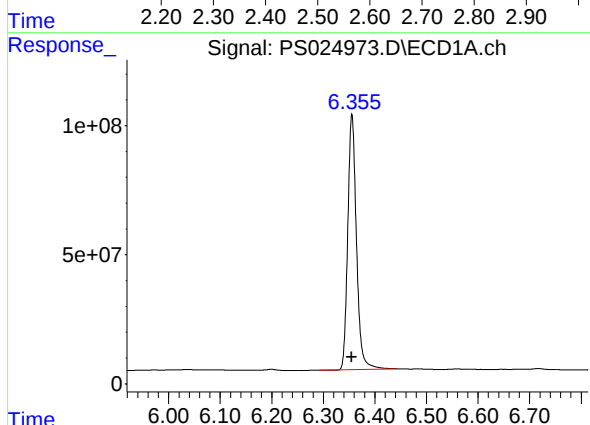


#4 2,4-DCAA

R.T.: 6.356 min
Delta R.T.: 0.000 min
Response: 1156330976
Conc: 516.72 ng/ml

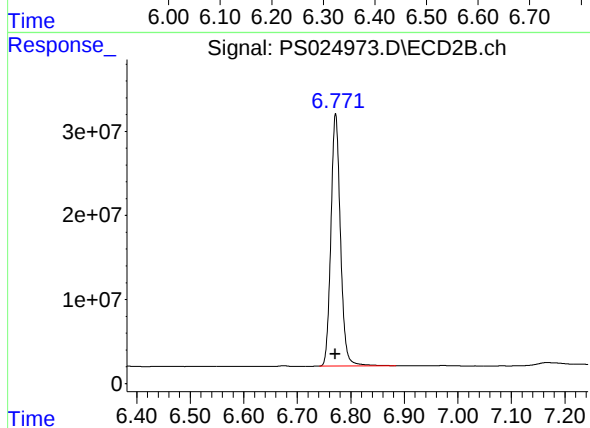

#4 2,4-DCAA


R.T.: 6.772 min
Delta R.T.: 0.000 min
Response: 370810795
Conc: 511.78 ng/ml

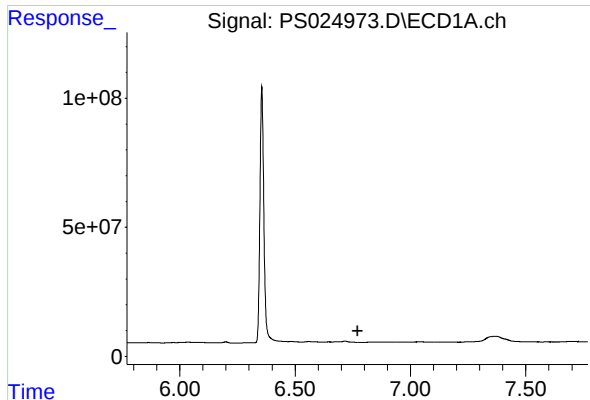

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.771 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

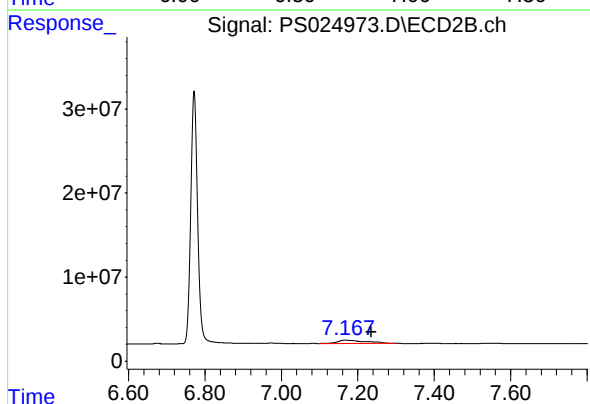


#7 MCPA

R.T.: 7.168 min
Delta R.T.: -0.068 min
Response: 20108652
Conc: 6.11 ug/ml

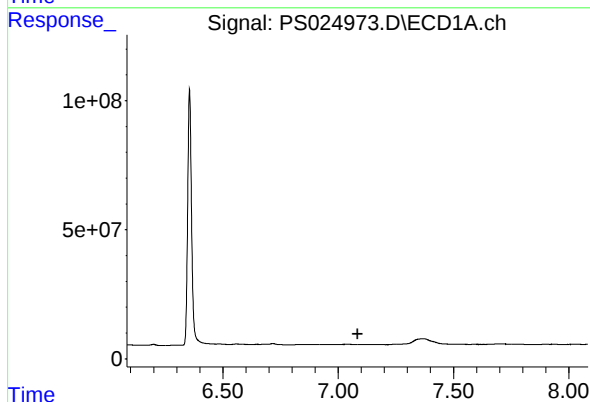


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

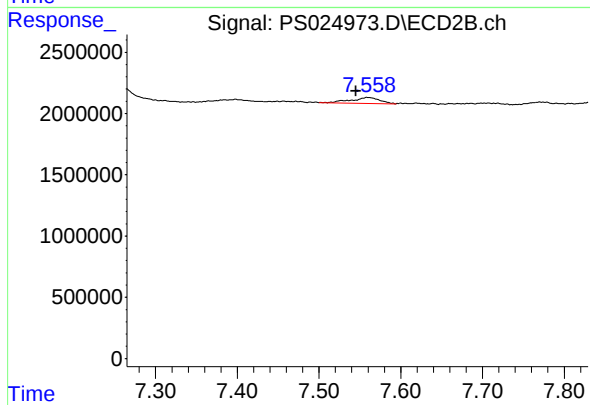

#8 DICHLORPROP


R.T.: 7.559 min
Delta R.T.: 0.014 min
Response: 1138388
Conc: 1.45 ng/ml

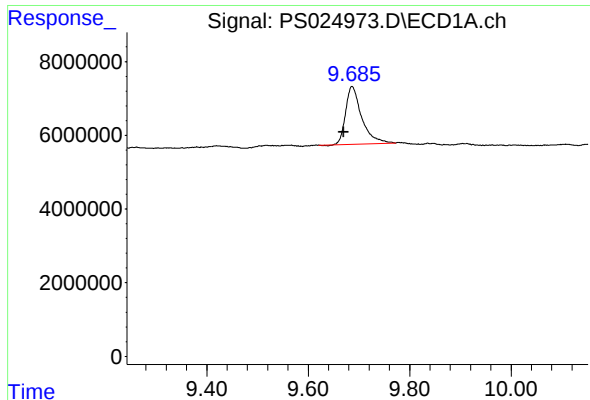

#15 Picloram


R.T.: 9.687 min
Delta R.T.: 0.017 min
Response: 34472576
Conc: 1.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

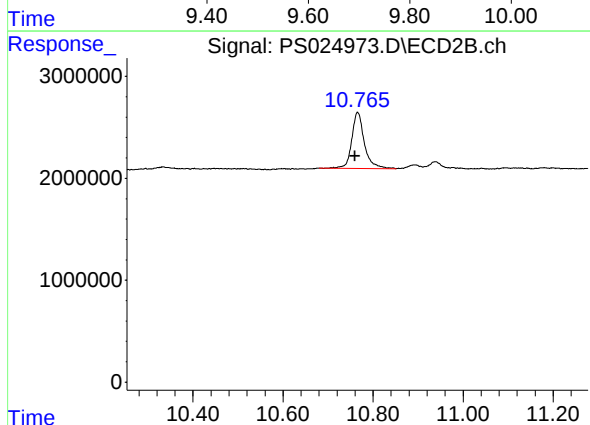


#15 Picloram

R.T.: 10.766 min
Delta R.T.: 0.006 min
Response: 10673937
Conc: 1.63 ng/ml

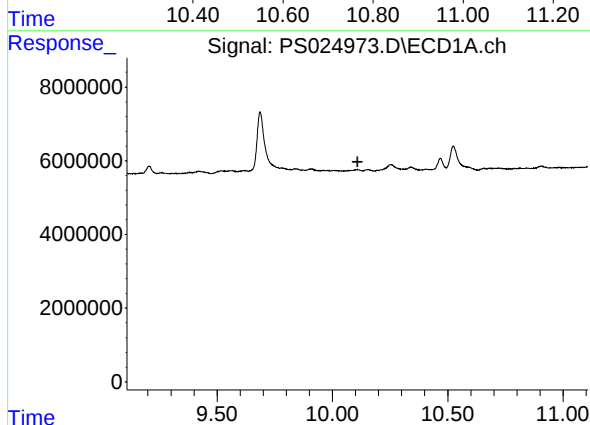

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.109 min
Response: 0
Conc: N.D.

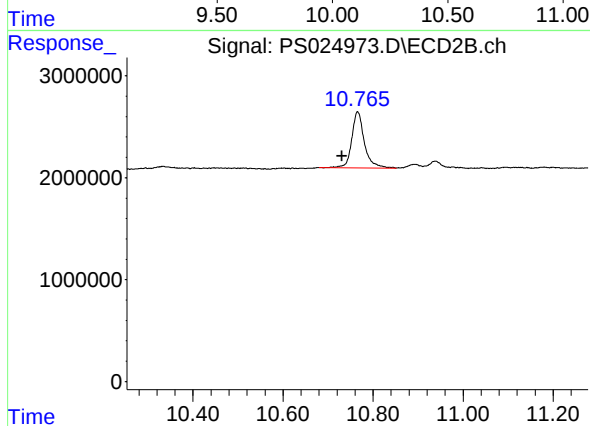

#16 DCPA

R.T.: 10.766 min
Delta R.T.: 0.034 min
Response: 10673937
Conc: 1.97 ng/ml