

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS113020\
 Data File : PS013361.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Nov 2020 14:29
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 15:53:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110220.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 03 03:59:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.213	6.912	416.6E6	218.4E6	466.063	561.228
Target Compounds							
6) T	MCP	0.000	7.237f	0	30785498	N.D.	23.259
9) T	2,4-D	8.370f	7.979	25679981	8103694	27.182	15.270 #
12) T	2,4,5-T	9.423f	0.000	28138754	0	5.317	N.D. #
15) T	Picloram	11.053f	11.036	118.1E6	80776285	17.965	22.379



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS113020\
Data File : PS013361.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Nov 2020 14:29
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 15:53:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110220.M
Quant Title : 8080.M
QLast Update : Tue Nov 03 03:59:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

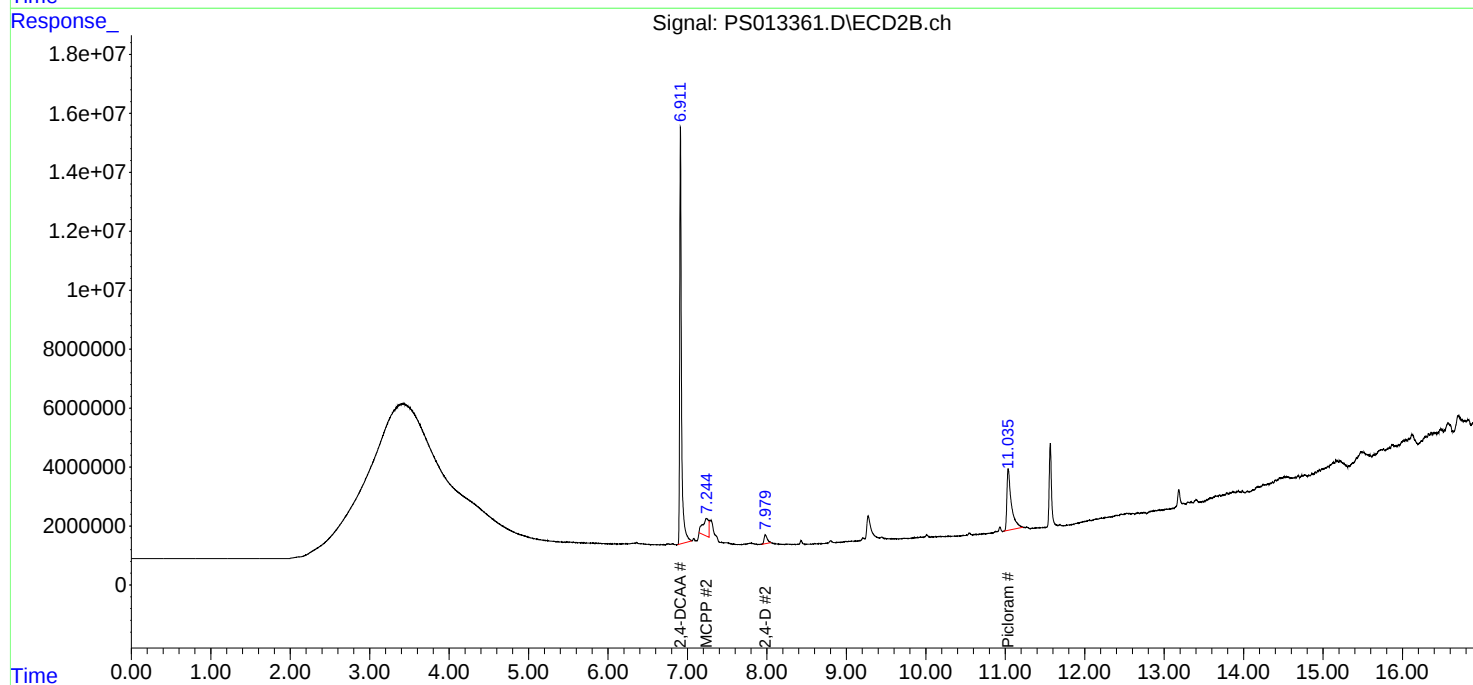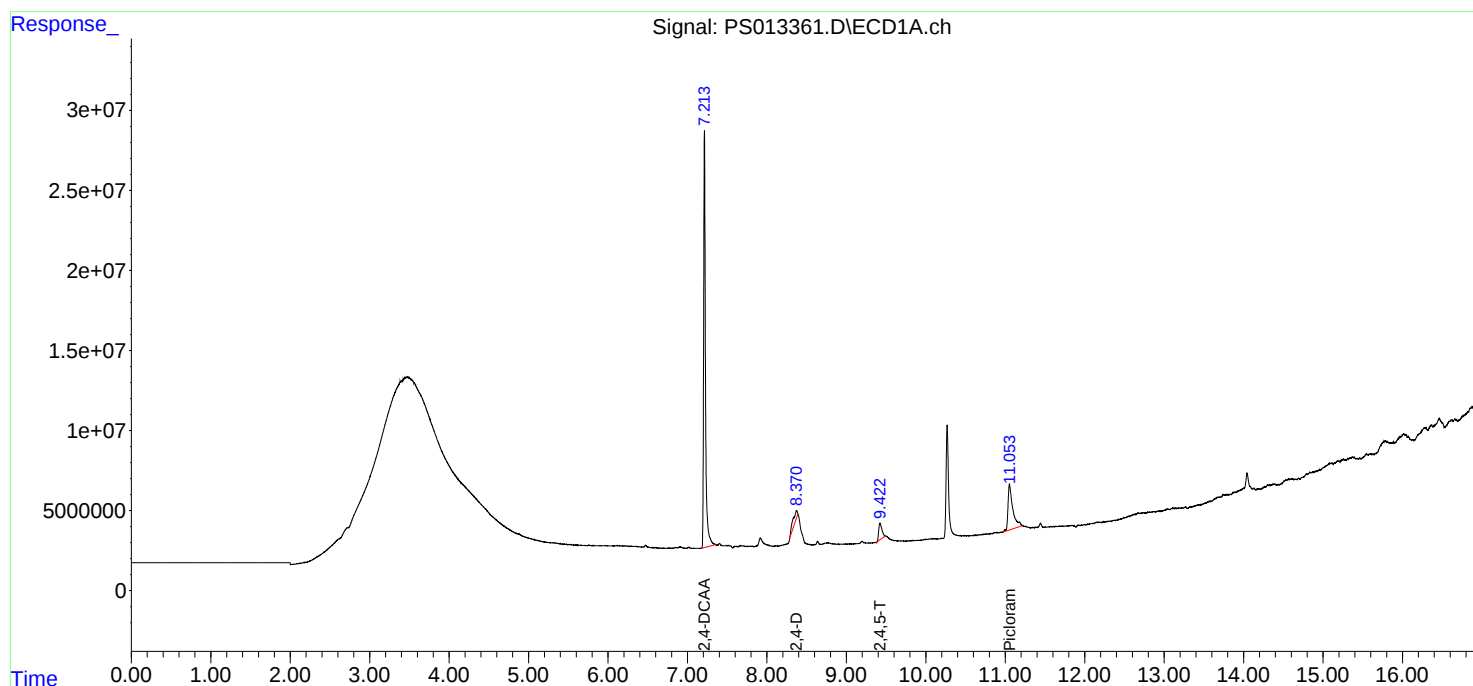


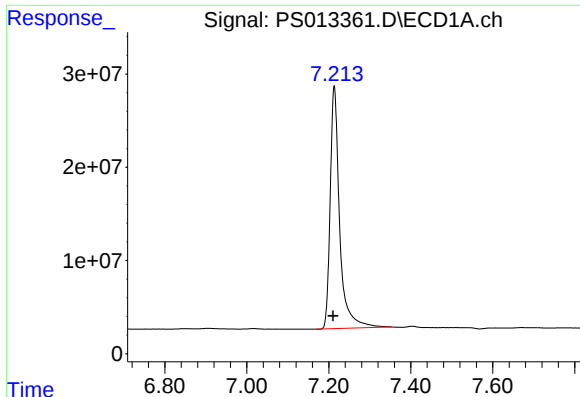

#4 2,4-DCAA


R.T.: 7.213 min
Delta R.T.: 0.003 min
Response: 416627020
Conc: 466.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

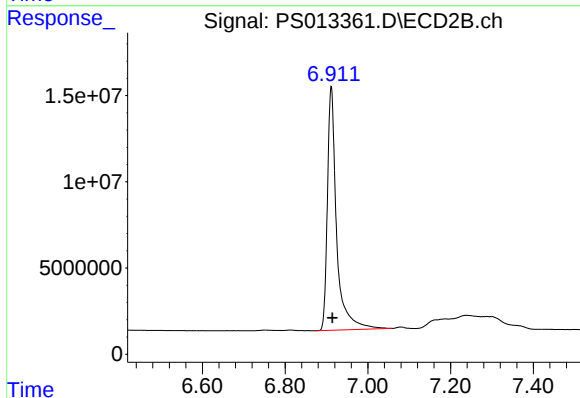


#4 2,4-DCAA

R.T.: 6.912 min
Delta R.T.: -0.002 min
Response: 218368027
Conc: 561.23 ng/ml

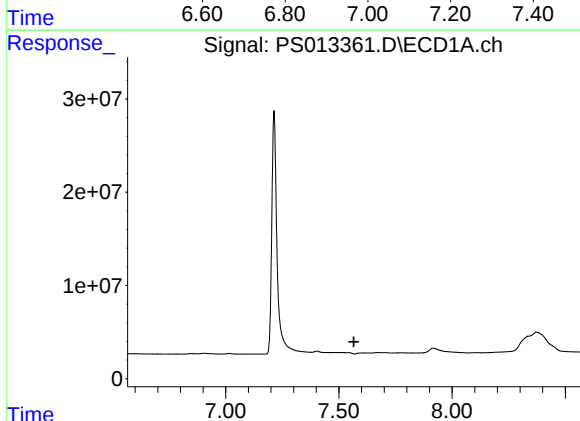


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.567 min
Response: 0
Conc: N.D.

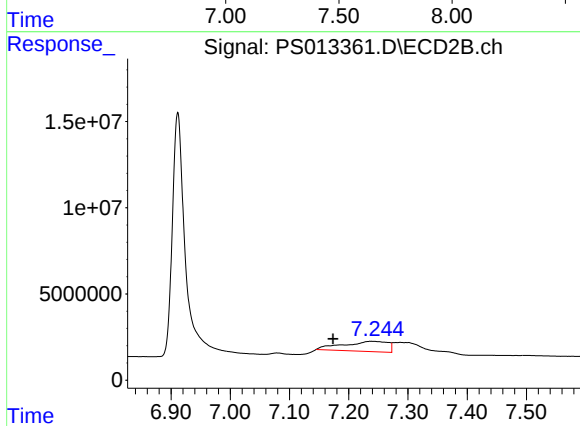

#6 MCP


R.T.: 7.237 min
Delta R.T.: 0.063 min
Response: 30785498
Conc: 23.26 ug/ml

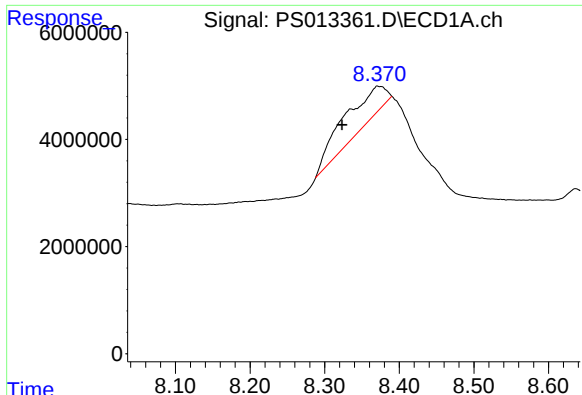

#9 2,4-D


R.T.: 8.370 min
Delta R.T.: 0.047 min
Response: 25679981
Conc: 27.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

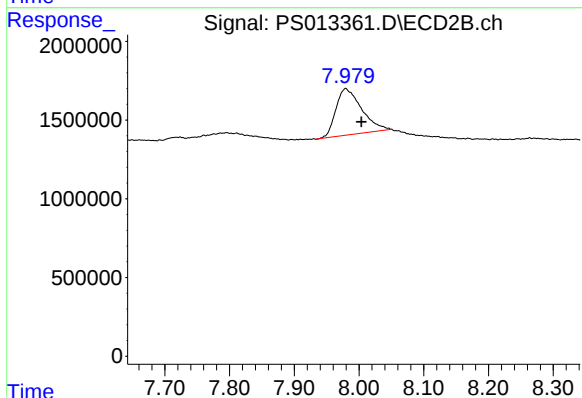


#9 2,4-D

R.T.: 7.979 min
Delta R.T.: -0.024 min
Response: 8103694
Conc: 15.27 ng/ml

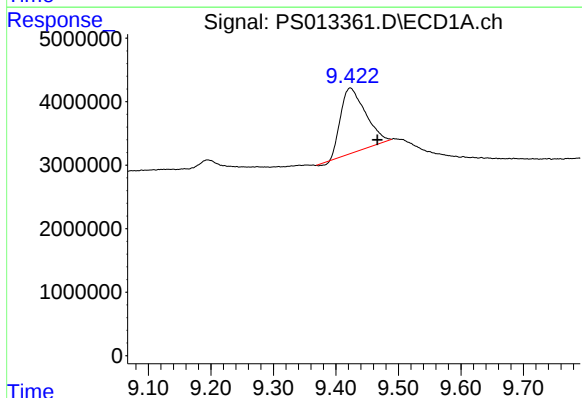


#12 2,4,5-T

R.T.: 9.423 min
Delta R.T.: -0.044 min
Response: 28138754
Conc: 5.32 ng/ml

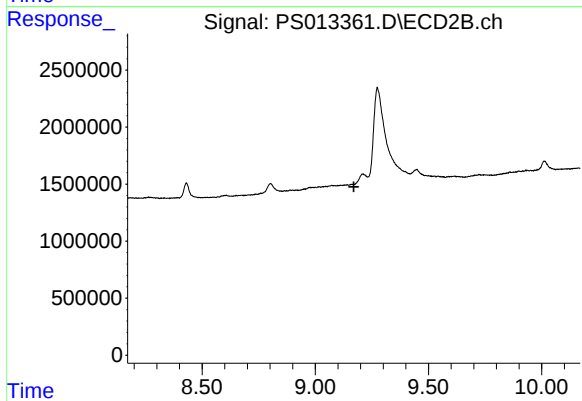

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.170 min
Response: 0
Conc: N.D.

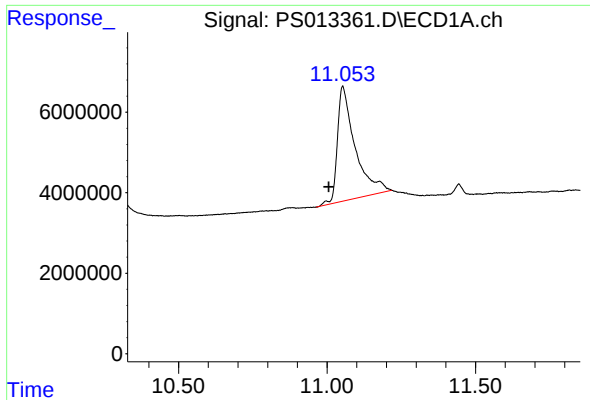

#15 Picloram

R.T.: 11.053 min
Delta R.T.: 0.047 min
Response: 118134631
Conc: 17.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

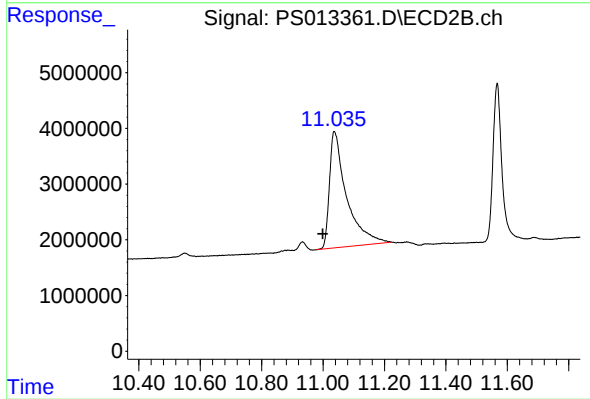

#15 Picloram

R.T.: 11.036 min
Delta R.T.: 0.037 min
Response: 80776285
Conc: 22.38 ng/ml