

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS113020\
 Data File : PS013372.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Nov 2020 21:02
 Operator : DD\AJ
 Sample : L4900-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 01 02:49:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110220.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 03 03:59:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.212	6.913	252.7E6	133.1E6	282.665	342.055
Target Compounds							
1) T	Dalapon	2.989f	2.590	84457284	119.8E6	79.826	225.973 #
2) T	3,5-DICHL...	0.000	6.044	0	1901503	N.D.	3.091
5) T	DICAMBA	7.386	7.045	7848467	4764375	2.198	2.870 #
6) T	MCP	0.000	7.123f	0	560400	N.D.	<MDL
7) T	MCPA	7.717	0.000	164.0E6	0	42.956	N.D. #
8) T	DICHLORPROP	0.000	7.748f	0	10413989	N.D.	23.300
10) T	Pentachlo...	8.683f	0.000	9184913	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	8.739f	0	17092922	N.D.	7.376
12) T	2,4,5-T	9.398f	0.000	39554158	0	7.474	N.D. #
15) T	Picloram	10.982	0.000	10058477	0	1.530	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS113020\
Data File : PS013372.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Nov 2020 21:02
Operator : DD\AJ
Sample : L4900-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 01 02:49:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110220.M
Quant Title : 8080.M
QLast Update : Tue Nov 03 03:59:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

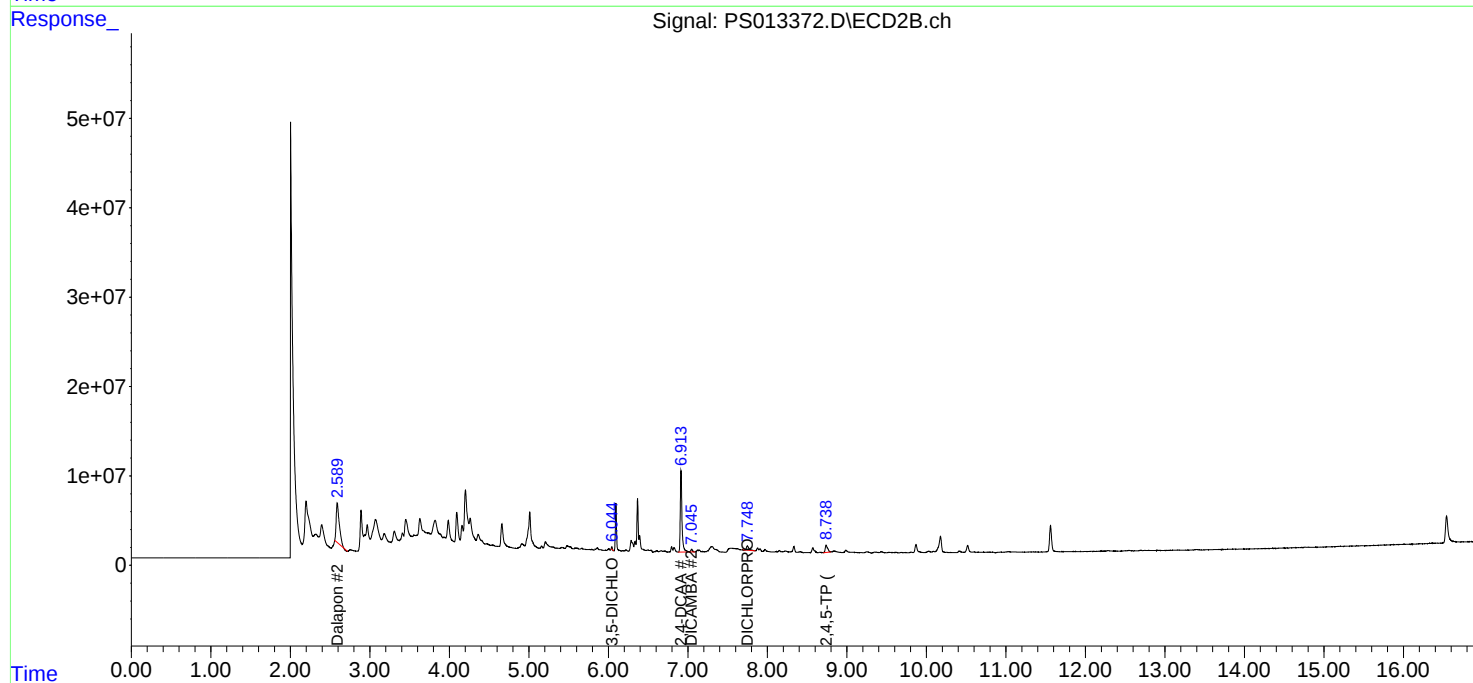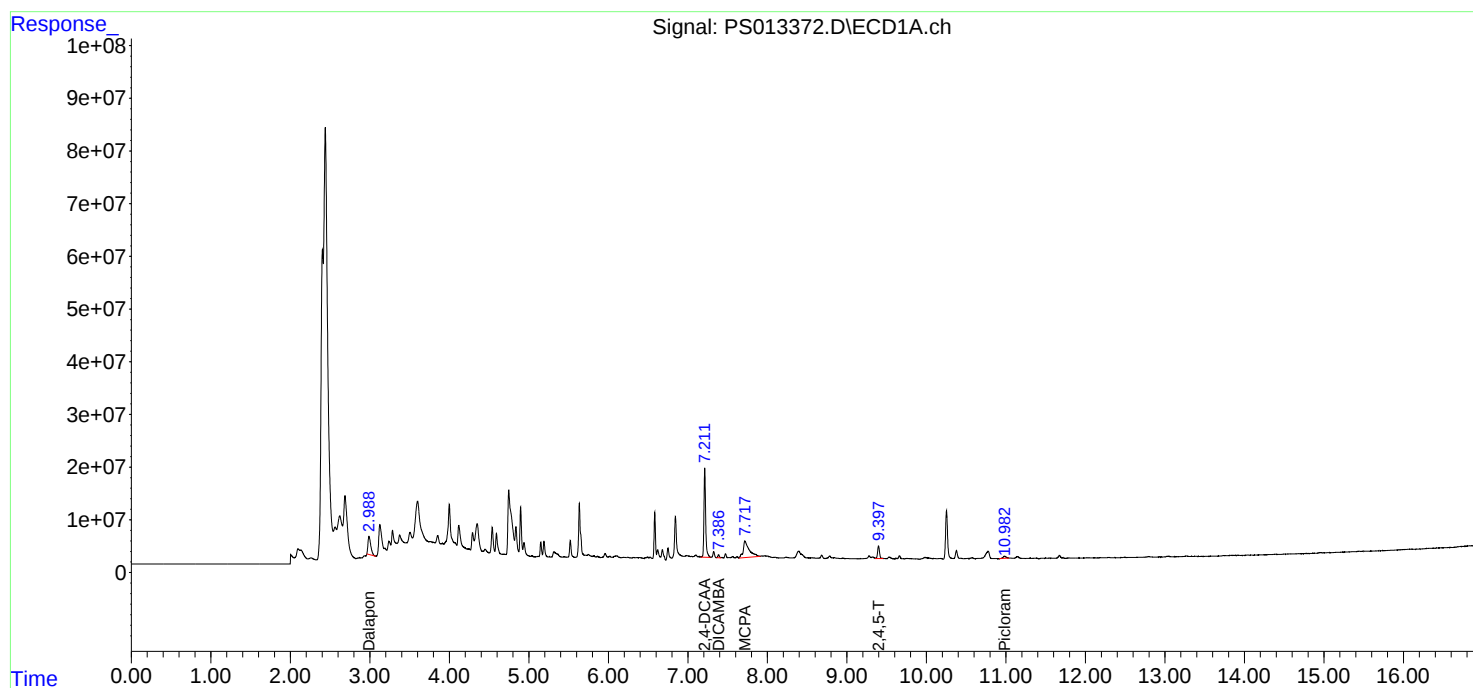


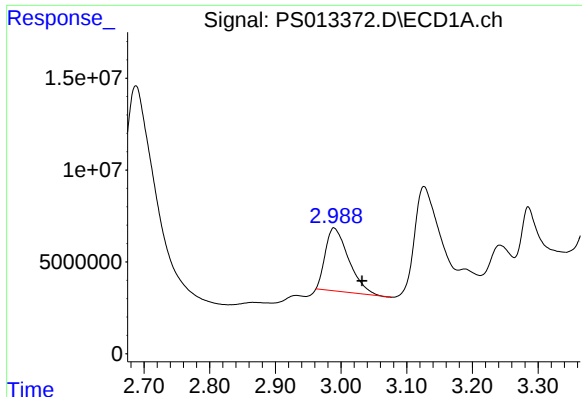

#1 Dalapon


R.T.: 2.989 min
Delta R.T.: -0.043 min
Response: 84457284
Conc: 79.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

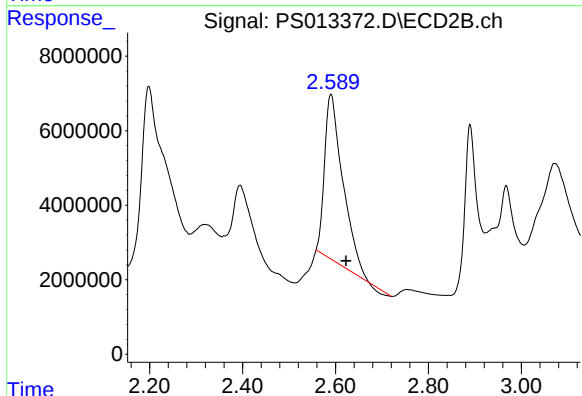


#1 Dalapon

R.T.: 2.590 min
Delta R.T.: -0.033 min
Response: 119760084
Conc: 225.97 ng/ml

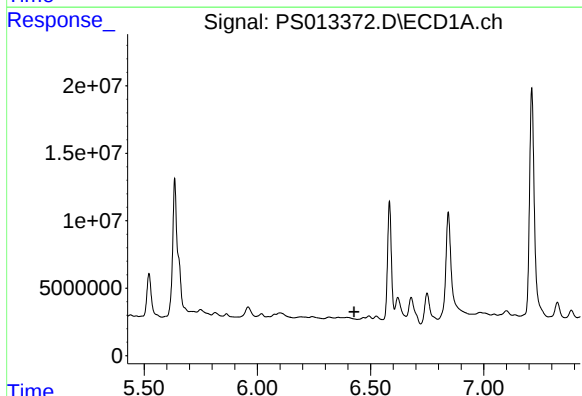


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.427 min
Response: 0
Conc: N.D.

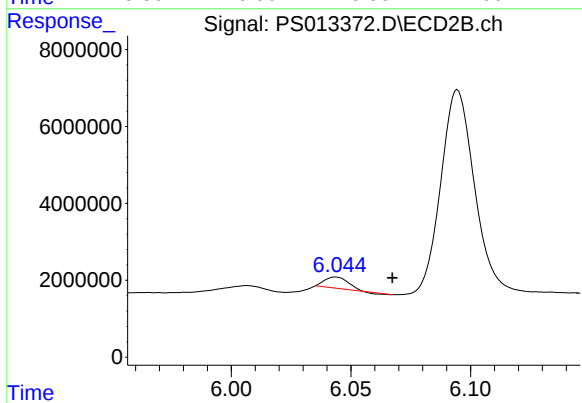

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.044 min
Delta R.T.: -0.024 min
Response: 1901503
Conc: 3.09 ng/ml

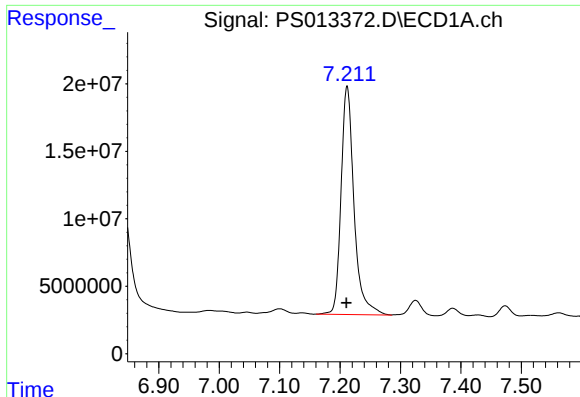

#4 2,4-DCAA


R.T.: 7.212 min
Delta R.T.: 0.001 min
Response: 252682214
Conc: 282.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

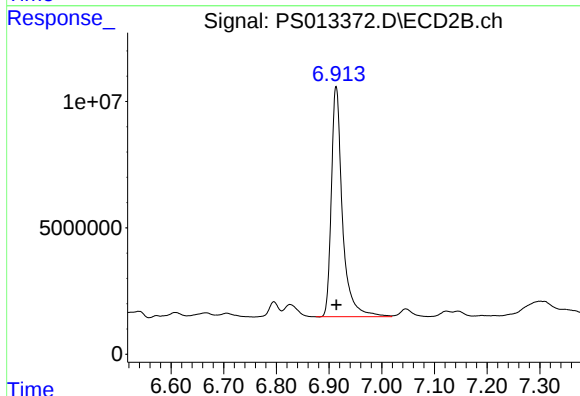


#4 2,4-DCAA

R.T.: 6.913 min
Delta R.T.: 0.000 min
Response: 133090089
Conc: 342.06 ng/ml

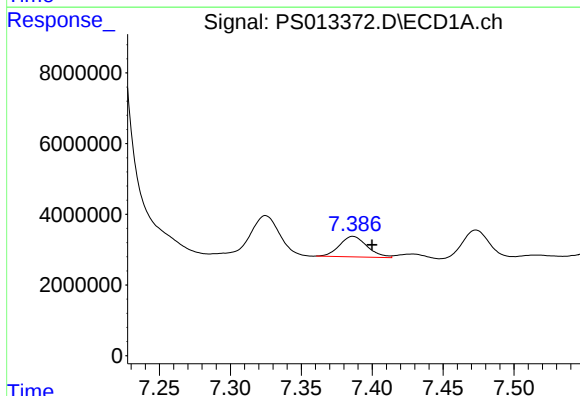


#5 DICAMBA

R.T.: 7.386 min
Delta R.T.: -0.013 min
Response: 7848467
Conc: 2.20 ng/ml

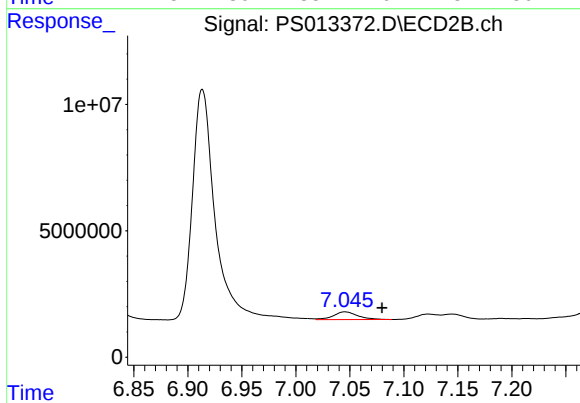

#5 DICAMBA


R.T.: 7.045 min
Delta R.T.: -0.035 min
Response: 4764375
Conc: 2.87 ng/ml

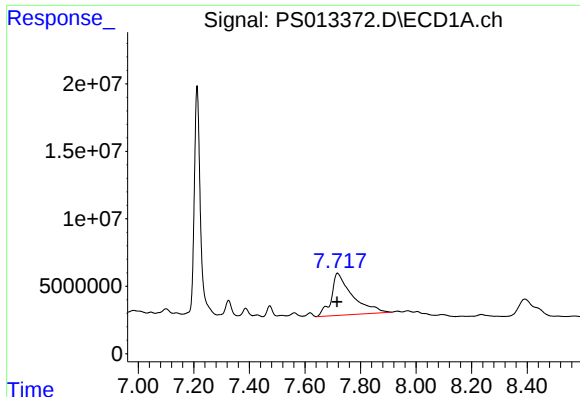

#7 MCPA


R.T.: 7.717 min
Delta R.T.: 0.001 min
Response: 164024164
Conc: 42.96 ug/ml

Instrument :
ECD_S
ClientSampleId :

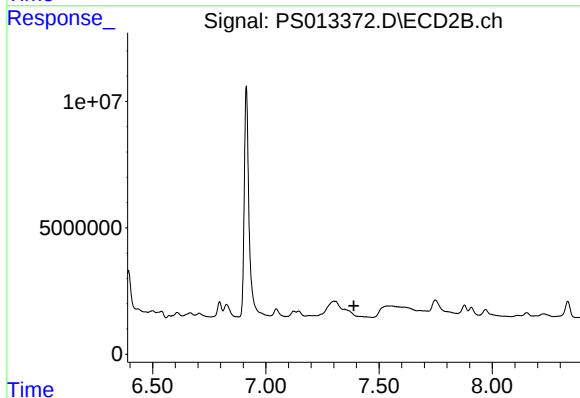


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.389 min
Response: 0
Conc: N.D.

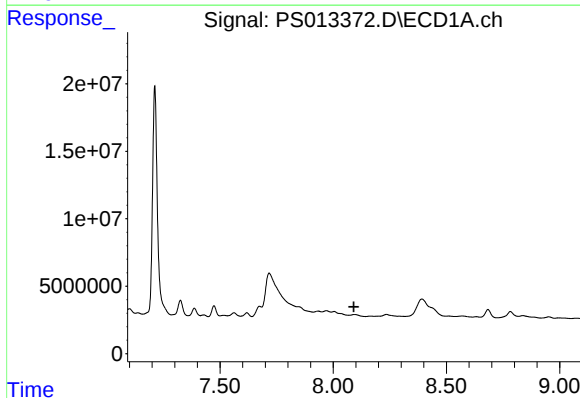


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.092 min
Response: 0
Conc: N.D.

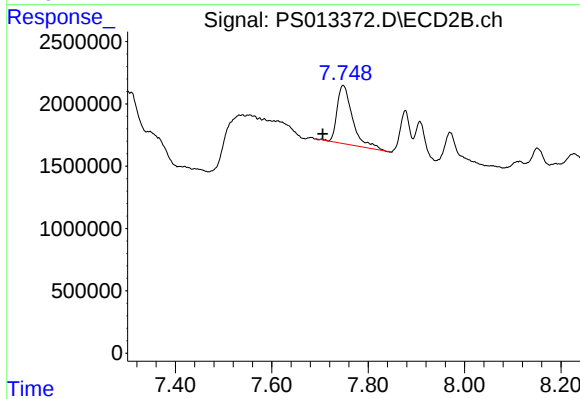

#8 DICHLORPROP


R.T.: 7.748 min
Delta R.T.: 0.043 min
Response: 10413989
Conc: 23.30 ng/ml

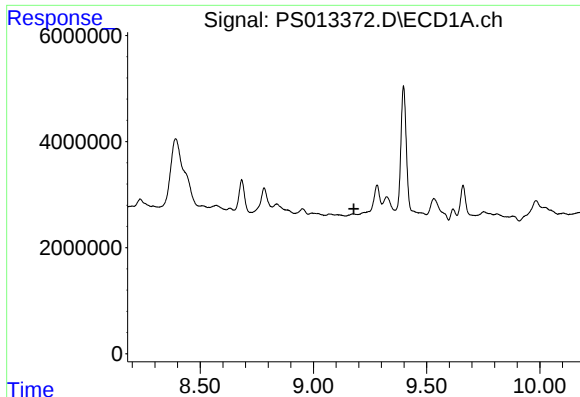

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.179 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

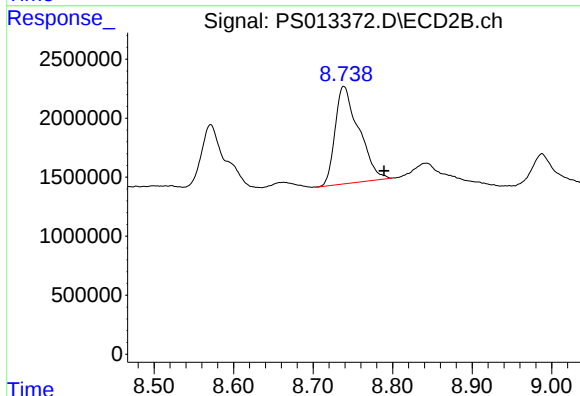


#11 2,4,5-TP (SILVEX)

R.T.: 8.739 min
Delta R.T.: -0.051 min
Response: 17092922
Conc: 7.38 ng/ml

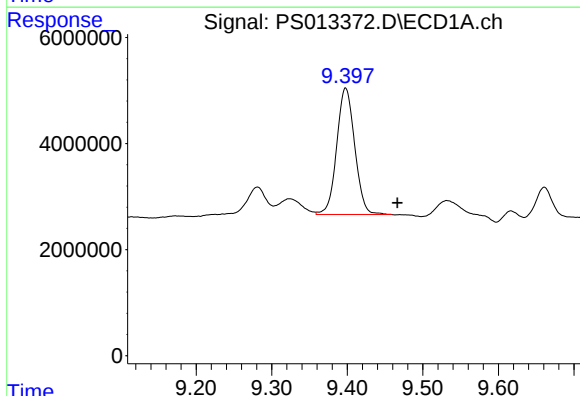


#12 2,4,5-T

R.T.: 9.398 min
Delta R.T.: -0.069 min
Response: 39554158
Conc: 7.47 ng/ml

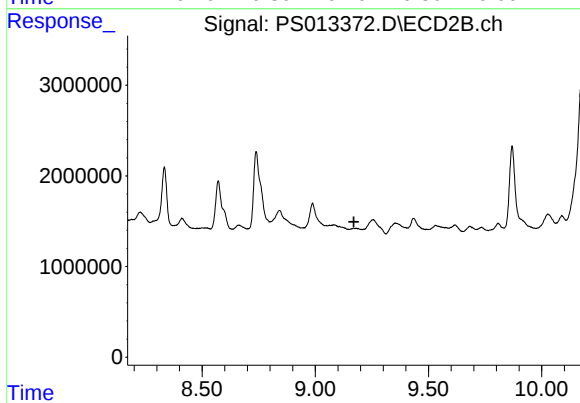

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.170 min
Response: 0
Conc: N.D.

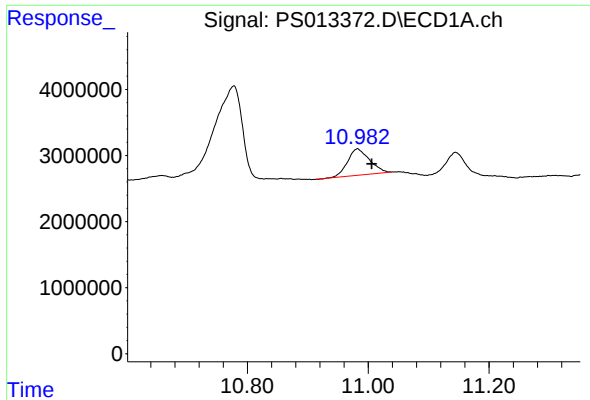

#15 Picloram

R.T.: 10.982 min
Delta R.T.: -0.024 min
Response: 10058477
Conc: 1.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

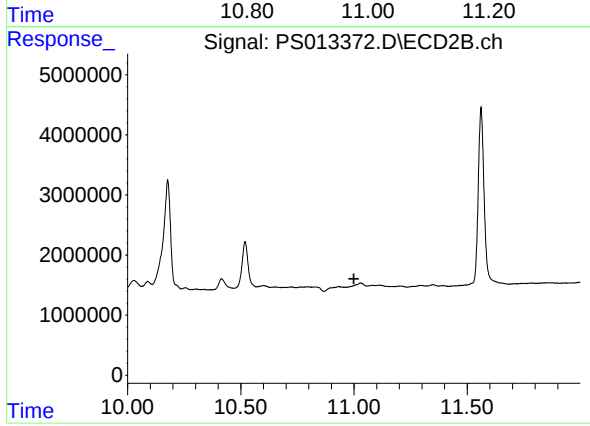

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.999 min
Response: 0
Conc: N.D.