

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS113020\
 Data File : PS013376.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Nov 2020 22:34
 Operator : DD\AJ
 Sample : L4903-08
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 01 02:50:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110220.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 03 03:59:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.212	6.914	263.6E6	139.6E6	294.842	358.668
Target Compounds							
1) T	Dalapon	2.990f	2.589	85217713	115.0E6	80.545	217.067 #
2) T	3,5-DICHL...	0.000	6.095	0	40691792	N.D.	66.147
5) T	DICAMBA	7.387	7.046	7325828	4447621	2.051	2.679 #
7) T	MCPA	7.723	0.000	145.7E6	0	38.163	N.D. #
8) T	DICHLORPROP	0.000	7.747f	0	10977676	N.D.	24.561
9) T	2,4-D	0.000	7.970	0	4376525	N.D.	8.247
10) T	Pentachlo...	8.684f	0.000	10619379	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	8.738f	0	17432443	N.D.	7.522
12) T	2,4,5-T	9.398f	0.000	34757059	0	6.568	N.D. #
15) T	Picloram	10.982	0.000	8396746	0	1.277	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS113020\
Data File : PS013376.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Nov 2020 22:34
Operator : DD\AJ
Sample : L4903-08
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 01 02:50:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110220.M
Quant Title : 8080.M
QLast Update : Tue Nov 03 03:59:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

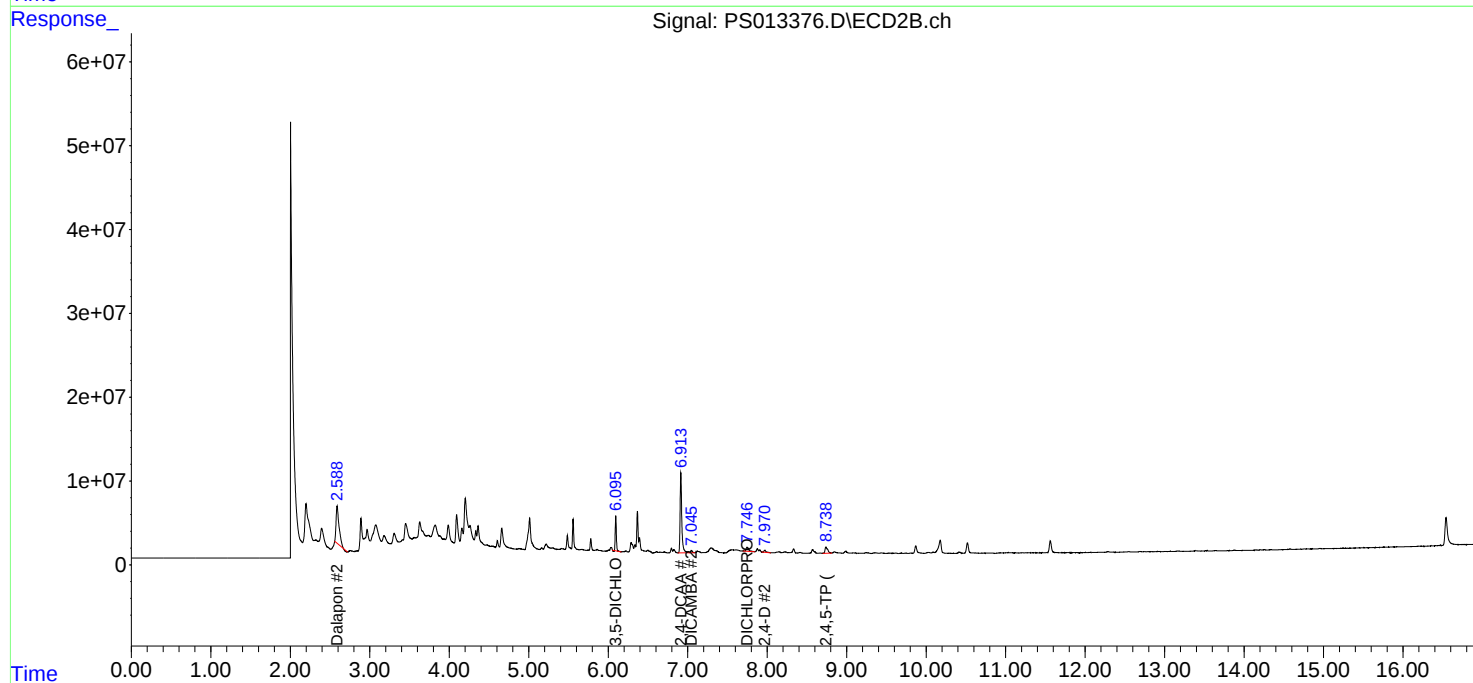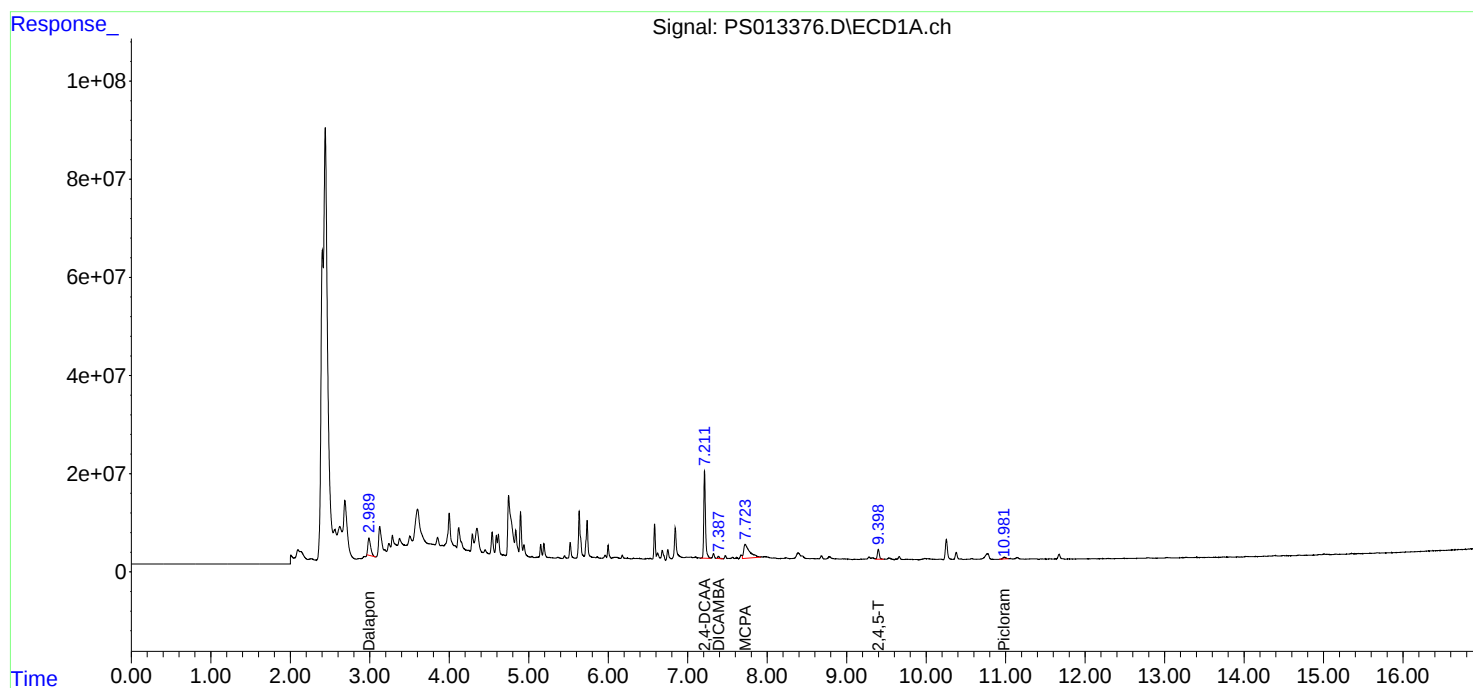


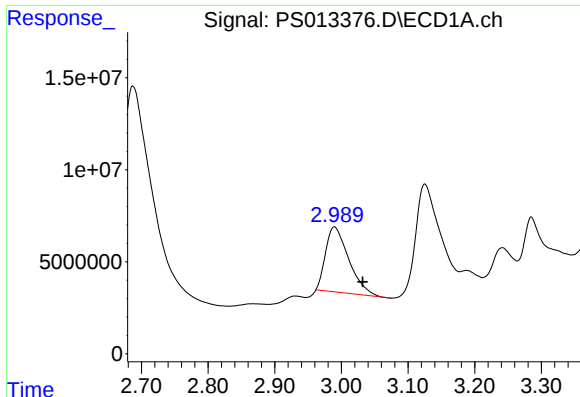

#1 Dalapon


R.T.: 2.990 min
Delta R.T.: -0.042 min
Response: 85217713
Conc: 80.55 ng/ml

Instrument :
ECD_S
ClientSampleId :

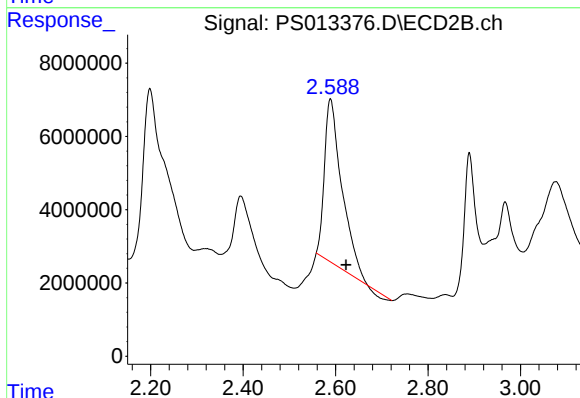


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.034 min
Response: 115040251
Conc: 217.07 ng/ml

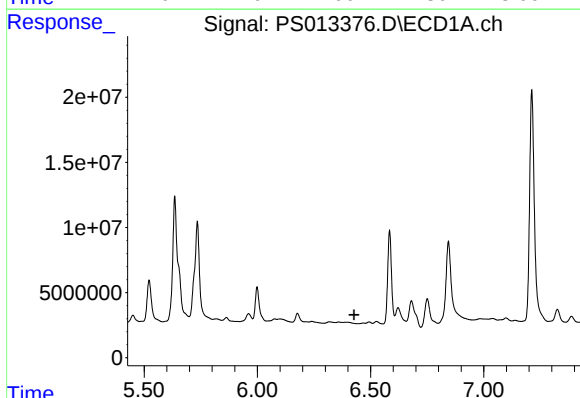


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.427 min
Response: 0
Conc: N.D.

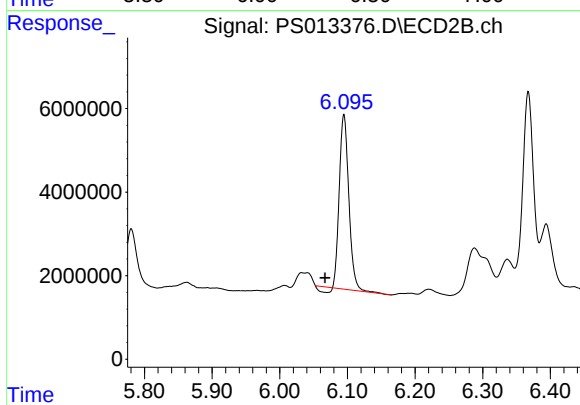

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.095 min
Delta R.T.: 0.028 min
Response: 40691792
Conc: 66.15 ng/ml

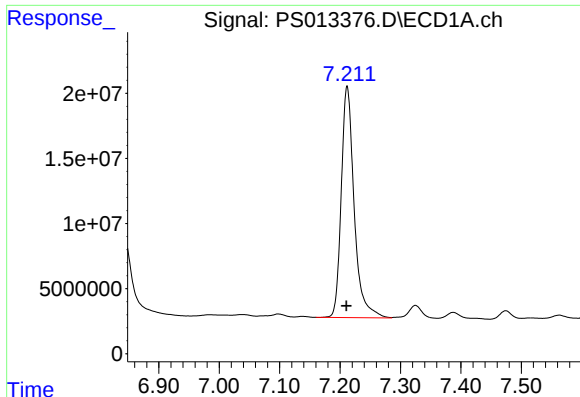

#4 2,4-DCAA


R.T.: 7.212 min
Delta R.T.: 0.001 min
Response: 263567785
Conc: 294.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

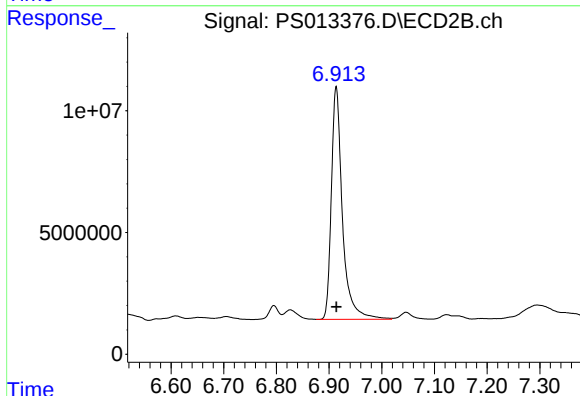


#4 2,4-DCAA

R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 139554038
Conc: 358.67 ng/ml

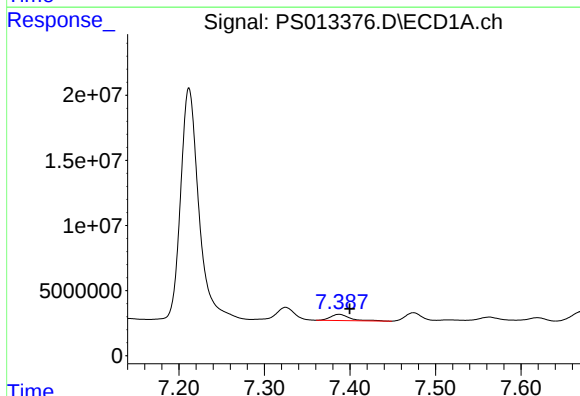


#5 DICAMBA

R.T.: 7.387 min
Delta R.T.: -0.013 min
Response: 7325828
Conc: 2.05 ng/ml

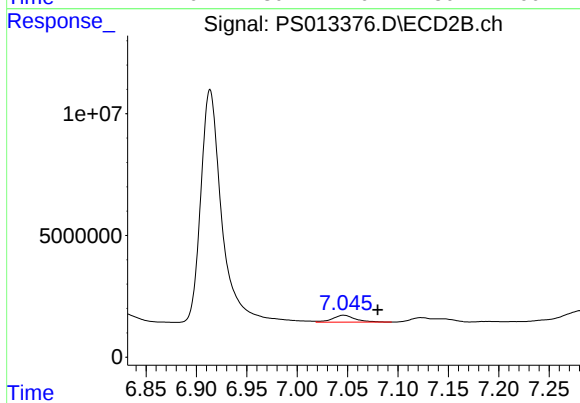

#5 DICAMBA


R.T.: 7.046 min
Delta R.T.: -0.034 min
Response: 4447621
Conc: 2.68 ng/ml

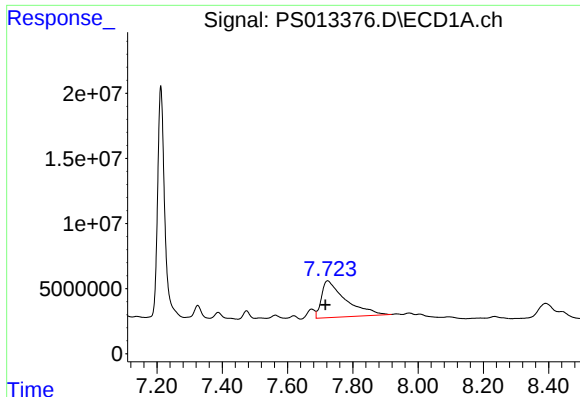

#7 MCPA


R.T.: 7.723 min
Delta R.T.: 0.007 min
Response: 145723987
Conc: 38.16 ug/ml

Instrument :
ECD_S
ClientSampleId :

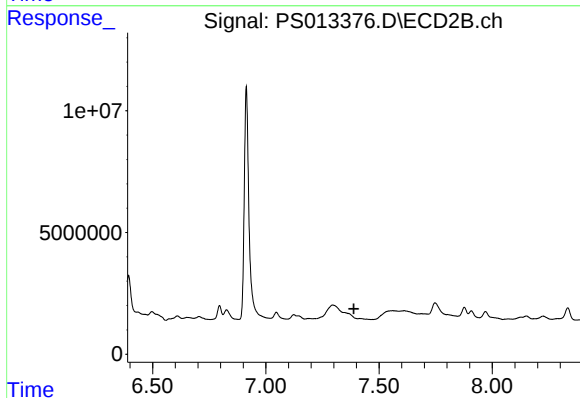


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.389 min
Response: 0
Conc: N.D.

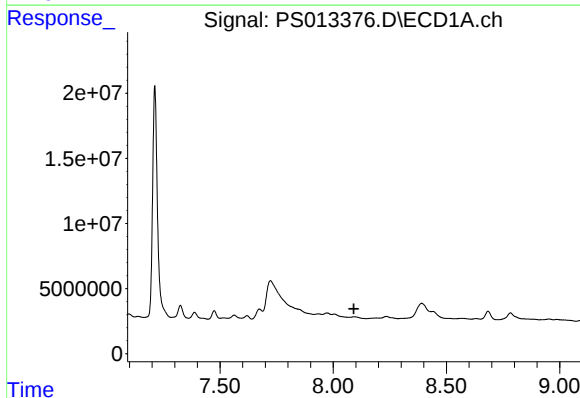


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.092 min
Response: 0
Conc: N.D.

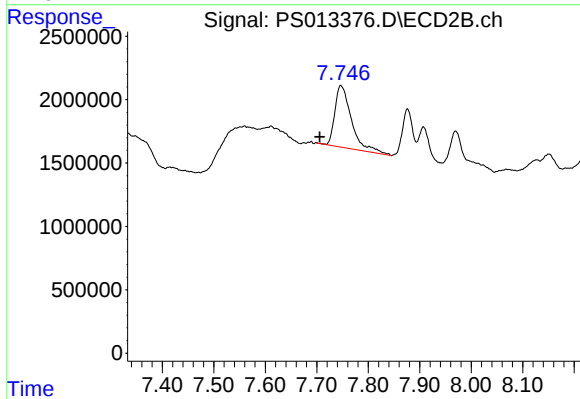

#8 DICHLORPROP


R.T.: 7.747 min
Delta R.T.: 0.041 min
Response: 10977676
Conc: 24.56 ng/ml

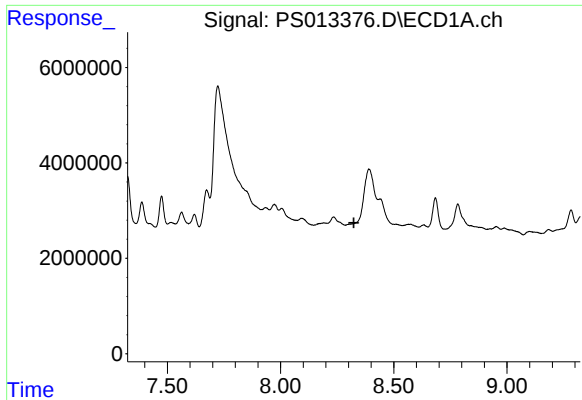

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.324 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

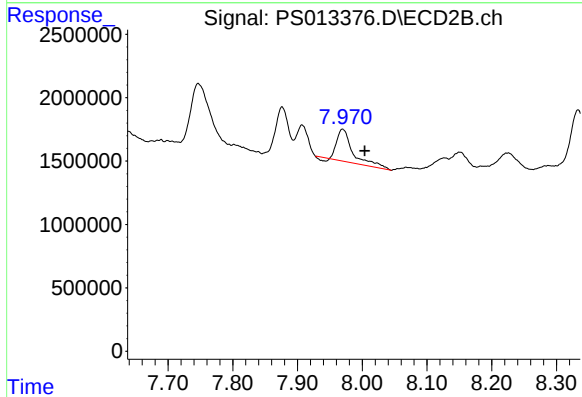


#9 2,4-D

R.T.: 7.970 min
Delta R.T.: -0.034 min
Response: 4376525
Conc: 8.25 ng/ml

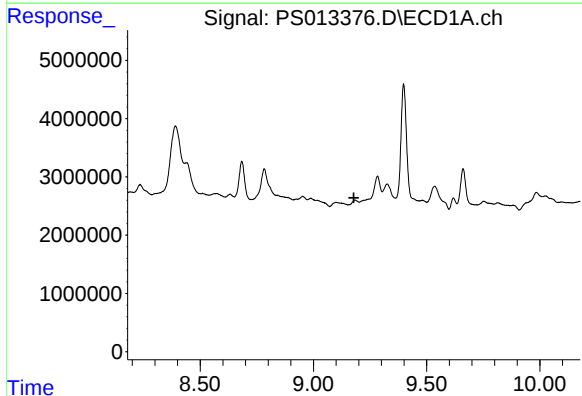


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.179 min
Response: 0
Conc: N.D.

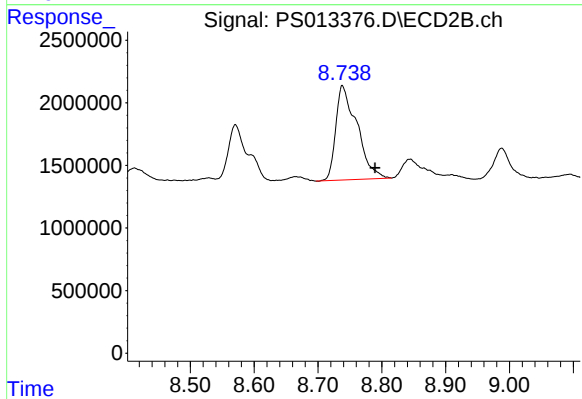

#11 2,4,5-TP (SILVEX)


R.T.: 8.738 min
Delta R.T.: -0.051 min
Response: 17432443
Conc: 7.52 ng/ml

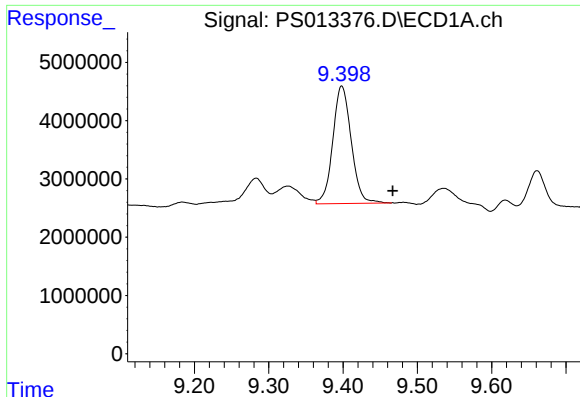

#12 2,4,5-T


R.T.: 9.398 min
Delta R.T.: -0.068 min
Response: 34757059
Conc: 6.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

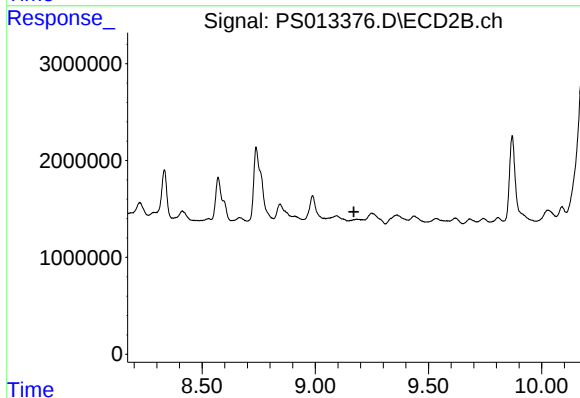


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.170 min
Response: 0
Conc: N.D.

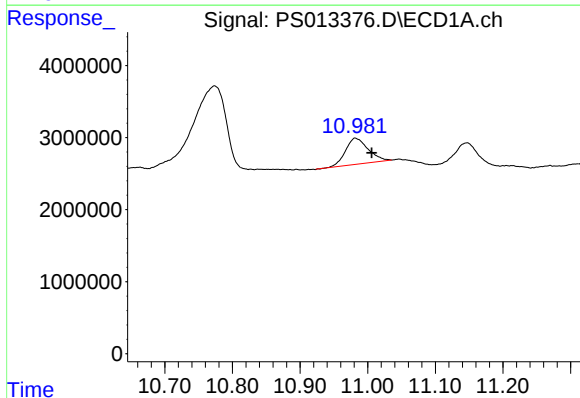

#15 Picloram

R.T.: 10.982 min
Delta R.T.: -0.024 min
Response: 8396746
Conc: 1.28 ng/ml

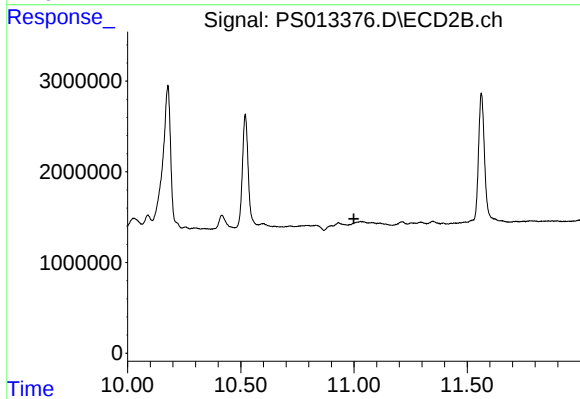

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.999 min
Response: 0
Conc: N.D.