

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS113020\
 Data File : PS013353.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Nov 2020 11:11
 Operator : DD\AJ
 Sample : L4880-08
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 KENS-B4-112320-6-8

Manual Integrations
 APPROVED

Ankita
 12/1/2020 9:52:43 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 13:55:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110220.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 03 03:59:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.213	6.909	279.3E6	134.5E6	312.451m	345.561m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS113020\
Data File : PS013353.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Nov 2020 11:11
Operator : DD\AJ
Sample : L4880-08
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
KENS-B4-112320-6-8


Manual Integrations
APPROVED

Ankita
12/1/2020 9:52:43 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 13:55:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110220.M
Quant Title : 8080.M
QLast Update : Tue Nov 03 03:59:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

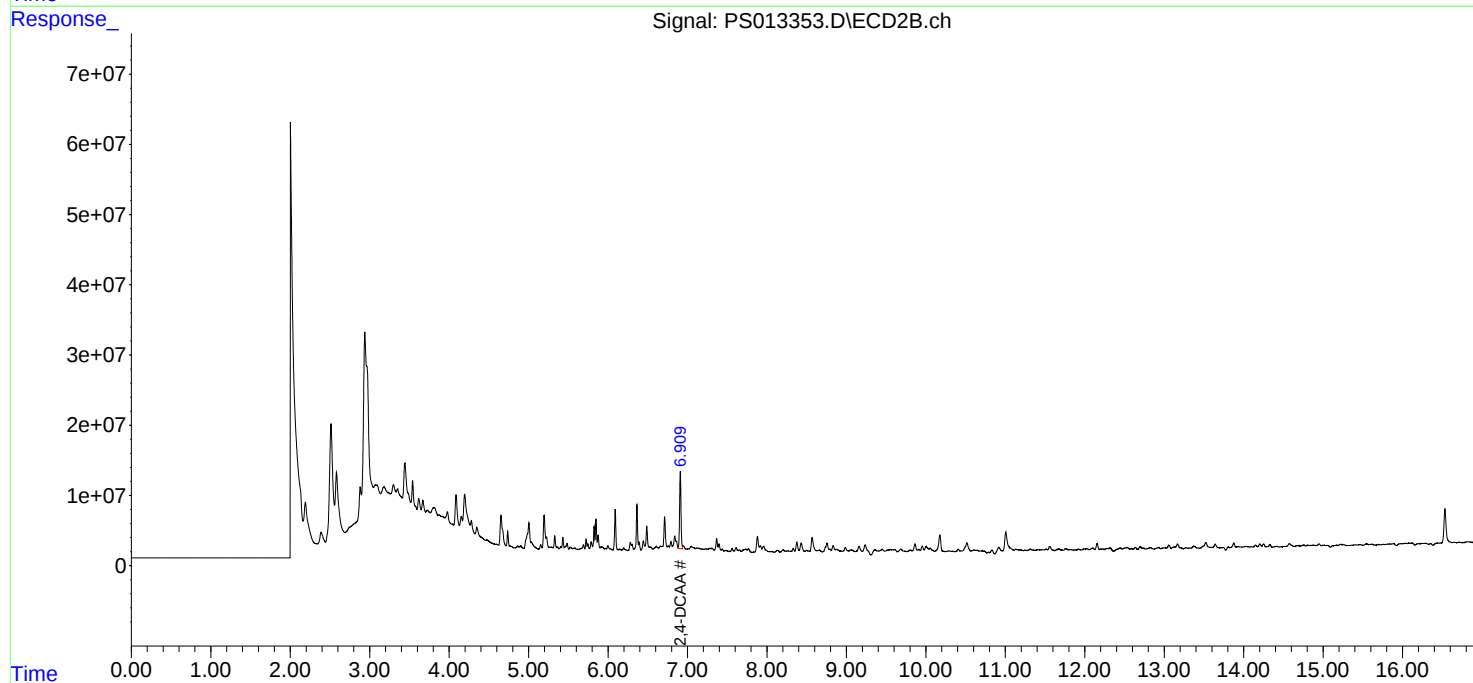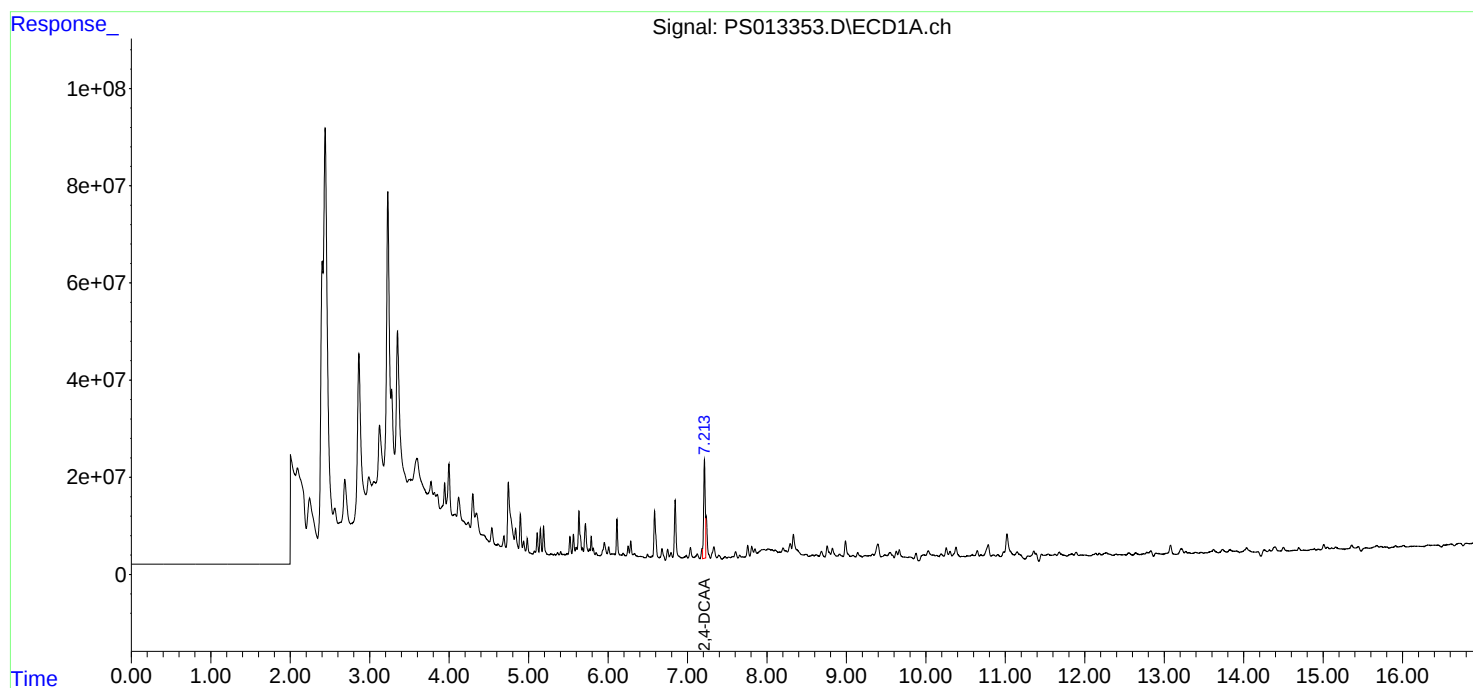

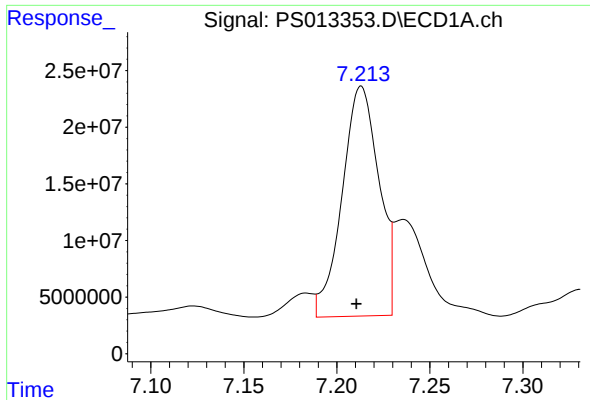


#4 2,4-DCAA

R.T.: 7.213 min
Delta R.T.: 0.002 min
Response: 279308656
Conc: 312.45 ng/ml m

Instrument :
ECD_S
ClientSampleId :
KENS-B4-112320-6-8

Manual Integrations
APPROVED

Ankita
12/1/2020 9:52:43 AM

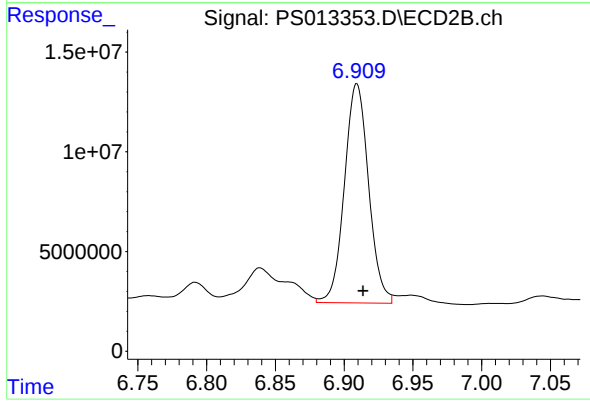

#4 2,4-DCAA

R.T.: 6.909 min
Delta R.T.: -0.005 min
Response: 134453918
Conc: 345.56 ng/ml m