

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS113023\
 Data File : PS024982.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Nov 2023 09:17
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 23:27:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	6.394	0.000	4403030	0	1.968	N.D.	#
Target Compounds								
1) T	Dalapon	2.510	2.564	10672145	6493631	3.701	5.661	#
2) T	3,5-DICHL...	5.697	0.000	2557326	0	<MDL	N.D.	#
3) T	4-Nitroph...	0.000	6.371	0	379924	N.D.	<MDL	
5) T	DICAMBA	0.000	6.973f	0	7197733	N.D.	2.323	
6) T	MCP	6.682	6.973f	1728152	7197733	<MDL	3.470	#
7) T	MCPA	0.000	7.183f	0	18847447	N.D.	5.730	
8) T	DICHLORPROP	0.000	7.558	0	2969744	N.D.	3.775	
9) T	2,4-D	7.247	7.769f	33207225	864255	10.933	<MDL	#
11) T	2,4,5-TP ...	0.000	8.608	0	115445	N.D.	<MDL	
12) T	2,4,5-T	0.000	8.982	0	816912	N.D.	<MDL	
13) T	2,4-DB	0.000	9.473	0	1318001	N.D.	2.381	
15) T	Picloram	9.682	10.763	48653806	15928066	2.497	2.434	
16) T	DCPA	0.000	10.763	0	15928066	N.D.	2.939	



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS113023\
Data File : PS024982.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Nov 2023 09:17
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 23:27:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

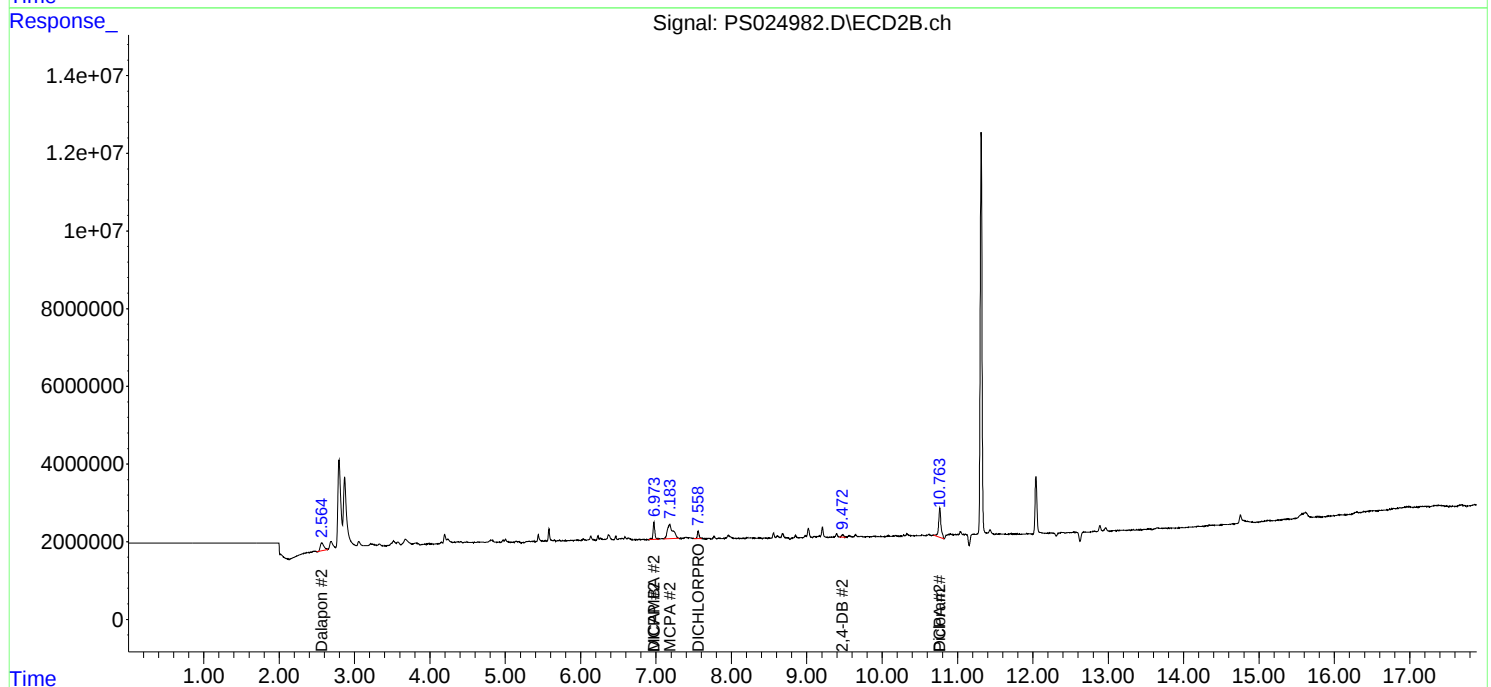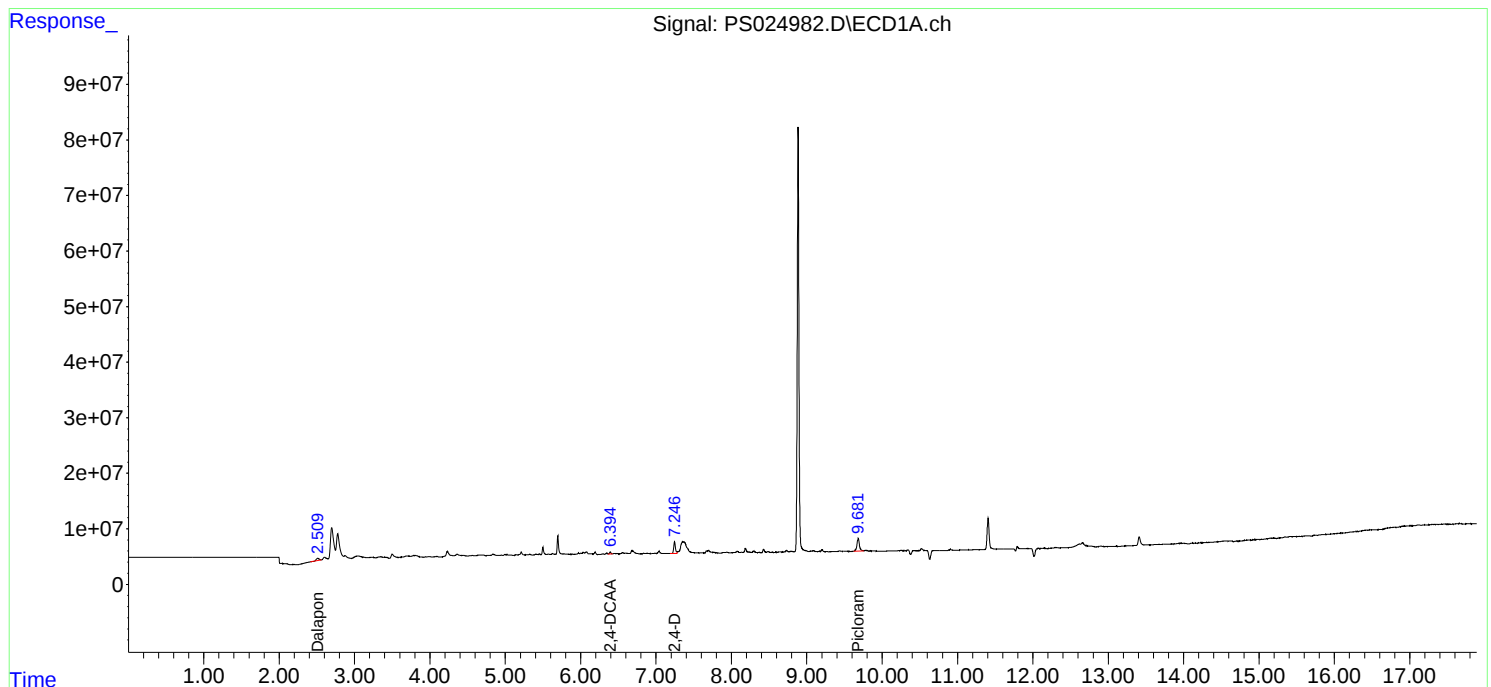


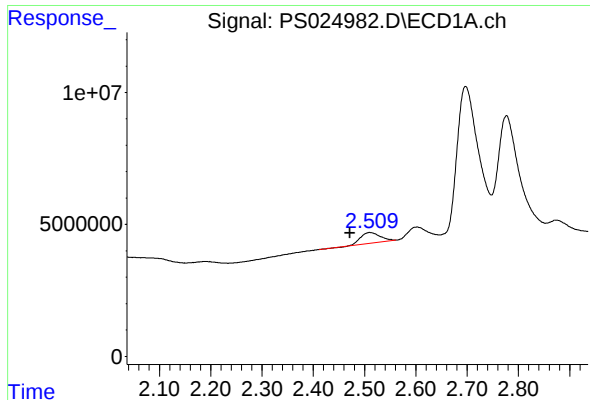

#1 Dalapon


R.T.: 2.510 min
Delta R.T.: 0.038 min
Response: 10672145
Conc: 3.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

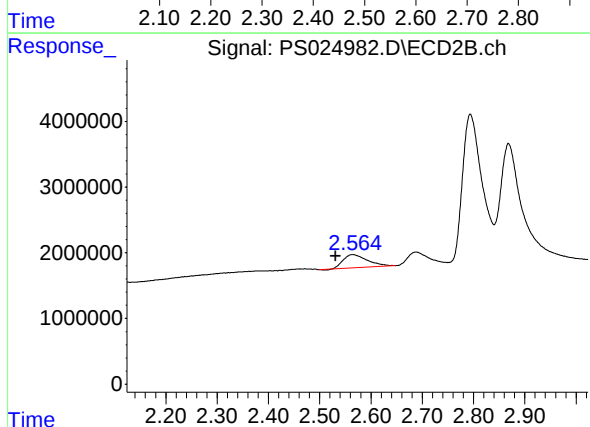


#1 Dalapon

R.T.: 2.564 min
Delta R.T.: 0.033 min
Response: 6493631
Conc: 5.66 ng/ml

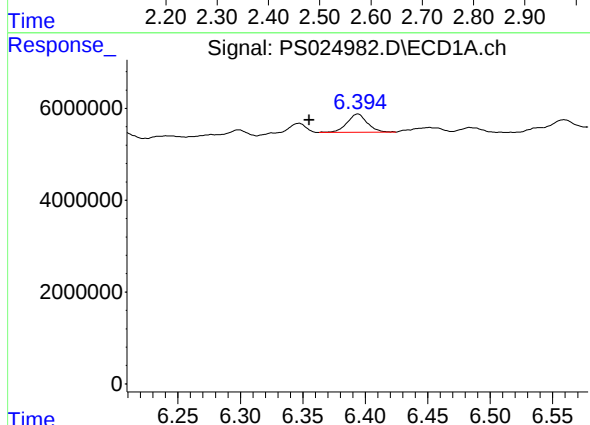


#4 2,4-DCAA

R.T.: 6.394 min
Delta R.T.: 0.039 min
Response: 4403030
Conc: 1.97 ng/ml

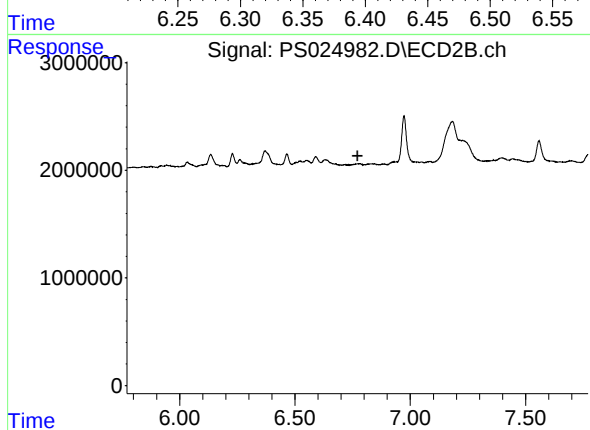

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 6.771 min
Response: 0
Conc: N.D.

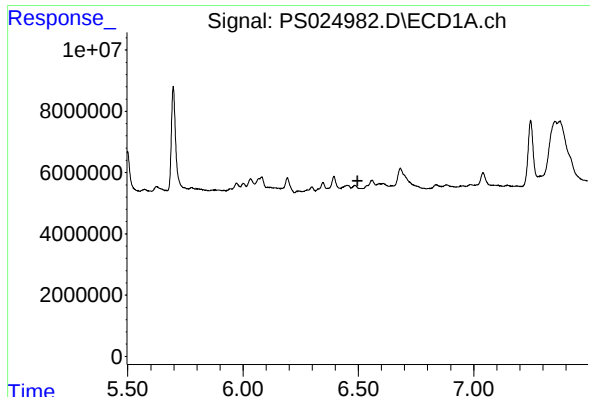

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.496 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

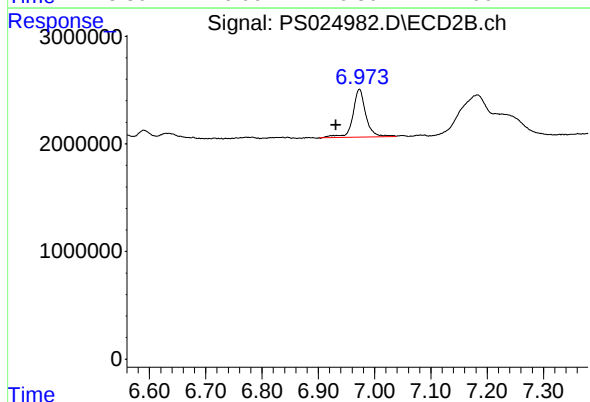


#5 DICAMBA

R.T.: 6.973 min
Delta R.T.: 0.041 min
Response: 7197733
Conc: 2.32 ng/ml

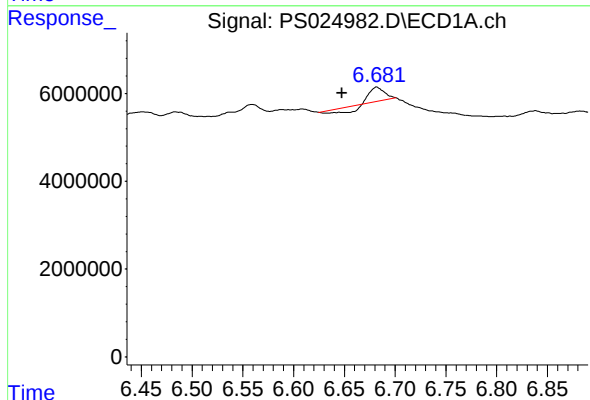


#6 MCPP

R.T.: 6.682 min
Delta R.T.: 0.034 min
Response: 1728152
Conc: N.D.

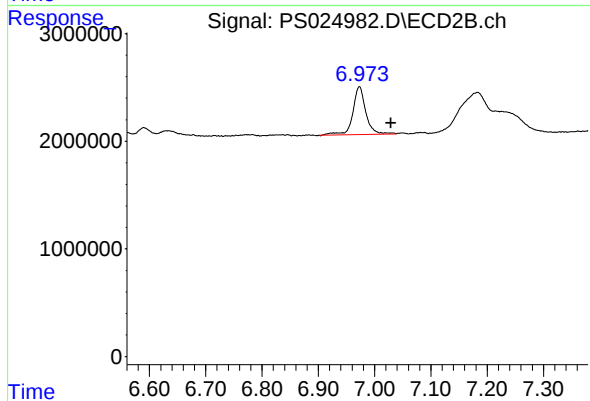

#6 MCPP


R.T.: 6.973 min
Delta R.T.: -0.057 min
Response: 7197733
Conc: 3.47 ug/ml

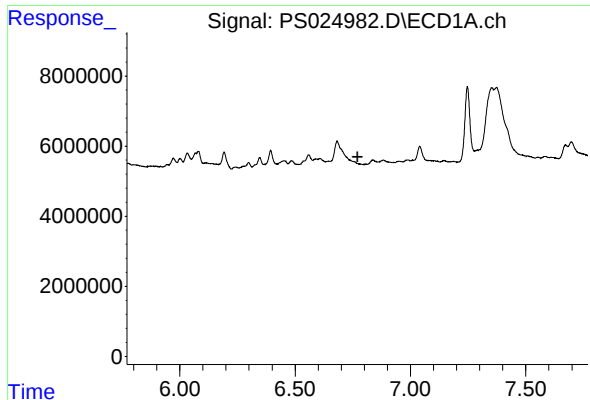

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.771 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

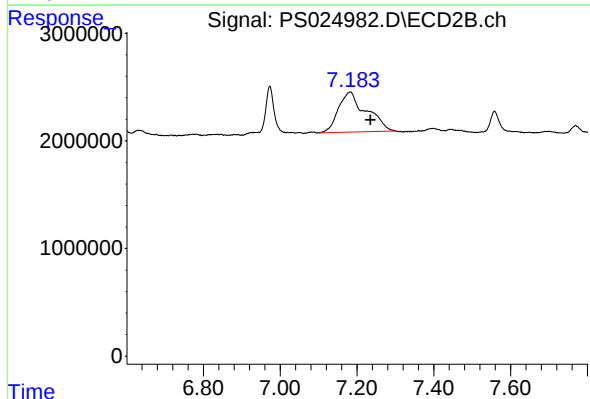


#7 MCPA

R.T.: 7.183 min
Delta R.T.: -0.052 min
Response: 18847447
Conc: 5.73 ug/ml

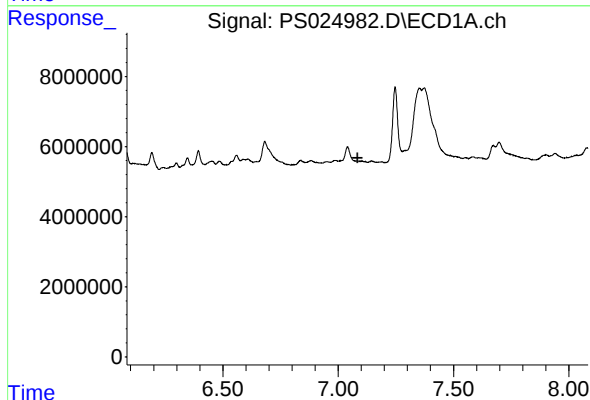


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

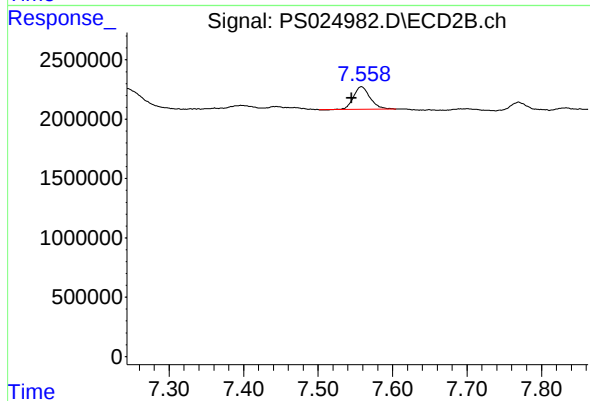

#8 DICHLORPROP


R.T.: 7.558 min
Delta R.T.: 0.013 min
Response: 2969744
Conc: 3.78 ng/ml

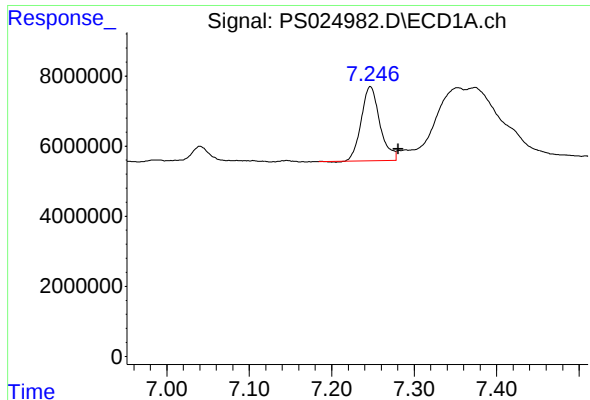

#9 2,4-D


R.T.: 7.247 min
Delta R.T.: -0.034 min
Response: 33207225
Conc: 10.93 ng/ml

Instrument :
ECD_S
ClientSampleId :

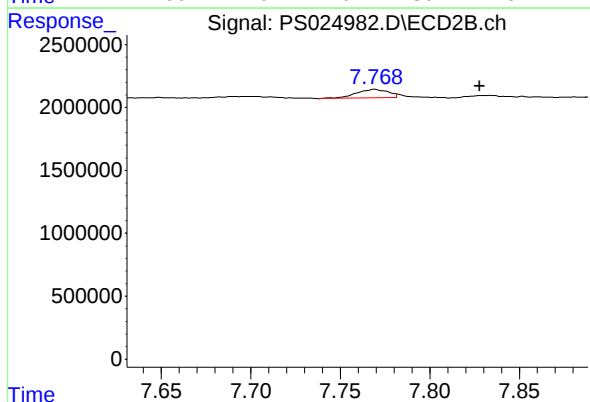


#9 2,4-D

R.T.: 7.769 min
Delta R.T.: -0.059 min
Response: 864255
Conc: N.D.

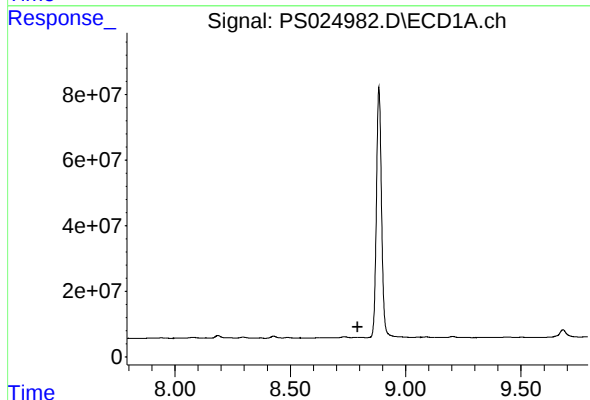


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.791 min
Response: 0
Conc: N.D.

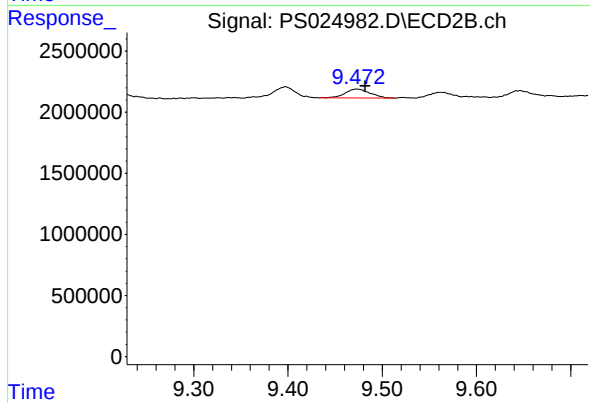

#13 2,4-DB


R.T.: 9.473 min
Delta R.T.: -0.009 min
Response: 1318001
Conc: 2.38 ng/ml

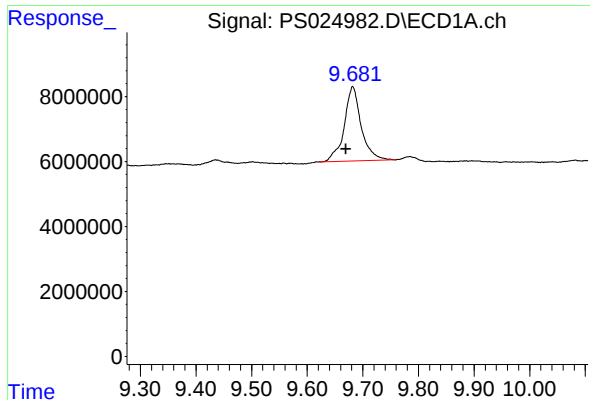

#15 Picloram


R.T.: 9.682 min
Delta R.T.: 0.012 min
Response: 48653806
Conc: 2.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

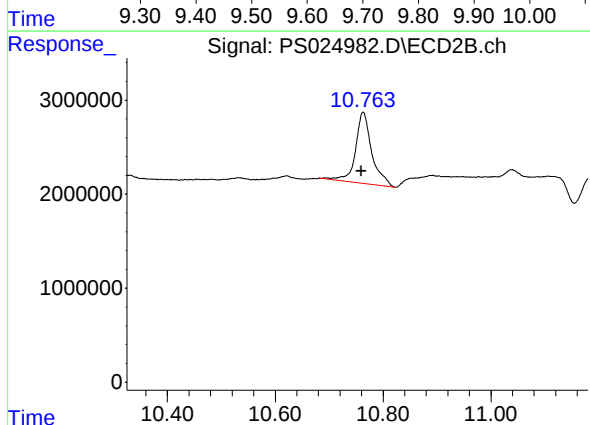


#15 Picloram

R.T.: 10.763 min
Delta R.T.: 0.003 min
Response: 15928066
Conc: 2.43 ng/ml

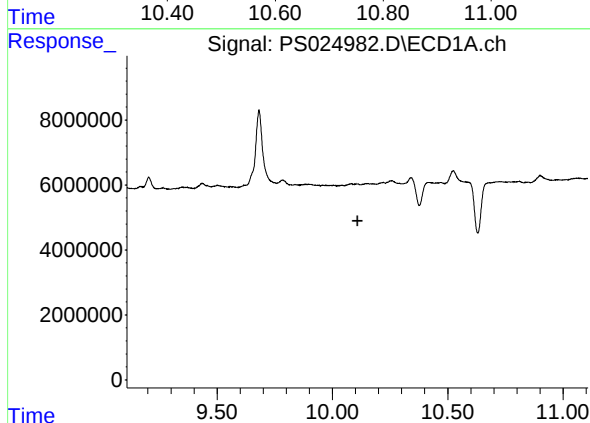

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.109 min
Response: 0
Conc: N.D.

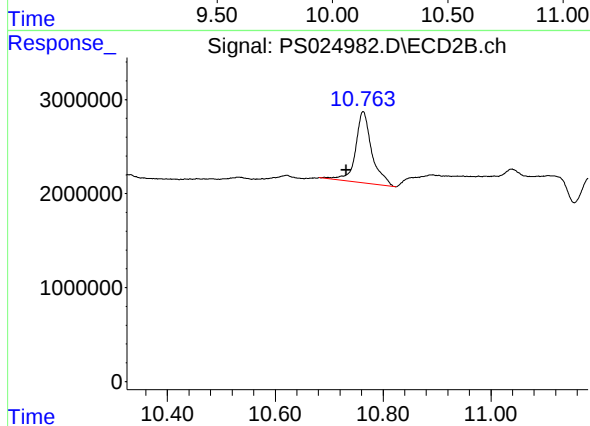

#16 DCPA

R.T.: 10.763 min
Delta R.T.: 0.031 min
Response: 15928066
Conc: 2.94 ng/ml