

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS113023\
 Data File : PS024983.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Nov 2023 09:41
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 23:27:45 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.355	6.771	1173.8E6	375.5E6	524.543	518.246
Target Compounds							
1) T	Dalapon	2.513f	2.565	9791278	5482817	3.395	4.780 #
3) T	4-Nitroph...	0.000	6.367	0	374222	N.D.	<MDL
5) T	DICAMBA	0.000	6.972f	0	1444201	N.D.	<MDL
6) T	MCP	0.000	6.972f	0	1444201	N.D.	<MDL
7) T	MCPA	0.000	7.166f	0	20725019	N.D.	6.301
8) T	DICHLORPROP	0.000	7.558	0	1503735	N.D.	1.912
9) T	2,4-D	7.248	0.000	7238734	0	2.383	N.D. #
11) T	2,4,5-TP ...	0.000	8.608	0	163585	N.D.	<MDL
12) T	2,4,5-T	0.000	8.982	0	690521	N.D.	<MDL
15) T	Picloram	9.683	10.763	33463759	9821974	1.717	1.501
16) T	DCPA	0.000	10.763	0	9821974	N.D.	1.812



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS113023\
Data File : PS024983.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Nov 2023 09:41
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 23:27:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

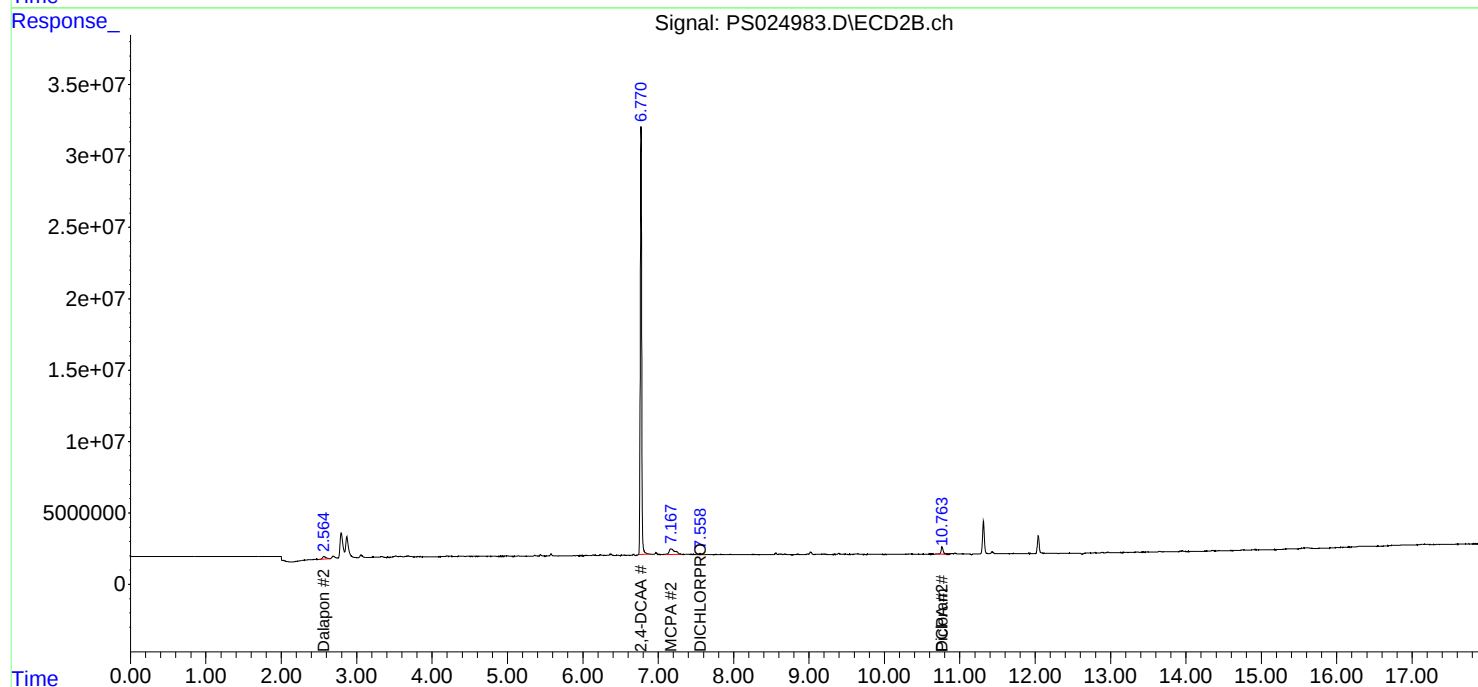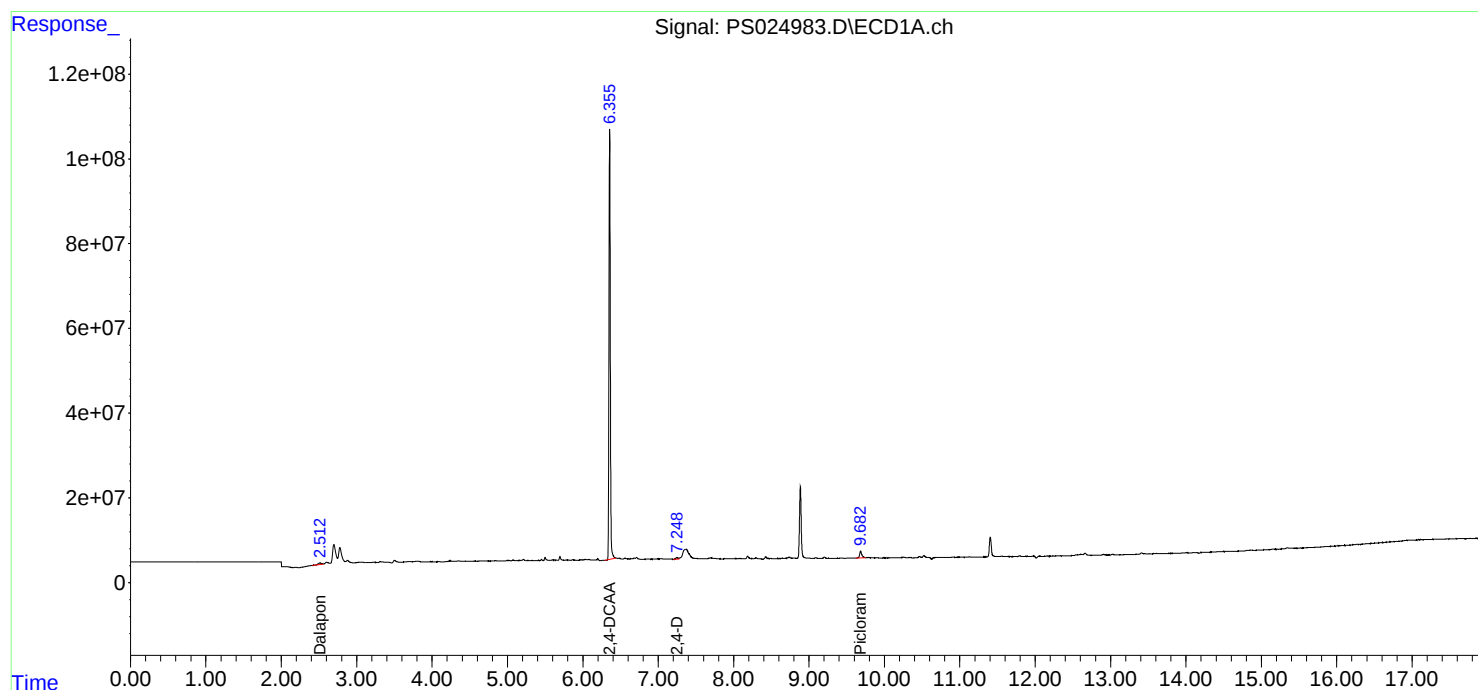


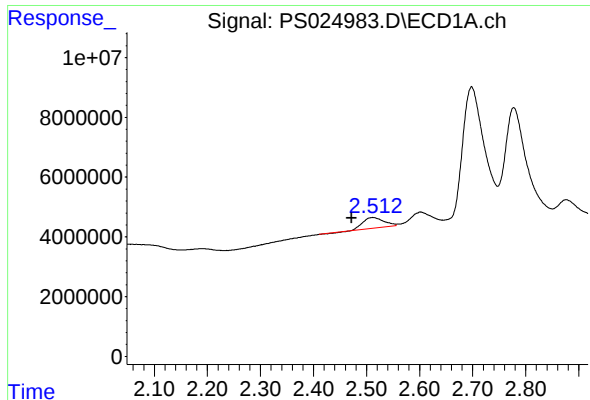

#1 Dalapon


R.T.: 2.513 min
Delta R.T.: 0.041 min
Response: 9791278
Conc: 3.40 ng/ml

Instrument :
ECD_S
ClientSampleId :

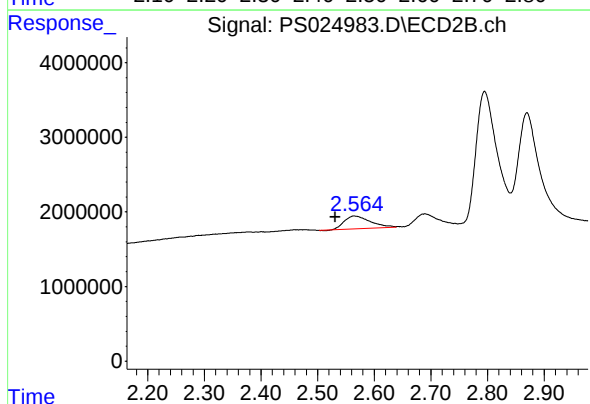


#1 Dalapon

R.T.: 2.565 min
Delta R.T.: 0.033 min
Response: 5482817
Conc: 4.78 ng/ml

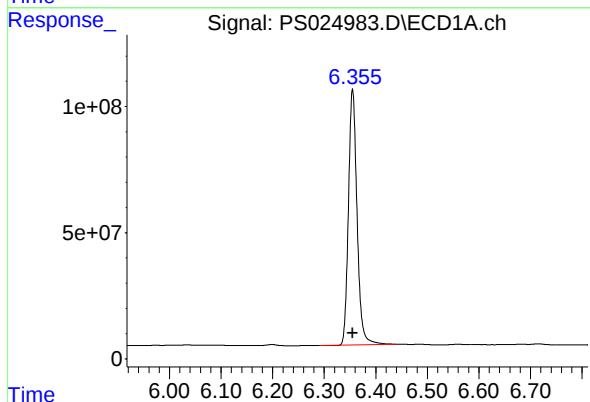


#4 2,4-DCAA

R.T.: 6.355 min
Delta R.T.: 0.000 min
Response: 1173845022
Conc: 524.54 ng/ml

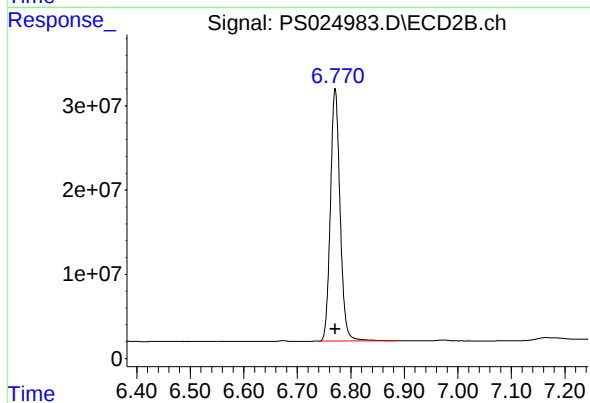

#4 2,4-DCAA


R.T.: 6.771 min
Delta R.T.: 0.000 min
Response: 375497516
Conc: 518.25 ng/ml

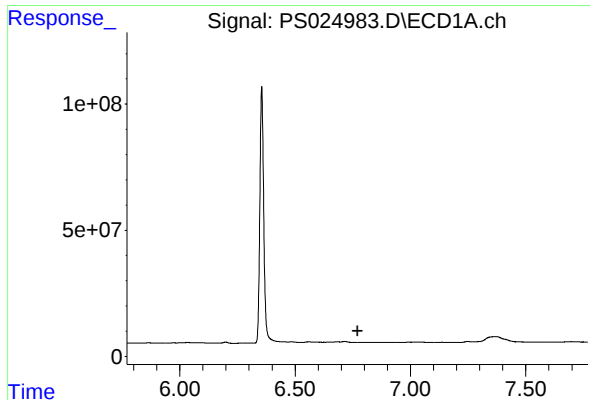

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.771 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

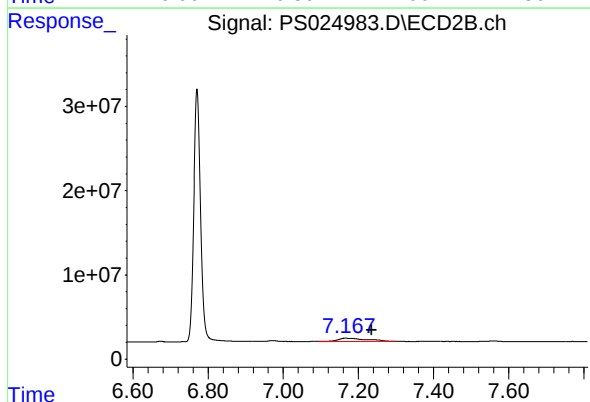


#7 MCPA

R.T.: 7.166 min
Delta R.T.: -0.069 min
Response: 20725019
Conc: 6.30 ug/ml

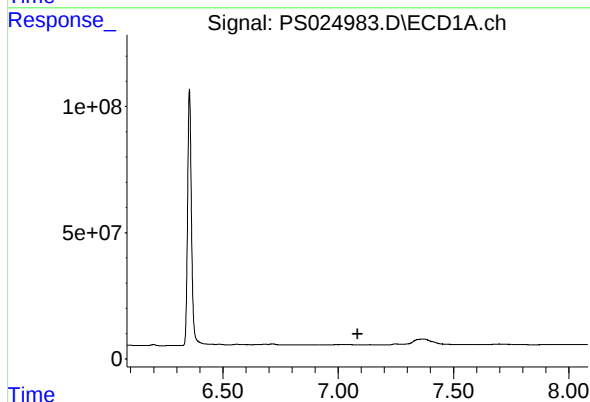


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

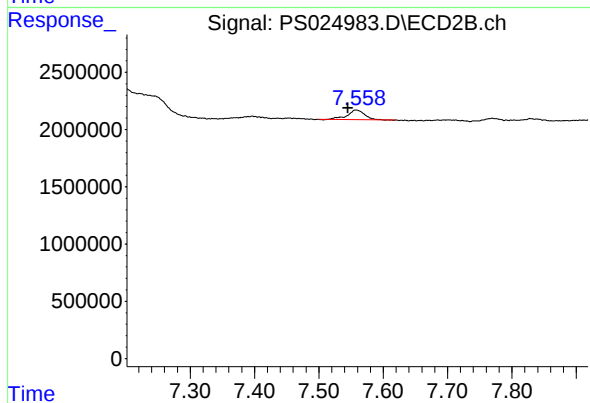

#8 DICHLORPROP


R.T.: 7.558 min
Delta R.T.: 0.013 min
Response: 1503735
Conc: 1.91 ng/ml

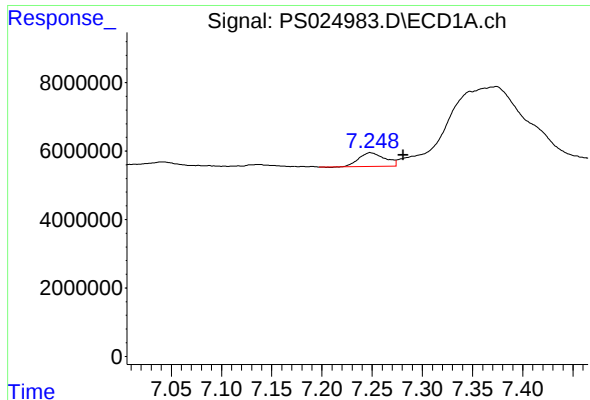

#9 2,4-D


R.T.: 7.248 min
Delta R.T.: -0.033 min
Response: 7238734
Conc: 2.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

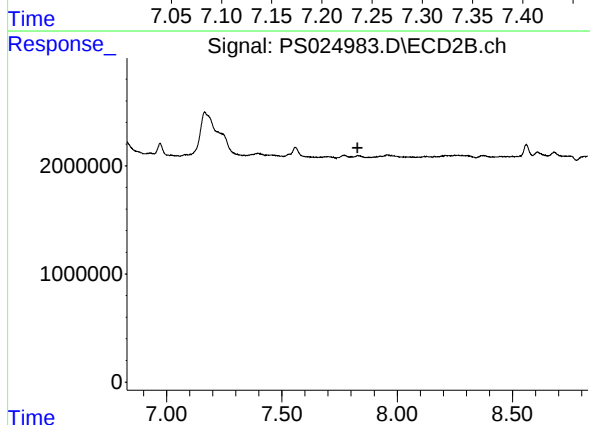


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.828 min
Response: 0
Conc: N.D.

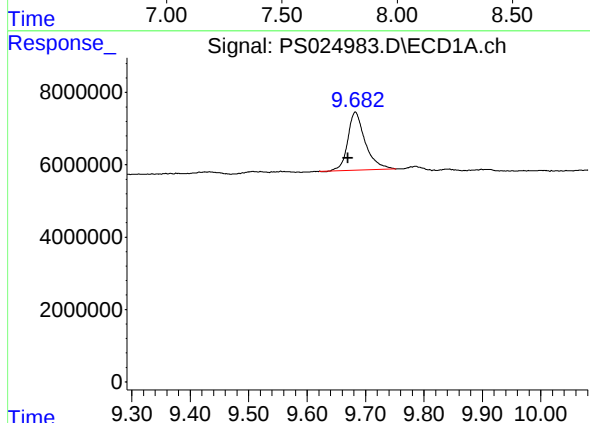


#15 Picloram

R.T.: 9.683 min
Delta R.T.: 0.013 min
Response: 33463759
Conc: 1.72 ng/ml

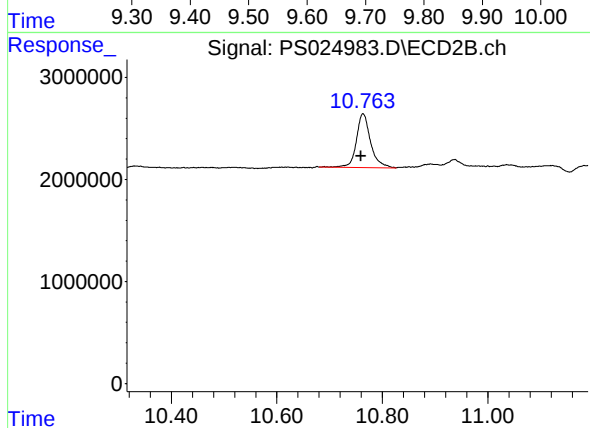

#15 Picloram


R.T.: 10.763 min
Delta R.T.: 0.003 min
Response: 9821974
Conc: 1.50 ng/ml

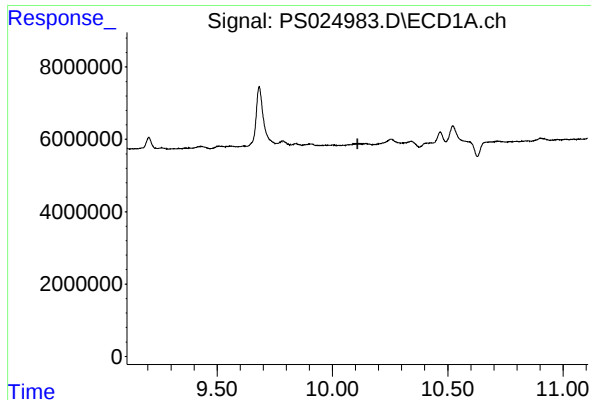

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.109 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

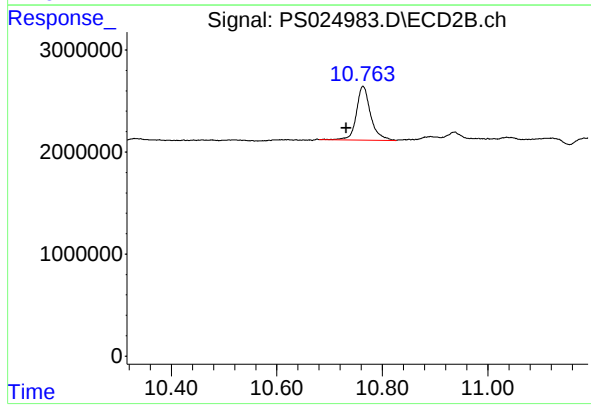

#16 DCPA

R.T.: 10.763 min
Delta R.T.: 0.032 min
Response: 9821974
Conc: 1.81 ng/ml