

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS113023\
 Data File : PS024990.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Nov 2023 13:52
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 23:29:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.355	6.771	1177.1E6	379.3E6	525.976	523.455
Target Compounds							
1) T	Dalapon	2.509	2.565	7944814	4760320	2.755	4.150 #
5) T	DICAMBA	0.000	6.930	0	471953	N.D.	<MDL
6) T	MCPP	6.678	7.085f	6310783	836064	<MDL	<MDL #
8) T	DICHLORPROP	0.000	7.557	0	5252090	N.D.	6.676
9) T	2,4-D	7.247	7.831	8240491	329384	2.713	<MDL #
10) T	Pentachlo...	0.000	8.251	0	574904	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.610	0	37505	N.D.	<MDL
12) T	2,4,5-T	8.290	8.981	7337162	1395472	<MDL	<MDL #
13) T	2,4-DB	0.000	9.475	0	1441026	N.D.	2.604
14) T	DINOSEB	0.000	9.810	0	628046	N.D.	<MDL
15) T	Picloram	9.679	10.762	18820261	5258196	<MDL	<MDL #
16) T	DCPA	0.000	10.729	0	1689935	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS113023\
Data File : PS024990.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Nov 2023 13:52
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 23:29:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

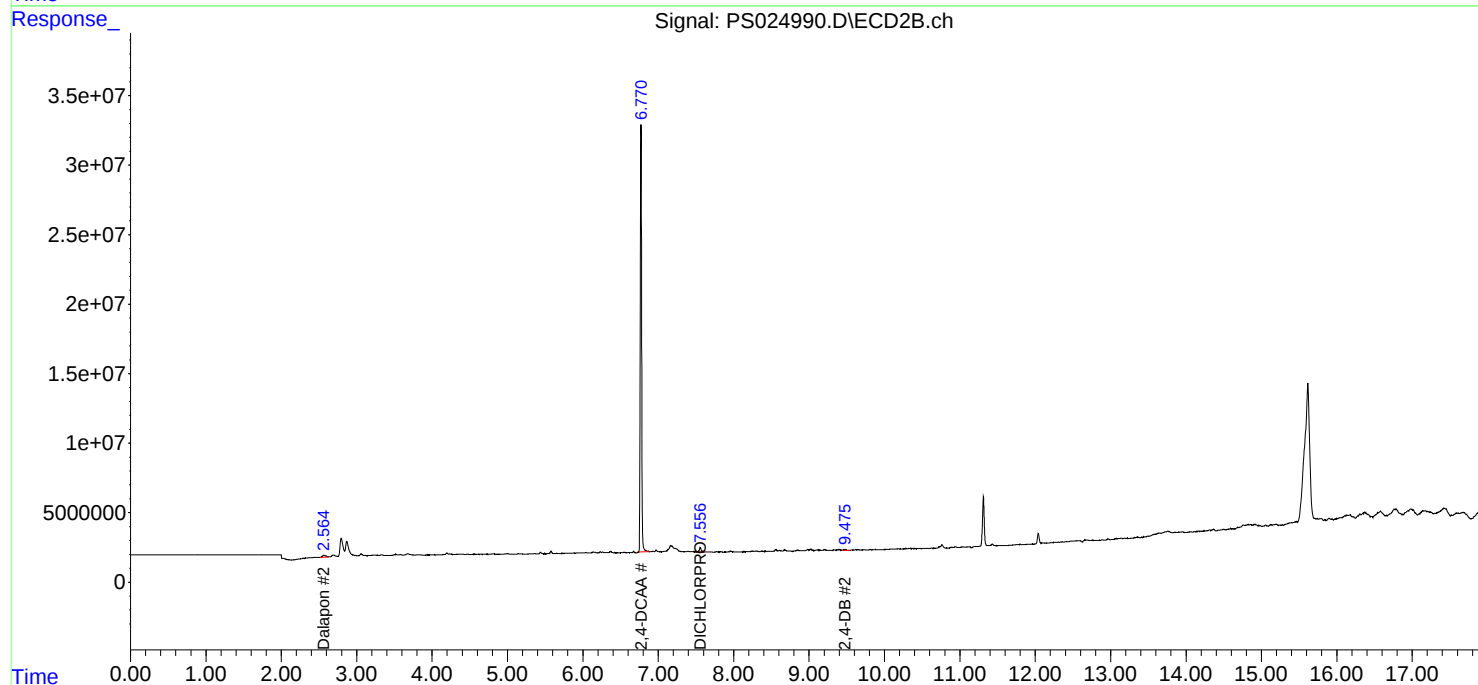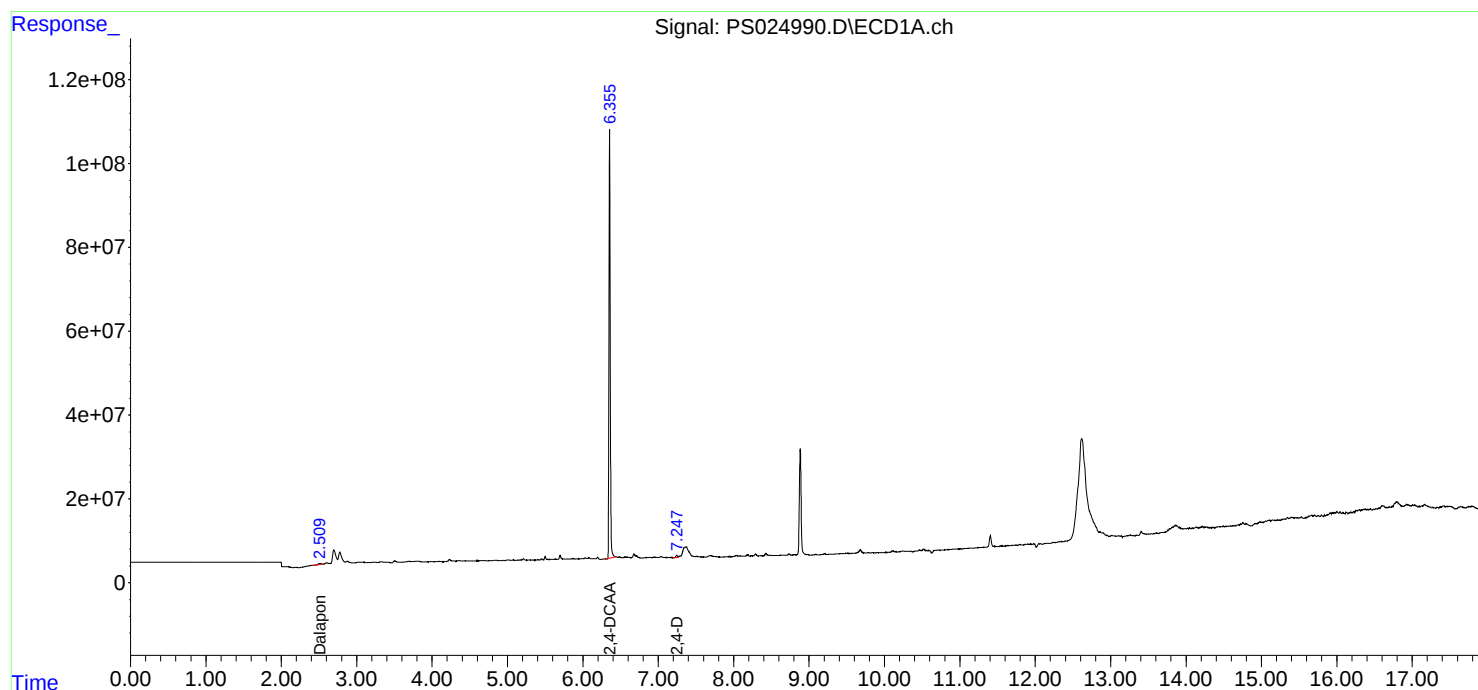


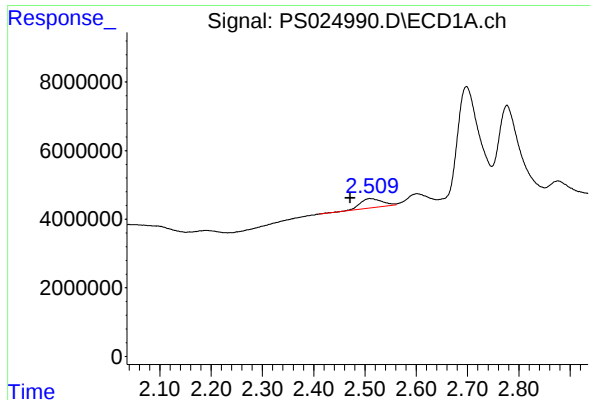

#1 Dalapon


R.T.: 2.509 min
Delta R.T.: 0.037 min
Response: 7944814
Conc: 2.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

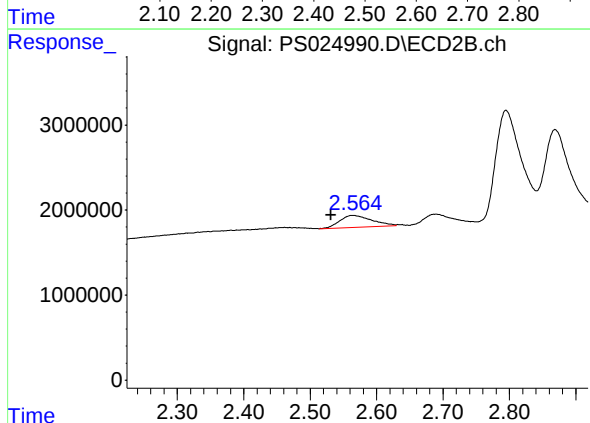


#1 Dalapon

R.T.: 2.565 min
Delta R.T.: 0.033 min
Response: 4760320
Conc: 4.15 ng/ml

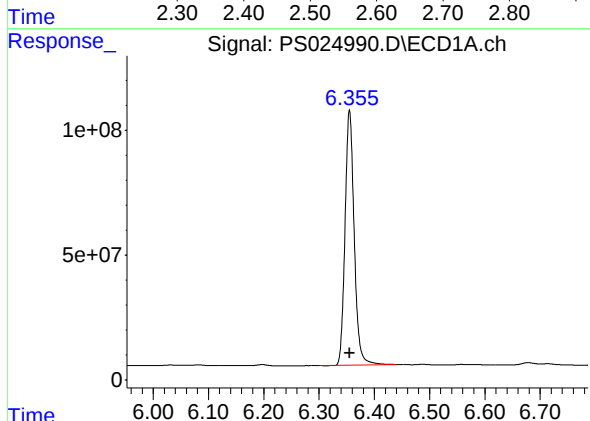


#4 2,4-DCAA

R.T.: 6.355 min
Delta R.T.: 0.000 min
Response: 1177052341
Conc: 525.98 ng/ml

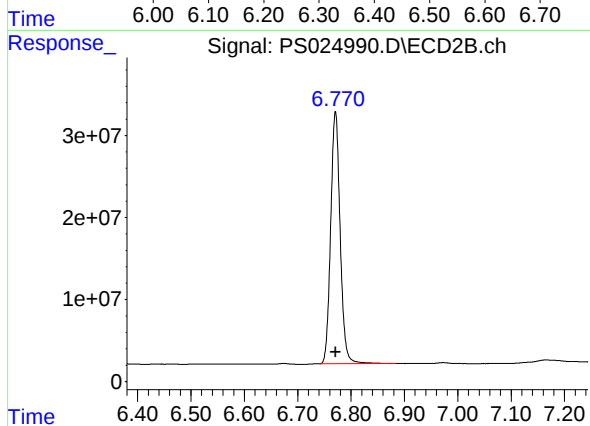

#4 2,4-DCAA


R.T.: 6.771 min
Delta R.T.: 0.000 min
Response: 379271810
Conc: 523.46 ng/ml

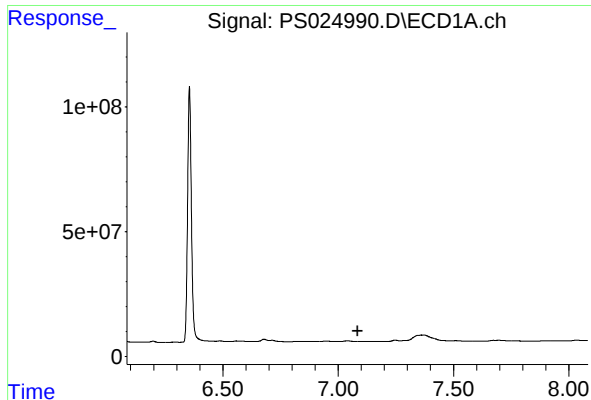

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

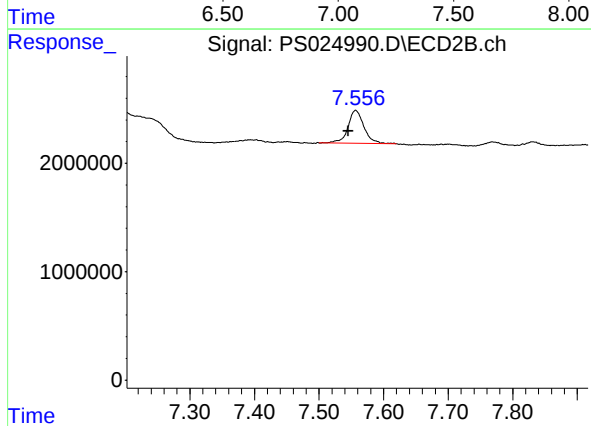


#8 DICHLORPROP

R.T.: 7.557 min
Delta R.T.: 0.012 min
Response: 5252090
Conc: 6.68 ng/ml

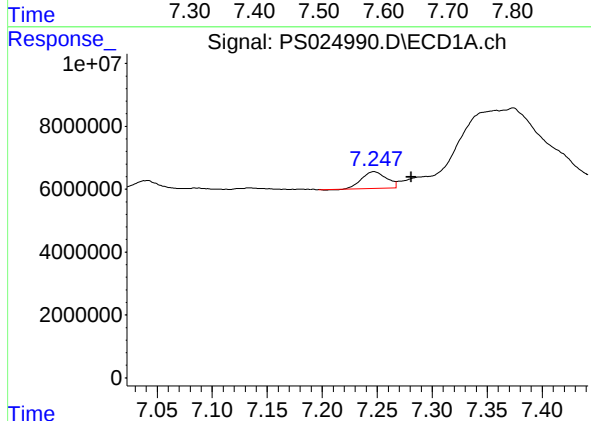


#9 2,4-D

R.T.: 7.247 min
Delta R.T.: -0.034 min
Response: 8240491
Conc: 2.71 ng/ml

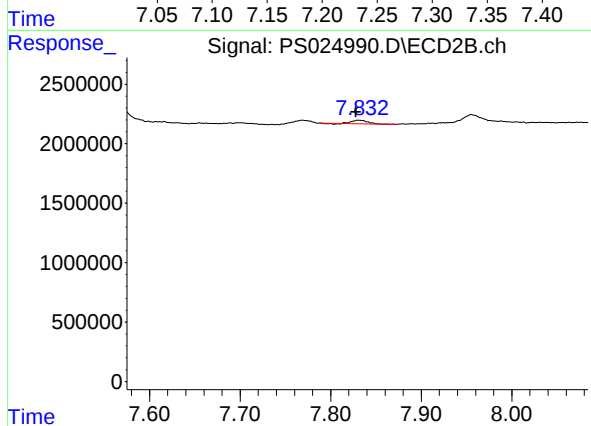

#9 2,4-D


R.T.: 7.831 min
Delta R.T.: 0.003 min
Response: 329384
Conc: N.D.

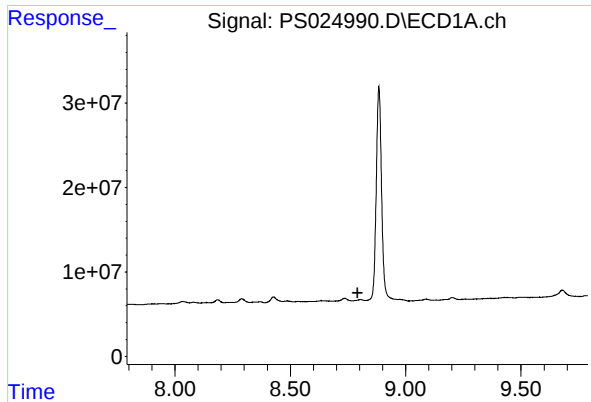

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.791 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

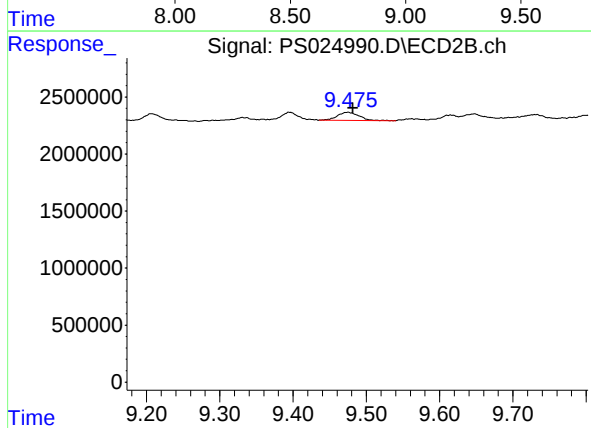

#13 2,4-DB

R.T.: 9.475 min
Delta R.T.: -0.007 min
Response: 1441026
Conc: 2.60 ng/ml