

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120122\
 Data File : PS021265.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2022 15:38
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 03:22:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111622.M
 Quant Title : 8080.M
 QLast Update : Thu Nov 17 00:46:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.407	6.840	1179.4E6	864.6E6	542.418	571.772
Target Compounds							
1) T	Dalapon	2.500	0.000	291086	0	<MDL	N.D. #
3) T	4-Nitroph...	6.241	6.435	13847746	3659959	10.250	4.163 #
5) T	DICAMBA	0.000	7.012	0	3996701	N.D.	<MDL
6) T	MCP	6.669f	7.062f	865314	7067547	<MDL	1.355 #
7) T	MCPA	6.909f	0.000	174482	0	<MDL	N.D. #
8) T	DICHLORPROP	7.174	7.654	-700257	21446725	N.D.	12.561
9) T	2,4-D	0.000	7.877f	0	7651635	N.D.	3.763
10) T	Pentachlo...	7.566	8.378	1020300	3232524	<MDL	<MDL #
11) T	2,4,5-TP ...	8.130	8.745	14799787	6865810	1.069	<MDL #
12) T	2,4,5-T	8.398	9.099	29210785	9053608	2.075	<MDL #
13) T	2,4-DB	8.895	9.611	2740857	3479704	1.199	2.972 #
14) T	DINOSEB	9.888f	0.000	45113076	0	3.933	N.D. #
15) T	Picloram	9.748	10.908	16413385	9287132	<MDL	<MDL #
16) T	DCPA	10.192	10.908f	1464027	9287132	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120122\
Data File : PS021265.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2022 15:38
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 03:22:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111622.M
Quant Title : 8080.M
QLast Update : Thu Nov 17 00:46:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

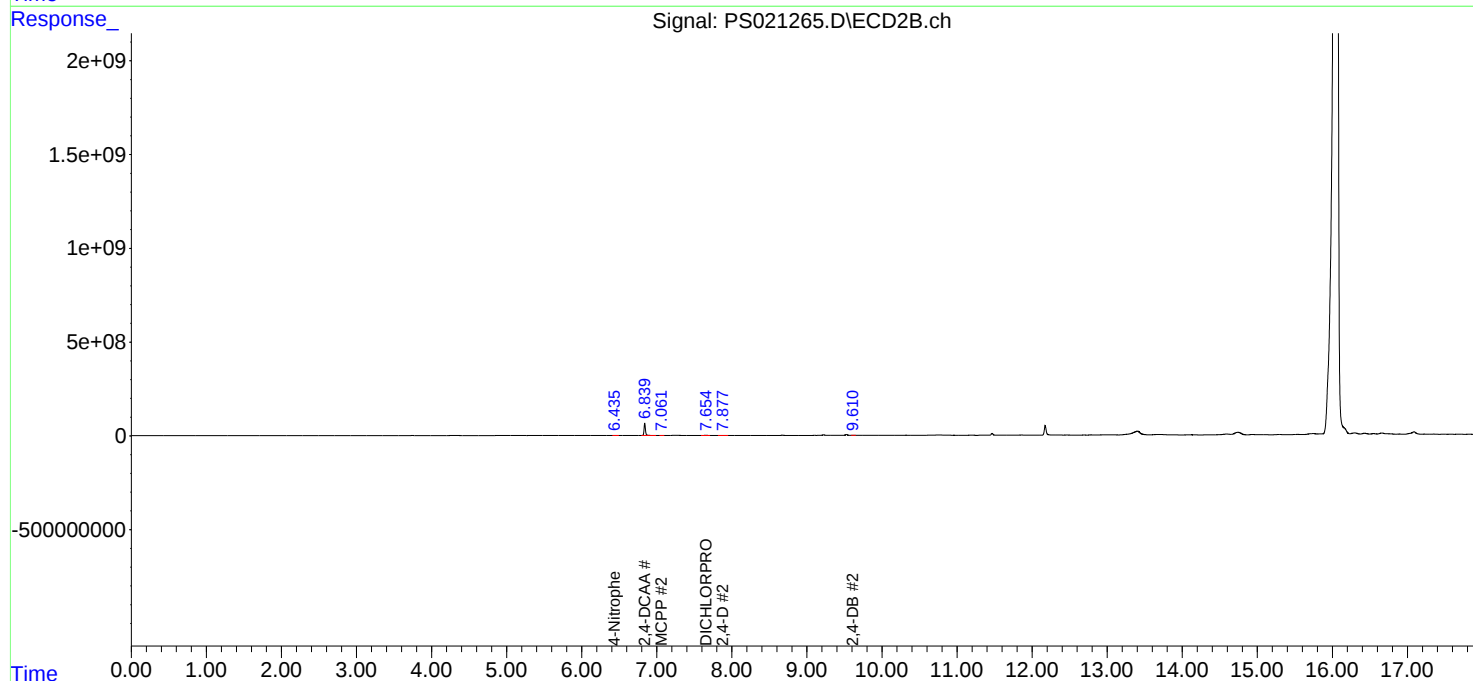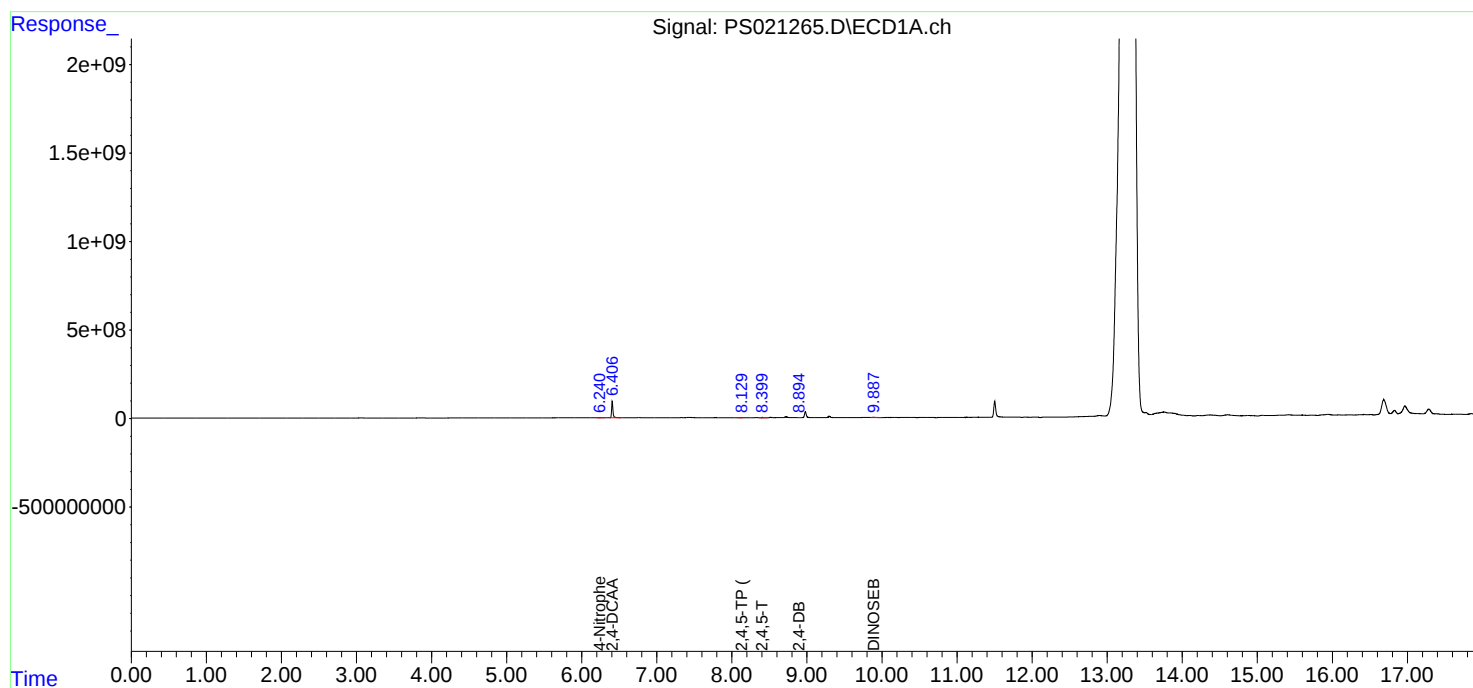


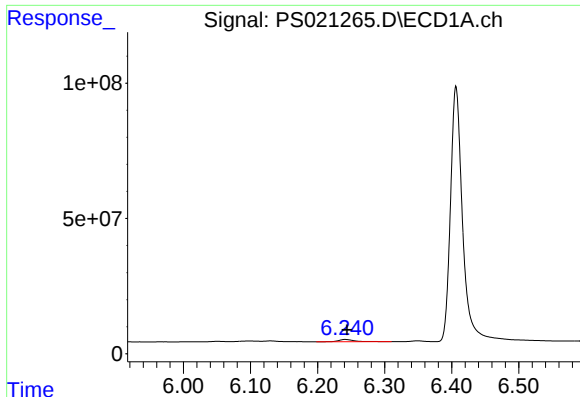

#3 4-Nitrophenol


R.T.: 6.241 min
Delta R.T.: -0.003 min
Response: 13847746
Conc: 10.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

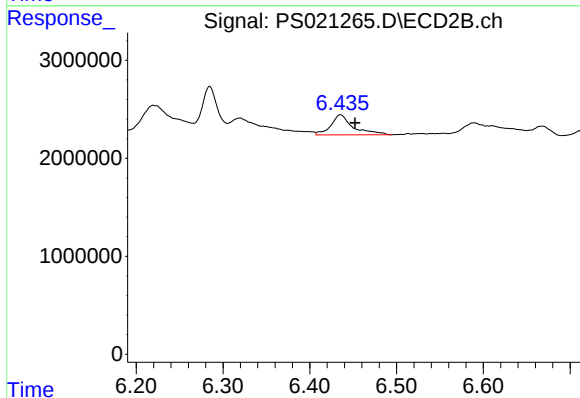


#3 4-Nitrophenol

R.T.: 6.435 min
Delta R.T.: -0.017 min
Response: 3659959
Conc: 4.16 ng/ml

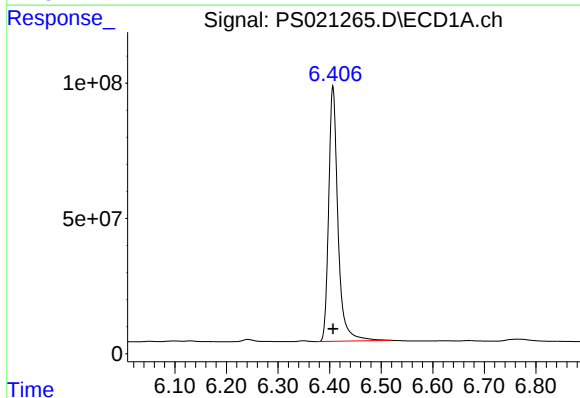


#4 2,4-DCAA

R.T.: 6.407 min
Delta R.T.: 0.000 min
Response: 1179376001
Conc: 542.42 ng/ml

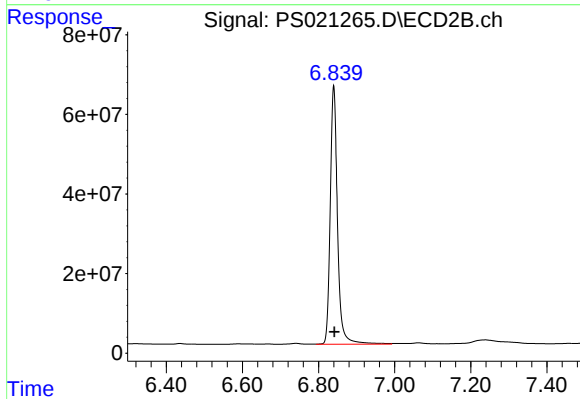

#4 2,4-DCAA


R.T.: 6.840 min
Delta R.T.: -0.002 min
Response: 864586725
Conc: 571.77 ng/ml

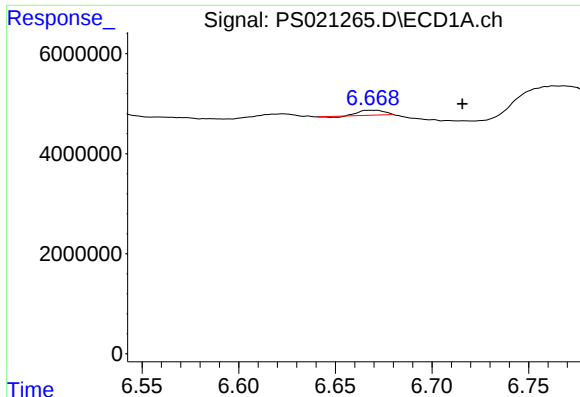

#6 MCP


R.T.: 6.669 min
Delta R.T.: -0.047 min
Response: 865314
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

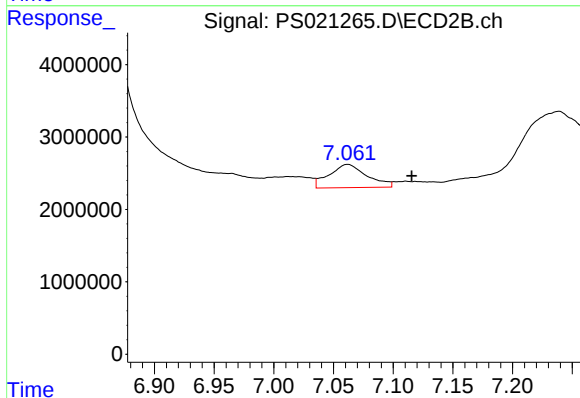


#6 MCP

R.T.: 7.062 min
Delta R.T.: -0.054 min
Response: 7067547
Conc: 1.36 ug/ml

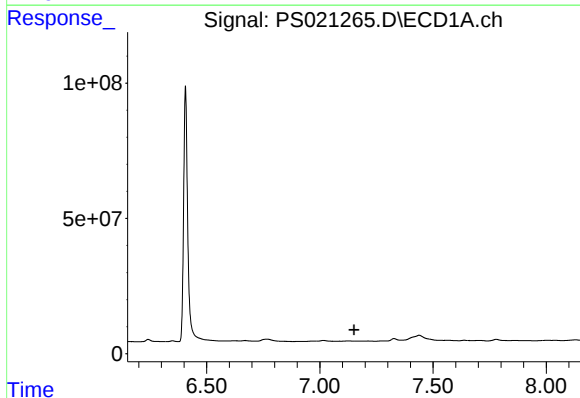


#8 DICHLORPROP

R.T.: 7.174 min
Delta R.T.: 0.023 min
Response: -700257
Conc: N.D.

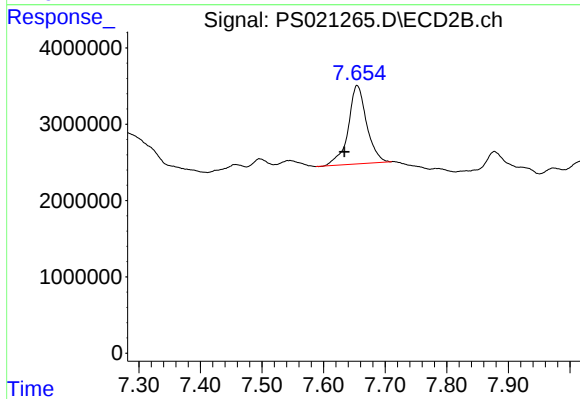

#8 DICHLORPROP


R.T.: 7.654 min
Delta R.T.: 0.021 min
Response: 21446725
Conc: 12.56 ng/ml

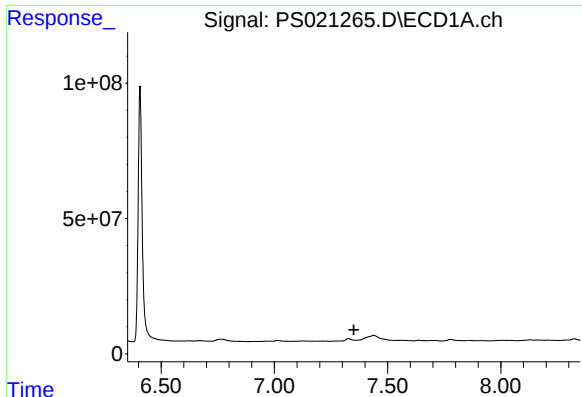

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.351 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

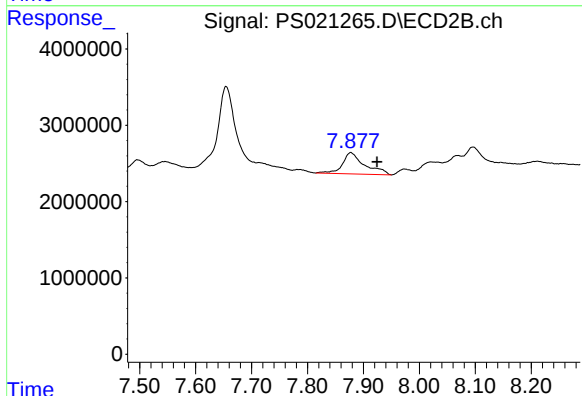


#9 2,4-D

R.T.: 7.877 min
Delta R.T.: -0.047 min
Response: 7651635
Conc: 3.76 ng/ml

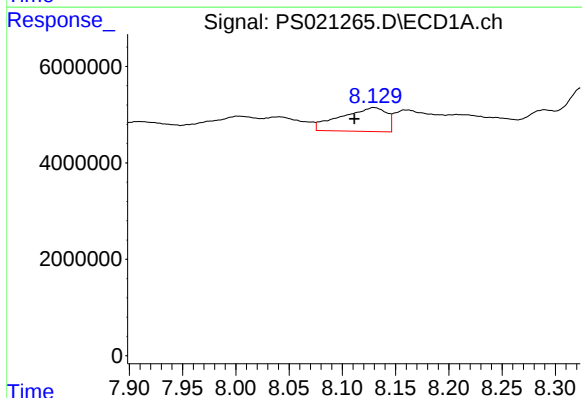


#11 2,4,5-TP (SILVEX)

R.T.: 8.130 min
Delta R.T.: 0.018 min
Response: 14799787
Conc: 1.07 ng/ml

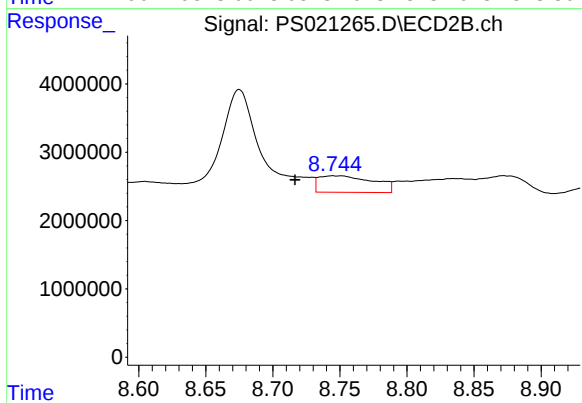

#11 2,4,5-TP (SILVEX)


R.T.: 8.745 min
Delta R.T.: 0.028 min
Response: 6865810
Conc: N.D.

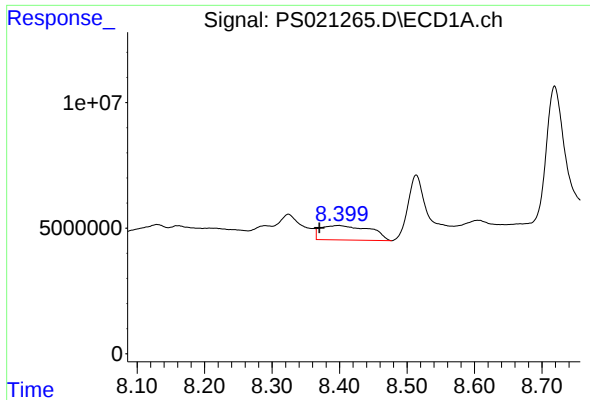

#12 2,4,5-T


R.T.: 8.398 min
Delta R.T.: 0.028 min
Response: 29210785
Conc: 2.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

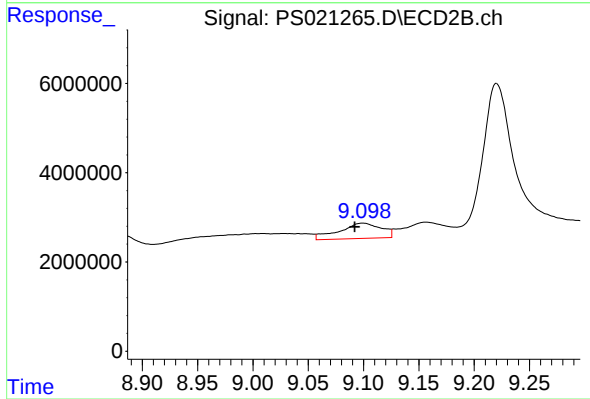


#12 2,4,5-T

R.T.: 9.099 min
Delta R.T.: 0.007 min
Response: 9053608
Conc: N.D.

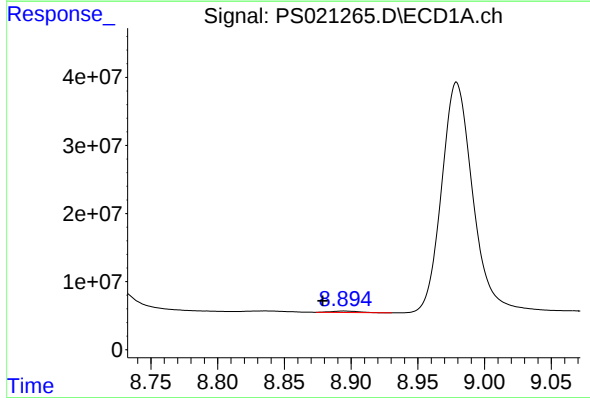


#13 2,4-DB

R.T.: 8.895 min
Delta R.T.: 0.016 min
Response: 2740857
Conc: 1.20 ng/ml

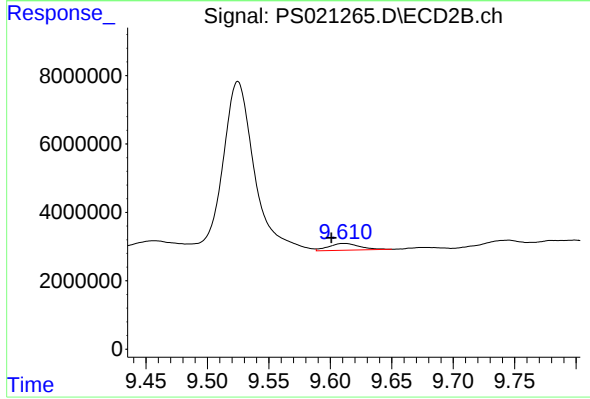

#13 2,4-DB


R.T.: 9.611 min
Delta R.T.: 0.010 min
Response: 3479704
Conc: 2.97 ng/ml

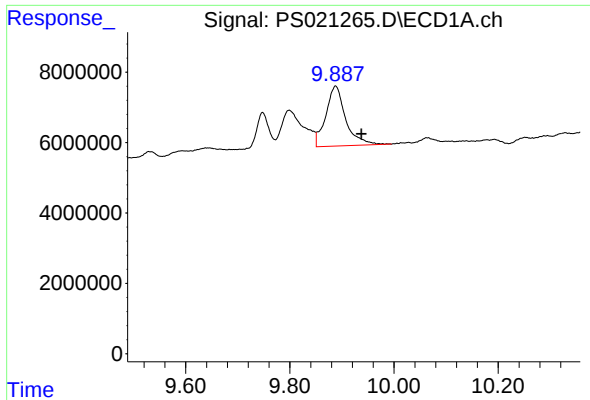

#14 DINOSEB

R.T.: 9.888 min
Delta R.T.: -0.049 min
Response: 45113076
Conc: 3.93 ng/ml

Instrument :
ECD_S
ClientSampleId :

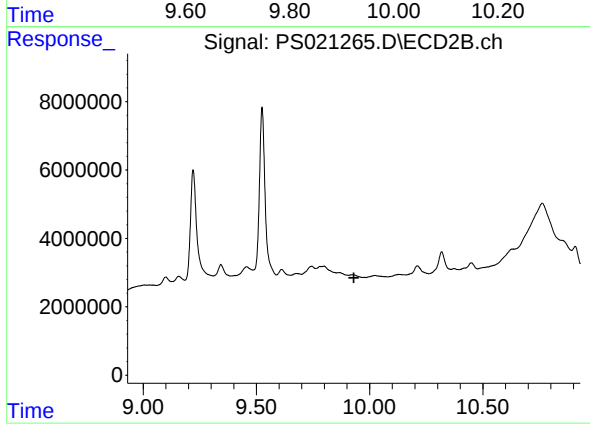

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.930 min
Response: 0
Conc: N.D.