

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120122\
 Data File : PS021267.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Dec 2022 17:49
 Operator : AR\AJ
 Sample : PB149366BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB149366BL

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/02/2022
 Supervised By :Ankita Jodhani 12/02/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 02 03:22:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111622.M
 Quant Title : 8080.M
 QLast Update : Thu Nov 17 00:46:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.404	6.839	1369.2E6	1068.2E6	629.730	706.452
Target Compounds							
13) T	2,4-DB	8.897	9.612	18089.0E6	19627.5E6	7914.388m	16766.067m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120122\
Data File : PS021267.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Dec 2022 17:49
Operator : AR\AJ
Sample : PB149366BL
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
PB149366BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/02/2022
Supervised By : Ankita Jodhani 12/02/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 02 03:22:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111622.M
Quant Title : 8080.M
QLast Update : Thu Nov 17 00:46:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

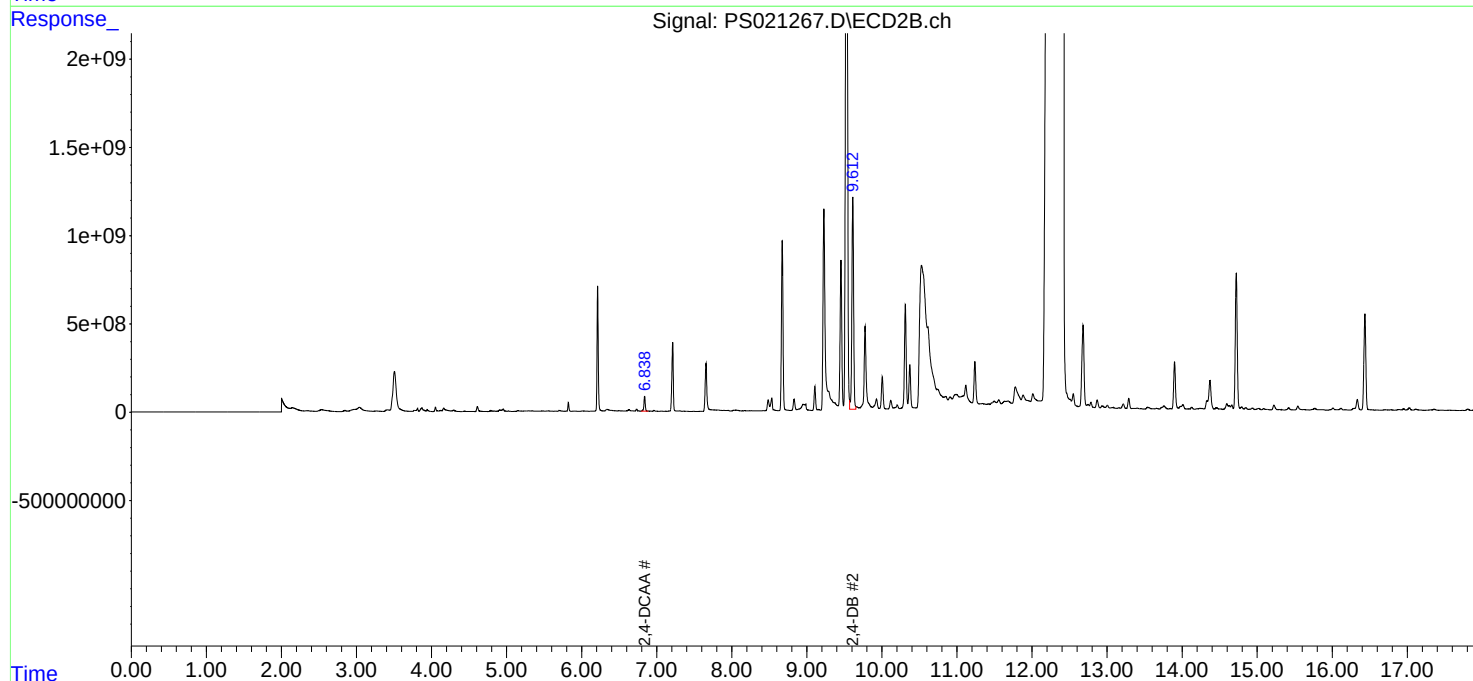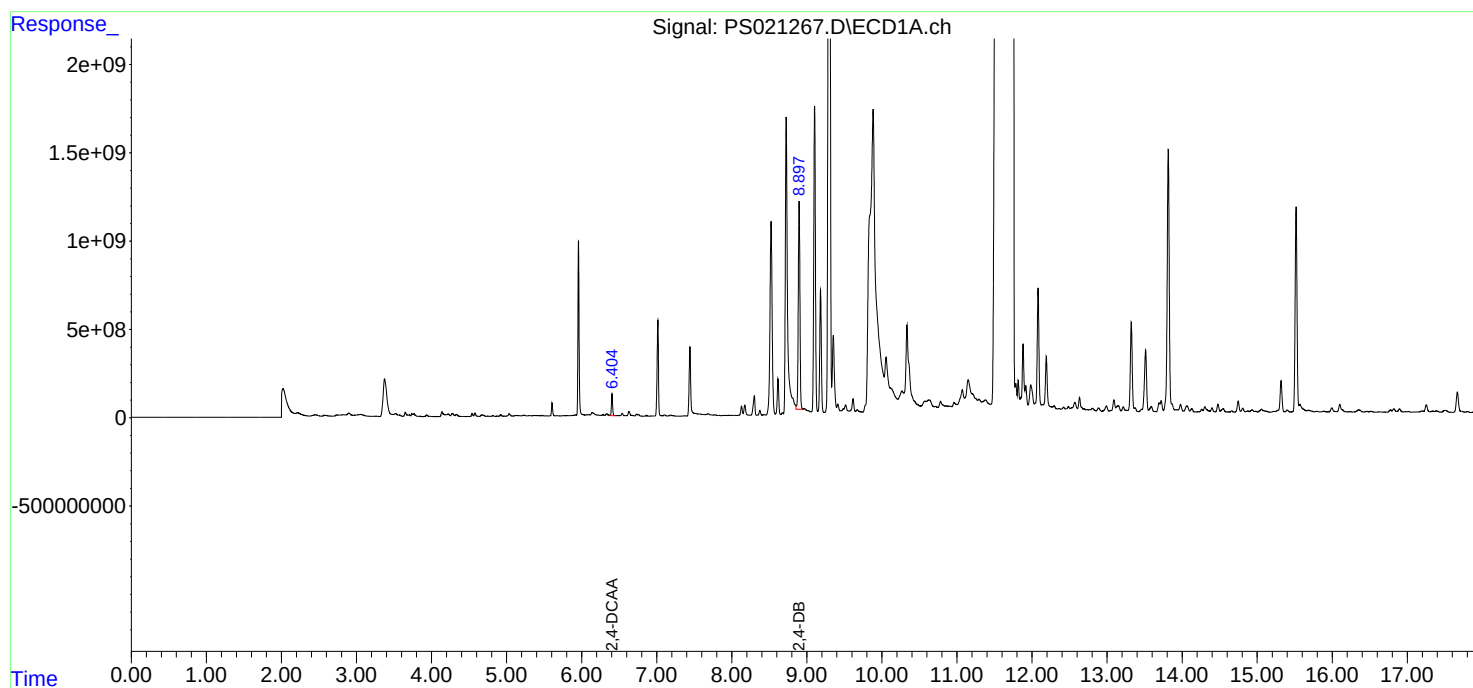

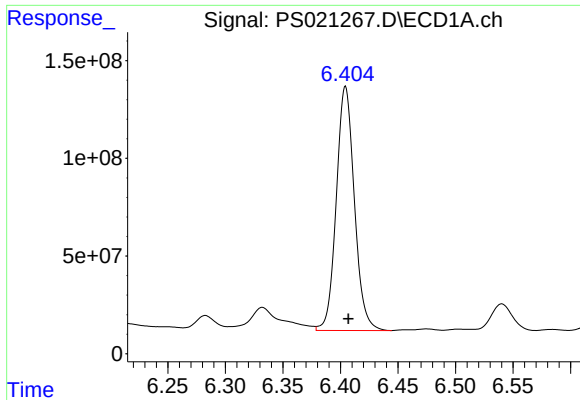


#4 2,4-DCAA

R.T.: 6.404 min
Delta R.T.: -0.002 min
Response: 1369218820
Conc: 629.73 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB149366BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/02/2022
Supervised By :Ankita Jodhani 12/02/2022

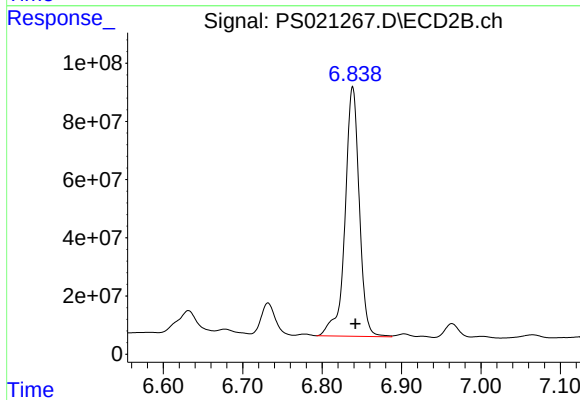


#4 2,4-DCAA

R.T.: 6.839 min
Delta R.T.: -0.003 min
Response: 1068238143
Conc: 706.45 ng/ml

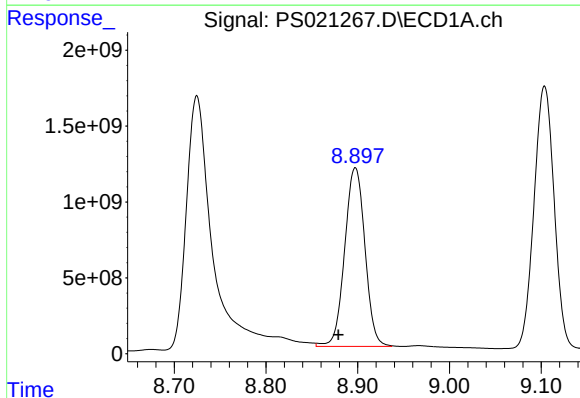

#13 2,4-DB

R.T.: 8.897 min
Delta R.T.: 0.018 min
Response: 18089044991
Conc: 7914.39 ng/ml m

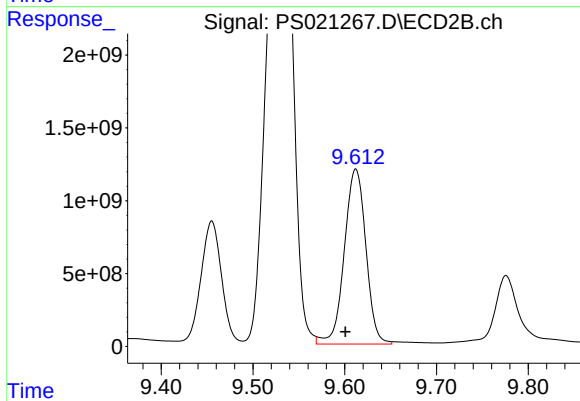

#13 2,4-DB

R.T.: 9.612 min
Delta R.T.: 0.011 min
Response: 19627520560
Conc: 16766.07 ng/ml m