

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120220\
 Data File : PS013397.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Dec 2020 19:53
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 03:04:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 03 02:59:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.216	6.919	376.4E6	205.2E6	404.236	521.676 #
Target Compounds							
5) T	DICAMBA	0.000	7.087	0	2724909	N.D.	1.621
7) T	MCPA	0.000	7.346f	0	241992	N.D.	<MDL
12) T	2,4,5-T	9.467	0.000	16094709	0	2.911	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120220\
Data File : PS013397.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2020 19:53
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 03:04:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
Quant Title : 8080.M
QLast Update : Thu Dec 03 02:59:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

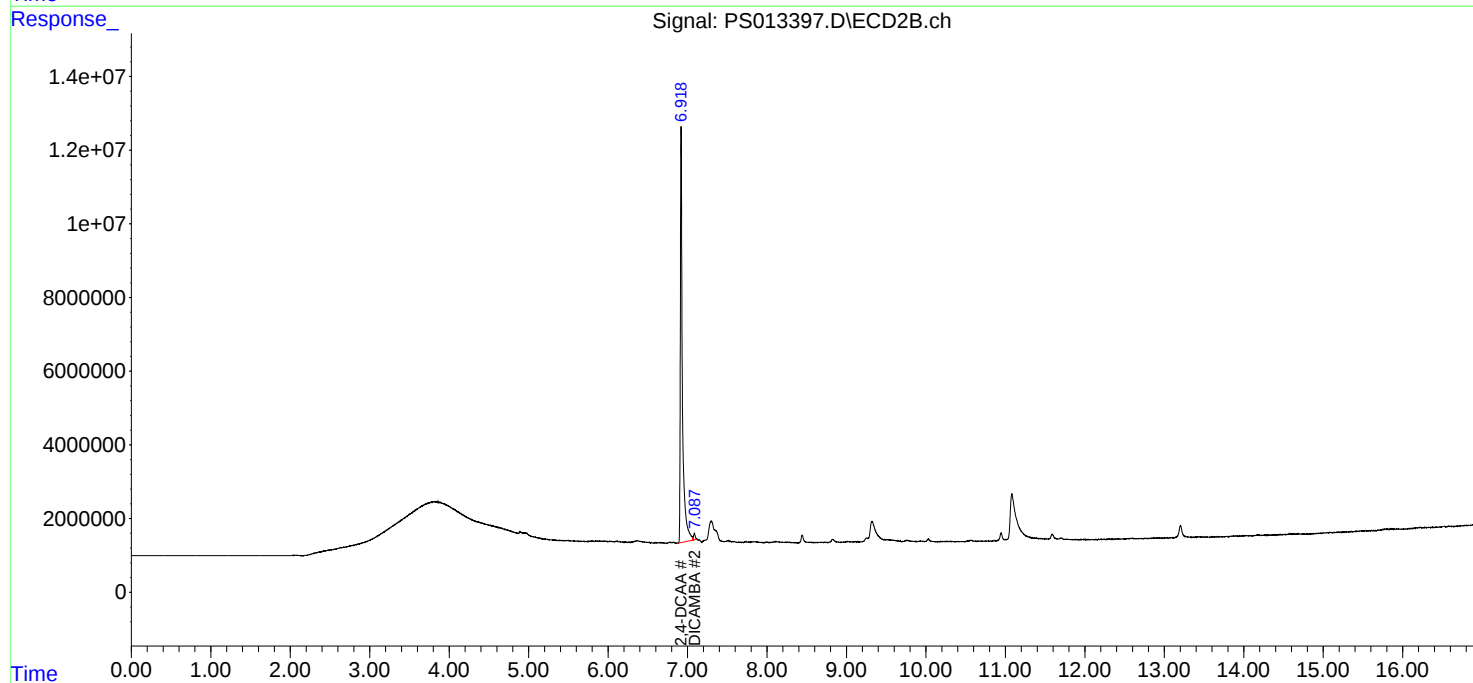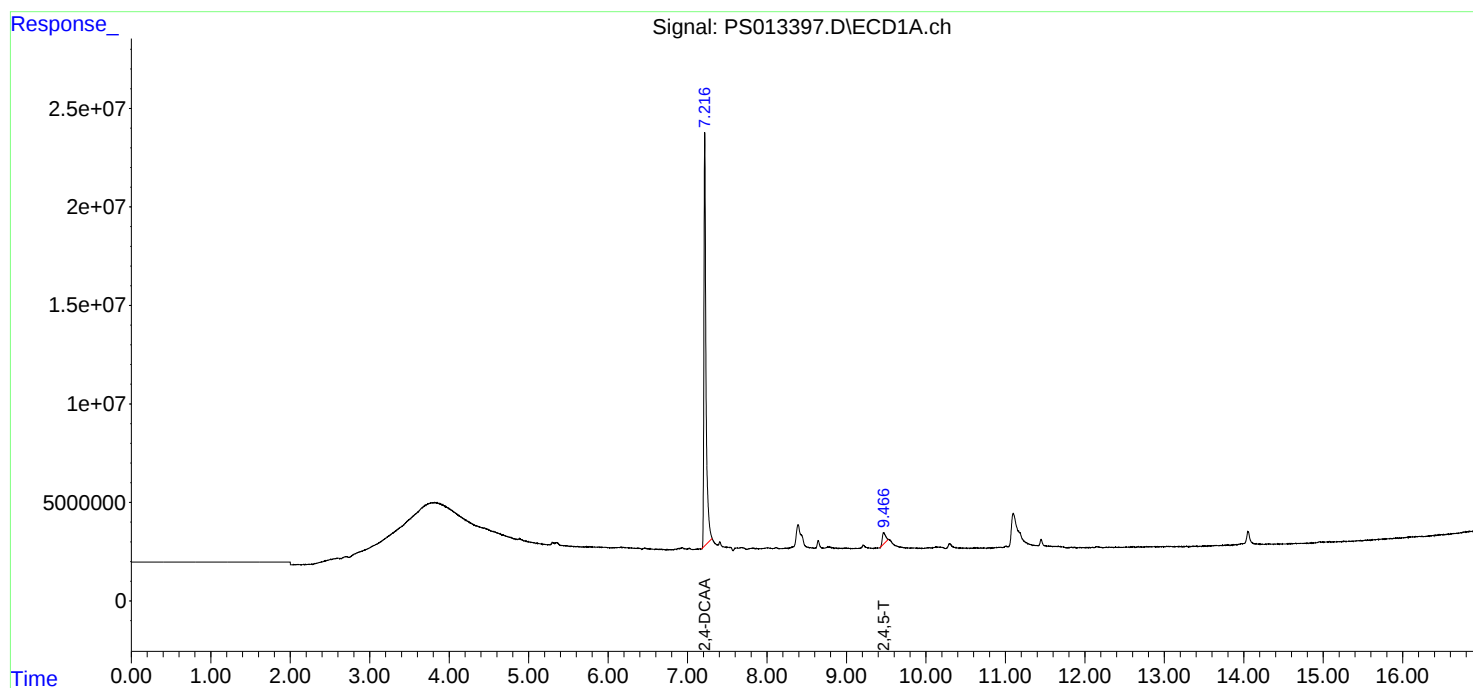


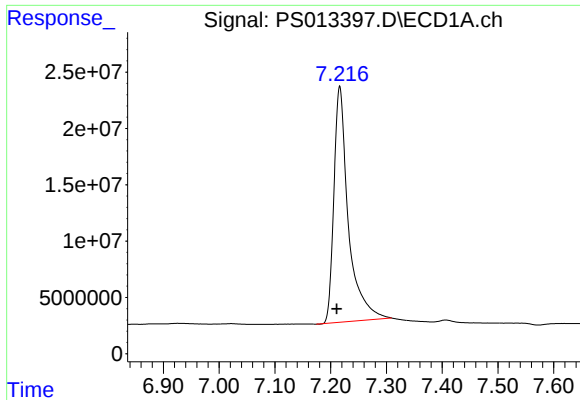

#4 2,4-DCAA


R.T.: 7.216 min
Delta R.T.: 0.005 min
Response: 376368054
Conc: 404.24 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

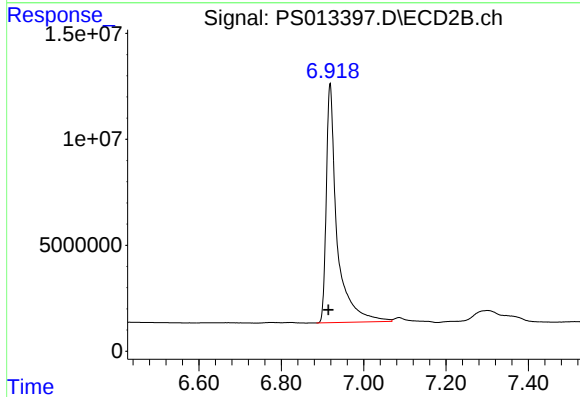


#4 2,4-DCAA

R.T.: 6.919 min
Delta R.T.: 0.005 min
Response: 205207344
Conc: 521.68 ng/ml

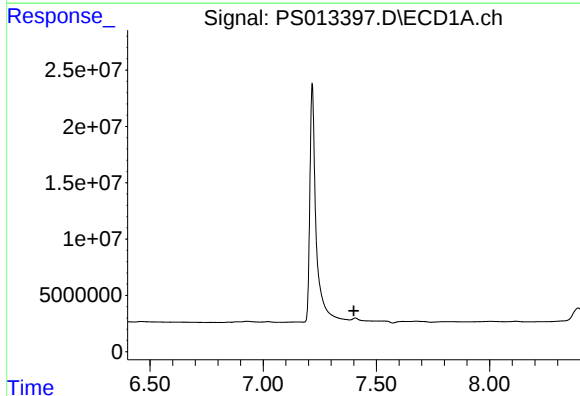


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.401 min
Response: 0
Conc: N.D.

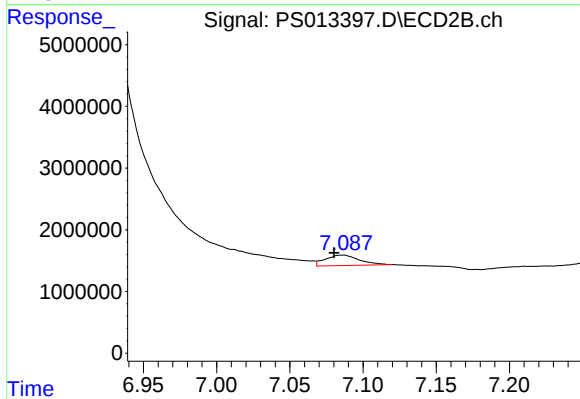

#5 DICAMBA


R.T.: 7.087 min
Delta R.T.: 0.007 min
Response: 2724909
Conc: 1.62 ng/ml

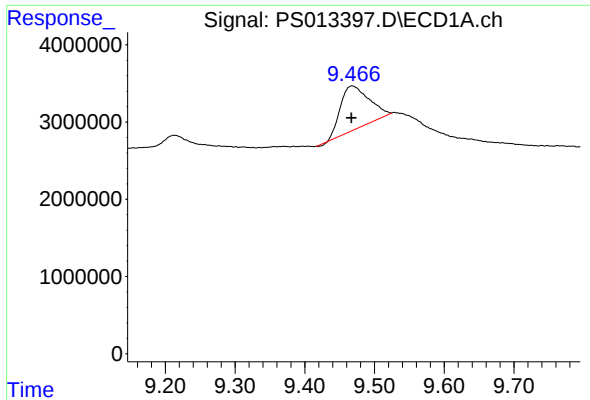

#12 2,4,5-T

R.T.: 9.467 min
Delta R.T.: 0.000 min
Response: 16094709
Conc: 2.91 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

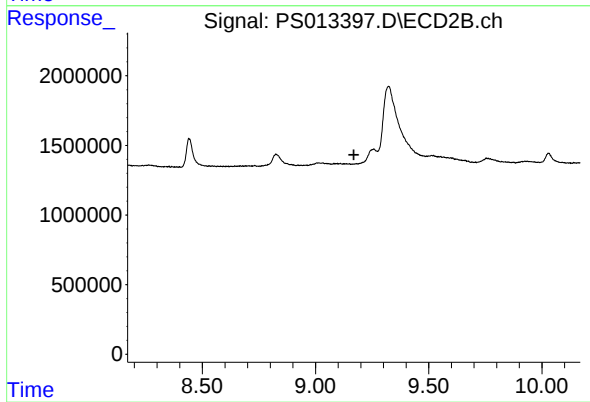

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.170 min
Response: 0
Conc: N.D.