

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120220\
 Data File : PS013393.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Dec 2020 18:21
 Operator : DD\AJ
 Sample : HSTDICC750
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 01:11:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 03 01:08:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.211	6.914	690.6E6	289.9E6	750.000	750.000
Target Compounds							
1) T	Dalapon	3.031	2.622	730.5E6	354.4E6	682.500	682.500
2) T	3,5-DICHL...	6.428	6.068	887.1E6	428.8E6	697.500	697.500
3) T	4-Nitroph...	7.046	6.527	309.2E6	165.1E6	682.500	682.500
5) T	DICAMBA	7.401	7.080	2598.7E6	1179.4E6	705.000	705.000
6) T	MCPD	7.567	7.174	193.5E6	93233369	70.500	70.500
7) T	MCPA	7.717	7.389	272.5E6	142.1E6	69.750	69.750
8) T	DICHLORPROP	8.092	7.705	644.6E6	310.0E6	705.000	705.000
9) T	2,4-D	8.324	8.004	722.7E6	378.7E6	705.000	705.000
10) T	Pentachlo...	8.630	8.427	9533.8E6	3983.2E6	712.500	712.500
11) T	2,4,5-TP ...	9.179	8.789	3784.1E6	1663.7E6	712.500	712.500
12) T	2,4,5-T	9.467	9.170	3921.3E6	1603.0E6	712.500	712.500
13) T	2,4-DB	10.021	9.678	674.2E6	210.8E6	712.500	712.500
14) T	DINOSEB	11.171	10.004	2942.1E6	1162.3E6	705.000	705.000
15) T	Picloram	11.009	11.001	5119.0E6	2518.3E6	712.500	712.500
16) T	DCPA	11.437	10.930	4845.1E6	2168.3E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120220\
Data File : PS013393.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2020 18:21
Operator : DD\AJ
Sample : HSTDICC750
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 01:11:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
Quant Title : 8080.M
QLast Update : Thu Dec 03 01:08:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

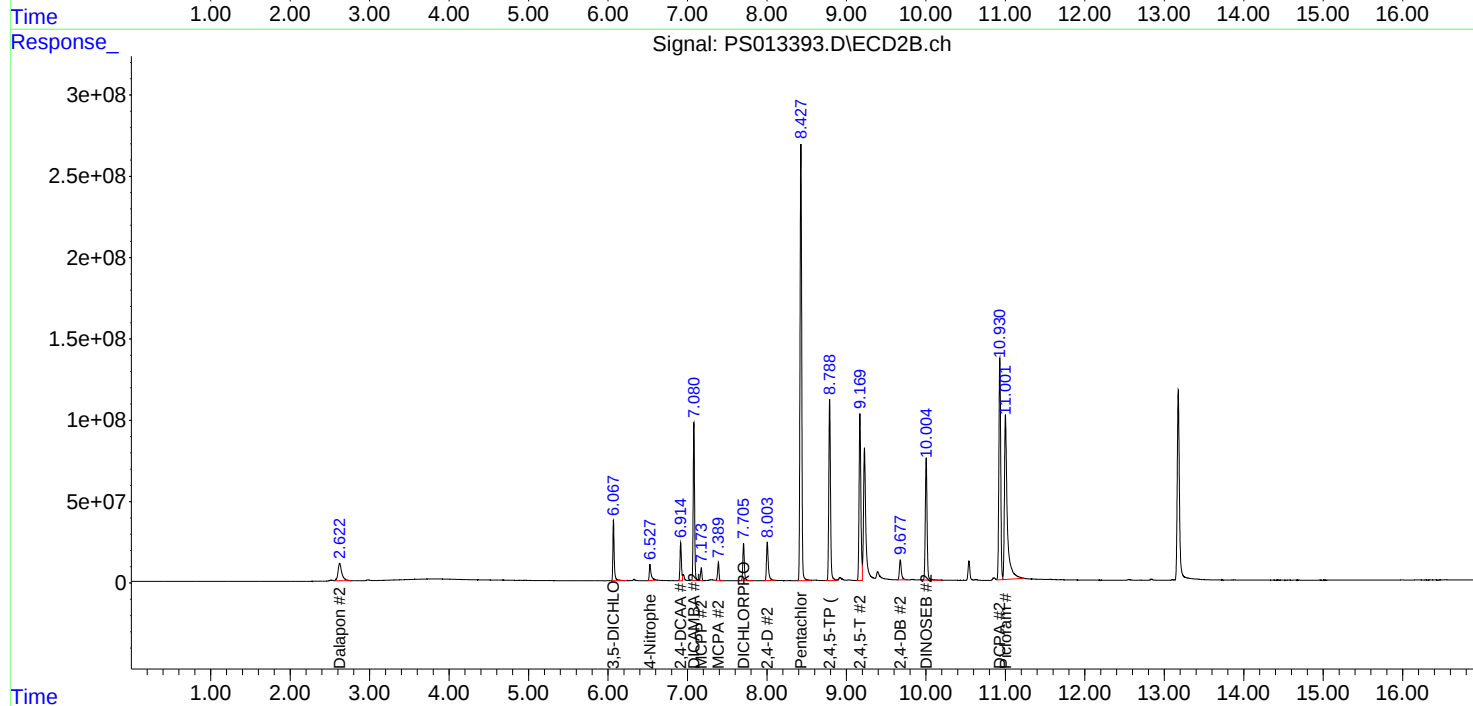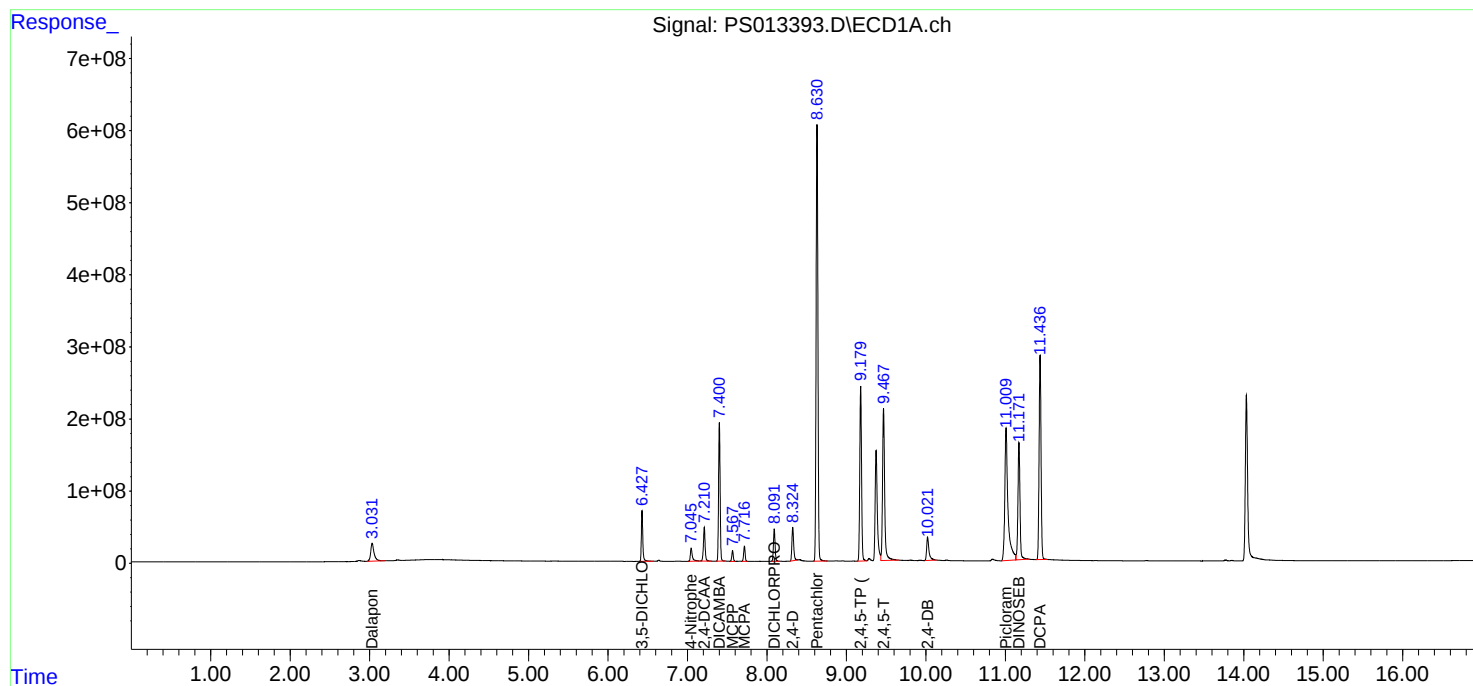


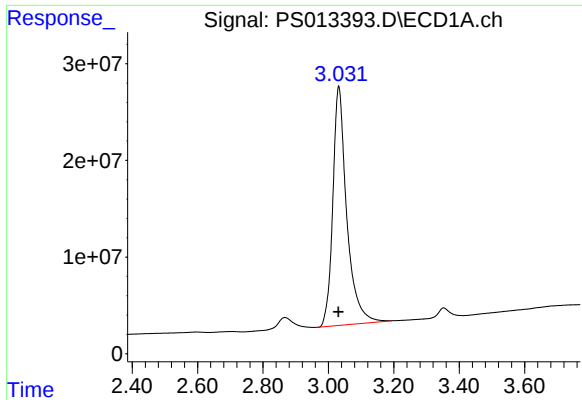

#1 Dalapon


R.T.: 3.031 min
Delta R.T.: 0.000 min
Response: 730485655
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

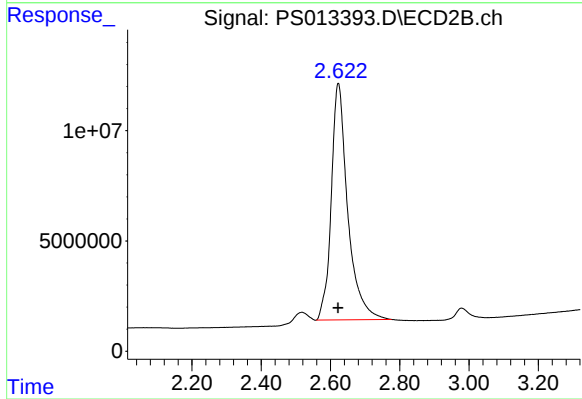


#1 Dalapon

R.T.: 2.622 min
Delta R.T.: 0.000 min
Response: 354363217
Conc: 682.50 ng/ml

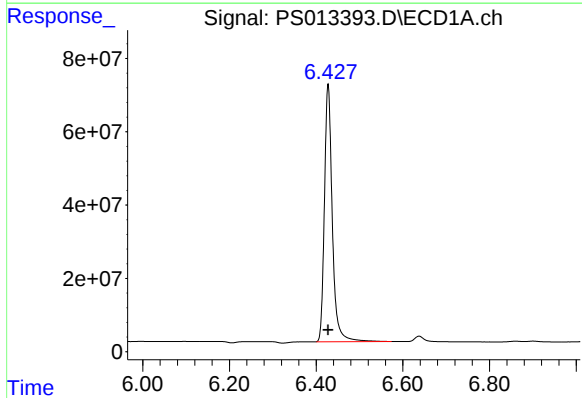


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.428 min
Delta R.T.: 0.000 min
Response: 887063844
Conc: 697.50 ng/ml

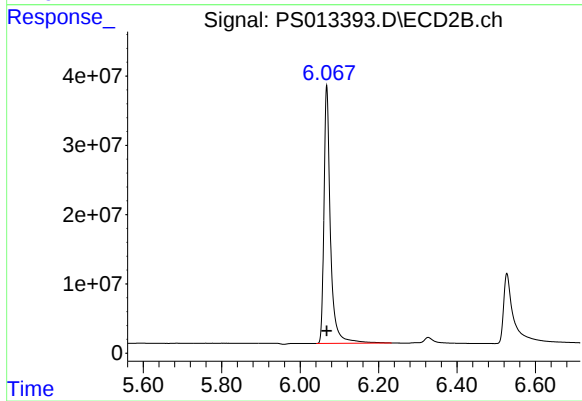

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.068 min
Delta R.T.: 0.000 min
Response: 428816632
Conc: 697.50 ng/ml

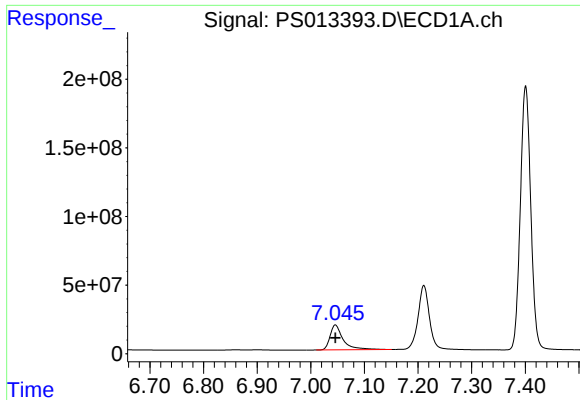

#3 4-Nitrophenol


R.T.: 7.046 min
Delta R.T.: 0.000 min
Response: 309246641
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

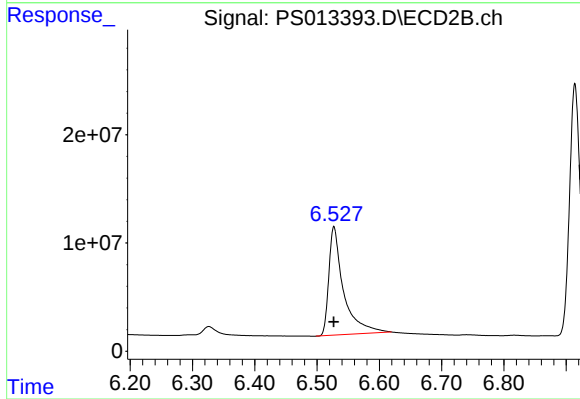


#3 4-Nitrophenol

R.T.: 6.527 min
Delta R.T.: 0.000 min
Response: 165079135
Conc: 682.50 ng/ml

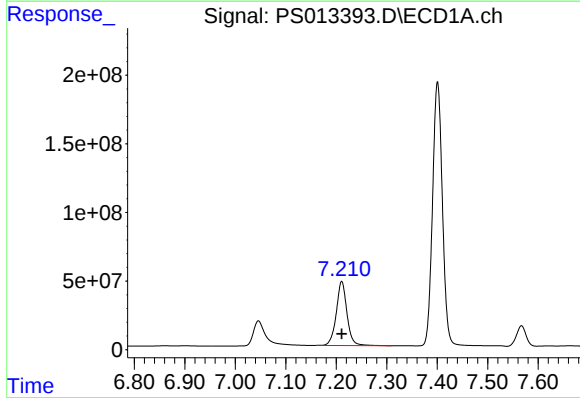


#4 2,4-DCAA

R.T.: 7.211 min
Delta R.T.: 0.000 min
Response: 690551612
Conc: 750.00 ng/ml

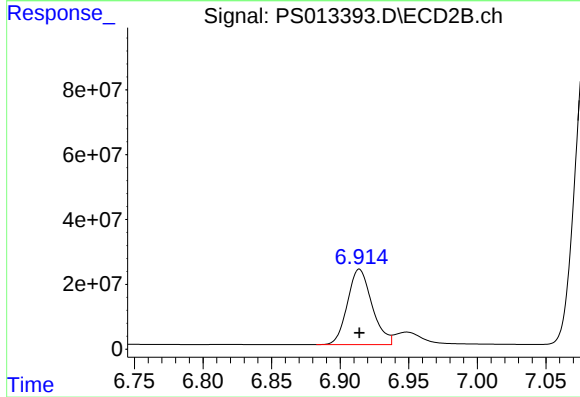

#4 2,4-DCAA


R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 289945615
Conc: 750.00 ng/ml

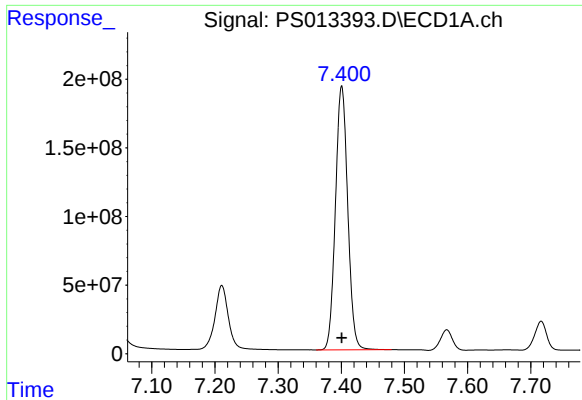

#5 DICAMBA


R.T.: 7.401 min
Delta R.T.: 0.000 min
Response: 2598744795
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

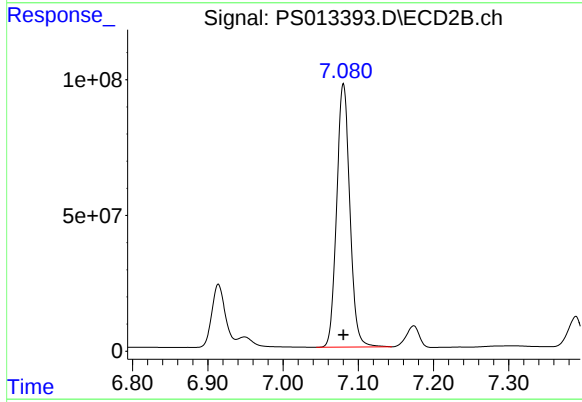


#5 DICAMBA

R.T.: 7.080 min
Delta R.T.: 0.000 min
Response: 1179413385
Conc: 705.00 ng/ml

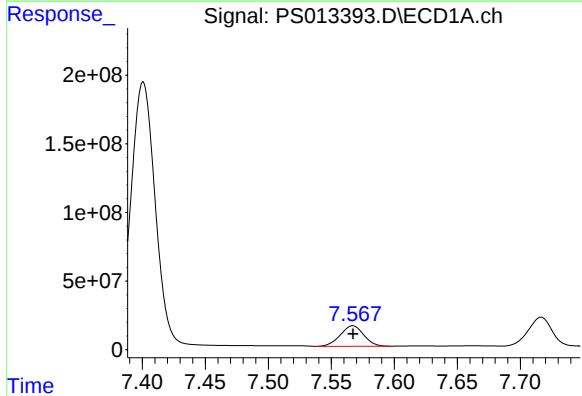


#6 MCP

R.T.: 7.567 min
Delta R.T.: 0.000 min
Response: 193500480
Conc: 70.50 ug/ml

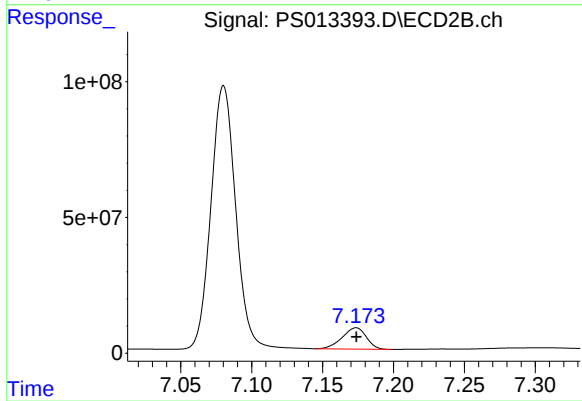

#6 MCP


R.T.: 7.174 min
Delta R.T.: 0.000 min
Response: 93233369
Conc: 70.50 ug/ml

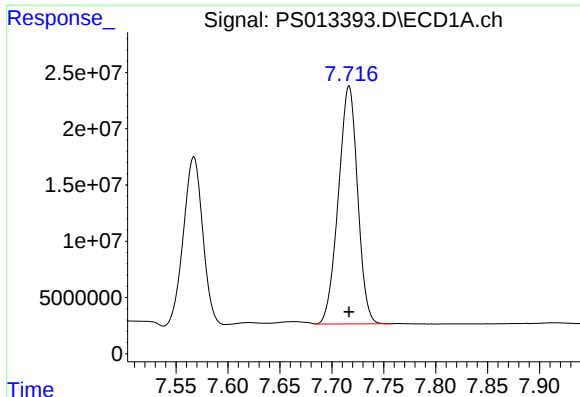

#7 MCPA


R.T.: 7.717 min
Delta R.T.: 0.000 min
Response: 272462528
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

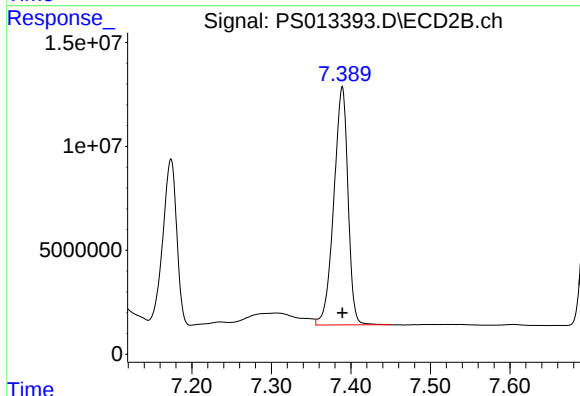


#7 MCPA

R.T.: 7.389 min
Delta R.T.: 0.000 min
Response: 142051590
Conc: 69.75 ug/ml

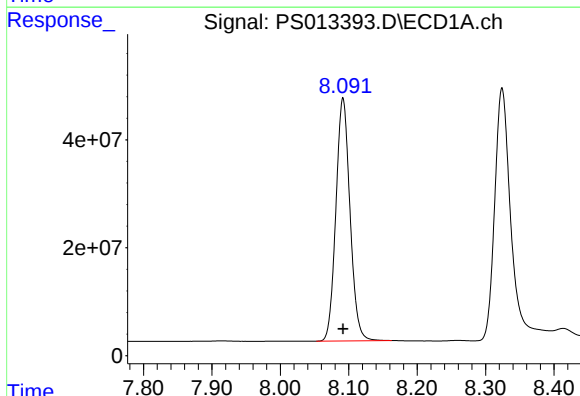


#8 DICHLORPROP

R.T.: 8.092 min
Delta R.T.: 0.000 min
Response: 644569611
Conc: 705.00 ng/ml

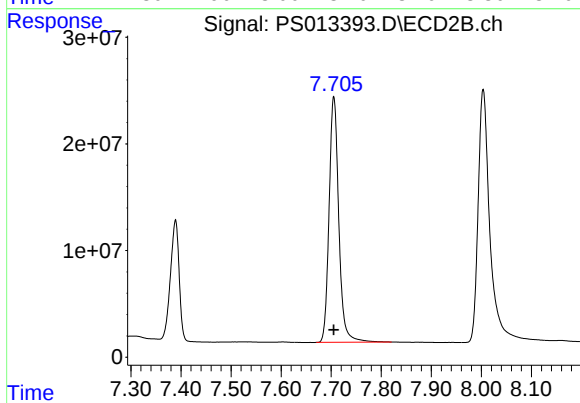

#8 DICHLORPROP


R.T.: 7.705 min
Delta R.T.: 0.000 min
Response: 310047469
Conc: 705.00 ng/ml

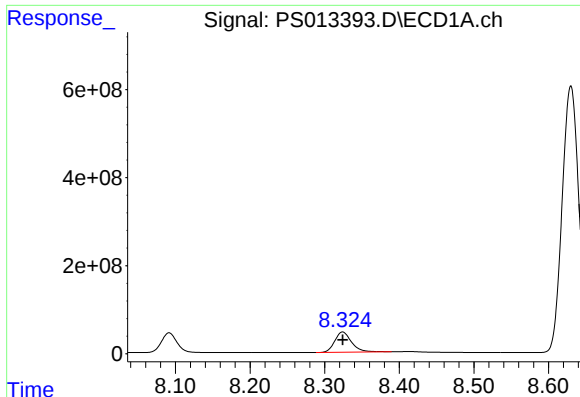

#9 2,4-D


R.T.: 8.324 min
Delta R.T.: 0.000 min
Response: 722660499
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

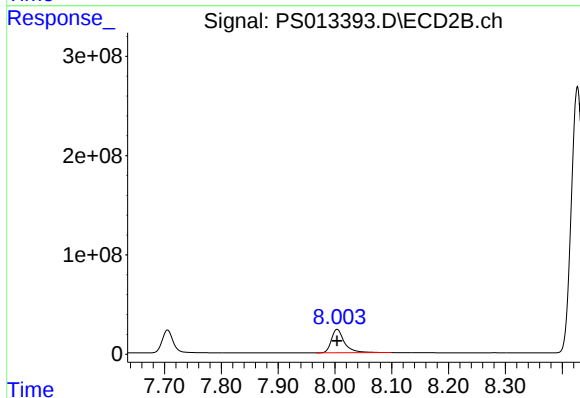


#9 2,4-D

R.T.: 8.004 min
Delta R.T.: 0.000 min
Response: 378714030
Conc: 705.00 ng/ml

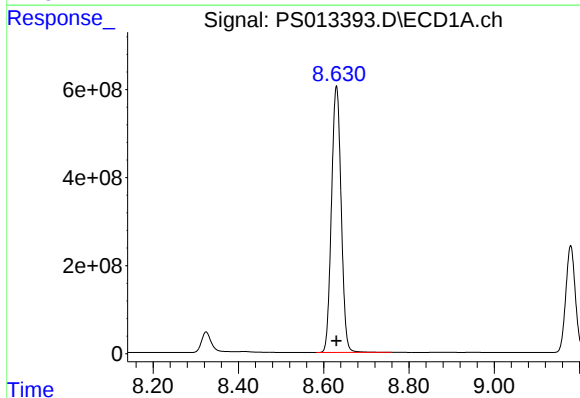


#10 Pentachlorophenol

R.T.: 8.630 min
Delta R.T.: 0.000 min
Response: 9533812225
Conc: 712.50 ng/ml

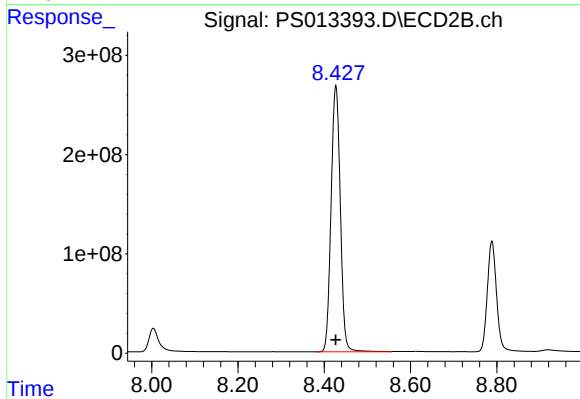

#10 Pentachlorophenol


R.T.: 8.427 min
Delta R.T.: 0.000 min
Response: 3983230809
Conc: 712.50 ng/ml

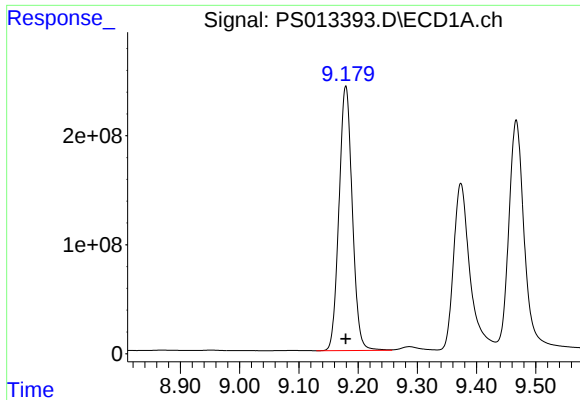

#11 2,4,5-TP (SILVEX)


R.T.: 9.179 min
Delta R.T.: 0.000 min
Response: 3784136941
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

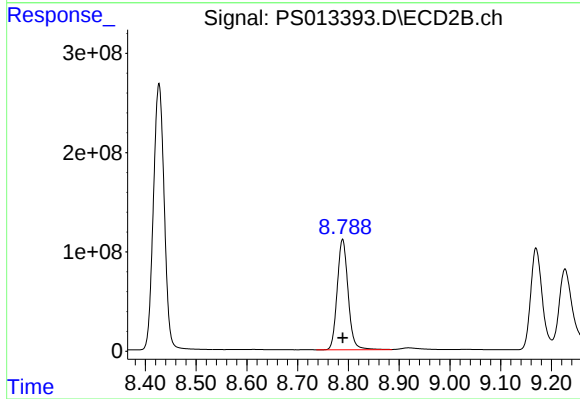


#11 2,4,5-TP (SILVEX)

R.T.: 8.789 min
Delta R.T.: 0.000 min
Response: 1663740879
Conc: 712.50 ng/ml

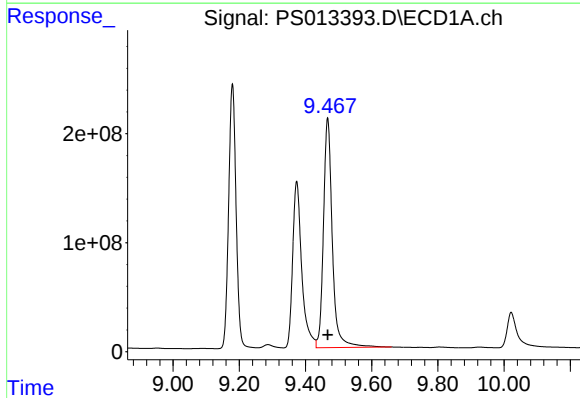


#12 2,4,5-T

R.T.: 9.467 min
Delta R.T.: 0.000 min
Response: 3921316126
Conc: 712.50 ng/ml

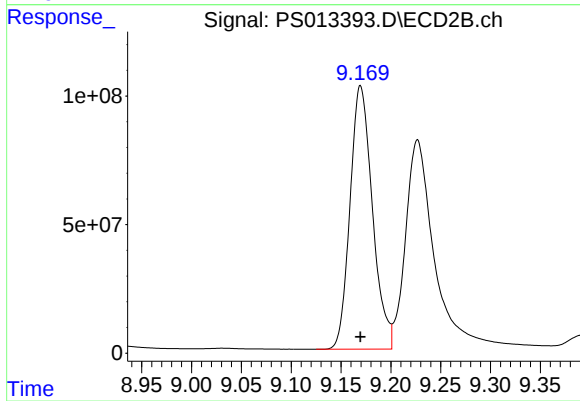

#12 2,4,5-T


R.T.: 9.170 min
Delta R.T.: 0.000 min
Response: 1602966499
Conc: 712.50 ng/ml

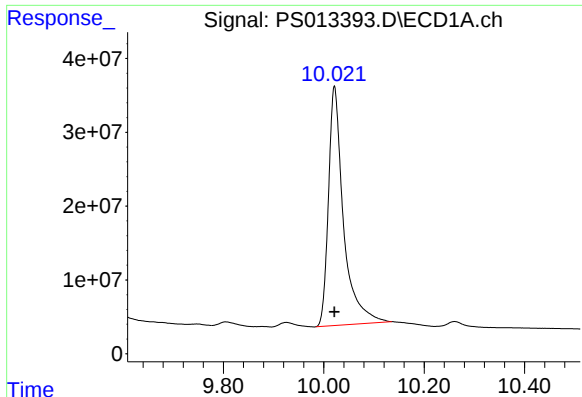

#13 2,4-DB


R.T.: 10.021 min
Delta R.T.: 0.000 min
Response: 674242518
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

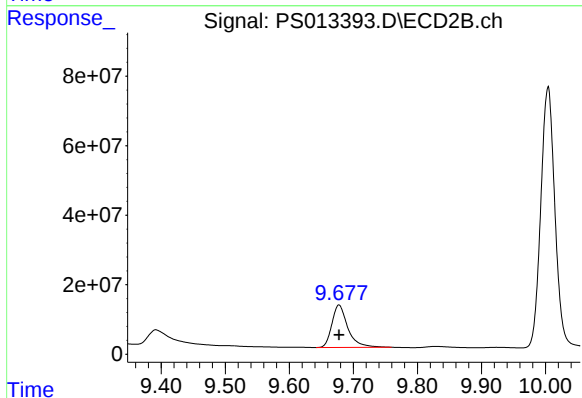


#13 2,4-DB

R.T.: 9.678 min
Delta R.T.: 0.000 min
Response: 210842996
Conc: 712.50 ng/ml

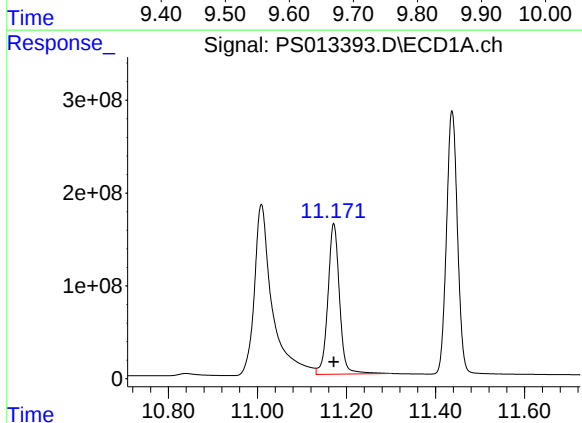


#14 DINOSEB

R.T.: 11.171 min
Delta R.T.: 0.000 min
Response: 2942137863
Conc: 705.00 ng/ml

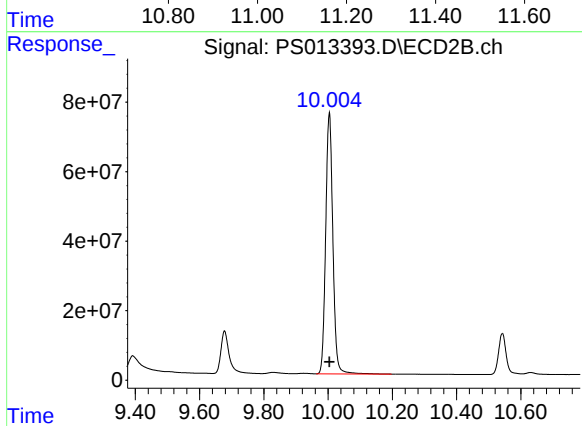

#14 DINOSEB


R.T.: 10.004 min
Delta R.T.: 0.000 min
Response: 1162334580
Conc: 705.00 ng/ml

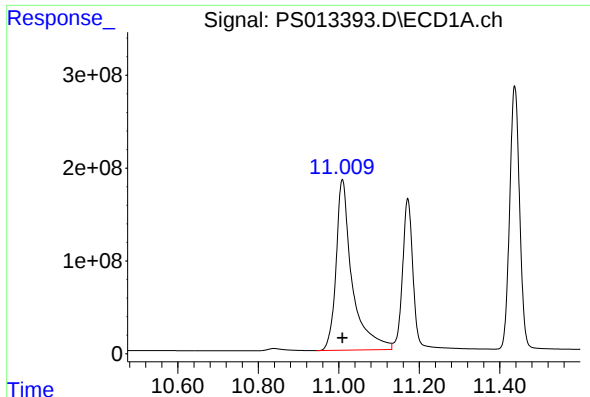

#15 Picloram


R.T.: 11.009 min
Delta R.T.: 0.000 min
Response: 5119024103
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

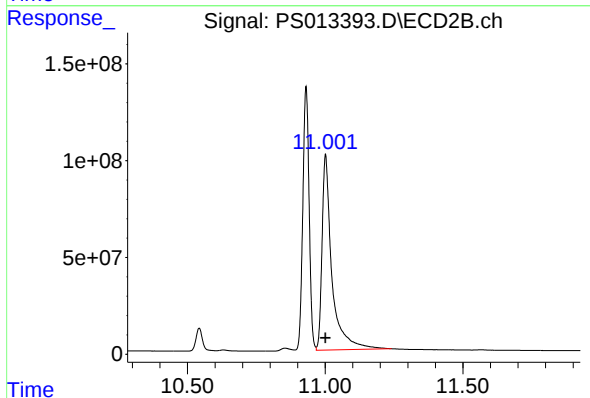


#15 Picloram

R.T.: 11.001 min
Delta R.T.: 0.000 min
Response: 2518326478
Conc: 712.50 ng/ml

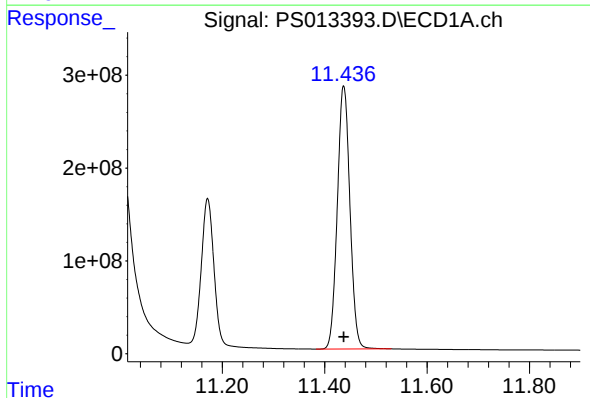

#16 DCPA

R.T.: 11.437 min
Delta R.T.: 0.000 min
Response: 4845063465
Conc: 720.00 ng/ml

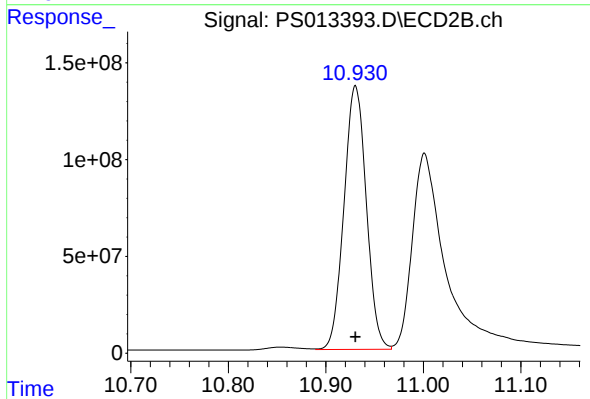

#16 DCPA

R.T.: 10.930 min
Delta R.T.: 0.000 min
Response: 2168347483
Conc: 720.00 ng/ml