

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120220\
 Data File : PS013398.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Dec 2020 20:16
 Operator : DD\AJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 03:04:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 03 02:59:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.211	6.914	704.9E6	297.9E6	757.042	757.260
Target Compounds							
1) T	Dalapon	3.032	2.624	741.3E6	361.9E6	690.061	688.648
2) T	3,5-DICHL...	6.428	6.068	905.1E6	438.1E6	706.154	704.988
3) T	4-Nitroph...	7.046	6.527	312.6E6	167.9E6	693.892	704.371
5) T	DICAMBA	7.401	7.080	2653.3E6	1208.0E6	718.481	718.769
6) T	MCPD	7.567	7.174	198.9E6	95645664	73.253	72.176
7) T	MCPA	7.717	7.389	279.9E6	145.6E6	71.619	70.003
8) T	DICHLORPROP	8.092	7.705	658.5E6	317.7E6	711.507	710.948
9) T	2,4-D	8.325	8.003	736.2E6	386.6E6	731.291	716.539
10) T	Pentachlo...	8.630	8.426	9704.9E6	4064.8E6	724.105	720.831
11) T	2,4,5-TP ...	9.180	8.789	3862.0E6	1701.0E6	724.477	724.523
12) T	2,4,5-T	9.467	9.170	3987.3E6	1644.1E6	721.175	736.914
13) T	2,4-DB	10.021	9.677	690.2E6	217.0E6	751.376	741.776
14) T	DINOSEB	11.171	10.004	2985.2E6	1182.5E6	704.417	715.415
15) T	Picloram	11.008	11.001	5264.3E6	2601.5E6	764.283	747.168
16) T	DCPA	11.437	10.930	4957.2E6	2223.6E6	730.970	731.150



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120220\
Data File : PS013398.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2020 20:16
Operator : DD\AJ
Sample : HSTDCCC750
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 03:04:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
Quant Title : 8080.M
QLast Update : Thu Dec 03 02:59:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

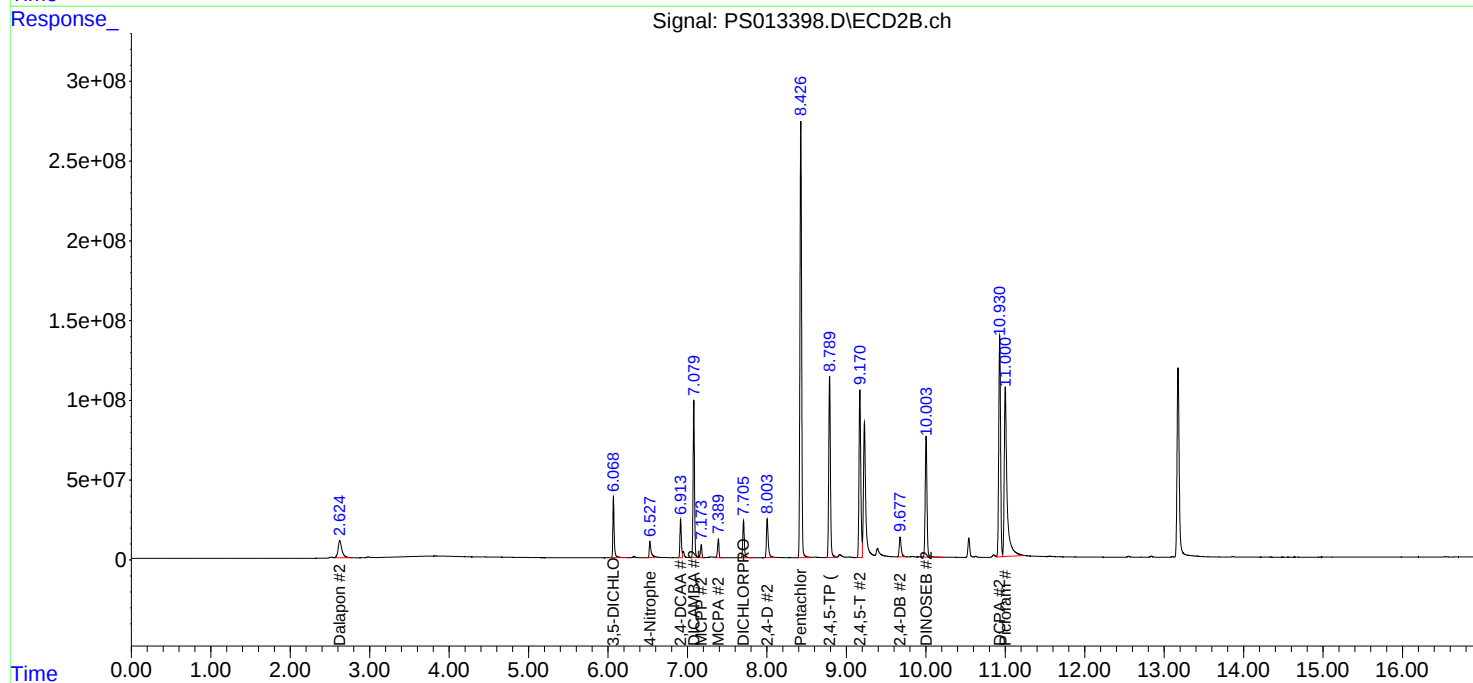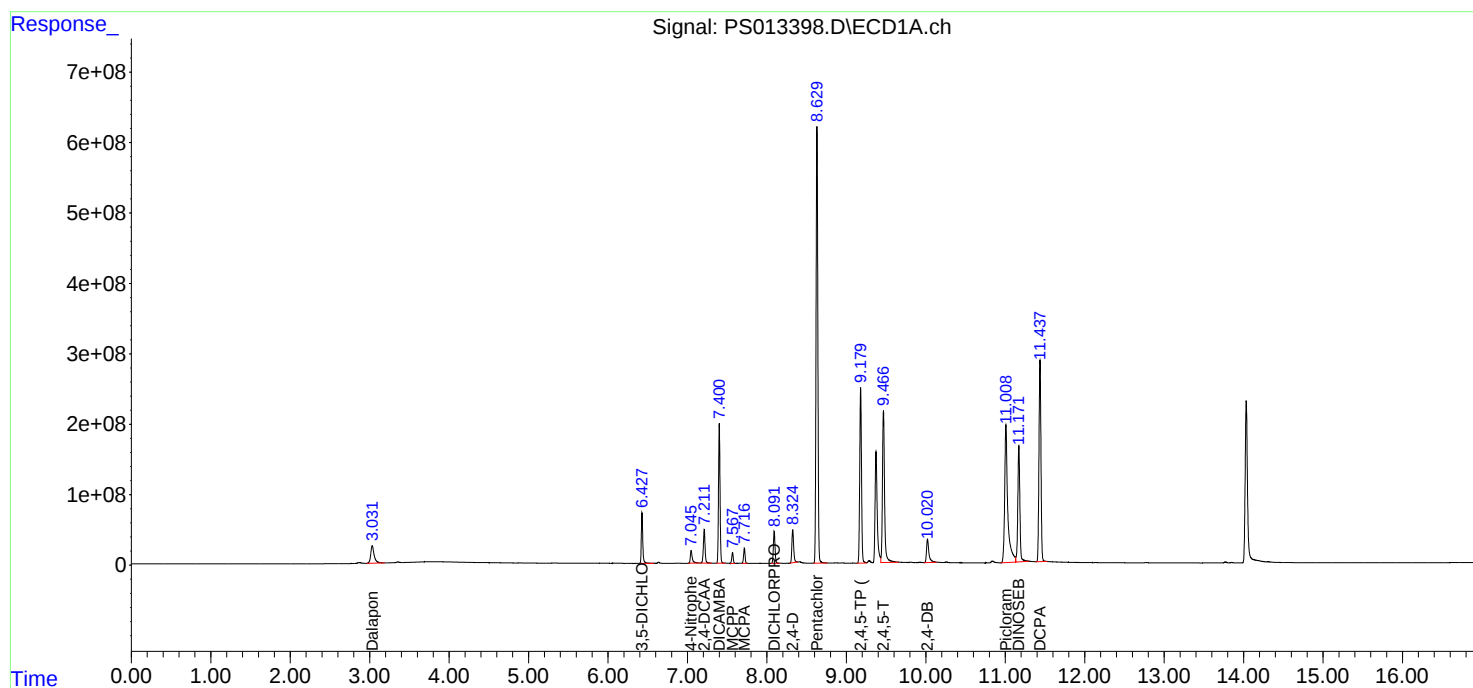


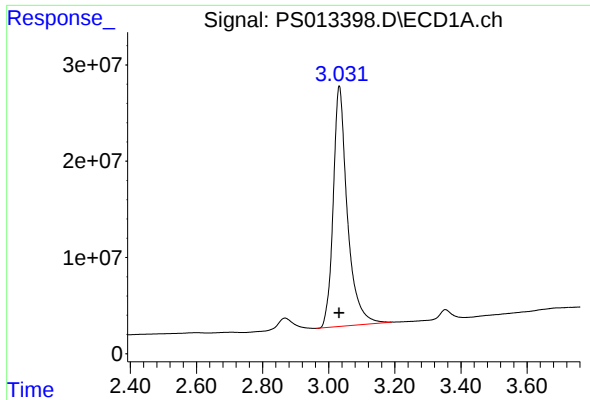

#1 Dalapon


R.T.: 3.032 min
Delta R.T.: 0.000 min
Response: 741265579
Conc: 690.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

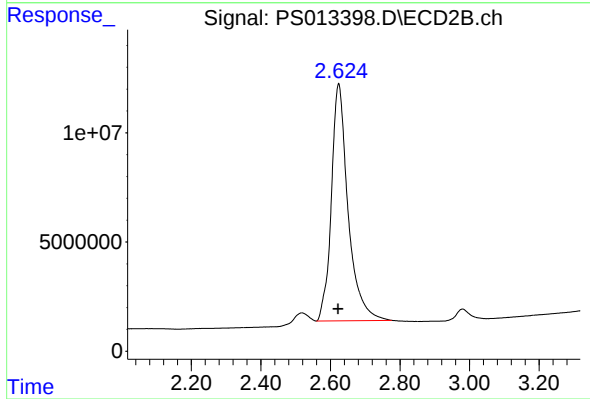


#1 Dalapon

R.T.: 2.624 min
Delta R.T.: 0.002 min
Response: 361905769
Conc: 688.65 ng/ml

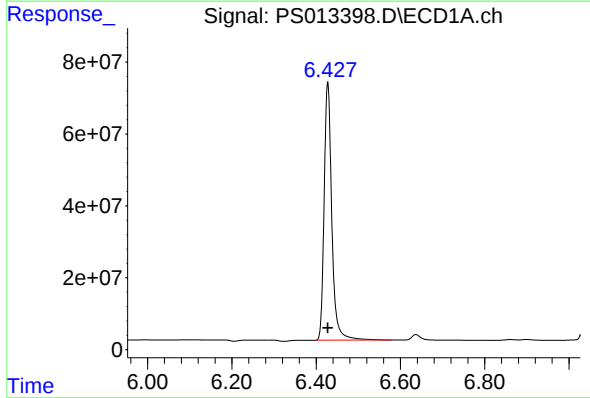


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.428 min
Delta R.T.: 0.000 min
Response: 905082316
Conc: 706.15 ng/ml

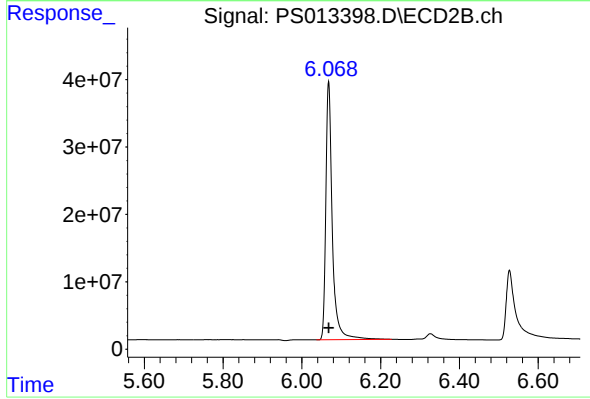

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.068 min
Delta R.T.: 0.000 min
Response: 438056277
Conc: 704.99 ng/ml

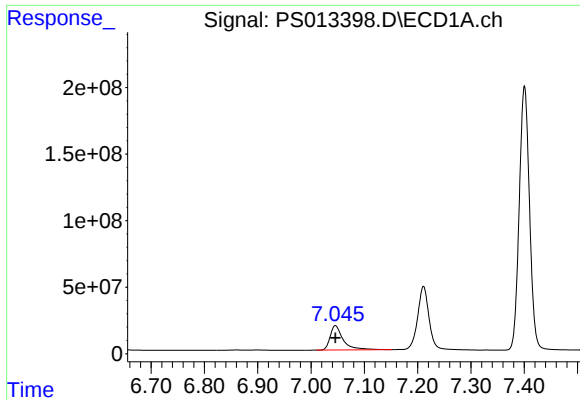

#3 4-Nitrophenol


R.T.: 7.046 min
Delta R.T.: 0.000 min
Response: 312648708
Conc: 693.89 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

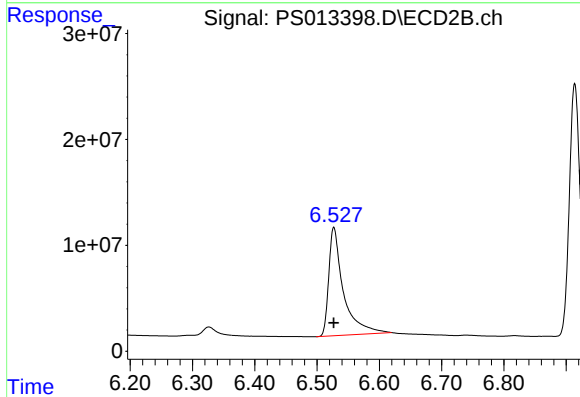


#3 4-Nitrophenol

R.T.: 6.527 min
Delta R.T.: 0.000 min
Response: 167886344
Conc: 704.37 ng/ml

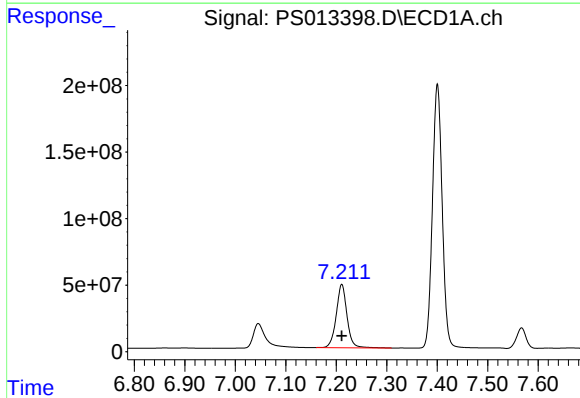


#4 2,4-DCAA

R.T.: 7.211 min
Delta R.T.: 0.000 min
Response: 704850582
Conc: 757.04 ng/ml

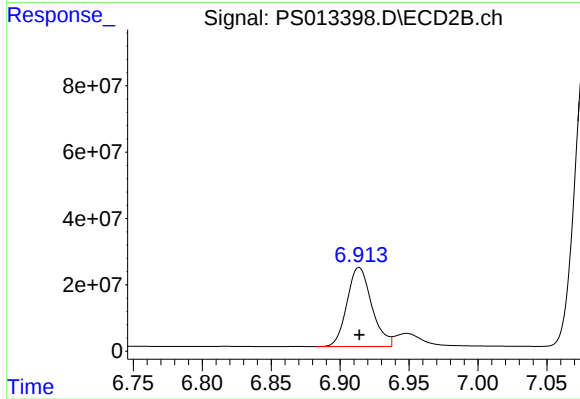

#4 2,4-DCAA


R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 297876658
Conc: 757.26 ng/ml

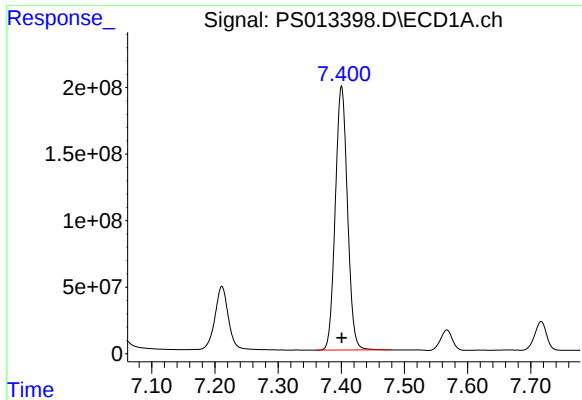

#5 DICAMBA


R.T.: 7.401 min
Delta R.T.: 0.000 min
Response: 2653265330
Conc: 718.48 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

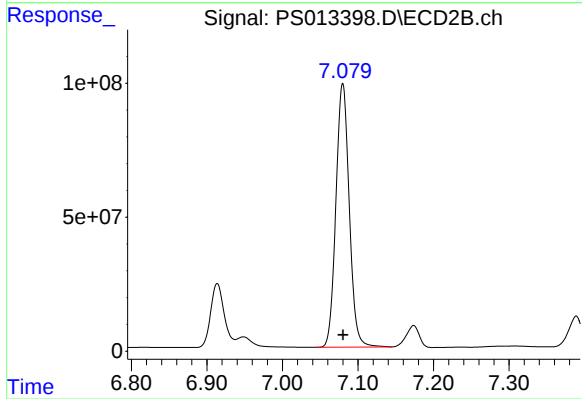


#5 DICAMBA

R.T.: 7.080 min
Delta R.T.: 0.000 min
Response: 1207974397
Conc: 718.77 ng/ml

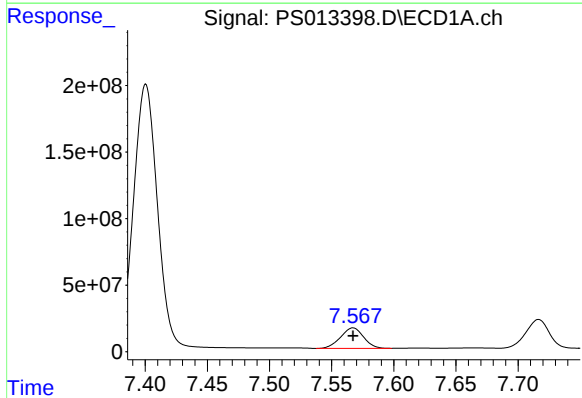


#6 MCP

R.T.: 7.567 min
Delta R.T.: 0.000 min
Response: 198903521
Conc: 73.25 ug/ml

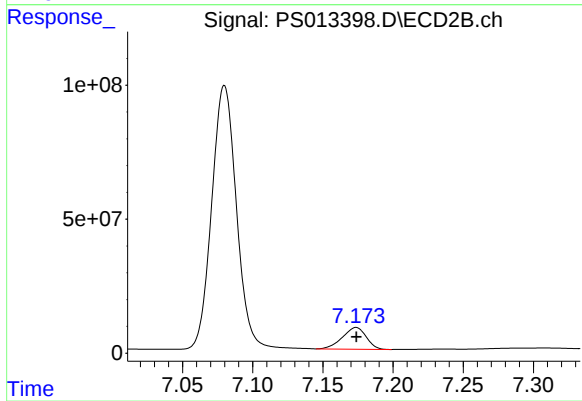

#6 MCP


R.T.: 7.174 min
Delta R.T.: 0.000 min
Response: 95645664
Conc: 72.18 ug/ml

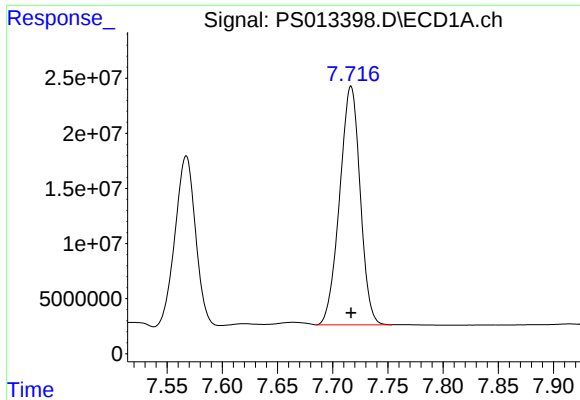

#7 MCPA


R.T.: 7.717 min
Delta R.T.: 0.000 min
Response: 279930959
Conc: 71.62 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

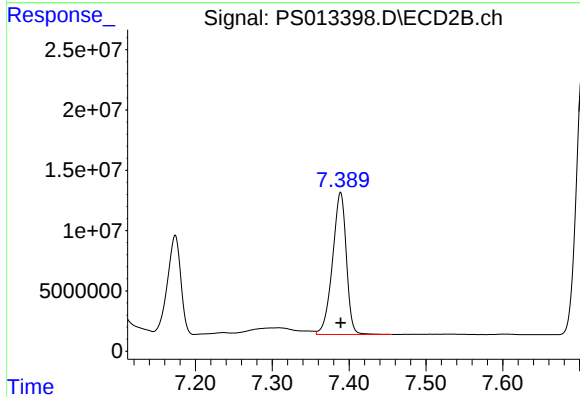


#7 MCPA

R.T.: 7.389 min
Delta R.T.: 0.000 min
Response: 145580712
Conc: 70.00 ug/ml

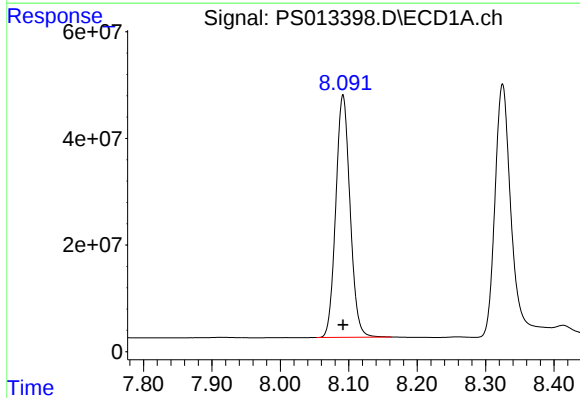


#8 DICHLORPROP

R.T.: 8.092 min
Delta R.T.: 0.000 min
Response: 658539574
Conc: 711.51 ng/ml

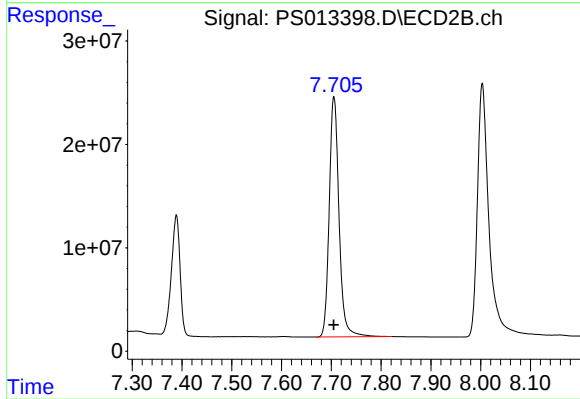

#8 DICHLORPROP


R.T.: 7.705 min
Delta R.T.: 0.000 min
Response: 317731347
Conc: 710.95 ng/ml

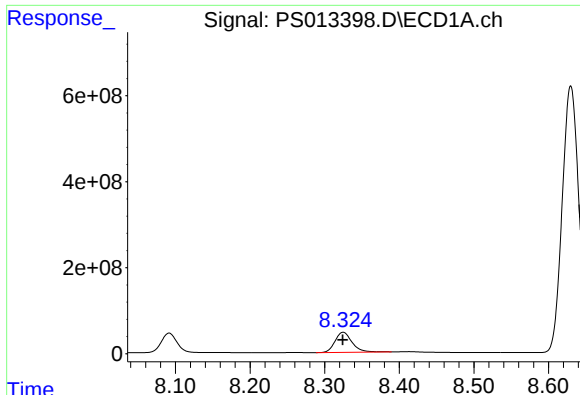

#9 2,4-D


R.T.: 8.325 min
Delta R.T.: 0.000 min
Response: 736164208
Conc: 731.29 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

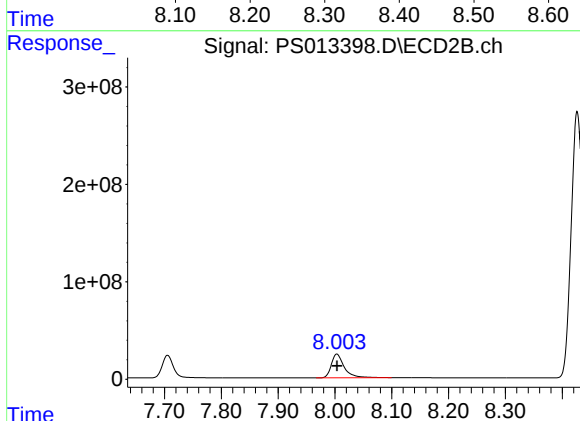


#9 2,4-D

R.T.: 8.003 min
Delta R.T.: 0.000 min
Response: 386642859
Conc: 716.54 ng/ml

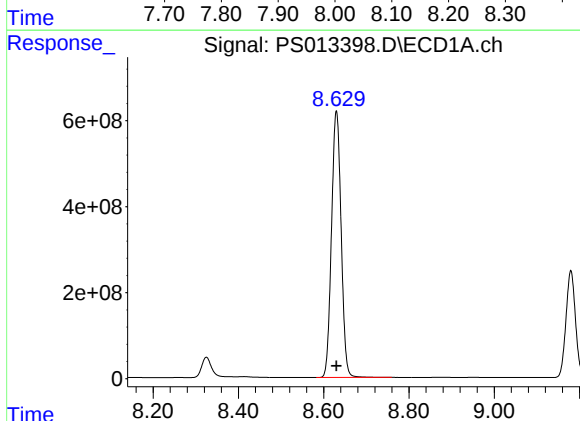


#10 Pentachlorophenol

R.T.: 8.630 min
Delta R.T.: 0.000 min
Response: 9704895284
Conc: 724.11 ng/ml

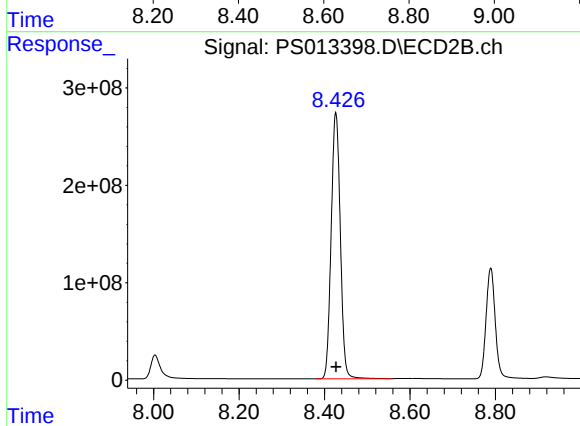

#10 Pentachlorophenol


R.T.: 8.426 min
Delta R.T.: 0.000 min
Response: 4064810674
Conc: 720.83 ng/ml

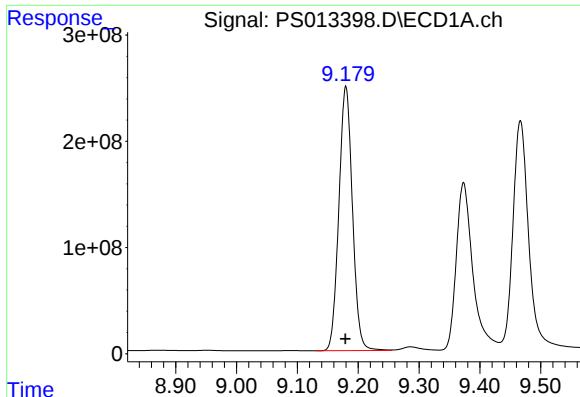

#11 2,4,5-TP (SILVEX)


R.T.: 9.180 min
Delta R.T.: 0.000 min
Response: 3862028454
Conc: 724.48 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

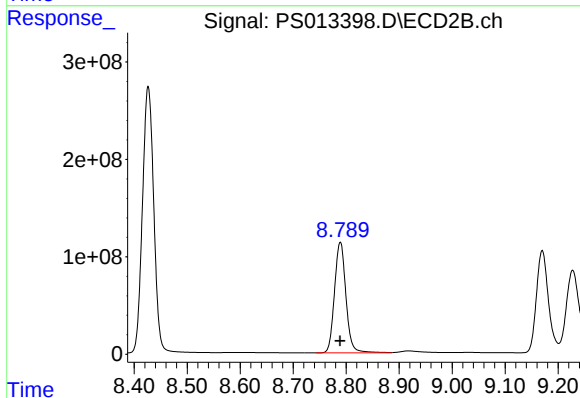


#11 2,4,5-TP (SILVEX)

R.T.: 8.789 min
Delta R.T.: 0.000 min
Response: 1700955495
Conc: 724.52 ng/ml

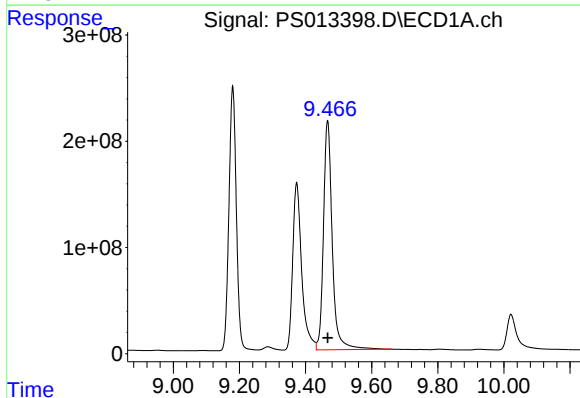


#12 2,4,5-T

R.T.: 9.467 min
Delta R.T.: 0.000 min
Response: 3987296601
Conc: 721.17 ng/ml

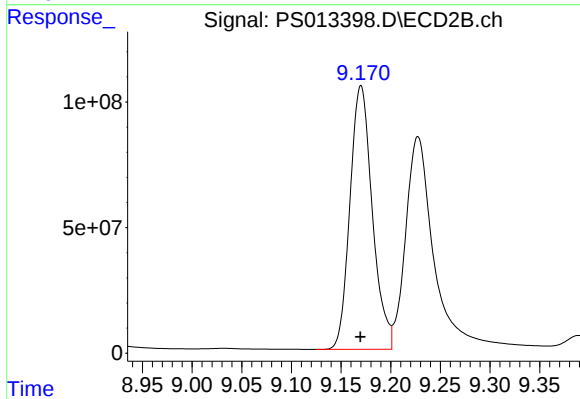

#12 2,4,5-T


R.T.: 9.170 min
Delta R.T.: 0.000 min
Response: 1644116983
Conc: 736.91 ng/ml

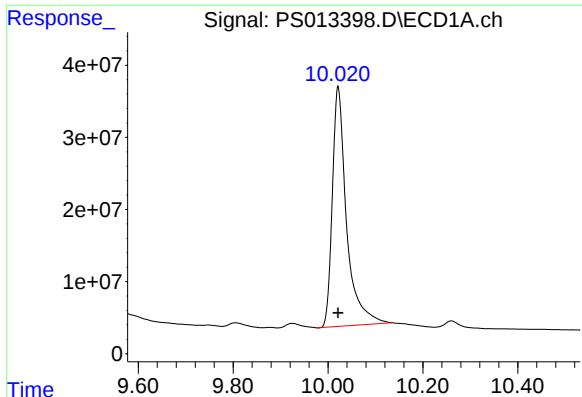

#13 2,4-DB


R.T.: 10.021 min
Delta R.T.: 0.000 min
Response: 690232918
Conc: 751.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

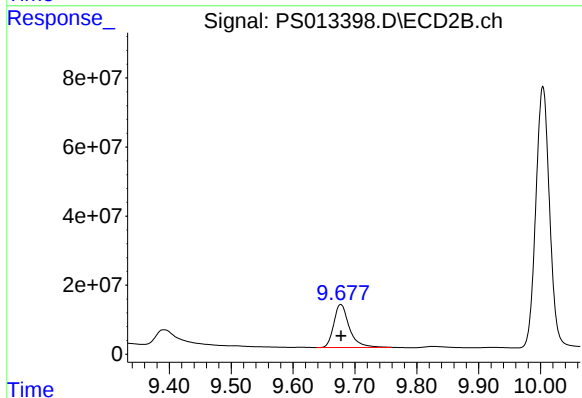


#13 2,4-DB

R.T.: 9.677 min
Delta R.T.: 0.000 min
Response: 216960140
Conc: 741.78 ng/ml

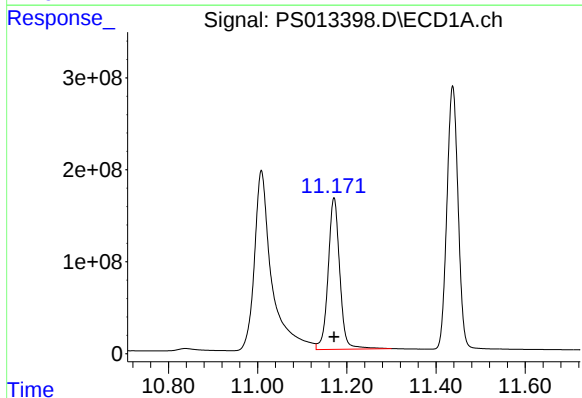


#14 DINOSEB

R.T.: 11.171 min
Delta R.T.: 0.000 min
Response: 2985209715
Conc: 704.42 ng/ml

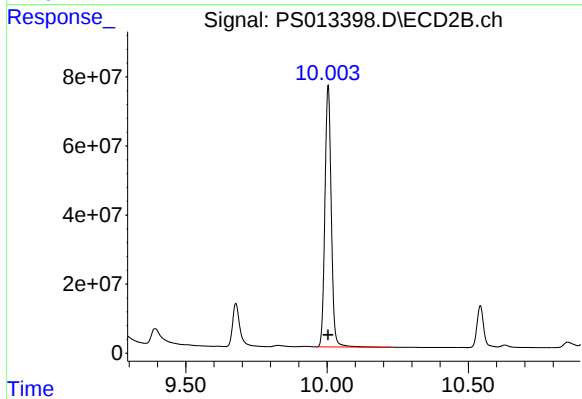

#14 DINOSEB


R.T.: 10.004 min
Delta R.T.: 0.000 min
Response: 1182505352
Conc: 715.41 ng/ml

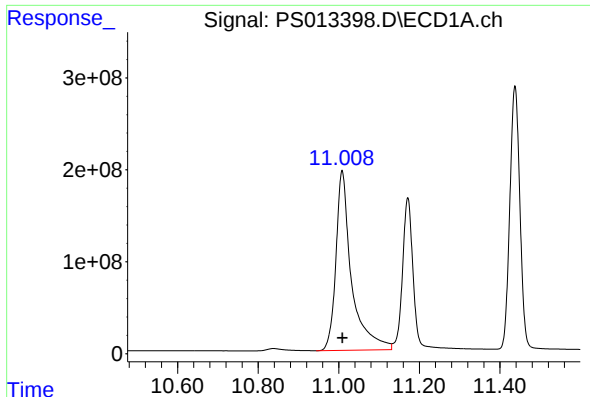

#15 Picloram


R.T.: 11.008 min
Delta R.T.: 0.000 min
Response: 5264344290
Conc: 764.28 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

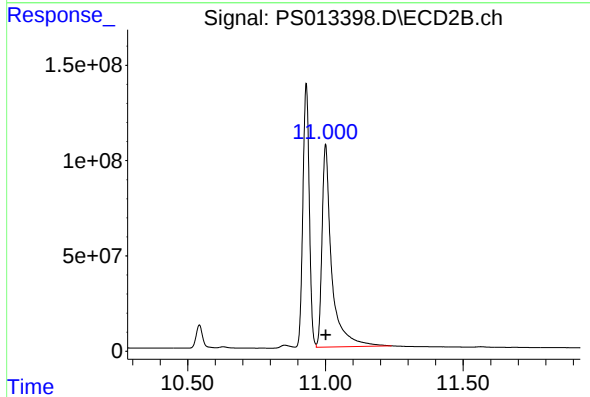


#15 Picloram

R.T.: 11.001 min
Delta R.T.: 0.000 min
Response: 2601473162
Conc: 747.17 ng/ml

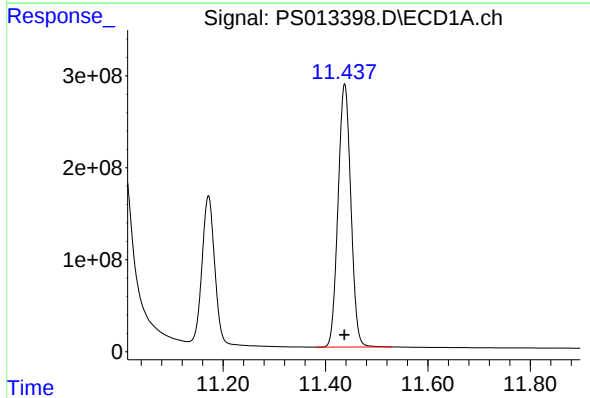

#16 DCPA

R.T.: 11.437 min
Delta R.T.: 0.000 min
Response: 4957184664
Conc: 730.97 ng/ml

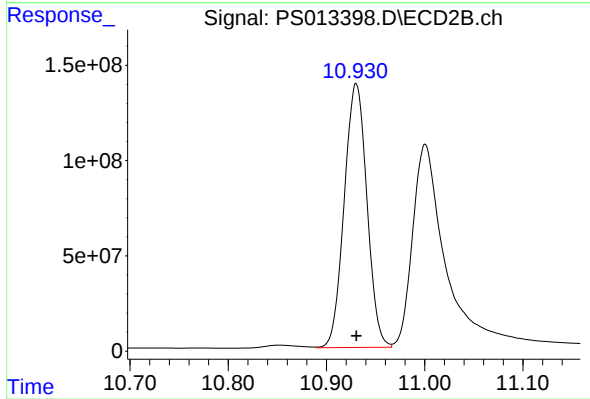

#16 DCPA

R.T.: 10.930 min
Delta R.T.: 0.000 min
Response: 2223607849
Conc: 731.15 ng/ml