

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120222\
 Data File : PS021283.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Dec 2022 12:58
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 04:41:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111622.M
 Quant Title : 8080.M
 QLast Update : Thu Nov 17 00:46:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.408	6.841	1040.4E6	829.4E6	478.479	548.490
Target Compounds							
1) T	Dalapon	2.536	0.000	674967	0	<MDL	N.D. #
3) T	4-Nitroph...	6.253	0.000	4624303	0	3.423	N.D. #
7) T	MCPA	6.794f	0.000	10665785	0	1.110	N.D. #
10) T	Pentachlo...	7.588	8.356	649340	415480	<MDL	<MDL #
11) T	2,4,5-TP ...	8.121	8.696	8781261	6272817	<MDL	<MDL #
12) T	2,4,5-T	8.364	9.138f	4025865	1311487	<MDL	<MDL #
13) T	2,4-DB	8.893	9.556f	-235200	1787032	N.D.	1.527
14) T	DINOSEB	9.881f	0.000	24746616	0	2.158	N.D. #
15) T	Picloram	0.000	10.877	0	889455	N.D.	<MDL
16) T	DCPA	10.206	10.877	1064702	889455	<MDL	<MDL #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120222\
Data File : PS021283.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2022 12:58
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 04:41:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111622.M
Quant Title : 8080.M
QLast Update : Thu Nov 17 00:46:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

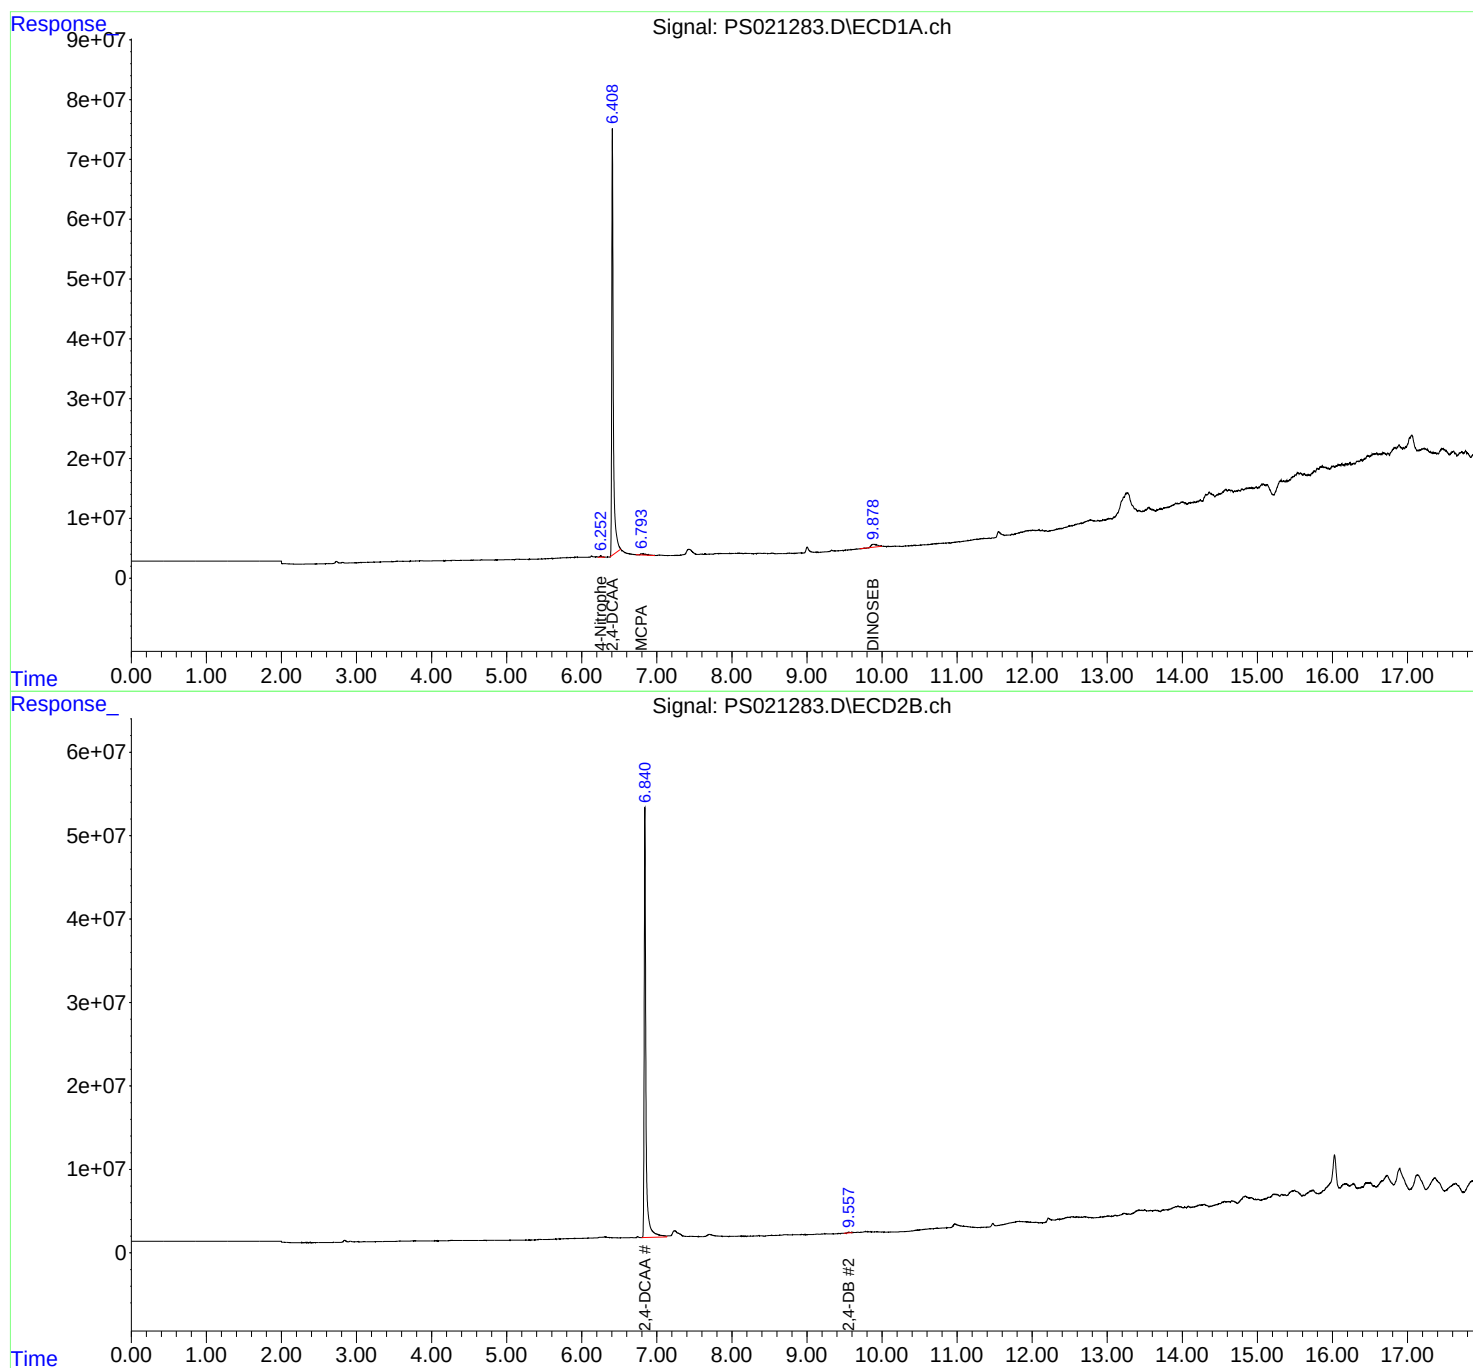


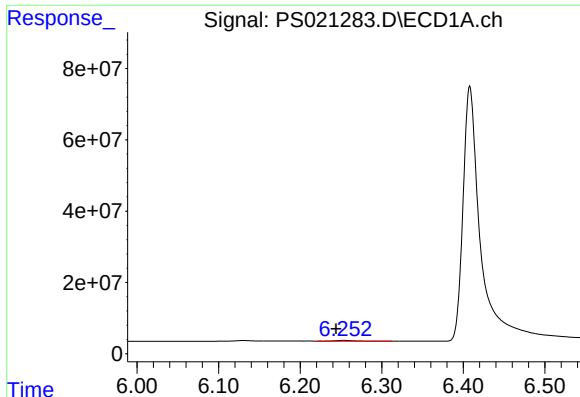

#3 4-Nitrophenol


R.T.: 6.253 min
Delta R.T.: 0.009 min
Response: 4624303
Conc: 3.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

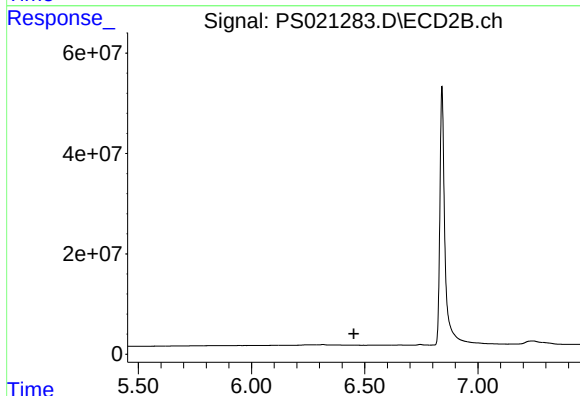


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.452 min
Response: 0
Conc: N.D.

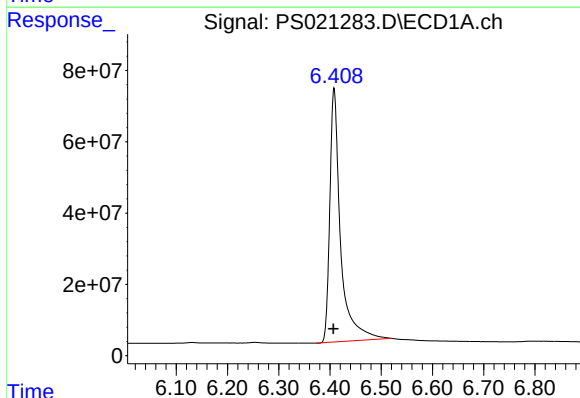


#4 2,4-DCAA

R.T.: 6.408 min
Delta R.T.: 0.001 min
Response: 1040353969
Conc: 478.48 ng/ml

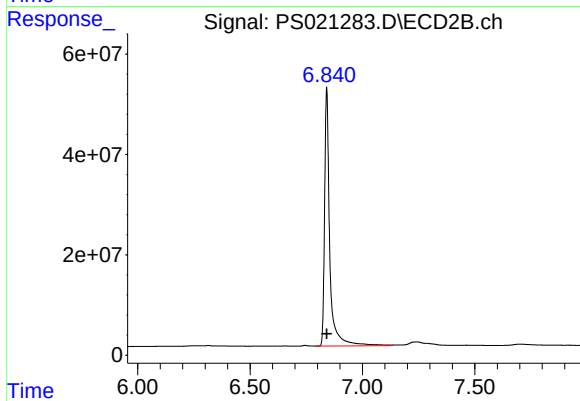

#4 2,4-DCAA


R.T.: 6.841 min
Delta R.T.: 0.000 min
Response: 829381337
Conc: 548.49 ng/ml

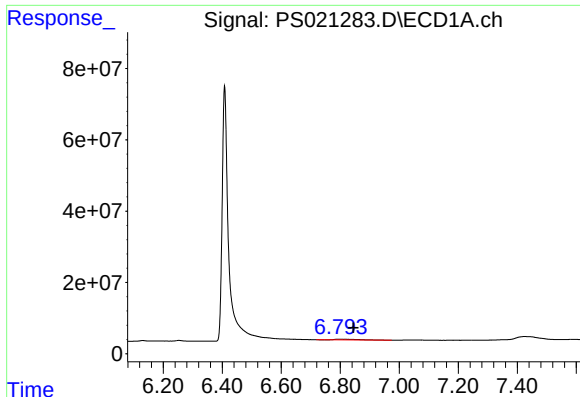

#7 MCPA


R.T.: 6.794 min
Delta R.T.: -0.051 min
Response: 10665785
Conc: 1.11 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

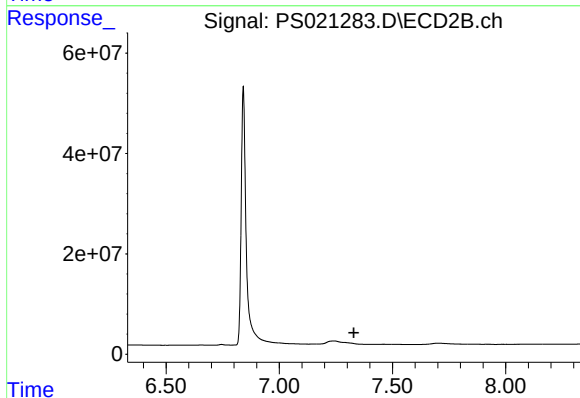


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.330 min
Response: 0
Conc: N.D.

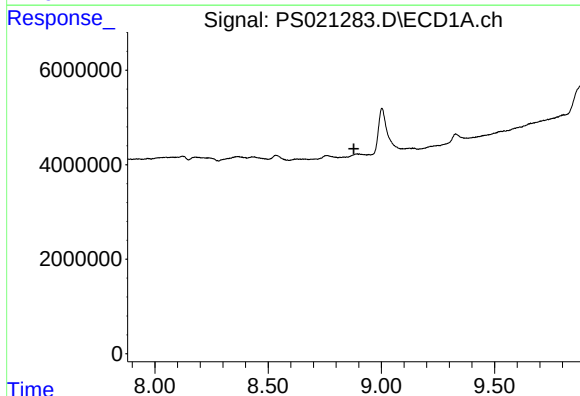


#13 2,4-DB

R.T.: 8.893 min
Delta R.T.: 0.014 min
Response: -235200
Conc: N.D.

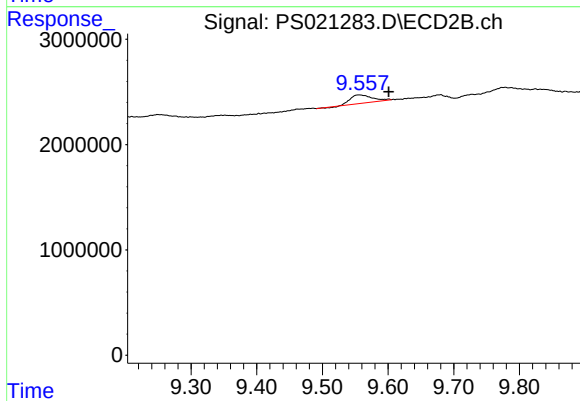

#13 2,4-DB


R.T.: 9.556 min
Delta R.T.: -0.044 min
Response: 1787032
Conc: 1.53 ng/ml

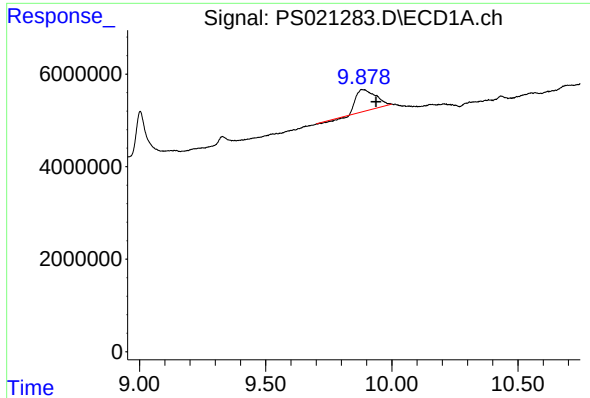

#14 DINOSEB

R.T.: 9.881 min
Delta R.T.: -0.056 min
Response: 24746616
Conc: 2.16 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

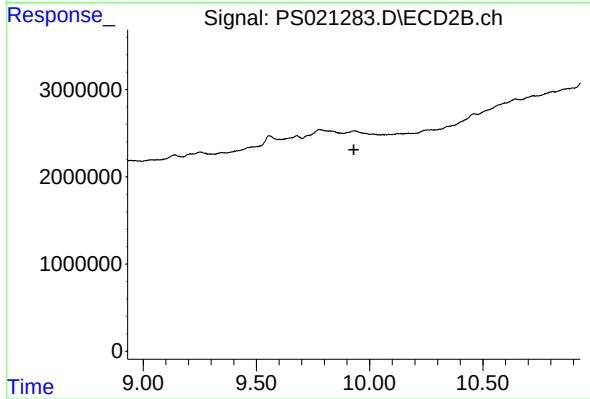

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.930 min
Response: 0
Conc: N.D.