

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120222\
 Data File : PS021307.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Dec 2022 23:50
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 04:49:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111622.M
 Quant Title : 8080.M
 QLast Update : Thu Nov 17 00:46:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.405	6.838	1132.5E6	838.7E6	520.838	554.646
Target Compounds							
1) T	Dalapon	2.467	0.000	820047	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.790	6.033	190118	653804	<MDL	<MDL #
3) T	4-Nitroph...	6.244	6.435	5090214	688402	3.768	<MDL #
5) T	DICAMBA	6.618f	7.005	3502119	2067667	<MDL	<MDL #
6) T	MCPD	6.749	7.062f	20543196	1944850	3.041	<MDL #
7) T	MCPA	6.817	7.374f	389478	794203	<MDL	<MDL #
8) T	DICHLORPROP	7.205f	7.652	-1591594	27892411	N.D.	16.336
9) T	2,4-D	0.000	7.922	0	1123500	N.D.	<MDL
10) T	Pentachlo...	0.000	8.383	0	3858726	N.D.	<MDL
11) T	2,4,5-TP ...	8.127	8.744	47190923	12538961	3.408	1.260 #
12) T	2,4,5-T	8.351	9.097	4350592	51935859	<MDL	5.596 #
13) T	2,4-DB	8.894	9.607	5615618	8784536	2.457	7.504 #
14) T	DINOSEB	9.977	0.000	1066818	0	<MDL	N.D. #
15) T	Picloram	9.793	10.909	13065633	43345479	<MDL	3.358 #
16) T	DCPA	10.190	10.909f	1594946	43345479	<MDL	3.620 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120222\
Data File : PS021307.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2022 23:50
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 04:49:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111622.M
Quant Title : 8080.M
QLast Update : Thu Nov 17 00:46:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

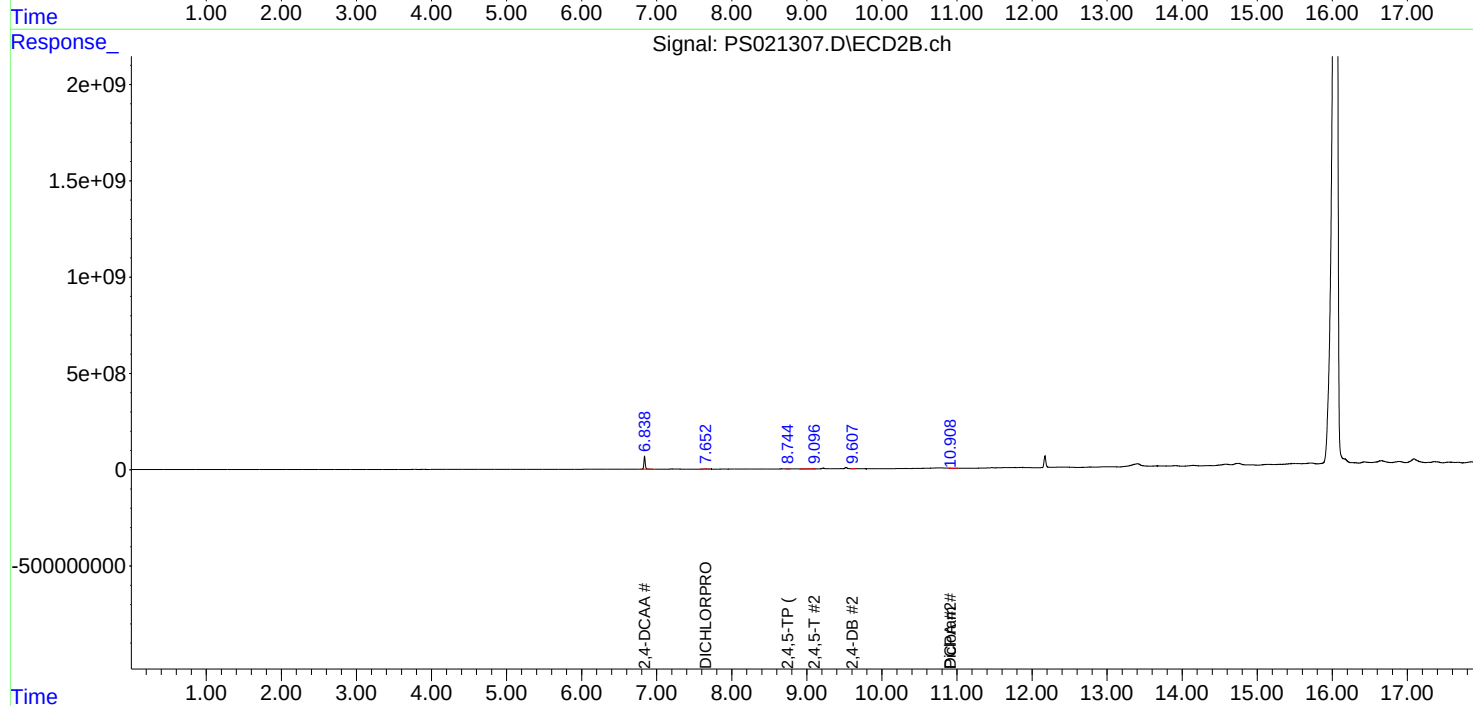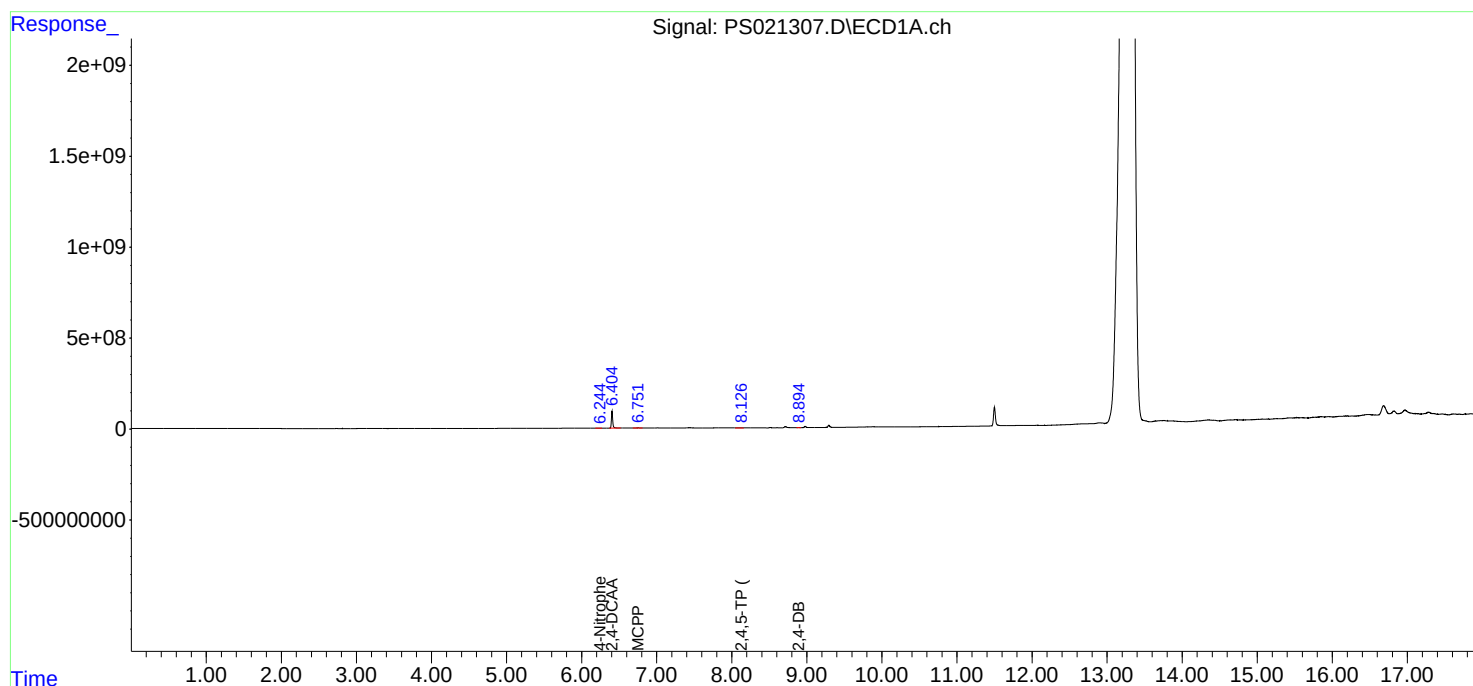


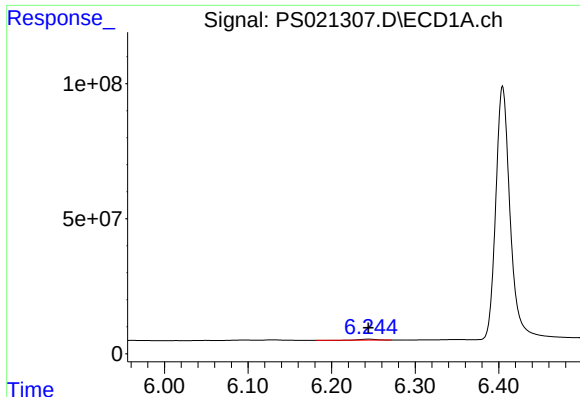

#3 4-Nitrophenol


R.T.: 6.244 min
Delta R.T.: 0.000 min
Response: 5090214
Conc: 3.77 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

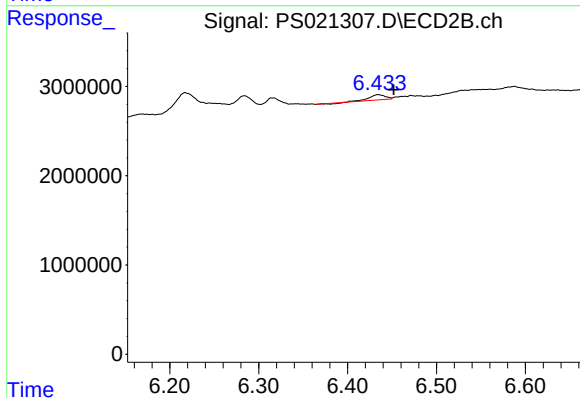


#3 4-Nitrophenol

R.T.: 6.435 min
Delta R.T.: -0.017 min
Response: 688402
Conc: N.D.

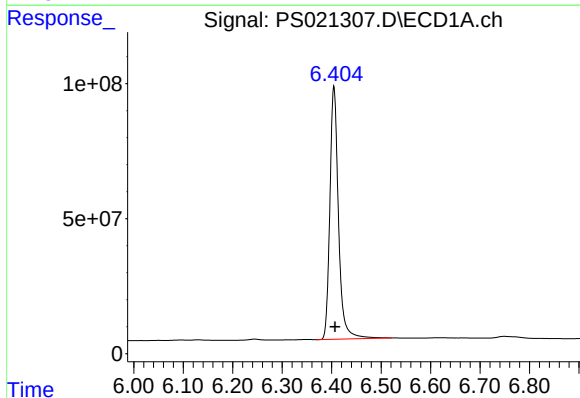


#4 2,4-DCAA

R.T.: 6.405 min
Delta R.T.: -0.002 min
Response: 1132456138
Conc: 520.84 ng/ml

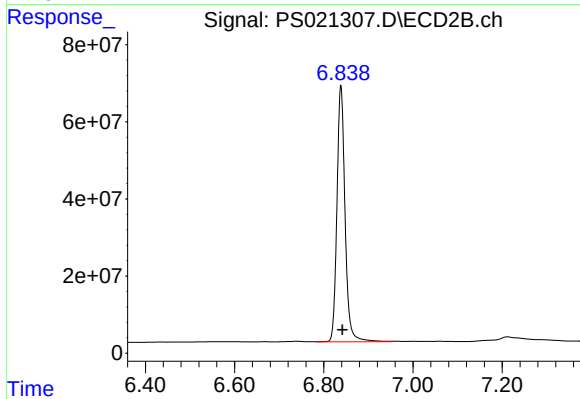

#4 2,4-DCAA


R.T.: 6.838 min
Delta R.T.: -0.003 min
Response: 838690557
Conc: 554.65 ng/ml

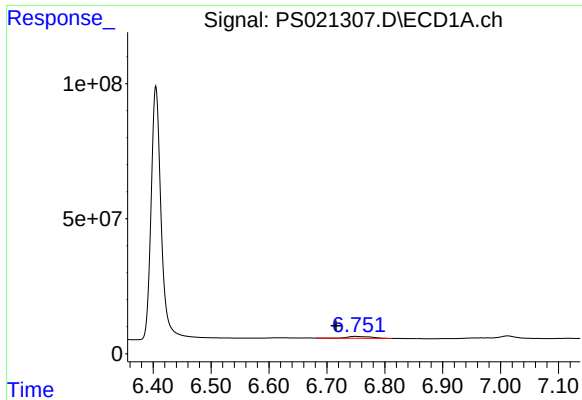

#6 MCP


R.T.: 6.749 min
Delta R.T.: 0.033 min
Response: 20543196
Conc: 3.04 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

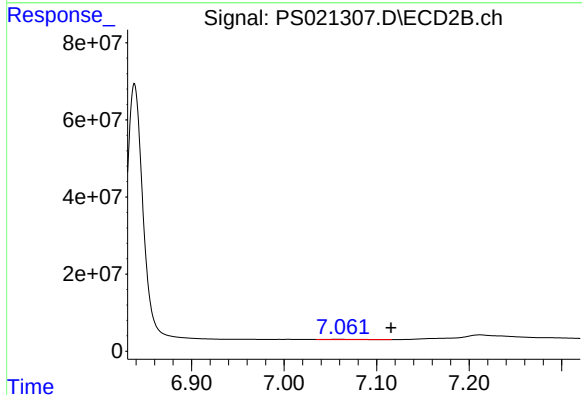


#6 MCP

R.T.: 7.062 min
Delta R.T.: -0.054 min
Response: 1944850
Conc: N.D.

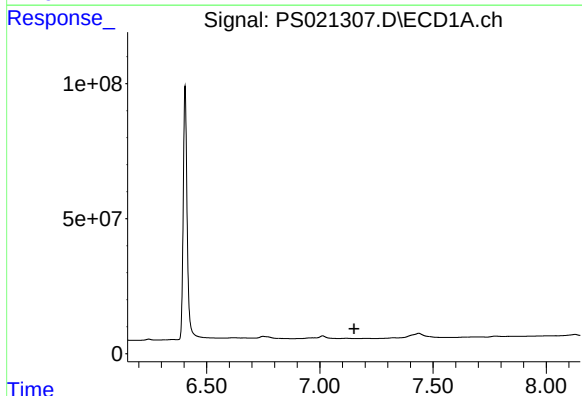


#8 DICHLORPROP

R.T.: 7.205 min
Delta R.T.: 0.054 min
Response: -1591594
Conc: N.D.

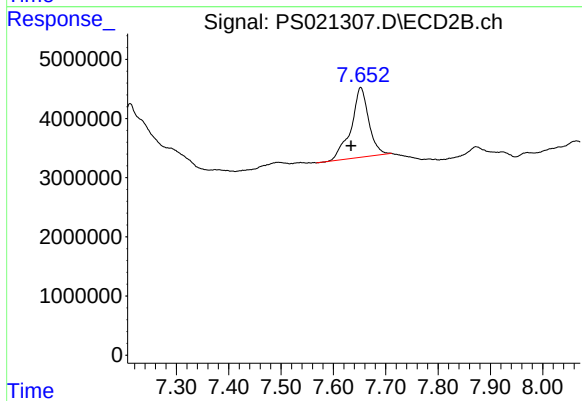

#8 DICHLORPROP


R.T.: 7.652 min
Delta R.T.: 0.018 min
Response: 27892411
Conc: 16.34 ng/ml

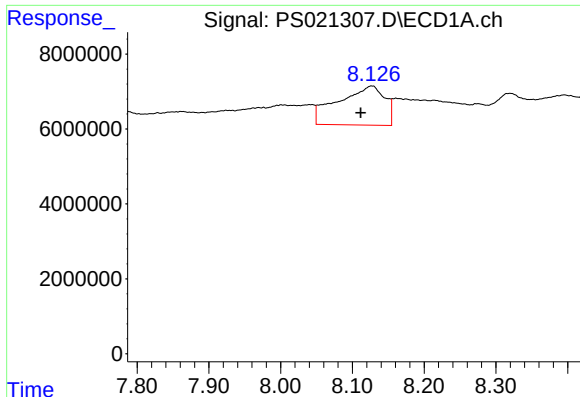

#11 2,4,5-TP (SILVEX)


R.T.: 8.127 min
Delta R.T.: 0.016 min
Response: 47190923
Conc: 3.41 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

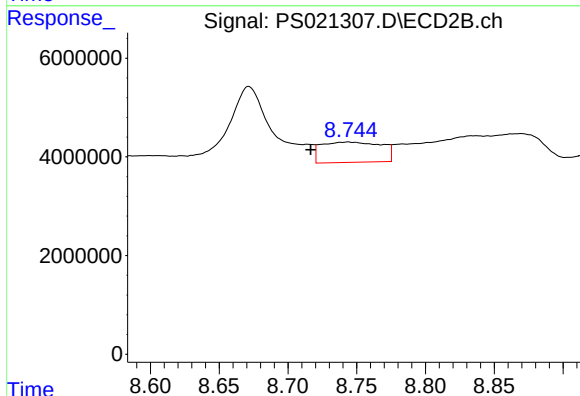


#11 2,4,5-TP (SILVEX)

R.T.: 8.744 min
Delta R.T.: 0.027 min
Response: 12538961
Conc: 1.26 ng/ml

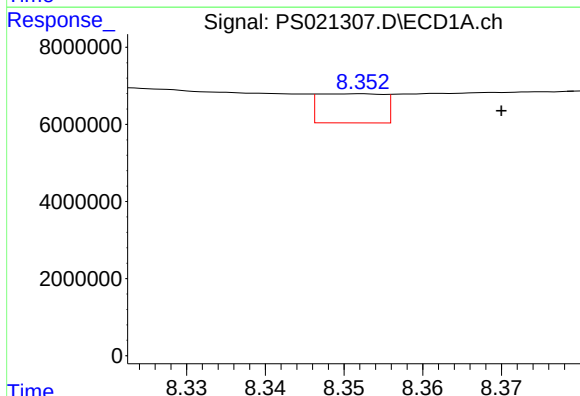


#12 2,4,5-T

R.T.: 8.351 min
Delta R.T.: -0.019 min
Response: 4350592
Conc: N.D.

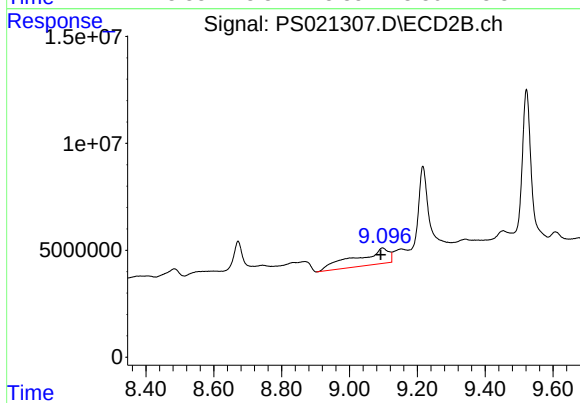

#12 2,4,5-T


R.T.: 9.097 min
Delta R.T.: 0.005 min
Response: 51935859
Conc: 5.60 ng/ml

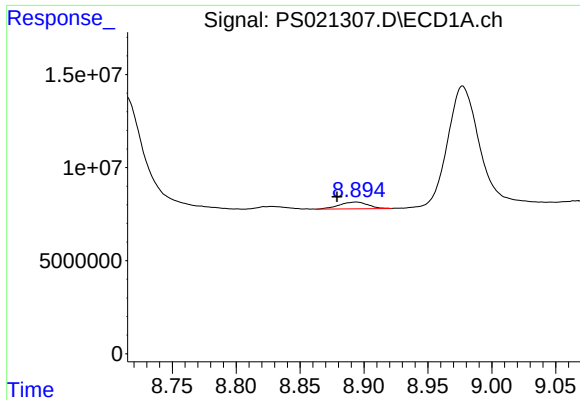

#13 2,4-DB


R.T.: 8.894 min
Delta R.T.: 0.015 min
Response: 5615618
Conc: 2.46 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

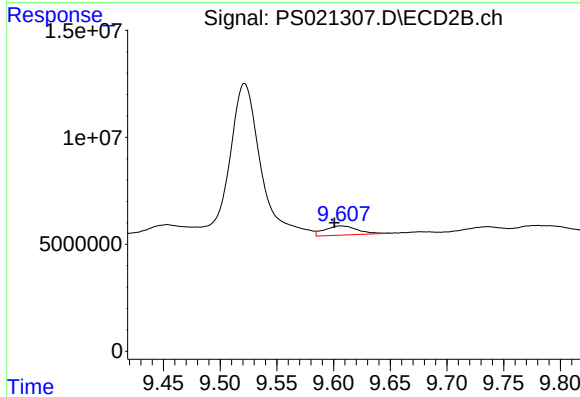


#13 2,4-DB

R.T.: 9.607 min
Delta R.T.: 0.006 min
Response: 8784536
Conc: 7.50 ng/ml

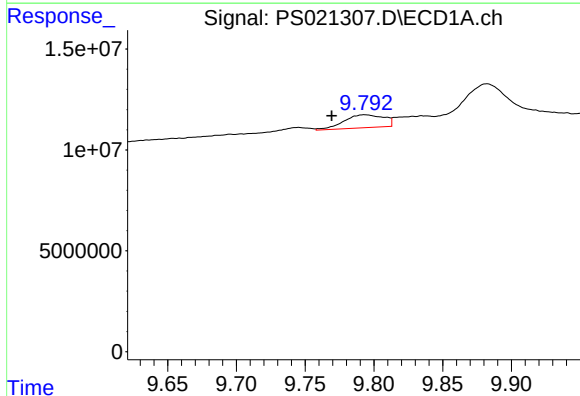


#15 Picloram

R.T.: 9.793 min
Delta R.T.: 0.024 min
Response: 13065633
Conc: N.D.

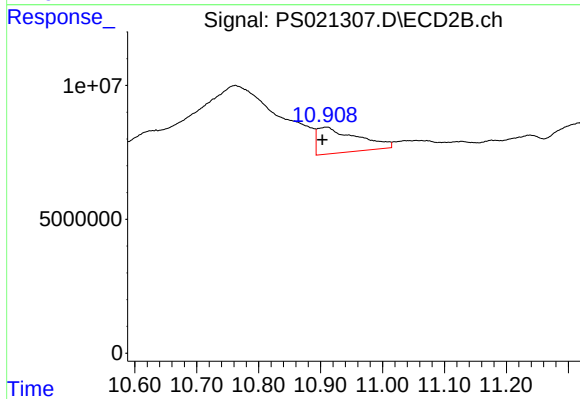

#15 Picloram


R.T.: 10.909 min
Delta R.T.: 0.006 min
Response: 43345479
Conc: 3.36 ng/ml

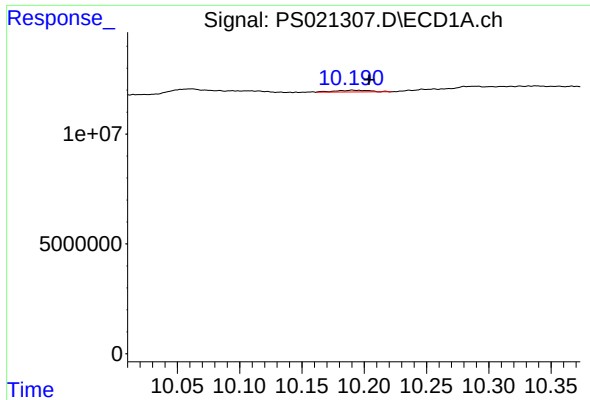

#16 DCPA

R.T.: 10.190 min
Delta R.T.: -0.014 min
Response: 1594946
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

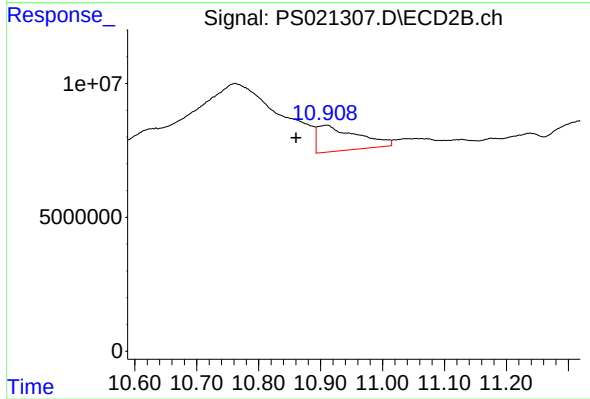

#16 DCPA

R.T.: 10.909 min
Delta R.T.: 0.049 min
Response: 43345479
Conc: 3.62 ng/ml