

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120222\
 Data File : PS021287.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Dec 2022 14:34
 Operator : AR\AJ
 Sample : N5795-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-10

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/06/2022
 Supervised By :Ankita Jodhani 12/06/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 05 08:48:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111622.M
 Quant Title : 8080.M
 QLast Update : Thu Nov 17 00:46:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.403	6.838	1132.0E6	670.4E6	520.636	443.382
Target Compounds							
13) T	2,4-DB	8.896	9.611	16895.7E6	18259.8E6	7392.284m	15597.762 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120222\
Data File : PS021287.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2022 14:34
Operator : AR\AJ
Sample : N5795-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
TP-10


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/06/2022
Supervised By : Ankita Jodhani 12/06/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 05 08:48:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111622.M
Quant Title : 8080.M
QLast Update : Thu Nov 17 00:46:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

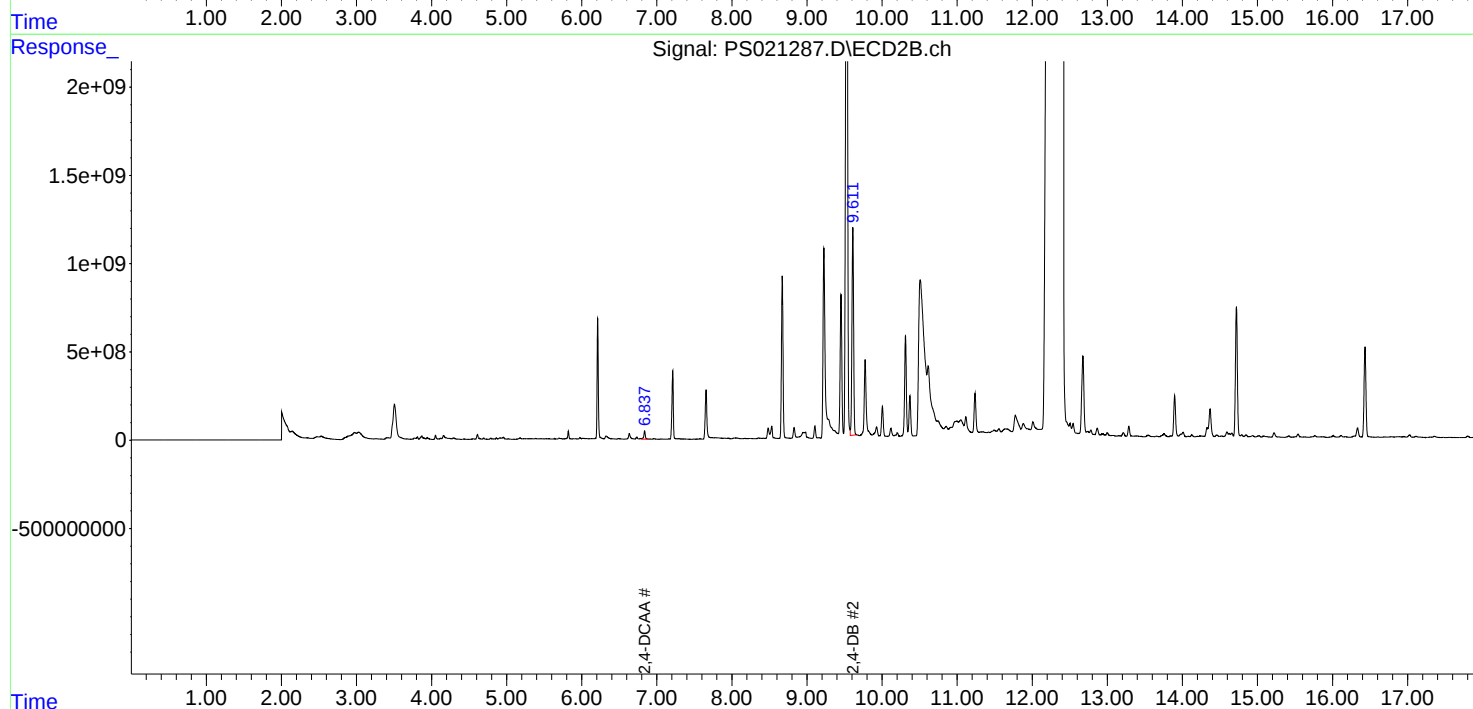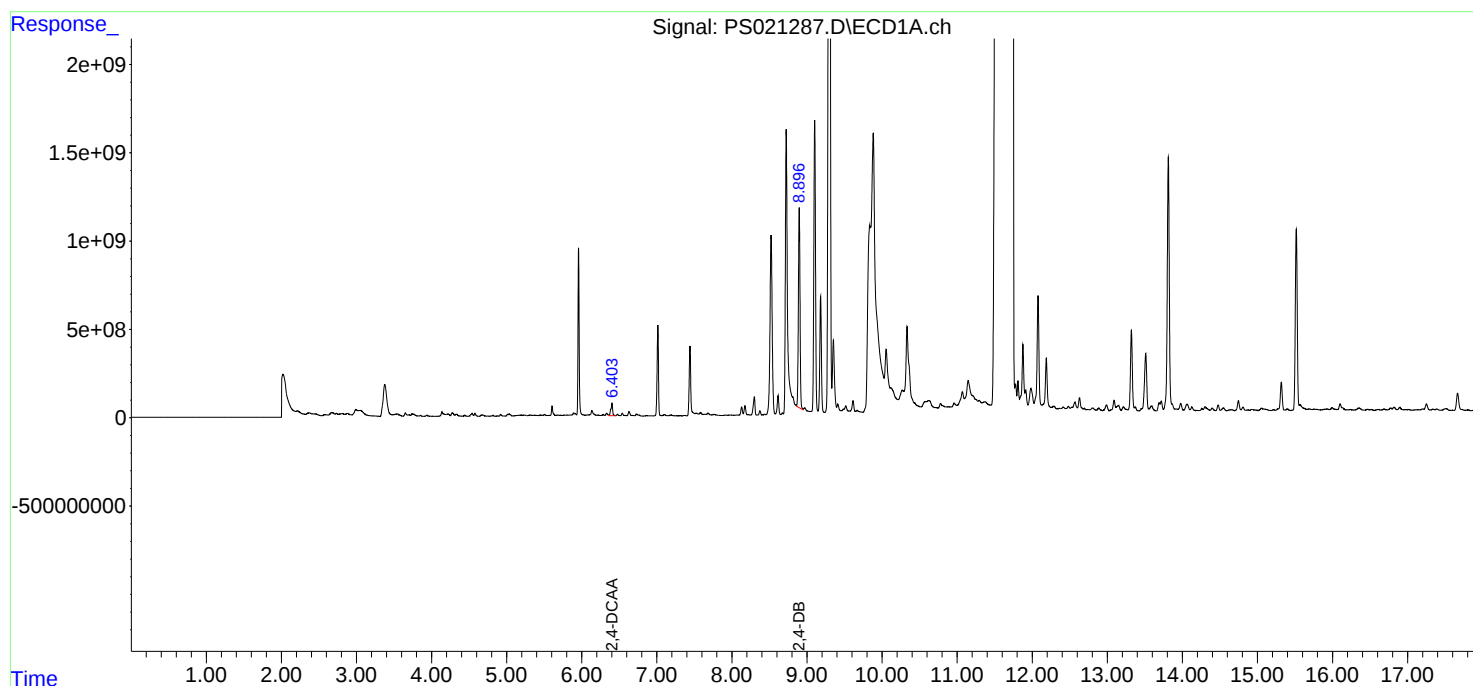

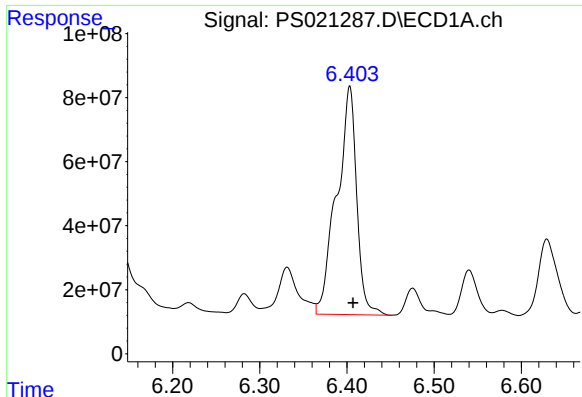


#4 2,4-DCAA

R.T.: 6.403 min
Delta R.T.: -0.004 min
Response: 1132015341
Conc: 520.64 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-10


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/06/2022
Supervised By :Ankita Jodhani 12/06/2022

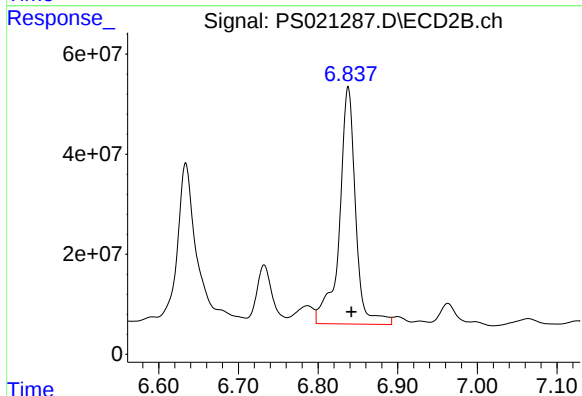


#4 2,4-DCAA

R.T.: 6.838 min
Delta R.T.: -0.004 min
Response: 670445172
Conc: 443.38 ng/ml

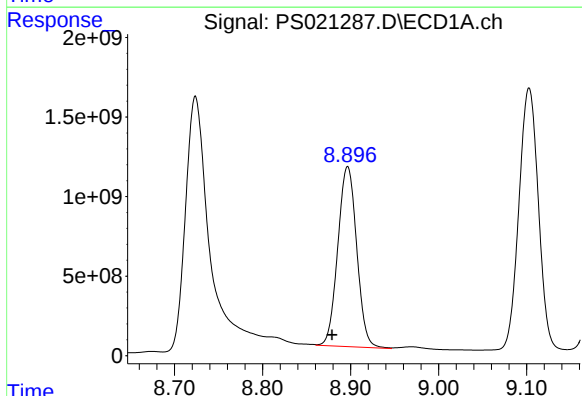

#13 2,4-DB

R.T.: 8.896 min
Delta R.T.: 0.017 min
Response: 16895728634
Conc: 7392.28 ng/ml m

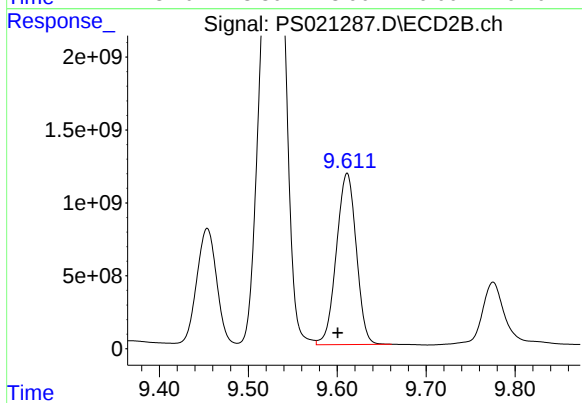

#13 2,4-DB

R.T.: 9.611 min
Delta R.T.: 0.010 min
Response: 18259821140
Conc: 15597.76 ng/ml