

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120324\
 Data File : PS028668.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Dec 2024 07:32
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 09:58:13 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 26 14:44:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	7.223	0.000	598101	0	<MDL	N.D.	#
Target Compounds								
1) T	Dalapon	2.674f	2.720f	23334176	4663410	8.041	2.135	#
2) T	3,5-DICHL...	6.448f	0.000	1216595	0	<MDL	N.D.	#
3) T	4-Nitroph...	7.012	0.000	1168064	0	<MDL	N.D.	#
5) T	DICAMBA	7.413	7.925	997288	13577027	<MDL	2.205	#
6) T	MCPD	0.000	8.037	0	10387842	N.D.	2.412	#
7) T	MCPA	7.772	8.242f	575933	11008702	<MDL	1.774	#
8) T	DICHLORPROP	8.122	0.000	975396	0	<MDL	N.D.	#
10) T	Pentachlo...	8.650	0.000	866828	0	<MDL	N.D.	#
11) T	2,4,5-TP ...	9.228	0.000	1350378	0	<MDL	N.D.	#
12) T	2,4,5-T	9.525	10.293	3835437	4114604	<MDL	<MDL	#
15) T	Picloram	11.123	12.333	25834510	11804097	<MDL	<MDL	#
16) T	DCPA	11.597	0.000	1181334	0	<MDL	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120324\
Data File : PS028668.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Dec 2024 07:32
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 09:58:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
Quant Title : 8080.M
QLast Update : Tue Nov 26 14:44:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

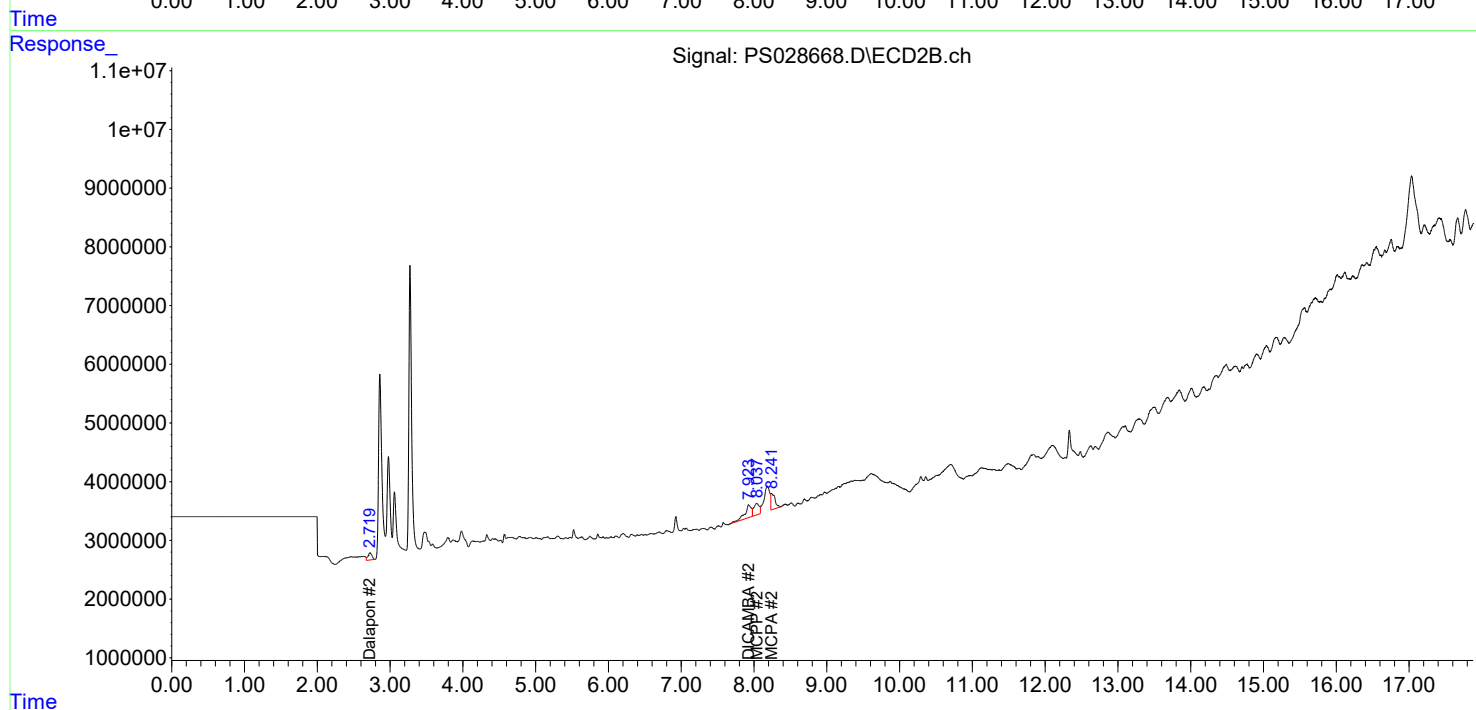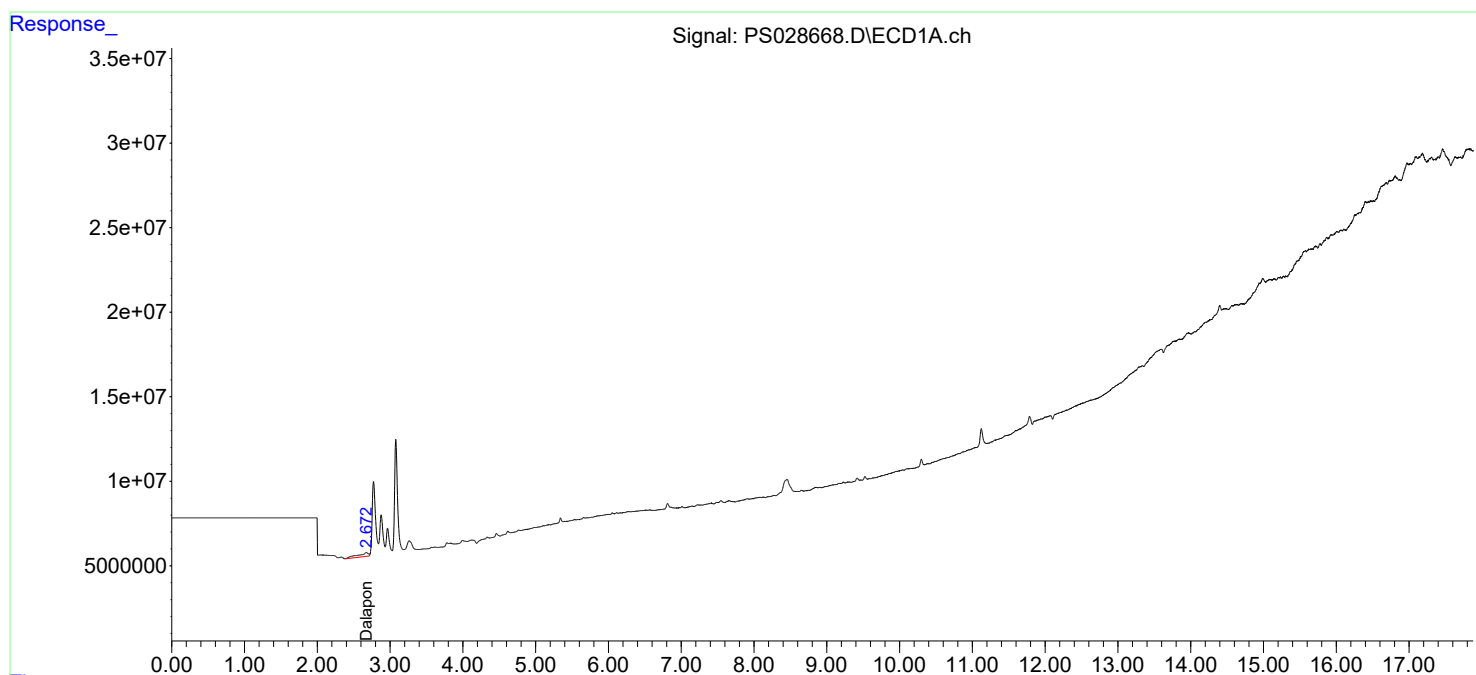


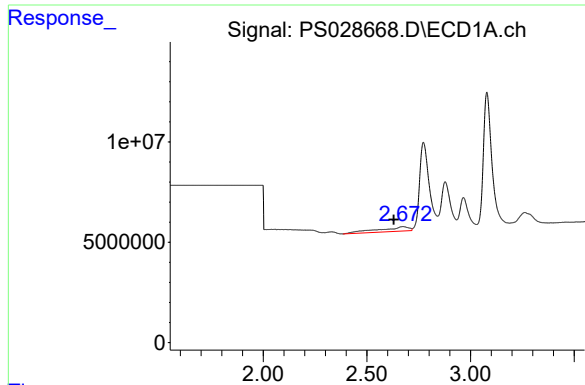

#1 Dalapon


R.T.: 2.674 min
Delta R.T.: 0.044 min
Response: 23334176
Conc: 8.04 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

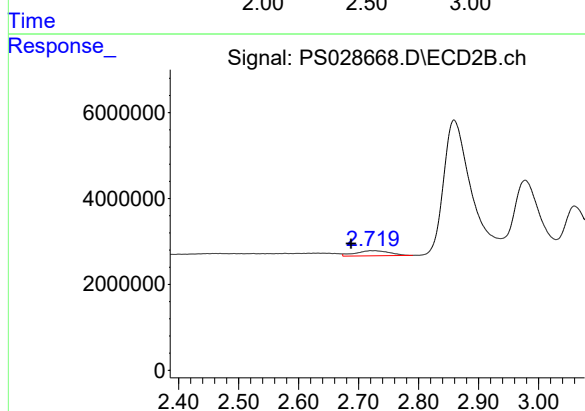


#1 Dalapon

R.T.: 2.720 min
Delta R.T.: 0.032 min
Response: 4663410
Conc: 2.14 ng/ml

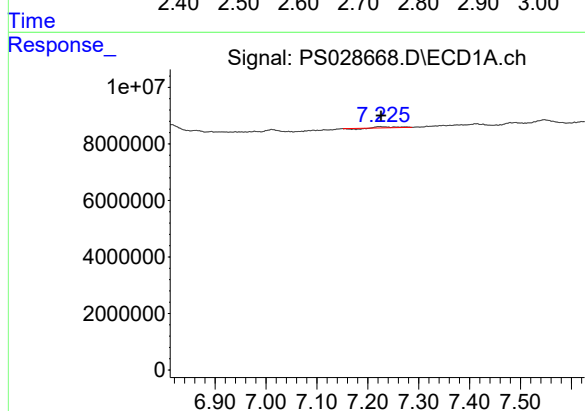


#4 2,4-DCAA

R.T.: 7.223 min
Delta R.T.: -0.003 min
Response: 598101
Conc: N.D.

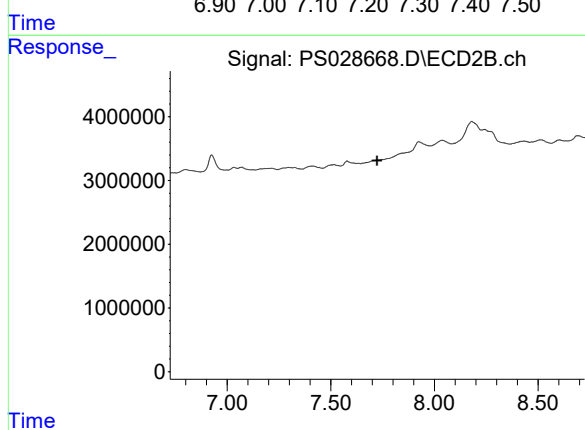

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.725 min
Response: 0
Conc: N.D.

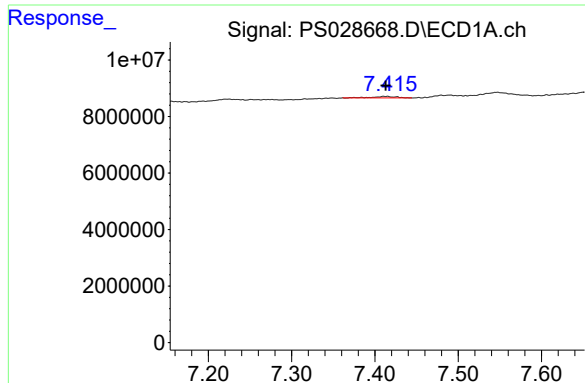

#5 DICAMBA


R.T.: 7.413 min
Delta R.T.: 0.000 min
Response: 997288
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

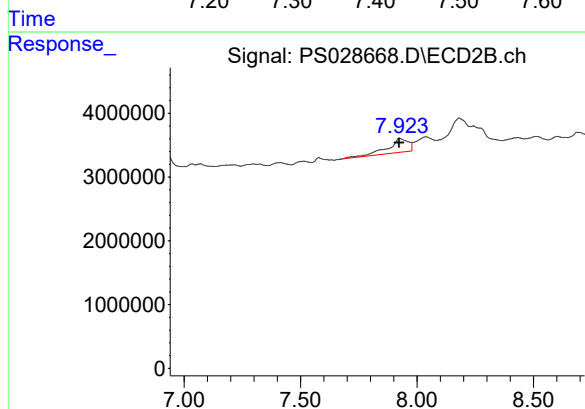


#5 DICAMBA

R.T.: 7.925 min
Delta R.T.: 0.000 min
Response: 13577027
Conc: 2.21 ng/ml

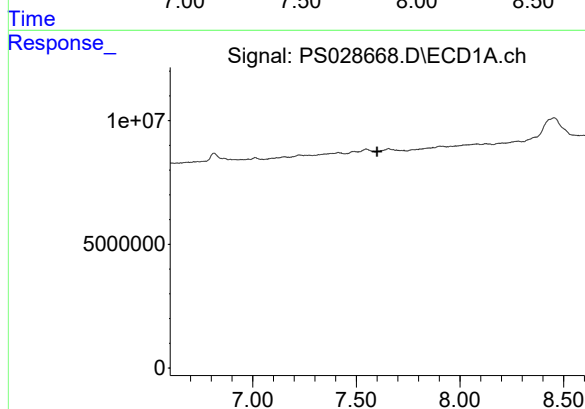


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 7.601 min
Response: 0
Conc: N.D.

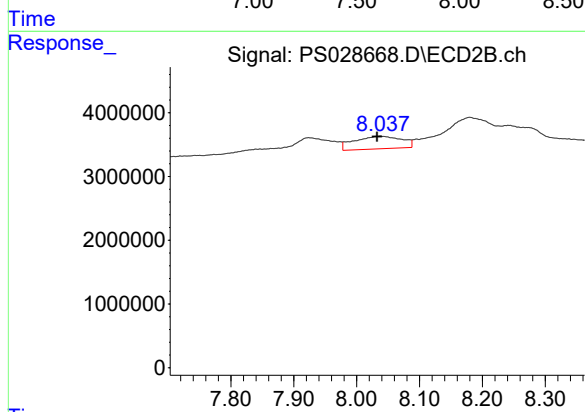

#6 MCPP


R.T.: 8.037 min
Delta R.T.: 0.005 min
Response: 10387842
Conc: 2.41 ug/ml

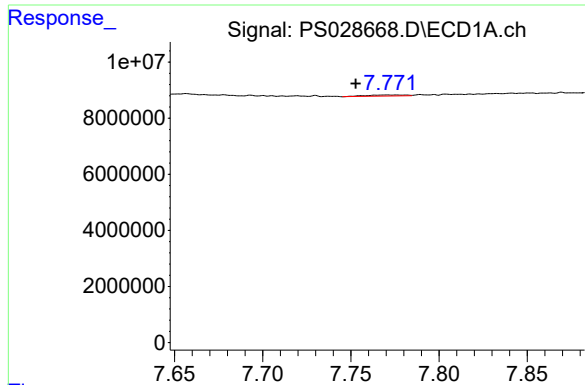

#7 MCPA

R.T.: 7.772 min
Delta R.T.: 0.019 min
Response: 575933
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

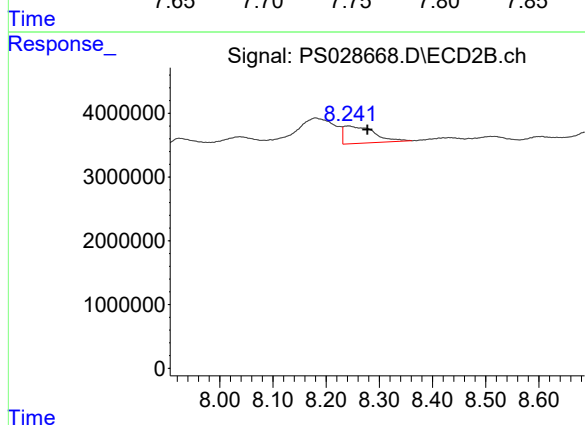

#7 MCPA

R.T.: 8.242 min
Delta R.T.: -0.037 min
Response: 11008702
Conc: 1.77 ug/ml