

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120324\
 Data File : PS028669.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Dec 2024 07:56
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 09:58:21 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 26 14:44:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S	2,4-DCAA	7.227	7.723	1335.1E6	595.6E6	497.722	442.146
------	----------	-------	-------	----------	---------	---------	---------

Target Compounds

1) T	Dalapon	2.675f	0.000	19764050	0	6.811	N.D.	#
2) T	3,5-DICHL...	6.385	0.000	488341	0	<MDL	N.D.	#
3) T	4-Nitroph...	7.023	0.000	4525380	0	2.633	N.D.	#
5) T	DICAMBA	0.000	7.921	0	3003396	N.D.	<MDL	
7) T	MCPA	0.000	8.242f	0	10238634	N.D.	1.650	
8) T	DICHLORPROP	8.131	0.000	446442	0	<MDL	N.D.	#
10) T	Pentachlo...	8.650	0.000	1225152	0	<MDL	N.D.	#
11) T	2,4,5-TP ...	9.228	9.874	1415064	198313	<MDL	<MDL	#
12) T	2,4,5-T	9.524	10.291	3304325	6084626	<MDL	<MDL	#
13) T	2,4-DB	10.115	0.000	1099917	0	<MDL	N.D.	#
14) T	DINOSEB	11.313	0.000	1148857	0	<MDL	N.D.	#
15) T	Picloram	11.122	12.332	34408700	16957038	1.157	1.315	
16) T	DCPA	11.595	0.000	1151257	0	<MDL	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120324\
Data File : PS028669.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Dec 2024 07:56
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 09:58:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
Quant Title : 8080.M
QLast Update : Tue Nov 26 14:44:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

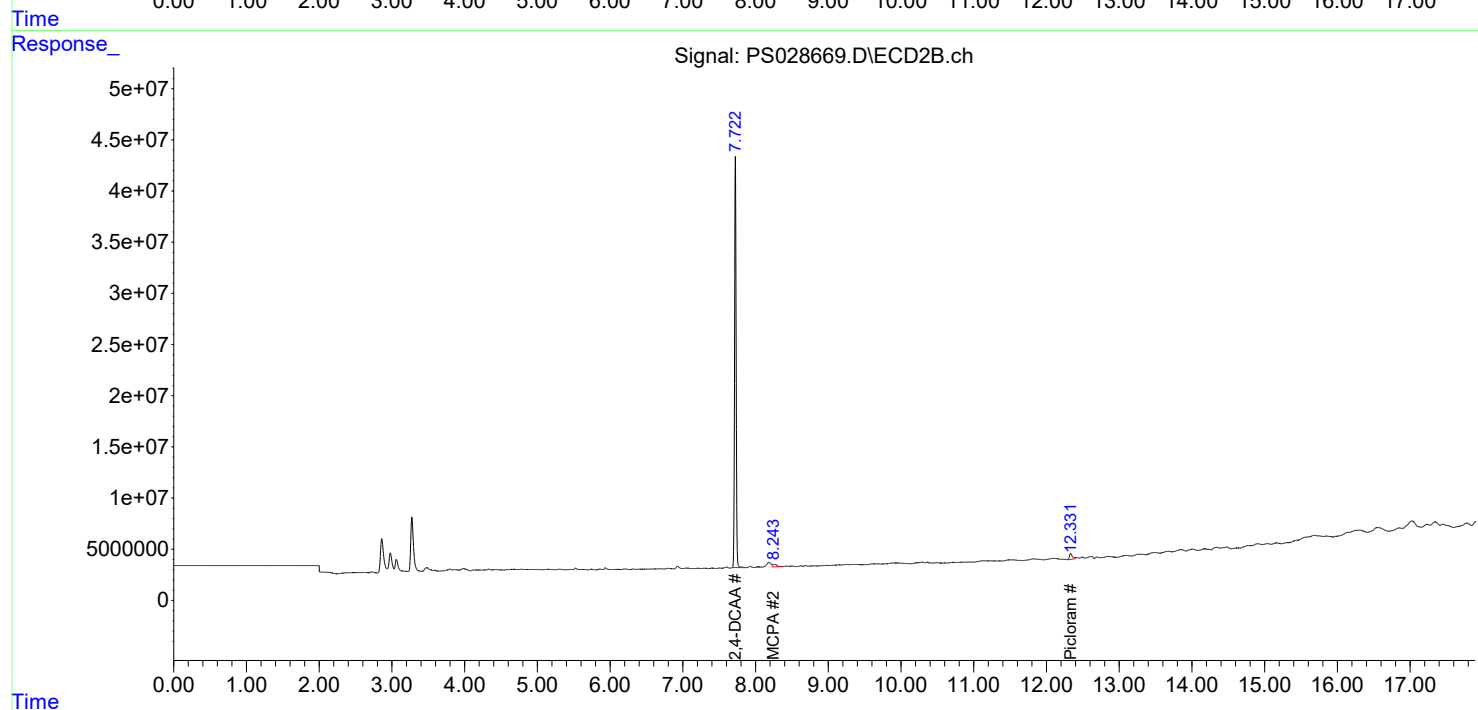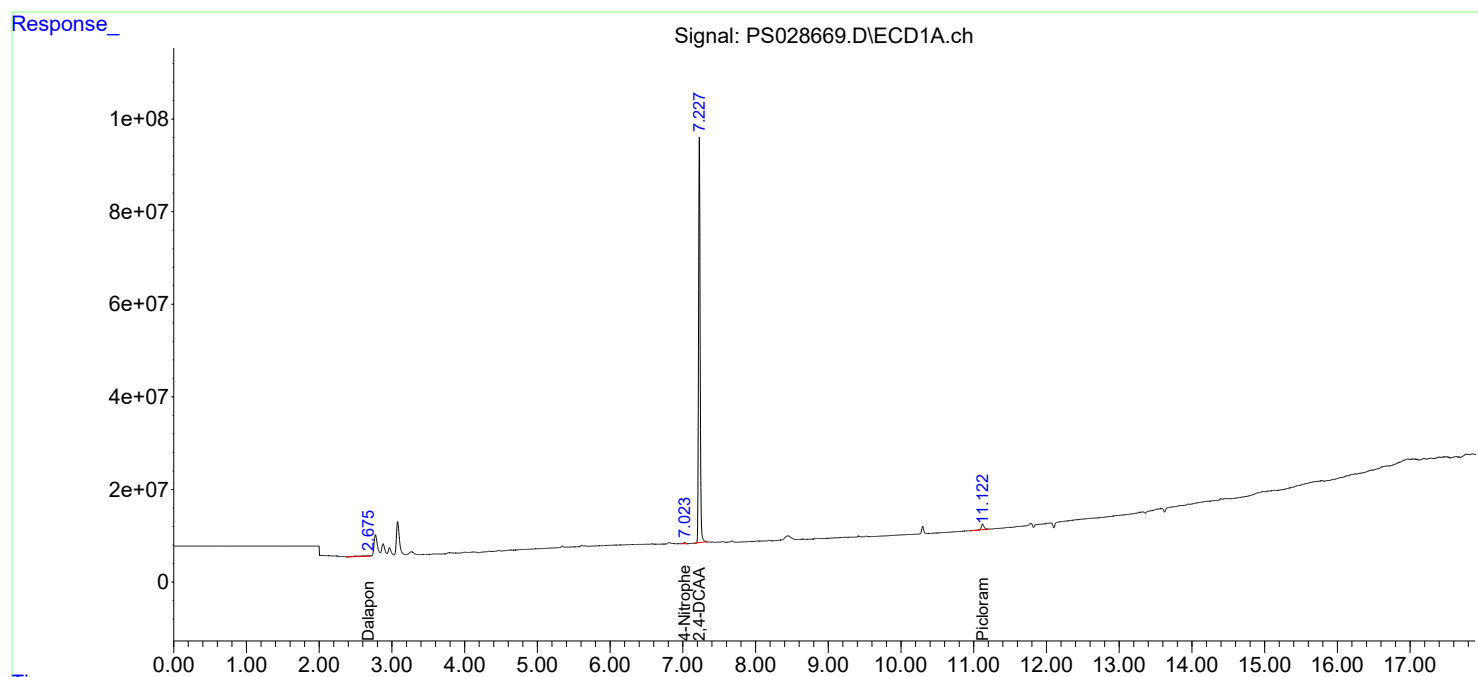


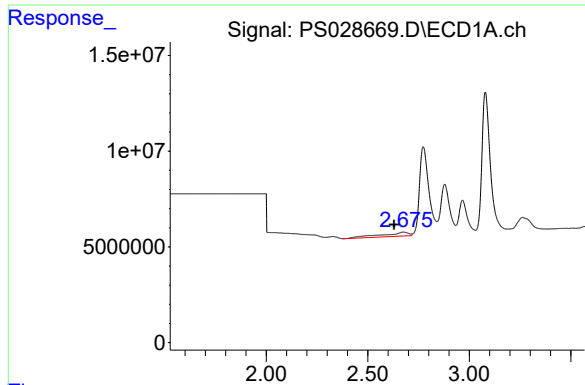

#1 Dalapon


R.T.: 2.675 min
Delta R.T.: 0.045 min
Response: 19764050
Conc: 6.81 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

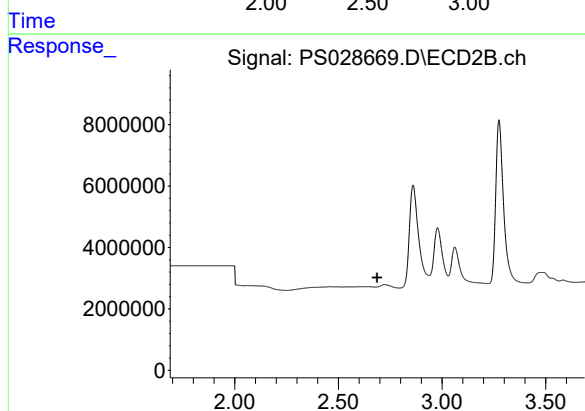


#1 Dalapon

R.T.: 0.000 min
Exp R.T.: 2.688 min
Response: 0
Conc: N.D.

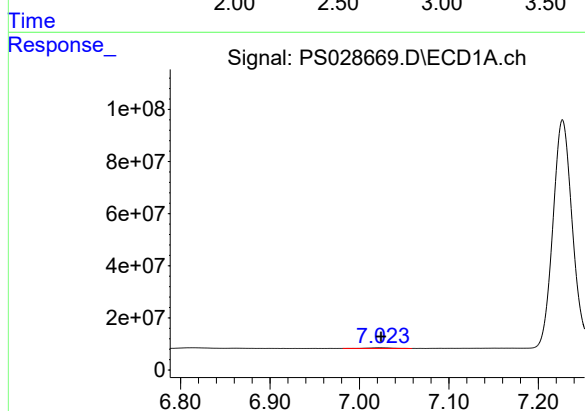


#3 4-Nitrophenol

R.T.: 7.023 min
Delta R.T.: -0.002 min
Response: 4525380
Conc: 2.63 ng/ml

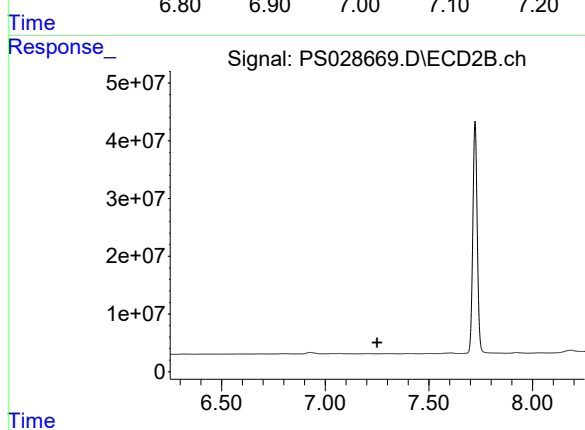

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.251 min
Response: 0
Conc: N.D.

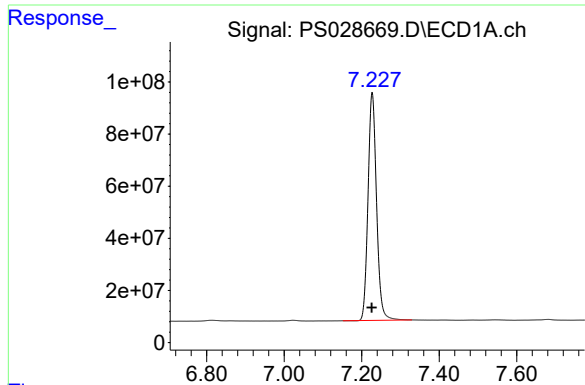

#4 2,4-DCAA


R.T.: 7.227 min
Delta R.T.: 0.001 min
Response: 1335060252
Conc: 497.72 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

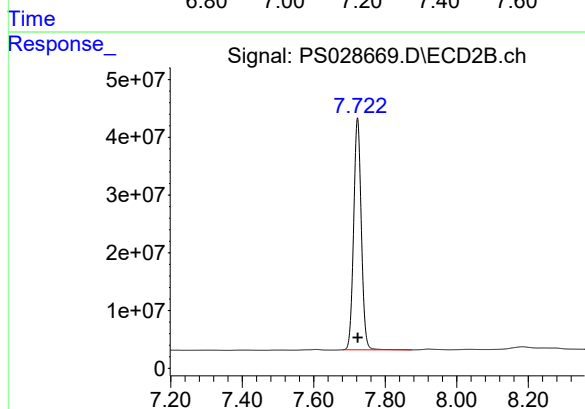


#4 2,4-DCAA

R.T.: 7.723 min
Delta R.T.: -0.002 min
Response: 595584133
Conc: 442.15 ng/ml

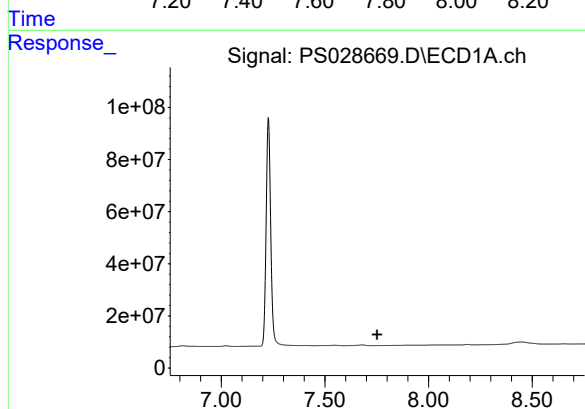


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 7.753 min
Response: 0
Conc: N.D.

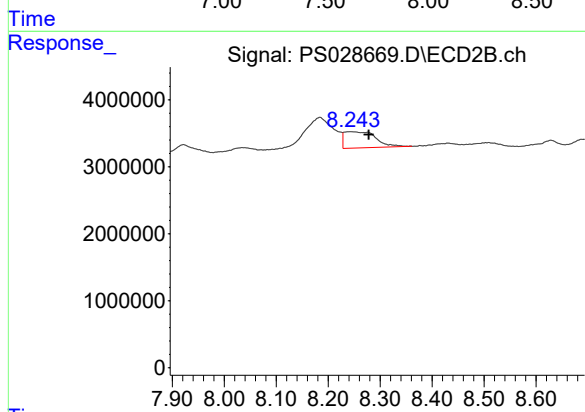

#7 MCPA


R.T.: 8.242 min
Delta R.T.: -0.036 min
Response: 10238634
Conc: 1.65 ug/ml

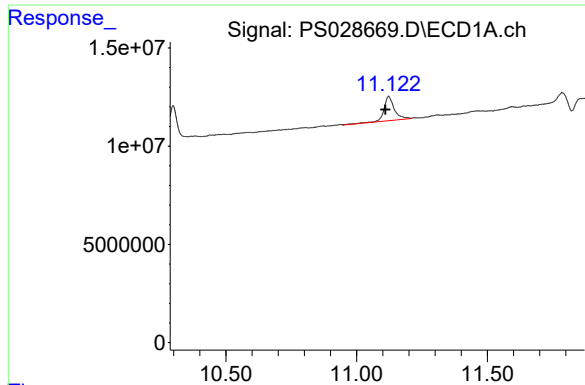

#15 Picloram

R.T.: 11.122 min
Delta R.T.: 0.011 min
Response: 34408700
Conc: 1.16 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

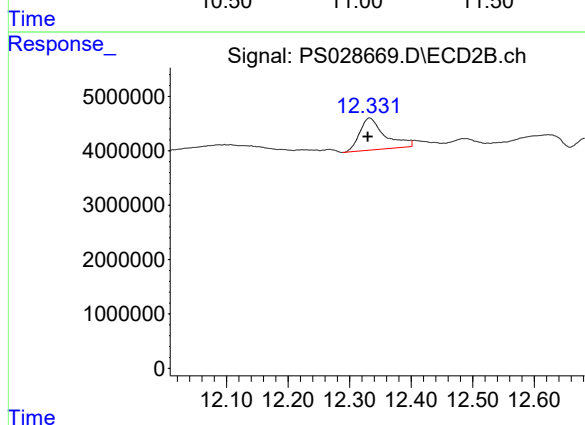

#15 Picloram

R.T.: 12.332 min
Delta R.T.: 0.003 min
Response: 16957038
Conc: 1.32 ng/ml