

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120325\
 Data File : PS032582.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Dec 2025 12:58
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 13:21:30 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120325.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 03 12:35:19 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.037	7.389	1877.9E6	1696.3E6	339.981	316.407
Target Compounds							
1) T	Dalapon	0.000	2.497f	0	7845546	N.D.	1.075
2) T	3,5-DICHL...	6.161f	6.395	21229886	2895058	2.862	<MDL #
6) T	MCP	0.000	7.723f	0	6038502	N.D.	<MDL
7) T	MCPA	7.524	7.921	1808197	25863674	<MDL	1.558 #
9) T	2,4-D	0.000	8.623	0	2640016	N.D.	<MDL
10) T	Pentachlo...	8.425f	9.084	5985923	6443706	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	9.502	0	6240407	N.D.	<MDL
12) T	2,4,5-T	0.000	9.923	0	3305291	N.D.	<MDL
13) T	2,4-DB	0.000	10.446f	0	19138777	N.D.	4.698
14) T	DINOSEB	0.000	10.878	0	24259334	N.D.	1.341
15) T	Picloram	0.000	11.959	0	31936260	N.D.	<MDL
16) T	DCPA	0.000	11.819f	0	34710660	N.D.	1.020


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120325\
Data File : PS032582.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Dec 2025 12:58
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 13:21:30 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120325.M
Quant Title : 8080.M
QLast Update : Wed Dec 03 12:35:19 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

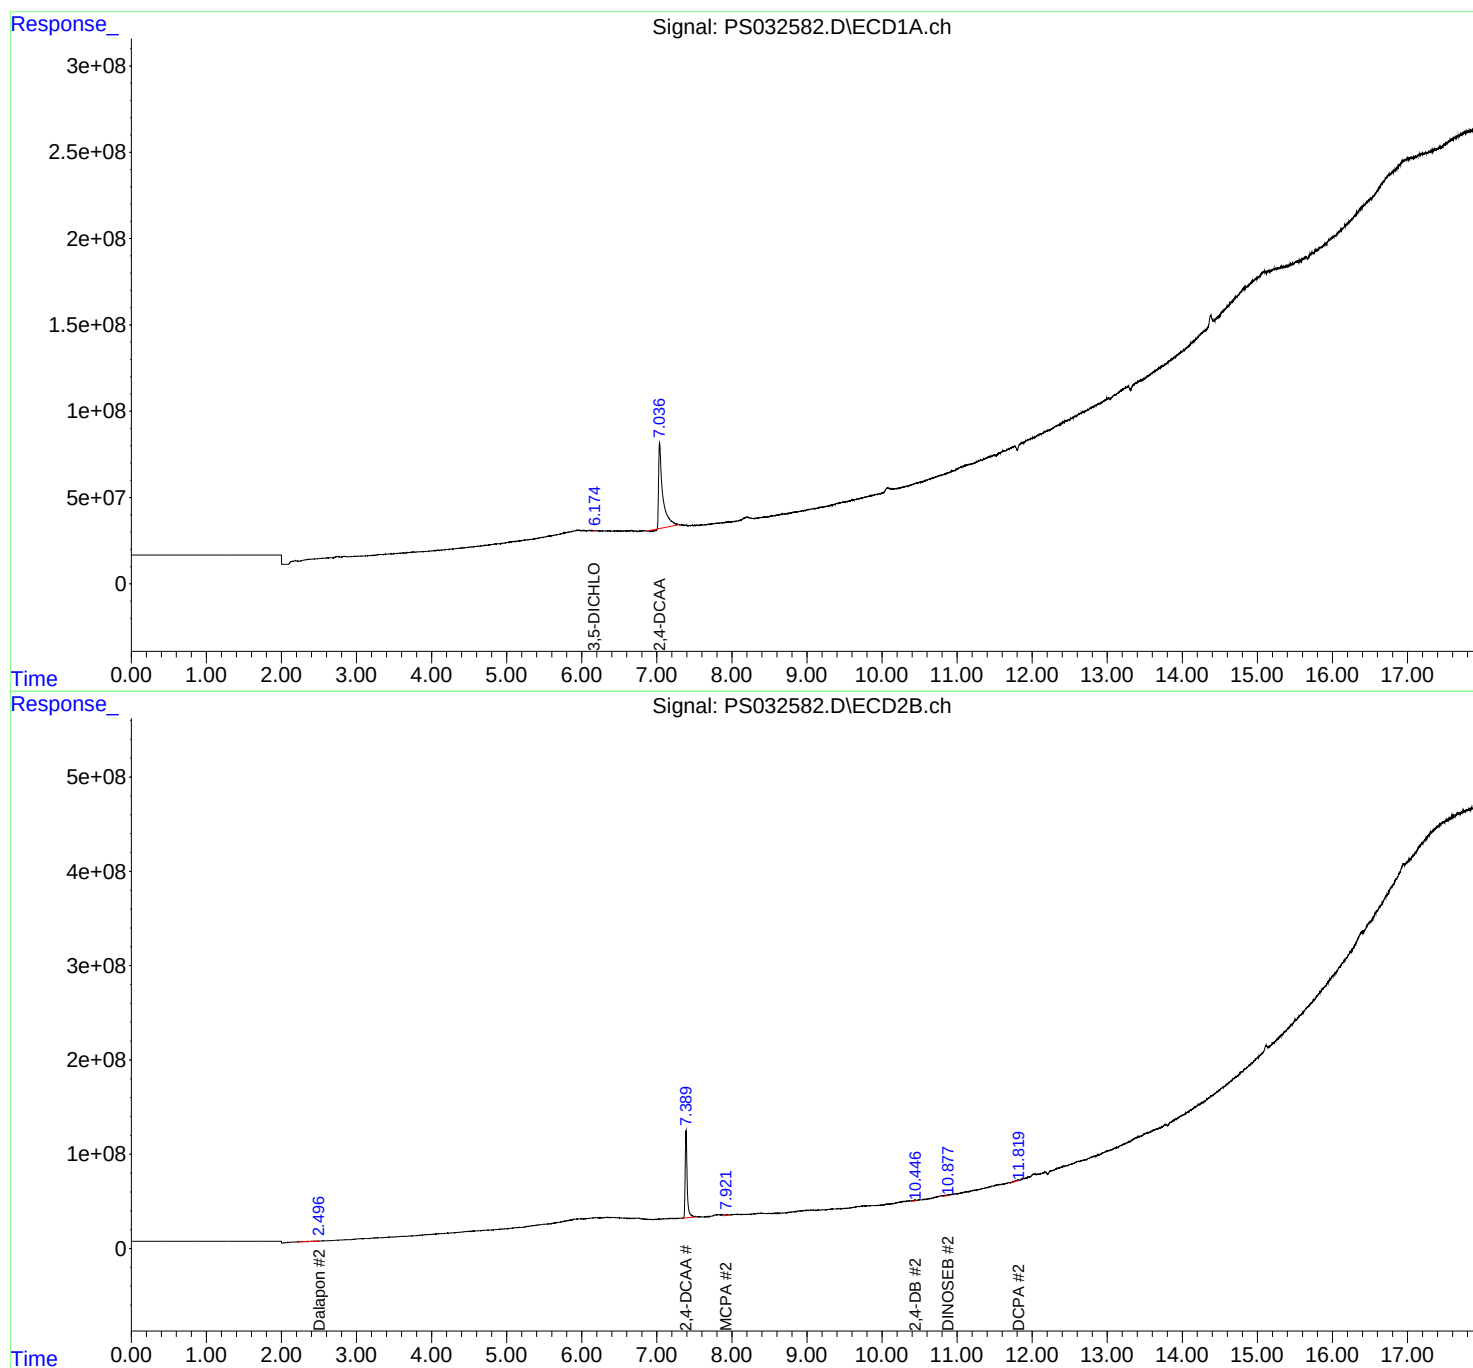


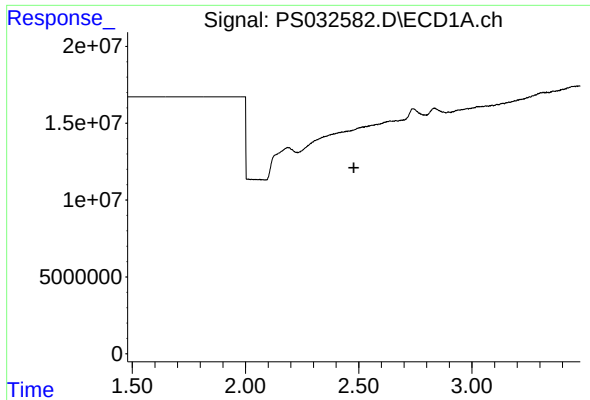

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

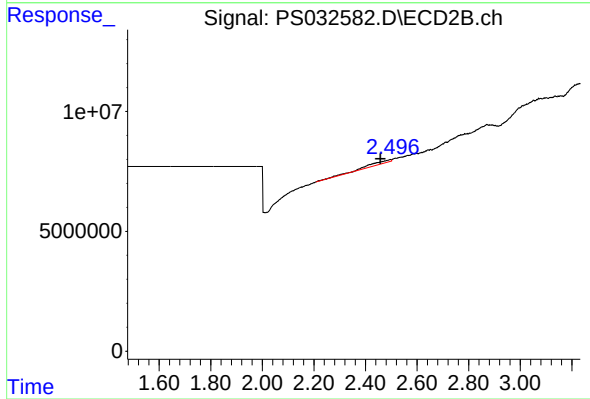


#1 Dalapon

R.T.: 2.497 min
Delta R.T.: 0.039 min
Response: 7845546
Conc: 1.07 ng/ml

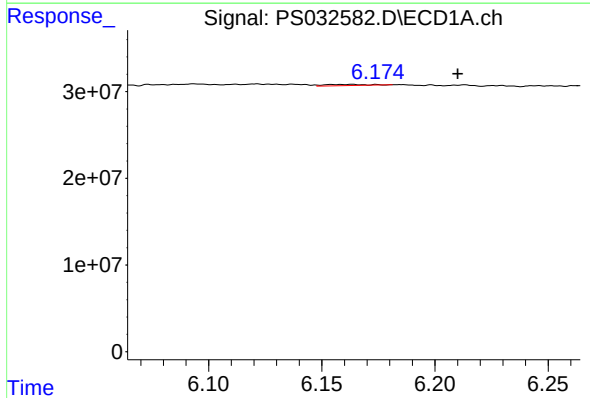


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.161 min
Delta R.T.: -0.049 min
Response: 21229886
Conc: 2.86 ng/ml

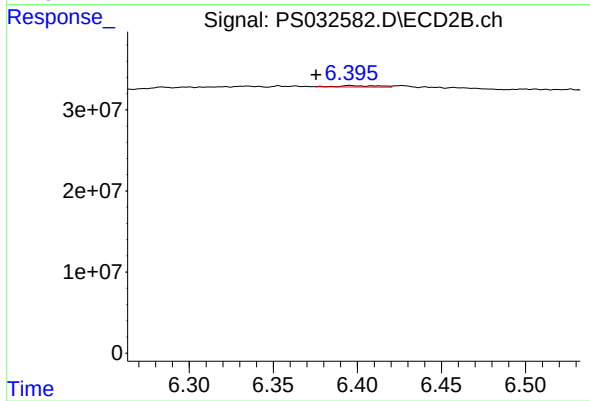

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.395 min
Delta R.T.: 0.020 min
Response: 2895058
Conc: N.D.

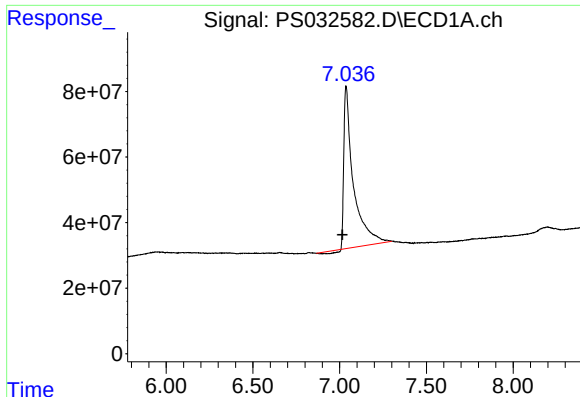

#4 2,4-DCAA


R.T.: 7.037 min
Delta R.T.: 0.020 min
Response: 1877934706
Conc: 339.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

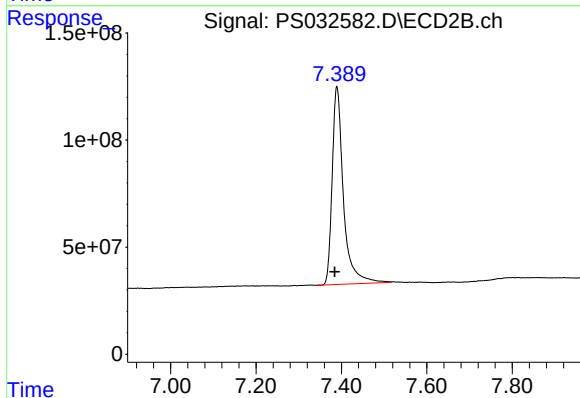


#4 2,4-DCAA

R.T.: 7.389 min
Delta R.T.: 0.005 min
Response: 1696325206
Conc: 316.41 ng/ml

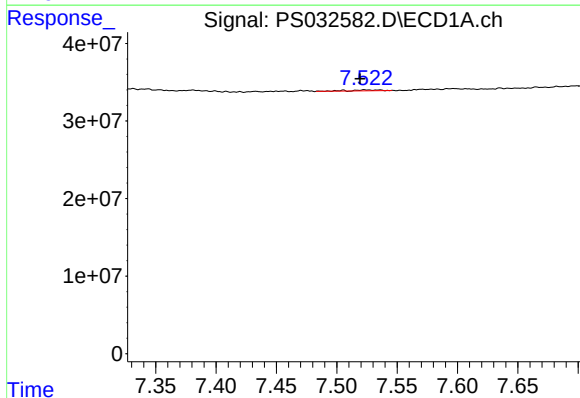


#7 MCPA

R.T.: 7.524 min
Delta R.T.: 0.005 min
Response: 1808197
Conc: N.D.

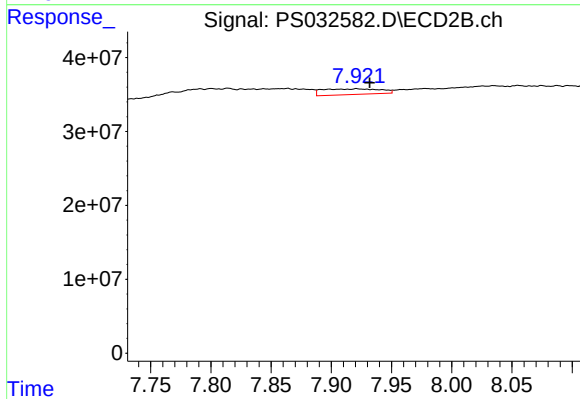

#7 MCPA


R.T.: 7.921 min
Delta R.T.: -0.011 min
Response: 25863674
Conc: 1.56 ug/ml

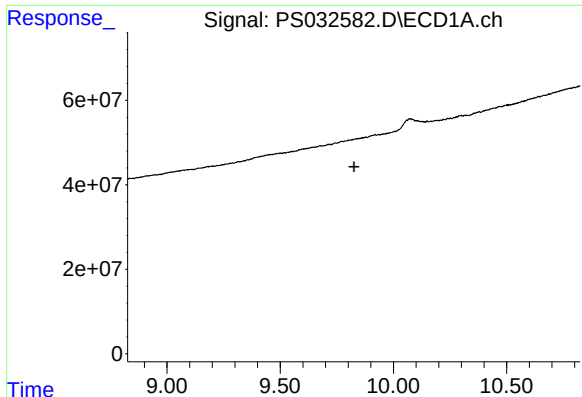

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.826 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

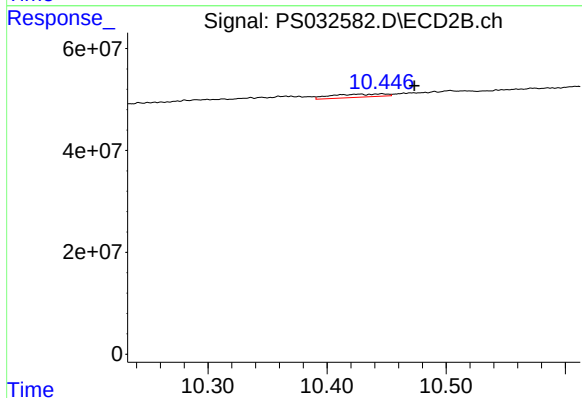


#13 2,4-DB

R.T.: 10.446 min
Delta R.T.: -0.027 min
Response: 19138777
Conc: 4.70 ng/ml

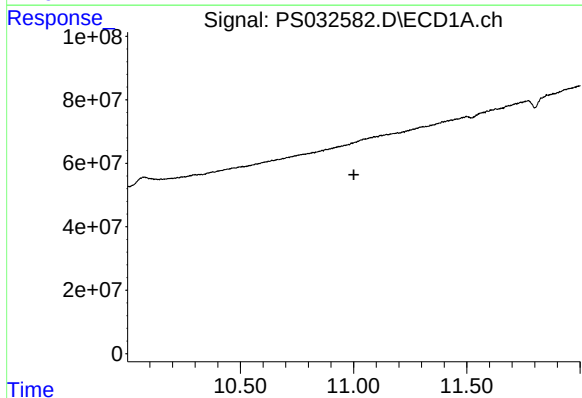


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 11.001 min
Response: 0
Conc: N.D.

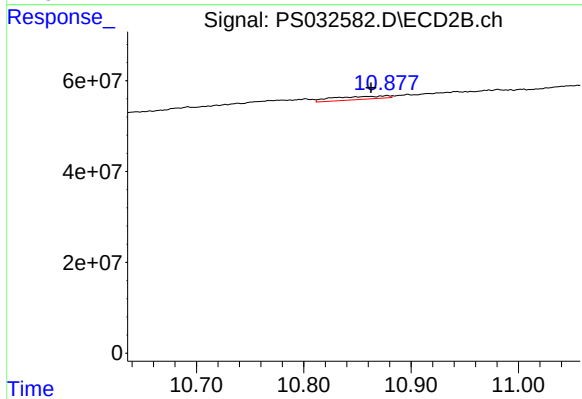

#14 DINOSEB


R.T.: 10.878 min
Delta R.T.: 0.015 min
Response: 24259334
Conc: 1.34 ng/ml

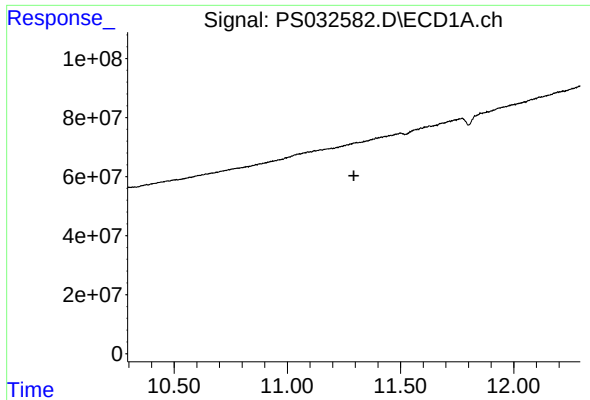

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.293 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

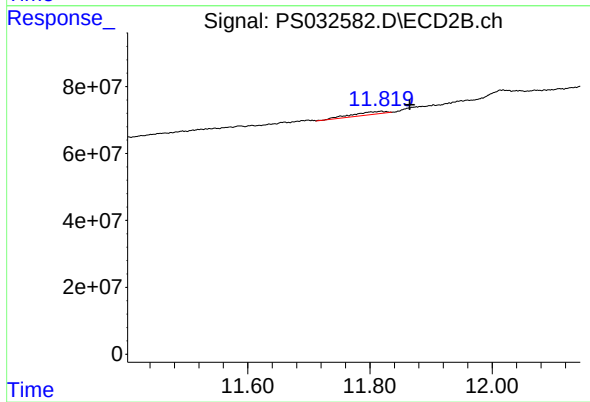

#16 DCPA

R.T.: 11.819 min
Delta R.T.: -0.047 min
Response: 34710660
Conc: 1.02 ng/ml